

Evaluation of a fixation-based tuning mechanism for large aperture tunable lenses in a presbyopia correction prototype

Agarwala, Rajat¹; Severitt, Björn¹; Hosp, Benedikt¹; Wahl, Siegfried^{1,2}

¹ ZEISS Vision Science Lab, Institute for Ophthalmic Research, University of Tübingen, Maria-von-Lindenstraße 6, Tübingen, Germany

² Carl Zeiss Vision International GmbH, Turnstraße 27, Aalen, Germany

6312



Purpose

Presbyopia is an inevitable refractive error that affects people starting in their late 40s. Over the recent years, various mechanisms have been developed to tune power of optical lenses with dynamic focus ability for presbyopia correction.^{1,2}

We developed and tested an algorithm to utilize fixations from an eye tracker and depth data from LIDAR camera to tune the focus of the wearer's prototype to the fixation distance.


Methods

This study consisted of seven healthy participants with a mean age of 26 ± 3.1 years old and mean spherical refractive error of -1.03 ± 1.34 D.

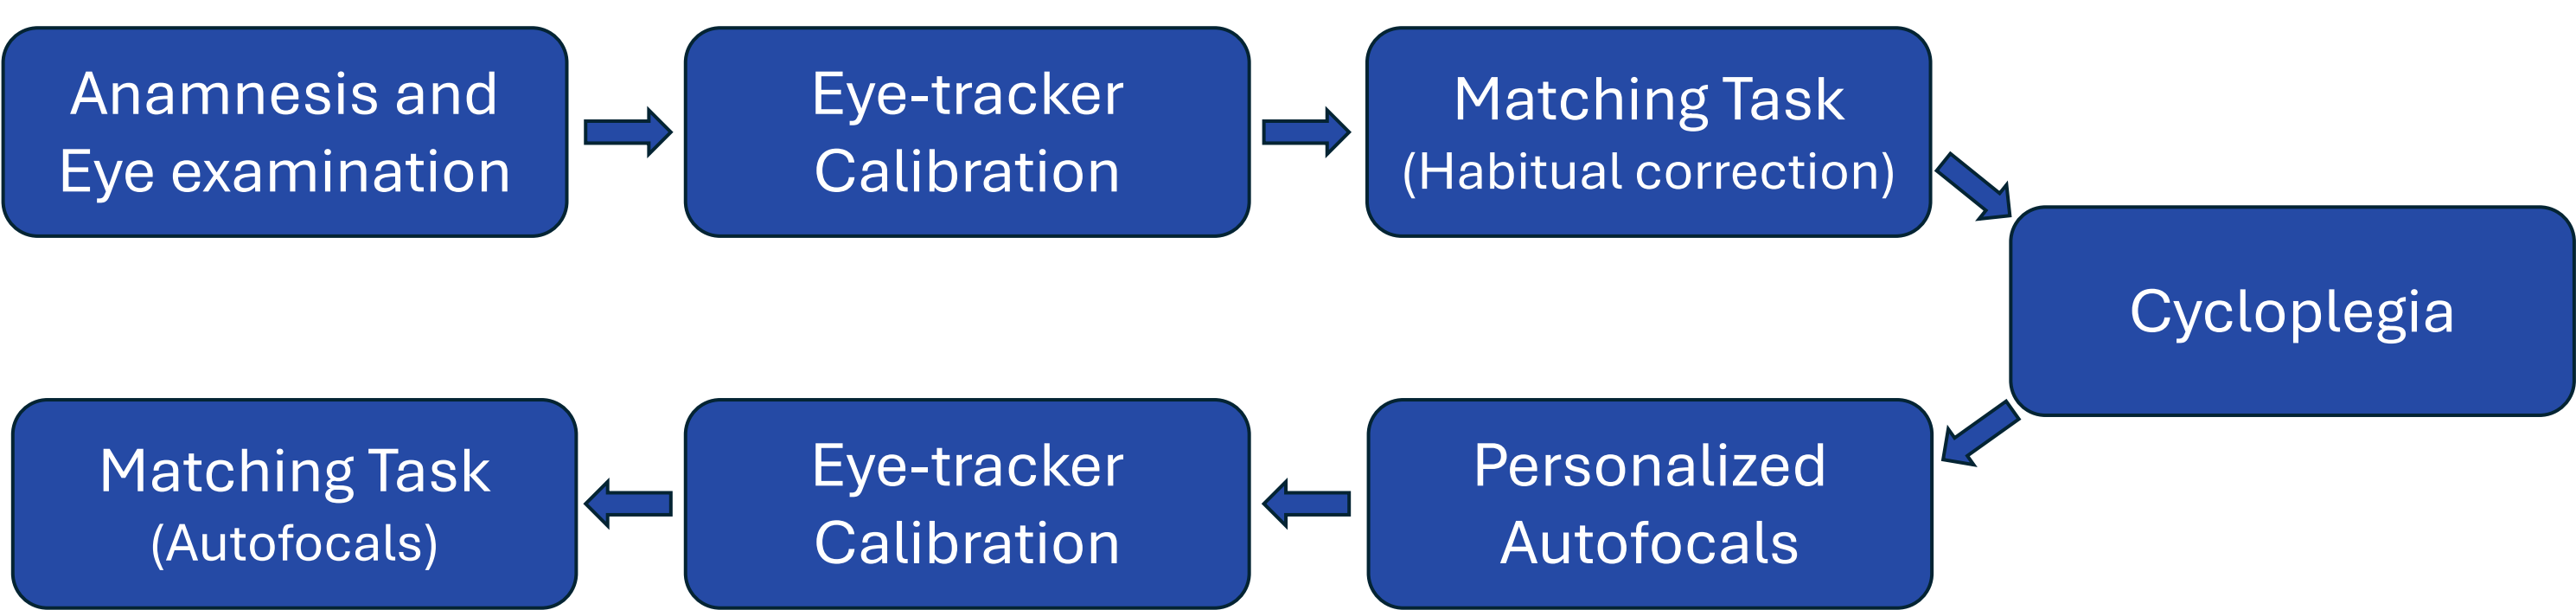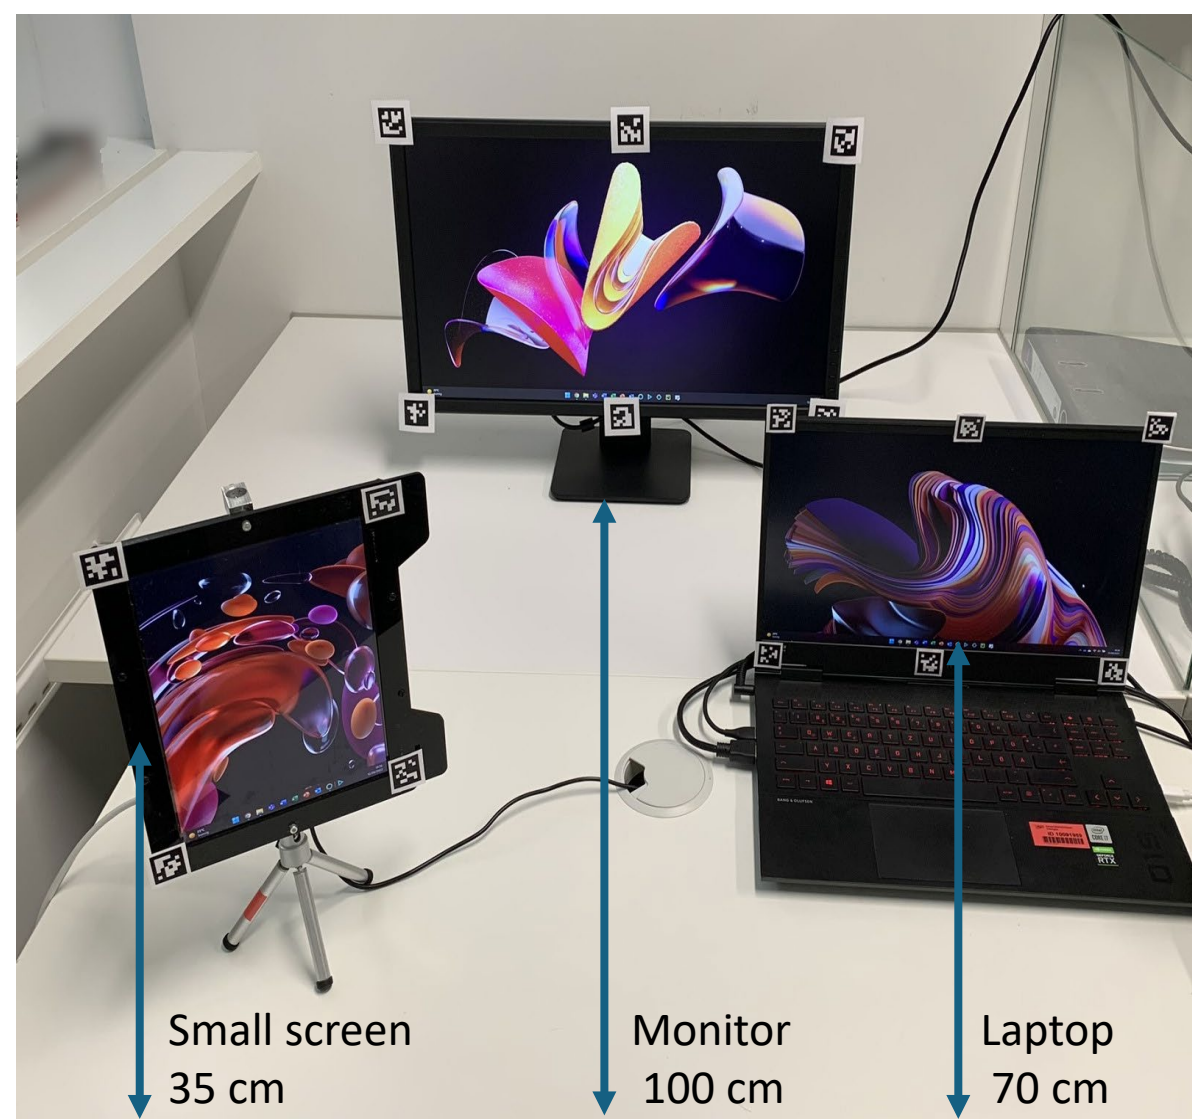

Matching Task

Landolt C rings

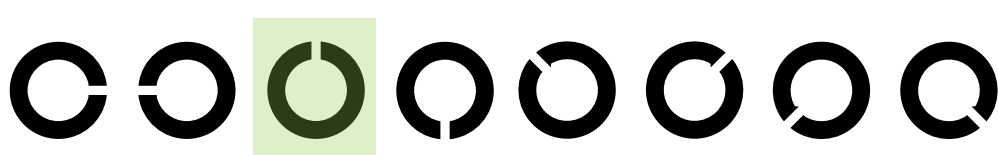

Sloan Optotypes



Matching optotypes?

Match: True/False


Subject responses:

Match: True/False

Response Time


3 repetitions

30 trials for each repetition

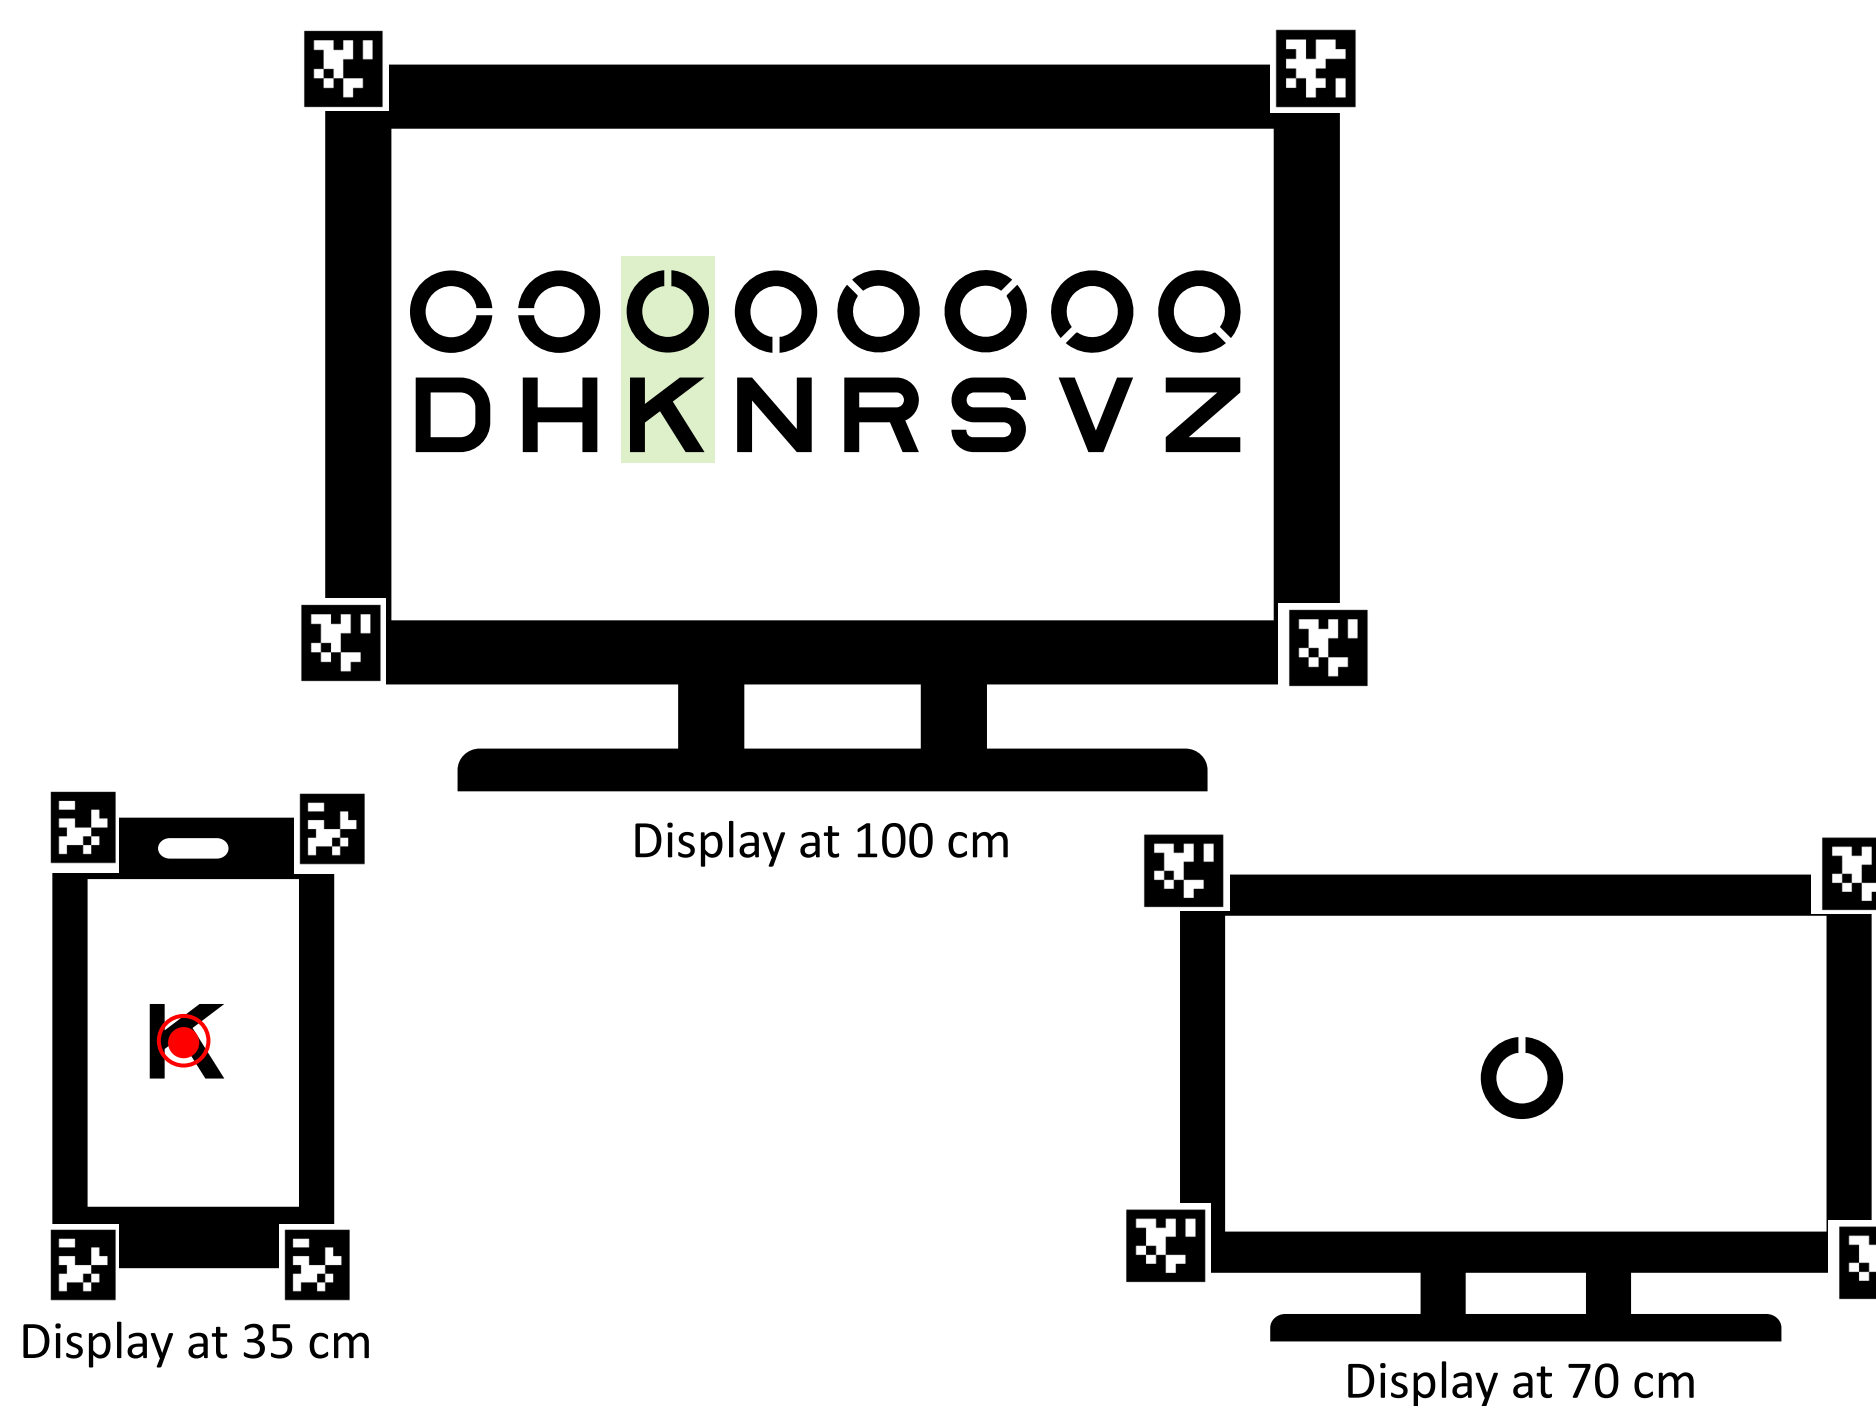



Results

The response time was higher and accuracy marginally lower for the autofocal condition as compared to the habitual correction, however, no statistical difference was observed between the two conditions for the matching task.

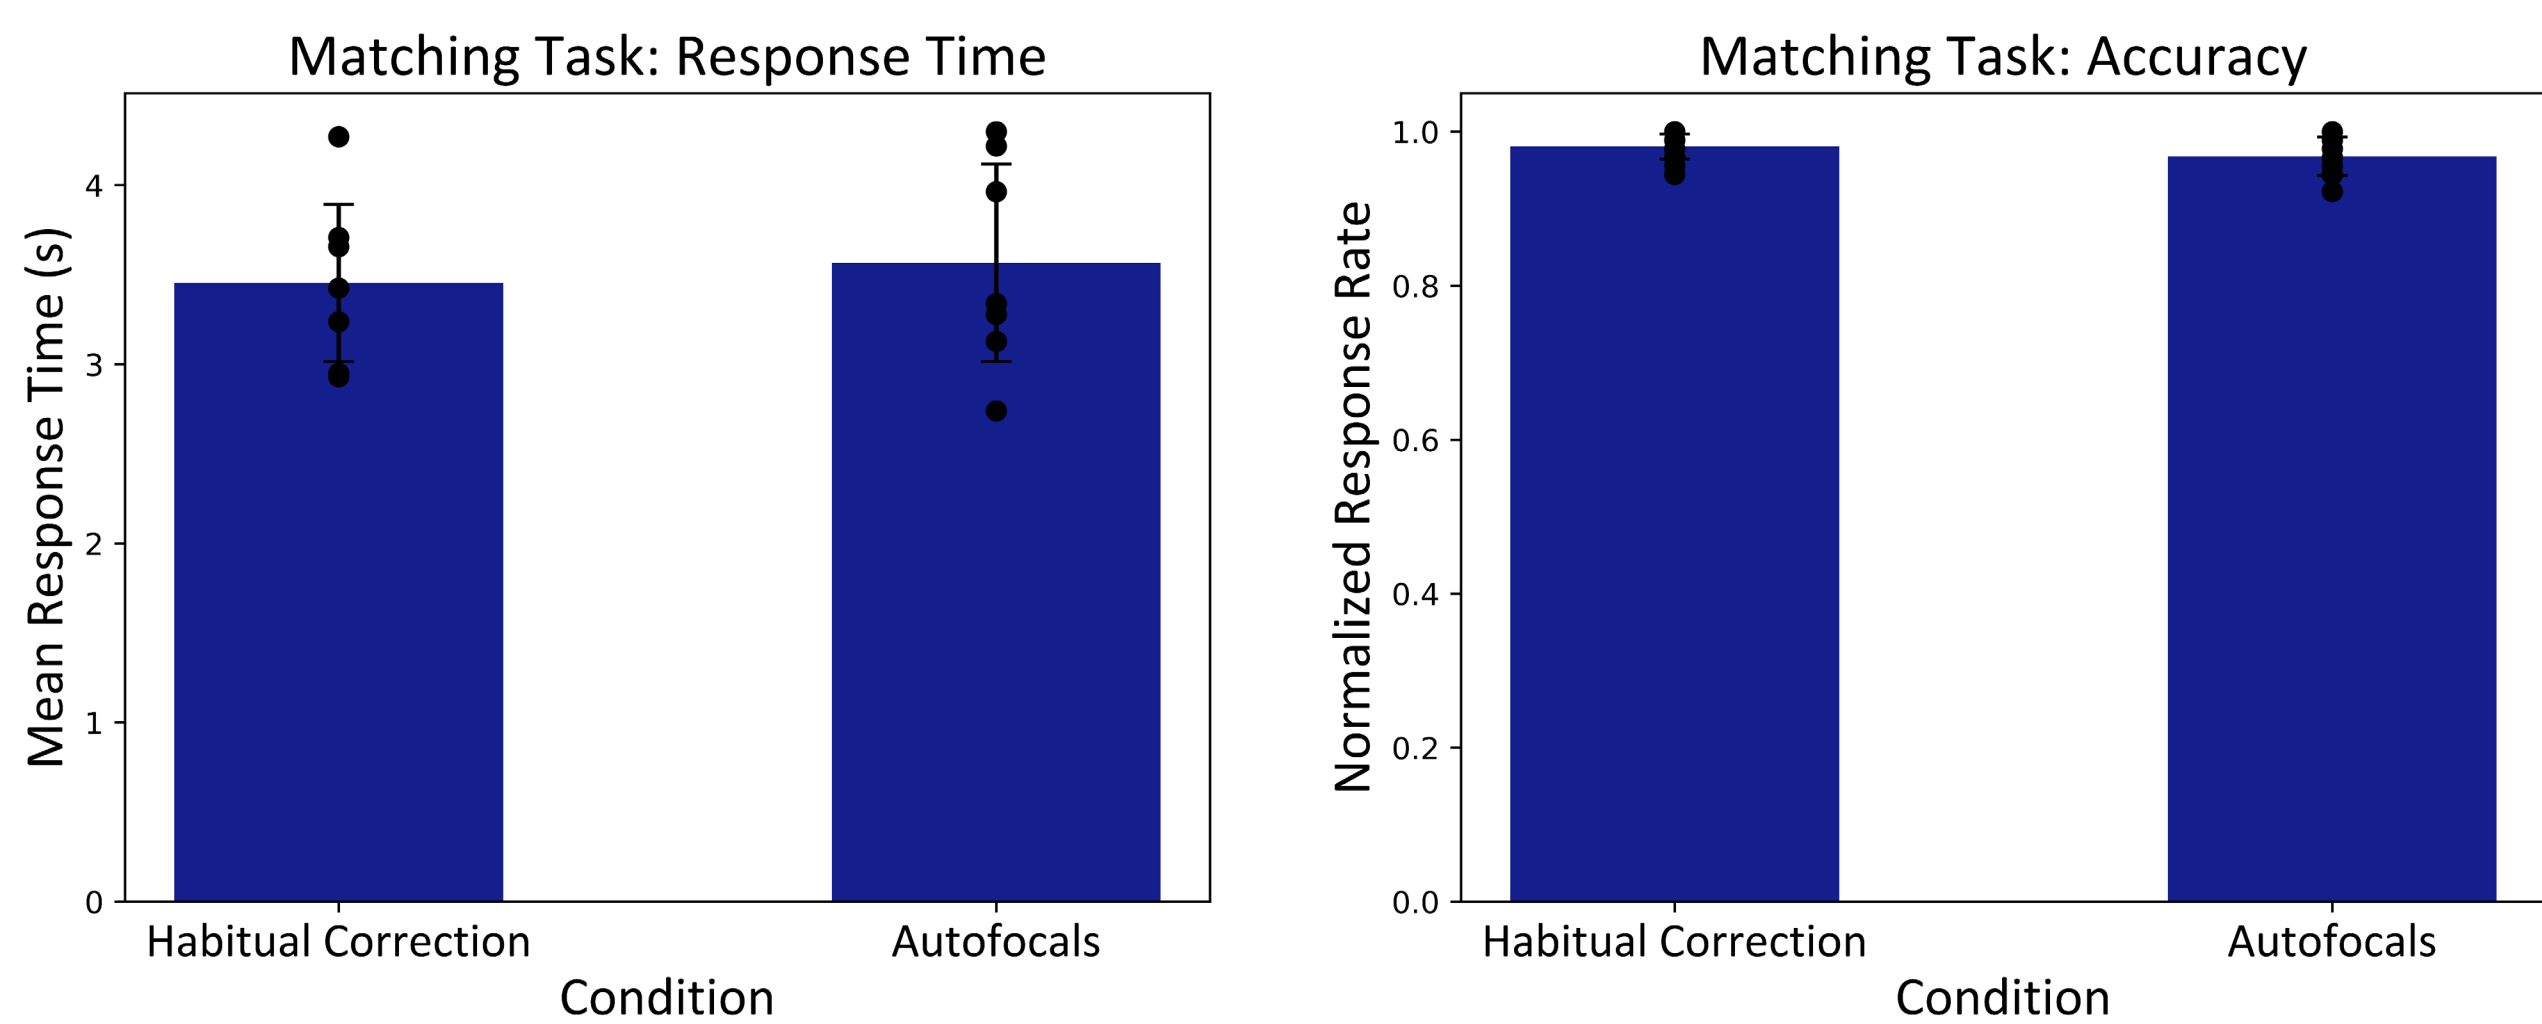

➤ The performance of the participants was similar between habitual correction and autofocal condition.

- Response time changes over repetitions did not depict any kind of learning effect.
- The participants employed different strategies for performing the matching task.

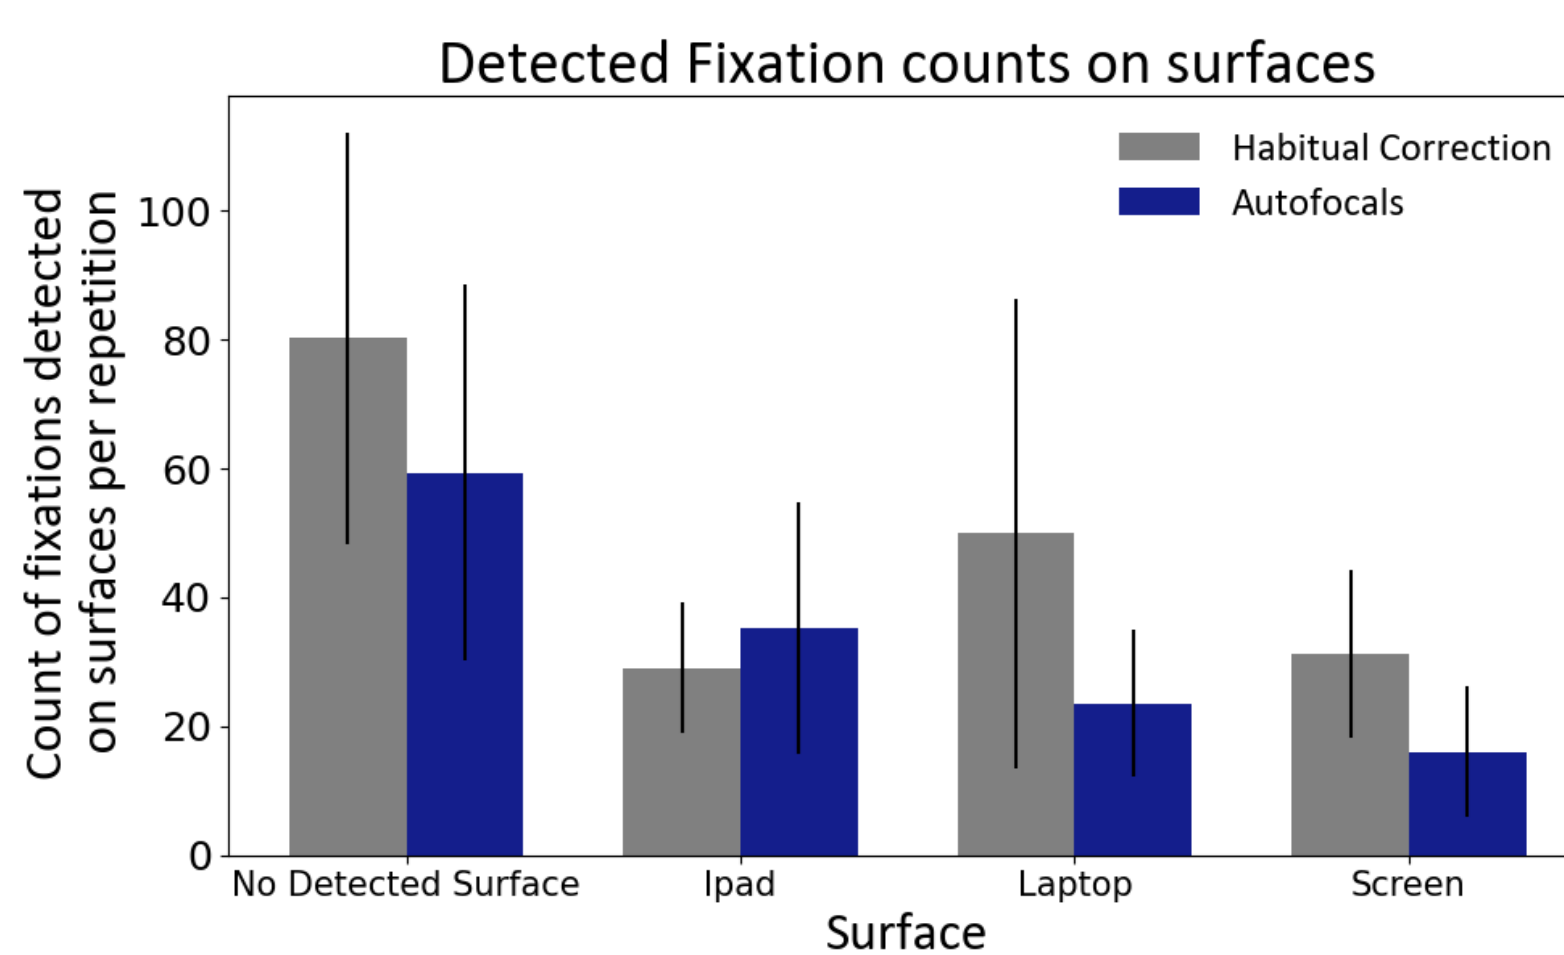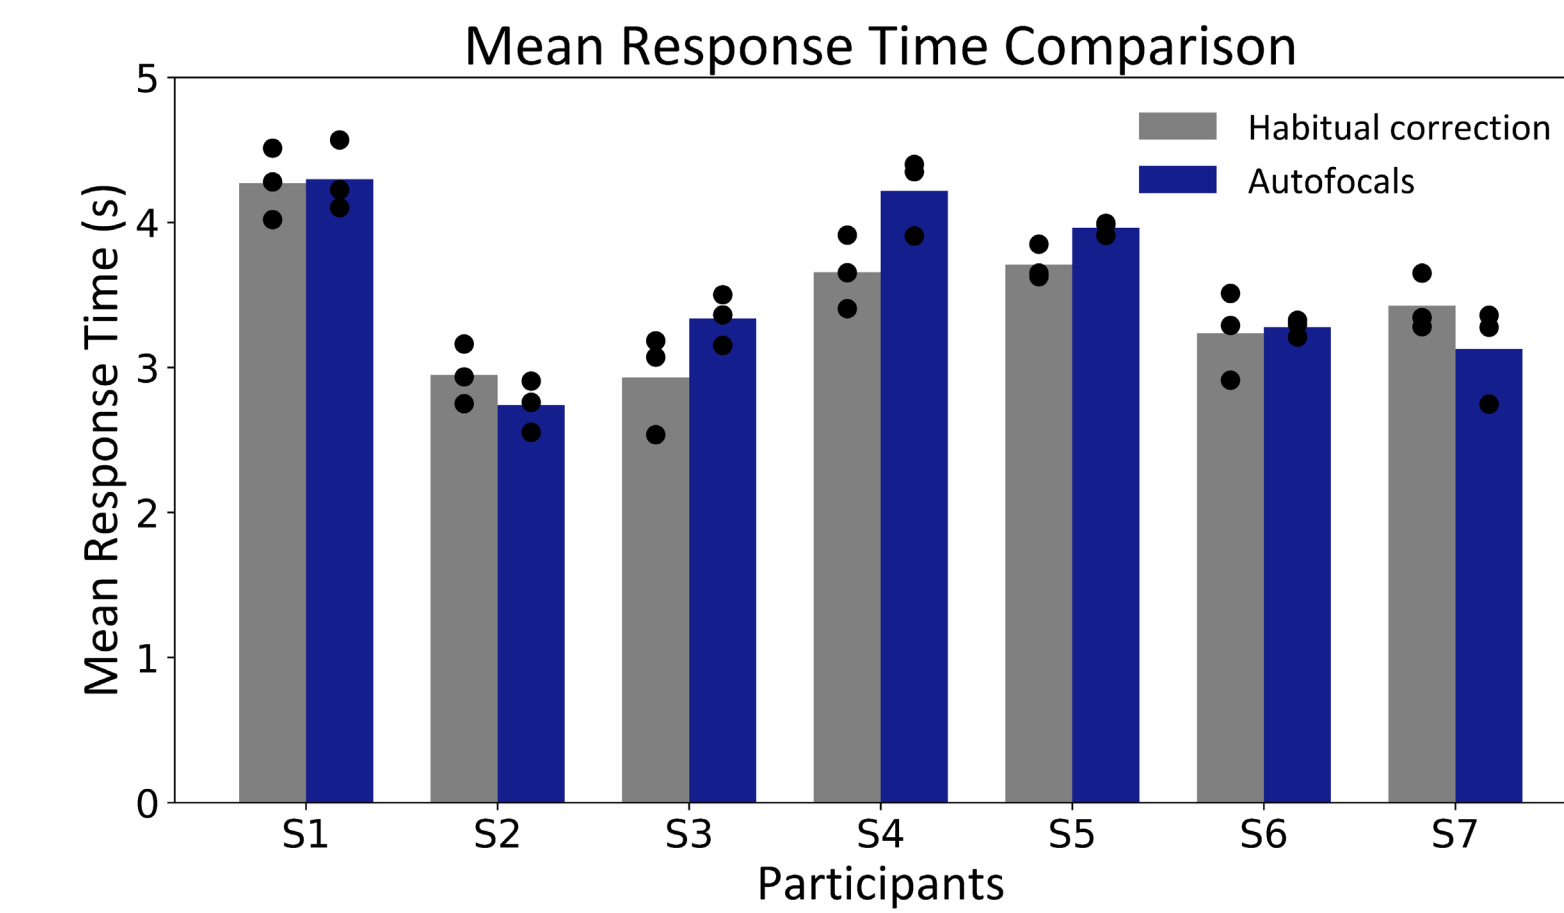

- Fixations were detected in real-time using dispersion-based method from Pupil Labs.
- Inter-participant differences were observed in fixation counts over surfaces.

Conclusion

The results of this study demonstrates that the participants performed the task with multiple focus distances, similarly with their habitual correction and the developed autofocals.

Thus, it can be concluded that our fixation-based feedback system is feasible for presbyopia correction with focus tunable lenses.

References

1. Nitish Padmanaban, Robert Konrad, and Gordon Wetzstein. 2019. Autofocals: Evaluating gaze-contingent eyeglasses for presbyopes. Science advances 5, 6 (2019).
2. Juan Mompeán, Juan L Aragón, and Pablo Artal. 2020. Portable device for presbyopia correction with optoelectronic lenses driven by pupil response. Scientific Reports 10, 1 (2020), 1–9.