

ContiLNN: Mitigating Slice Sampling Discontinuity with Liquid Neural Networks for Medical Image Restoration

Jialei He^{a,b,1}, Enhe Liu^{a,b,1}, Sifan Song^b, Pengfei Jin^c, Jionglong Su^b, Hongbin Wang^a, Zhixiang Lu^b, Yanhao Huang^{a,b}, Anteng Cai^{a,b}, Zhengyong Jiang^b, Jiaman Ding^{a,*}, S. Kevin Zhou^{d,*}, Jinfeng Wang^{a,*}

^aFaculty of Information Engineering and Automation, Kunming University of Science and Technology, Kunming, Yunnan, 650504, China

^bAcademy of Artificial Intelligence and Advanced Technology, Xi'an Jiaotong-Liverpool University, Suzhou, Jiangsu, 215123, China

^cDepartment of Radiology, Massachusetts General Hospital and Harvard Medical School, Boston, Massachusetts, 02115, United States

^dSchool of BME & Suzhou Institute for Advanced Research, Center for Medical Imaging, Robotics, Analytic Computing & Learning (MIRACLE), University of Science and Technology of China, Suzhou, Jiangsu, 215000, China

Abstract

Anatomical continuity provides complementary information for medical image restoration, yet exploiting neighboring slices requires accounting for both local anatomy and variations in slice sampling. We introduce ContiLNN, which augments two-dimensional restoration networks with bidirectional closed-form continuous-time (Bi-CfC) modules to model cross-slice context through liquid neural dynamics while retaining in-plane feature extraction. Slice-index intervals modulate gates determined by local features and hidden states, allowing propagation to respond to sampling variations and anatomical context. Closed-form updates avoid iterative numerical integration. Alongside reconstruction supervision, cross-slice consistency aligns first- and second-order intensity differences with high-quality references to preserve anatomical variation. Distillation from a frozen two-dimensional backbone helps retain in-plane fidelity. Across five training seeds, ContiLNN improves mean peak signal-to-noise ratio (PSNR) by 0.1907, 1.0176 and 1.2482 dB over the two-dimensional baseline for CT denoising, MRI super-resolution and reduced-count PET restoration, respectively, while reducing root mean squared error in all three tasks. On the held-out CT patient, PSNR improves consistently, with a standard deviation of 0.0026 dB across seeds; gains are greater for MRI and PET. PET ablations support ordered propagation beyond additional pointwise capacity. Under contiguous training, Bi-CfC achieves higher fidelity than a bidirectional gated recurrent unit (Bi-GRU) with similar parameter counts and arithmetic costs across all tested sampling conditions, with lower measured latency and memory use. We also investigate the performance of both operators under sparse and irregular context using mixed-gap training. Experiments with fewer training patients and a second backbone further support data efficiency and backbone compatibility.

Keywords: Medical image restoration, 2.5D restoration, Liquid neural networks, Slice-axis modeling

1. Introduction

Medical image restoration seeks to recover anatomical information from acquisitions constrained by radiation dose, scan duration or signal availability. Lower-dose CT reduces radiation exposure at the cost of increased noise (McCollough et al., 2017; Moen et al., 2021). In MRI, higher spatial resolution competes with acquisition time and signal-to-noise ratio, motivating super-resolution methods that recover structural detail from lower-resolution observations (Chatterjee et al., 2024). In PET, lower administered tracer activity can reduce radiation exposure, and shorter acquisitions can reduce scan burden; both reduce detected counts, increasing noise and making local uptake differences harder to distinguish (Jang et al., 2024; Luo et al., 2022). These tasks estimate high-quality (HQ) images from low-quality (LQ) inputs. Advances in convolutional,

Transformer and state-space networks have substantially improved in-plane recovery, providing efficient backbones for a range of medical restoration tasks (Zamir et al., 2022; Yang et al., 2026a; Chan et al., 2026; Yang et al., 2024; Chen et al., 2026; Yang et al., 2026b).

The anatomical evidence in a volume extends beyond any individual slice. Adjacent images sample structures that evolve along the slice axis, yet independent two-dimensional (2D) processing does not explicitly retain this ordered relationship (Fig. 1A). The imbalance between in-plane and through-plane information is a recognized challenge in volumetric medical image modeling (Dong et al., 2022).

A relevant clinical application arises when only a subset of slices from an existing image series is available for retrospective restoration. The available slices may be regularly or irregularly spaced in the original index sequence, so adjacent inputs need not correspond to consecutive slices in the source series. Their original indices preserve this distinction. This setting motivates cross-slice feature propagation that uses neighboring anatomy while accounting for the index gaps between available

*Corresponding authors.

Email address: Jf.Jacob.Wang@gmail.com (Jinfeng Wang)

¹Jialei He and Enhe Liu contributed equally to this work.

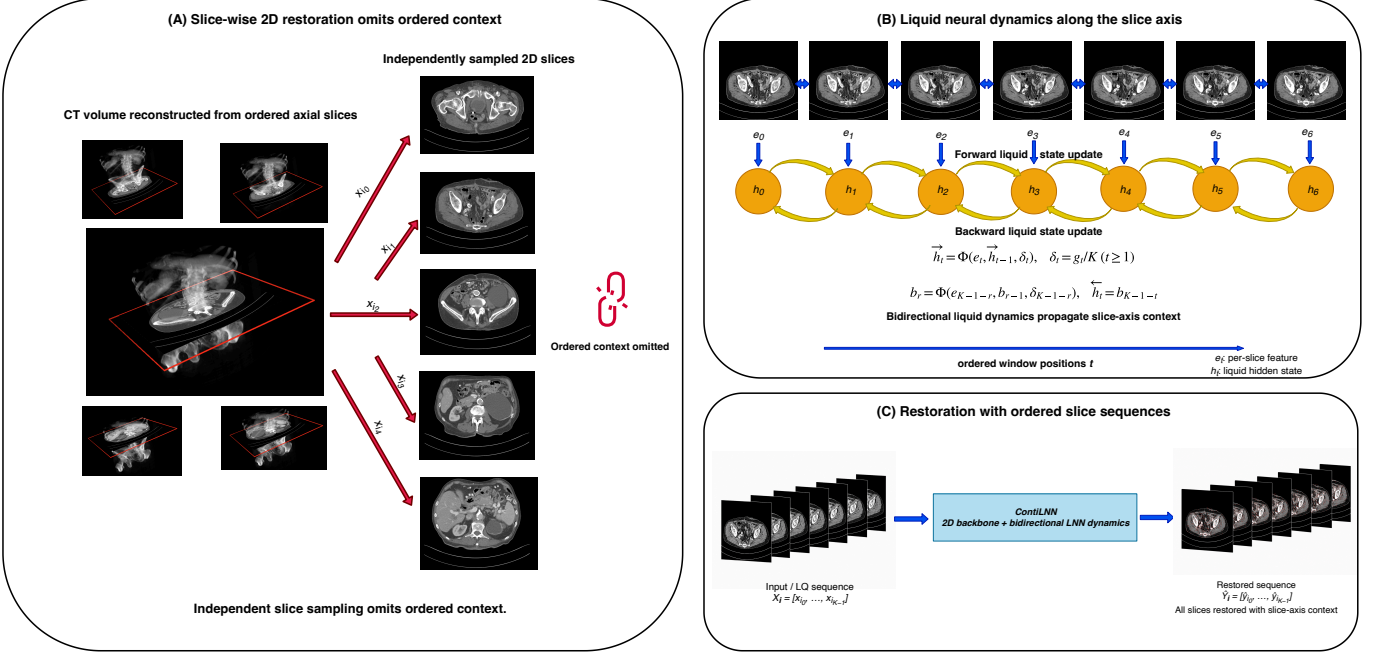


Figure 1: Ordered-slice restoration with ContiLNN. (A) Independent 2D processing. (B) Bidirectional liquid propagation. (C) One restored output per observed slice. Original slice indices i_t identify the K inputs x_{i_t} and outputs $\hat{y}_{i_t}$; t denotes window position. The direction-specific closed-form continuous-time (CfC) update Φ propagates states h_t using features e_t and normalized intervals δ_t derived from gaps g_t . The backward traversal state b_t is realigned to the original order; interval conventions and alignment are defined in Eqs. 4 and 10.

observations, with a restored output retained at each supplied position.

Local 2.5D modeling combines in-plane feature extraction with information from neighboring slices. Three-dimensional (3D) restoration networks instead model context through volumetric feature maps, as in convolutional models for MRI super-resolution (Chatterjee et al., 2024) and Spach Transformer for PET denoising (Jang et al., 2024). Storage for these feature maps scales with their spatial extent and channel width. Neighboring CT slices have also been incorporated into convolutional encoder-decoders (Shan et al., 2018). Adjacent-slice supervision and multi-view inference provide further ways to use through-plane information (Zhang et al., 2021; Chen et al., 2025). These approaches establish several roles for local anatomical context. ContiLNN represents this context as an evolving sequence of feature states, with an explicit slice-index interval and a restored output at every supplied position.

Liquid neural networks provide a continuous-time model of input-dependent state evolution (Hasani et al., 2021). Closed-form continuous-time networks (CfCs) approximate this evolution through interval-dependent updates without repeated numerical integration (Hasani et al., 2022). Their explicit interval input is particularly relevant when the separation between observations varies. For medical image restoration, we propagate states in slice order and condition each update on a normalized slice-index interval. Forward and backward states then communicate information between preceding and following observations (Fig. 1B). This links the anatomical ordering of the input to the dynamics used to refine its features.

Here we introduce ContiLNN, which augments 2D restora-

tion backbones with bidirectional liquid dynamics along the slice axis. Each local sequence retains the correspondence between its input slices and restored outputs (Fig. 1C). Bidirectional CfC (Bi-CfC) modules propagate context at selected levels of the feature hierarchy, while two complementary regularizers guide the resulting images: cross-slice consistency preserves first- and second-order intensity changes in the HQ sequence, and distillation from a frozen 2D backbone retains agreement with its in-plane estimates. We develop this design on Restore-RWKV (Yang et al., 2026a) and apply it to DAS-Mamba (Chan et al., 2026) to examine compatibility with a second backbone.

Our contributions are threefold:

1. **Liquid dynamics for medical image restoration.** We introduce ContiLNN to propagate anatomical information across ordered slices through bidirectional liquid dynamics. Slice-index intervals condition the closed-form updates, allowing state propagation to respond to sampling changes.
2. **Augmentation of 2D restoration backbones.** Bi-CfC modules refine selected feature pathways while retaining the backbone’s in-plane blocks. Cross-slice intensity consistency and 2D backbone distillation jointly preserve reference anatomical variation and in-plane fidelity.
3. **Evaluation across modalities and sampling settings.** CT, MRI and PET experiments assess restoration quality. Case-level analyses, comparisons of two operators under regular, sparse and irregular sampling, limited-patient training, backbone studies and ablations assess sampling adaptation, data efficiency and backbone compatibility.

2. Related work

2.1. Medical image restoration

Learning-based restoration has progressed from local residual prediction to efficient modeling of long-range image structure. Convolutional restoration networks learn local image priors from paired images or neighboring observations (Shan et al., 2018; Zhang et al., 2021). Transformer models extend the spatial reach of these representations through attention, improving the recovery of fine structures and long-range dependencies (Liang et al., 2021; Zamir et al., 2022). RWKV combines recurrent inference with parallelizable training, and its visual adaptations provide another route to efficient spatial modeling (Peng et al., 2023; Duan et al., 2025). MambaIR, DenoMamba, CT-Mamba, Restore-RWKV and DASMamba apply state-space or recurrent-style representations to natural and medical image restoration (Gu and Dao, 2024; Guo et al., 2025; Öztürk et al., 2026; Li et al., 2025; Yang et al., 2026a; Chan et al., 2026). These methods supply the in-plane feature hierarchies on which ContiLNN builds. Whereas our previous work FedFTN (Zhou et al., 2023) addresses institutional heterogeneity through personalized federated learning for low-count PET denoising, ContiLNN models cross-slice anatomical context through interval-conditioned bidirectional liquid dynamics for CT, MRI, and PET restoration.

2.2. Slice-axis context

The choice of spatial representation determines how neighboring slices contribute to a prediction. Slice-wise networks are compatible with high-resolution images, whereas volumetric networks directly couple in-plane and through-plane structure. Anisotropic sampling complicates this balance because a fixed number of neighboring slices can span substantially different anatomical extents (Dong et al., 2022). Consequently, slice count alone does not describe the context available to a model; the sampling intervals also matter.

Restoration methods use through-plane information in several distinct ways. Hybrid 2D/3D convolution can aggregate neighboring CT slices for center-slice denoising (Shan et al., 2018), while volumetric MRI networks learn features across all three spatial axes for super-resolution (Chatterjee et al., 2024). Other approaches use adjacent slices as training supervision or combine predictions from multiple views (Zhang et al., 2021; Chen et al., 2025). Slice-based reconstruction addresses a related problem by recovering volumes or anatomical surfaces from sparse observations (Xu et al., 2023; Xiao et al., 2025). ContiLNN maintains an ordered feature sequence and restores every supplied slice. Its interval inputs are derived from the original index gaps between selected observations, allowing feature updates to respond to both local image content and the sampling of neighboring context.

2.3. Liquid neural dynamics

Continuous-time models describe how a hidden representation evolves between observations. Neural ordinary differential equations (ODEs) express this evolution through a learned

vector field (Chen et al., 2018), while latent ODE models provide continuous-time latent representations for irregularly observed sequences (Rubanova et al., 2019). Liquid time-constant networks introduce input-dependent dynamics, allowing the effective transition to vary with the observation (Hasani et al., 2021). CfCs approximate these dynamics with closed-form updates that retain an explicit dependence on the supplied interval (Hasani et al., 2022).

This dependence offers a useful connection between continuous-time modeling and slice sampling. An update can respond to a larger index gap without treating it as the same transition as two consecutive slices. ContiLNN applies this principle to dense features at corresponding in-plane locations, with two directions of propagation supplying complementary anatomical context. We evaluate Bi-CfC across sparse and irregular neighboring contexts after contiguous training, and investigate mixed-gap training separately as a way to broaden exposure to sampling variations.

2.4. Consistency and distillation

Consistency regularization encourages agreement under input or model perturbations (Tarvainen and Valpola, 2017; Laine and Aila, 2017), while knowledge distillation transfers information through predictions from a reference model (Hinton et al., 2015). In restoration, these constraints complement direct fidelity to the reference image. For an ordered slice sequence, neighboring reference images need not have identical intensities: anatomical boundaries and uptake patterns can change substantially with position. We therefore match the first- and second-order differences of restored and reference sequences. A separate 2D backbone distillation term encourages agreement with predictions from a frozen, pretrained 2D backbone. These two forms of regularization preserve useful in-plane estimates while learning the additional information supplied by neighboring slices.

3. Method

3.1. Ordered-slice restoration

ContiLNN restores a local sequence of observed slices while preserving their positional correspondence. Let $X = \{x_i\}_{i=1}^N$ denote an LQ volume with N ordered slices and $Y = \{y_i\}_{i=1}^N$ its HQ reference. A local window contains $K \leq T$ slices, where T is the maximum window length. Its increasing original indices are $i = (i_0, \dots, i_{K-1})$, and its paired input and reference sequences are

$$\begin{aligned} X_i &= [x_{i_0}, \dots, x_{i_{K-1}}], \\ Y_i &= [y_{i_0}, \dots, y_{i_{K-1}}]. \end{aligned} \quad (1)$$

The model learns $\mathcal{F}_\theta : X_i \mapsto \widehat{Y}_i$, where θ denotes its trainable parameters and $\widehat{Y}_i = [\widehat{y}_{i_0}, \dots, \widehat{y}_{i_{K-1}}]$ contains one restored image for each input position. Every output receives direct supervision from the corresponding HQ slice.

The slice-index gap specifies the sampling interval between consecutive observations in the window:

$$g_t = i_t - i_{t-1}, \quad t = 1, \dots, K-1. \quad (2)$$

Fixed gaps of one, two and three select consecutive slices, every second slice and every third slice, respectively. Indices are retained from the source series before slice selection rather than reassigned consecutively afterwards. For example, available slices with indices [1, 3, 5, 7] have successive gaps (2, 2, 2), whereas indices [1, 2, 3, 5, 6] give gaps (1, 1, 2, 1). These gaps describe the separation between available observations in the original index sequence. ContiLNN restores each supplied slice at its corresponding position.

3.2. Bidirectional liquid dynamics

The bidirectional closed-form continuous-time module, denoted Bi-CfC, is the slice-axis operator of ContiLNN (Fig. 2B). Its hidden state propagates over ordered slice features, with an explicit interval input associated with each observation. The continuous-time formulation motivating this operator represents state evolution as

$$\frac{dh^l(q)}{dq} = G_\theta^l(h^l(q), e^l(q)), \quad (3)$$

where q is a continuous evolution coordinate, l indexes a feature level, h^l is its hidden state, e^l is the input feature and G_θ^l is a learned vector field. CfC develops interval-dependent neural transitions from an approximate closed-form treatment of liquid dynamics (Hasani et al., 2022). Based on this approximation, we use the default gated CfC parameterization to evaluate the state directly from the current feature, incoming state and supplied interval, without a numerical ODE solver.

We distinguish position within a window from the interval supplied to the dynamics. The index gaps are normalized by the actual number of observations K to obtain the interval inputs defined below. For $K > 1$, the within-window position and interval input are

$$p_t = \frac{t}{K-1}, \quad \delta_t = \begin{cases} g_1/K, & t = 0, \\ g_t/K, & t = 1, \dots, K-1. \end{cases} \quad (4)$$

The normalization uses the actual number of observations K , including short windows. Under fixed-gap sampling, every observation receives g/K ; contiguous input gives $1/K$. The position p_t specifies relative order, whereas δ_t supplies the slice-index interval attached to the current observation. Both branches preserve this feature–interval pairing. The single-slice boundary convention is specified in Supplementary Section A.

At each in-plane location, let $f_t^l \in \mathbb{R}^{C_l}$ be the channel vector of slice i_t , where C_l is the feature width. A learned affine position projection P_{pos}^l gives

$$e_t^l = f_t^l + P_{\text{pos}}^l(p_t). \quad (5)$$

The embedded feature e_t^l retains the original observation’s within-window position in both traversal directions. The resulting feature and interval are supplied together to the directional cell.

The cell first forms a joint representation of the current feature and incoming state. For one feature level and direction,

suppress the superscripts and write $C = C_l$ and $M = M_l$, where M_l is the width of the cell’s internal feature network. With $e_t, h_{t-1} \in \mathbb{R}^C$, the joint representation and candidate states are

$$z_t = \rho(W_z[e_t; h_{t-1}] + v_z), \quad (6)$$

$$c_t^{(j)} = \tanh(W_j z_t + v_j), \quad j \in \{1, 2\}.$$

Here $[\cdot; \cdot]$ denotes channel concatenation, $W_z \in \mathbb{R}^{M \times 2C}$ and $v_z \in \mathbb{R}^M$ are learned parameters, and ρ is the scaled hyperbolic-tangent activation specified in Supplementary Section A. Thus, $z_t \in \mathbb{R}^M$ combines present image content with the recurrent context. Each candidate head has weights $W_j \in \mathbb{R}^{C \times M}$ and bias $v_j \in \mathbb{R}^C$, producing $c_t^{(j)} \in (-1, 1)^C$. The internal width M is distinct from the recurrent-state width C .

Two further affine heads determine how the supplied interval modulates the mixture:

$$\eta_t = Q_a(z_t) = W_a z_t + v_a, \quad (7)$$

$$\xi_t = Q_b(z_t) = W_b z_t + v_b,$$

$$\alpha_t = \sigma(\delta_t \eta_t + \xi_t).$$

The matrices $W_a, W_b \in \mathbb{R}^{C \times M}$ and biases $v_a, v_b \in \mathbb{R}^C$ are learned independently of the candidate heads. The vectors η_t and ξ_t are the interval coefficient and intercept, respectively; the scalar δ_t is broadcast across channels. The elementwise sigmoid σ yields $\alpha_t \in (0, 1)^C$. Because the affine coefficient η_t can take either sign, different feature channels can respond differently to a larger interval.

The updated state is a channelwise convex combination of the two candidates:

$$h_t = (1 - \alpha_t) \odot c_t^{(1)} + \alpha_t \odot c_t^{(2)} \quad (8)$$

$$= c_t^{(1)} + \alpha_t \odot (c_t^{(2)} - c_t^{(1)}).$$

Here $\odot$ denotes the elementwise product. Each state channel lies between its two candidate values, keeping the directional hidden state in $(-1, 1)^C$ before the subsequent affine feature projection. We denote the complete transition in Eqs. 6–8 by $\Phi_\theta(e_t, h_{t-1}, \delta_t)$. Both candidates depend on h_{t-1} , allowing the update to retain information from previously visited observations.

The gate provides an explicit, content-dependent response to sampling. Holding the incoming feature e_t and state h_{t-1} fixed gives

$$\frac{\partial h_t}{\partial \delta_t} = \alpha_t \odot (1 - \alpha_t) \odot \eta_t \odot (c_t^{(2)} - c_t^{(1)}), \quad (9)$$

$$\left| \frac{\partial h_t}{\partial \delta_t} \right| \leq \frac{1}{4} |\eta_t| \odot |c_t^{(2)} - c_t^{(1)}|.$$

Absolute values and the inequality are elementwise. The derivative isolates the direct response to the interval from changes carried through the recurrent state: its sign and magnitude depend on the learned coefficient, gate and candidate separation. The model therefore adapts its state update to the supplied sampling interval and local features while retaining algebraic evaluation of each transition.

Independent forward and backward cells apply this transition to the ordered sequence. Let $r = 0, \dots, K-1$ index backward

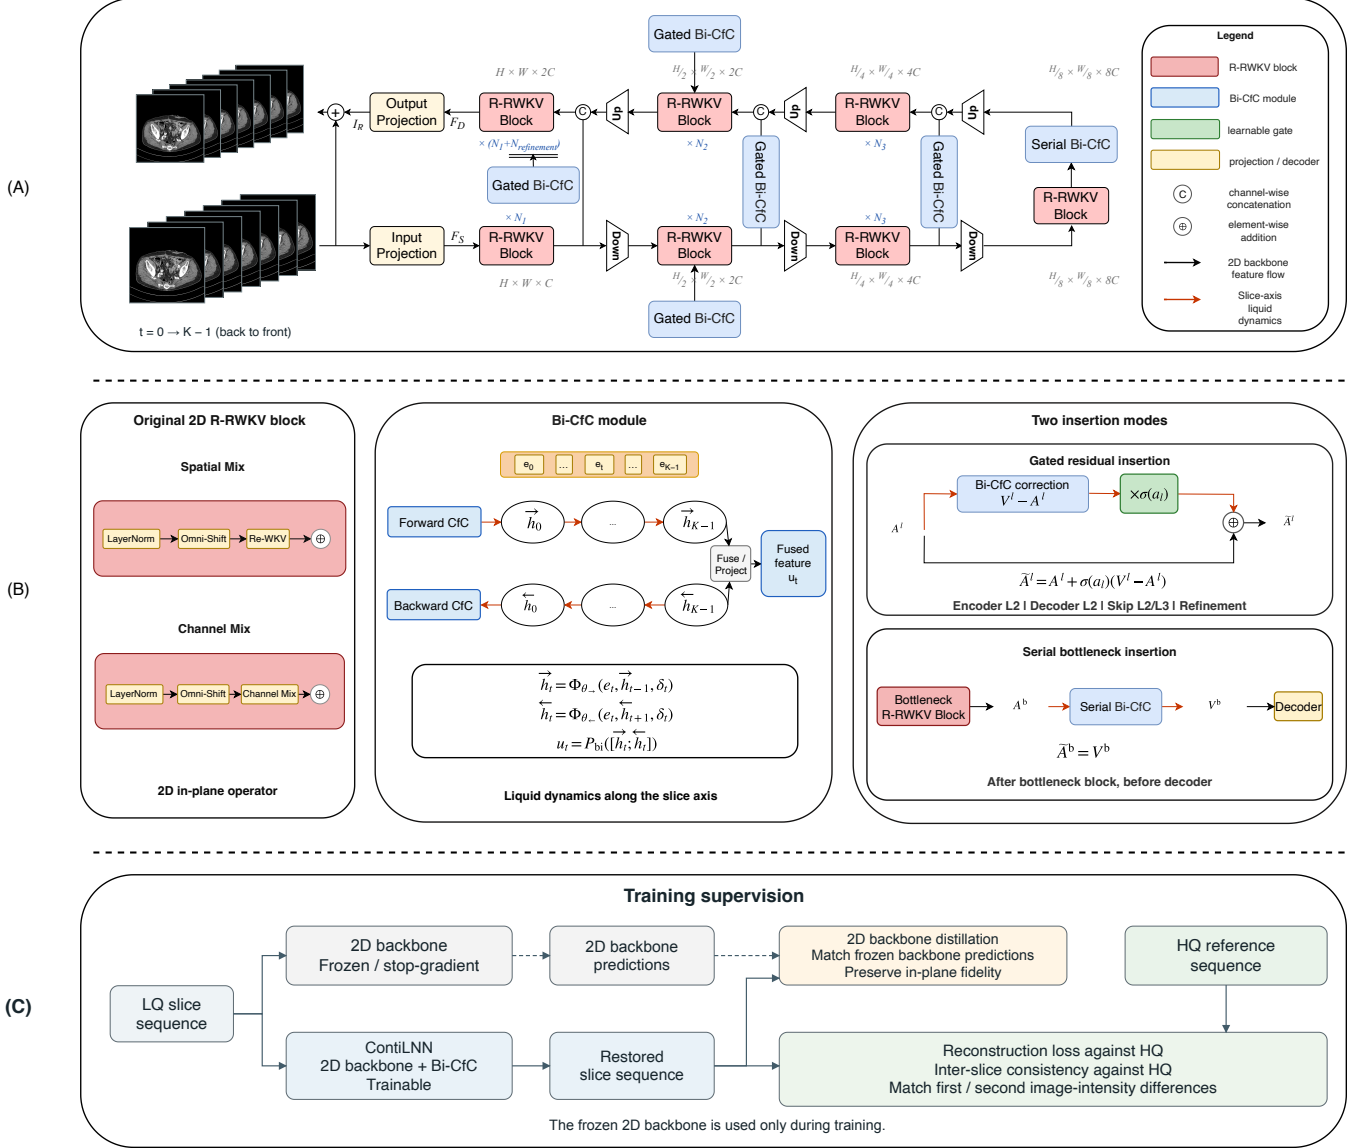


Figure 2: ContilLNN architecture based on Restore-RWKV (Yang et al., 2026a). (A) Bi-CfC modules augment selected feature pathways; the paired CT sequences show the same seven observed positions, ordered back to front. (B) Backbone blocks, the bidirectional liquid operator, and gated residual or serial insertion. Reverse traversal preserves feature–interval pairing (Eq. 10). (C) Training supervision. High-quality references supervise reconstruction and first- and second-order inter-slice intensity differences. A frozen 2D backbone supplies single-slice predictions for distillation during training; the ContilLNN backbone and Bi-CfC modules remain trainable.

traversal, and let b_r^l be its recurrent state. The recurrences and alignment to the original positions are

$$\begin{aligned} \vec{h}_t^l &= \Phi_{\theta_{\rightarrow}}^l(e_t^l, \vec{h}_{t-1}^l, \delta_t^l), \\ b_r^l &= \Phi_{\theta_{\leftarrow}}^l(e_{K-1-r}^l, b_{r-1}^l, \delta_{K-1-r}^l), \\ \overleftarrow{h}_t^l &= b_{K-1-t}^l. \end{aligned} \quad (10)$$

Here $\theta_{\rightarrow}$ and $\theta_{\leftarrow}$ are separate parameter sets for the same cell architecture, with initial states $\vec{h}_{-1}^l = b_{-1}^l = 0$. Reversing the feature–interval pairs preserves e_t^l and δ_t^l at original position t . For irregular inputs, δ_t^l is a sampling descriptor associated with observation t ; the index separation to position $t+1$ would instead correspond to δ_{t+1}^l . The implemented backward branch

retains the observation-specific descriptor. An example of this pairing is provided in Supplementary Section A.

An affine projection fuses the two states aligned at each original position:

$$\begin{aligned} u_t^l &= P_{bi}^l([\vec{h}_t^l; \overleftarrow{h}_t^l]) \\ &= W_{bi}^l[\vec{h}_t^l; \overleftarrow{h}_t^l] + v_{bi}^l. \end{aligned} \quad (11)$$

The learned weights $W_{bi}^l \in \mathbb{R}^{C_l \times 2C_l}$ and bias $v_{bi}^l \in \mathbb{R}^{C_l}$ return a refined vector $u_t^l \in \mathbb{R}^{C_l}$. Each output thus combines preceding and following observations at the same slice position before being returned to the backbone’s feature layout.

3.3. Backbone augmentation

Bi-CfC acts on slice sequences extracted from an otherwise two-dimensional feature hierarchy. The R-RWKV block is the original in-plane building block of Restore-RWKV: its omnidirectional token shift (Omni-Shift) aggregates local spatial information, and its recurrent WKV attention (Re-WKV) models longer-range dependencies across in-plane scan directions (Yang et al., 2026a). ContiLNN retains these operations and adds Bi-CfC at selected feature pathways (Fig. 2A,B). For a batch of B windows, let A^l be the backbone feature tensor with spatial dimensions $H_l \times W_l$. A rearrangement $\mathcal{R}_l$ exposes the ordered channel vectors at each spatial location:

$$\begin{aligned} A^l &\in \mathbb{R}^{BK \times C_l \times H_l \times W_l} \xrightarrow{\mathcal{R}_l} F^l \in \mathbb{R}^{BH_l W_l \times K \times C_l}, \\ U^l &= \Psi_l(F^l, \delta), \quad V^l = \mathcal{R}_l^{-1}(U^l). \end{aligned} \quad (12)$$

Here U^l is the processed feature sequence and V^l its restored 2D layout. The rearrangement separates the batch and slice dimensions before grouping the batch and spatial locations. The operator Ψ_l applies the position embedding, bidirectional updates and fusion in Eqs. 5–11; δ contains the K interval inputs. The same operator is shared across in-plane locations, and $\mathcal{R}_l^{-1}$ restores the original tensor layout.

The two insertion modes have complementary roles. Serial insertion introduces sequence information at the bottleneck before decoding; gated residual insertion learns the correction strength along the remaining selected pathways (Fig. 2B):

$$\tilde{A}^l = \begin{cases} V^l, & l \in \mathcal{S}_b, \\ A^l + \sigma(a_l)(V^l - A^l), & l \in \mathcal{S}_g, \\ A^l, & l \notin \mathcal{S}_b \cup \mathcal{S}_g. \end{cases} \quad (13)$$

Here $\mathcal{S}_b$ and $\mathcal{S}_g$ identify the bottleneck and gated pathways, a_l is a learnable scalar gate logit, and σ is the sigmoid function. Subsequent backbone blocks process $\tilde{A}^l$ in their original 2D layout.

Restore-RWKV supplies the principal backbone, with Bi-CfC augmenting its intermediate encoder and decoder blocks, selected skips, bottleneck and late refinement pathway. The same insertion roles are applied to DASMamba to examine backbone compatibility. Supplementary Section A reports the representative Restore-RWKV topology and module settings. This design enables slice-axis modeling within existing feature hierarchies while keeping sequence propagation local to one patient or scan.

The selected pathways address different stages of restoration. Intermediate encoder and decoder features provide reduced-resolution representations that retain local structure for cross-slice exchange. Skip-path modules carry this context from encoding to decoding, while serial bottleneck processing makes the deepest representation sequence-aware before upsampling. The late refinement pathway supplies a final contextual correction. Gates regulate the contribution of the transformed sequence features along the remaining pathways, allowing their strength to be learned jointly with the in-plane backbone.

3.4. Training objective

The training objective combines reconstruction, cross-slice consistency and 2D backbone distillation (Fig. 2C). ContiLNN restores each input sequence, while a frozen copy of the pre-trained 2D backbone processes the same slices independently to provide distillation targets. Paired HQ images supervise reconstruction and cross-slice intensity differences; the frozen backbone predictions guide preservation of in-plane fidelity. Gradients update the ContiLNN backbone and Bi-CfC modules, but do not pass through the frozen backbone, which is used only during training. The resulting objective is

$$\mathcal{L} = \mathcal{L}_{\text{rec}} + \lambda_{\text{cons}} \mathcal{L}_{\text{cons}} + \lambda_{\text{KD}} \mathcal{L}_{\text{KD}}, \quad (14)$$

where λ_{cons} and λ_{KD} weight cross-slice consistency and 2D backbone distillation. For the Restore-RWKV backbone,

$$\begin{aligned} \mathcal{L}_{\text{rec}} &= \frac{1}{K} \sum_{t=0}^{K-1} \|\widehat{y}_{i_t} - y_{i_t}\|_1, \\ \mathcal{L}_{\text{KD}} &= \frac{1}{K} \sum_{t=0}^{K-1} \|\widehat{y}_{i_t} - \bar{y}_{i_t}\|_1, \end{aligned} \quad (15)$$

where $\|\cdot\|_1$ denotes mean absolute error over image pixels and $\bar{y}_{i_t}$ is the prediction of the frozen 2D backbone for x_{i_t} . The ContiLNN backbone and Bi-CfC parameters remain trainable. For DASMamba, its native reconstruction penalties are retained within $\mathcal{L}_{\text{rec}}$, while the remaining workflow follows ContiLNN-RWKV.

Cross-slice consistency follows anatomical change in the reference sequence. Define the first and second finite differences as

$$\begin{aligned} D_1 y_t &= y_{i_{t+1}} - y_{i_t}, \\ D_2 y_t &= y_{i_{t+1}} - 2y_{i_t} + y_{i_{t-1}}, \end{aligned} \quad (16)$$

with identical definitions for predictions. The consistency objective is

$$\begin{aligned} \mathcal{L}_{\text{cons}} &= \mathcal{L}_{\text{cons}}^{(1)} + \beta_2 \mathcal{L}_{\text{cons}}^{(2)}, \\ \mathcal{L}_{\text{cons}}^{(1)} &= \frac{1}{K-1} \sum_{t=0}^{K-2} \|D_1 \widehat{y}_t - D_1 y_t\|_1, \\ \mathcal{L}_{\text{cons}}^{(2)} &= \frac{1}{K-2} \sum_{t=1}^{K-2} \|D_2 \widehat{y}_t - D_2 y_t\|_1, \end{aligned} \quad (17)$$

where β_2 weights second-order changes. The corresponding term is zero when a short window contains too few slices to evaluate its difference. These are finite differences over the observed sequence, including any index gaps. The first-order term matches the intensity change between successive observations; the second-order term matches how this change varies across the local sequence. Equivalently, defining the restoration error as $r_t = \widehat{y}_{i_t} - y_{i_t}$ gives

$$\begin{aligned} D_1 \widehat{y}_t - D_1 y_t &= D_1 r_t, \\ D_2 \widehat{y}_t - D_2 y_t &= D_2 r_t. \end{aligned} \quad (18)$$

The penalties thus constrain inter-slice variation in restoration error while retaining the anatomical changes encoded by the

reference. Reconstruction anchors the absolute intensity of each output, and distillation retains agreement with the pre-trained in-plane estimate. Numerical weights are listed in Supplementary Section A.

3.5. Inference

Restoration covers the full set of observed slices through local, case-specific windows. Training retains short terminal windows, and inference combines predictions from overlapping window tilings. For slice i , let $\mathcal{W}(i)$ be the set of windows that contain it and $\hat{y}_i^{(w)}$ the prediction from window w . The fused output is

$$\hat{y}_i = \frac{1}{|\mathcal{W}(i)|} \sum_{w \in \mathcal{W}(i)} \hat{y}_i^{(w)}. \quad (19)$$

Here $|\mathcal{W}(i)|$ is the number of windows covering slice i . Outputs are returned to their original slice order. The tilings retain every eligible real slice, and each hidden state is initialized within its own window. The window length and tiling offsets are specified in Supplementary Section A. Sparse and irregular context use the same position-aligned output principle, allowing the sampling experiments to change contextual support while retaining the evaluated images.

4. Experiments

4.1. Datasets

We evaluate anatomical restoration across three modalities with distinct degradations: CT denoising, MRI super-resolution and reduced-count PET restoration. The case-disjoint partitions and preprocessing follow the established restoration benchmarks (Yang et al., 2026a; Chan et al., 2026). Low-quality (LQ) and high-quality (HQ) images denote the degraded input and paired reference, respectively.

The CT benchmark derives from the ten-patient training set released for the American Association of Physicists in Medicine (AAPM) Low Dose CT Grand Challenge, which provides paired quarter-dose and normal-dose images (McCollough et al., 2017). The training, validation and test partitions contain eight, one and one patients, respectively, with 2,039, 128 and 211 slices. Quarter-dose images serve as inputs and normal-dose images as references.

For MRI, we use T2-weighted images from IXI (IXI Project, n.d.). The source allocation is 405/59/114 subjects for training/validation/testing, yielding 40,500/5,828/11,400 available slices; the validation reader supplies 58 readable subjects, as detailed in Supplementary Section A. LQ images are reconstructed after retaining the central 6.25% of two-dimensional k-space, corresponding to four-fold degradation along each in-plane axis. The slice-axis sampling is retained in this super-resolution task.

The PET cohort comprises 159 scans acquired with a PolarStar m660 system, originating from the dataset described by Yang et al. (2024). The training, validation and test partitions contain 120, ten and 29 scans, respectively. After exclusion of air-only slices, these partitions contain 8,350/684/2,044 paired

images. Reduced-count inputs are generated from list-mode data with a reduction factor of 12. Modality-specific intensity normalization and evaluation windows are specified in Supplementary Section A.

4.2. Experimental setup

We reproduce the 2D backbones using their released training procedures and initialize ContiLNN from the checkpoint with the highest validation score. A frozen copy of the corresponding backbone supplies predictions for 2D backbone distillation, while the ContiLNN backbone and Bi-CfC modules are trained jointly. As illustrated in Fig. 2, the architecture augments in-plane feature extraction with slice-axis propagation and uses the frozen backbone only to guide training. Contiguous slice windows are used for the principal restoration results in Table 1 and the operator comparisons in Tables 2 and 5; mixed-gap training is investigated separately in Supplementary Section H. The representative ContiLNN-RWKV optimization settings, window configurations and loss weights are collected in Supplementary Section A, together with the common workflow used for DAS-Mamba.

Restoration quality is measured using peak signal-to-noise ratio (PSNR), the structural similarity index measure (SSIM) (Wang et al., 2004), and root mean squared error (RMSE). Metrics are calculated in the modality’s restored intensity scale, averaged within each patient or scan, and then averaged across cases with equal weight. ContiLNN estimates in Table 1 are means and sample standard deviations (SDs) across five training seeds. Case-level statistical analyses are presented separately below. CT results describe the single held-out patient in its benchmark partition.

4.3. Quantitative results

Ordered slice-axis modeling improves fidelity across the three evaluated restoration tasks (Table 1). Relative to Restore-RWKV, mean PSNR increases by 0.1907, 1.0176 and 1.2482 dB on CT, MRI and PET, respectively, accompanied by higher SSIM and lower RMSE. The agreement across these metrics connects the use of neighboring anatomy with improved intensity accuracy and structural fidelity. On the held-out CT patient, the improvement is consistent across training seeds, with a PSNR SD of 0.0026 dB.

The improvements persist across the observed seed variation. Every ContiLNN-RWKV training seed yields higher PSNR and SSIM and lower RMSE than the baseline in each modality. At one SD below the mean, PSNR remains 0.19, 0.99 and 1.15 dB above the baseline for CT, MRI and PET, respectively. This separation indicates that the benefit of neighboring anatomical context is maintained across the evaluated initializations.

Integration with DASMamba supports the use of slice-axis dynamics with a second in-plane representation. Mean PSNR increases by 0.1934, 0.3604 and 1.1264 dB on CT, MRI and PET, respectively, with corresponding RMSE reductions of 0.1817, 1.0886 and 0.0095 (Table 1). PET also improves in SSIM, while the CT and MRI SSIM estimates are lower than those of their DASMamba baselines by 0.0051 and 0.0050,

Table 1: Restoration results for MRI super-resolution, CT denoising and reduced-count PET restoration. Published reference results in the upper and lower blocks follow the Restore-RWKV and DASMamba studies, respectively (Yang et al., 2026a; Chan et al., 2026); the upper published block uses joint training across the three modalities. In the lower published block, * marks methods re-implemented by the DASMamba authors. Each block ends with the corresponding backbone reproduced separately for each modality and its ContiLNN counterpart. The reproduced backbones use single-slice (2D) input, whereas ContiLNN uses local ordered-slice (2.5D) input. ContiLNN values are mean±sample standard deviation across five training seeds. Bold values indicate improvements over the corresponding reproduced backbone within each block. PSNR is reported in dB.

Method	MRI super-resolution			CT denoising			PET restoration		
	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$
<i>Published reference results: Restore-RWKV study</i>									
ARGAN (Luo et al., 2022)	30.0800	0.9083	35.7999	32.9200	0.9111	9.2110	36.7500	0.9389	0.0907
DenoMamba (Öztürk et al., 2026)	30.3200	0.9091	34.6972	33.1800	0.9115	8.9512	36.8100	0.9367	0.0895
MambaIR (Guo et al., 2025)	31.3100	0.9305	31.3150	33.5000	0.9165	8.6345	37.1700	0.9458	0.0864
AirNet (Li et al., 2022)	31.3900	0.9316	31.1141	33.6200	0.9176	8.5226	37.1700	0.9451	0.0864
DRMC (Yang et al., 2023)	29.5500	0.9032	38.1691	33.2800	0.9153	8.8674	36.1900	0.9376	0.0960
AMIR (Yang et al., 2024)	32.0300	0.9396	29.0988	33.7000	0.9182	8.4520	37.1200	0.9475	0.0876
Restore-RWKV routing (Yang et al., 2026a)	32.1000	0.9408	28.9507	33.7400	0.9189	8.4148	37.3200	0.9479	0.0852
Restore-RWKV (reproduced) (Yang et al., 2026a)	32.0650	0.9403	29.0337	33.7642	0.9189	8.3950	37.2722	0.9474	0.0860
ContiLNN-RWKV (ours)	33.0826±0.0261	0.9485±0.0003	25.9882±0.0809	33.9549±0.0026	0.9208±0.0003	8.2132±0.0030	38.5204±0.0938	0.9535±0.0013	0.0752±0.0009
<i>Published reference results: DASMamba study</i>									
NAFNet* (Chen et al., 2022)	31.9078	0.9376	29.5394	33.7848	0.9200	8.3742	37.2672	0.9453	0.0859
CODEFormer* (Zhou et al., 2022)	31.8879	0.9371	29.5584	33.8066	0.9203	8.3532	37.2846	0.9448	0.0856
XFormer* (Zhang et al., 2024)	31.9122	0.9373	29.4700	33.7610	0.9200	8.3947	37.2542	0.9450	0.0859
Histoformer* (Sun et al., 2025)	31.9210	0.9378	29.4177	33.8115	0.9206	8.3480	37.3628	0.9472	0.0850
VmambaIR* (Shi et al., 2025)	31.9277	0.9380	29.3439	33.7627	0.9203	8.3943	37.3673	0.9468	0.0847
DASMamba-S (Chan et al., 2026)	31.7919	0.9355	29.8132	33.7948	0.9202	8.3646	37.2895	0.9460	0.0857
DASMamba (reproduced) (Chan et al., 2026)	32.1426	0.9450	28.6841	33.8374	0.9270	8.3262	37.3532	0.9395	0.0849
ContiLNN-DASMamba (ours)	32.5030±0.0438	0.9400±0.0016	27.5955±0.1229	34.0308±0.0163	0.9219±0.0003	8.1445±0.0142	38.4796±0.1090	0.9519±0.0014	0.0754±0.0007

Table 2: Bi-CfC and Bi-GRU under contiguous training on the 29-case PET test cohort. Both variants use the same insertion sites, objective and training budget. The slice-index gap g specifies the separation between neighboring observations; irregular windows mix $g \in \{1, 2, 3\}$. All settings evaluate the same original target slices with different neighboring context. Bold indicates the better operator within each test condition.

Test context	Slice-axis operator	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$
Gap $g = 1$	Bi-GRU	38.5176	0.9538	0.0753
	Bi-CfC	38.5868	0.9546	0.0744
Gap $g = 2$	Bi-GRU	37.6217	0.9462	0.0826
	Bi-CfC	37.7136	0.9476	0.0817
Gap $g = 3$	Bi-GRU	36.5295	0.9366	0.0940
	Bi-CfC	36.6652	0.9393	0.0927
Irregular gaps $\{1, 2, 3\}$	Bi-GRU	37.8544	0.9465	0.0802
	Bi-CfC	37.9494	0.9479	0.0793

respectively. The consistent PSNR and RMSE improvements across both backbones support architectural compatibility, with the accompanying SSIM differences retained in the paired results.

4.4. Sampling robustness

Bi-CfC is evaluated against Bi-GRU to examine restoration when neighboring slices are sparsely or irregularly available (Table 2). Both variants are trained on contiguous windows, retaining the same backbone initialization, insertion sites, full objective and training budget. At test time, sampling changes the neighboring context while preserving the original images, slice indices and evaluated target slices.

Uniform gaps $g = 1, 2, 3$ select consecutive, every second and every third slices, respectively. For full seven-slice irregular windows, the six transitions comprise two occurrences of each gap. Sparse evaluation uses interleaved slice sequences,

whereas irregular evaluation combines overlapping windows; both protocols retain the same eligible targets across the 29 test cases.

Under contiguous training, Bi-CfC achieves higher PSNR and SSIM and lower RMSE than Bi-GRU in all four test contexts (Table 2; Supplementary Fig. S6A). Its PSNR advantage increases from 0.0693 dB at $g = 1$ to 0.1357 dB at $g = 3$. Relative to each operator’s $g = 1$ result, PSNR decreases by 1.9216 dB for Bi-CfC and 1.9881 dB for Bi-GRU at $g = 3$, indicating modestly smaller degradation as neighboring observations become more widely separated. Bi-CfC also has lower measured latency and peak allocated memory than Bi-GRU under the common profiling workload (Table 4; Supplementary Fig. S6B).

An additional mixed-gap study examines whether exposure to varied sampling gaps improves restoration under altered neighboring context. Both operators benefit under sparse and ir-

regular conditions, with no uniform ranking across metrics and contexts after mixed-gap training (Supplementary Section H).

4.5. Data efficiency

Limited paired cohorts provide a second test of the information contributed by neighboring anatomy. We train PET models using nested subsets of six and 12 patients, corresponding to 5% and 10% of the training cohort, while retaining the full validation and test partitions (Table 3). Budget-matched training assigns the same total number of target-slice presentations to Restore-RWKV and ContiLNN. Full refinement additionally trains the sequence model from the corresponding 2D checkpoint; both strategies use the same patients. Exposure budgets and schedules are detailed in Supplementary Section A.

Under the matched target-slice exposure budget, ContiLNN improves PSNR by 0.5914 and 0.5889 dB at the 5% and 10% patient fractions, respectively, with higher SSIM and lower RMSE. Full refinement uses additional optimization on the same patient subsets and yields further PSNR and RMSE improvements. Its SSIM decreases at 5% and increases at 10% relative to matched-budget ContiLNN. The matched-budget results support improved use of limited paired data, while the separate refinement results describe the effect of additional optimization.

4.6. Qualitative results

ContiLNN preserves local structure across the three modalities. The CT examples retain clearer soft-tissue interfaces and small high-contrast structures (Fig. 3A). MRI contours follow the HQ reference more closely (Fig. 3B), while PET uptake patterns show clearer local contrast (Fig. 3C). The matched regions of interest and error maps locate these improvements.

Orthogonal MRI views extend this assessment beyond individual in-plane slices (Supplementary Section G, Figs. S4 and S5). The enlarged regions highlight narrow tissue interfaces and branching boundaries in both the H–W and D-axis views; ContiLNN follows their HQ appearance more closely than Restore-RWKV in these selected regions. The D–W and D–H reformats retain all 100 processed slices, allowing these local structures to be examined across the available slice sequence.

Boundary regions provide a focused assessment of cross-slice continuity: as anatomy varies along the slice axis, the relative contributions of neighboring tissues within a fixed local region change, producing intensity transitions that a restoration model should preserve. We examine three locations (P1–P3) in each modality (Fig. 4). In CT, P1 and P3 lie near posterior paraspinal soft-tissue boundaries, while P2 lies beside the vertebral body at a soft-tissue interface. In MRI, P1 and P3 sample soft-tissue interfaces near the skull base, and P2 samples a tissue–air interface in the nasal region. In PET, P1–P3 sample pelvic, abdominal and lateral body regions with distinct uptake contrasts. The profiles thus probe both relatively stable local intensities and more pronounced changes as structures pass through the sampled region.

Agreement with the reference involves preserving the level and shape of these intensity changes. At CT P2, ContiLNN

reduces the intensity deviation across all seven positions, including the terminal drop in the baseline profile. At MRI P2, it follows the reference peak at relative position -1 and trough at $+1$, retaining the sharp transition. At PET P3, it more closely follows the rise and subsequent decline in reference uptake. For these three displayed profiles, the mean absolute deviation from the reference over seven positions decreases from 0.290 to 0.135, from 0.150 to 0.066 and from 0.257 to 0.085, respectively, on the normalized intensity scale defined in the caption. Together, these examples link the visible boundary regions to reduced local intensity error and better preservation of reference variation along the slice axis.

Additional refinement is visible along the lung-facing margins of central thoracic soft tissue and near posterior structures beside the vertebral body (Fig. 5, lower row). Across slices 202–208, the highlighted regions remain associated with these interfaces as their contours change. Relative to the LQ input, Restore-RWKV reduces error across broader soft-tissue regions (upper row), with further reductions near anatomical boundaries after ContiLNN refinement (lower row). The recurring reductions at corresponding interfaces complement the intensity variations at the selected locations in Fig. 4, providing spatial and local profile evidence of restoration along the slice sequence. This pattern is consistent with neighboring anatomical information contributing to local boundary refinement.

4.7. Case-level analysis

Restoration gains extend across the held-out MRI and PET cohorts. We analyze paired case-level differences from complete saved output volumes, defining positive differences as higher PSNR or SSIM and lower RMSE. Significance is evaluated with paired two-sided Wilcoxon signed-rank tests (Wilcoxon, 1945) and Holm adjustment across the six modality–metric tests (Holm, 1979). Median differences are accompanied by 95% case-bootstrap confidence intervals (Efron, 1979); the evaluation settings are given in Supplementary Section A.

All 114 MRI subjects and all 29 PET scans improve in PSNR, SSIM and RMSE (Fig. 6A–D). Median PSNR gains are 1.0443 dB for MRI and 1.1711 dB for PET, with 95% confidence intervals of [1.0154, 1.0681] and [1.0636, 1.3666] dB, respectively (Fig. 6E). Median SSIM increases are 0.0084 and 0.0060, and median absolute RMSE reductions are 2.0425 and 0.0104. All six adjusted p values are below 1.2×10^{-8} . The distributions therefore associate the aggregate improvement with consistent case-level benefits throughout these two test cohorts.

4.8. Ablation studies

Computational cost. Selective insertion adds 6.56 million parameters and 22.88 billion multiply–accumulate operations (GMACs) per slice to Restore-RWKV (Table 4). For a matched seven-image workload, the median forward time per slice increases by 8.97 ms, from 16.72 to 25.69 ms, while peak allocated inference memory changes from 987.00 to 995.03 MB. Per-slice time is amortized over one seven-slice forward pass; data loading and overlapping-window fusion are outside this

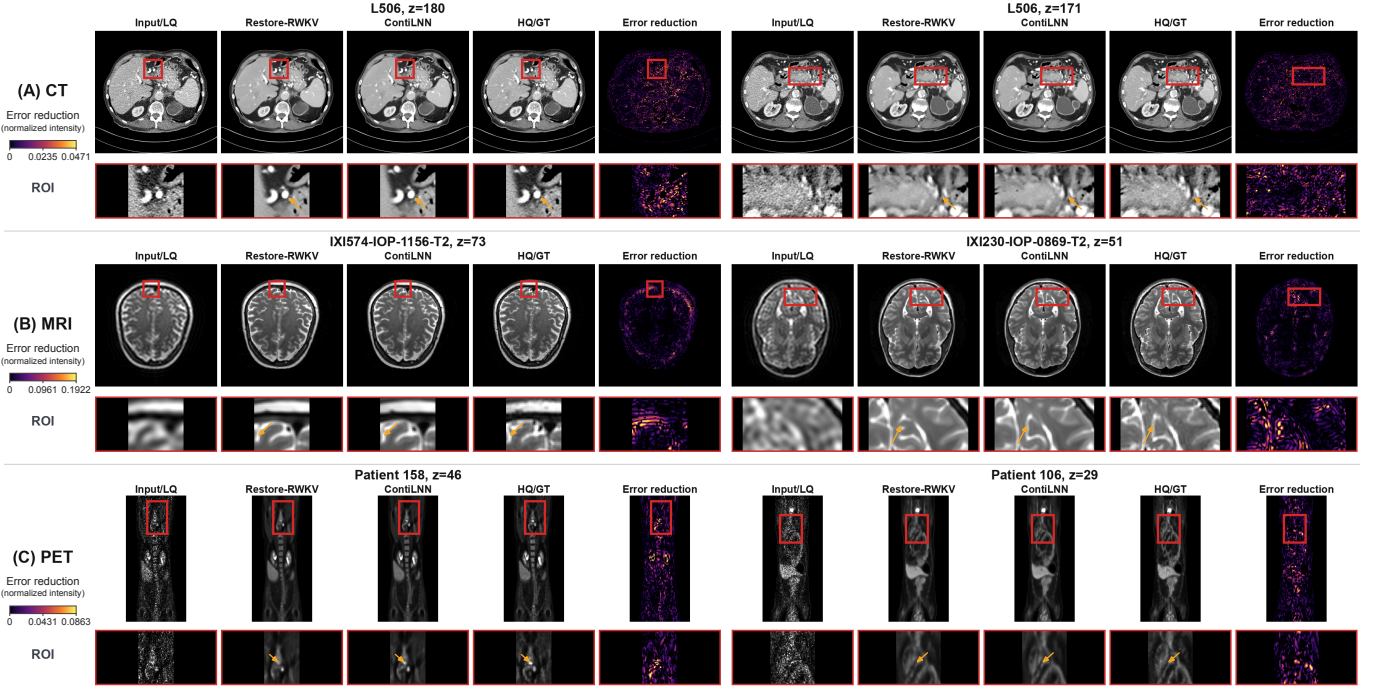


Figure 3: Restoration examples for (A) CT, (B) MRI and (C) PET, with two examples per modality. Columns contain LQ inputs, Restore-RWKV and ContiLNN outputs, HQ references (ground truth, GT), and Error-reduction maps. Boxed regions are enlarged below; orange arrows identify corresponding local structures and intensity transitions. Brighter colors indicate larger positive reductions in absolute error relative to Restore-RWKV, measured in normalized display intensity. Error increases are clipped to zero. Each modality shares one color scale; display masking and saturation settings are given in Supplementary Section A.

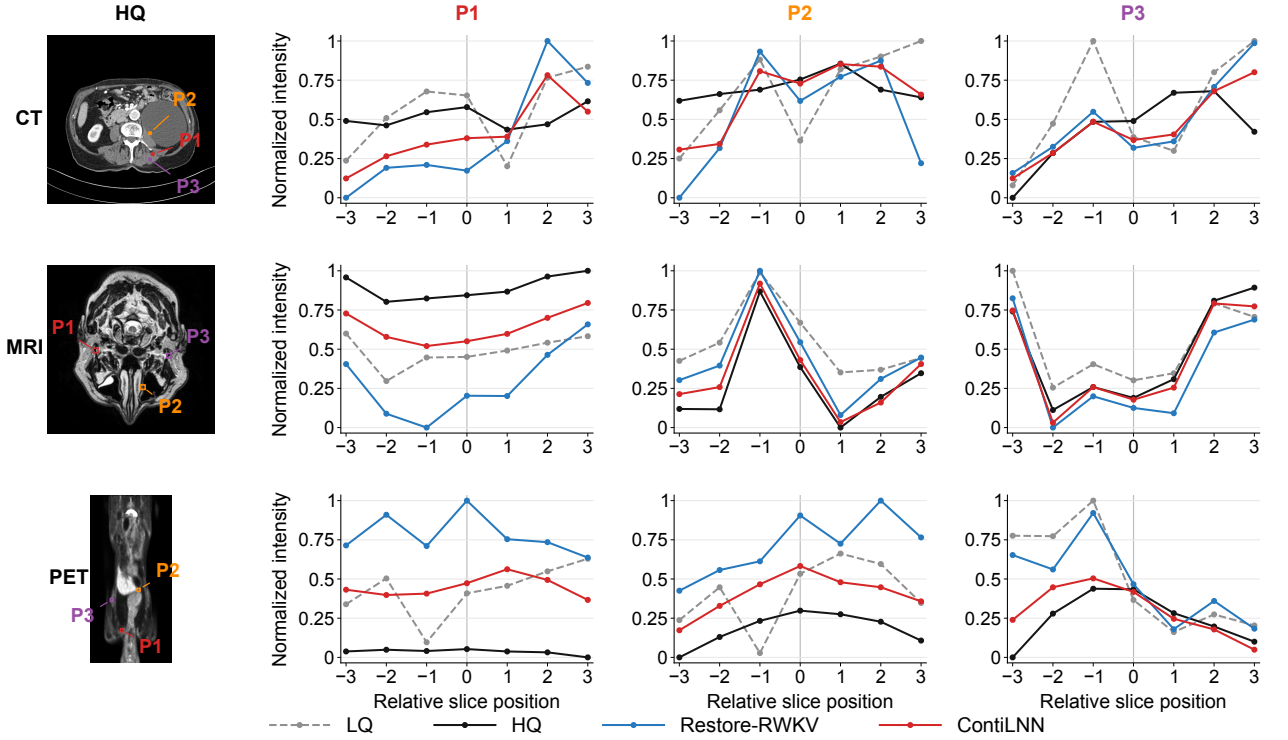


Figure 4: Intensity profiles across seven ordered CT, MRI and PET slices. P1–P3 mark tissue interfaces or uptake transitions. Each profile averages a 7×7 region centered at the marked location and is normalized using the joint range of the LQ, HQ, Restore-RWKV and ContiLNN profiles at that location. The horizontal axis gives relative slice position; colors and line styles identify the four image sequences.

Table 3: PET restoration with 5% and 10% of the training patients. Patient subsets are nested, with the validation and test cohorts unchanged. Budget-matched training uses the same number of slice presentations as Restore-RWKV; full refinement adds optimization on the same patient subset. Bold highlights the ContiLNN results.

Patient budget	Training strategy	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$
5%	Restore-RWKV	36.2923	0.9372	0.0973
5%	Budget-matched ContiLNN	36.8837	0.9390	0.0911
5%	Full-refinement ContiLNN	37.2385	0.9343	0.0875
10%	Restore-RWKV	36.5217	0.9389	0.0947
10%	Budget-matched ContiLNN	37.1106	0.9408	0.0886
10%	Full-refinement ContiLNN	37.2121	0.9430	0.0875

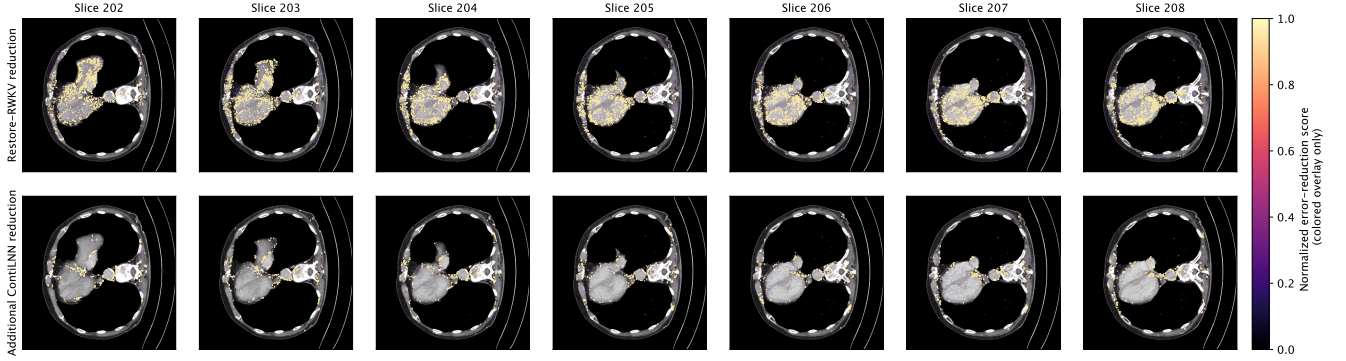


Figure 5: Spatial error reduction across seven adjacent CT slices: Restore-RWKV relative to LQ (top), and ContiLNN relative to Restore-RWKV (bottom). Colored overlays indicate positive reductions in absolute error against HQ; each row shares one color scale.

Table 4: Computational cost and PET restoration gains. Profiling uses 128×128 images, 32-bit precision and one NVIDIA A800 GPU: seven independent slices for Restore-RWKV ($B = 7$), or one seven-slice window for each ContiLNN-RWKV variant. MLP and Bi-GRU denote multilayer perceptron and bidirectional gated recurrent unit. M denotes 10^6 parameters; GMAC denotes 10^9 multiply-accumulate operations. Latency is median forward time per slice; memory is peak allocated GPU memory. Each Δ is the model’s result minus the reproduced Restore-RWKV result in Table 5 (37.2722 dB PSNR, 0.9474 SSIM, 0.0860 RMSE). Positive PSNR/SSIM and negative RMSE differences indicate improvement. Profiling details are in Supplementary Section A.

Model	Computational cost					PET metric differences		
	Params. (M)	GMAC/ slice	GMAC/ window	Latency/ slice (ms)	Memory (MB)	Δ PSNR $\uparrow$ (dB)	Δ SSIM $\uparrow$	Δ RMSE $\downarrow$
Restore-RWKV	28.37	37.46	262.21	16.72	987.00	0.0000	0.0000	0.0000
ContiLNN-RWKV, MLP	34.92	60.32	422.26	21.23	1835.22	-0.3039	-0.0039	+0.0031
ContiLNN-RWKV, Bi-GRU	34.91	60.50	423.51	54.42	2315.80	+1.2454	+0.0064	-0.0107
ContiLNN-RWKV, Bi-CfC	34.93	60.34	422.39	25.69	995.03	+1.3146	+0.0072	-0.0116

Table 5: PET ablation on the 29-case test cohort. ContiLNN variants share the pretrained backbone initialization, insertion locations, training budget and evaluation procedure. The MLP processes slices independently; Bi-GRU and Bi-CfC use the same bidirectional slice context. $\mathcal{L}_{\text{full}}$ denotes the full training objective. Bold indicates the highest PSNR and SSIM and the lowest RMSE.

ID	Setting	Slice-axis operator	Objective	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$
A	Restore-RWKV	None	$\mathcal{L}_{\text{rec}}$	37.2722	0.9474	0.0860
B	ContiLNN, reconstruction only	Bi-CfC	$\mathcal{L}_{\text{rec}}$	38.4166	0.9533	0.0760
C	ContiLNN, pointwise MLP	Slice-independent MLP	$\mathcal{L}_{\text{full}}$	36.9683	0.9435	0.0891
D	ContiLNN, recurrent alternative	Bi-GRU	$\mathcal{L}_{\text{full}}$	38.5176	0.9538	0.0753
E	ContiLNN, full objective	Bi-CfC	$\mathcal{L}_{\text{full}}$	38.5868	0.9546	0.0744

measurement. Profiling uses the same device, precision and image dimensions, specified in Supplementary Section A.

A slice-independent multilayer perceptron (MLP) inserted at the same pathways has nearly identical model size and arith-

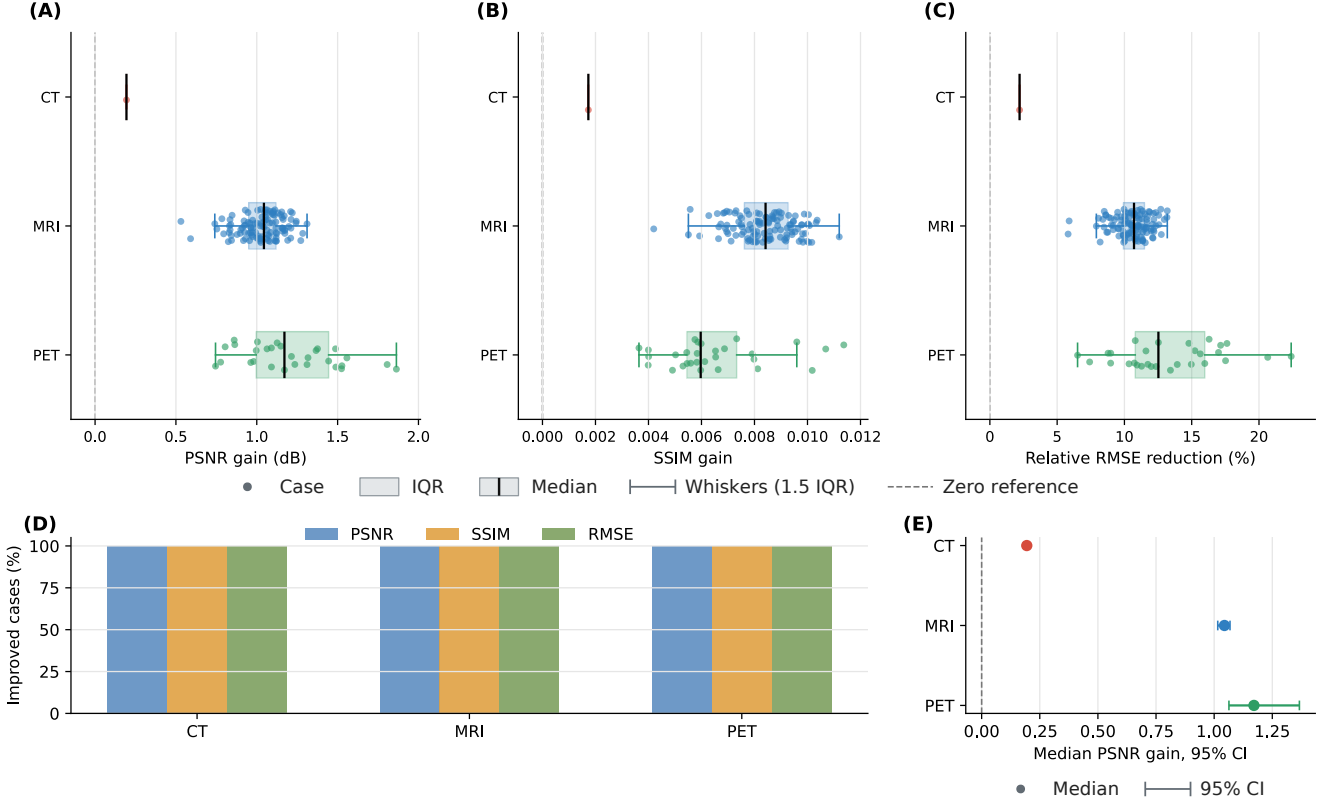


Figure 6: Case-level improvements over Restore-RWKV. (A)–(C) PSNR gain, SSIM gain and relative RMSE reduction; positive values favor ContiLNN. Points show all cases. Boxes span the interquartile range (IQR), with median lines and whiskers ending at the most extreme observations within 1.5 IQR of the box. Dashed lines mark zero. (D) Percentage of improved cases. (E) Median PSNR gains with 95% percentile confidence intervals from 10,000 case-bootstrap resamples for MRI and PET. CT has one test case and is descriptive, without a confidence interval.

metic cost to Bi-CfC. Its latency is lower, at 21.23 ms per slice, but its peak allocated memory is higher, at 1,835.22 MB. This resource profile enables an ablation of ordered propagation against a pointwise operator with closely matched capacity and computation.

A bidirectional gated recurrent unit (Bi-GRU) alternative is evaluated under the same profiling conditions. Bi-GRU and Bi-CfC closely match in parameter count (34.91 versus 34.93 million) and arithmetic cost (423.51 versus 422.39 GMACs per window). Bi-CfC reduces median window latency from 380.92 to 179.85 ms (52.8%) and peak allocated memory from 2,315.80 to 995.03 MB (57.0%), showing that matched capacity and arithmetic cost do not imply matched execution cost.

Architecture and objective. The PET ablations examine pointwise capacity, ordered-operator choice and training regularization (Table 5). Reconstruction-only Bi-CfC improves PSNR by 1.1444 dB over the 2D backbone. With the full objective, it exceeds the slice-independent MLP by 1.6185 dB in PSNR and 0.0111 in SSIM, with RMSE reduced by 0.0147, supporting propagation beyond pointwise capacity. Bi-GRU retains the same bidirectional context, full objective, initialization, insertion sites and training budget. Relative to this recurrent alternative, Bi-CfC improves PSNR by 0.0693 dB and SSIM by 0.0008, reduces RMSE by 0.0009, and has lower measured la-

tency and memory use (Table 4). Together with the sampling comparison in Table 2 and the resource measurements in Table 4, these results support Bi-CfC as the preferred sequence operator for ContiLNN under the evaluated conditions.

Consistency and distillation provide a further improvement to Bi-CfC: the full objective adds 0.1702 dB in PSNR and 0.0013 in SSIM, while reducing RMSE by 0.0016. The broader architecture study supports selective insertion at intermediate and bottleneck features, with gated updates along the remaining pathways (Supplementary Section B). Component-wise loss analysis is provided in Section C, and sequence length is examined in Section D. The completed 2D training trajectory in Supplementary Section F documents the initialization used for refinement.

We assess local anatomy by varying context around a fixed PET center image, using the same trained ContiLNN-RWKV checkpoint (Fig. 7A). Ordered local context is the default condition. Reversal retains the local images in the opposite order; center repetition removes distinct neighboring observations; nonlocal same-case sampling retains patient-specific appearance while replacing local anatomy. Each condition is evaluated at the same ten center positions per scan across all 29 test scans.

As shown in Fig. 7B and the results in Table 6, reversing the local sequence reduces PSNR by 0.2565 dB. Preceding and

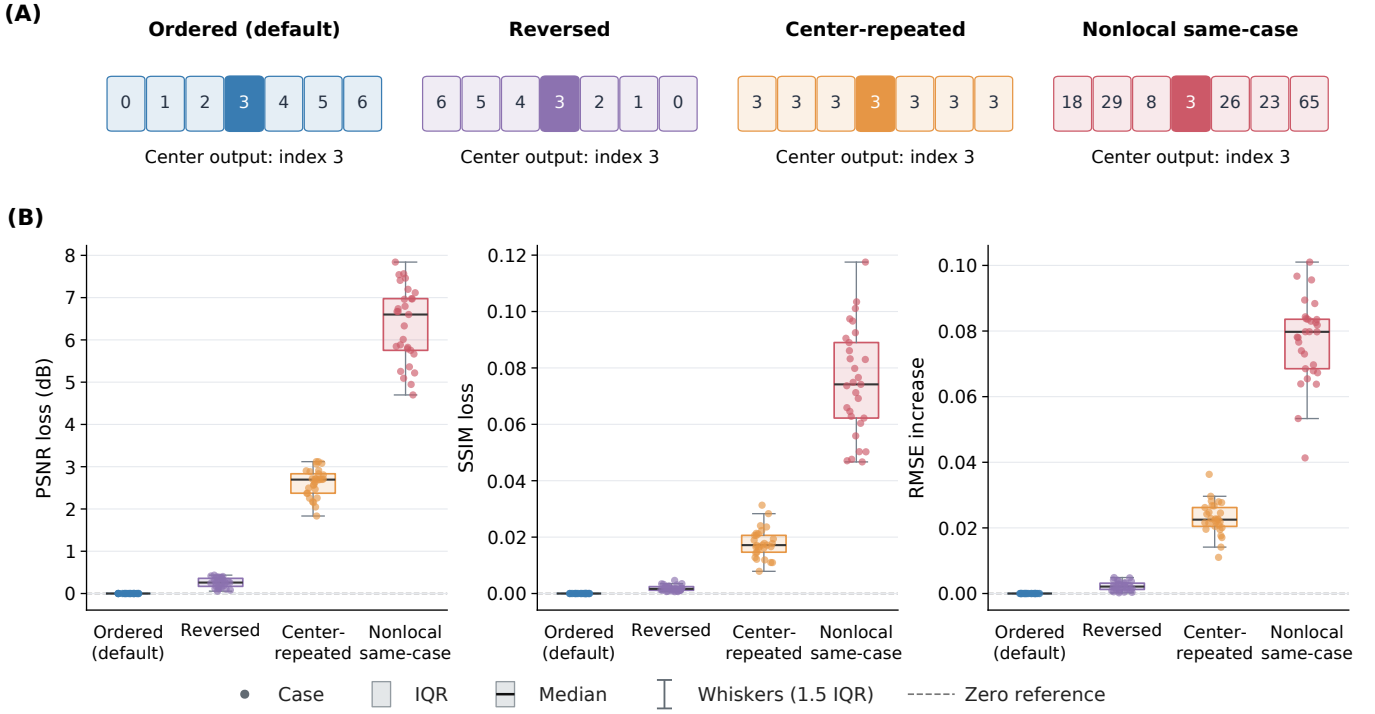


Figure 7: PET context perturbations. (A) Ordered, reversed, center-repeated and nonlocal same-case inputs, illustrated using Patient 10 at center index 3; every condition retains the evaluated center image. (B) PSNR loss, SSIM loss and RMSE increase for 29 test scans using the same trained checkpoint. Points show all cases; box-plot conventions follow Fig. 6A–C. Differences are relative to ordered context, whose zero value is marked by dashed lines.

Table 6: PET restoration under the context perturbations illustrated in Fig. 7. The same trained ContiLNN-RWKV checkpoint is held fixed across all four conditions. Ten center slices are evaluated in each of the 29 test cases. Metrics are averaged over centers within each case and then across cases; Δ PSNR is relative to ordered context. Bold indicates the best PSNR, SSIM and RMSE across these conditions.

Context	Cases	Centers	PSNR $\uparrow$	Δ PSNR	SSIM $\uparrow$	RMSE $\downarrow$
Ordered (default)	29	290	38.719844	0.000000	0.954441	0.073956
Reversed	29	290	38.463333	-0.256511	0.952564	0.076172
Center-repeated	29	290	36.104738	-2.615106	0.936650	0.096815
Nonlocal same-case	29	290	32.368766	-6.351078	0.879486	0.150989

following content remains available to the bidirectional operator, while its positional arrangement changes. Center repetition and nonlocal same-case sampling reduce PSNR by 2.6151 and 6.3511 dB, respectively. These changes associate restoration quality with both the locality and ordering of the supplied observations, with the larger deterioration following the removal of distinct local neighbors. Supplementary Section E describes the paired analysis, and Supplementary Table S6 supplies the per-case absolute metrics and changes relative to ordered context.

5. Discussion

5.1. Anatomical context and restoration

Earlier restoration studies established complementary uses of adjacent slices through volumetric feature extraction and neighboring-slice supervision (Shan et al., 2018; Zhang et al., 2021). ContiLNN builds on this anatomical information

through ordered feature propagation within a 2D restoration hierarchy. The PET ablations distinguish additional pointwise capacity from cross-slice propagation and compare two operators with the same bidirectional context. Context perturbations further show larger losses when distinct local neighbors are removed or replaced than when their order is reversed (Table 6). This pattern suggests that local anatomical content supplies an important source of information, with its ordering making an additional contribution to restoration fidelity.

The two regularizers address different aspects of using this information. Reference-based differences encourage predictions to follow the intensity changes of the anatomical sequence, including transitions at tissue interfaces. Knowledge distillation transfers information through reference predictions (Hinton et al., 2015); here, 2D backbone distillation uses a frozen, pretrained backbone to provide an in-plane reference as ContiLNN incorporates neighboring observations. Their complementary role is supported by the loss-component analysis in

Supplementary Section C. The resulting design combines access to neighboring anatomy with supervision of how the restored sequence should vary.

Across CT, MRI and PET, this combination improves fidelity under different degradation processes. Local image examples, orthogonal MRI views and intensity profiles relate the gains to anatomical interfaces and uptake transitions, while the MRI and PET case-level analyses show how those gains extend across the evaluated cohorts. Together, these results support local anatomical continuity as a useful source of complementary information for restoration.

5.2. Sampling and efficiency

Restoration from incomplete image series requires using neighboring observations whose separation may vary along the slice axis. Retaining the original indices distinguishes consecutive slices from observations separated by omitted positions. CfC incorporates the resulting normalized index gaps into its closed-form state updates without iterative numerical integration (Hasani et al., 2022). Under the principal contiguous-training protocol, Bi-CfC maintains higher restoration fidelity than Bi-GRU across the tested sparse and irregular contexts. The mixed-gap study shows that broader sampling exposure benefits both operators, with closely matched performance under that training strategy. Together with lower measured latency and peak allocated memory than Bi-GRU, these findings support Bi-CfC as the preferred slice-axis operator for ContiLNN in the evaluated setting.

The limited-patient PET experiments examine the value of the same context under constrained training data. Improvements at matched target-slice exposure indicate more effective use of the available observations. Additional refinement addresses a complementary setting by allocating further optimization to models trained on the same patients. The two settings connect sequence modeling with data efficiency while distinguishing the contribution obtained at a matched exposure budget from that obtained through continued training.

Integration with Restore-RWKV and DASMamba (Yang et al., 2026a; Chan et al., 2026) separates in-plane representation learning from cross-slice information exchange. PSNR and RMSE gains with both backbones support this division of roles across the two tested architectures. Operator choice also affects the resources required for this exchange. Under the matched seven-slice, 32-bit NVIDIA A800 profiling conditions, Bi-CfC reduces median window latency by 52.8% and peak allocated memory by 57.0% relative to Bi-GRU, despite closely matched parameter counts and arithmetic costs (Table 4). The limited-patient and operator studies therefore identify complementary benefits in the use of training data and inference resources.

5.3. Limitations

The current evidence is based on fixed restoration benchmarks and local slice windows. Physical slice-spacing metadata are unavailable in the preprocessed data used here, so the experiments assess index-defined sampling rather than adaptation to calibrated anatomical distances. Window length and index gaps jointly determine the anatomical extent of the available context.

The CT test partition contains one patient; the small variation across training seeds characterizes training repeatability on that patient rather than between-patient robustness. Generalization across acquisition protocols has not yet been evaluated. Adding slice-axis propagation also increases the parameter count and arithmetic cost relative to the original 2D backbone.

5.4. Future directions

Physical slice coordinates derived from Digital Imaging and Communications in Medicine (DICOM) metadata could connect the updates more directly to anatomical distance and acquisition geometry. Adaptive context lengths and selective propagation across feature levels could further match contextual exchange to sampling density and local anatomical variation. Comparisons with slice-axis convolution and attention under matched budgets would help characterize these choices. Evaluation across centers and acquisition protocols, together with downstream tasks and reader studies, would extend the assessment of restoration quality to broader imaging workflows. By improving the quality of available slices while preserving their original positions, ContiLNN may help recover useful anatomical information from incomplete image series in retrospective clinical workflows.

6. Conclusion

ContiLNN augments two-dimensional medical image restoration with bidirectional liquid dynamics over ordered slice positions. Slice-index intervals condition state propagation on the supplied sampling, while joint restoration preserves an output for every observed slice. Experiments across CT, MRI and PET demonstrate improved fidelity. Experiments with limited paired training cohorts (5% and 10% of PET training patients) and a second restoration backbone (DASMamba) support data efficiency and architectural compatibility, while the PET ablations support ordered propagation and complementary regularization. Under contiguous training, Bi-CfC achieves higher fidelity than Bi-GRU across the tested sampling conditions, alongside lower measured inference latency and peak allocated memory. Additional mixed-gap experiments show that broader sampling exposure can improve both operators. These findings support Bi-CfC as the preferred operator in the evaluated ContiLNN framework and liquid dynamics as a practical approach to incorporating anatomical continuity into 2D restoration networks.

Data availability

The CT data derive from the ten-patient training set of the AAPM Low Dose CT Grand Challenge (McCollough et al., 2017), and the MRI data from the IXI project (IXI Project, n.d.). The PolarStar m660 PET cohort is described in the original AMIR study (Yang et al., 2024). The preprocessed benchmark datasets used in this study were obtained from the Restore-RWKV repository (<https://github.com/Yaziwel/Restore-RWKV>); their source cohorts and preprocessing are described in

Section 4.1. Access and reuse are subject to the terms of the respective source data providers. No new clinical imaging data were collected.

Code availability

The source code, experiment configurations, and evaluation scripts are publicly available at <https://github.com/Noah-hjl/ContiLNN>.

Declaration of generative AI and AI-assisted technologies in the manuscript preparation process

During the preparation of this manuscript, the authors used ChatGPT and Codex (OpenAI) for language editing, manuscript organization, LaTeX preparation, literature checking, and assistance with plotting and layout code. The authors reviewed and verified the resulting text, references, and relevant code outputs, edited the material as needed, and take full responsibility for the content of the published article. Medical images presented as evidence originate from research data and model outputs, not generative AI.

Ethics statement

This work involved secondary analysis of pre-existing data released for research use and included no new participant recruitment or imaging acquisition. The source cohorts and acquisition protocols are described in the cited dataset publications.

Declaration of competing interest

Given his role as Associate Editor of Medical Image Analysis, S. Kevin Zhou had no involvement in the peer review of this article and had no access to information regarding its peer review. Full responsibility for the editorial process for this article was delegated to another journal editor.

Funding

This research received no specific grant from any funding agency in the public, commercial, or not-for-profit sectors.

Acknowledgements

The authors acknowledge the High-Performance Computing Platform of Xi'an Jiaotong-Liverpool University for providing the computational resources used in this study.

References

- Chan, S.C.K., Shi, L., Huang, B., Wong, T.T.W., 2026. Directional adaptive shuffle-based visual state-space models for medical image restoration, in: Medical Image Computing and Computer Assisted Intervention – MICCAI 2025, Springer, Cham. pp. 160–170. doi:10.1007/978-3-032-05169-1_16.
- Chatterjee, S., Sciarra, A., Dünnwald, M., Ashoka, A.B.T., Vasudeva, M.G.C., Saravanan, S., Sambandham, V.T., Tummala, P., Oeltze-Jafra, S., Speck, O., Nürnberger, A., 2024. Beyond nyquist: A comparative analysis of 3D deep learning models enhancing MRI resolution. *J. Imaging* 10, 207. doi:10.3390/jimaging10090207.
- Chen, H., Yang, Z., Hou, H., Zhang, H., Wei, B., Zhou, G., Xu, Y., 2026. All-in-one medical image restoration with latent diffusion-enhanced vector-quantized codebook prior, in: Medical Image Computing and Computer Assisted Intervention – MICCAI 2025, Springer, Cham. pp. 67–77. doi:10.1007/978-3-032-05325-1_7.
- Chen, L., Chu, X., Zhang, X., Sun, J., 2022. Simple baselines for image restoration, in: Computer Vision – ECCV 2022, Springer, Cham. pp. 17–33. doi:10.1007/978-3-031-20071-7_2.
- Chen, R.T.Q., Rubanova, Y., Bettencourt, J., Duvenaud, D.K., 2018. Neural ordinary differential equations, in: Advances in Neural Information Processing Systems. URL: <https://proceedings.neurips.cc/paper/2018/hash/69386f6bb1dfed68692a24c8686939b9-Abstract.html>.
- Chen, T., Hou, J., Zhou, Y., Xie, H., Chen, X., Liu, Q., Guo, X., Xia, M., Duncan, J.S., Liu, C., Zhou, B., 2025. 2.5D multi-view averaging diffusion model for 3D medical image translation: Application to low-count PET reconstruction with CT-less attenuation correction. *IEEE Trans. Med. Imaging* 44, 4239–4250. doi:10.1109/TMI.2025.3570342.
- Dong, Z., He, Y., Qi, X., Chen, Y., Shu, H., Coatrieux, J.L., Yang, G., Li, S., 2022. MNet: Rethinking 2D/3D networks for anisotropic medical image segmentation, in: International Joint Conference on Artificial Intelligence, pp. 870–876. doi:10.24963/ijcai.2022/122.
- Duan, Y., Wang, W., Chen, Z., Zhu, X., Lu, L., Lu, T., Qiao, Y., Li, H., Dai, J., Wang, W., 2025. Vision-RWKV: Efficient and scalable visual perception with RWKV-like architectures, in: International Conference on Learning Representations. URL: https://proceedings.iclr.cc/paper_files/paper/2025/hash/ce65173b994cf7c925c71b482ee14a8d-Abstract-Conference.html.
- Efron, B., 1979. Bootstrap methods: Another look at the jackknife. *Ann. Stat.* 7, 1–26. doi:10.1214/aos/1176344552.
- Gu, A., Dao, T., 2024. Mamba: Linear-time sequence modeling with selective state spaces, in: First Conference on Language Modeling. URL: <https://openreview.net/forum?id=tEYskw1VY2>.
- Guo, H., Li, J., Dai, T., Ouyang, Z., Ren, X., Xia, S.T., 2025. MambaIR: A simple baseline for image restoration with state-space model, in: Computer Vision – ECCV 2024, Springer, Cham. pp. 222–241. doi:10.1007/978-3-031-72649-1_13.
- Hasani, R., Lechner, M., Amini, A., Liebenwein, L., Ray, A., Tschaikowski, M., Teschl, G., Rus, D., 2022. Closed-form continuous-time neural networks. *Nat. Mach. Intell.* 4, 992–1003. doi:10.1038/s42256-022-00556-7.
- Hasani, R., Lechner, M., Amini, A., Rus, D., Grosu, R., 2021. Liquid time-constant networks, in: Proceedings of the AAAI Conference on Artificial Intelligence, pp. 7657–7666. doi:10.1609/aaai.v35i9.16936.
- Hinton, G., Vinyals, O., Dean, J., 2015. Distilling the knowledge in a neural network, in: NIPS Deep Learning and Representation Learn-

- ing Workshop. URL: <https://research.google/pubs/distilling-the-knowledge-in-a-neural-network/>.
- Holm, S., 1979. A simple sequentially rejective multiple test procedure. *Scand. J. Stat.* 6, 65–70. URL: <https://www.jstor.org/stable/4615733>.
- [dataset] IXI Project, n.d. IXI dataset. Information eXtraction from Images, EPSRC project GR/S21533/02. URL: <https://brain-development.org/ixi-dataset/>. accessed 5 September 2026.
- Jang, S.I., Pan, T., Li, Y., Heidari, P., Chen, J., Li, Q., Gong, K., 2024. Spach transformer: Spatial and channel-wise transformer based on local and global self-attentions for PET image denoising. *IEEE Trans. Med. Imaging* 43, 2036–2049. doi:10.1109/TMI.2023.3336237.
- Laine, S., Aila, T., 2017. Temporal ensembling for semi-supervised learning, in: International Conference on Learning Representations. URL: <https://openreview.net/forum?id=BJ6Ofqge>.
- Li, B., Liu, X., Hu, P., Wu, Z., Lv, J., Peng, X., 2022. All-in-one image restoration for unknown corruption, in: Proceedings of the IEEE/CVF Conference on Computer Vision and Pattern Recognition, pp. 17452–17462. URL: https://openaccess.thecvf.com/content/CVPR2022/html/Li_All-in-One_Image_Restoration_for_Unknown_Corruption_CVPR_2022_paper.html.
- Li, L., Wei, W., Yang, L., Zhang, W., Dong, J., Liu, Y., Huang, H., Zhao, W., 2025. CT-Mamba: A hybrid convolutional state space model for low-dose CT denoising. *Comput. Med. Imaging Graph.* 124, 102595. doi:10.1016/j.compmedimag.2025.102595.
- Liang, J., Cao, J., Sun, G., Zhang, K., Van Gool, L., Timofte, R., 2021. SwinIR: Image restoration using swin transformer, in: IEEE/CVF International Conference on Computer Vision Workshops, pp. 1833–1844. doi:10.1109/ICCVW54120.2021.00210.
- Luo, Y., Zhou, L., Zhan, B., Fei, Y., Zhou, J., Wang, Y., Shen, D., 2022. Adaptive rectification based adversarial network with spectrum constraint for high-quality PET image synthesis. *Med. Image Anal.* 77, 102335. doi:10.1016/j.media.2021.102335.
- McCollough, C.H., Bartley, A.C., Carter, R.E., Chen, B., Drees, T.A., Edwards, P., Holmes, III, D.R., Huang, A.E., Khan, F., Leng, S., McMillan, K.L., Michalak, G.J., Nunez, K.M., Yu, L., Fletcher, J.G., 2017. Low-dose CT for the detection and classification of metastatic liver lesions: Results of the 2016 low dose CT grand challenge. *Med. Phys.* 44, e339–e352. doi:10.1002/mp.12345.
- Moen, T.R., Chen, B., Holmes, III, D.R., Duan, X., Yu, Z., Yu, L., Leng, S., Fletcher, J.G., McCollough, C.H., 2021. Low-dose CT image and projection dataset. *Med. Phys.* 48, 902–911. doi:10.1002/mp.14594.
- Öztürk, Ş., Duran, O.C., Çukur, T., 2026. DenoMamba: A fused state-space model for low-dose CT denoising. *IEEE J. Biomed. Health Inform.* 30, 5353–5366. doi:10.1109/JBHI.2025.3629034.
- Peng, B., Alcaide, E., Anthony, Q., Albalak, A., Arcadinho, S., Biderman, S., Cao, H., Cheng, X., Chung, M., Derczynski, L., Du, X., Grella, M., Gv, K., He, X., Hou, H., Kazienko, P., Koccon, J., Kong, J., Koptyra, B., Lau, H., Lin, J., Mantri, K.S.I., Mom, F., Saito, A., Song, G., Tang, X., Wind, J., Woźniak, S., Zhang, Z., Zhou, Q., Zhu, J., Zhu, R.J., 2023. RWKV: Reinventing RNNs for the transformer era, in: Findings of the Association for Computational Linguistics: EMNLP 2023, Association for Computational Linguistics, Singapore. pp. 14048–14077. URL: <https://aclanthology.org/2023.findings-emnlp.936/>, doi:10.18653/v1/2023.findings-emnlp.936.
- Rubanova, Y., Chen, R.T.Q., Duvenaud, D.K., 2019. Latent ordinary differential equations for irregularly-sampled time series, in: Advances in Neural Information Processing Systems. URL: <https://proceedings.neurips.cc/paper/2019/hash/42a6845a557bef704ad8ac9cb4461d43-Abstract.html>.
- Shan, H., Zhang, Y., Yang, Q., Kruger, U., Kalra, M.K., Sun, L., Cong, W., Wang, G., 2018. 3-d convolutional encoder-decoder network for low-dose CT via transfer learning from a 2-d trained network. *IEEE Trans. Med. Imaging* 37, 1522–1534. doi:10.1109/TMI.2018.2832217.
- Shi, Y., Xia, B., Jin, X., Wang, X., Zhao, T., Xia, X., Xiao, X., Yang, W., 2025. VmambaIR: Visual state space model for image restoration. *IEEE Trans. Circuits Syst. Video Technol.* 35, 5560–5574. URL: <https://ieeexplore.ieee.org/document/10843251/>, doi:10.1109/TCSVT.2025.3530090.
- Sun, S., Ren, W., Gao, X., Wang, R., Cao, X., 2025. Restoring images in adverse weather conditions via histogram transformer, in: Computer Vision – ECCV 2024, Springer, Cham. pp. 111–129. doi:10.1007/978-3-031-72670-5_7.
- Tarvainen, A., Valpola, H., 2017. Mean teachers are better role models: Weight-averaged consistency targets improve semi-supervised deep learning results, in: Advances in Neural Information Processing Systems. URL: <https://proceedings.neurips.cc/paper/2017/hash/68053af2923e00204c3ca7c6a3150cf7-Abstract.html>.
- Wang, Z., Bovik, A.C., Sheikh, H.R., Simoncelli, E.P., 2004. Image quality assessment: From error visibility to structural similarity. *IEEE Trans. Image Process.* 13, 600–612. doi:10.1109/TIP.2003.819861.
- Wilcoxon, F., 1945. Individual comparisons by ranking methods. *Biom. Bull.* 1, 80–83. doi:10.2307/3001968.
- Xiao, J., Zheng, W., Wang, W., Xia, Q., Yan, Z., Guo, Q., Wang, X., Nie, S., Zhang, S., 2025. Slice2Mesh: 3D surface reconstruction from sparse slices of images for the left ventricle. *IEEE Trans. Med. Imaging* 44, 1541–1555. doi:10.1109/TMI.2024.3514869.
- Xu, J., Moyer, D., Gagoski, B., Iglesias, J.E., Grant, P.E., Golland, P., Adalsteinsson, E., 2023. NeSVoR: Implicit neural representation for slice-to-volume reconstruction in MRI. *IEEE Trans. Med. Imaging* 42, 1707–1719. doi:10.1109/TMI.2023.3236216.
- Yang, Z., Chen, H., Qian, Z., Yi, Y., Zhang, H., Zhao, D., Wei, B., Xu, Y., 2024. All-in-one medical image restoration via task-adaptive routing, in: Medical Image Computing and Computer Assisted Intervention – MICCAI 2024, Springer, Cham. pp. 67–77. URL: https://papers.miccai.org/miccai-2024/paper/0787_paper.pdf, doi:10.1007/978-3-031-72104-5_7.
- Yang, Z., Li, J., Zhang, H., Zhao, D., Wei, B., Xu, Y., 2026a. Restore-RWKV: Efficient and effective medical image restoration with RWKV. *IEEE J. Biomed. Health Inform.* 30, 513–526. doi:10.1109/JBHI.2025.3588555.
- Yang, Z., Zhang, J., Yi, Y., Liang, J., Wei, B., Xu, Y., 2026b. TAT: Task-adaptive transformer for all-in-one medical image restoration, in: Medical Image Computing and Computer Assisted Intervention – MICCAI 2025, Springer, Cham. pp. 565–575. doi:10.1007/978-3-032-05325-1_54.
- Yang, Z., Zhou, Y., Zhang, H., Wei, B., Fan, Y., Xu, Y., 2023. DRMC: A generalist model with dynamic routing for multi-center PET image synthesis, in: Medical Image Computing and Computer Assisted Intervention – MICCAI 2023, Springer, Cham. pp. 36–46. doi:10.1007/978-3-031-43898-1_4.
- Zamir, S.W., Arora, A., Khan, S., Hayat, M., Khan, F.S., Yang, M.H., 2022. Restormer: Efficient transformer for high-resolution image restoration, in: IEEE/CVF Conference on Computer Vision and Pattern Recognition, pp. 5718–5729. URL: https://openaccess.thecvf.com/content/CVPR2022/html/Zamir_Restormer_Efficient_Transformer_for_High-Resolution_Image_Restoration_CVPR_2022_paper.html, doi:10.1109/CVPR52688.2022.00564.
- Zhang, J., Zhang, Y., Gu, J., Dong, J., Kong, L., Yang, X., 2024.

- Xformer: Hybrid x-shaped transformer for image denoising, in: International Conference on Learning Representations. URL: https://proceedings.iclr.cc/paper_files/paper/2024/hash/393367b4ccf1d56e51276243d5cb85c4-Abstract-Conference.html.
- Zhang, Z., Liang, X., Zhao, W., Xing, L., 2021. Noise2Context: Context-assisted learning 3D thin-layer for low-dose CT. *Med. Phys.* 48, 5794–5803. doi:10.1002/mp.15119.
- Zhou, B., Xie, H., Liu, Q., Chen, X., Guo, X., Feng, Z., Hou, J., Zhou, S.K., Li, B., Rominger, A., Shi, K., Duncan, J.S., Liu, C., 2023. FedFTN: Personalized federated learning with deep feature transformation network for multi-institutional low-count PET denoising. *Medical Image Analysis* 90, 102993. doi:10.1016/j.media.2023.102993.
- Zhou, S., Chan, K.C.K., Li, C., Loy, C.C., 2022. Towards robust blind face restoration with codebook lookup transformer, in: *Advances in Neural Information Processing Systems*, pp. 30599–30611. URL: https://proceedings.neurips.cc/paper_files/paper/2022/hash/c573258c38d0a3919d8c1364053c45df-Abstract-Conference.html, doi:10.52202/068431-2218.

Supplementary Material for ContiLNN

Jialei He, Enhe Liu, Sifan Song, Pengfei Jin, Jionglong Su, Hongbin Wang,
Zhixiang Lu, Yanhao Huang, Anteng Cai, Zhengyong Jiang,
Jiaman Ding*, S. Kevin Zhou*, and Jinfeng Wang*

* Corresponding authors.

A Implementation details

A.1 Slice windows and liquid modules

We use ordered windows of at most $T = 7$ slices and retain short terminal windows. Under the default contiguous strategy, training partitions each case into non-overlapping windows and shuffles their order between epochs. For a window containing $K \leq T$ observations with a constant slice-index gap g , the interval supplied to the liquid cell is $\delta = g/K$. Thus, consecutive slices use $g = 1$ and $\delta = 1/K$. The separate within-window position encoding is linearly spaced from 0 to 1 when $K > 1$, and is 0 for a single-slice window. Normalization uses the actual K , including terminal windows. A fixed-gap single-slice window receives $\delta_0 = g$. Interval inputs are not clipped to $[0, 1]$. Position encoding specifies relative order, while each interval records the gap associated with that observation in the original forward order.

For irregular sampling, the first gap is repeated to supply an interval for the initial observation. Features and their associated intervals are reversed together for the backward branch. For example, indices $[0, 1, 3, 6, 7, 9, 12]$ give

$$\delta = \frac{1}{7}[1, 1, 2, 3, 1, 2, 3], \quad \delta^{\text{rev}} = \frac{1}{7}[3, 2, 1, 3, 2, 1, 1], \quad (1)$$

where δ^{rev} lists the interval inputs in backward traversal order. This convention preserves the sampling information paired with each feature; it does not recompute intervals from reverse-direction transitions between slice positions.

The Restore-RWKV configuration uses a base width of 48, encoder-stage block counts of $[4, 6, 6, 8]$, and four refinement blocks. Six bidirectional closed-form continuous-time (Bi-CfC) modules follow the six encoder-L2 blocks, and six follow the decoder-L2 blocks. One module is placed on each of the L2 and L3 skip pathways, one at the bottleneck before decoding, and one after the refinement pathway. These placements give 16 Bi-CfC modules and 15 external gates. The bottleneck uses serial insertion; all other selected pathways use gated residual insertion. Gate logits initialize at 0, except for the final refinement gate, which initializes at -4 .

Each directional CfC cell uses the default gated update, with one internal feed-forward layer of width $M_l = 256$, no dropout and no sparsity mask. The scaled hyperbolic-tangent activation in the joint feature map is $\rho(a) = 1.7159 \tanh(0.666a)$, applied elementwise. The two candidate heads use ordinary hyperbolic-tangent activations; the interval coefficient and gate intercept are unrestricted affine outputs. The implemented gate is $\sigma(\delta_t \eta_t + \xi_t)$, and the state is $(1 - \alpha_t) \odot c_t^{(1)} + \alpha_t \odot c_t^{(2)}$, following the default CfC parameterization described in the main manuscript. The internal width M_l is distinct from the recurrent-state width C_l , which equals the feature-channel count at pathway l . Forward and backward cells have separate parameters. The position projection maps one scalar to C_l channels, and the bidirectional fusion maps $2C_l$ channels to C_l ; both affine projections include a learned bias. The source-code names `ff1`, `ff2`, `time_a` and `time_b` correspond to the two candidate heads, interval coefficient and gate intercept in the main formulation, respectively.

At inference, two window tilings begin at offsets 0 and 3 in the case’s slice sequence. Each tiling retains its terminal window, and predictions at positions covered by both tilings are averaged. The original slice order is restored after fusion. All windows are formed within individual cases.

A.2 Restore-RWKV training

The 2D Restore-RWKV baseline is trained for 300,000 optimizer updates using Adam, a batch size of four slices, and an L_1 reconstruction loss. Cosine decay reduces the learning rate from 2×10^{-4} to 10^{-6} . The checkpoint with the highest validation peak signal-to-noise ratio (PSNR) initializes ContiLNN and supplies predictions from a frozen copy of the 2D backbone for distillation.

ContiLNN training uses 128×128 patches and three NVIDIA A800 GPUs, with one sequence per GPU. AdamW optimizes the complete model with zero weight decay. The initial learning rates are 2×10^{-4} for the 2D backbone and Bi-CfC parameters and 5×10^{-4} for the external gates, with cosine decay to 10^{-6} . Training uses automatic mixed precision and gradient clipping at a norm of 1.0. CT and PET have a 60-epoch cap; MRI has a 100-epoch cap. Early stopping is enabled after 15 epochs, with patience 10 and a minimum validation-PSNR improvement of 0.0005 dB. The five-seed results in main Table 1 use seeds 42, 2026, 3407, 777, and 12345.

The full Restore-RWKV objective uses $\lambda_{\text{cons}} = 0.30$, $\beta_2 = 2.0$, and $\lambda_{\text{KD}} = 0.05$, with unit reconstruction weight. The first- and second-order consistency terms use finite differences between the selected observations. In the reconstruction-only PET ablation, both λ_{cons} and λ_{KD} are zero. The multilayer perceptron (MLP) and bidirectional gated recurrent unit (Bi-GRU) ablations use the full objective. Bi-GRU replaces Bi-CfC while retaining its

insertion sites, initialization, training budget and evaluation workflow. The reference 2D backbone is frozen, while the ContiLNN backbone and added modules remain trainable.

The MRI source split allocates 405, 59, and 114 cases to training, validation, and testing. The implemented validation reader supplies 58 readable cases, and validation scores are calculated over those 58 cases. CT, MRI, and PET use their respective data readers and case-grouping rules.

A.3 DASMamba integration

ContiLNN-DASMamba follows the same backbone-initialization, ordered-window training, 2D backbone distillation and evaluation workflow as ContiLNN-RWKV. Its native spatial and Fourier-domain reconstruction terms are retained alongside the cross-slice consistency and distillation objectives. Detailed hyperparameters are reported for ContiLNN-RWKV as the representative implementation.

A.4 Sampling robustness

The PET sampling study compares Bi-CfC and Bi-GRU under contiguous and mixed-gap training. For each operator, the mixed-gap configuration retains the backbone initialization, insertion sites, objective, optimization settings and training budget of its contiguous-training counterpart. Each mixed-gap training window uses a constant gap selected from $\{1, 2, 3\}$. The three gaps contribute approximately equal numbers of windows, while the total windows and optimizer updates per epoch match contiguous training. A seven-observation window spans 7, 13, or 19 original slice positions for gaps 1, 2, or 3, respectively. Validation uses consecutive slices with the original two-tiling fusion. Sparse testing uses interleaved slice sequences, and irregular testing combines overlapping windows. All eligible original target slices are retained for evaluation across sampling conditions, with case-level metrics computed over the same test cohort. Mixed-gap training uses 16-bit mixed precision with a fixed loss scale of 128 and gradient clipping at 1.0. Complete results for both training strategies are reported in Section H.

A.5 Data efficiency

The PET data-efficiency experiments use training seed 42 and nested subsets of 6 and 12 patients, corresponding to 5% and 10% of the 120 training patients. The validation and test cohorts remain fixed. A slice presentation is counted whenever one target slice contributes to training; this makes the exposure budget comparable between independent-slice and sequence training.

Restore-RWKV receives 1.2 million slice presentations from random initialization. Budget-matched ContiLNN uses 0.6 million presentations for the 2D pathway, then activates Bi-CfC for a further 0.6 million presentations. The transition uses the checkpoint at that fixed exposure, with a frozen copy supplying the distillation targets during sequence training. Full refinement starts from the ratio-matched Restore-RWKV checkpoint after its 1.2-million-presentation schedule and adds a sequence-training budget derived from the full-data refinement schedule.

Both sequence-training strategies use AdamW, a global batch of three sequences, and peak learning rates of 2×10^{-4} for backbone and Bi-CfC parameters and 5×10^{-4} for gates. The learning rates warm up over the first 5% of the sequence-training exposure and then decay to 10^{-6} . Consistency and distillation weights increase linearly over the first 10% to 0.30 and 0.05, respectively; the second-order consistency weight is 2.0. The complete ContiLNN model remains trainable. Training uses a fixed mixed-precision loss scale of 128, gradient clipping at 1.0, and no early stopping. These schedules are indexed by slice exposure rather than epoch count.

A.6 Intensity processing

Training uses intensity ranges of $[-1024, 3072]$ Hounsfield units (HU) for CT, $[0, 4095]$ for MRI and $[0, 20]$ for PET. Random 128×128 crops, rotations and flips are applied consistently across the slices in each training window. Evaluation follows inverse normalization and truncation to $[-160, 240]$ HU for CT, $[0, 4095]$ for MRI and $[0, 20]$ for PET.

For the error-reduction maps in main Figure 3, I denotes displayed grayscale intensity normalized to $[0, 1]$. The plotted quantity is

$$E^+ = \max(|I_{\text{RWKV}} - I_{\text{HQ}}| - |I_{\text{ContiLNN}} - I_{\text{HQ}}|, 0). \quad (2)$$

The subscripts identify the two predictions and the HQ reference. Values are displayed where $0.035 < I_{\text{HQ}} < 0.985$, with pixels outside this mask set to zero. Inside the mask, zero includes unchanged error and error increases clipped to zero. The two examples within each modality share one color scale, which saturates at the 99th percentile of their pooled positive ROI values. These display settings do not change the reconstruction metrics.

A.7 Computational profiling

Inference is profiled on an NVIDIA A800 GPU using 32-bit floating-point precision and 128×128 images. The baseline processes a batch of seven independent slices, while the Bi-CfC, MLP and Bi-GRU variants each process one window of seven slices. Timing is measured after 20 warm-up passes and summarized by the median of 100 repetitions, with GPU synchronization around each repetition. Per-slice latency and arithmetic cost are obtained by dividing the window totals by seven. These latencies measure an amortized model forward pass; they exclude data loading, window assembly and the overlapping-tiling fusion used for full-volume restoration. Peak allocated memory is recorded after warm-up; memory values labelled MB use 2^{20} bytes. One GMAC denotes 10^9 multiply-accumulate operations. Peak

reserved memory is 1,168 MB for Bi-CfC, 2,692 MB for the pointwise MLP and 3,000 MB for Bi-GRU; the main table reports allocated memory for all models. The Bi-GRU and Bi-CfC variants contain 34.50 and 34.52 million trainable parameters, respectively, of which 6.54 and 6.55 million belong to their ordered operators. Their median seven-slice window latencies are 380.92 and 179.85 ms, respectively.

A.8 Evaluation and statistical settings

The structural similarity index measure (SSIM) uses an 11×11 Gaussian window with standard deviation 1.5. The dynamic range used in the image-quality metrics is determined from the corresponding target slice. Slice-level metrics are averaged within each case before aggregation across cases. Multi-seed estimates report the mean and sample standard deviation across the five training seeds.

Paired case analyses use the models trained with seed 2026 for CT and MRI and seed 3407 for PET. Case-bootstrap intervals use 10,000 resamples and random seed 20260708. The statistical significance level is 0.05; the paired Wilcoxon tests, Holm adjustment, and confidence-interval interpretation are specified in the main manuscript. The CT test cohort contains one case, for which the reported measurements describe that case.

B Architecture ablation

The architecture study examines propagation direction and recurrent cell (Fig. S1A), bottleneck and refinement placement (B), encoder and decoder depth (C, D), insertion mode (E), and skip pathways (F). The complete CT results are provided in Table S1. The grouped PSNR differences connect each family of alternatives to its insertion-path decision; H8 is the selected topology.

Intermediate encoder and decoder pathways provide more effective insertion sites than extending liquid modules across all feature levels. Fully serial integration also yields lower fidelity than the selected combination of serial bottleneck processing and gated feature updates. Within the skip-path variants, gated insertion at L2 and L3 gives the highest PSNR and lowest RMSE, supporting the H8 topology.

Table S1: CT architecture ablation. Results use the same Restore-RWKV reference and evaluation protocol; Δ PSNR is relative to this reference. The selected configuration is marked in bold.

Group	ID	Configuration	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$	Δ PSNR
Baseline	A-CT	Restore-RWKV, no slice-axis module	33.7642	0.9189	8.3950	0.0000
Direction/core	C1	One-direction CfC	33.7907	0.9193	8.3676	+0.0265
	C2	One-direction LTC	33.7643	0.9187	8.3928	+0.0001
	C3	Bidirectional CfC	33.8150	0.9193	8.3446	+0.0508
	C4	Bidirectional LTC	33.7694	0.9187	8.3889	+0.0052
Bottleneck/ refinement	C5	Strict encoder insertion with bottleneck CfC	33.9058	0.9204	8.2586	+0.1416
	C7	Encoder, bottleneck, and gated refinement CfC	33.9034	0.9203	8.2606	+0.1392
	C8	Parallel refinement CfC only	33.8255	0.9196	8.3355	+0.0613
Encoder depth	D1	Encoder L1 only	33.7963	0.9187	8.3639	+0.0321
	D2	Encoder L2 only	33.8975	0.9203	8.2672	+0.1333
	D3	Encoder L3 only	33.8681	0.9199	8.2937	+0.1039
	D4	Encoder L1+L2+L3	33.8854	0.9198	8.2777	+0.1212
Decoder depth	E1	Decoder L1 only	33.8195	0.9195	8.3414	+0.0553
	E2	Decoder L2 only	33.8660	0.9200	8.2967	+0.1018
	E3	Decoder L3 only	33.8617	0.9199	8.3001	+0.0975
	E4	Decoder L1+L2+L3	33.8271	0.9193	8.3330	+0.0629
Path combina- tion	F1	Encoder L2 + bottleneck + decoder L2 + gated refinement	33.9071	0.9205	8.2582	+0.1429
	F2	Encoder L2 + bottleneck + decoder L2, no refinement	33.9045	0.9204	8.2604	+0.1403
	F3	Encoder L2/L3 + bottleneck + decoder L2/L3 + gated refinement	33.8365	0.9195	8.3242	+0.0723
	F4	Encoder L2/L3 + bottleneck + decoder L2/L3, no refinement	33.8557	0.9199	8.3062	+0.0915
	F5	Encoder L2 + bottleneck + decoder L2 + serial refinement	33.9062	0.9205	8.2588	+0.1420
	F6	F5 with serial CfC on skip L2	33.8979	0.9203	8.2663	+0.1337
	G1	Fully serial encoder L2 + bottleneck + decoder L2 + refinement	33.8471	0.9200	8.3123	+0.0829

Continued on next page

Table S1 continued

Group	ID	Configuration	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$	Δ PSNR
	G2	Fully serial encoder L2 + bottleneck + decoder L2, no refinement	33.5083	0.9158	8.6396	-0.2559
	G3	Fully serial encoder L2/L3 + bottleneck + decoder L2/L3 + refinement	33.7892	0.9192	8.3691	+0.0250
	G4	Fully serial encoder L2/L3 + bottleneck + decoder L2/L3, no refinement	33.5101	0.9157	8.6380	-0.2541
Skip pathway	H1	Gated skip L1 on the F1 backbone	33.9017	0.9205	8.2630	+0.1375
	H2	Gated skip L2 on the F1 backbone	33.9017	0.9204	8.2631	+0.1375
	H3	Gated skip L3 on the F1 backbone	33.9075	0.9205	8.2576	+0.1433
	H4	Serial skip L1 on the F1 backbone	33.8811	0.9201	8.2821	+0.1169
	H5	Serial skip L3 on the F1 backbone	33.9078	0.9205	8.2577	+0.1436
	H6	Gated skip L1+L2+L3 on the F1 backbone	33.9031	0.9204	8.2615	+0.1389
	H7	Serial skip L1+L2+L3 on the F1 backbone	33.8914	0.9203	8.2732	+0.1272
	H8	Gated skip L2+L3 on the F1 backbone (selected)	33.9095	0.9205	8.2560	+0.1453
	H9	Serial skip L2+L3 on the F1 backbone	33.9085	0.9204	8.2568	+0.1443

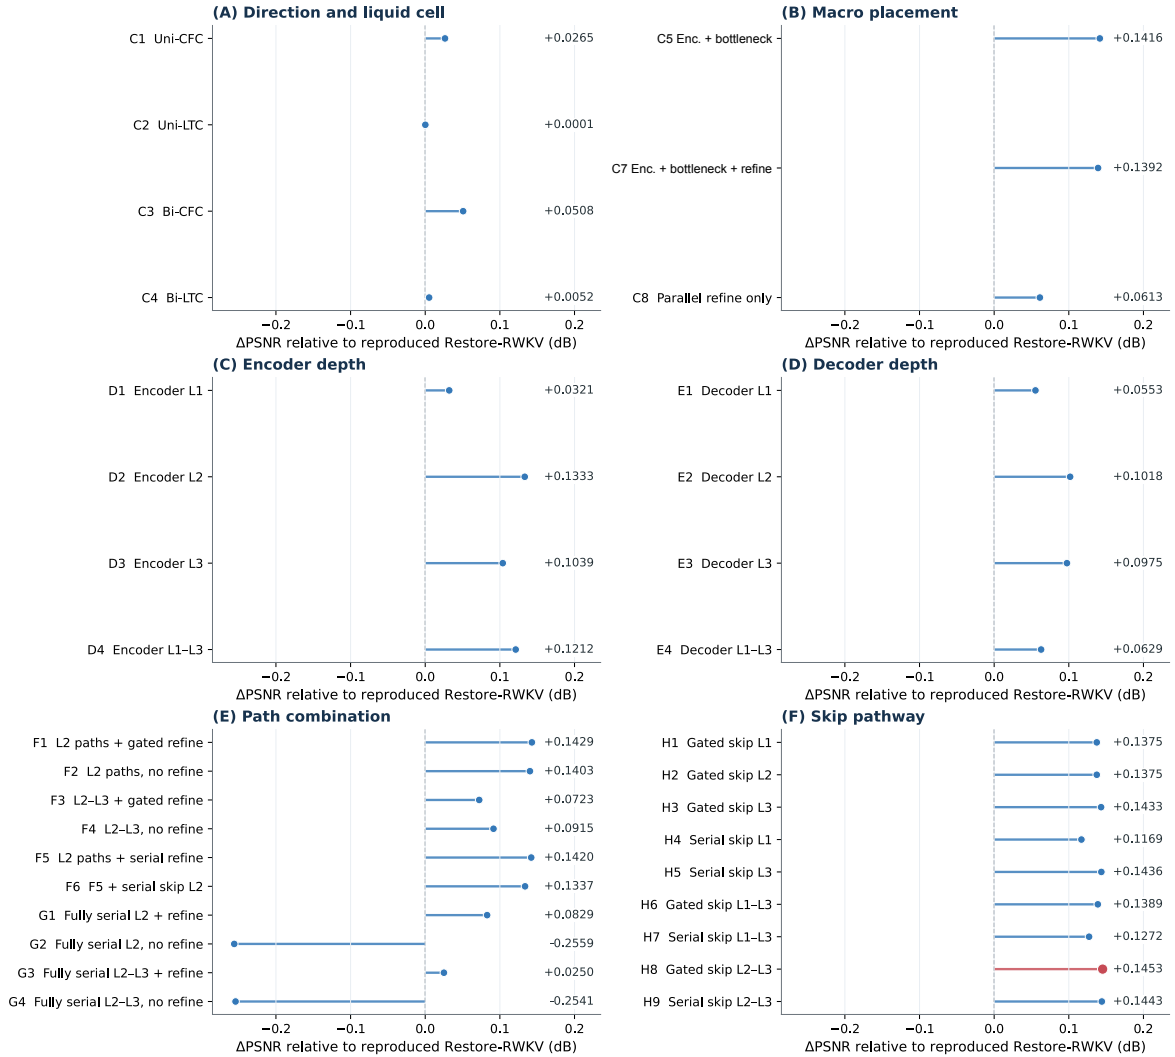


Figure S1: CT architecture ablation, expressed as PSNR differences from Restore-RWKV. (A) Propagation direction and cell type. (B) Bottleneck and refinement placement. (C, D) Encoder and decoder depth. (E) Pathway combinations. (F) Skip pathways. H8 denotes the selected topology.

C Objective decomposition

The component-wise CT ablation isolates the contribution of each supervision term under the selected architecture. Each setting in Table S2 removes one term while preserving the remaining model, initialization, and training set-

tings. Removing cross-slice consistency causes the largest PSNR reduction. The second-order term and 2D backbone distillation each provide further improvement, supporting their complementary roles under the selected architecture.

Table S2: CT loss-component ablation under the selected architecture, seed 42. Components are removed from the full objective one at a time. Bold indicates the best value in each metric column.

Setting	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$
Full objective	33.954120	0.921013	8.213643
Without distillation	33.923577	0.920509	8.241692
Without cross-slice consistency	33.874285	0.919479	8.290462
Without second-order consistency	33.910046	0.920077	8.256208

D Sequence length

The CT sequence-length study evaluates $T \in \{5, 7, 9, 11\}$ using training seed 42 and a 10-epoch budget. Validation PSNR at epochs 3, 5, and 10, the highest validation PSNR, and the test metrics are reported in Table S3. Seven slices achieved the highest validation PSNR. The validation trajectories and their highest observed values are displayed in panels A and B of Fig. S2, respectively.

Table S3: CT sequence-length analysis with training seed 42 and a 10-epoch budget. Validation and test each use one case. Bold marks the selected seven-slice window.

T	Val. epoch 3	Val. epoch 5	Val. epoch 10	Best val. (epoch)	Test PSNR	Test SSIM	Test RMSE
5	31.7210	31.7450	31.7619	31.7619 (10)	33.8825	0.9202	8.2806
7	31.7079	31.7542	31.7705	31.7719 (8)	33.8941	0.9201	8.2697
9	31.7047	31.7393	31.7574	31.7574 (10)	33.8760	0.9200	8.2865
11	31.7032	31.7311	31.7490	31.7528 (9)	33.8528	0.9194	8.3079

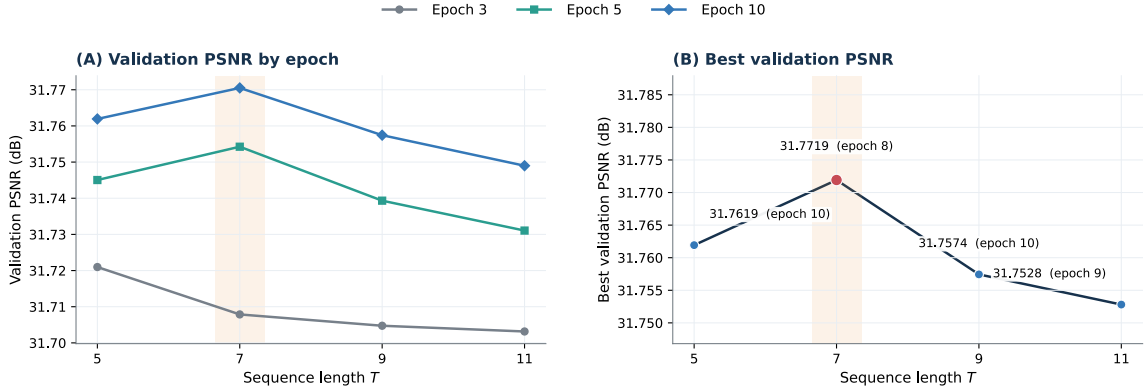


Figure S2: CT sequence-length analysis. (A) Validation PSNR at epochs 3, 5, and 10. (B) Highest validation PSNR, with the corresponding epoch annotated. Shading identifies the selected seven-slice window.

E Context perturbations

The PET context study evaluates ordered context (default), reversed local order, center repetition and nonlocal same-case sampling using the same trained ContiLNN-RWKV checkpoint. The target center image and the ten evaluated center positions within each of the 29 test scans remain fixed. Table S4 reports mean changes relative to ordered context with 95% case-bootstrap confidence intervals. Table S6 provides the 116 case-condition records, including absolute PSNR, SSIM and RMSE and signed differences from the ordered result for the same case. For these signed differences, negative PSNR or SSIM values and positive RMSE values indicate deterioration; the loss convention used in Table S4 is stated in its caption.

Table S4: PET case-level changes relative to the common ordered-context reference. The same trained checkpoint is used in all conditions. Values are means with 95% percentile confidence intervals from 10,000 case-bootstrap resamples. Positive values denote PSNR or SSIM loss, or RMSE increase. Per-case absolute metrics and signed changes are reported in Table S6.

Perturbation	PSNR loss (dB)	SSIM loss	RMSE increase
Reversed	0.2565 [0.2160, 0.2962]	0.0019 [0.0015, 0.0022]	0.0022 [0.0017, 0.0027]
Center-repeated	2.6151 [2.4952, 2.7333]	0.0178 [0.0160, 0.0197]	0.0229 [0.0211, 0.0246]
Nonlocal same-case	6.3511 [6.0307, 6.6710]	0.0750 [0.0681, 0.0820]	0.0770 [0.0725, 0.0816]

F PET Stage-A trajectory

The PET Restore-RWKV baseline completed 300,000 optimizer updates, with validation every 1,000 updates. The complete validation trajectory is provided in Fig. S3. PSNR reached its highest value of 38.1207 dB at update 87,000, with SSIM 0.9541 and root mean squared error (RMSE) 0.0813. The remaining 213 validation evaluations did not exceed that PSNR, and the checkpoint at update 87,000 was retained for subsequent refinement.

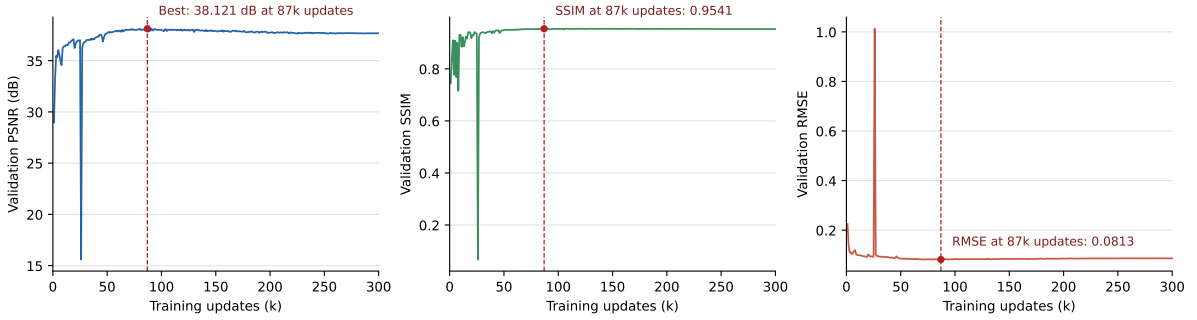


Figure S3: PET Stage-A validation trajectory across 300,000 optimizer updates. The dashed line marks the highest validation PSNR at update 87,000. All 300 recorded values are displayed for PSNR, SSIM, and RMSE.

G MRI orthogonal views

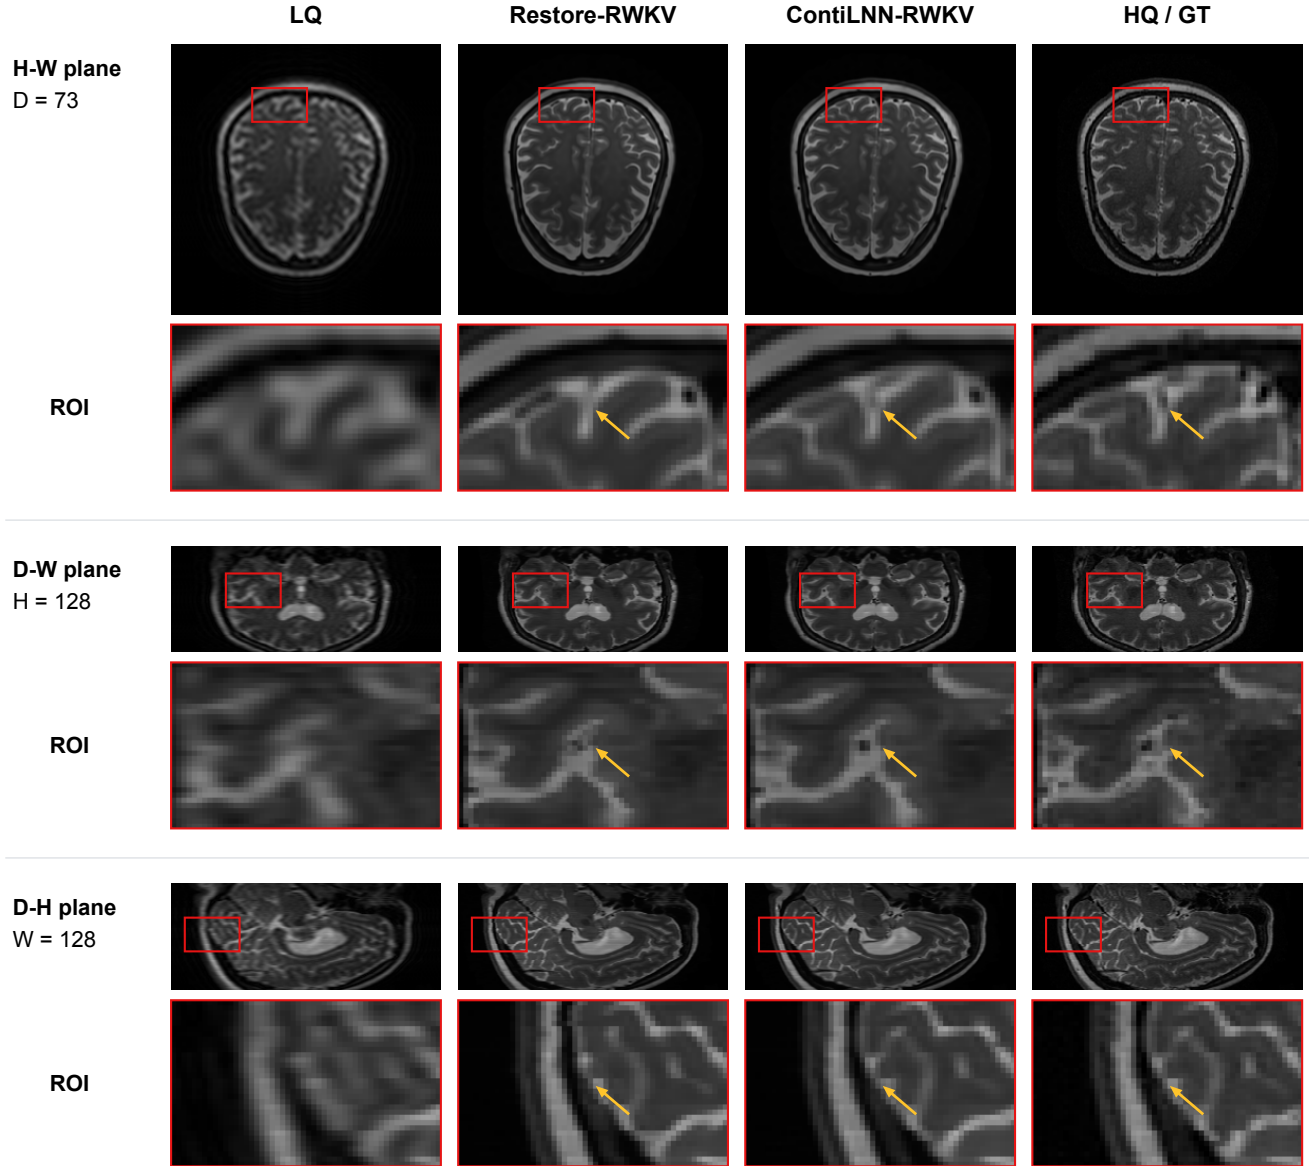


Figure S4: MRI restoration in three orthogonal index-space planes for IXI574-IOP-1156-T2. Columns show LQ, Restore-RWKV, ContiLNN-RWKV and HQ images. Red boxes mark matched regions of interest, enlarged below; yellow arrows indicate corresponding local structures. D , H and W denote slice index, row and column, respectively (zero-based). The full planes retain the complete available field of view across the 100 processed slices. All panels share the display range $[0, 4095]$ and use index-space aspect ratios; physical spacing is unavailable in the processed data.

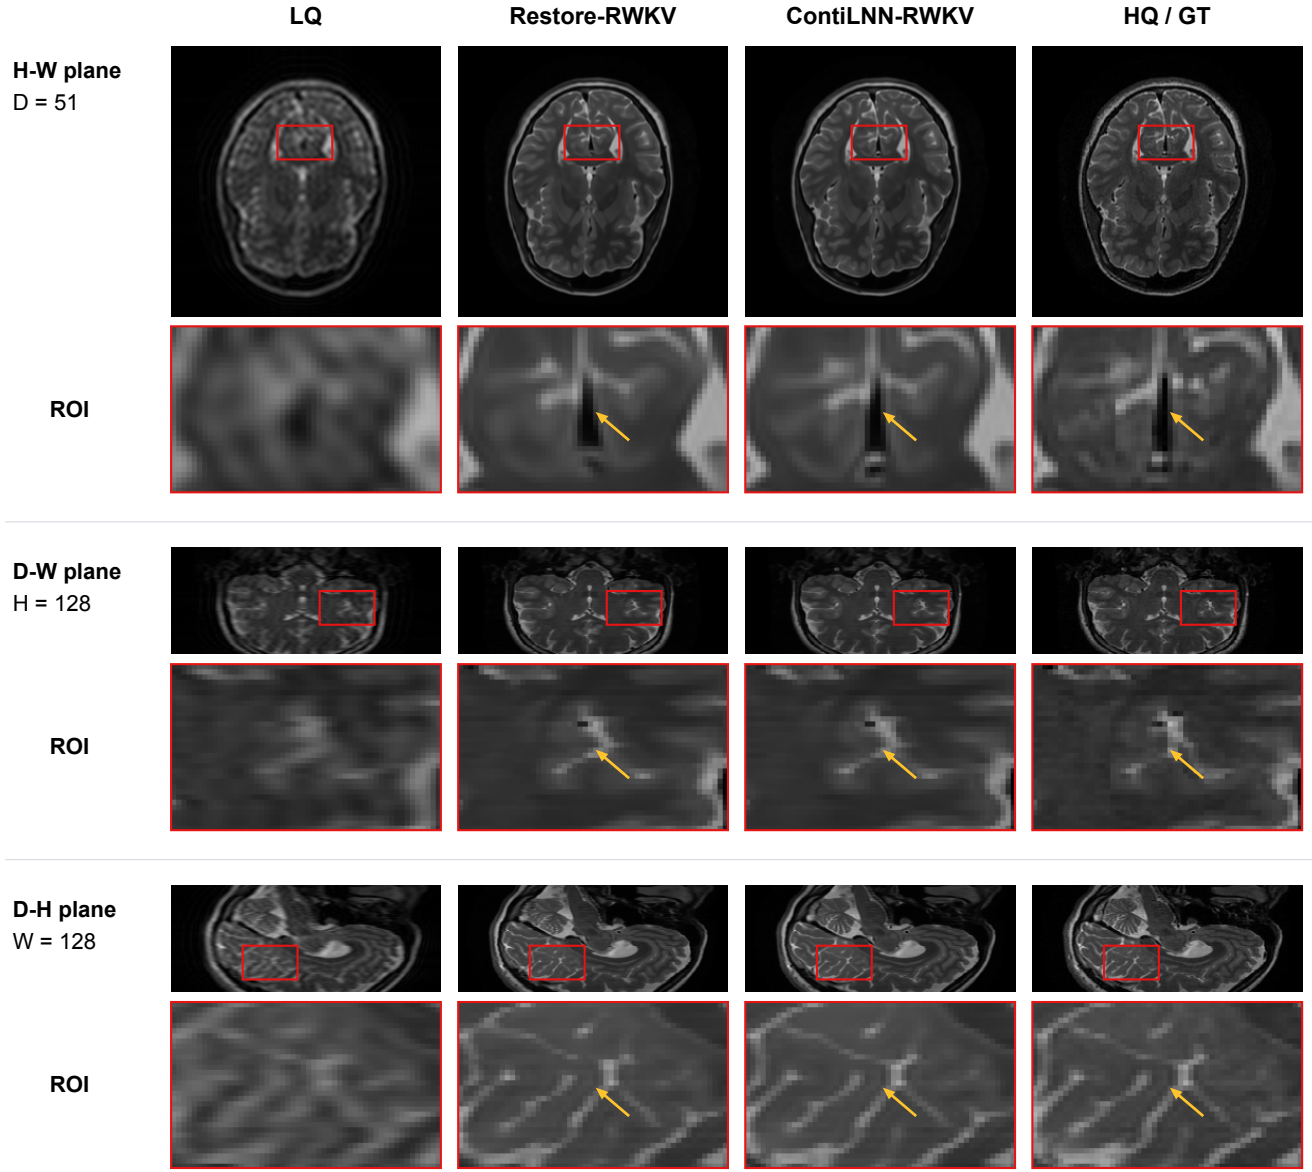


Figure S5: MRI restoration in three orthogonal index-space planes for IXI230-IOP-0869-T2. Red-boxed regions are enlarged below each full plane, with yellow arrows marking corresponding local structures. The four columns use identical coordinates and display settings. As in Fig. S4, D , H and W denote zero-based slice, row and column indices; all 100 processed slices are retained in the D -axis reformats. The display range is $[0, 4095]$, and aspect ratios follow array indices rather than physical distances.

H Additional mixed-gap training study

Mixed-gap training examines whether exposure to varied slice-index gaps improves restoration when neighboring context becomes sparse or irregular (Table S5). Relative to contiguous training, Bi-CfC gains 0.5525, 1.3300 and 0.4032 dB in PSNR at $g = 2$, $g = 3$ and irregular sampling, respectively. The corresponding gains for Bi-GRU are 0.6530, 1.4685 and 0.4535 dB. Both operators also improve in SSIM and RMSE in these three settings.

At $g = 1$, contiguous training retains PSNR advantages of 0.1568 dB for Bi-CfC and 0.0635 dB for Bi-GRU. After mixed-gap training, Bi-GRU achieves marginally higher PSNR at the three uniform gaps, whereas Bi-CfC retains higher SSIM across all four contexts and performs better in all three metrics under irregular sampling.

These results identify mixed-gap training as a complementary strategy for restoration with partially available neighboring context. The benefit extends to both sequence operators, indicating that exposure to varied training gaps contributes to the observed adaptation.

Table S5: Additional PET sampling experiments on the 29-case test cohort. Both operators are evaluated after contiguous and mixed-gap training at uniform gaps $g = 1, 2, 3$ and irregular combinations of these gaps. Mixed-gap training uses a constant gap within each window and varies the gap across windows. Bold indicates the better training strategy for each operator and test context.

Operator	Test context	Training	PSNR $\uparrow$	SSIM $\uparrow$	RMSE $\downarrow$
Bi-GRU	$g = 1$	Contiguous	38.5176	0.9538	0.0753
		Mixed-gap	38.4541	0.9522	0.0757
	$g = 2$	Contiguous	37.6217	0.9462	0.0826
		Mixed-gap	38.2747	0.9517	0.0772
	$g = 3$	Contiguous	36.5295	0.9366	0.0940
		Mixed-gap	37.9980	0.9504	0.0796
	Irregular	Contiguous	37.8544	0.9465	0.0802
		Mixed-gap	38.3080	0.9518	0.0768
Bi-CfC	$g = 1$	Contiguous	38.5868	0.9546	0.0744
		Mixed-gap	38.4301	0.9527	0.0759
	$g = 2$	Contiguous	37.7136	0.9476	0.0817
		Mixed-gap	38.2661	0.9521	0.0772
	$g = 3$	Contiguous	36.6652	0.9393	0.0927
		Mixed-gap	37.9952	0.9510	0.0796
	Irregular	Contiguous	37.9494	0.9479	0.0793
		Mixed-gap	38.3527	0.9522	0.0764

I Contiguous-training performance and inference cost

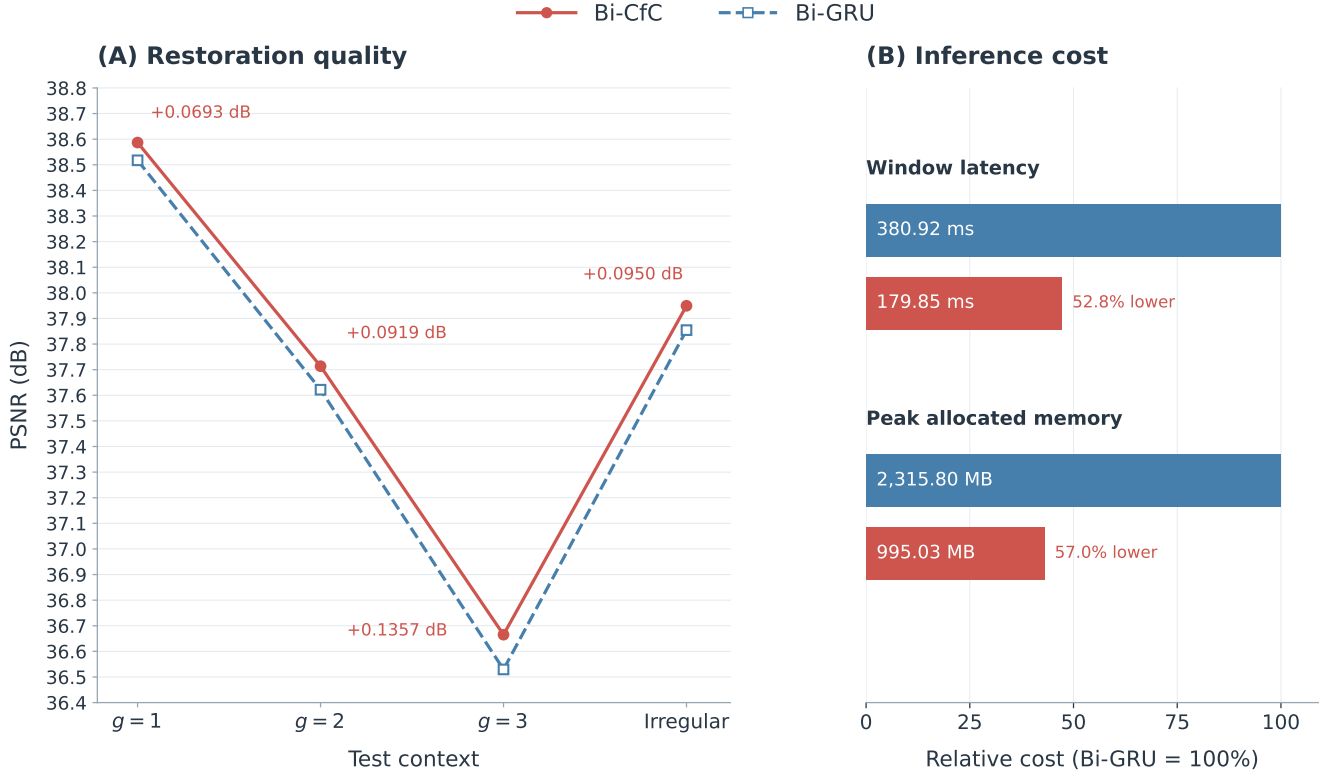


Figure S6: Bi-CfC and Bi-GRU trained on contiguous slices. (A) Mean PET PSNR across 29 test cases under four sampling conditions (main Table 2); annotations show Bi-CfC minus Bi-GRU. Lines connect categorical conditions for visual comparison. (B) Seven-slice window latency and peak allocated GPU memory under the main Table 4 profiling conditions, normalized to Bi-GRU; labels report absolute values and relative reductions.

J Case-level PET context results

Table S6: PET context-perturbation results for all 29 test cases under four conditions (116 records). Each metric is the mean over the same ten evaluated center slices within a case. Δ denotes the condition result minus the ordered-context result for the same case; negative PSNR or SSIM changes and positive RMSE changes indicate deterioration. PSNR and its change are in dB; SSIM is dimensionless and RMSE retains the original evaluation units. Metrics and differences are rounded independently to six decimal places.

Case	Context	PSNR	Δ PSNR	SSIM	Δ SSIM	RMSE	Δ RMSE
Patient 10	Ordered (default)	36.761593	0.000000	0.948692	0.000000	0.073840	0.000000
Patient 10	Reversed	36.449061	-0.312532	0.946832	-0.001860	0.077593	0.003753
Patient 10	Center-repeated	34.391667	-2.369926	0.928067	-0.020624	0.094301	0.020461
Patient 10	Nonlocal same-case	31.008852	-5.752742	0.859689	-0.089003	0.142358	0.068518
Patient 101	Ordered (default)	38.906556	0.000000	0.952976	0.000000	0.062351	0.000000
Patient 101	Reversed	38.850965	-0.055590	0.952068	-0.000908	0.062559	0.000207
Patient 101	Center-repeated	36.193087	-2.713469	0.935912	-0.017064	0.081845	0.019493
Patient 101	Nonlocal same-case	33.117327	-5.789229	0.888393	-0.064584	0.115678	0.053326
Patient 103	Ordered (default)	39.423093	0.000000	0.958721	0.000000	0.061477	0.000000
Patient 103	Reversed	39.186257	-0.236837	0.957317	-0.001405	0.063164	0.001687
Patient 103	Center-repeated	36.511077	-2.912017	0.941561	-0.017161	0.083987	0.022510
Patient 103	Nonlocal same-case	31.880395	-7.542698	0.887479	-0.071242	0.149856	0.088379
Patient 106	Ordered (default)	38.440922	0.000000	0.957367	0.000000	0.084605	0.000000
Patient 106	Reversed	38.069264	-0.371658	0.954919	-0.002448	0.087901	0.003296
Patient 106	Center-repeated	35.742716	-2.698206	0.939603	-0.017764	0.106971	0.022366
Patient 106	Nonlocal same-case	31.840640	-6.600282	0.877543	-0.079823	0.168198	0.083593
Patient 112	Ordered (default)	37.647933	0.000000	0.949370	0.000000	0.079394	0.000000
Patient 112	Reversed	37.213270	-0.434663	0.947025	-0.002346	0.084175	0.004781
Patient 112	Center-repeated	34.939279	-2.708655	0.930451	-0.018919	0.104146	0.024752
Patient 112	Nonlocal same-case	30.240319	-7.407614	0.845936	-0.103434	0.174975	0.095581
Patient 124	Ordered (default)	35.552508	0.000000	0.930709	0.000000	0.082582	0.000000
Patient 124	Reversed	35.216282	-0.336226	0.927213	-0.003497	0.085478	0.002896
Patient 124	Center-repeated	33.083976	-2.468532	0.907105	-0.023605	0.105432	0.022850
Patient 124	Nonlocal same-case	29.728979	-5.823529	0.834091	-0.096619	0.162336	0.079753
Patient 125	Ordered (default)	34.246244	0.000000	0.920016	0.000000	0.051651	0.000000
Patient 125	Reversed	33.987126	-0.259118	0.916571	-0.003445	0.053259	0.001608
Patient 125	Center-repeated	32.412747	-1.833497	0.903842	-0.016174	0.062665	0.011014
Patient 125	Nonlocal same-case	29.153594	-5.092650	0.833906	-0.086110	0.092980	0.041330
Patient 126	Ordered (default)	34.311084	0.000000	0.927582	0.000000	0.096870	0.000000
Patient 126	Reversed	34.131184	-0.179900	0.924329	-0.003253	0.099125	0.002254
Patient 126	Center-repeated	32.056365	-2.254719	0.899263	-0.028319	0.123565	0.026695
Patient 126	Nonlocal same-case	29.613399	-4.697686	0.810051	-0.117531	0.166570	0.069699
Patient 129	Ordered (default)	35.778501	0.000000	0.937247	0.000000	0.079079	0.000000
Patient 129	Reversed	35.400782	-0.377718	0.934703	-0.002544	0.083189	0.004110
Patient 129	Center-repeated	33.405693	-2.372808	0.916115	-0.021132	0.100654	0.021576
Patient 129	Nonlocal same-case	30.415584	-5.362917	0.836156	-0.101091	0.146956	0.067877
Patient 142	Ordered (default)	35.583863	0.000000	0.937662	0.000000	0.077916	0.000000
Patient 142	Reversed	35.191704	-0.392158	0.934590	-0.003072	0.081630	0.003714
Patient 142	Center-repeated	33.089205	-2.494658	0.913623	-0.024039	0.100648	0.022732
Patient 142	Nonlocal same-case	30.329091	-5.254772	0.847152	-0.090510	0.143359	0.065443
Patient 145	Ordered (default)	38.446787	0.000000	0.959709	0.000000	0.075416	0.000000
Patient 145	Reversed	38.160992	-0.285794	0.957976	-0.001733	0.078248	0.002832
Patient 145	Center-repeated	35.758012	-2.688774	0.942517	-0.017193	0.099953	0.024537
Patient 145	Nonlocal same-case	31.776824	-6.669962	0.867212	-0.092497	0.158932	0.083515
Patient 146	Ordered (default)	37.617776	0.000000	0.951471	0.000000	0.098457	0.000000
Patient 146	Reversed	37.203507	-0.414269	0.949493	-0.001978	0.103322	0.004865
Patient 146	Center-repeated	35.446814	-2.170962	0.934857	-0.016614	0.121174	0.022717
Patient 146	Nonlocal same-case	32.671686	-4.946090	0.888647	-0.062825	0.165737	0.067280
Patient 15	Ordered (default)	40.962795	0.000000	0.971458	0.000000	0.075801	0.000000
Patient 15	Reversed	40.712937	-0.249859	0.969814	-0.001644	0.078246	0.002445
Patient 15	Center-repeated	38.253667	-2.709128	0.956811	-0.014647	0.103506	0.027705
Patient 15	Nonlocal same-case	34.631902	-6.330893	0.923857	-0.047601	0.158798	0.082997
Patient 150	Ordered (default)	38.129044	0.000000	0.955725	0.000000	0.077390	0.000000
Patient 150	Reversed	37.880455	-0.248589	0.953694	-0.002030	0.078965	0.001575
Patient 150	Center-repeated	35.868792	-2.260253	0.936367	-0.019358	0.095018	0.017628
Patient 150	Nonlocal same-case	32.463270	-5.665774	0.872491	-0.083234	0.141190	0.063800

Continued on the next page

Table S6 continued

Case	Context	PSNR	Δ PSNR	SSIM	Δ SSIM	RMSE	Δ RMSE
Patient 158	Ordered (default)	35.070730	0.000000	0.931075	0.000000	0.103789	0.000000
Patient 158	Reversed	34.668173	-0.402558	0.926429	-0.004646	0.107839	0.004050
Patient 158	Center-repeated	32.009709	-3.061022	0.899749	-0.031326	0.140108	0.036318
Patient 158	Nonlocal same-case	29.852387	-5.218343	0.833674	-0.097401	0.188120	0.084331
Patient 20	Ordered (default)	39.811874	0.000000	0.971265	0.000000	0.092518	0.000000
Patient 20	Reversed	39.621685	-0.190189	0.970323	-0.000942	0.093760	0.001242
Patient 20	Center-repeated	37.181179	-2.630695	0.960268	-0.010997	0.122151	0.029633
Patient 20	Nonlocal same-case	33.928895	-5.882979	0.924185	-0.047080	0.176277	0.083759
Patient 3	Ordered (default)	41.752468	0.000000	0.977102	0.000000	0.064732	0.000000
Patient 3	Reversed	41.638737	-0.113731	0.976417	-0.000685	0.065159	0.000428
Patient 3	Center-repeated	39.191530	-2.560938	0.966135	-0.010968	0.086218	0.021486
Patient 3	Nonlocal same-case	34.790951	-6.961518	0.914884	-0.062218	0.142699	0.077967
Patient 34	Ordered (default)	42.556716	0.000000	0.978345	0.000000	0.070179	0.000000
Patient 34	Reversed	42.264116	-0.292600	0.977177	-0.001167	0.072261	0.002082
Patient 34	Center-repeated	39.723645	-2.833071	0.970473	-0.007872	0.096387	0.026208
Patient 34	Nonlocal same-case	35.095562	-7.461154	0.928046	-0.050299	0.166897	0.096718
Patient 36	Ordered (default)	39.139292	0.000000	0.949931	0.000000	0.068756	0.000000
Patient 36	Reversed	39.024307	-0.114985	0.949092	-0.000839	0.069624	0.000868
Patient 36	Center-repeated	37.091457	-2.047835	0.937786	-0.012145	0.085815	0.017059
Patient 36	Nonlocal same-case	31.942837	-7.196455	0.884026	-0.065905	0.158198	0.089442
Patient 41	Ordered (default)	38.679674	0.000000	0.960796	0.000000	0.064076	0.000000
Patient 41	Reversed	38.537203	-0.142472	0.959681	-0.001115	0.065132	0.001057
Patient 41	Center-repeated	36.102895	-2.576779	0.944291	-0.016505	0.083653	0.019577
Patient 41	Nonlocal same-case	32.834068	-5.845606	0.900435	-0.060361	0.127958	0.063882
Patient 65	Ordered (default)	41.390868	0.000000	0.969749	0.000000	0.070523	0.000000
Patient 65	Reversed	41.104567	-0.286300	0.968606	-0.001143	0.072962	0.002439
Patient 65	Center-repeated	38.271384	-3.119483	0.953104	-0.016645	0.097286	0.026763
Patient 65	Nonlocal same-case	33.550288	-7.840580	0.893146	-0.076603	0.171536	0.101013
Patient 68	Ordered (default)	43.532892	0.000000	0.976940	0.000000	0.071733	0.000000
Patient 68	Reversed	43.363515	-0.169377	0.976288	-0.000652	0.073002	0.001269
Patient 68	Center-repeated	40.414518	-3.118374	0.964177	-0.012763	0.099909	0.028176
Patient 68	Nonlocal same-case	36.863854	-6.669038	0.926691	-0.050249	0.153561	0.081828
Patient 78	Ordered (default)	40.748344	0.000000	0.965842	0.000000	0.077276	0.000000
Patient 78	Reversed	40.389416	-0.358928	0.963137	-0.002705	0.080435	0.003159
Patient 78	Center-repeated	37.941662	-2.806682	0.943516	-0.022327	0.105228	0.027951
Patient 78	Nonlocal same-case	34.737163	-6.011181	0.919173	-0.046669	0.159874	0.082597
Patient 88	Ordered (default)	37.900479	0.000000	0.945639	0.000000	0.067376	0.000000
Patient 88	Reversed	37.785339	-0.115139	0.944122	-0.001518	0.067898	0.000522
Patient 88	Center-repeated	35.205895	-2.694584	0.924304	-0.021335	0.087426	0.020050
Patient 88	Nonlocal same-case	31.105505	-6.794974	0.871470	-0.074169	0.147157	0.079781
Patient 90	Ordered (default)	40.654854	0.000000	0.955710	0.000000	0.061844	0.000000
Patient 90	Reversed	40.265983	-0.388872	0.953713	-0.001997	0.064289	0.002445
Patient 90	Center-repeated	37.573345	-3.081509	0.939819	-0.015891	0.083660	0.021817
Patient 90	Nonlocal same-case	33.090787	-7.564067	0.880834	-0.074876	0.138461	0.076617
Patient 94	Ordered (default)	41.247117	0.000000	0.962865	0.000000	0.064122	0.000000
Patient 94	Reversed	40.966248	-0.280869	0.961544	-0.001321	0.066236	0.002114
Patient 94	Center-repeated	38.533897	-2.713220	0.950953	-0.011912	0.085782	0.021661
Patient 94	Nonlocal same-case	34.509461	-6.737656	0.906964	-0.055901	0.142272	0.078150
Patient 95	Ordered (default)	38.715439	0.000000	0.953354	0.000000	0.068347	0.000000
Patient 95	Reversed	38.610673	-0.104766	0.952163	-0.001192	0.069059	0.000712
Patient 95	Center-repeated	35.812634	-2.902805	0.932745	-0.020610	0.092550	0.024203
Patient 95	Nonlocal same-case	31.746436	-6.969003	0.870358	-0.082997	0.148146	0.079799
Patient 96	Ordered (default)	39.941632	0.000000	0.965331	0.000000	0.059480	0.000000
Patient 96	Reversed	39.860771	-0.080861	0.964630	-0.000701	0.059839	0.000360
Patient 96	Center-repeated	37.788493	-2.153139	0.951008	-0.014322	0.073622	0.014142
Patient 96	Nonlocal same-case	32.825961	-7.115670	0.891644	-0.073686	0.132477	0.072998
Patient 98	Ordered (default)	39.924393	0.000000	0.956135	0.000000	0.063137	0.000000
Patient 98	Reversed	39.682137	-0.242256	0.954499	-0.001636	0.064639	0.001502
Patient 98	Center-repeated	37.042061	-2.882332	0.938419	-0.017716	0.083982	0.020845
Patient 98	Nonlocal same-case	32.948196	-6.976197	0.886951	-0.069183	0.137132	0.073995