


## **Supplementary Information**

### **Accelerated Diffusion Weighted Magnetic Resonance Imaging at 7 T: Joint Reconstruction for Shift-Encoded Navigator-based Interleaved Echo Planar Imaging (JETS-NAViEPI)**


Zhengguo Tan, Patrick A. Liebig, Robin M. Heidemann, Frederik B. Laun, Florian Knoll

Here we aim to reproduce the results. Another subject was recruited and measured by all protocols listed in Table 1 in the main manuscript.


**8th DW image from 4-shot iEPI @ 1 mm ISO**

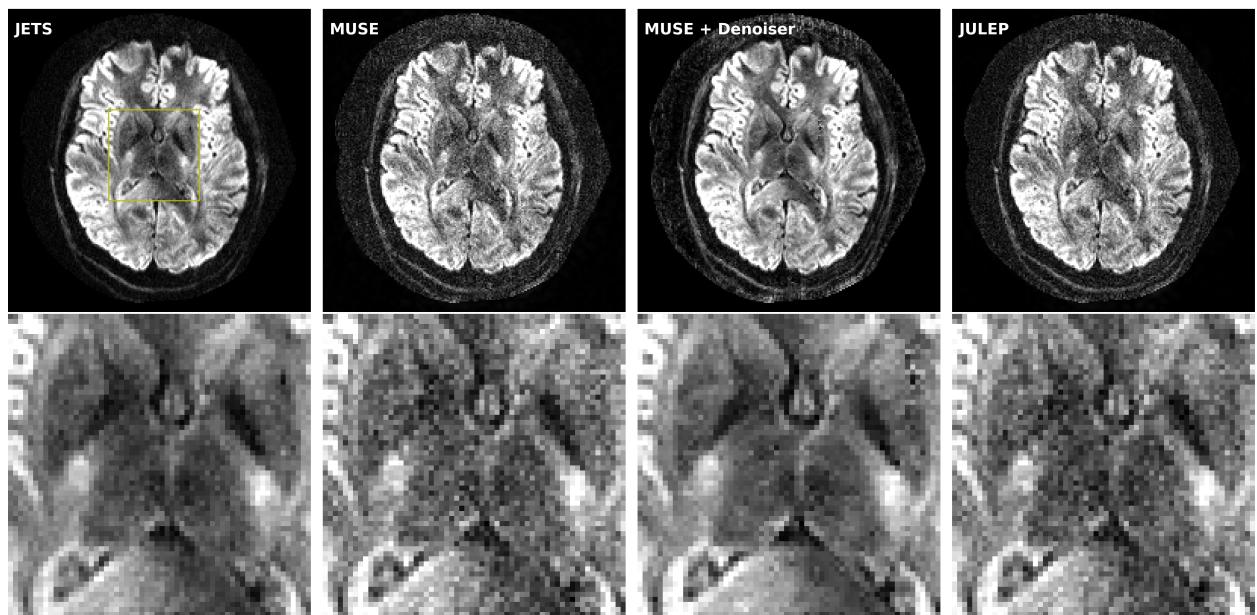


SI Figure S1: Reproducing Protocol #1. Reconstructed DW images (the 8th diffusion encoding) based on 4-shot iEPI acquisition with 1 mm isotropic resolution. Four reconstruction methods are compared (from left to right): JETS, MUSE, MUSE with denoiser, and JULEP. The 2nd row displays the magnified views of the yellow square.

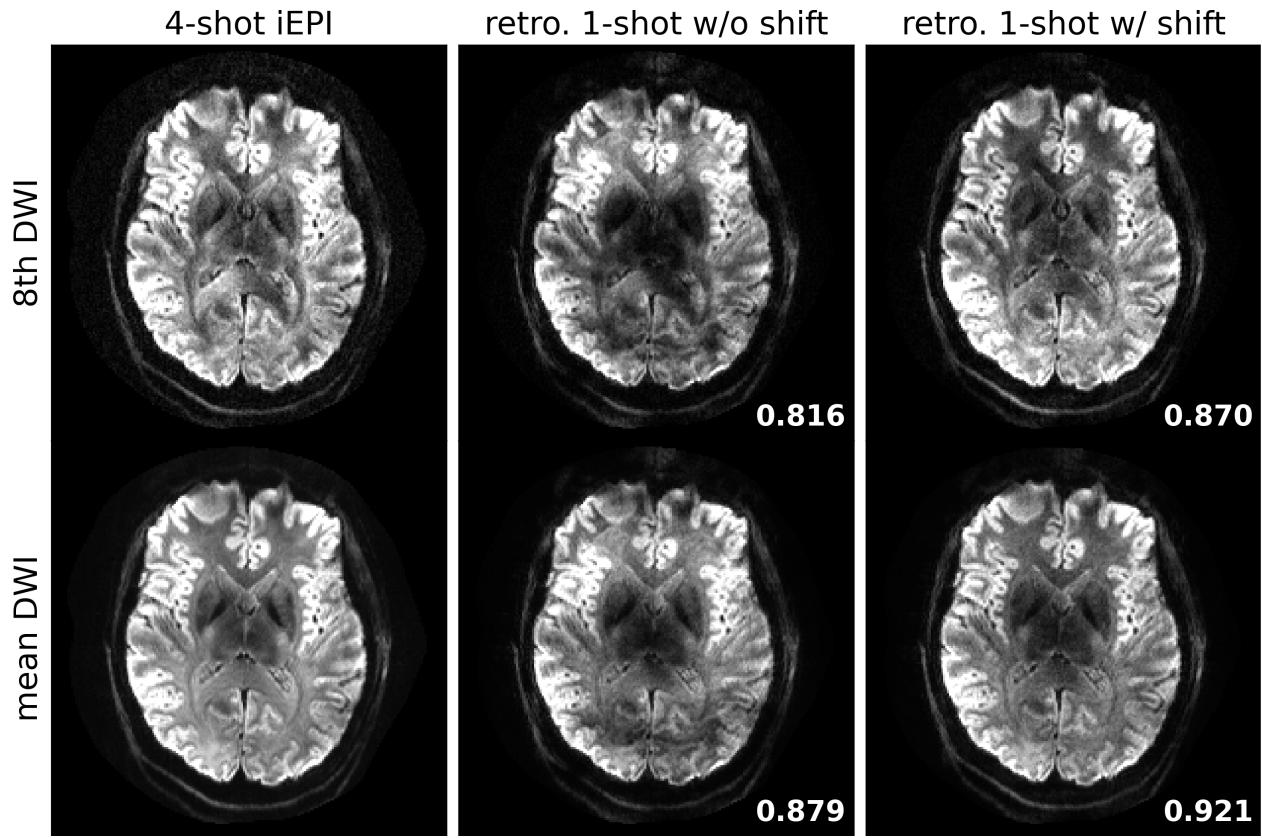


SI Figure S2: Reproducing Protocol #1. Quantitative validation of the proposed  $k_y$ -shift encoding sampling pattern based on 4-shot iEPI acquisition with 1 mm isotropic resolution. (Top) the 8th diffusion encoding and (bottom) mean DWI over 20 diffusion encodings. (1st column) JETS reconstruction of 4-shot iEPI acquisition is used as the ground truth. The 2nd and the 3rd column displays JETS reconstruction of retrospectively undersampled 1-shot acquisition without and with  $k_y$  shifting, respectively.

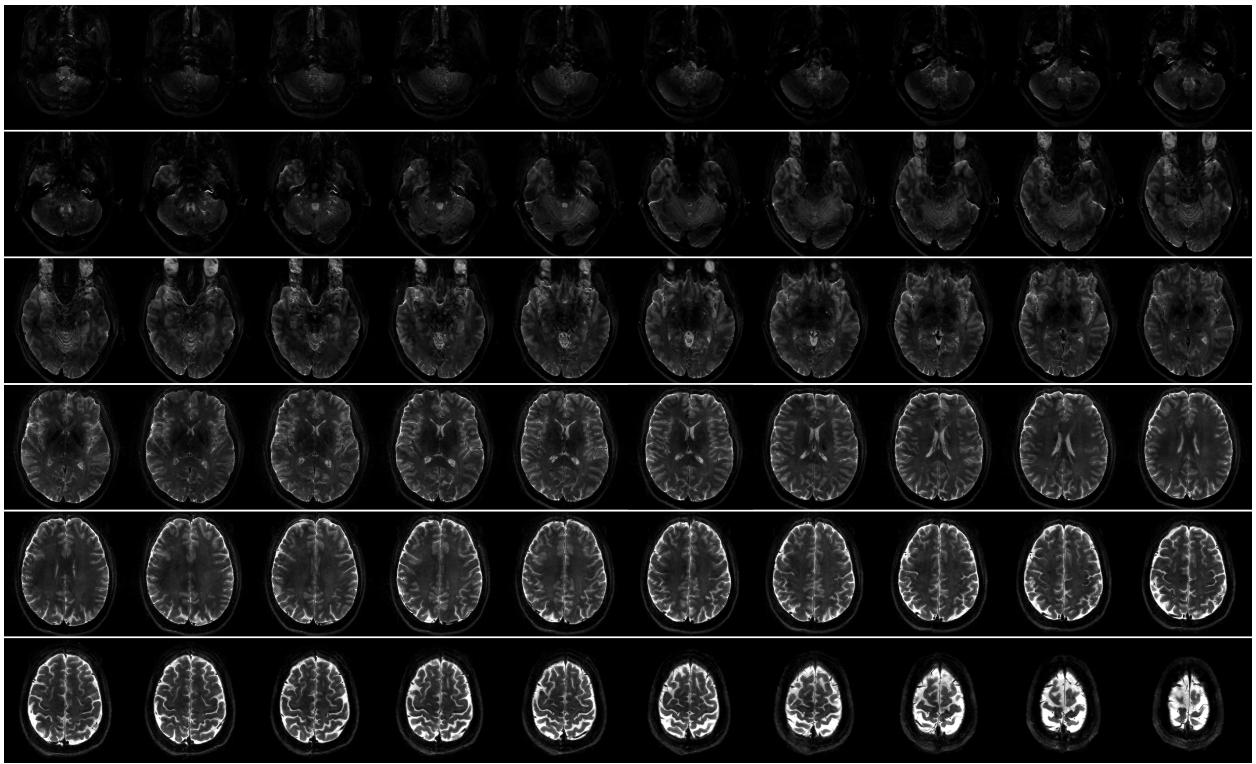

SI Figure S3: Reproducing Protocol #3. Reconstructed  $b_0$  images from the 3-scan trace acquisition with the voxel size  $0.5 \times 0.5 \times 2.0 \text{ mm}^3$ .

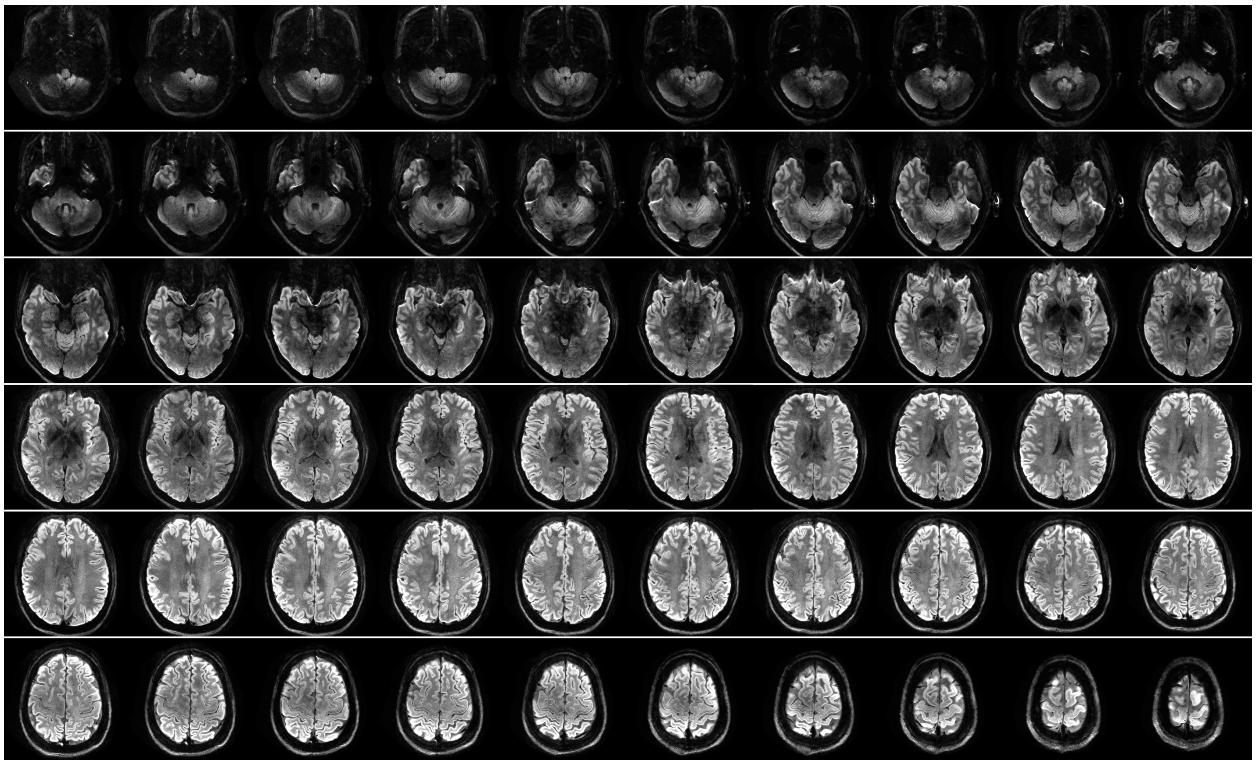

SI Figure S4: Reproducing Protocol #3. Reconstructed TRACE images from the 3-scan trace acquisition with the voxel size  $0.5 \times 0.5 \times 2.0 \text{ mm}^3$ .

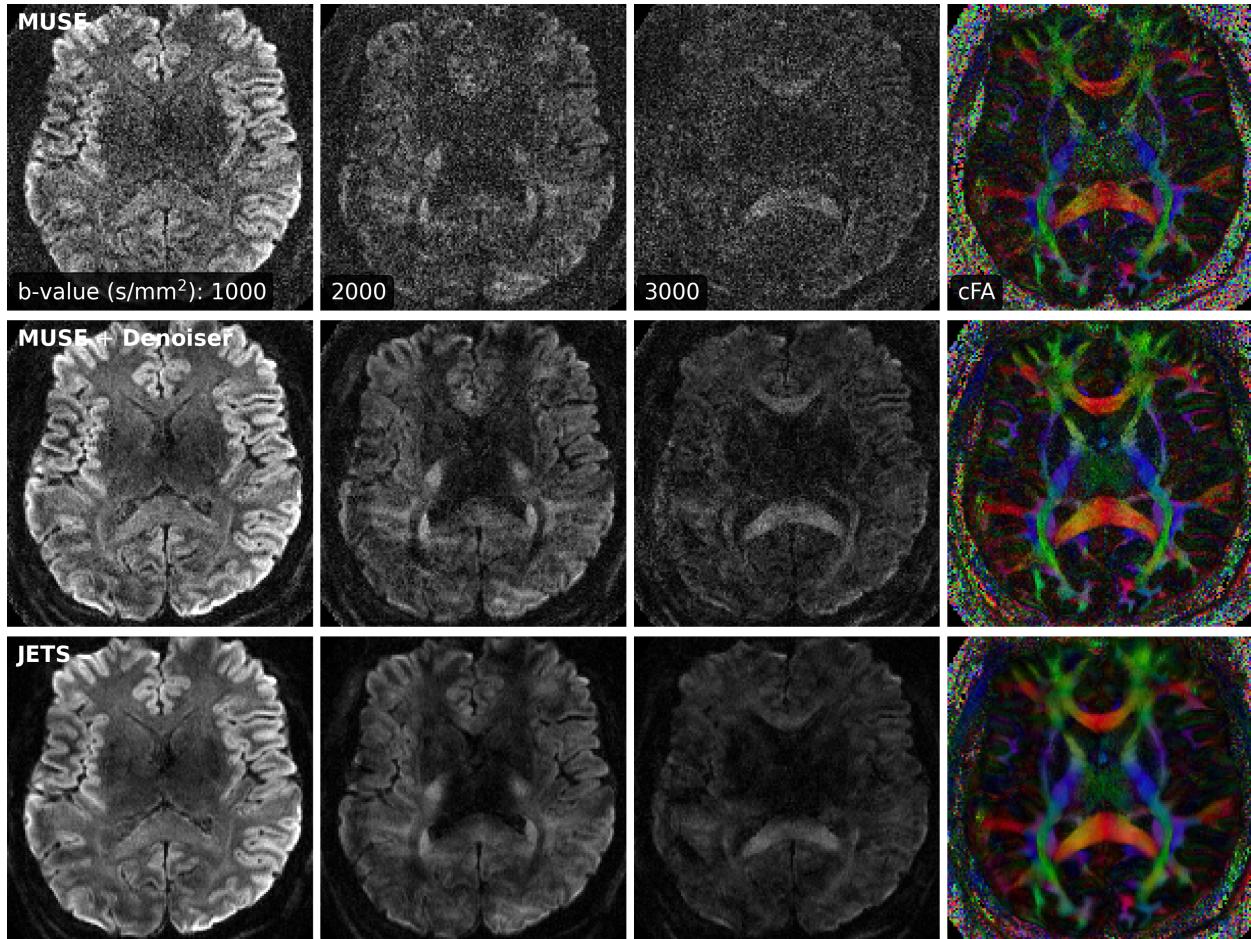

SI Figure S5: Reproducing Protocol #2. The FOV and bandwidth were adapted as 200 mm and 1086 Hz/pixel, respectively. Comparison of three-shell DWIs and cFA maps reconstructed by (top to bottom) MUSE, MUSE with the local-PCA denoiser, and the proposed JETS method, respectively.