



# Normalized Maximum Temperature Rise by Implant Configuration

(a) 12.7 cm Ti-rod

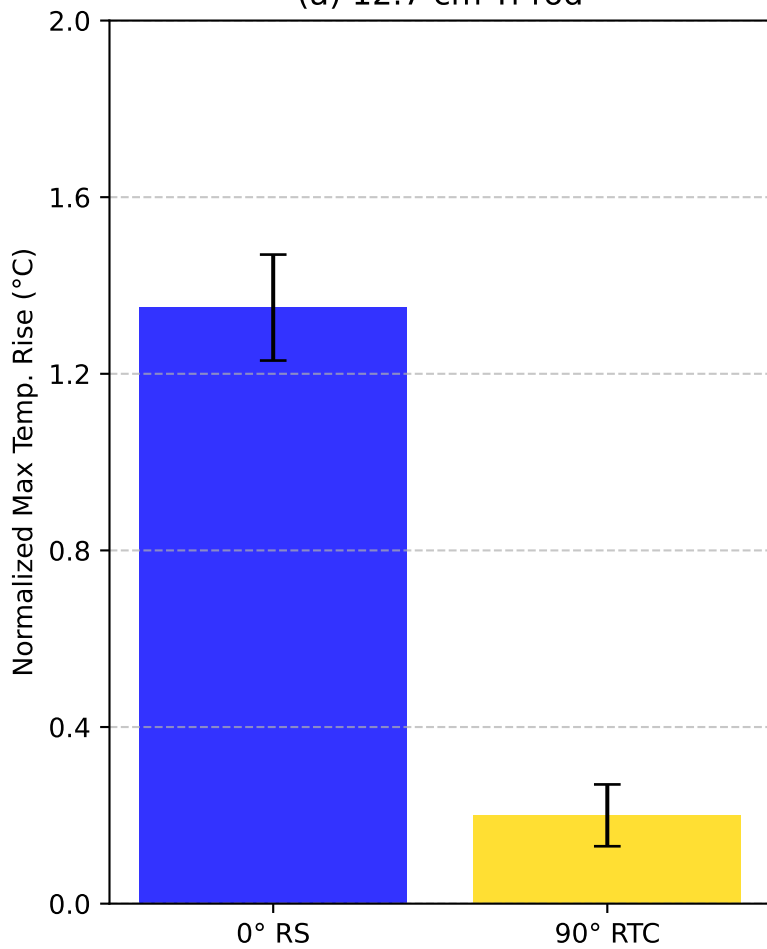

(b) 19 cm Bipolar Lead

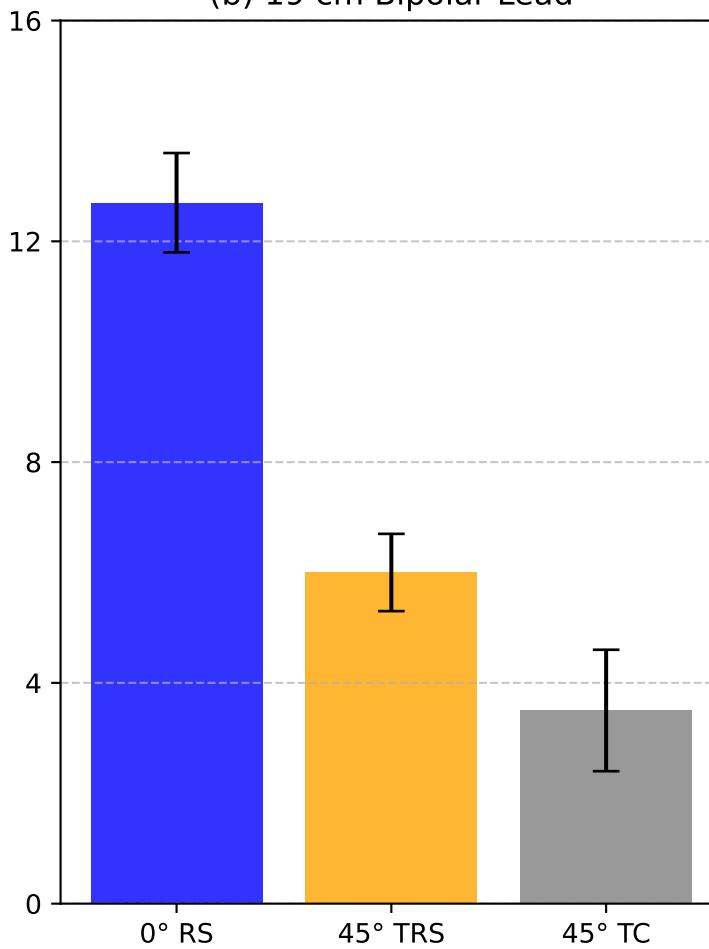

(c) 19 cm Bipolar Lead

