HridayMitra custom hardware: 8-electrode bioimpedance front end + ESP32 (legs path shown)

Bottom row: LTspice at each test point (legs path, 5 kHz, 1 kΩ skin contacts). Result: Z = 578.4 Ω (exact 578.5 Ω). Same values as the KiCad schematic (ERC 0) and the LTspice netlists. Monitoring, not diagnosis.

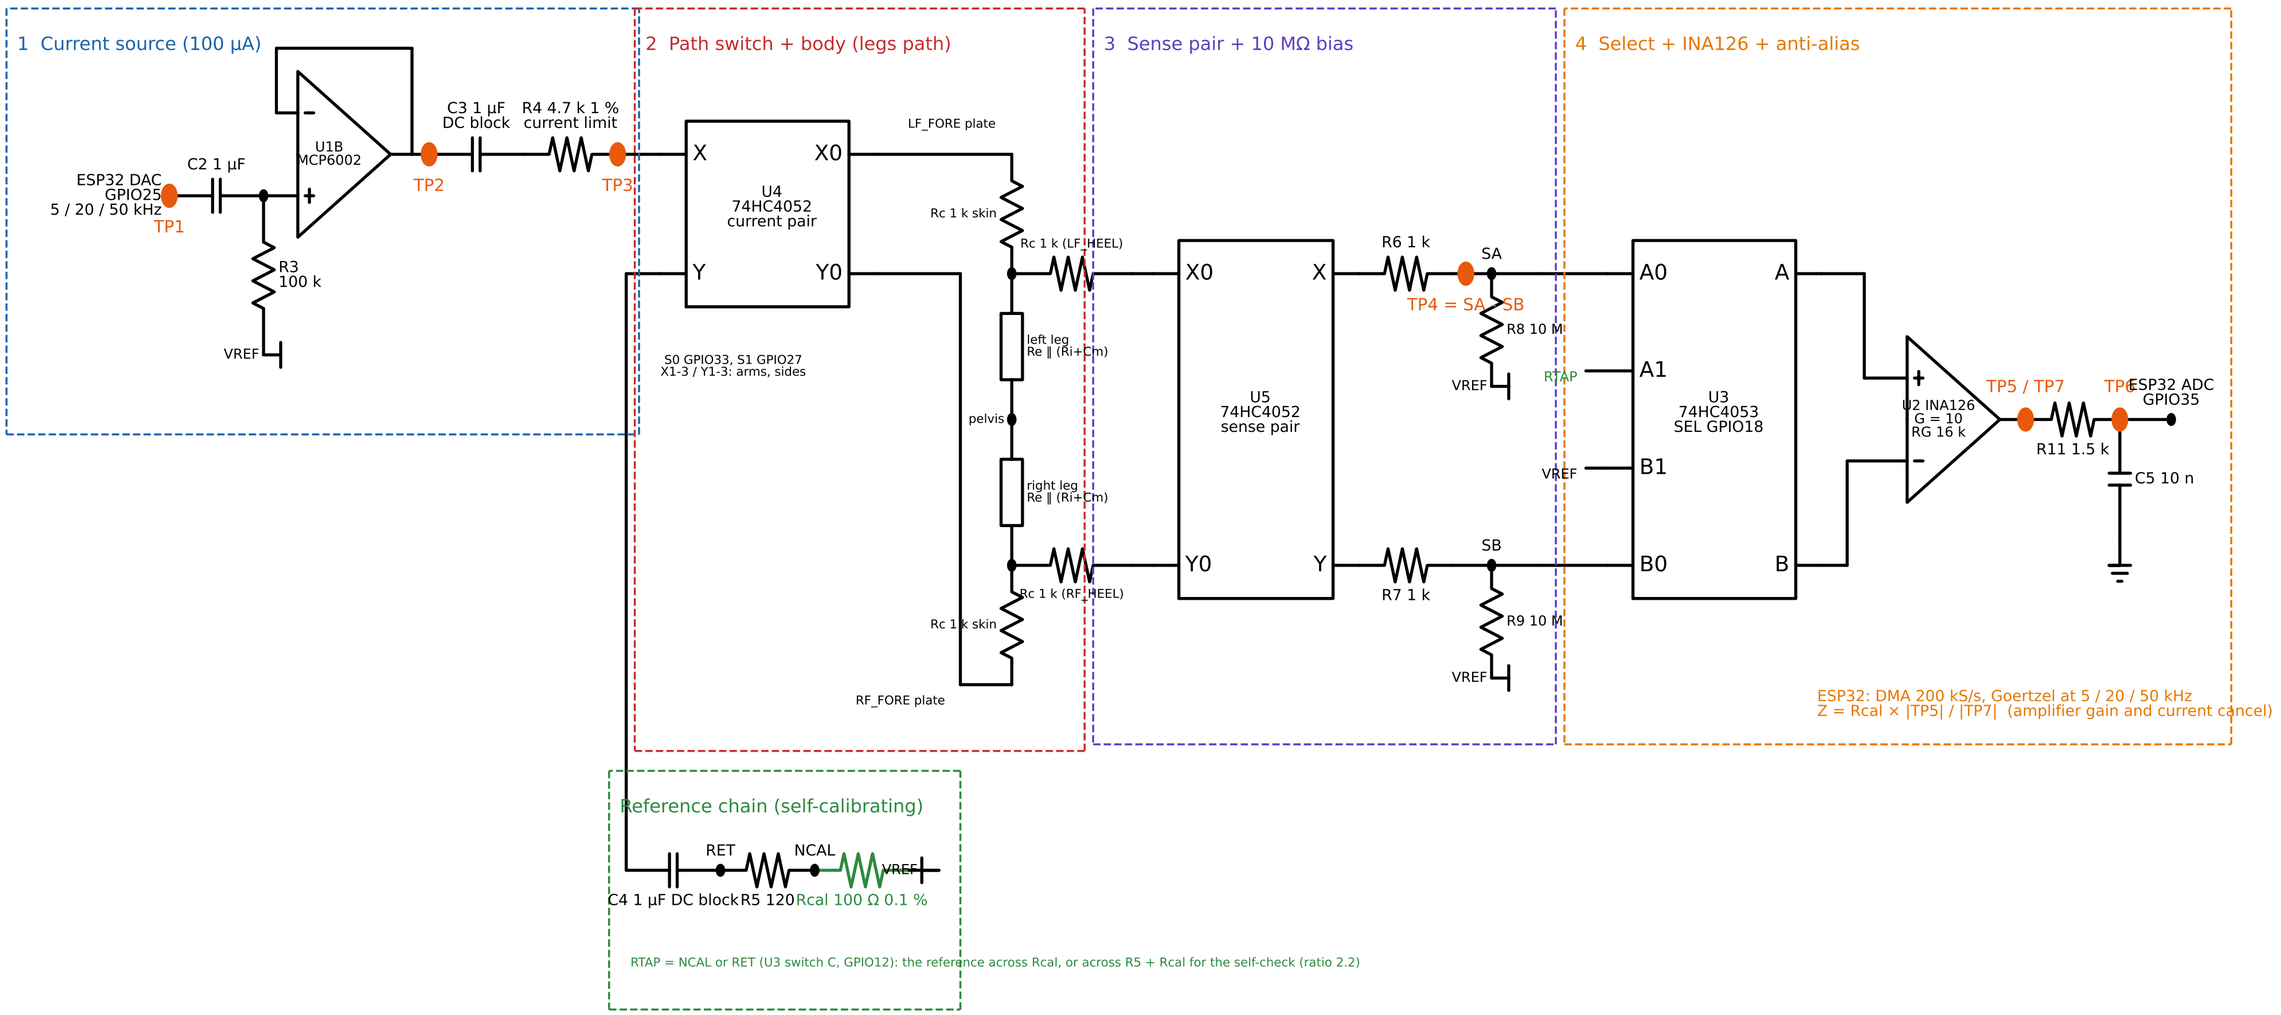
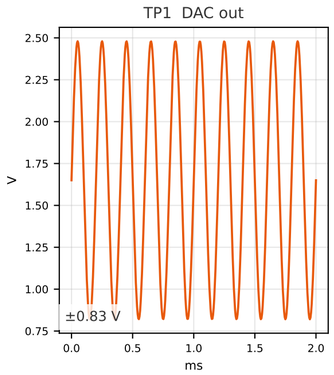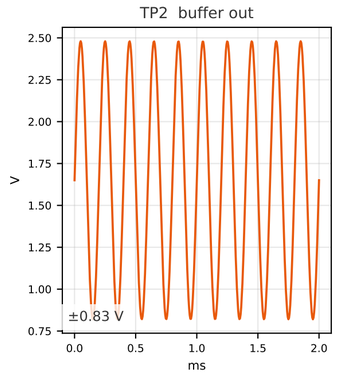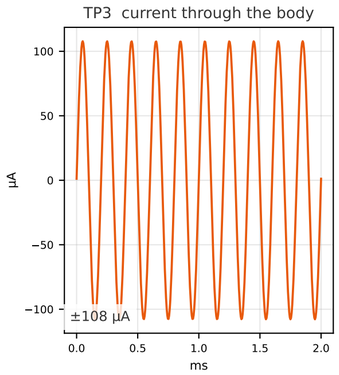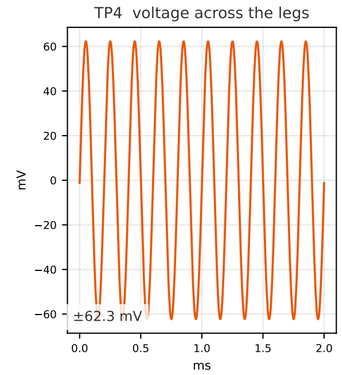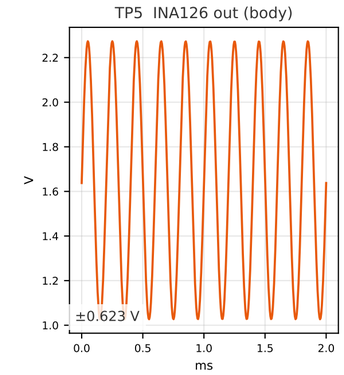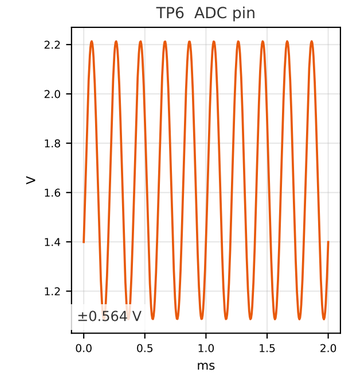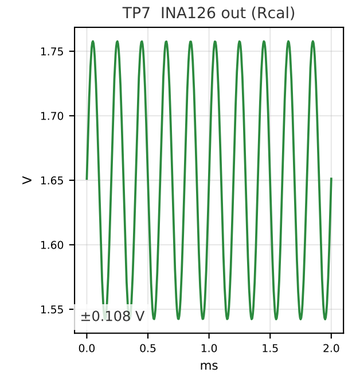
Patient safety (IEC 60601-1 type BF, LTspice): C3 and C4 in series block DC; R4 limits the current; every single fault stays ≥ 12.8× under the limit. CHARGE / USE switch (SW6) cuts both charger wires while measuring: leakage 0.19 µA instead of 339 µA.