


EMG recording and analysis report

Generated on: 2026-09-14 10:06

Test identifier: P01

File: ejemplo.edf

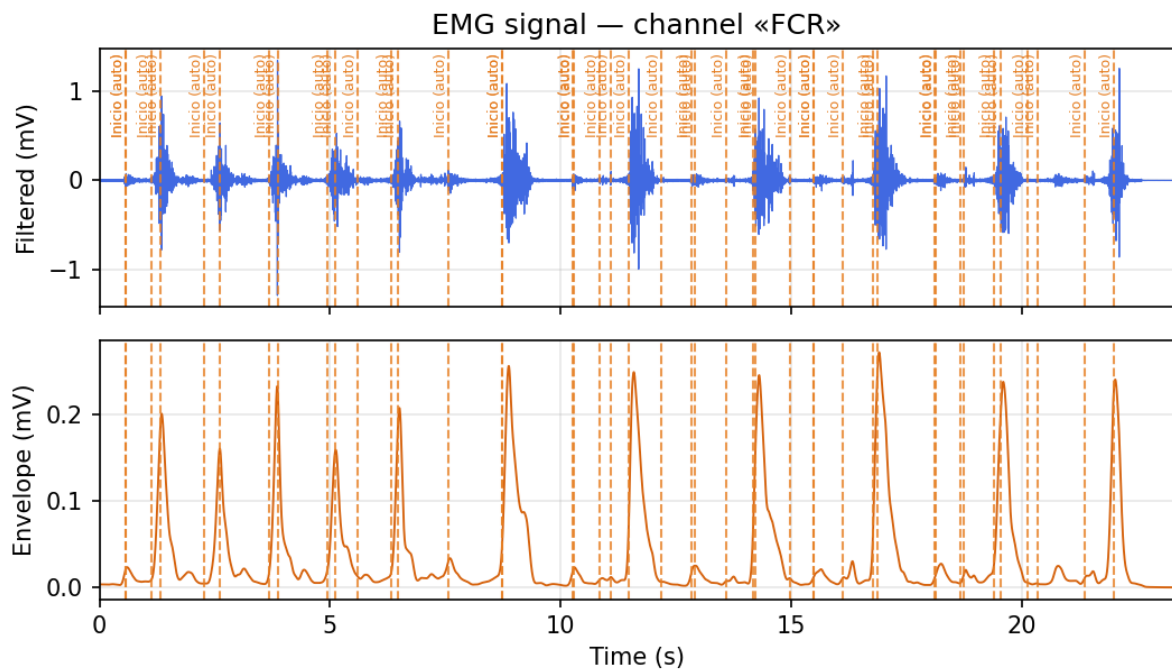

Metrics

Metric	Value
Duration	23.3 s
Analysed window	116.70-140.00 s of 140.0 s
Global RMS	0.0876 mV
Mean frequency (MNF)	142.3 Hz
Median frequency (MDF)	126.5 Hz
iEMG	0.806 mV·s
Fatigue evidence	Not conclusive — the trend does not fit (+0.22 Hz/s, $R^2=0.01$). Fatigue needs a con

Calibration (maximal voluntary contraction)


Muscle	Reference	Source
FCR	0.271 mV	calibration in this recording
ECR	0.197 mV	calibration in this recording

Calibration repetitions

Muscle	Repetition	Value
FCR	1	0.271 mV
FCR	2	0.220 mV
FCR	3	0.193 mV

FCR	4	0.166 mV
FCR	5	0.157 mV
FCR	6	0.200 mV
ECR	1	0.160 mV
ECR	2	0.138 mV
ECR	3	0.197 mV
ECR	4	0.159 mV
ECR	5	0.178 mV
ECR	6	0.163 mV

Contractions

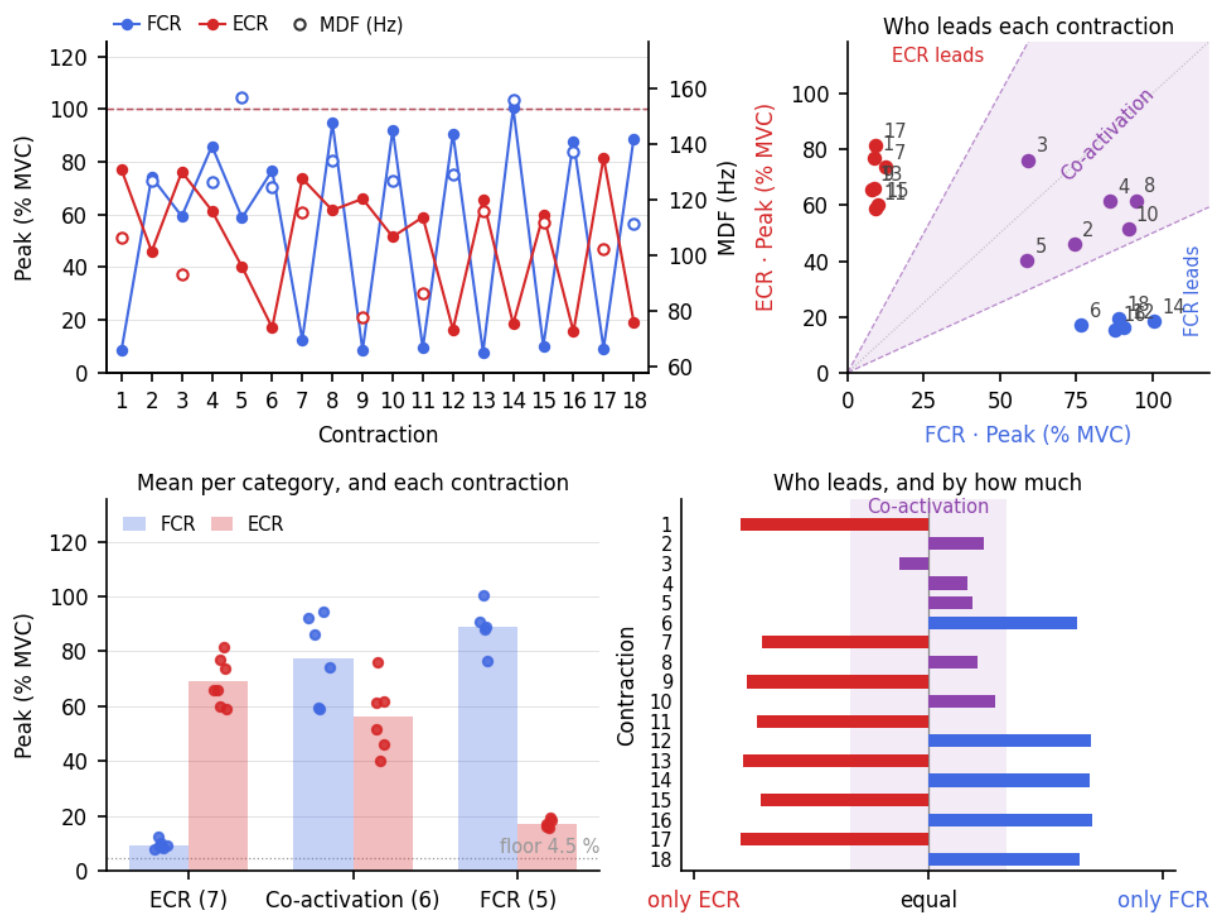

#	Start (s)	Duration (s)
1	0.5	0.42
2	1.2	1.02
3	2.4	0.95
4	3.7	0.97
5	4.9	1.05
6	6.3	0.54
7	7.2	0.63
8	8.6	0.75
9	10.2	0.52

10	11.4	0.65
11	12.8	0.55
12	14.1	0.75
13	15.4	0.57
14	16.7	0.75
15	18.1	0.54
16	19.3	0.72
17	20.1	1.20
18	21.5	1.12

Co-activation (Falconer-Winter)

Whole recording — accept the fragments for one value per window

Window	FCR — Mean activation (%)	EMG — Mean activation (%)	CMC — Co-activation index
Whole recording (0.0–23.3 s)	12	10	31 %

Configuration used

Parameter	Value
Sampling rate	1000 Hz
Channel	FCR
Band-pass	20.0-450.0 Hz
Notch (mains)	50.0 Hz
Envelope (low-pass)	5.0 Hz
RMS window	50.0 ms
Detection sensitivity (k)	4.4
Device	not stored in the EDF