
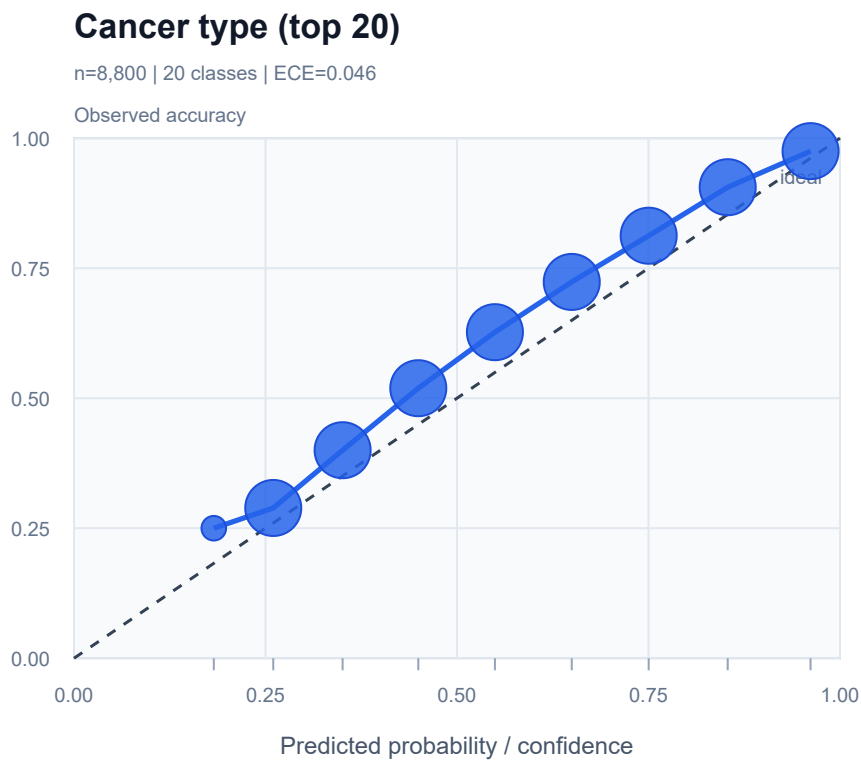
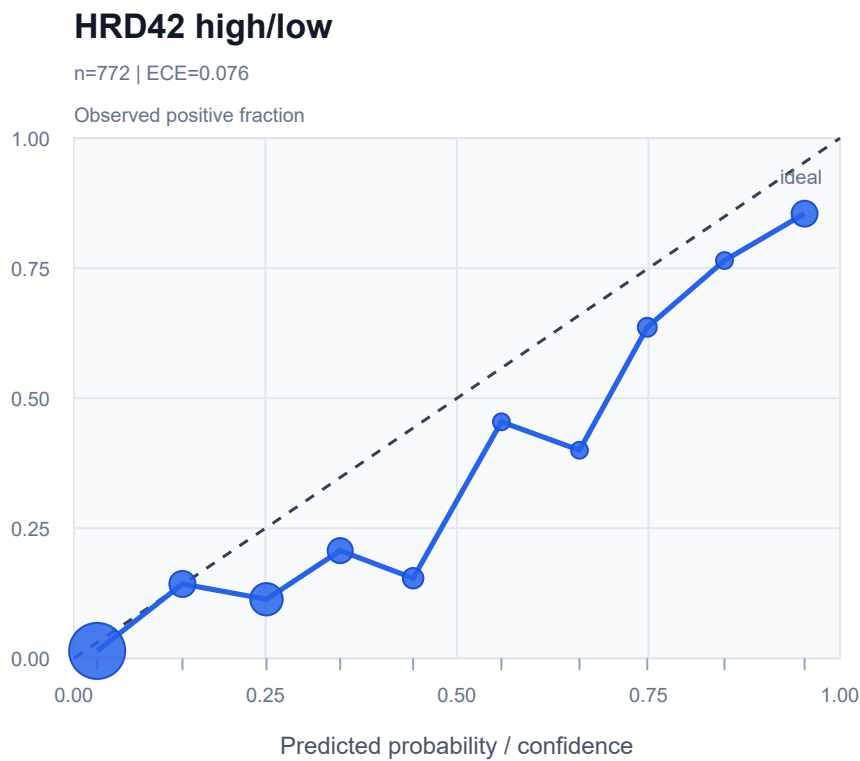
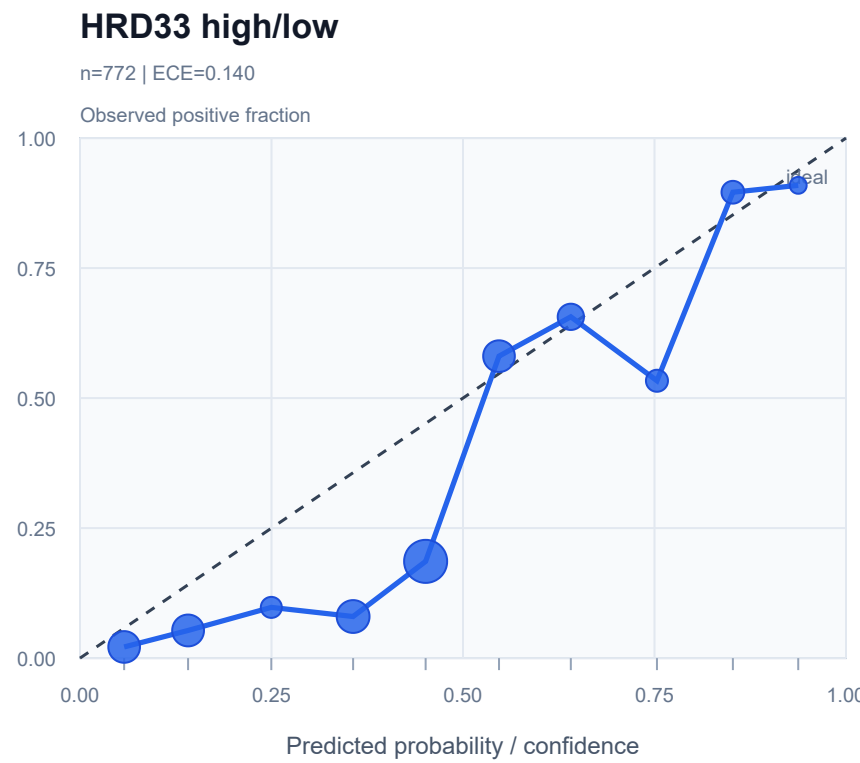
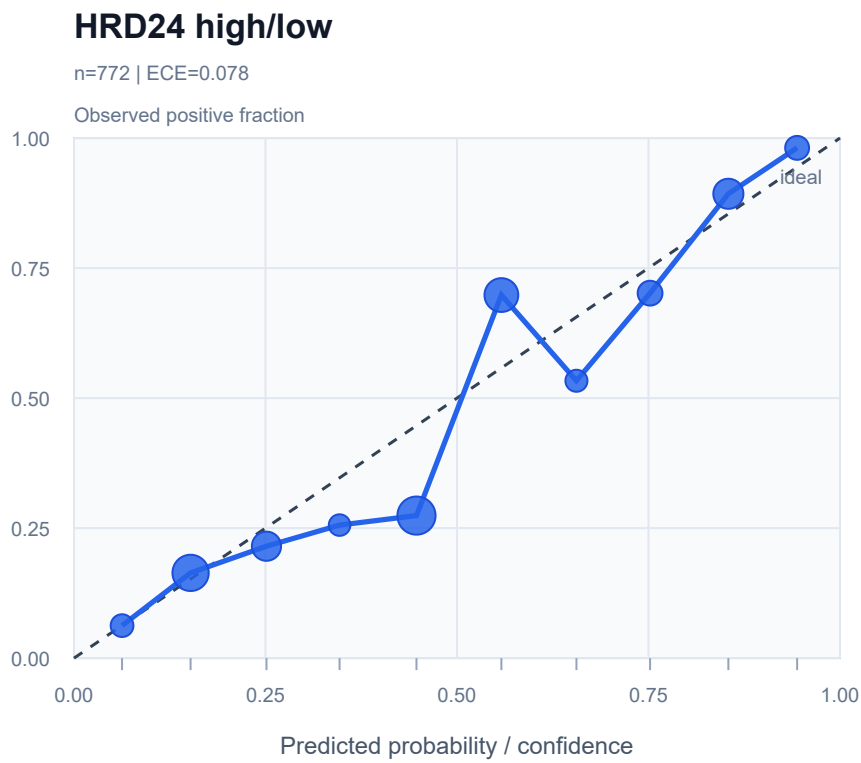


Supplementary Figure S2. Calibration and reliability

Canonical 5-fold OOF reliability for Signatures + Bio MAF v4 with XGBoost. Multiclass panels plot model confidence against correctness.

Circle area reflects bin sample count; dashed line is perfect calibration.
Empty probability columns are excluded before multiclass confidence is computed.

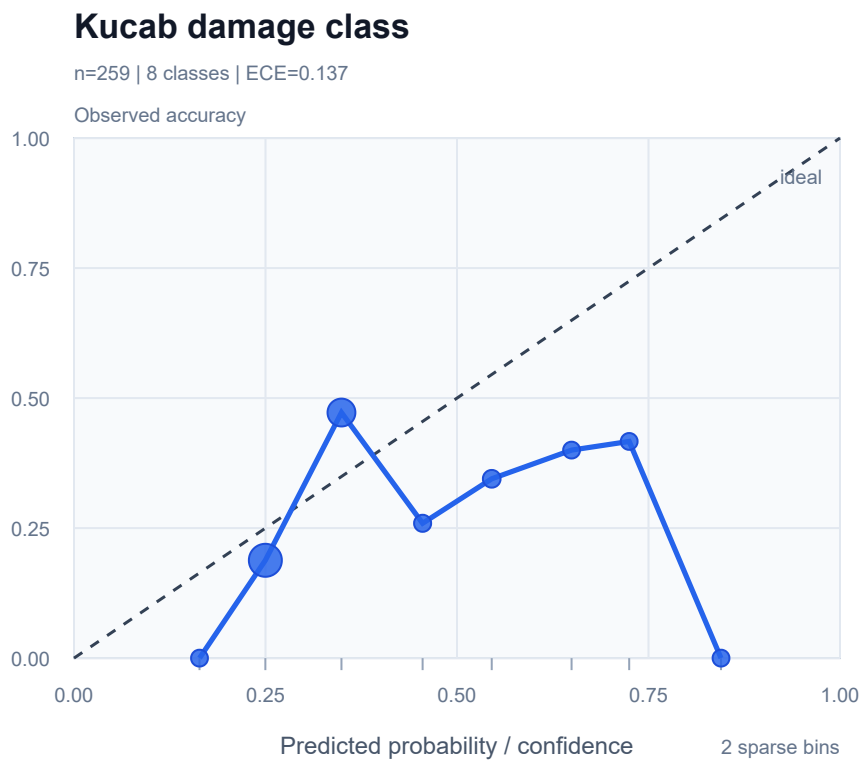

----- perfect calibration

—●— observed OOF bin