
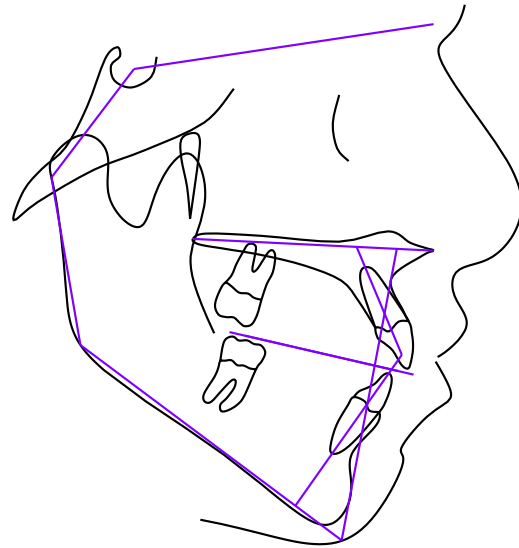


Patient

RANA EID HOSNY, F - 9

Analysis type **Eastman**

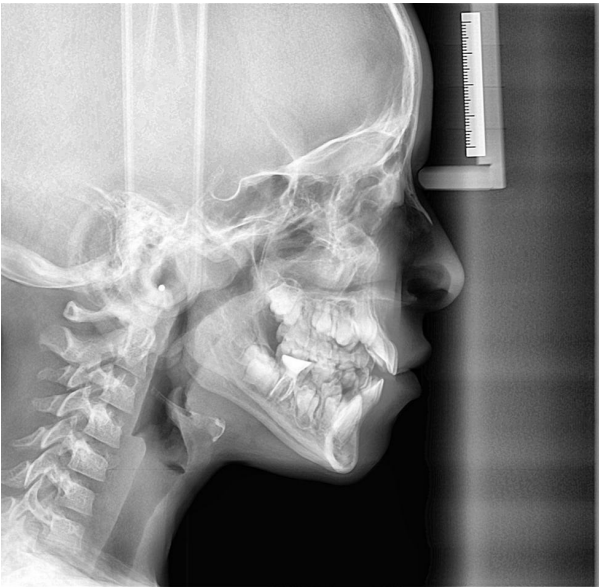


MEASUREMENT		NORMAL VALUE	VALUE	DIFFERENCE	BIAS
Other					
Angle SNA	°	81.0±5.0	72.0	-9.0	•
Angle SNB	°	78.0±5.0	70.7	-7.3	•
ANB (corrected)	°		5.4		
UIA	°	109.0±5.0	115.5	6.5	•
LIA	°	93.0±5.0	88.4	-4.6	
Interincisal angle	°	133.0±10.0	122.1	-10.9	•
MMPA	°	27.0±5.0	34.0	7.0	•
Overjet	mm	2.0±2.0	3.5	1.5	
-1i/A-Pg	mm	1.0±1.0	3.1	2.1	••

Patient

RANA EID HOSNY, F - 9

Analysis type **ABO American Bo...**

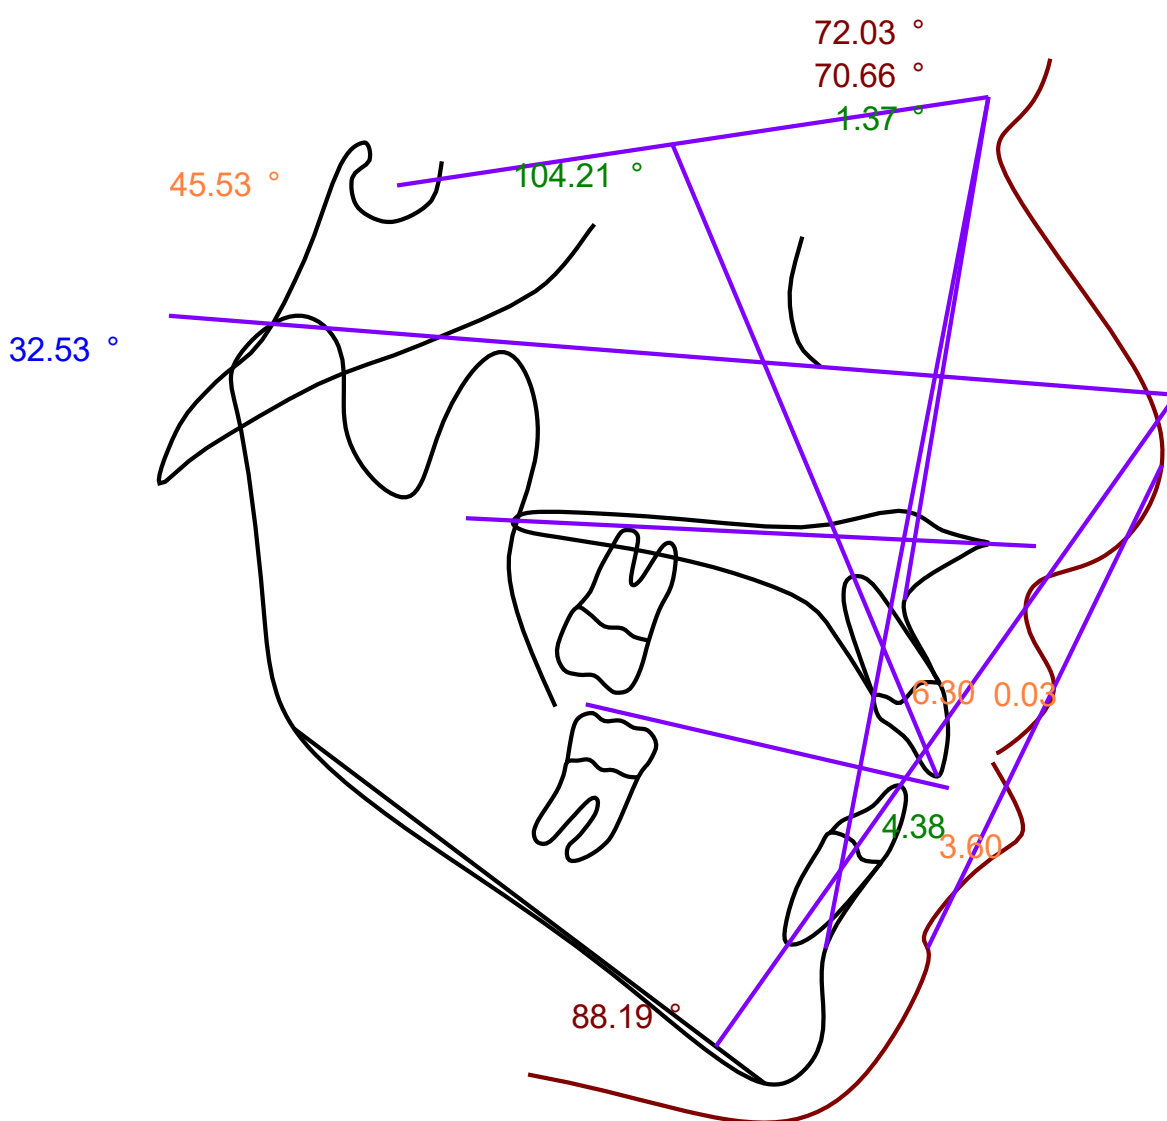

Patient

RANA EID HOSNY, F - 9

Analysis type **ABO American Bo...**

MEASUREMENT		NORMAL VALUE	VALUE	DIFFERENCE	BIAS
Skeletal Analysis					
Angle SNA	°	82.0±2.0	72.0	-10.0	●●●
Angle SNB	°	80.0±2.0	70.7	-9.3	●●●
ANB	°	2.0±4.0	1.4	-0.6	
SN-MP-abo	°	32.0±6.0	45.5	13.5	●●
FMA-abo	°	25.0±4.0	32.5	7.5	●
Dental Analysis					
+1i/NA	mm	4.0±1.0	6.3	2.3	●●
+1/SN	°	103.0±4.0	104.2	1.2	
-1i/NB	mm	4.0±1.0	4.4	0.4	
-1/MP-abo	°	99.0±1.0	88.2	-10.8	●●●
Overjet	mm	3.5±2.5	3.5	0.0	
Overbite	mm	2.0±2.5	-1.8	-3.8	●
Facial Analysis					
Ls/E-line	mm	-4.0±2.0	0.0	4.0	●●
Li'/E-line	mm	-2.0±2.0	3.6	5.6	●●