

What's New in Voltus IC Power Integrity Solution

Product Version 26.10
May 2026

© 2026 Cadence Design Systems, Inc. All rights reserved.
Cadence Design Systems, Inc. All rights reserved.
Printed in the United States of America.

Cadence Design Systems, Inc., 2655 Seely Avenue, San Jose, CA 95134, USA

Open SystemC, Open SystemC Initiative, OSCI, SystemC, and SystemC Initiative are trademarks or registered trademarks of Open SystemC Initiative, Inc. in the United States and other countries and are used with permission.

Trademarks: Trademarks and service marks of Cadence Design Systems, Inc. contained in this document are attributed to Cadence with the appropriate symbol. For queries regarding Cadence's trademarks, contact the corporate legal department at the address shown above or call 800.862.4522. All other trademarks are the property of their respective holders.

All other trademarks are the property of their respective holders.

Restricted Permission: This publication is protected by copyright law and international treaties and contains trade secrets and proprietary information owned by Cadence. Unauthorized reproduction or distribution of this publication, or any portion of it, may result in civil and criminal penalties. Except as expressly permitted below, this publication may not be copied, reproduced, modified, published, uploaded, posted, transmitted, or distributed in any way, including automated processes, training or services involving a large language model, foundation model, deep machine learning, generative artificial intelligence, or any other similar process or technology, without prior written permission from Cadence. Unless otherwise agreed to by Cadence in writing, customers are granted permission to print one (1) hard copy of this publication subject to the following conditions:

1. the publication may be used only in accordance with a written agreement between Cadence and its customer;
2. the publication may not be modified in any way;
3. any authorized copy of the publication or portion thereof must include all original copyright, trademark, and other proprietary notices and this permission statement;
4. the information contained in this document cannot be used in the development of like products or software, whether for internal or external use, and shall not be used for the benefit of any other party, whether or not for consideration

Disclaimer: Information in this publication is subject to change without notice and does not represent a commitment on the part of Cadence. The information contained herein is the proprietary and confidential information of Cadence or its licensors, and is supplied subject to, and may be used only by Cadence's customer in accordance with, a written agreement between Cadence and its customer. Except as may be explicitly set forth in such agreement, Cadence does not make, and

expressly disclaims, any representations or warranties as to the completeness, accuracy or usefulness of the information contained in this document. Cadence does not warrant that use of such information will not infringe any third party rights, nor does Cadence assume any liability for damages or costs of any kind that may result from use of such information.

Cadence is committed to using respectful language in our code and communications. We are also active in the removal and replacement of inappropriate language from existing content. This product documentation may however contain material that is no longer considered appropriate but still reflects long-standing industry terminology. Such content will be addressed at a time when the related software can be updated without end-user impact.

Restricted Rights: Use, duplication, or disclosure by the Government is subject to restrictions as set forth in FAR52.227-14 and DFAR252.227-7013 et seq. or its successor.

Contents

About This Manual	5
Related Documents	5
Voltus IC Power Integrity Solution Product Documentation	5
Voltus Stylus Common UI Product Documentation	6
1	7
Release Overview	7
Release 26.10 Overview	7
Changes to Command Options and Defaults	7
New Command Parameters	7
Obsolete Command Parameters	10
2	11
Licensing	11
Release 26.10 Enhancements	11
New Voltus Product Option	11
3	13
Library Generation and Extraction	13
Release 26.10 Enhancements	14
New Parameter Introduced for Standard Cell PGV Verification	14
Support to Specify Additional LibGen Variables	15
MIMCap PGV Characterization	15
Ability to Generate New Tech PGV with Updated Tap Node Distance	15
Ability to Characterize Single Triangular Current Waveform	16
Support for Specifying the TSV Subckt File during Power-Grid Library Generation	17
Ability to Reuse Electrical Data for Macro PGV Generation	18
Support for XDSPF and PGBD Inputs made Obsolete	18
4	19
Static and Dynamic Power Analysis	19
Release 26.10 Enhancements	19
Partition SPEF Support	19
Default Change for Unified Power Switch Flow in XP Flow	20
Enhanced Support for Logical Hierarchy and Domain-Based Activities	20

Support Added for Ignoring Unconstrained Nets and Pins with Valid Timing Data	21
Scaling Capacitance by Slew Ratio	21
New Parameter to Force Propagation	22
off_pg_nets Parameter Enhanced to Support Reporting of Bulk Pin Leakage	22
Custom Output Directory for Thermal Results	23
Instance-Based FIT Reporting with New Parameters	23
Reporting of Cell Usage Statistics	23
5	25
Rail Analysis	25
Release 26.10 Enhancements	27
Enhanced Rail Analysis Reporting with Average Effective Resistance	27
Generates Multiple RLRP and REFF Reports in a Single Run	27
Separate Timing and Switching Window EIV Reports	28
New Parameter to Specify the Lifetime Rating Factor	29
Voltus InsightAI Command Enhanced	29
New Parameter for Violation Magnitude-Based Repair with External Signoff Tool Consistency	33
SHE Parameter File Specification	33
Partial Net Coverage Reporting in SPEF	33
Ability to Compress Rail Output Files	34
set_power_data Command Enhanced	34
Voltus InsightAI Reporting Capabilities	35
Enhanced Voltus InsightAI Commands for Timing Path Protection during PG Reinforcement	37
Generation of Voltus InsightAI Database	37
create_die_model Command Enhanced	38
Support to Exclude Taps in a PGV	39
create_current_region Command Enhanced	39
Runtime Optimization for Reading the DEF files	39
Support to Suppress the Negative RC values	40
convert_gds_to_def Command Enhanced	40
Voltus InsightAI Enhancements	40
read_power_rail_results Command Enhanced	41
Single Partition Support During Extraction	41
Support to Read Power Data to Identify PTI Files	42
Ability to Reuse HPT Data	42
set_die_model Command Enhanced	43

6	44
Multi-Die IR Analysis	44
Release 26.10 Enhancements	44
Voltus IR Co-simulation with Multi-die and Package	44

About This Manual

This manual provides information about Product Version 26.1 of the Cadence® Voltus™ IC Power Integrity Solution suite, also known as Voltus. The Voltus family encompasses the following products:

- Voltus IC Power Integrity Solution - L
- Voltus IC Power Integrity Solution - XL

Related Documents

For more information about Voltus, see the following documents. You can access these and other Cadence documents using the Cadence Help documentation system.

Voltus IC Power Integrity Solution Product Documentation

- [*Voltus Known Problems and Solutions*](#)
Describes important Cadence Change Requests (CCRs) for Voltus, including solutions for working around known problems.
- [*Voltus Text Command Reference*](#)
Describes the Voltus text commands, including syntax and examples.
- [*Voltus Menu Reference*](#)
Provides information specific to the forms and commands available from the Voltus graphical user interface.
- [*Voltus User Guide*](#)
Provides information on using various Voltus features.
- README file
Contains installation, compatibility, and other prerequisite information, including a list of Cadence Change Requests (CCRs) that were resolved in this release. You can read this file online at downloads.cadence.com.

Voltus Stylus Common UI Product Documentation

- [*Voltus Stylus Common UI Text Reference Manual*](#)
Describes the Voltus Stylus Common UI text commands, including syntax and examples.
- [*Voltus Stylus Common UI User Guide*](#)
Provides information on using various Voltus Stylus Common UI features.

Release Overview

- [Release 26.10 Overview](#)
 - [Changes to Command Options and Defaults](#)

Release 26.10 Overview

Changes to Command Options and Defaults

New Command Parameters

The following table lists the command parameters that were added to the Voltus IC Power Integrity software. The second column identifies the corresponding chapter in *Voltus Text Command Reference* where the command is documented.

New Parameters	Chapter
<code>analyze_self_heat</code> <code>-parameter_file</code>	Self-Heating Effect Analysis Commands
<code>check_pg_library</code> <code>-libgen_command_file</code>	Power-Grid Library Commands
<code>convert_gds_to_def</code> <code>-tech_gds_layermap</code>	Rail Analysis Commands
<code>create_current_region</code> <code>-on_interdie_bump</code>	Rail Analysis Commands
<code>create_die_model</code> <code>-local_reference_ground</code> <code>-suppress_negative_res</code>	Rail Analysis Commands

<pre>get_ir_insight -cap_lower_limit -cap_upper_limit -report_mode</pre>	Rail Analysis Commands
<pre>get_voltus_insight_mode -timing_protection_config</pre>	Rail Analysis Commands
<pre>read_power_rail_results -force</pre>	Rail Analysis Commands
<pre>report_power -cell_fit_file -output_cell_fit_file</pre>	Power Calculation Commands
<pre>set_advanced_pg_library_mode -pgv_path -reuse_electrical_data -spectre_standalone_simulation -use_physical_view_from_techpgv</pre>	Power-Grid Library Commands
<pre>set_default_switching_activity -pg_net</pre>	Power Calculation Commands
<pre>set_die_model -static_current</pre>	Rail Analysis Commands
<pre>set_pg_library_mode -tsv_subckt_modelfile_list</pre>	Power-Grid Library Commands
<pre>set_power_analysis_mode -effective_load_cap_method -effective_load_cap_slew_threshold_limit -enable_force_propagation - honor_default_switching_activity_in_scheduling -ignore_unconstraint_net_with_timing_data -off_pg_bulk_leakage -partition_spef -show_cell_usage_stats</pre>	Power Calculation Commands

<code>set_power_data</code> <code>-cell</code> <code>-power_directory</code>	Rail Analysis Commands
<code>set_self_heat_analysis_mode</code> <code>-parameter_file</code>	Self-Heating Effect Analysis Commands
<code>set_signal_em_analysis_mode</code> <code>-lifetime_rating_factor_file</code> <code>-report_unannotated_shapes</code>	Signal ElectroMigration Commands
<code>set_thermal_analysis_mode</code> <code>-thermal_output_dir</code>	Power Calculation Commands
<code>set_rail_analysis_mode</code> <code>-cell_eval_tap_layer_file</code> <code>-inst_ignore_file</code> <code>-lifetime_rating_factor_file</code> <code>-report_compress_level</code> <code>-single_partition_extraction_layer</code> <code>-single_partition_extraction_layer_list</code> <code>-xp_reuse_hpt_directory</code> <code>-xp_reuse_parse_def_directory</code>	Rail Analysis Commands

<pre>set_voltus_insight_mode -all_scenario_ranking -disable_layer -groundREFF_threshold -groundRLRP_threshold -initialize -input_insight_db -instance_mapping -output_insight_db -master_list -master_mapping -path_group -powerREFF_threshold -powerRLRP_threshold -scenario_ranking -timing_protection_config -violation_input</pre>	Rail Analysis Commands
--	---------------------------

Obsolete Command Parameters

The following obsolete text command parameters have been removed from the software.

```
set_advanced_pg_library_mode
-import_xdspf_list_file
-pgdb_layermap
-pgdb_list_file
-xdspf_layermap
```

These parameters have not been replaced.

Licensing

- [Release 26.10 Enhancements](#)
 - [New Voltus Product Option](#)

Release 26.10 Enhancements

New Voltus Product Option

This release introduces the following product option:

Name	Short Name	Product Number	TCL Option	Description
------	------------	----------------	------------	-------------

Voltus InsightAI Multi- Dimensional Option	Voltus InsightAI MD Opt	VTS208	vtsvimd	This option enables the following advanced IR features within Innovus: • Multi-Dimension fixing in a single run by honoring the impact of multiple vectors, multiple PVTs, multiple EIV measurements, and multiple domains with varying thresholds • Hierarchical context in block-level IR fixing including multiple instantiations • Advanced reporting and debugging  VTS208 is an additional option required on top of Innovus Voltus InsightAI Option (INVS58). The licenses required to enable the advanced IR fixing features are: INVS 100 (Innovus Base) + INVS Technology Node Option + INVS58 + VTS208 (1 or more depending on usage)
--	-------------------------------	--------	---------	--

Library Generation and Extraction


- Release 26.10 Enhancements
 - New Parameter Introduced for Standard Cell PGV Verification
 - Support to Specify Additional LibGen Variables
 - MIMCap PGV Characterization
 - Ability to Generate New Tech PGV with Updated Tap Node Distance
 - Ability to Characterize Single Triangular Current Waveform
 - Support for Specifying the TSV Subckt File during Power-Grid Library Generation
 - Ability to Reuse Electrical Data for Macro PGV Generation
 - Support for XDSPF and PGBD Inputs made Obsolete

Release 26.10 Enhancements

New Parameter Introduced for Standard Cell PGV Verification

A new parameter, `-spectre_standalone_simulation`, has been added to the `set_advanced_pg_library_mode` command to support verification of power-gate parameters (Idsat, Ileakage, and Ron) and coupled capacitance in Spectre. Earlier, the Spectre setup did not contain computation equations (that is, `.measure` statements). Now, when the `-spectre_standalone_simulation` parameter is set to `true`, the generated setup file includes `.measure` statements. You can use this setup file directly in Spectre to understand and verify the underlying computational processes.

The table below displays a snippet of the computation equations extracted from the `.sp` file:

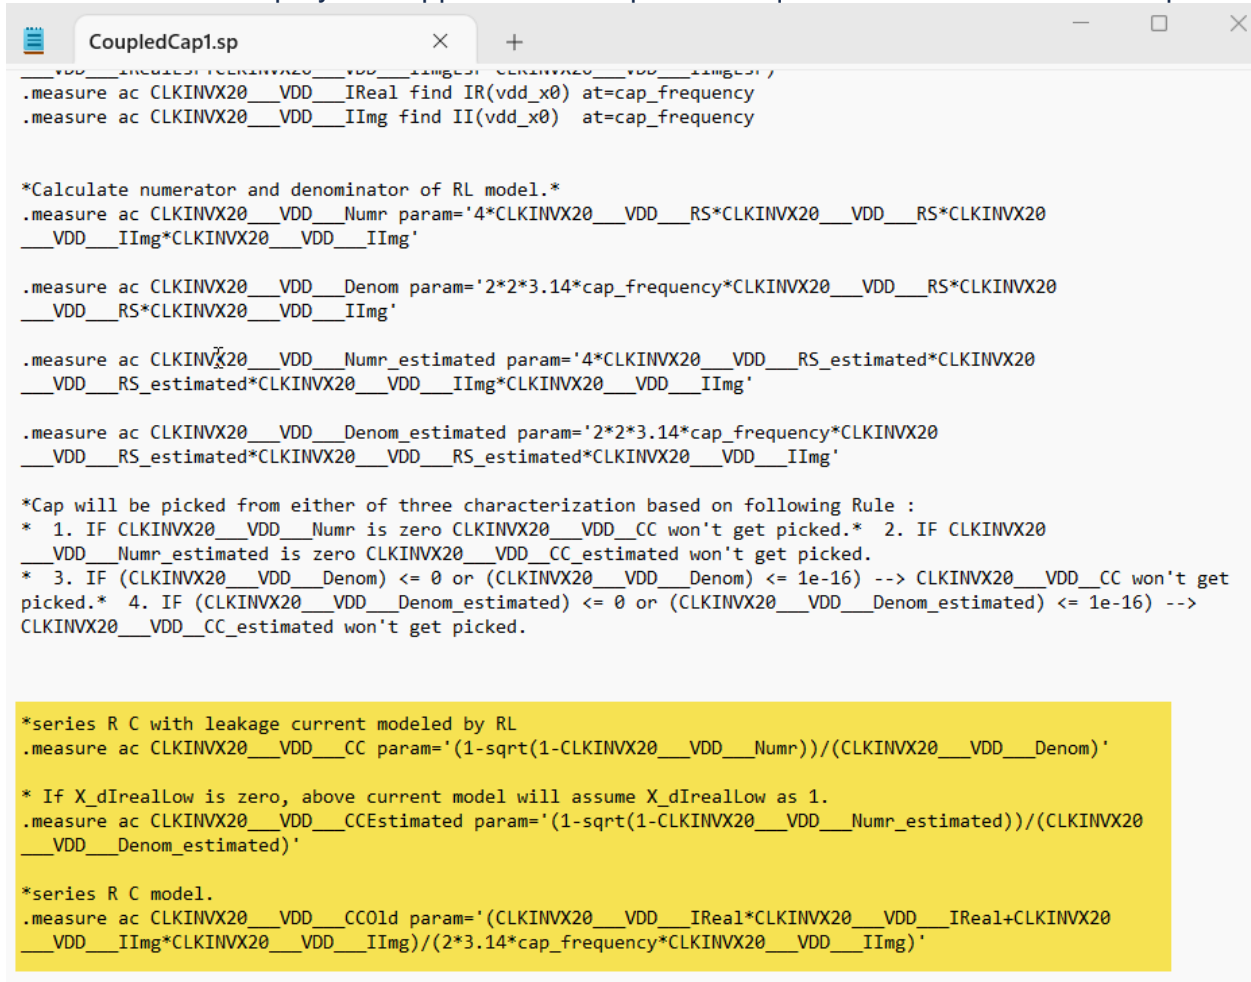

```
CoupledCap1.sp
__VDD__ IReal find IR(vdd_x0) at=cap_frequency
__VDD__ IImg find II(vdd_x0) at=cap_frequency

*Calculate numerator and denominator of RL model.*
__VDD__ Numr param='4*CLKINX20__VDD__RS*CLKINX20__VDD__RS*CLKINX20
__VDD__ IImg*CLKINX20__VDD__IImg'

__VDD__ Denom param='2*2*3.14*cap_frequency*CLKINX20__VDD__RS*CLKINX20
__VDD__ RS*CLKINX20__VDD__IImg'

__VDD__ Numr_estimated param='4*CLKINX20__VDD__RS_estimated*CLKINX20
__VDD__ RS_estimated*CLKINX20__VDD__IImg*CLKINX20__VDD__IImg'

__VDD__ Denom_estimated param='2*2*3.14*cap_frequency*CLKINX20
__VDD__ RS_estimated*CLKINX20__VDD__RS_estimated*CLKINX20__VDD__IImg'

*Cap will be picked from either of three characterization based on following Rule :
* 1. IF CLKINX20__VDD__Numr is zero CLKINX20__VDD__CC won't get picked.* 2. IF CLKINX20
__VDD__ Numr_estimated is zero CLKINX20__VDD__CC_estimated won't get picked.
* 3. IF (CLKINX20__VDD__Denom) <= 0 or (CLKINX20__VDD__Denom) <= 1e-16 --> CLKINX20__VDD__CC won't get
picked.* 4. IF (CLKINX20__VDD__Denom_estimated) <= 0 or (CLKINX20__VDD__Denom_estimated) <= 1e-16 -->
CLKINX20__VDD__CC_estimated won't get picked.

*series R C with leakage current modeled by RL
__VDD__ CC param='(1-sqrt(1-CLKINX20__VDD__Numr))/(CLKINX20__VDD__Denom)'

* If X_dIrealLow is zero, above current model will assume X_dIrealLow as 1.
__VDD__ CCEstimated param='(1-sqrt(1-CLKINX20__VDD__Numr_estimated))/(CLKINX20
__VDD__ Denom_estimated)'

*series R C model.
__VDD__ CC0ld param='(CLKINX20__VDD__IReal*CLKINX20__VDD__IReal+CLKINX20
__VDD__ IImg*CLKINX20__VDD__IImg)/(2*3.14*cap_frequency*CLKINX20__VDD__IImg)'
```

This parameter is applicable only for standard cell PGV generation (`-celltype stdcells`).

Support to Specify Additional LibGen Variables

You can now specify the additional LibGen variables using the `-libgen_command_file` parameter of the `check_pg_library` command to verify the consistency between the OBS via geometries and port geometries and ensure that the LEF result aligns with the PGV result.

For example, using the `-libgen_command_file` parameter, you can enable the additional LibGen variables `copy_intersecting_obs_vias_to_ports` and `input_type check_lef_pgv_compatibility`, respectively, to verify the consistency between the generated PGV and the original LEF file.

Use Model:

```
check_pg_library -libgen_command_file filename
```

MIMCap PGV Characterization

The Metal-Insulator-Metal Capacitor (MIMCap) PGV generation flow has been introduced for the simplified modeling of MIMCap cells. Since MIMCaps are inherently parallel-plate structures and do not involve MOSFET devices, this flow enables more accurate and efficient capacitance extraction.

You can generate PGV using either GDS or SPICE inputs for a MIMCap cell:

- **Standard Cell MIMCap PGV Generation:** Only SPICE netlist is considered, and no GDS data is provided for characterizing the MIMCap. The `.param capflag_mim=1` parameter should be specified in the Spice models for MIMCap computation.
- **Macro PGV Generation:** GDS data is used for characterizing MIMCap and an XTC command file is required to specify layer operations to derive the MIMCap shapes.

Ability to Generate New Tech PGV with Updated Tap Node Distance

Now, Voltus allows you to change the tap node distance of LEF based PGVs (standard cells and LEF macros) by only generating a new tech PGV, without regenerating the entire PGV. To support this enhancement, a new option `-use_physical_view_from_techpgv` has been added to the `set_advanced_pg_library_mode` command. The default value of the parameter is `false`.

You can generate a tech PGV with new tap distance as follows:

1. Specify the settings to update the tap node distance through the command line.

TCL command:

```
set_advanced_pg_library_mode  
-tap_node_distance (With new tap distance)  
-use_physical_view_from_techpgv true
```

2. Pass the powergate information if a powergate cell is present.

For example:

```
set_pg_library_mode -powergate_parameters {...}
```

3. Generate the output for power-grid library generation.

```
generate_pg_library -output tech_pgv
```

The generated report will have a note related to "use_physical_view_in_emir" flag set as shown in the following snippet:

This PGV has "use_physical_view_in_emir" flag set.

Cell	PowerNets	Capacitance	PowerGrid Views
DECAP1	VDD(0.9000) VSS(0.0000)	5.00000e-15 5.00000e-15	TECH(12 taps) TECH(12 taps)
Cell Type = DECOUPLING CAP			
INFO: This is a decap cell.			
Cell_Status: PASS			

You can pass the new generated library with the previously generated PGVs during rail analysis, so that the updated tech PGV is used for tap node distance and electrical parameters (currents, capacitances) come from original PGVs.

Ability to Characterize Single Triangular Current Waveform

Now, the `SINGULAR_TRIANGULAR` syntax is supported in the Datasheet method to characterize a single triangular current waveform for the specified mode. By default, the Datasheet method continues to generate dual peak - a main peak and an additional pre-charge peak.



Syntax:

```
SINGLE_TRIANGULAR mode1 mode2
```

Example:

The following is the trigger file format for singular peak and dual peak:

Singular Peak	Dual Peak (default)
---------------	---------------------
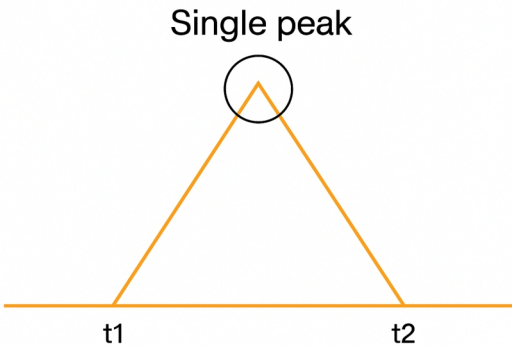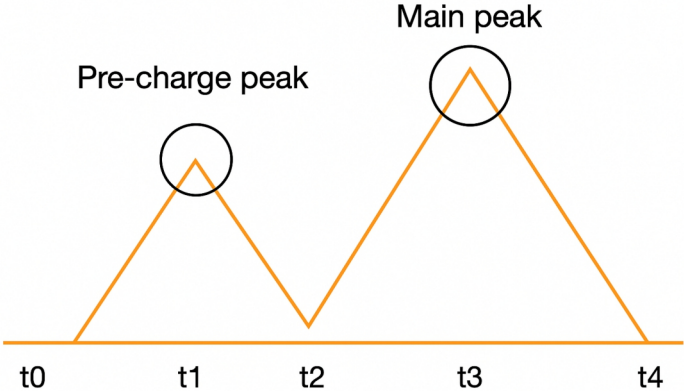
<pre> CURRENT_CHARACTERIZATION_METHOD DATASHEET CELL ARM_32x64 SINGLE_TRIANGULAR_READ MODE READ CONDITIONAL_INPUT = (!CEN & !WEN) CONDITIONAL_PIN CLK { RISE } DATASHEET DELAY 1.6879ns DATASHEET_INPUT_SLEW 5.962569e-03ns DATASHEET_OUTPUT_SLEW 5.968207e-03ns DATASHEET_PARAMETER {{ VDDG2 0.1715pf 1.355e-06mW} {VDDG 0.1715pf 3.62e-06mW} {VDD 0.1715pf 2.614e-06mW}} PEAK_CURRENT {{VDDG2 0.25mA {VDDG 0.2mA} {VDDG 0.15mA}}} END_MODE </pre>	<pre> CURRENT_CHARACTERIZATION_METHOD DATASHEET CELL ARM_32x64 MODE READ CONDITIONAL_INPUT = (!CEN & !WEN) CONDITIONAL_PIN CLK { RISE } DATASHEET DELAY 1.6879ns DATASHEET_INPUT_SLEW 5.962569e-03ns DATASHEET_OUTPUT_SLEW 5.968207e-03ns DATASHEET_PARAMETER {{ VDDG2 0.1715pf 1.355e- 06mW} {VDDG 0.1715pf 3.62e-06mW} {VDD 0.1715pf 2.614e-06mW}} PEAK_CURRENT {{VDDG2 0.25mA {VDDG 0.2mA} {VDDG 0.15mA}}} END_MODE </pre>
	

Support for Specifying the TSV Subckt File during Power-Grid Library Generation

Now, you can use the `-tsv_subckt_modelfile_list` parameter of the `set_pg_library_mode` command to specify the name of external Through Silicon Via (TSV) subckt model files to be used for 3D-IC extraction. You can specify a list of files separated by space. Each file contains the subckt model information for TSV. The specified file has the Spice format.

A sample file is shown below:

```
.subckt TSV top bottom
```

```
R1 top n2 0.03075
R2 n2 bottom 0.03075
C1 n2 0 28f
.ends
```

Use Model:

```
set_pg_library_mode -tsv_subckt_modelfile_list filename1 filename2 ...
```

Ability to Reuse Electrical Data for Macro PGV Generation

Macro PGV generation flow has been optimized to enable the reuse of electrical data from an old PGV to create a new PGV. The simulation steps are skipped for reused PGV flows, which results in reduced runtime.

To support this enhancement, two new parameters have been added to the `set_advanced_pg_library_mode` command:

- `-pgv_path`: Specifies the path of the cell library from which the electrical data will be used to create a new PGV.
- `-reuse_electrical_data`: When set to true, specifies to reuse the electrical data from the old PGV and only process the physical part in the new PGV. The default value is `false`.

Use Model:

```
set_advanced_pg_library_mode -pgv_path <path> -reuse_electrical_data true
```

Support for XDSPF and PGDB Inputs made Obsolete

The following parameters of `set_advanced_pg_library_mode` command are now obsolete. These parameters are no longer supported for PGV generation.

- `-import_xdspf_list_file`
- `-pgdb_layermap`
- `-pgdb_list_file`
- `-xdspf_layermap`

Static and Dynamic Power Analysis

- Release 26.10 Enhancements
 - Partition SPEF Support
 - Default Change for Unified Power Switch Flow in XP Flow
 - Enhanced Support for Logical Hierarchy and Domain-Based Activities
 - Support Added for Ignoring Unconstrained Nets and Pins with Valid Timing Data
 - Scaling Capacitance by Slew Ratio
 - New Parameter to Force Propagation
 - `off_pg_nets` Parameter Enhanced to Support Reporting of Bulk Pin Leakage
 - Custom Output Directory for Thermal Results
 - Instance-Based FIT Reporting with New Parameters
 - Reporting of Cell Usage Statistics

Release 26.10 Enhancements

Partition SPEF Support

The `set_power_analysis_mode` command now includes the `-partition_spef` parameter to generate block-level SPEF files from a flat SPEF file. This enhancement allows you to process input SPEF data and automatically generate partition-level SPEF chunks. The `set_power_analysis_mode -partition_spef` parameter is supported only in the extensively parallel (XP) mode for full-chip designs using flat SPEF files.

The use model of this feature is:

```
specifiy_spef { flat.spef.gz }
```

```
set_power_analysis_mode -partition_spef true
```

Default Change for Unified Power Switch Flow in XP Flow

The default value for the `set_power_analysis_mode -unified_power_switch_flow` parameter has been changed to `true` in the XP flow.

This change aligns the default behavior with the existing `set_rail_analysis_mode -unified_power_switch_flow` parameter, which is already set to `true` by default in the XP flow, ensuring consistency across both power and rail analysis modes. Due to this default behavior change, you may observe differences in power and current analysis results compared to previous versions. If you need to maintain the previous behavior, explicitly set `set_power_analysis_mode -unified_power_switch_flow false` in your scripts.

Enhanced Support for Logical Hierarchy and Domain-Based Activities

Voltus has been enhanced to support multiple activities per block. Previously, the tool honored only a single activity for each block. With this enhancement, you can now define different switching activities for different domains and/or logical hierarchies within the same DEF block during stable flop scheduling.

To enable this functionality, the following parameters have been introduced:

- `set_default_switching_activity -pg_net <netname>` - Specifies the name of the power net for domain-based switching activity assignment.
- `set_power_analysis_mode -honor_default_switching_activity_in_scheduling {true|false}` - Controls whether default switching activity settings are applied during hierarchy/domain-based scheduling.

This feature improves accuracy for complex hierarchical designs with varying switching characteristics and optimizes flop scheduling based on realistic switching activity patterns.

Example:

Following is an example of domain-based activity specification in the dynamic vectorless flow:

```
set_default_switching_activity -seq_activity 0.7 -input_activity 0.7 macro_activity 0.5  
-clock_gates_output 2 -pg_net VDDM
```

Support Added for Ignoring Unconstrained Nets and Pins with Valid Timing Data

Some nets/pins lack timing constraints (no associated clock) but contain valid timing data with arrival windows in the TWF file. Previously, the tool applied default frequency toggles to these unconstrained nets, which could cause false IR violation warnings due to high voltage drop.

You can now use the `set_power_analysis_mode -ignore_unconstraint_net_with_timing_data true` parameter to exclude unconstrained nets from toggle generation. This enhancement eliminates false IR violation reports and provides better control over toggle generation.

Scaling Capacitance by Slew Ratio

When using the lumped capacitor model, long net lines may cause reduction of effective capacitance (Ceff) due to high resistance shielding and low slew ratio. This can lead to overly optimistic delay estimate during Liberty lookups of lower load.

In this release, the following parameters have been added to the `set_power_analysis_mode` command to adjust and scale the load capacitance using the slew ratio:

- `-effective_load_cap_method {lumped | max | avg | min}` - Specifies the method to determine the slew ratio. This parameter has the following arguments:
 - `lumped` - the slew ratio is 1, which indicates that a lumped capacitance is used.
 - `max` - the slew ratio is calculated as $\max(\text{slew of all drivers}) / \max(\text{slew of all receivers})$
 - `min` - the slew ratio is calculated as $\min(\text{slew of all drivers}) / \min(\text{slew of all receivers})$
 - `avg` - the slew ratio is calculated as $\text{avg}(\text{slew of all drivers}) / \text{avg}(\text{slew of all receivers})$
- `-effective_load_cap_slew_threshold_limit <float between 0 and 1>` - the minimum threshold value for slew ratio to prevent effective capacitance from being derated beyond realistic limits.

This enhancement eliminates over optimism and enables more accurate modeling for long nets.

Example:

```
set_power_analysis_mode -method dynamic_vectorless -enable_state_propagation true\  
-enable_xp true -effective_load_cap_method max\  
-effective_load_cap_slew_threshold_limit 0.9
```

New Parameter to Force Propagation


In the dynamic vectorless flow, Voltus performs logic simulation by generating the state of an instance's output pins based on the states of its input pins. Occasionally, the output may become fixed or constant. In these scenarios, you can use the `set_power_analysis_mode -enable_force_propagation true` parameter to ensure that the output toggles are according to the clock signal rather than the input pin states. This parameter assigns clock activity to outputs when input propagation is not feasible, thereby enhancing overall activity.

off_pg_nets Parameter Enhanced to Support Reporting of Bulk Pin Leakage

The `set_power_analysis_mode -off_pg_bulk_leakage` parameter has been introduced to account for the leakage power through an instance's bulk pin when it is connected to a power-ground (PG) rail in the ON state.

```
set_power_analysis_mode \  
  -off_pg_nets { vddlsw } \  
  -off_pg_bulk_leakage {true | false}
```

The following diagram illustrates that the instance contributes bulk pin leakage to the ON state rail (**vdd**) through the *VBP* pin and zero leakage to the OFF state rail (*vddlsw*) through the VDD pin.

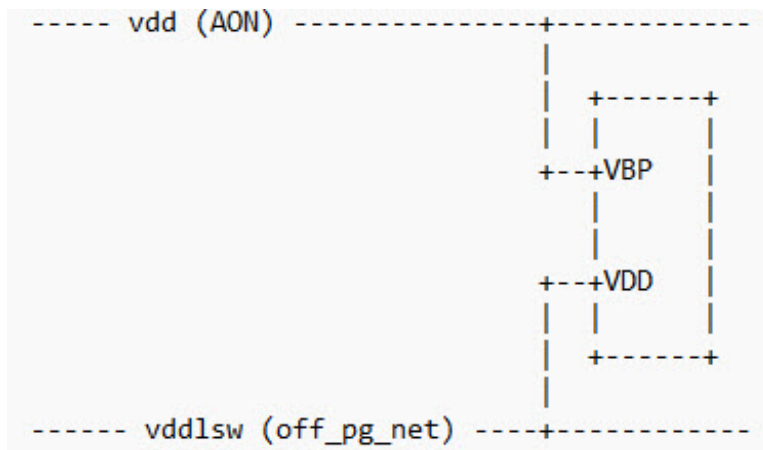

Custom Output Directory for Thermal Results

You can now use the `set_thermal_analysis_mode -thermal_output_dir` parameter to specify a custom output directory for thermal analysis results instead of using the default `ThermalDir`. This enhancement gives you better control over where your output files are stored, making it easier to manage results across multiple runs.

Example:

Use the `-thermal_output_dir` parameter to define your preferred directory path:

```
set_thermal_analysis_mode -tool_path $CELSIUSTOOL \  
                          -boundary_condition_file bc_75.txt \  
                          -temperature_map_file temperatureMap_75 \  
                          -thermal_output_dir thermal_dir_new \  
                          -power_map_file vtm_output/top.vtm.txt  
  
analyze_thermal
```

Instance-Based FIT Reporting with New Parameters

In this release, two new parameters are added to the `report_power` command to generate instance-level FIT report based on cell-level data:

- `-cell_fit_file filename` - Specifies a file that accepts a cell-based FIT input table with two columns: cell name and FIT value.
- `-output_cell_fit_file filename` - Specifies the name of the output file for the generated FIT report, which includes three columns: instance name, corresponding cell name, and computed FIT value.

This enhancement ensures greater visibility into instance-level risks and supports more efficient debug and review of high-FIT contributors. Instance-based FIT report is supported only in the XP mode.

Reporting of Cell Usage Statistics

The `-show_cell_usage_stats {true | false}` parameter has been added to the `set_power_analysis_mode` command. It provides cell usage statistics alongside power values, indicating the number of cells used from a specific library and the corresponding power percentage. This helps identify libraries with the greatest and least impact on power consumption.

You must ensure that this parameter is specified before using the `report_power` command, as

demonstrated below:

```
set_power_analysis_mode -show_cell_usage_stats true  
report_power -outfile pl.rpt
```

Following is a snippet from the report:

Cell usage statistics:

```
Library jlos_h , 88 cells ( 7.351713%) , 6.56434e-06 mW ( 0.554089% )  
Library jlos_l , 123 cells ( 10.275689%) , 0.000799809 mW ( 67.511081% )  
Library jlos , 986 cells ( 82.372597%) , 0.000378334 mW ( 31.934830% )
```

The `-show_cell_usage_stats` parameter is applicable only to the static power calculation, Verilog-based (`-static_netlist verilog`) flow.

Rail Analysis

- Release 26.10 Enhancements
 - Enhanced Rail Analysis Reporting with Average Effective Resistance
 - Generates Multiple RLRP and REFF Reports in a Single Run
 - Separate Timing and Switching Window EIV Reports
 - New Parameter to Specify the Lifetime Rating Factor
 - Voltus InsightAI Command Enhanced
 - New Parameter for Violation Magnitude-Based Repair with External Signoff Tool Consistency
 - SHE Parameter File Specification
 - Partial Net Coverage Reporting in SPEF
 - Ability to Compress Rail Output Files
 - `set_power_data` Command Enhanced
 - Voltus InsightAI Reporting Capabilities
 - Enhanced Voltus InsightAI Commands for Timing Path Protection during PG Reinforcement
 - Generation of Voltus InsightAI Database
 - `create_die_model` Command Enhanced
 - Support to Exclude Taps in a PGV
 - `create_current_region` Command Enhanced
 - Runtime Optimization for Reading the DEF files
 - Support to Suppress the Negative RC values
 - `convert_gds_to_def` Command Enhanced
 - Voltus InsightAI Enhancements

- `read_power_rail_results` Command Enhanced
- Single Partition Support During Extraction
- Support to Read Power Data to Identify PTI Files
- Ability to Reuse HPT Data
- `set_die_model` Command Enhanced

Release 26.10 Enhancements

Enhanced Rail Analysis Reporting with Average Effective Resistance

A new argument, `avg`, has been added to the `set_rail_analysis_mode -reff_pin_report_method` parameter to improve reporting reliability for signoff analysis. When analyzing large macro cells, instances at different physical locations can exhibit varying effective resistance (`reff`) values. These location-dependent variations can introduce instability in signoff results, making it challenging to achieve consistent and reliable analysis outcomes.

The `avg` argument addresses this challenge by providing averaged effective resistance values, which offer greater stability compared to individual node measurements.

Usage Models

- `-reff_pin_report_method avg` - Reports only the average effective resistance value for instance pins with multiple nodes
- `-reff_pin_report_method {worst avg best}` - Reports comprehensive effective resistance data: best, worst, and average values for instance pins with multiple nodes

Generates Multiple RLRP and REFF Reports in a Single Run

The `set_rail_analysis_mode` command has been enhanced with improved `-reff_pin_report_method` and `-rlrp_pin_report_method` parameters that now support generating multiple report types simultaneously. This enhancement accelerates closure of RLRP and REFF issues by having all necessary report variants readily available for comparison and analysis. Each report type is automatically saved to a separate file, making it easy to access specific analysis results.

Example:

```
set_rail_analysis_mode -reff_pin_report_method { best avg worst}
```

Output files:

```
net.best.effr  
net.avg.effr  
net.worst.effr  
domain_effr.best.rpt  
domain_effr.avg.rpt  
domain_effr.worst.rpt
```

Separate Timing and Switching Window EIV Reports

The `set_rail_analysis_mode -eiv_eval_window` parameter has been enhanced to provide greater flexibility in EIV report generation during rail analysis. Rail analysis reporting now supports generating separate EIV reports for both timing and switching windows within a single analysis run. Previously, you could use the `both` argument to generate a single combined report containing both switching and timing-window EIV data. Now, you can use the `-eiv_eval_window {switching timing}` parameter to generate distinct reports for each window type in a single run. This enhancement allows easier post-processing and review of specific EIV analysis results, generating both report types simultaneously without additional runs.

Example:

The following image shows the EIV reports for the switching window, timing window, and both:

VERSION	"3.0"
CREATION	
CREATOR	
PROGRAM	"VOLTUS"
DIVIDERCHAR	"/"
DESIGN	"super_filter"
UNITS	VOLTAGE VOLT 1
INSTANCE_COUNT	480
NOMINAL_VOLTAGE	0.9
POWER_NET	VDD_external
GROUND_NET	VSS
WINDOW	SWITCHING
RP_VALUE	IV/EIV
RP_FORMAT	DETAIL
RP_INST_LIMIT	2000000000
RP_THRESHOLD	-1e+06
RP_PIN_NAME	TRUE
MICRON_UNITS	10000
TIME_UNITS	ns

① SWITCHING

VERSION	"3.0"
CREATION	
CREATOR	
PROGRAM	"VOLTUS"
DIVIDERCHAR	"/"
DESIGN	"super_filter"
UNITS	VOLTAGE VOLT 1
INSTANCE_COUNT	480
NOMINAL_VOLTAGE	0.9
POWER_NET	VDD_external
GROUND_NET	VSS
WINDOW	TIMING
RP_VALUE	IV/EIV
RP_FORMAT	DETAIL
RP_INST_LIMIT	2000000000
RP_THRESHOLD	-1e+06
RP_PIN_NAME	TRUE
MICRON_UNITS	10000
TIME_UNITS	ns

② TIMING

VERSION	"3.0"
CREATION	
CREATOR	
PROGRAM	"VOLTUS"
DIVIDERCHAR	"/"
DESIGN	"super_filter"
UNITS	VOLTAGE VOLT 1
INSTANCE_COUNT	480
NOMINAL_VOLTAGE	0.9
POWER_NET	VDD_external
GROUND_NET	VSS
WINDOW	SWITCHING_AND_TIMING
RP_VALUE	IV/EIV
RP_FORMAT	DETAIL
RP_INST_LIMIT	2000000000
RP_THRESHOLD	-1e+06
RP_PIN_NAME	TRUE
MICRON_UNITS	10000
TIME_UNITS	ns

③ SWITCHING+TIMING

The type of report generated is based on the following use models:

- `-eiv_eval_window {both}` - Reports 3 Only (*Default Behavior)
- `-eiv_eval_window {switching}` - Reports 1 Only
- `-eiv_eval_window {timing}` - Reports 2 Only
- `-eiv_eval_window {switching timing}` - Reports 1 and 2
- `-eiv_eval_window {switching both}` - Reports 1 and 3
- `-eiv_eval_window {timing both}` - Reports 2 and 3

When multiple EIV methods (best and worstavg) are enabled, the file naming convention for the EIV

reports is based on the EIV method and EIV evaluation window, as shown in the following examples:

```
VDD_VSS.worstavg.timing.iv  
VDD_VSS.worstavg.switching.iv  
VDD_VSS.best.timing.iv
```

New Parameter to Specify the Lifetime Rating Factor

A new parameter, `-lifetime_rating_factor_file`, has been introduced for both the `set_rail_analysis_mode` and `set_signal_em_analysis_mode` commands. This parameter allows you to specify a lifetime rating factor file that contains `jmax_life` values for each layer. These values are defined based on temperature and lifetime pairs. When you provide this file, EM analysis will automatically select the appropriate `jmax_life` factor for each layer according to the specific temperature-lifetime combinations defined within the file. The lifetime and EM temperature can be specified using the `-lifetime hours` and `-em_temperature °C` parameters.

Following is a snippet of the lifetime rating factor file:

*Rating factor of M0/V0/M1/V1/M2/V3/M3...					
TEMPERATURE	90	95	100	105	110 ...
LifeTime					

0.5	2.578	2.242	2.024	1.774	1.547
1	2.520	2.191	1.979	1.734	1.512
2	2.430	2.113	1.908	1.672	1.458
3	2.382	2.072	1.871	1.639	1.430
...					

Voltus InsightAI Command Enhanced

The `set_voltus_insight_mode` command now includes new parameters to support enhanced scenario-based configuration (differing EIV method, EIV evaluation window, and thresholds). These parameters allow scenarios to be defined for various groups or collections within the same repair/report session, enabling greater precision and flexibility. Instead of using uniform threshold or EIV values across all instances, you can customize settings based on:

- Instance collections

- Master blocks
- Rail database directories

Example: If general clock threshold is set to 10% and data threshold to 12%, a critical instance group can have a stricter 9% threshold. All the 3 threshold settings are honored in the same session. This allows multiple scenarios with different threshold configurations to run simultaneously in a single session.

New Parameters	Description
<code>-disable_layer filename</code>	
	Specifies the name of the file that contains the list of layers to be disabled or excluded during pre-route and post-route RPG. The format of the file is: <pre>Layer1 Layer2 Layer3</pre>
<code>-instance_mapping filename</code>	

	Specifies the name of the file that contains the mapping between a scenario and its corresponding instance files. Each scenario has its own set of instance files. Each line in an instance file defines either an instance name or a block instance name. Following is a snippet of the instance mapping file (<i>instance_mapping.txt</i>): <pre>SCENARIO_1 {instance1.txt instance2.txt} SCENARIO_2 {instance1.txt}</pre> The content of the 2 instance files is shown below: <pre>instance1.txt ----- Inst_A* Inst_B* instance2.txt ----- Inst*</pre>
	<pre>-master_list {list_of_master_blocks}</pre>
	Specifies the list of master blocks to be reported for IR repair.
	<pre>-master_mapping filename</pre>

	Specifies the name of the file that contains the mapping between a scenario and its corresponding master files. Each scenario has its own set of master files. Each line in a master file defines one master block. Following is a snippet of the master mapping file (<code>master_mapping.txt</code>): <pre>SCENARIO_1 {master1.txt master2.txt} SCENARIO_2 {master1.txt}</pre> The content of the 2 master files is shown below: <pre>master1.txt ----- Top master2.txt ----- Super_filter</pre>
Enhanced Parameter	Description
<code>-db_mapping filename</code>	
	Specifies the name of the file that contains the mapping between a scenario and its corresponding rail directories. Each scenario can be mapped to multiple rail directories. Previously, a single scenario could map to only one rail directory. Following is a snippet of the rail database mapping file (<code>db_mapping.txt</code>): <pre>SCENARIO_1 {RailDB1 RailDB2} SCENARIO_2 {RailDB1}</pre>

New Parameter for Violation Magnitude-Based Repair with External Signoff Tool Consistency

A new parameter, `set_voltus_insight_mode -violation_input filename`, has been introduced, enabling repair operations based on violation specifications that align with an external signoff tool. This feature allows Voltus to replicate violation magnitudes for individual instances, ensuring consistent repair behavior between the external signoff tool and Voltus while eliminating the need for global threshold adjustments.

You can specify a text file containing a per-instance violation specification in the following format:

```
instance_name    threshold(mV)    violating_amount (mV)
```

Example:

```
inst_1    100    35
inst_2     80    20
```

For instance 1 (`inst_1`), an external signoff tool detected a 35mV violation against a 100mV threshold. This violation data allows Voltus to perform repairs using the same violation magnitude values reported by the external tool, ensuring consistency between the tools.

SHE Parameter File Specification

A new parameter, `-parameter_file`, has been introduced for both the `set_self_heat_analysis_mode` and `analyze_self_heat` commands. This parameter allows you to specify the self-heating effect (SHE) analysis parameter file name (`param.sh`) required for SHE calculations. This foundry-provided file contains essential alpha and beta coupling factors that the tool uses for coupledT calculations when modeling heat transfer from devices to metal layers.

Partial Net Coverage Reporting in SPEF

A new parameter, `set_signal_em_analysis_mode -report_unannotated_shapes {true | false}`, has been introduced to enhance visibility into partial net coverage within SPEF files. When this parameter is set to `true`, the `<report_name>.rpt.unannotated_shapes` is generated. This report identifies and lists nets that contain shapes without resistance annotations, or unanalyzed/ partially analyzed segments. The feature helps to detect incomplete parasitic extraction coverage and improve accuracy during validation and signoff workflows. The reporting of partial net coverage works only when `-effort_level` is set to `high`.

Use Model:

```
set_signal_em_analysis_mode -effort_level high -report_unannotated_shapes true
```

Report Format:

```
NET: <net_name>          <- Specifies the name of the analyzed simulation nets with
unannotated shapes
LAYER (x1 y1 x2 y2)      <- Layer name and shape coordinates
```

Sample Report:

```
NET: Net_A
LAYER (x1          y1          x2          y2)
M2    (30.2850    12.0800    37.6150    12.2200)
M2    (30.2000    12.0650    30.2850    12.2350)
...
```

 This parameter is applicable only when running in the DP mode; it is not supported in the XP mode.

Ability to Compress Rail Output Files

A new parameter, `-report_compress_level`, has been added to the `set_rail_analysis_mode` command to compress the rail output files in the GNU Zip format. The compressed files will have the suffix `.gz`.

Use Model:

```
set_rail_analysis_mode -report_compress_level {0 | 1-9}
```

- 0: default, no compression
- 1-9: the compression levels vary from 1 to 9. 1 provides the fastest compression speed but at a lower ratio, so the file size will be larger. 9 provides the highest compression ratio but at a lower speed.

set_power_data Command Enhanced

The `-cell` parameter has been added to the `set_power_data` command to specify power from the block-level run for the multiple instances of the same block. Therefore, you no longer need to specify power for each instance separately. This option is useful when power is calculated for hierarchical partitions of the design.

Use model:


```
set_power_data -cell cellname
```

Example:

```
set_power_data -cell BlockA -format current {file1, file2, file3 ...}
```

Voltus InsightAI Reporting Capabilities

A new REPORTS directory has been added at the root level to better organize the Voltus InsightAI analysis results. The following diagram illustrates the directory structure:

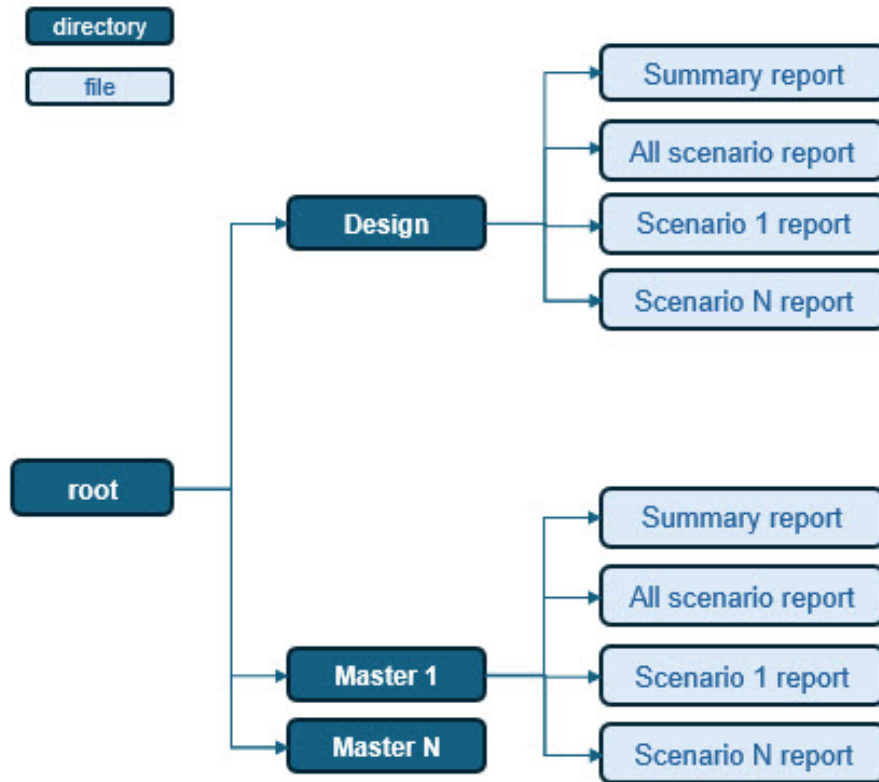

Here, the number of subdirectories created depends on the hierarchical structure of the design. The REPORTS directory includes the following:

- The Design directory contains the reports for the complete design.
- Each hierarchical master, including the top level, has its own directory that contains the corresponding reports.

Example

For a design with master blocks A and B, the following four directories are created:

- Design – full design reports
- Top Block – top-level reports
- Master Block A – reports for master block A

- Master Block B – reports for master block B

To support this enhancement, the following parameters have been introduced:

<code>set_voltus_insight_mode</code>	
<code>-all_scenario_ranking {wiv tiv}</code>	Specifies that all scenarios are ranked either based on the total number of violations (TIV) or worst violations (WIV).
<code>-scenario_ranking {wiv tiv powerrlrp powerreff groundrlrp groundreff}</code>	
	Specifies that the scenario ranking is done for a single scenario.
<code>-groundREFF_threshold value</code>	Specifies that the violation report contains only instances that have values less than the specified ground REFF threshold.
<code>-groundRLRP_threshold value</code>	Specifies that the violation report contains only instances that have values less than the specified ground RLRP threshold.
<code>-powerREFF_threshold value</code>	Specifies that the violation report contains only instances that have values less than the specified power REFF threshold.
<code>-powerRLRP_threshold value</code>	Specifies that the violation report contains only instances that have values less than the specified ground RLRP threshold.
<code>get_ir_insight</code>	
<code>-report_mode {summary_only detailed}</code>	Controls the type of reports generated.

Example

```
set_voltus_insight_mode -config config.txt -domain ALL -db_mapping db_mapping.txt
get_ir_insight -report_mode detailed
```

Enhanced Voltus InsightAI Commands for Timing Path Protection during PG Reinforcement

The `set_voltus_insight_mode` and `get_voltus_insight_mode` commands now include new parameters to help protect timing paths during PG stripe reinforcement.

set_voltus_insight_mode	
<code>-path_group {ALL reg2reg}</code>	
	Specifies which timing paths to protect during <code>reinforce_pg</code> .
<code>-timing_protection_config filename</code>	
	Defines timing degradation thresholds per timing view using a configuration file.
<code>-initialize</code>	
	Saves the current power settings before running the Insight repair commands using internal power/rail values. After InsightAI-based analysis, this parameter enables restoration of the original power settings.
get_voltus_insight_mode	
<code>-timing_protection_config filename</code>	
	Specifies to automatically generate the timing protection configuration file. This file includes the timing degradation thresholds per timing view.

Generation of Voltus InsightAI Database

Voltus has been enhanced to generate the InsightAI database from rail analysis results. This database can be directly used for subsequent IR drop fixing operations, eliminating the need to reload the rail results. In addition, the database preserves the reinforce power-grid information, which is then applied to support incremental power-grid fixing. To enable this workflow, two new parameters have been added to the `set_voltus_insight_mode` command: `input_insight_db` and `output_insight_db`.

Use Model

1. Generate the output database using the `-output_insight_db` parameter. The database is stored in the path: `<output_db>/master_directory`.
The indicative structure of the database is as following:
`<output_db>/master1/`
`<output_db>/master2/`
`<output_db>/master3/`
2. Use the generated database as the input database specified with `-input_insight_db`. The specified database will be one of the master databases generated using `-output_insight_db`. You can then run `reinforce_pg` without loading the entire rail database, enabling you to fix issues without reloading the rail result.

Example:

1st Step: Output Database Generation

```
set_voltus_insight_mode -config <insight_config> -import_analysis_data -db_mapping  
<db_mapping_file> -output_insight_db <output_db>  
get_ir_insight -mode repair_directive_only | report_and_repair_directive
```

The database is generated under the directory `<output_db>`

2nd Step: Insight Database Fixing

```
set_voltus_insight_mode -config -input_insight_db <output_db>  
reinforce_pg -auto_ir_fix postroute
```

create_die_model Command Enhanced

The `-local_reference_ground` parameter has been added to the `create_die_model` command to assign a ground source as reference ground locally for sources in the current file `.isrc`. You can specify the reference node in the PLOC file as "RefGnd=PortName" to compute the isrc of port by considering reference ground locally during die-model generation.

Use model:

```
create_die_model \  
-local_reference_ground true \  
-port_grouping_by_ploc_files true \  
-generate_SIPi_port_definition_file true \  
-disable_isrc_node_zero true \ (make isrc with ref ground)  
-disable_global_node_zero false (keep global node zero in ckt)
```

Support to Exclude Taps in a PGV

Now, you can exclude the taps for a particular cell and pin of the specified layer by using the `-cell_eval_tap_layer_file` parameter of the `set_rail_analysis_mode` command. The power-gate taps cannot be changed by this parameter.

The parameter allows you to specify a file in the following format:

```
CELL_NAME PIN_NAME LAYER_NAME
```

The file supports wildcards (*) for cell name. You can specify `top`, `bottom`, or `all` for the layer name.

File Format Example:

```
=== $file ===  
CELL_NAME PIN_NAME LAYER_NAME  
BUF_* VDD METAL_1
```

create_current_region Command Enhanced

A new parameter, `-on_interdie_bump`, has been added to the `create_current_region` command to create tap nodes only on non-vsrc PLOC nodes. When the option is set to `true`, the number of total tap changes to include the tap nodes only on non-vsrc PLOC. You can check the change in total taps in the “Grid Statistics of Net XXX” section of the log file at `<state`

```
directory>/logs/design_report/dmg/ext_report.log
```

Use Model:

```
create_current_region -on_interdie_bump true
```

Runtime Optimization for Reading the DEF files

Voltus has been enhanced to parse the largest DEF file on the master machine. You can then reuse the data of the parsed-DEF file from the specified directory using the `-`

`xp_reuse_parse_def_directory` parameter of the `set_rail_analysis_mode` command in the XP mode. This enhancement significantly reduces the runtime required for reading the large DEF files.

Use Model:

```
set_rail_analysis_mode -xp_reuse_parse_def_directory directory_name
```

Example:

```
set_rail_analysis_mode -xp_reuse_parse_def_directory  
/DefHierReport/rail_dynamic/core_125C_dynamic_1
```

Support to Suppress the Negative RC values

A new parameter, `-suppress_negative_res`, has been added to the `create_die_model` command to suppress the negative resistor and capacitor (RC) values during die-model generation. When this parameter is set to `true`, the generated netlist contains positive RC values with voltage-controlled (VC), current-controlled(CC), and function-controlled (FC) sources to ensure accuracy and stability in the die models.

Use model:

```
create_die_model -suppress_negative_res true
```

convert_gds_to_def Command Enhanced

The `-tech_gds_layermap` parameter has been added to the `convert_gds_to_def` command to support the reading of GDS layermap file with DEF or LEF names. You can use this parameter to specify a file that contains layer mapping between GDS and tech layers. Now, you do not need to convert the DEF or LEF layers to qrcTechLayer for the layer map file.

The format of the layer mapping file is:

```
<layer_name> <layer_type> <gds layer#> <gds layer data type>
```

`<layer_type>` specifies the type of def or lef layer.

`<tech layer name>` specifies the name of the def or lef layer to map to the GDSII layer number.

`<gds>` specifies the keyword for the GDS layer mapping.

`<gds layer#>` specifies the layer number of the GDSII layer.

Example:

```
m0 TEXT 55 2
```

Voltus InsightAI Enhancements

The following new parameters have been added to the `get_ir_insight` commands to identify aggressor candidates with maximum switching currents to guide power integrity improvements:

Parameter	Description
<code>-cap_lower_limit</code>	Specifies the minimum load capacitance value driven by aggressor candidates in the <code>eco_report</code> mode.

- cap_upper_limit	Specifies the maximum load capacitance value driven by aggressor candidates in the <code>eco_report</code> mode.
----------------------	--

read_power_rail_results Command Enhanced

Starting this release, you can use the `-force` option of the `read_power_rail_results` command to block the pop-up window that appears when the `read_power_rail_results -reset` parameter is specified. The pop-up window displays a confirmation message for resetting the power and rail directories.

Use Model:

```
read_power_rail_results -reset -force
```

Single Partition Support During Extraction

Voltus now supports single partitioning when extracting the specified metal layers. This helps to minimize extraction fracturing at partition boundaries, leading to better RC grid quality. With this enhancement, the false EM violations on the partition boundaries can be avoided.

To support this, two new parameters are added to the `set_rail_analysis_mode` command:

- `-single_partition_extraction_layer` - Specifies to extract RC using a single partition on a top metal layer.

Use model:

```
set_rail_analysis_mode -single_partition_extraction_layer {METAL_LAYER }
```

Example:

```
set_rail_analysis_mode -single_partition_extraction_layer {METAL_8}
```

- `-single_partition_extraction_layer_list` - Specifies to extract RC using a single partition on multiple layers.

Use model:

```
set_rail_analysis_mode -single_partition_extraction_layer_list {METAL_LAYER_1  
METAL_LAYER_2 ..... }
```

Example:

```
set_rail_analysis_mode -single_partition_extraction_layer_list {METAL_5 METAL_8}
```

Ability to Exclude Instances during Rail Extraction

A new parameter, `-inst_ignore_file`, has been added to the `set_rail_analysis_mode` command to exclude the LEAF instances mentioned in the specified file during rail extraction.

Use Model:

```
set_rail_analysis_mode -inst_ignore_file {filename}
```

File Format:

```
Inst1  
Inst2  
.  
.  
.  
InstN
```

Support to Read Power Data to Identify PTI Files

The `-power_directory` parameter has been added to the `set_power_data` command to read the power data from the specified directory for cell power. You no longer need to define each PTI file individually. Instead, you can use this parameter to read `power_results.json` and automatically identify all the PTI files. If the `power_results.json` is not found in the specified directory, then the power data could be retrieved from `dir/voltus_power_output.latest`. When specified, the `-power_directory` parameter takes precedence and bypasses the `-format` parameter.

Use Model:

```
set_power_data -cell <cell name> -power_directory <power directory for cell power>
```

Example:

```
set_power_data -cell top_design -power_directory ./power
```

Ability to Reuse HPT Data

A new parameter, `-xp_reuse_hpt_directory`, has been added to the `set_rail_analysis_mode` command to support the reuse of hierarchical path tracing (HPT) data from the HPT directory of a previous run with the modified extraction options. With this enhancement, you no longer need to run HPT again if there are no DEF changes in the component section or logical connectivity and can use the earlier HPT data to avoid unnecessary runtime. The reuse of HPT data is also allowed if the DEF changes are related to routing shape only.

```
set_rail_analysis_mode -xp_reuse_hpt_directory <state directory>
```

set_die_model Command Enhanced

A new parameter `-static_current` has been added to the `set_die_model` command to use the average of PWL waveform as the static current for static rail analysis. Earlier, only the current value at $t=0$ from the PWL waveform was considered for static run.

Use Model:

```
set_die_model -static_current initial | average
```

Example:

```
set_die_model -static_current average
```

Multi-Die IR Analysis

- [Release 26.10 Enhancements](#)
 - [Voltus IR Co-simulation with Multi-die and Package](#)

Release 26.10 Enhancements

Voltus IR Co-simulation with Multi-die and Package

Advanced 2.5D and 3D packaging technologies (InFO, CoWoS, WoW) are increasingly complex for power integrity analysis due to heterogeneous chip integration and high-performance requirements, with hundreds of millions of instances. Voltus multi-die capability in XP mode delivers comprehensive chip-package-board power signoff co-analysis, enabling:

- Concurrent static/dynamic IR/EM analysis across dies and silicon interposers
- Accelerated runtime performance
- Net- and pin-based package specification for HBM die-models and stacked dies
- Full system PG connectivity and IR/EM verification through co-simulation

Note: Multi-die analysis is available exclusively in XP mode.

For more information, refer to [Voltus Multi-die IR Analysis](#).