




dummy_calib_tsbl_scan_raw {name == 4000 && channels == 0}

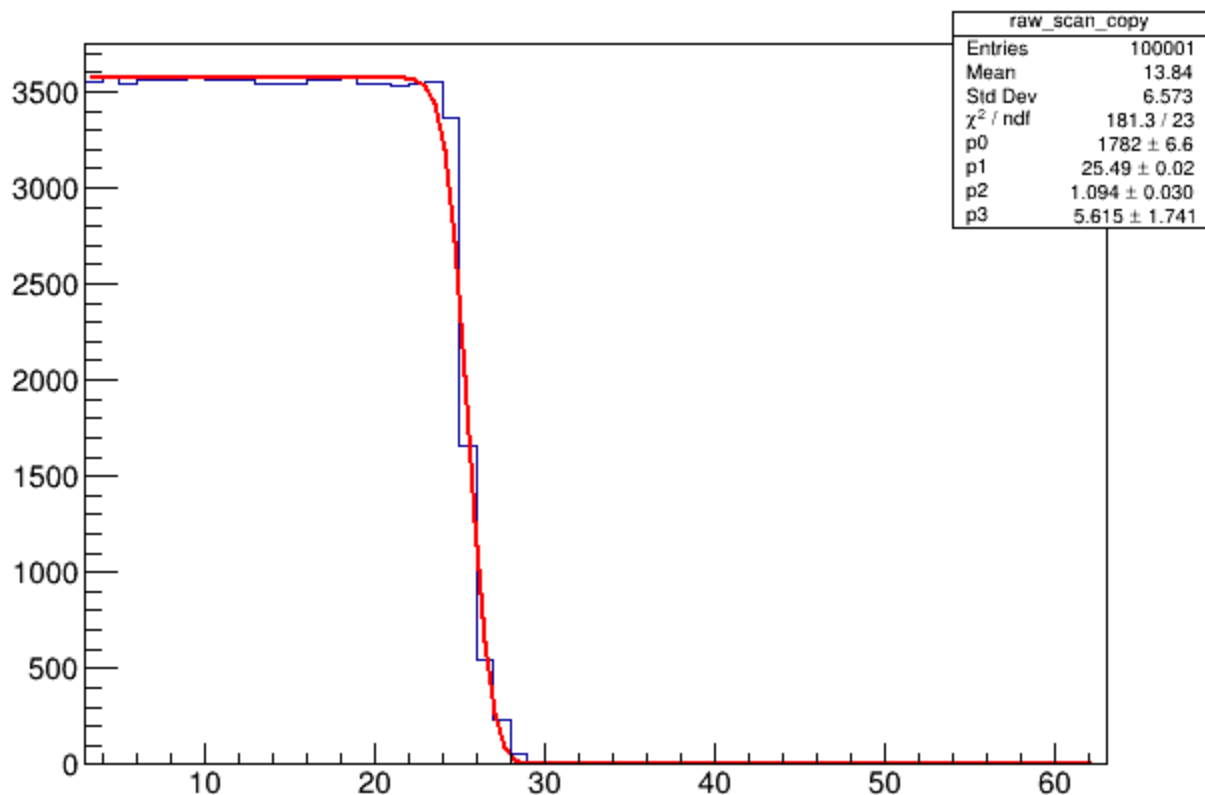


dummy_calib_tsbl_scan_raw {name == 4000 && channels == 1}

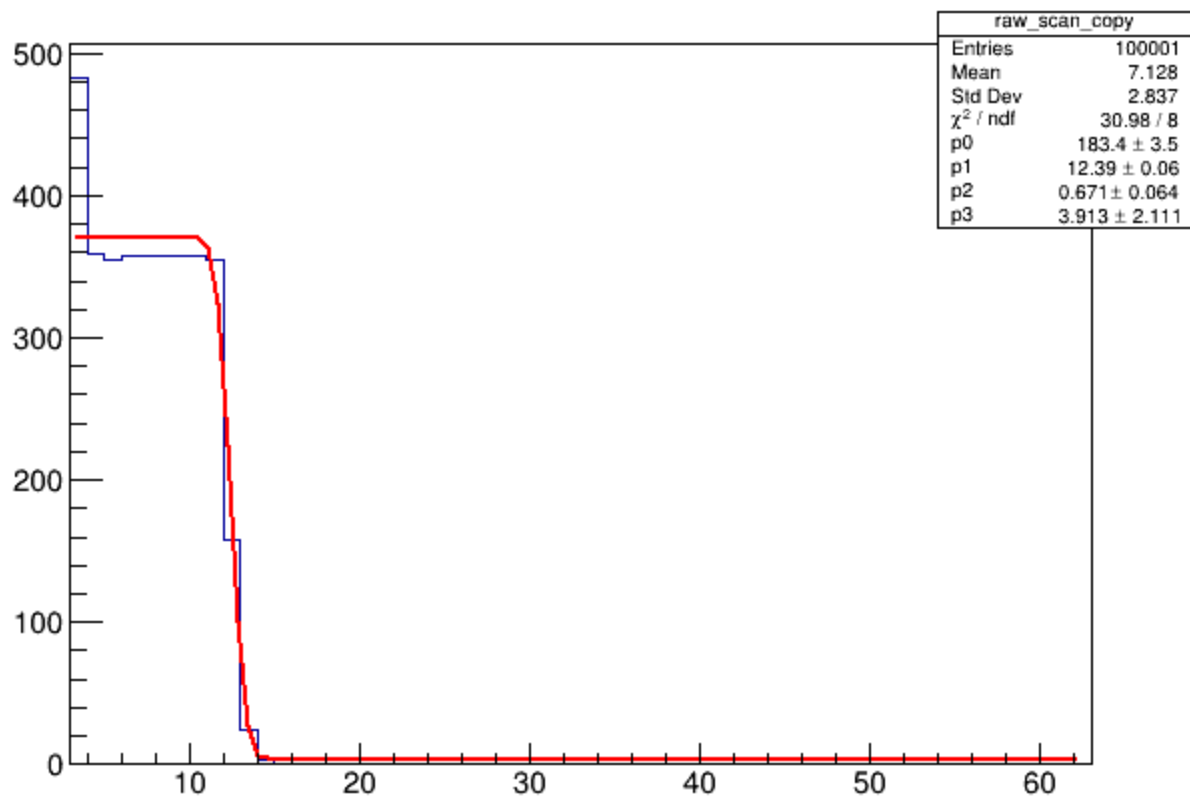


dummy_calib_tsbl_scan_raw {name == 4000 && channels == 2}

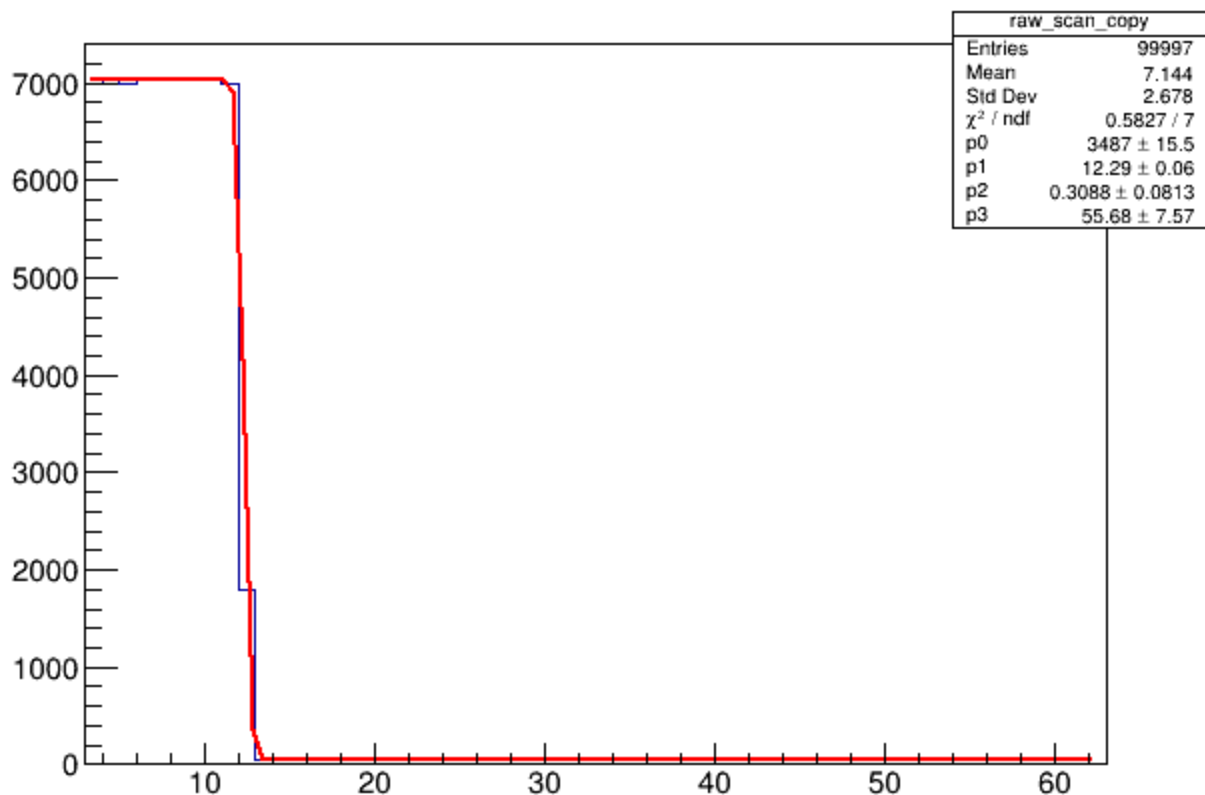


dummy_calib_tsbl_scan_raw {name == 4000 && channels == 3}

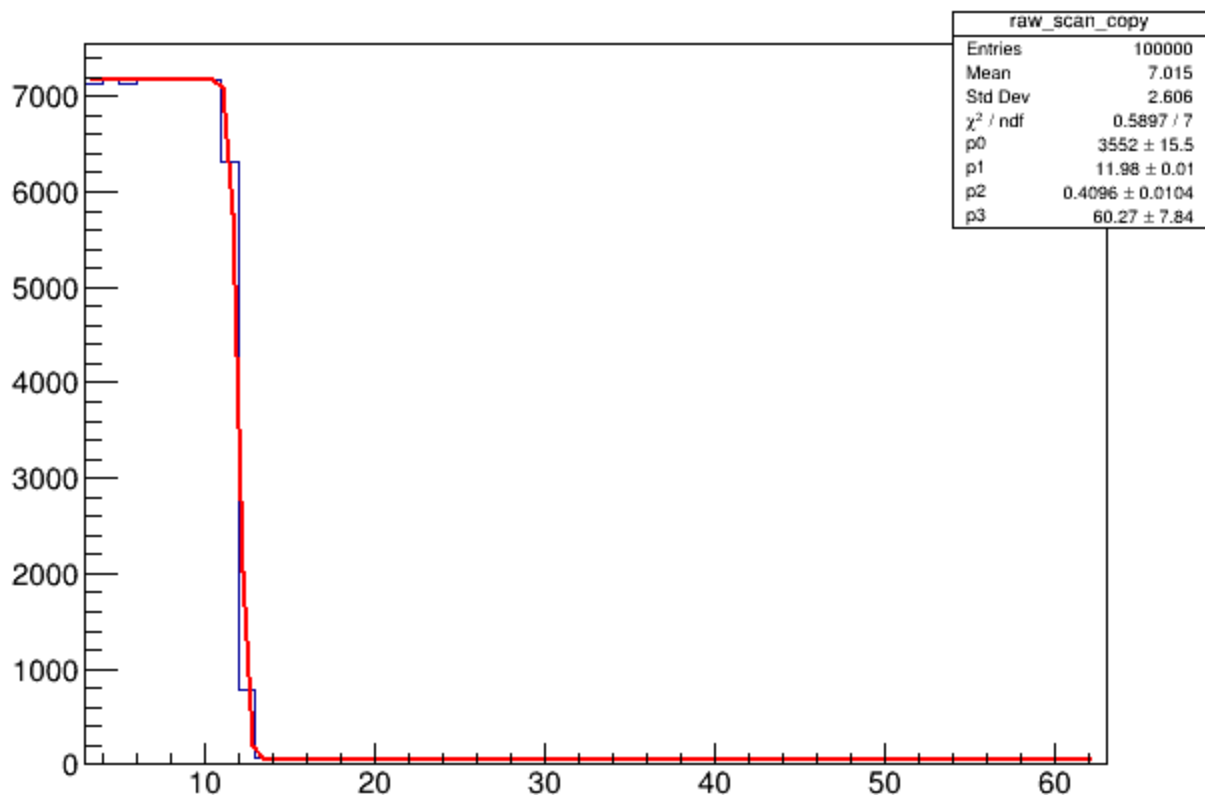

dummy_calib_tsbl_scan_raw {name == 4000 && channels == 4}

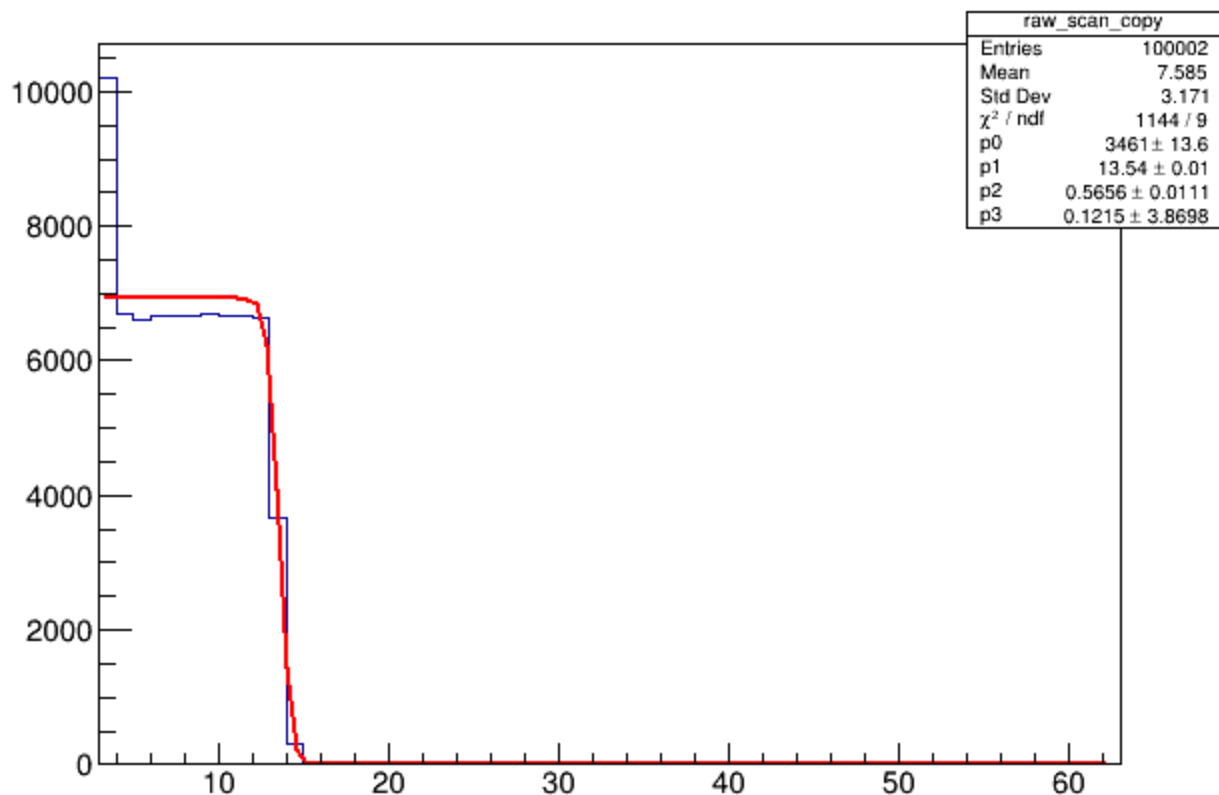


dummy_calib_tsbl_scan_raw {name == 4000 && channels == 5}

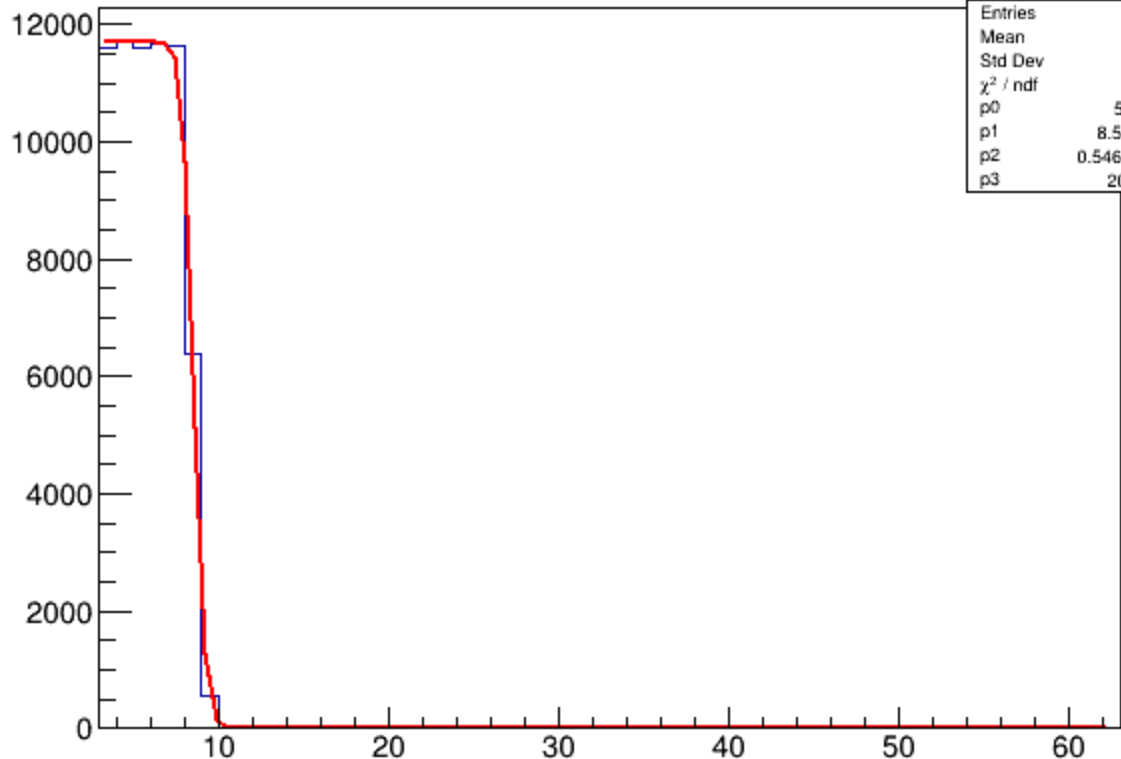

raw_scan_copy

Entries	100002
Mean	5.329
Std Dev	1.644
χ^2 / ndf	6.213 / 4
p0	5834 ± 25.1
p1	8.568 ± 0.009
p2	0.5464 ± 0.0082
p3	20.85 ± 4.88

dummy_calib_tsbl_scan_raw {name == 4000 && channels == 6}

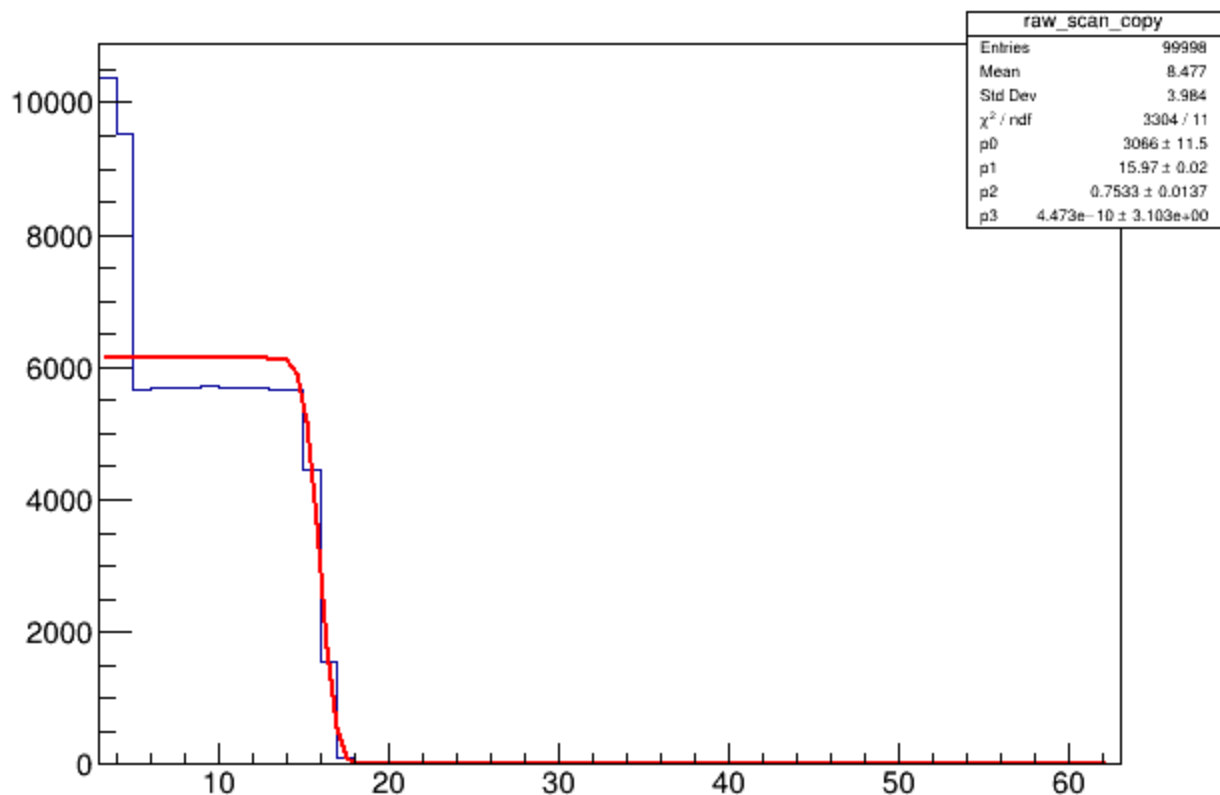

dummy_calib_tsbl_scan_raw {name == 4000 && channels == 7}

