

**SOLVENT DELIVERY MODULE  
FOR SHIMADZU HIGH PERFORMANCE  
LIQUID CHROMATOGRAPH  
LC-20AB**

**INSTRUCTION MANUAL**

Read the instruction manual thoroughly before you use the product.  
Keep this instruction manual for future reference.

**SHIMADZU CORPORATION**  
ANALYTICAL & MEASURING INSTRUMENTS DIVISION  
**KYOTO, JAPAN**

This page is intentionally left blank.

# Introduction

**Read this manual thoroughly before using the instrument.**

Thank you for purchasing this instrument. This manual describes: the installation, operation, hardware validation, cautions for use, and details on the accessories and options. Read the manual thoroughly before using the instrument. Use the instrument in accordance with the manual's instructions. Keep this manual for future reference.

## IMPORTANT

- Do not use this instrument before fully understanding the contents of this manual.
- Provide this documentation to the next user in the event that the instrument is borrowed or sold.
- If this documentation or the warning labels on the instrument become lost or damaged, promptly obtain replacements from your Shimadzu representative.
- To ensure safe operation, read the **Safety Instructions** before using the instrument.

## COPYRIGHT

- Copyright (C) 2004-2005 Shimadzu Corporation. All rights reserved. This publication may not be reproduced in whole or in part without written permission from Shimadzu Corporation. Since Shimadzu products are frequently upgraded and improved, information in this publication is subject to change without notice. We appreciate notification of any errors or omissions.

# Warranty and After-Sales Service

## Warranty

### 1. Validity

Please consult your Shimadzu representative for information about the extent of the warranty.

### 2. Term

The manufacturer will provide free replacement parts for, or repair free of charge, any instrument that fails during the warranty period, if the cause can be attributed to a defect in manufacturing.

### 3. Items Not Covered by the Warranty

The warranty does not cover malfunctions that result from:

- 1) misuse;
- 2) repairs or modifications made by any company other than the manufacturer or an approved company;
- 3) external factors;
- 4) operation under severe conditions such as environments, with high temperature, high humidity, corrosive gas, vibration, etc.;
- 5) fire, earthquake or other forces of nature;
- 6) moving or transporting the instrument after its initial installation;
- 7) the consumption of items or parts that can be regarded as consumable.  
(For example, the service life of an LCD display panel depends on the actual operating conditions.)

## After-Sales Service

If any problem occurs with this instrument, inspect it and take appropriate corrective action as described in the Section "[6 Troubleshooting](#)". If the problem persists, or symptoms not covered in the Troubleshooting section occur, contact your Shimadzu representative.

## Replacement Parts Availability

Replacement parts for this instrument will be available for a period of seven (7) years after the discontinuation of the product. Thereafter, such parts may cease to be available. Note, however, that the availability of parts not manufactured by Shimadzu shall be determined by the relevant manufacturers.

## Hardware Validation

Each LC component and the entire LC system should be checked periodically to ensure that they function normally, or the analysis data may not be reliable. To this end, it is necessary to carry out periodic hardware validation and keep records of the validation. There are two types of hardware validation - component validation and system validation. The purpose of component validation is to check that the individual components of the system function normally, while the system validation checks that the system as a whole (the several components in combination) functions normally.

Before shipment from the factory, this instrument was rigorously inspected. The results are summarized in the Inspection Certificate accompanying the instrument. To inspect the instrument performance after installation, repeat the Hardware Validation as described in "[7 Hardware Validation](#)".

 ["7 Hardware Validation" P. 7-1](#)

## Hardware Validation Contract

This is a contract under which a qualified Shimadzu-approved engineer performs periodic component and system validation, and provides reports of the results. Details of the contract can be obtained from your Shimadzu representative.

# Safety Instructions

- To ensure safe operation of the instrument, read these Safety Instructions carefully before use.
- Observe all of the **WARNINGS** and **CAUTIONS** described in this section. They are extremely important for safety.
- In this manual, warnings and cautions are indicated using the following conventions;

<b>⚠ WARNING</b>	Indicates a potentially hazardous situation which, if not avoided, could result in moderate to serious injury or possibly death.
<b>⚠ CAUTION</b>	Indicates a potentially hazardous situation which, if not avoided, may result in minor injury or equipment damage.
<b>NOTE</b>	Emphasizes additional information that is provided to ensure the proper use of this instrument.

## ■ Application Precautions


<b>⚠ WARNING</b>
This instrument is a solvent delivery module for use with a high performance liquid chromatography system.
<b>Use this instrument ONLY for the intended purpose.</b>
Using this instrument for any other purpose could cause accidents.

## ■ Installation Site Precautions

### **⚠ WARNING**

- The solvents used in high performance liquid chromatograph are flammable and toxic. The room where the instrument is installed should be well ventilated; otherwise, solvent vapors could cause poisoning or ignite and cause a fire.**
- High performance liquid chromatograph uses large amounts of flammable organic solvents. Use of open flame in the vicinity of this instrument must be strictly prohibited. Do not install the instrument in the same room with any other equipment that emits or could potentially emit sparks, since sparks could cause a fire.**

Provide fire extinguishers for use in case of fire.

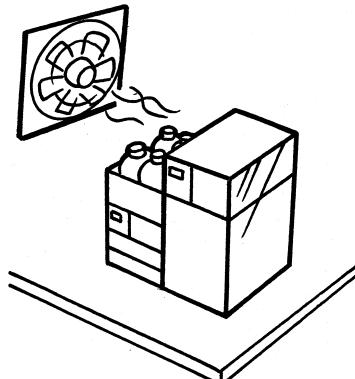

- Provide protective equipment near the instrument.**

If solvent gets into the eyes or on the skin, it must be flushed away immediately. Provide equipment, such as eye wash stations and safety showers, as close to the instrument as possible.




### **⚠ CAUTION**

- The weight of this instrument is 13kg. During installation, consider the entire weight combined with other LC components.**

The lab table on which this instrument is installed should be strong enough to support the total weight of the LC system. It should be level, stable and have depth of at least 600mm.

Otherwise, the instrument could tip over or fall off the table.

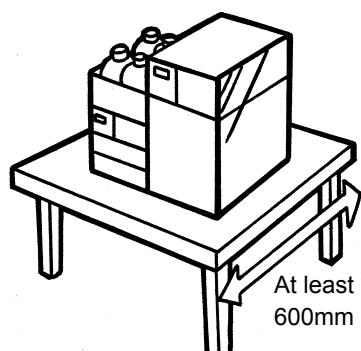

- Avoid installation sites that are exposed to corrosive gases or excessive dust.**

These adverse conditions may be detrimental to maintaining the instrument performance and may shorten its service life.

## ■ Installation Precautions

### ⚠ WARNING

- Take measures to prevent the instrument from falling in the event of an earthquake or other disaster.

Strong vibrations could cause the instrument to fall over, resulting in injury.

- The power supply voltages and power consumptions of this instrument are listed below. The power supply voltage of the instrument is indicated on the label on the back of the instrument. Connect the instrument only to a power supply of the voltage indicated; otherwise, fire or electric shock could result. Check that the power supply voltage is stable and that its current capacity is sufficient to operate all the components of the system. If not, the instrument will not operate at its rated performance.


Part No.	Power Supply Voltage (indicated on the instrument)	Power Consumption	Frequency
228-45002-31	AC100-120V (100-120V~)	180VA	50/60Hz
228-45002-32	AC100-120V (100-120V~)	180VA	50/60Hz
228-45002-38	AC220-240V (220-240V~)	180VA	50/60Hz

- **Ground the instrument.**

Grounding is necessary to prevent electric shock in the event of an accident or electrical discharge, and important for ensuring stable operation.

- **Do not place heavy objects on the power cord, and keep any hot items away.**

The cord could be damaged, resulting in fire, electrical shock or malfunction. If the cord becomes damaged, contact your Shimadzu representative immediately.

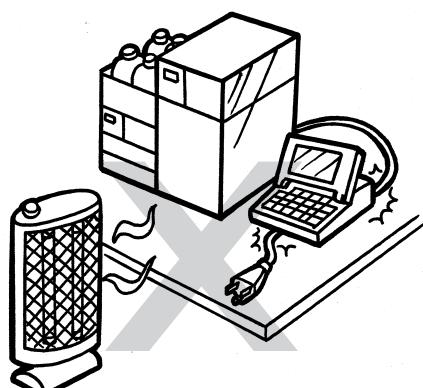

- **Do not modify the cord in any way. Do not bend it excessively or pull on it.**

The cord could be damaged, resulting in fire, electrical shock or malfunction. If the cord becomes damaged, contact your Shimadzu representative immediately.

## **⚠ CAUTION**

- When installing the instrument, be careful not to pinch your fingers between the system components, as this could result in injury.
- When opening the doors, be careful not to pinch your fingers as this could result in injury.



## ■ Operation Precautions

### **⚠ WARNING**

- Take thorough measures to prevent buildup of static electricity.

"Static Electricity Precautions" P.IX

Static electricity could result in fires or explosions.




- Always wear protective gloves and protective goggles when handling solvents and samples.  
If solvent gets into the eyes, blindness could result.  
Should solvent get into the eyes, flush immediately with large amounts of water and get medical attention.



- Always wear protective gloves when handling any toxic or biologically infectious samples.

- Never use a cracked reservoir bottle.  
If a helium degasser is used, pressure is exerted on the reservoir bottles and may cause cracks in the bottles.  
It could break the reservoir bottles and cause injury.

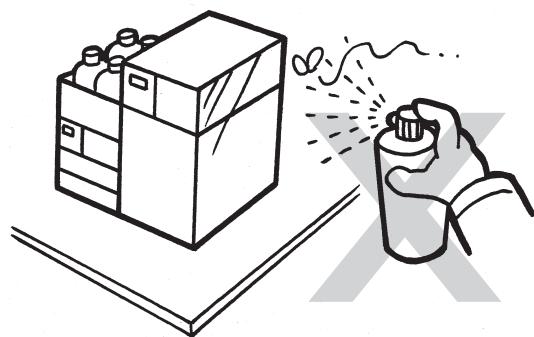

- Do not use flammable sprays (hair sprays, insecticide sprays, etc.) near the instrument.  
They could ignite and cause a fire.

■ Precautions for Instrument Inspection, Maintenance, Adjustment and Care

**⚠ WARNING**

- **Unplug the instrument before inspection, maintenance, or parts replacement.**

Otherwise, electrical shock or short-circuit accidents could occur.

- **Never remove the main cover.**

This may cause injury or malfunction of the instrument.

The main cover does not need to be removed for routine maintenance, inspection and adjustment. Have your Shimadzu representative perform any repairs requiring removal of the main cover.



- **Replace fuses only with fuses of the proper type and capacity.**

Any other fuses could cause a fire.

- **If the power cord plug gets dusty, remove the plug from the power outlet and wipe away the dust with a dry cloth.**

If dust is allowed to accumulate, fire could result.

- **Replacement parts must be of the specifications given in "1.3 Component Parts" or "9.3 Maintenance Parts".**

Use of any other parts may result in instrument damage and malfunction.

- **If any water gets onto the instrument, wipe it away immediately to prevent rust. Never use alcohol or thinner solvents for cleaning the instrument.**

They could cause discoloration.

- **Dispose of the waste liquid properly and in accordance with the instruction by your administrative department.**


# Static Electricity Precautions

Liquid chromatograph (LC) uses flammable organic solvent(s) as the mobile phase. LC systems are also often used where large amount of flammable substances are present. Thus, an accident can produce large scale damage. Operators must be constantly on guard against accidents involving fire or explosion.

The major cause of these accidents is static electricity. Devising preventative measures for static can be difficult, because the symptoms before an accident vary and can be hard to detect, since such accidents occur as a result of several simultaneous coincidences. Recommended methods for preventing static electricity accidents are provided below. Take thorough safety measures based on this information.

## ■ Typical Cause of Static Electricity Accidents

Static electricity accidents are generally caused by this sequence of events:

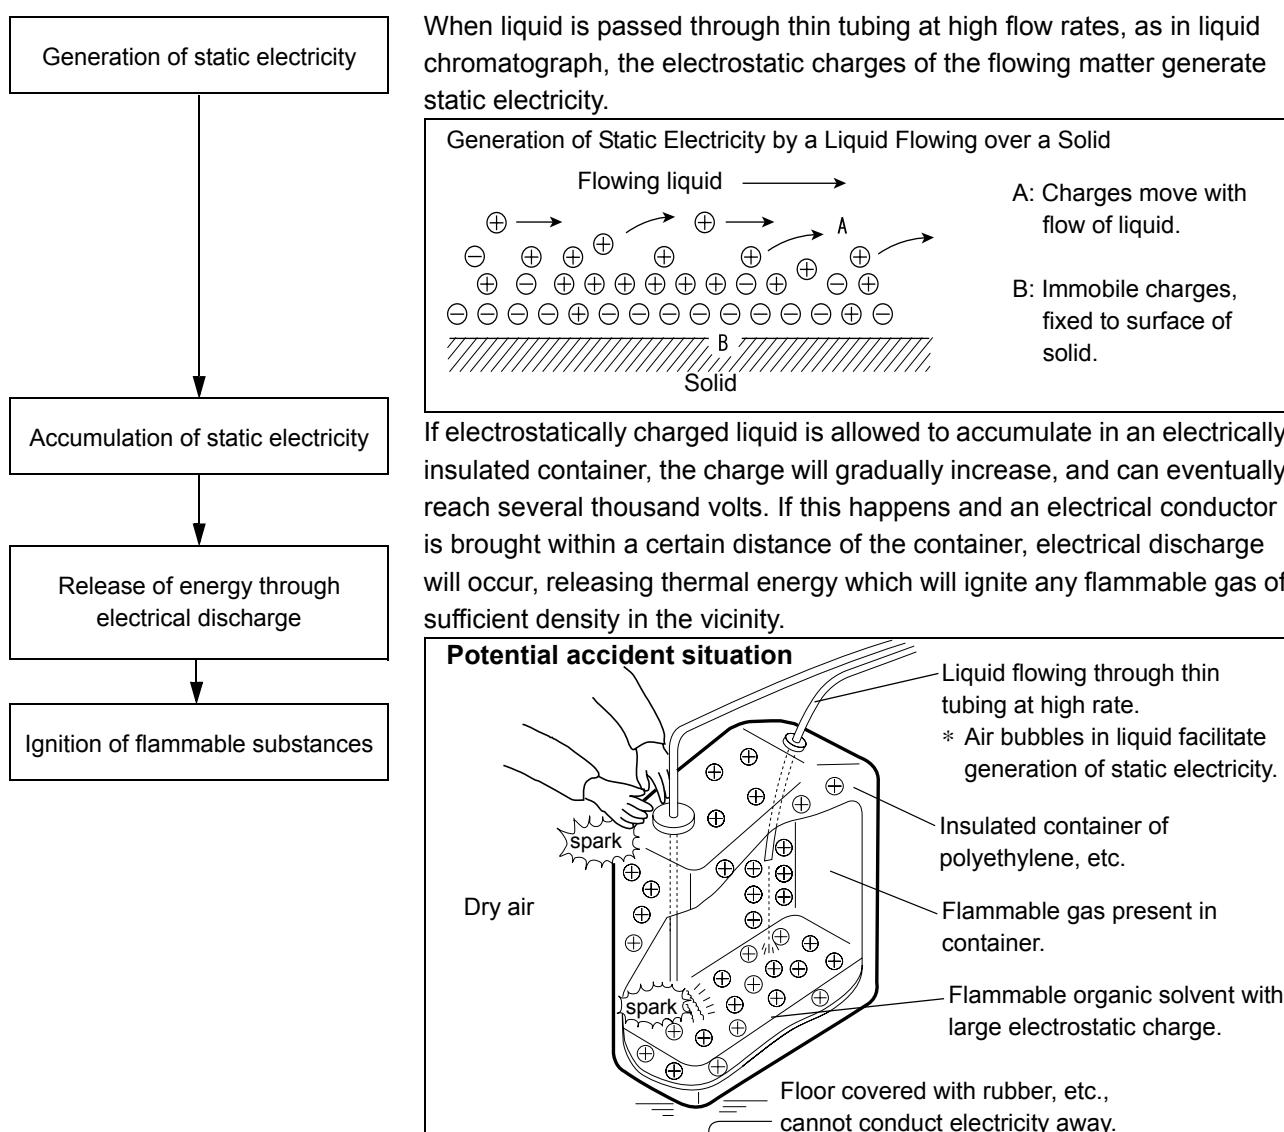

### ■ Preventing Static Electricity Accidents

The best way to prevent static electricity accidents is simply to prevent the occurrence and accumulation of electrostatic charges.

#### **⚠ CAUTION**

- It is important to take multiple preventive measures simultaneously.
- If large amounts of flammable solvents are collected in a large container, implement preventative measures 1, 2, and 3 below.

#### **Preventive Measure 1**

Use a metal container for the waste liquid, and ground the container.

This will ensure that the electrical charges of the container and liquid pass to the ground.

#### **Accessories for this measure**

- |                              |                       |
|------------------------------|-----------------------|
| (1) Grounding wire with clip | Part No. 228-21353-91 |
| (2) 18 Liter metal container | Part No. 038-00044    |
| (3) 4 Liter metal container  | Part No. 038-00043-01 |

#### **⚠ CAUTION**

- Be sure to ground the metal waste container properly.


If the grounding wire is not properly attached or connected to the ground, static electricity can build up in the container.

- Some metal containers have surfaces that are laminated or oxidized, and therefore do not conduct electricity. After grounding the metal container, use a tester to verify that electricity is conducted to the ground.

- If the liquid to be drained into the waste container is virtually non-conductive ( $10^{-10}$  S/m or less), it will be necessary to add properly conductive, and therefore safe, liquid to the tank.

This conductive liquid may be added beforehand.

#### **Preventive Measures for Static**

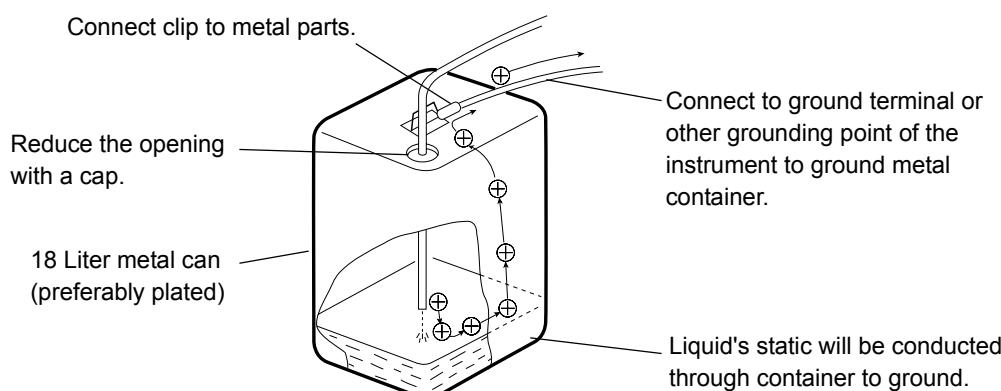

### **Preventive Measure 2**

Cover the spaces between the tubing and the sides of the inlet and outlet openings of the waste container with caps or other protective covering. This will prevent any sparks generated outside the container from getting inside.

#### **Accessories for this measure**

Caps for 18 liter or 4 liter containers (with three 3mm diameter openings)

Part No. 228-21354-91

### **Preventive Measure 3**

Keep electrostatically charged objects, including the human body, away from the waste liquid container.

To prevent electrostatic charging of the human body, take the following precautions:

- Wear anti-static clothing and shoes.
- Ground the human body with anti-static wrist straps. (For safety, the wrist strap should be connected to the ground using an intervening resistor of about  $1M\Omega$ .)
- Spread anti-static matting or the like on the floor, to make the floor conductive.



### **CAUTION**

- **Persons who have not taken anti-static precautions should touch some grounded metal object before coming near the waste liquid container, in order to drain static charges.**

### **Preventive Measure 4**

Use tubing with an inner diameter of at least 2mm for drain lines with high flow rates.



### **CAUTION**

- **Periodically check the tubing connections for leaks.**

Air bubbles in liquid can multiply the electrostatic charge by a factor of 20, 30 or more.

### **Preventive Measure 5**

If it is not possible to use a conductive waste liquid container, take the following precautions:

- Ensure that the end of the inflow tubing is always submerged inside the container. Also, place some type of grounded metal object, such as a ground wire connected to the instrument, into the liquid.

### **⚠ CAUTION**

**The above precaution will be ineffective for low conductivity (less than  $10^{-10}$  S/m) liquids.**

- **Use as small a container as possible to minimize damage in the event of fire.**
- **Keep the room at a proper humidity.**

Ambient humidity exceeding 65% will prevent static.

### **For Reference**

Anti-static equipment (anti-static clothing, shoes and matting) and charge measurement equipment (potentiometer) are sold by specialty manufacturers.

# Precautions for Mobile Phase Selection and Use



## CAUTION

- If PEEK resin parts are used in the plumbing, do not use the following mobile phases. These mobile phases weaken the PEEK resin, which could result in cracked plumbing and mobile phase leaks.

Concentrated sulfuric acid, concentrated nitric acid, dichloroacetic acid, acetone, tetrahydrofuran (THF), dichloromethane, chloroform, dimethyl sulfoxide (DMSO).

Note: Briefly using a weak solution of less than 0.5% acetone in water (e.g. in order to check gradient performance) will present no problems.


### NOTE

- Use only HPLC grade or comparable mobile phase, and filter it with a filter of 0.45 $\mu$ m mesh or finer before use to remove particulates and foreign matter.
- Halogen ions can corrode the stainless steel material (SUS316L) used in the plumbing, so avoid, as much as possible, mobile phases that contain halogen ions - such as KCl, NaCl and NH<sub>4</sub>Cl - or mobile phases that generate halogen ions in certain reactions. If such mobile phases must be used, clean all flow lines thoroughly with distilled water immediately after analysis.
- When SPD or a similar UV detector is used for high-sensitivity analysis, be sure to use HPLC grade mobile phases that have a low absorptivity of UV rays.
- Always degas the mobile phase, as air bubbles may tend to form during solvent mixing or during temperature or pressure changes. Air bubbles may cause pump malfunctions and detector signal noise.
- For boiling points, viscosities and other data relating to the mobile phases used,  
 "9.5 Mobile Phase Characteristics" P. 9-44

## Warning Labels

For safety operation, warning labels are affixed to where special attention is required. Should any of these labels peel off or be damaged, obtain replacements from Shimadzu Corporation.

Warning label (Part No. 228-42603)

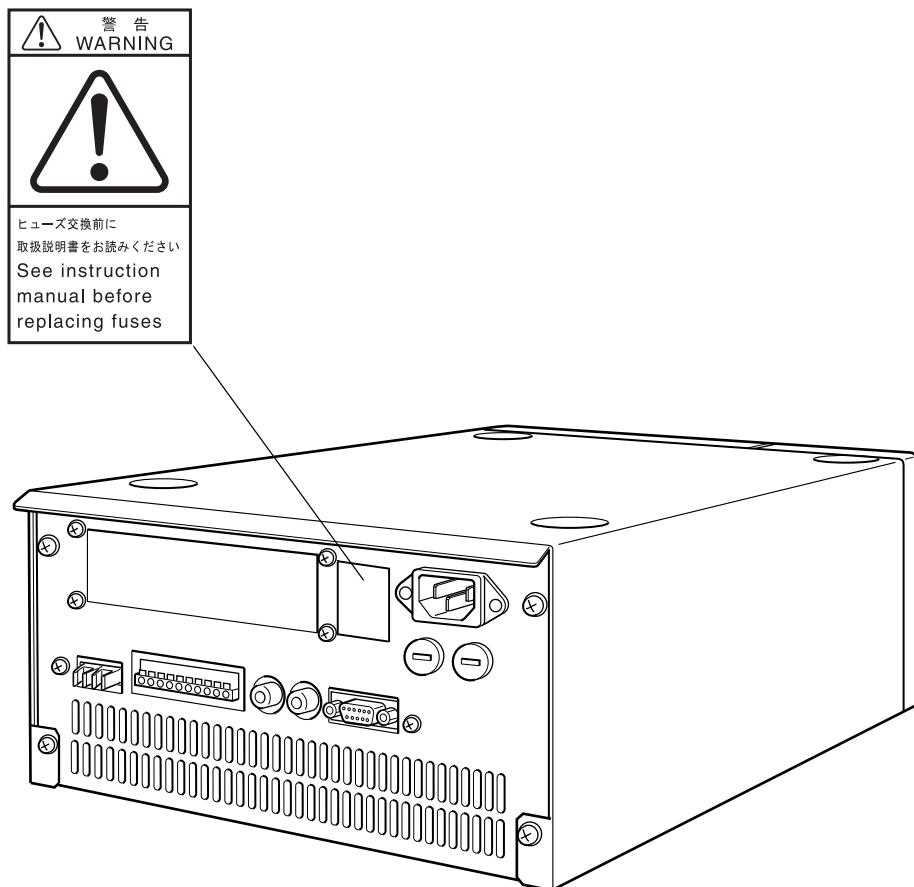

# Contents

---

Introduction .....	I
Warranty and After-Sales Service .....	II
Safety Instructions .....	IV
■ Application Precautions .....	IV
■ Installation Site Precautions .....	V
■ Installation Precautions .....	VI
■ Operation Precautions .....	VII
■ Precautions for Instrument Inspection, Maintenance, Adjustment and Care .....	VIII
Static Electricity Precautions .....	IX
■ Typical Cause of Static Electricity Accidents .....	IX
■ Preventing Static Electricity Accidents .....	X
Precautions for Mobile Phase Selection and Use .....	XIII
Warning Labels .....	XIV

## Chapter 1 Configuration

---

1.1 Overview .....	1-2
1.2 Features .....	1-2
1.3 Component Parts .....	1-3
■ Accessory Pack .....	1-4
1.4 Optional Parts .....	1-5

## Chapter 2 Parts Identification and Function

---

2.1 Front Cover .....	2-2
2.2 Behind Front Cover .....	2-3
2.3 Right Side and Base Panel .....	2-5
2.4 Back .....	2-6
2.5 Names and Functions of Displays and Keypad .....	2-7
2.5.1 Display Panel .....	2-7
2.5.2 Keypad .....	2-8

## Chapter 3 Preparation

---

3.1 Turning Power ON/OFF .....	3-2
3.2 Preparation before Operation .....	3-3

3.3	Checking Pressure Value .....	3-5
-----	-------------------------------	-----

## Chapter 4 Basic Operation

---

4.1	Setting Parameters .....	4-2
4.1.1	Prior to Key Operation .....	4-2
4.1.2	Setting Flow Rate .....	4-3
4.1.3	Setting the Concentration of Mobile Phase B .....	4-4
4.2	Operation .....	4-5
4.3	Plunger Rinsing When Buffer Solution is Used as Mobile Phase .....	4-6
4.3.1	Operation Method for Automatic Rinsing Kit .....	4-6
■	Preparation .....	4-6
■	Operation .....	4-7
4.3.2	Operation Method for Manual Rinsing .....	4-8
■	Connection .....	4-8
■	Operation .....	4-9
4.4	Replacing the Mobile Phase .....	4-10
4.4.1	When New Mobile Phase is Miscible with the Old Mobile Phase .....	4-10
4.4.2	When New Mobile Phase is not Miscible with the Old Mobile Phase .....	4-12
4.4.3	When Buffer Solution is Used as Mobile Phase .....	4-12
4.4.4	Rinse When Buffer Solution is Used .....	4-12

## Chapter 5 Application Operation

---

5.1	Display Panel .....	5-2
5.1.1	Types of Screens .....	5-2
5.1.2	Basic Setting Screen and Auxiliary Function Setting Screen .....	5-3
5.1.3	VP Function Screen .....	5-8
5.2	Parameter in Auxiliary Functions .....	5-12
5.2.1	List of Auxiliary Functions .....	5-12
■	Parameter Settings Group .....	5-12
■	File Operation Group .....	5-12
■	Control Settings Group .....	5-13
■	System Settings Group .....	5-13
■	Monitor Settings Group .....	5-13
5.2.2	Showing the Auxiliary Function Screen .....	5-14
5.2.3	Parameter Settings Group .....	5-15

■ Setting Maximum Pressure Limit [PMAX] .....	5-15
■ Setting Minimum Pressure Limit [PMIN] .....	5-15
■ Setting Solenoid Valve Position [SV] .....	5-16
■ Setting EVENT Output Terminals [EVENT] .....	5-17
■ Setting Fine Adjustment of Compressibility Compensation [ACOMP] [BCOMP] ....	5-17
■ Setting Purge Time [P-TIMER] .....	5-18
■ Setting Purge Flow Rate [P-FLOW] .....	5-18
■ Setting Maximum Pressure Limit during Purging [P-PMAX] .....	5-18
5.2.4 File Operation Group .....	5-19
■ File Number [FILE NUM] .....	5-19
■ Copying a File [FILE CPY] .....	5-19
■ Deleting a Time Program [FILE DEL] .....	5-19
5.2.5 Control Settings Group .....	5-20
■ Plunger Set [P-SET] .....	5-20
■ Zero Adjustment of Pressure Sensor [ZERO ADJ] .....	5-20
5.2.6 System Settings Group .....	5-21
■ Selecting Local/Remote Mode [LOCAL] .....	5-21
■ Setting Link Address [ADRS] .....	5-21
■ Disables Key Entry [KEY CLOSE] .....	5-21
■ Setting Brightness of Display Screen [BRIGHT] .....	5-22
■ External Signal Functions for EVENT Output Terminals [EXT-S] .....	5-22
■ Setting System Protection [S-PROT] .....	5-22
■ Selecting Flow Channel Valve Type [FCV TYPE] .....	5-23
■ Selecting a Unit of Pressure [PRS-UNIT] .....	5-23
■ Setting Pressure Recorder Range [RANGE] .....	5-23
■ Switching Remote Connector internal/external [CBM LINK] .....	5-23
■ Setting Operation of Buzzer [BEEP MODE] .....	5-24
5.2.7 Monitor Settings Group .....	5-24
■ Monitoring Program Elapsed Time [MON TIME] .....	5-24
■ Monitoring ID for Remote Control [MON ID] .....	5-25
■ Monitoring Flow Line of Solenoid Valve Unit [MON SV] .....	5-25
■ Monitoring Pump Revolution Counter [MON REVA] [MON REVB] .....	5-26
■ Monitoring Vacuum Pressure in Degasser Unit [DEGAS PRS] .....	5-26
5.3 VP Functions .....	5-27
5.3.1 List of VP Functions .....	5-27
■ Mobile Phase Monitor Group .....	5-27
■ Product Information Group .....	5-27
■ Maintenance Information Group .....	5-27
■ Validation Support Group .....	5-28
■ Calibration Support Group .....	5-28
5.3.2 Displaying the VP Functions .....	5-29
5.3.3 Mobile Phase Monitor Group .....	5-30
■ Showing/Setting Mobile Phase Volume [MOBILE PHASE A/B] .....	5-30
■ Setting Alarm Level of Remaining Mobile Phase [ALARM LEVEL] .....	5-30

---

5.3.4	Product Information Group .....	5-31
■	Showing Serial Number [SERIAL NUMBER] .....	5-31
■	Showing S/W Version No. [S/W ID] .....	5-31
5.3.5	Maintenance Information Group .....	5-31
■	Showing Total Operating Time [TOTAL OP TIME] .....	5-31
■	Showing Timing to Replace Plunger Seal [A/B SEAL DELIVERED] .....	5-32
■	Entering Replaced Part No. [PART REPLACEMENT] .....	5-32
■	Showing Maintenance Log [MAINTENANCE LOG] .....	5-32
■	Showing Error Log [ERROR LOG] .....	5-33
■	Showing Operation Log [OPERATION LOG] .....	5-33
5.3.6	Validation Support Group .....	5-34
■	Entering Date [DATE] .....	5-34
■	Entering Time [TIME] .....	5-34
■	Checking Memory [MEMORY CHECK] .....	5-35
■	Checking Pulsation [PULSE CHECK A/B] .....	5-35
■	Checking Flow Rate [FLOW CHECK A/B] .....	5-36
■	Setting Time Program to Check Concentration Accuracy of Gradient Mode [GE TEST PROGRAM] .....	5-36
■	Checking Leakage [LEAKAGE TEST] .....	5-37
■	Checking Leak Sensor [LEAK SENSOR TEST] .....	5-37
5.3.7	Calibration Support Group .....	5-38
■	Inputting Password [Input PASSWORD] .....	5-38
■	Setting Flow Rate Compensation Parameter (ALPHA) [FLOW COMP FACT A/B] .....	5-38
■	Setting Pressure Sensor Sensitivity Compensation Factor [PRESS COMP FACT] .....	5-38
■	Setting Operation Level of Leak Sensor [LEAK THR] .....	5-39
■	Setting Timing to replace Plunger Seal [SEAL REPLACEMENT] .....	5-39
■	Selecting Operation Mode [OP MODE] .....	5-39
■	Initializing Parameters [INITIALIZE PARAM] .....	5-39
■	Changing Passwords [CHANGE PASSWORD] .....	5-40
■	Showing/Setting CBM Parameter [CBM PARAMETER] .....	5-40
5.4	Creating Time Program .....	5-44
5.4.1	Time Program Command .....	5-44
5.4.2	Description of Time Program Screen .....	5-45
5.4.3	Time Program Creating Flow .....	5-46
5.4.4	Creating Time Program .....	5-47
5.4.5	Creating High-Pressure Gradient Programs .....	5-50
5.4.6	Deleting Steps .....	5-51
5.4.7	Starting and Stopping a Time Program .....	5-51
■	Starting a Time Program .....	5-51
■	Stopping a Time Program .....	5-51
5.4.8	Commands Used Only For Time Program .....	5-52
■	Setting Stop Command of Time Program [STOP] .....	5-52

---

■ Setting Loop Count of Time Program [LOOP] .....	5-52
■ Switching File [GOTO] .....	5-53
5.5 Control by CBM-20A or CBM-20Alite System Controller .....	5-54
5.5.1 Preparation .....	5-54
5.5.2 Basic Parameters .....	5-54
5.6 Control by SCL-10Avp or SCL-10A System Controller .....	5-55
5.6.1 Preparation .....	5-55
5.6.2 Basic Parameters .....	5-55
5.6.3 Attention .....	5-55
5.7 Connection to External Input/Output Terminals .....	5-56
5.7.1 External Input/Output Terminals .....	5-56
5.7.2 Connection of Event Cable .....	5-57

## Chapter 6 Troubleshooting

---

6.1 Troubleshooting and Corrective Action .....	6-2
6.2 Error Message .....	6-5

## Chapter 7 Hardware Validation

---

7.1 Overview of Hardware Validation .....	7-2
7.1.1 Hardware Validation .....	7-2
7.1.2 Types of Hardware Validation .....	7-2
7.2 Implementation of Hardware Validation .....	7-3
7.2.1 Periodic Validation .....	7-3
7.2.2 Daily Inspection .....	7-3
7.2.3 Validation After Maintenance .....	7-3
7.3 Validation Precautions .....	7-4
7.3.1 Environment .....	7-4
7.3.2 Installation Site .....	7-4
7.4 Equipment Required for Validation .....	7-5
■ Testing Equipment .....	7-5
■ Standard Reagents for Validation .....	7-6
■ Hardware Testing Supplies .....	7-6
7.5 Validation: Pump .....	7-7
7.5.1 Check Terms .....	7-7

7.5.2	ROM, RAM Self Diagnosis .....	7-7
■	Objective .....	7-7
■	Check Procedure .....	7-7
7.5.3	Firmware Version Check .....	7-8
■	Objective .....	7-8
■	Check Procedure .....	7-8
7.5.4	Display, LED Test .....	7-8
■	Objective .....	7-8
■	Check Procedure .....	7-8
7.5.5	Flow Rate's Control Parameter .....	7-9
■	Objective .....	7-9
■	Check Procedure .....	7-9
7.5.6	Pumping Stability Test .....	7-10
■	Objective .....	7-10
■	Items Required for Check .....	7-10
■	Check Procedure .....	7-10
■	Resetting after Check .....	7-12
7.5.7	Pressure Limiter Test .....	7-12
■	Objective .....	7-12
■	Items Required for Check .....	7-12
■	Check Procedure .....	7-12
7.5.8	Leak Sensor Test .....	7-15
■	Objective .....	7-15
■	Check Procedure .....	7-15
7.5.9	Flow Rate Accuracy Test .....	7-16
■	Objective .....	7-16
■	Items Required for Check .....	7-16
■	Check Procedure .....	7-16
■	Resetting after Check .....	7-18
7.6	Validation: Gradient Pump System .....	7-19
■	Objective .....	7-19
■	Items Required for Check .....	7-19
■	Check Procedure .....	7-19
7.7	System Validation .....	7-23
7.7.1	Validation of Isocratic LC system .....	7-23
■	Objective .....	7-23
■	Items Required for Validation .....	7-23
■	Checking and Preparing the LC system .....	7-24
■	Validation Procedure .....	7-25
■	Parameter Settings for Isocratic System Validation .....	7-26
7.7.2	Validation of Gradient LC System .....	7-27
■	Objective .....	7-27
■	Items Required for Validation .....	7-27

---

■ Checking and Preparing the LC System .....	7-27
■ Validation Procedure .....	7-28
■ Parameter Settings for Gradient System Validation .....	7-30
7.8 If Validation Fails .....	7-31

## Chapter 8 Maintenance

---

8.1 Periodic Inspection and Maintenance .....	8-2
8.1.1 Prior to Inspection and Maintenance .....	8-2
8.1.2 List of Periodic Inspection and Maintenance .....	8-3
8.1.3 Check after Inspection and Maintenance .....	8-4
8.2 Replacement of Plunger Seal .....	8-5
8.2.1 Before Removing Pump Head .....	8-5
8.2.2 Removing Pump Head .....	8-6
8.2.3 Replacing Plunger Seal .....	8-7
8.2.4 Installing Pump Head .....	8-8
8.2.5 Check after Replacement .....	8-9
8.3 Cleaning and Inspection (Replacement) of Plungers and Diaphragms .....	8-10
8.3.1 Removing Pump Head and Head Holder ASSY .....	8-10
■ When the Head Holder is difficult to remove .....	8-11
8.3.2 Cleaning and Inspecting (Replacing) of Plungers .....	8-11
8.3.3 Inspection (Replacement) of Diaphragms .....	8-12
8.3.4 Re-Installing after Inspection .....	8-12
8.3.5 Check after Cleaning and Inspection (Replacement)	8-14
■ If Air Is Leaked .....	8-14
8.4 Cleaning of Check Valves .....	8-15
8.5 Inspection (Replacement) and Ultrasonic Bath Cleaning of Check Valves .....	8-16
8.6 Inspection (Replacement) and Ultrasonic Bath Cleaning of Line Filter .....	8-19
■ Replacing Frit .....	8-20
8.7 Inspection (Replacement) and Ultrasonic Bath Cleaning of Suction Filter .....	8-21
8.8 Replacement of Drain Valve ASSY .....	8-22
8.9 Replacement of Fuse .....	8-24
8.10 Wiping of Leak Tray .....	8-25
8.11 Exterior Cleaning .....	8-26

# Chapter 9 Technical Information

---

9.1	Installation .....	9-2
9.1.1	Installation Site .....	9-2
■	Suitable Sites and Preparation .....	9-2
■	Required Installation Space .....	9-3
9.1.2	Installation .....	9-4
■	Remove the Shipping Screws .....	9-4
■	Installation .....	9-4
■	Stacking Brackets .....	9-4
9.1.3	Power Supply Connection .....	9-5
■	Connection to Power Outlet .....	9-5
■	Grounding .....	9-6
9.1.4	Prior to Plumbing .....	9-6
■	Types of Tubings and Connectors .....	9-6
■	Cutting Tubings .....	9-6
■	Connecting Tubings .....	9-8
■	Protective Plugs .....	9-9
9.1.5	Plumbing .....	9-10
■	Reservoir and Waste Container Preparation .....	9-11
■	Front Cover Removal .....	9-11
■	Suction Filter (Accessory) Installation .....	9-12
■	Drain Tubing (Accessory) Installation .....	9-13
■	Connecting Leakage Drain Tubing .....	9-14
■	Front Cover Installation .....	9-18
9.1.6	Installation of Manual Injector and Column .....	9-18
■	Installation of Manual Injector .....	9-18
■	Installation of Column Holder .....	9-20
9.1.7	Flow Line Plumbing .....	9-20
■	Manual Injector Plumbing .....	9-20
■	Plumbing between Pump Unit and Manual Injector .....	9-21
■	Plumbing between Manual Injector and Column .....	9-22
■	Plumbing between Column and Detector .....	9-23
9.1.8	Installation and Plumbing of Mixer (Option) .....	9-24
■	Preparation of Mixer .....	9-24
■	Mounting the Mixer on the Instrument .....	9-25
■	Mixer Plumbing .....	9-26
■	Mixer Cover Installation .....	9-27
9.1.9	Wiring .....	9-28
■	Connectors .....	9-28
■	Connecting the Optical Cable .....	9-29
■	Connection to System Controller .....	9-30
■	Connection to System Controller (in case of the installed CBM-20Alite) .....	9-31

---

■ Connection of [DGU/SOL.V] Connector .....	9-32
■ Connection of [PUMP PRESS] Connector .....	9-33
■ Connection of [DGU PRESS] Connector .....	9-33
9.1.10 Installation of Automatic Rinsing Kit (Optional) .....	9-34
9.2 Specifications .....	9-37
9.2.1 LC-20AB Pump Unit .....	9-37
9.2.2 High-Pressure Gradient System .....	9-38
■ High-Pressure Gradient System controlled by System Controller (CBM-20A) .....	9-38
■ High-Pressure Gradient System controlled by Pump Unit (LC-20AB) .....	9-38
9.3 Maintenance Parts .....	9-39
9.3.1 Consumable Parts .....	9-39
9.3.2 Replacement Parts .....	9-39
■ Mechanical Parts .....	9-39
■ Electrical Parts .....	9-40
9.3.3 Maintenance Kit .....	9-40
9.4 Introduction to HPLC System .....	9-41
9.4.1 Example of a Simple (Isocratic) System .....	9-41
■ Solvent Flow .....	9-41
■ Function of Components .....	9-41
9.4.2 Example of Autosampler System (1) .....	9-42
■ Solvent Flow .....	9-42
■ Function of Components .....	9-42
9.4.3 Example of Autosampler System (2) .....	9-43
■ Solvent Flow .....	9-43
■ Function of Components .....	9-43
9.5 Mobile Phase Characteristics .....	9-44

---

## Index

This page is intentionally left blank.

# 1

---

## Configuration

### Contents

1.1	Overview .....	1-2
1.2	Features .....	1-2
1.3	Component Parts .....	1-3
1.4	Optional Parts .....	1-5

## 1.1 Overview

LC-20AB (hereinafter to as the instrument) is a high-pressure gradient solvent delivery module equipped with two dual-plunger tandem-flow pumps. It offers improved accuracy and sensitivity in high-performance liquid chromatograph. In addition to the instrument, a high performance liquid chromatography system requires an autosampler, column oven, detector and system controller at a minimum, which should be purchased separately. Consult your Shimadzu representative regarding the components required for your system.

## 1.2 Features

- **Low Flow Pulsation and Pulsation Period Enable Precise Delivery**

By reducing the discharge volume per plunger stroke to the microvolume level ( $10\mu\text{L}$ ), and applying high-speed drive, the flow pulsation and pulsation period have been reduced to levels significantly lower than those for other instruments. This feature enables the use of high-sensitivity detectors, including refractive index detectors and electrochemical detectors, which are sensitive to flow pulsation. It also enables gradient delivery with a degree of precision not usually possible, even with micro-level flow rates.

- **Binary High-pressure Gradient Delivery with just One Unit**

A high-accuracy, high-pressure gradient with minimal time lag can be achieved with just one unit. It is also possible to select whether gradient control is performed from a system controller or the instrument itself.

- **Automatic Plunger Rinsing**

An optional automatic mechanism rinses the plunger and the back of the plunger seal, preventing premature seal failure due to crystallization of high-salt-concentration buffer solutions.

# 1.3 Component Parts

This instrument consists of the standard parts listed below. Check the parts against this list after unpacking. The standard parts provided depend on the power supply voltage. (See below.) After unpacking, verify that the correct types and quantity of parts have been provided.

The 2-digit numbers in the remark column in the table below indicate the power supply voltages for the part. -31 indicates use with a 100V power supply, -32 is a 120V power supply, and -38 a 220-240V power supply. These 2-digit figures refer to the last two digits in the product number of the instrument. -31 is for products destined for Japan, while -32 and -38 are for use in other countries.

Parts	Part No.	Q'ty	Remark
LC-20AB	-	1	
AC Power cord (for UL/CSA)	071-60825-01	1	-31, -32 only
AC Power cord (for VDE)	071-60825-51	1	-38 only
Adapter KPR-1	071-60813	1	-31 only
Suction filter	228-39181-95	2	
Instruction manual (Japanese version)	228-30882	1	-31 only
Instruction manual (English version)	228-30883	1	-32, -38 only
Accessory pack (See next page for contents.)	228-42650-93	1	
Signal cable	228-35047-92	1	
Event cable	228-28253-91	1	

## 1. Configuration

---

### ■ Accessory Pack

	Parts	Part No.	Q'ty	Remark
Tools	Wrench, 8 × 10	086-03006	2	
	Allen wrench 4mm	086-03805	1	
	Allen wrench A 3mm	670-18928-04	1	
	Allen wrench B 3mm	086-03804	1	
	Seal installer / remover	228-18886	1	
	Box driver	228-28767-91	1	
	File	670-18928-02	1	For cutting SUS tubing
Parts	Optical cable	070-92025-51	1	
	Tube clamp	046-00994-03	1	For securing tubings
	Bottle cap	228-18887	2	
	Lid	228-17644	2	
	Pipe clip	037-60177-05	1	For securing tubings
	Male nut, PEEK	228-18565	2	
	Male nut, 1.6MN	228-16001	2	
	Ferrule, 1.6F	228-16000-10	2	
	Drain tubing	228-25495-93	1	
	Rinse tubing	228-39184-92	2	
	Rinse tubing S	228-35463-91	4	
	Transparent tubing	228-42203	1	0.4m
	SUS pipe 1.6mm O.D. × 0.3mm I.D.	228-36993-96	1	2m
	Spiral tube wrap	018-26020-02	1	0.2m
	Syringe	046-00038-01	1	Volume: 20mL
	Syringe needle	228-18216-91	1	
	Frit	228-32744	1	For line filter
	Drain OUT, STD	228-42205	1	
	Drain OUT, CTO	228-42206	1	
	Silicone tubing	228-25162-03	1	1m
	Straight tubing connector	228-28163	1	
	L-type tubing connector	035-61561-12	1	
	Drain adapter	228-42204	1	
	Tubing holder	228-42209	3	
	Stop joint D	228-46054-91	1	
	Syringe tubing D	228-46055-91	1	Volume: 2.5mL

# 1.4 Optional Parts

Optional units available for this instrument are listed below.

For information about other optional units not listed below, contact your Shimadzu representative.

Option	Part No.	Features
Degasser (5 flow lines) DGU-20A <sub>5</sub>	228-45019-XX	Degasses mobile phase by passing through special tubing made of resin film, thereby reducing the pressure surrounding the tubing. Can separately degas up to 5 flow lines. Connected to pump unit.
Degasser (3 flow lines) DGU-20A <sub>3</sub>	228-45018-XX	Same as above, but able to separately degas up to 3 flow lines.
Degasser DGU-10B	228-45067-XX	Degasses up to four different mobile phases by means of helium. Can be switched ON/OFF at the instrument or with a system controller.
Low pressure gradient unit FCV-10ALvp	228-34700-XX	<ul style="list-style-type: none"> <li>Can switch between up to 4 liquids of mobile phases. (Low-pressure gradient is not possible.)</li> <li>Useful for auto rinsing of column and flow lines.</li> </ul>
Reservoir switching valves FCV-11AL	228-45048-XX	<ul style="list-style-type: none"> <li>Reservoir switching valves used for switching between pairs of reservoir bottles (for up to 3 flow lines).</li> <li>Each valve switches between two liquids serving one pump (for example, switches between mobile phase and rinse solution).</li> <li>FCV-11AL can perform switching for up to 3 pumps.</li> </ul>
Reservoir switching valve FCV-11ALS	228-45049-XX	<ul style="list-style-type: none"> <li>Switches between two liquids serving one pump (for example, switches between mobile phase and rinse solution).</li> <li>FCV-11ALS can perform switching for a single pump.</li> </ul>
Reservoir switching valve FCV-13AL	228-45016-XX	<ul style="list-style-type: none"> <li>Auto mobile-phase switching valve with 7 ports and 6 positions.</li> <li>Can switch between up to 6 reservoir bottles.</li> <li>FCV-13AL can be controlled via LC workstation and are connected through an option box vp to the system controller.</li> </ul>

## 1. Configuration

---

Option	Part No.	Features
Option box vp	228-45060-XX	Can house up to two FCV-11AL, FCV-11ALS or DGU-10B. Can be placed under pump to save space.
Reservoir box	228-45041-91	Holds up to seven 1-liter bottles.
SUS mixer	228-45093-91	Gradient mixer with excellent gradient performance. Capacity can be varied in 3 stages. Can be used for high-pressure, low-pressure or semi-micro gradient analysis.
Semi micro mixer	228-35830-92	Gradient mixer for semi micro with excellent gradient performance. Can be installed inside the instrument using a semi micro mixer installation kit (D/B) (228-45935-91).
Automatic rinsing kit	228-18803-92	For continuous automatic rinsing of the back side of the plunger seal, using a rinse solution. Used when system uses high-salt-concentration buffer solution.
Injector mounting plate	228-35659-92	Plate for installing manual injectors on the instrument.
Column holder	228-35655-94	For use if the column is installed on the instrument.
CBM-20Alite	228-45011-XX	CBM-20Alite system controller can be installed inside of the instrument.

# 2

---

## Parts Identification and Function

### Contents

2.1	Front Cover .....	2-2
2.2	Behind Front Cover .....	2-3
2.3	Right Side and Base Panel .....	2-5
2.4	Back .....	2-6
2.5	Names and Functions of Displays and Keypad .....	2-7

## 2.1 Front Cover

### Keypad

To operate and configure settings.

Press  to show the operation keys.


### Display panel

Comprising the display screen and LED indicator.  
Displays operational settings.

### Drain valve knob

To open the drain valve, turn this knob  
counterclockwise.

To close the valve, turn back as far as it will go.

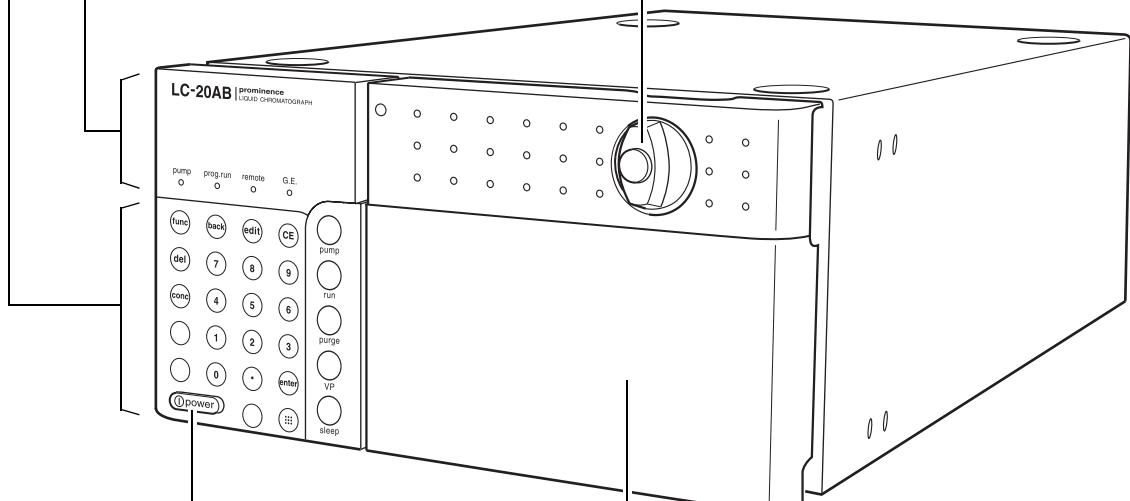


### Power switch

To switch the power ON/OFF.

Press the switch in to turn power ON.


Press again to turn power OFF.

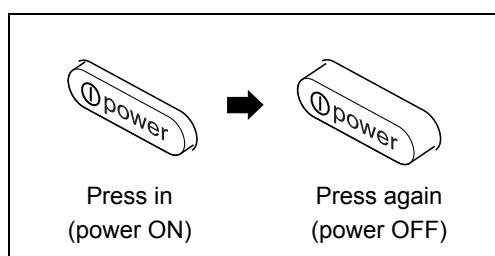

# 2.2 Behind Front Cover

The pump on the right (as viewed from the front) is pump A and the pump on the left is pump B. Each pump incorporates two of the parts marked with an asterisk.


2

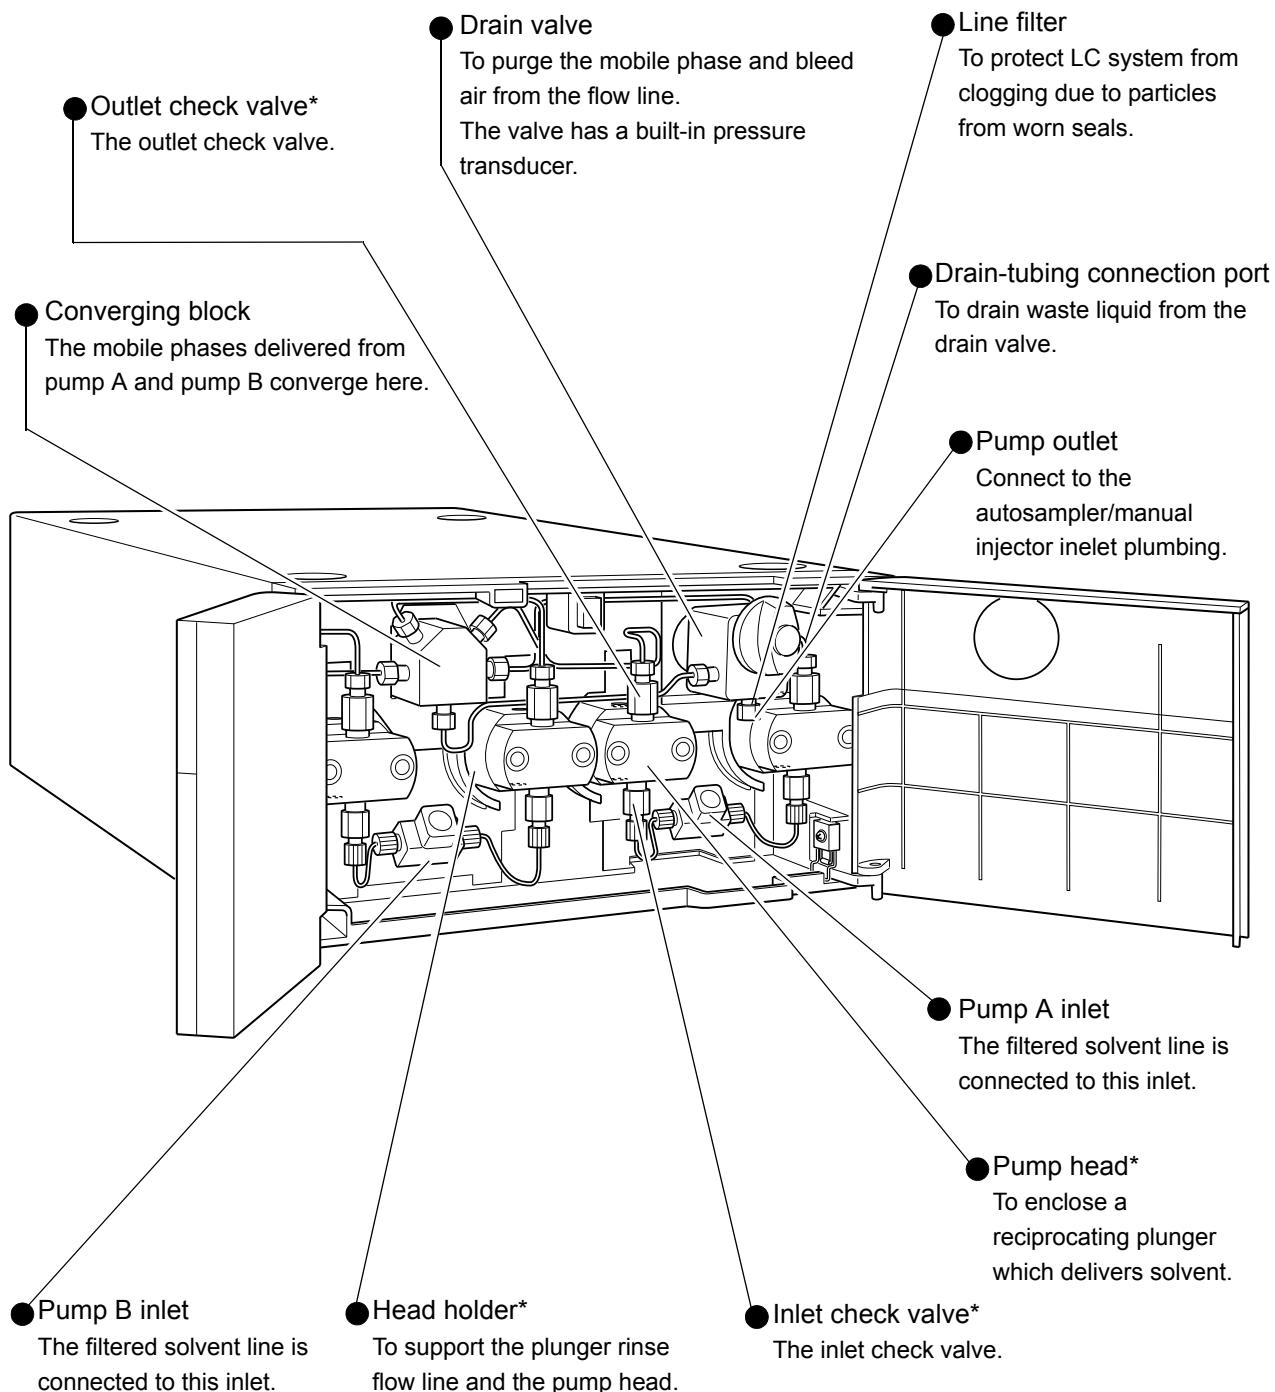

## 2. Parts Identification and Function

---

Each pump incorporates two of the parts marked with an asterisk.

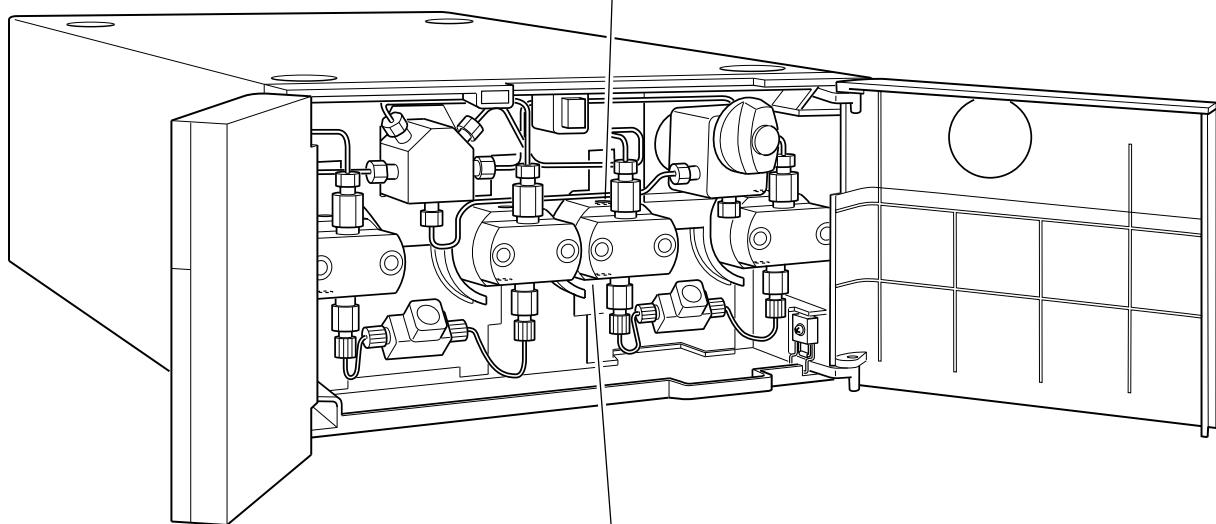

● Rinse-solution outlet\*

The outlet for the rinse flow line.


To connect rinse tubing to perform auto rinsing and manual rinsing.

● Rinse-solution inlet\*


The inlet for the rinse flow line.

To connect rinse tubing to perform auto rinsing and manual rinsing.

# 2.3 Right Side and Base Panel

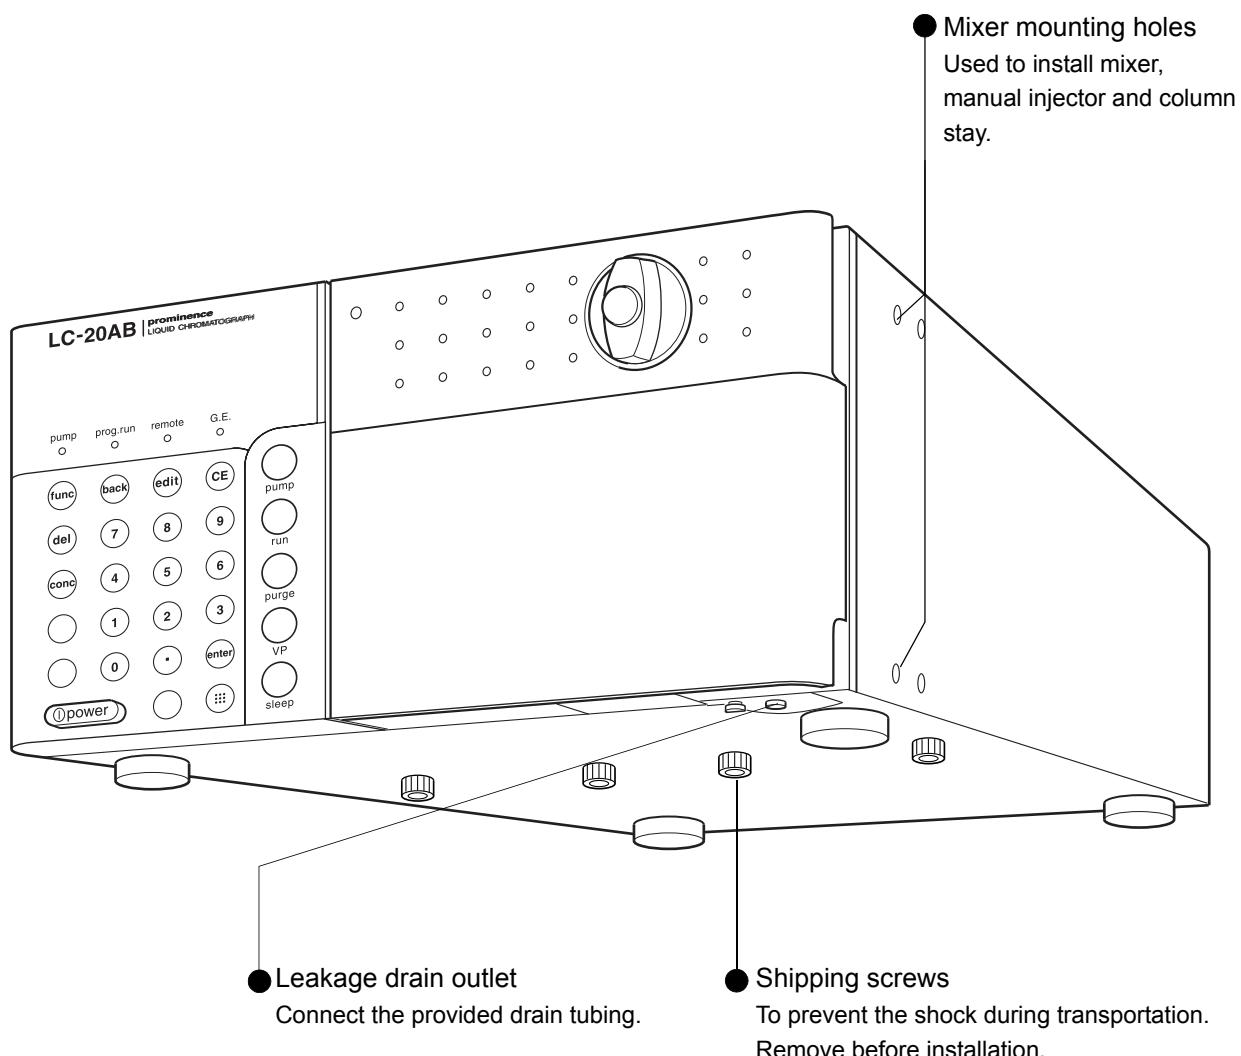

## 2.4 Back

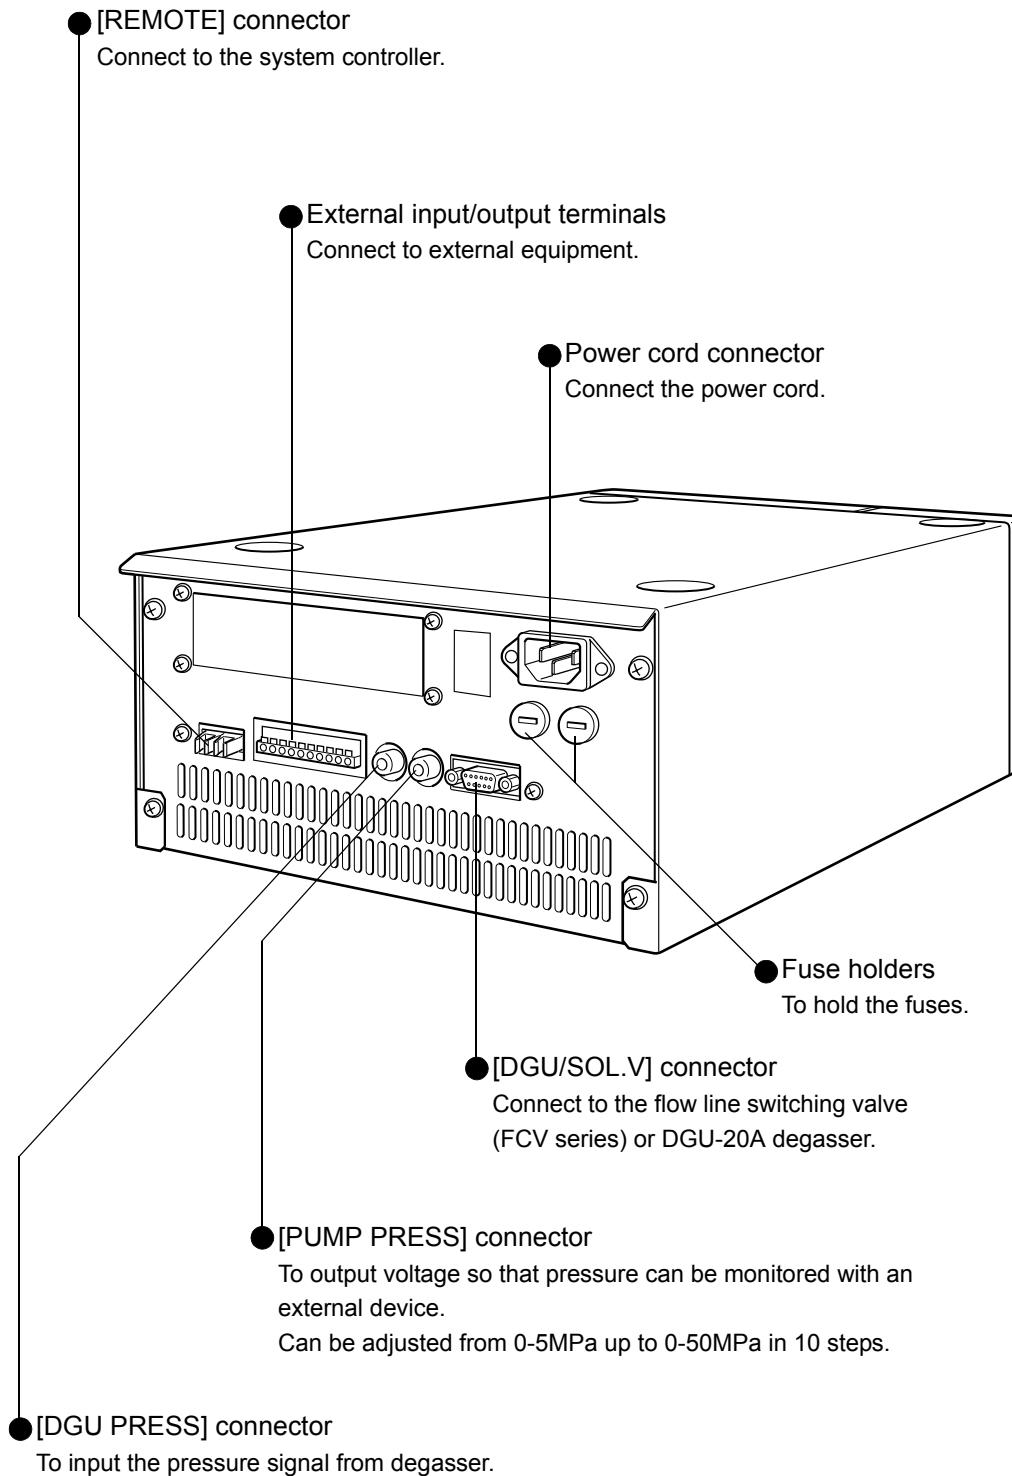


# 2.5 Names and Functions of Displays and Keypad

This instrument is controlled through the keypad.  
The display allows verification of the instruments status.

**NOTE**


The display screen may become hot when in use.

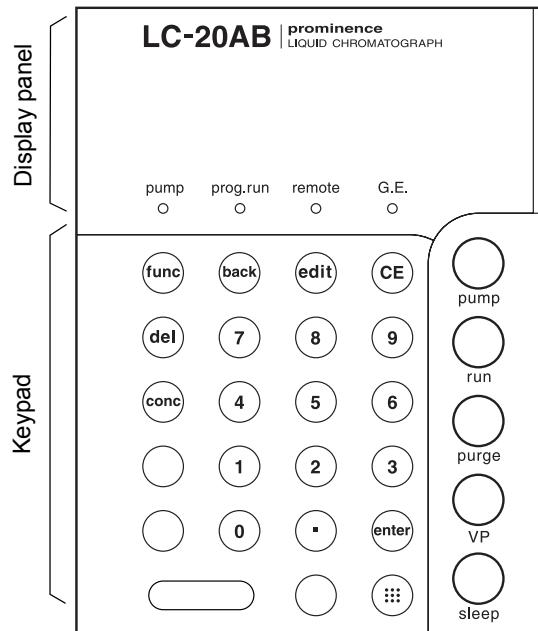

## 2.5.1 Display Panel

The display panel consists of a display screen and LED indicators.

Names and functions of the display screen and the indications are given below.

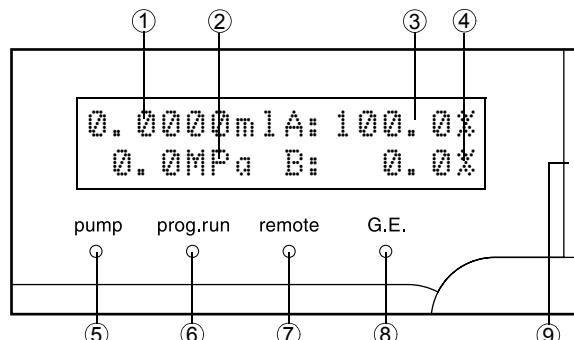


No.	Display or Indicator	Function
①	flow	Displays set flow rate (in mL/min).
②	pressure	Displays reading of pressure sensor (in units set with [PRS-UNIT] additional function).
③	ACONC	Displays concentration (%) of mobile phase A.
④	BCONC	Displays concentration (%) of mobile phase B.
⑤	pump (Pump indicator)	Illuminates when pump is running.
⑥	prog.run (Program indicator)	Illuminates when program is being executed.
⑦	remote (Remote mode indicator)	Illuminates when the instrument is controlled by system controller.
⑧	G.E. (Gradient mode indicator)	Illuminates when the instrument is running in gradient mode.
⑨	Status Indicator	Green : when power is ON. Red : when an error is generated. Orange : during sleep mode

## 2. Parts Identification and Function

### 2.5.2 Keypad

The 24 keys on the keypad are used to operate the instrument and set parameters.

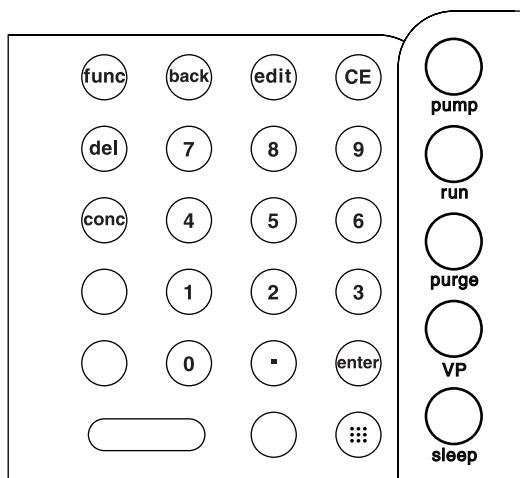

Key	Indicator	Function
	Display key	To show the operation keys.
	Pump key	To start and stop the pump.
	Run key	To start and stop the time program. (If time program is not registered, this key is inoperative.)
	Purge key	To start and stop purging. Purging stops automatically 3 minutes after it begins. Purging can be stopped also by pressing the . The duration of purging can be changed using [P-TIMER] of auxiliary function.
	VP key	To move from the initial screen to VP mode.
	Sleep key	To turn off the display screen. This key has no effect on operation.
	Delete key	To delete individual lines of time program on the display screen.
	Edit key	To activate edit mode of time program (from the initial screen).
	Clear key	<ul style="list-style-type: none"> <li>To initialize the screen.</li> <li>To clear the values input up to that time when entering the values.</li> <li>To clear error messages and cancel alarms.</li> </ul>
	Back key	<ul style="list-style-type: none"> <li>To scroll backward during time program editing.</li> <li>To scroll backward through auxiliary functions setting screens.</li> </ul>
	Concentration key	To set liquid concentrations in gradient analysis.
	Function key	<ul style="list-style-type: none"> <li>To scroll forward through basic functions.</li> <li>To scroll forward through auxiliary functions.</li> <li>To scroll during time program editing.</li> </ul>
	Enter key	To validate input values for each item setting.
	Numeric keypad	To enter numeric values for each item setting.

# 3

---

## Preparation

### Contents

3.1	Turning Power ON/OFF .....	3-2
3.2	Preparation before Operation.....	3-3
3.3	Checking Pressure Value.....	3-5

## 3.1 Turning Power ON/OFF

- 1** Press the power switch to turn the power ON.  
Press it again to turn the power OFF.



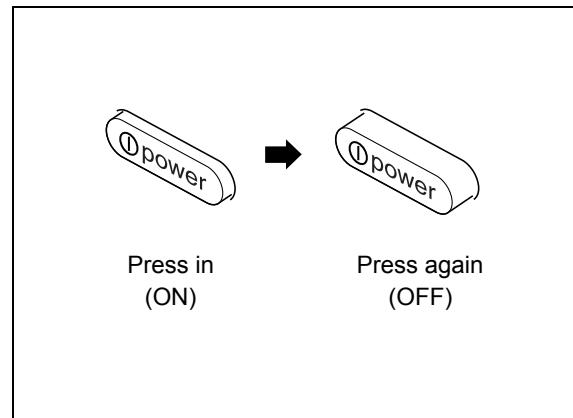


Fig. 3.1

- 2** When the power is first turned on, all the dots in the display matrix and all the indicators illuminate, as shown on the right.

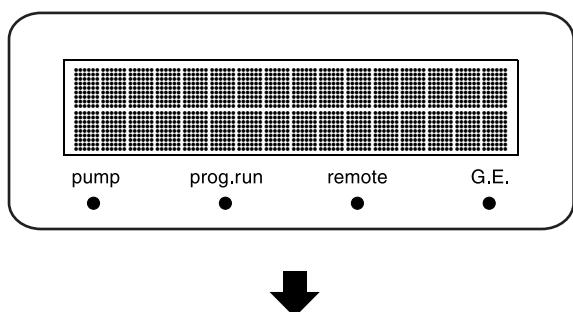

- 3** The memory is automatically tested, and after the memory check passes, the version number of the control program is displayed momentarily. The screen shown on the right appears and displays the ROM version [V\*.\*\*] in this example.

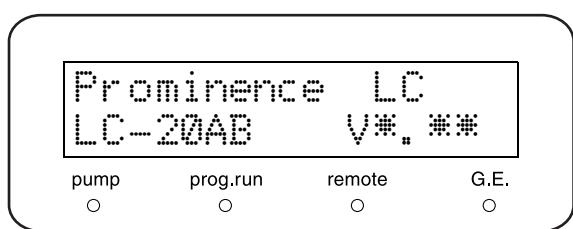


- 4** After displaying the ROM version, the initial screen appears as shown on the right. The status indicators turns green and the instrument is now operable.

### NOTE

- The values displayed on the initial screen are the values last set.
- If an error is detected, an alarm sounds and an error message appears.

"6.2 Error Message" P. 6-5

Initial Screen  
Flow rate [flow]

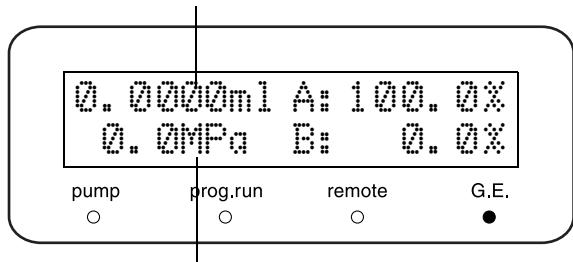

Pressure display [pressure]

# 3.2 Preparation before Operation

The pumps and internal plumbing of the pump are purged with nitrogen and dried prior to shipment. Prior to initial use (after installation) the pump must first be run for a short time using 2-propanol, in order to expel the air inside its flow lines. Then the instrument will be ready to receive the mobile phase to be used for analysis. The procedure is as follows.

- Pour approximately 100mL of 2-propanol into a beaker.

- Place two suction filters into the beaker.

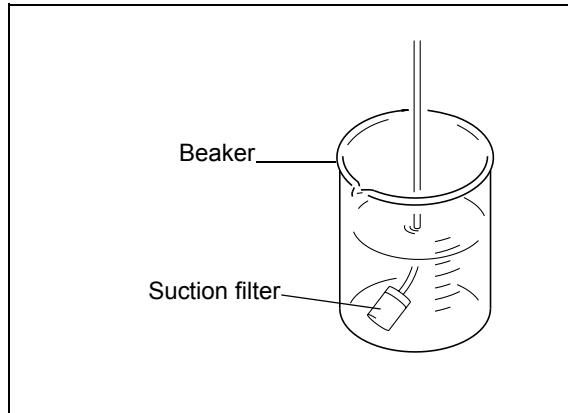


Fig. 3.2

- Connect one end of the SUS tubing (O.D. 1.6 x I.D. 0.3mm) provided to the pump outlet, and put the other end into the beaker.

- Connect one end of the drain tubing to the drain tubing connection port, and put the other end into the waste container.

- Turn the power ON.

The initial screen appears.

"3.1 Turning Power ON/OFF" P. 3-2

- Turn the drain valve knob 180° counterclockwise to open the drain valve.

- Press **func** twice and set the concentration of mobile phase B to 50%.

- Press **purge**.

The pumps run, and the pump indicator illuminates.

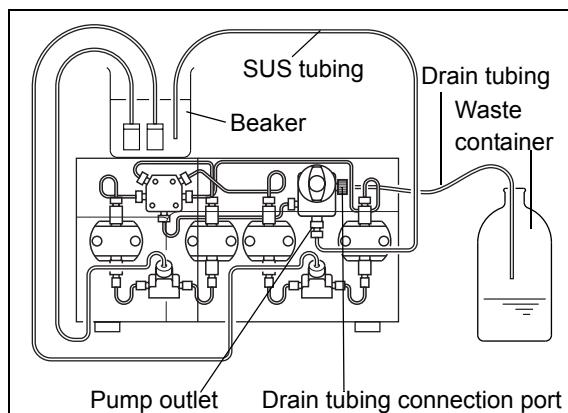


Fig. 3.3

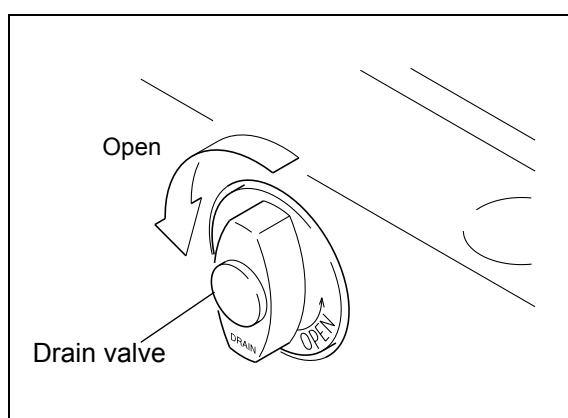


Fig. 3.4

### 3. Preparation

---

#### NOTE

If the drain valve knob is turned more than 180°, any mobile phase that drains out may contain air bubbles. This is normal.

- 9** When purging is over, press **func** once, to change the flow rate.

Set the flow rate to 5mL/min.


- 10** Turn the drain valve knob clockwise as far as possible, to close the drain valve.

- 11** Press **pump**.

The pumps run, and the pump indicator illuminates.

- 12** After about 15 minutes, press **pump** again.

The pump stops, and the pump indicator goes out. Preparation for operation is now completed.

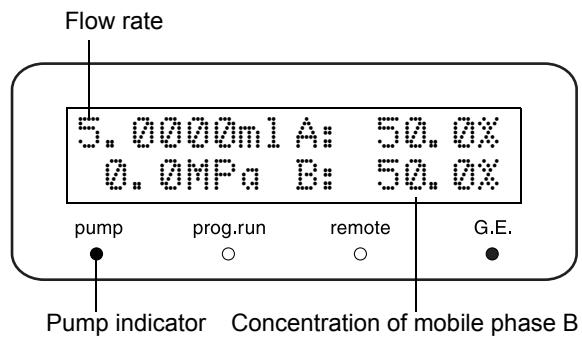

# 3.3 Checking Pressure Value

Before beginning operation, check the values of pressure.

- 1 Pour mobile phase in the reservoir, and put the suction filter inside the reservoir.  
The end of the drain tubing should be in the waste container, which is placed on the floor.

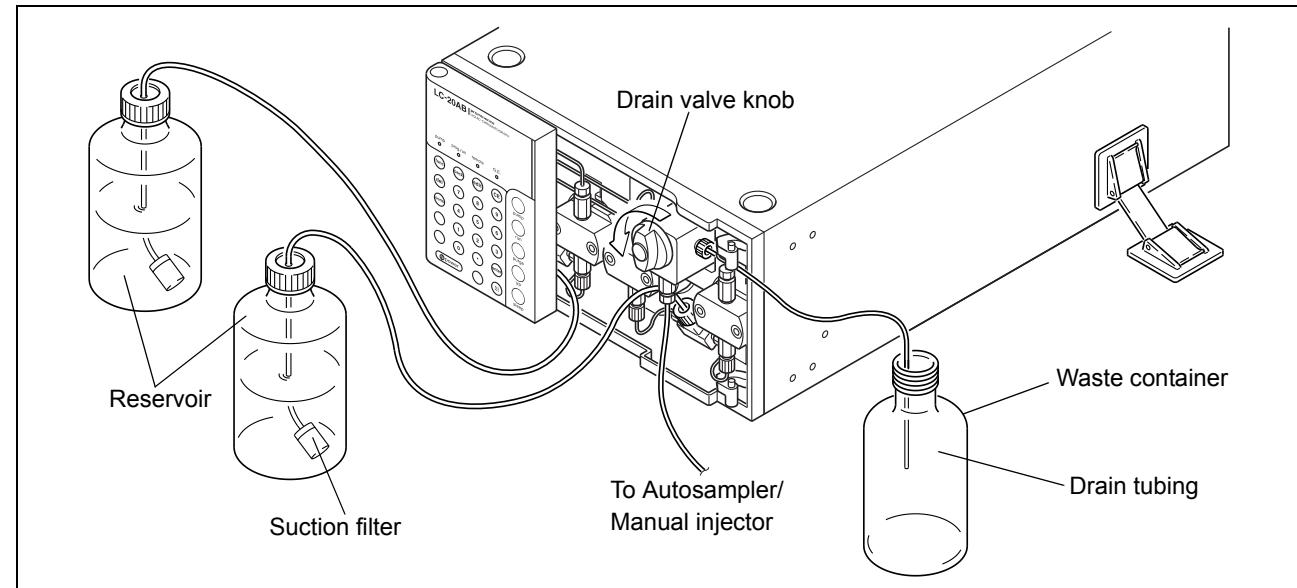


Fig. 3.5

- 2 To open the drain valve, turn the drain valve knob 180° counterclockwise.

**NOTE**

If the drain valve knob is turned more than 180°, any mobile phase that drains out may contain air bubbles. This is normal.

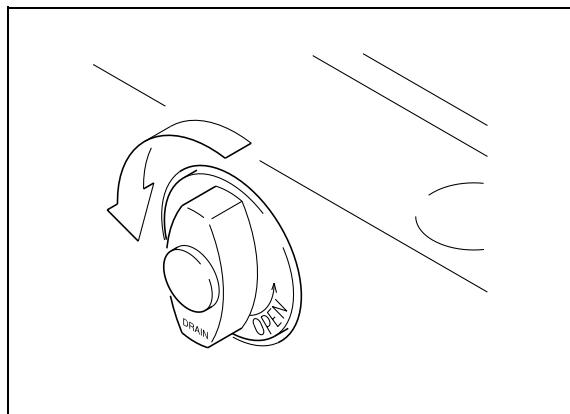


Fig. 3.6

### 3. Preparation

3 Press **CE** to return the initial screen.

4 Check that the [pressure] value shown on the screen is in the range of -0.3 to 0.3MPa.

**NOTE**

If not, zero the value of the pressure sensor with [ZERO ADJ] function.

☞ "Zero Adjustment of Pressure Sensor [ZERO ADJ]"  
P. 5-20

5 Press **func** twice and set the concentration of mobile phase B.

6 Press **purge**.

Pumping begins at a registered flow rate.

☞ "Setting Purge Flow Rate [P-FLOW]" P. 5-18

**NOTE**



Normally, pumping begins at the set flow rate as soon as **purge** is pressed. But in the following situations, pumping is initially carried out at low speed (for a few seconds) in order to detect the pump home position, before rising at the set flow rate:

- **purge** is pressed for the first time after the power is turned on.
- **purge** is pressed for the first time after a pressure upper limit of 22MPa or more has been activated.

7 Observe the condition of the mobile phase that flows from the end of the drain tubing for about 10 seconds.

The mobile phase should flow continuously and be free of air bubbles.

Initial Screen

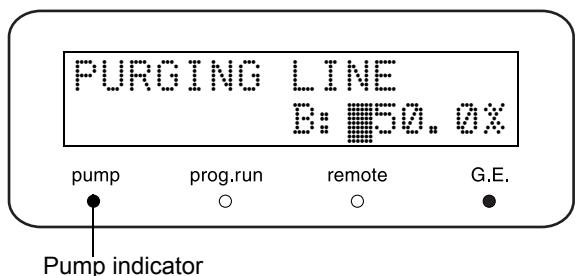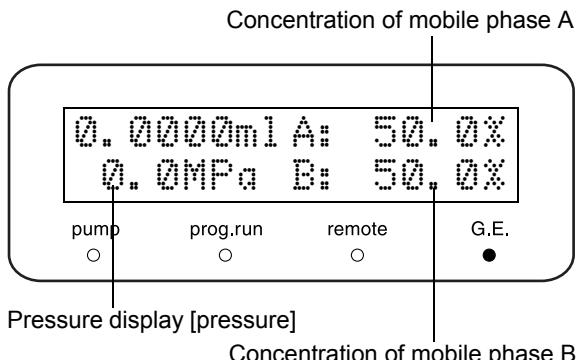

**8** Press **purge**.

The pump stops, and the pump indicator goes out.

**NOTE**

- If the flow of mobile phase starts and stops repeatedly in synchronization with pumping:  
There are probably air bubbles in the pump heads;  
press **purge** to expel air.
- If no mobile phase emerges:  
Attach the syringe needle to the disposable syringe (provided), insert the tip of the needle into the end of the drain tubing, and draw the mobile phase through the tubing.

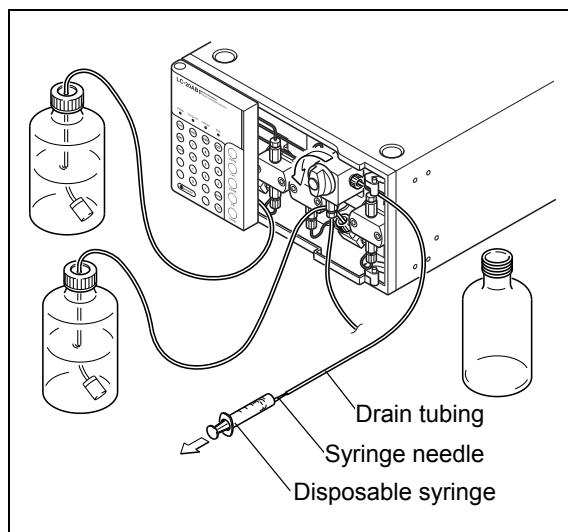


Fig. 3.7

### 3. Preparation

---

This page is intentionally left blank.

# 4

---

## Basic Operation

### Contents

4.1	Setting Parameters .....	4-2
4.2	Operation .....	4-5
4.3	Plunger Rinsing When Buffer Solution is Used as Mobile Phase .....	4-6
4.4	Replacing the Mobile Phase .....	4-10


# 4.1 Setting Parameters

Before operating this instrument, it is necessary to set the flow rate and the concentration of mobile phase B. The ranges, steps, initial values and their applicable modes of parameters are listed in the following table.

Parameter	Range	Steps	Initial Value
flow	0 ~ 10.0000 mL/min	0.0001 mL/min	0 mL/min
bconc	0.0 ~ 100.0%	0.1%	0.0%

## 4.1.1 Prior to Key Operation


Press  to show the operation key.

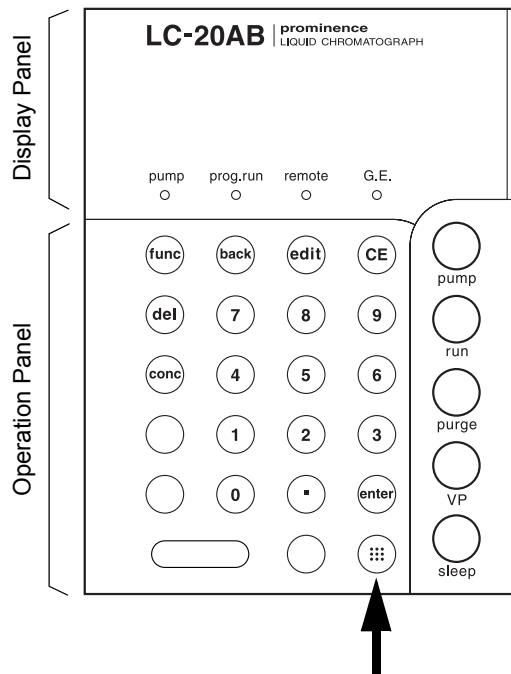



### 4.1.2 Setting Flow Rate

The following is the basic procedure for setting a flow rate.

- 1** Display the initial screen, either by turning the power on or by pressing **CE** several times.
- 2** Press **func**.  
The cursor blinks in the display field, prompting input of a new value.
- 3** Enter the new value using the numeric keypad, and press **enter**. The new value is set, and the screen returns to the initial screen.  
\* To cancel the new setting, press **CE**.

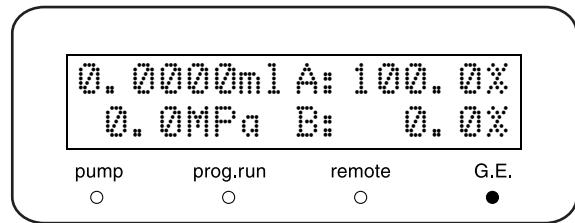

- 4** To change other parameters, press **func**.  
Pressing **func** accesses the items in the following sequence:  
[flow] → [bconc].  
When an item is accessed, the cursor blinks in the display field, prompting value input. Press **func** further to access the other auxiliary functions.
- 5** After setting a flow rate, press **CE** to return to the initial screen.

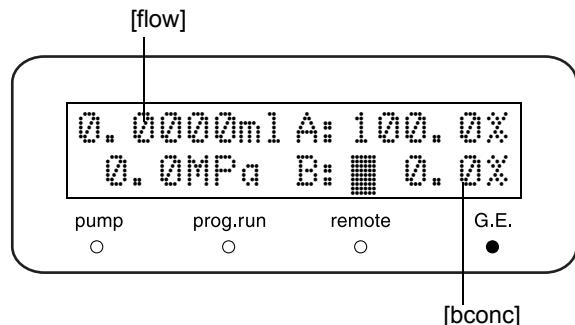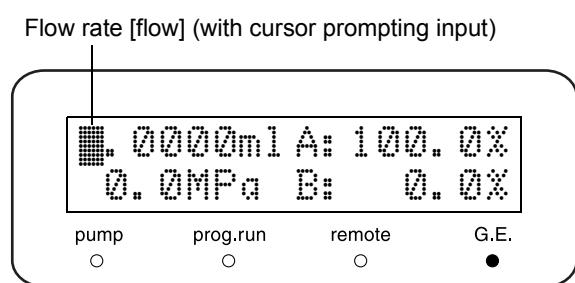


### 4.1.3 Setting the Concentration of Mobile Phase B

Use the following procedure to set the concentration of mobile phase B.

Here, [bconc] (the concentration of mobile phase B) is set to 20%.


- 1** On the initial screen, press **func** twice.  
The cursor blinks in the display field, prompting input of a new value.

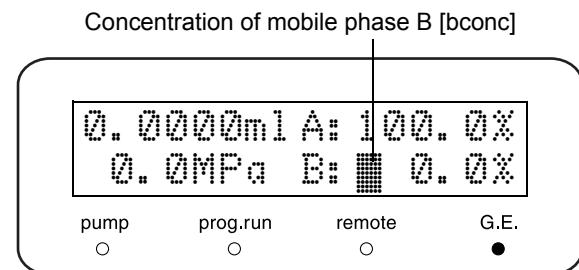

- 2** Press **2**, **0** and **enter**.  
The new value appears (as shown on the right) on the initial screen.

\* To cancel the new setting, press **CE**.


In the initial screen, the concentration of mobile phase A is automatically calculated and displayed.

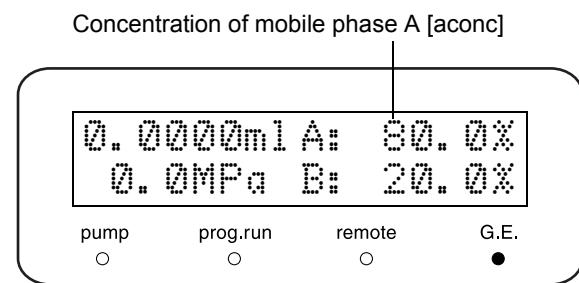


Concentration of mobile phase A [A:] (%) = 100 (%) - Concentration of mobile phase B [B:] (%)

## 4.2 Operation

- 1** Turn the drain valve knob clockwise as far as possible to close the drain valve.
- 2** Press **CE** to return to the initial screen.
- 3** Press **func** once, then, set the desired flow rate.  
Example: To set 1mL/min, press **1** and **enter**.
- 4** Press **func** twice and set the desired concentration of mobile phase B.  
Example: To set 20%, press **2**, **0**, and **enter**.

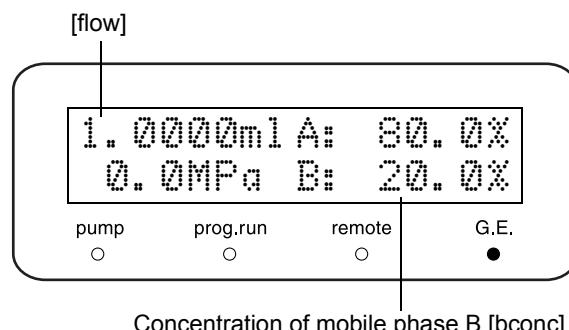

- 5** Press **pump**.  
The pumping starts, and the pump indicator illuminates.
- 6** Observe the pressure value on the screen to ensure that the pump outlet pressure is rising.
- 7** To stop operation, press **pump** again.  
The pumping stops, and the pump indicator goes out.

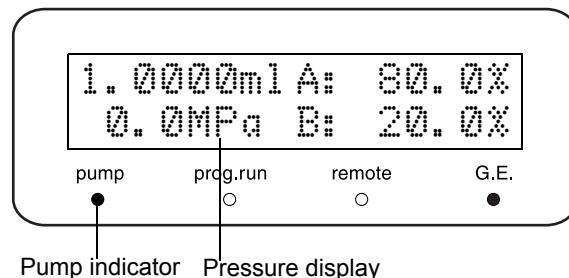

### ⚠ CAUTION

Close the drain valve if necessary. When it is left opened, mobile phase could flow out of the drain due to atmospheric pressure.

## 4.3 Plunger Rinsing When Buffer Solution is Used as Mobile Phase

When a buffer solution is used as the mobile phase, use distilled water to rinse the inner surfaces of the seals and the plunger surfaces.

### CAUTION

The seals and plungers must be rinsed frequently when a buffer solution is used as the mobile phase. Buffer solutions crystallize upon evaporation, and crystals could damage the plungers and plunger seals, which may cause the shortening of their service life.

---

### 4.3.1 Operation Method for Automatic Rinsing Kit

---

#### ■ Preparation

- 1** Mount the automatic rinsing kit to the instrument using the method described in "[9.1.10 Installation of Automatic Rinsing Kit \(Optional\)](#)" P. 9-34.
- 2** Pull the PTFE tubing connected to the automatic rinsing kit's outlet out of the conical flask.
- 3** Draw distilled water into the disposable syringe, and fill the rinse flow line with liquid.  
\* Attach a syringe needle to the tip of the disposable syringe before use.
- 4** Return the PTFE tubing connected to the automatic rinsing kit's outlet to the original state.

The arrows indicate the flow of the rinse solution.

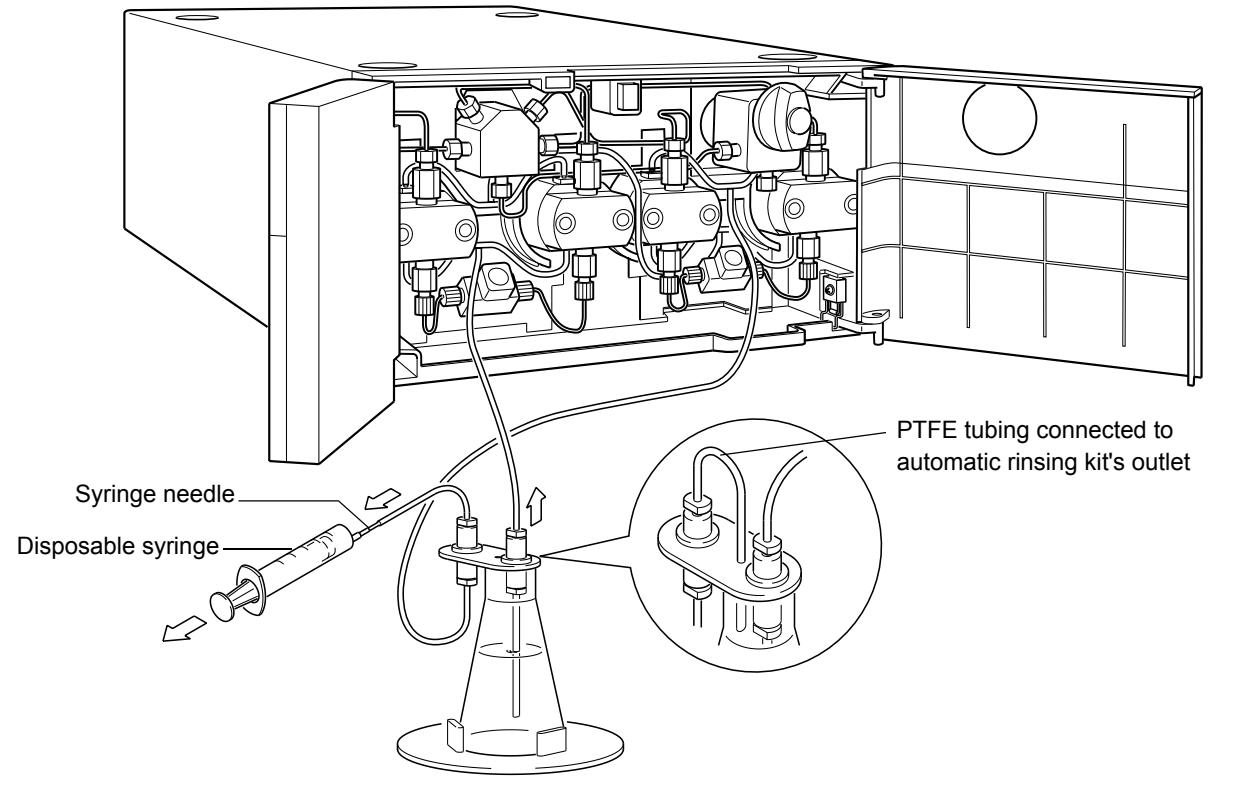


Fig. 4.1

#### ■ Operation

- 1** Set the flow rate to 3mL/min and set the concentration of mobile phase B to 50%.
- 2** Press **pump**. Pumping starts, and the pump indicator illuminates.
- 3** Check whether liquid is coming out of the tip of the PTFE tubing connected to the automatic rinsing kit's outlet.
- 4** If liquid is coming out, press **pump**. The pump indicator goes out and the pump stops.

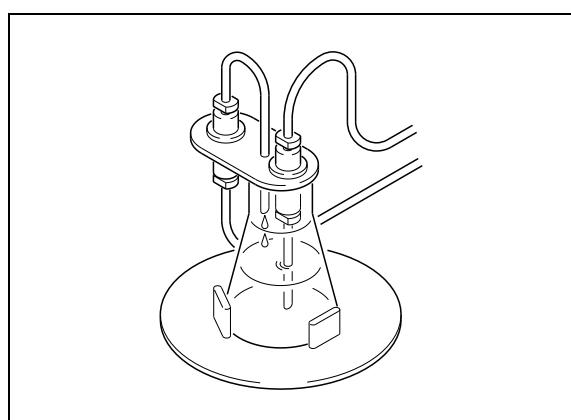
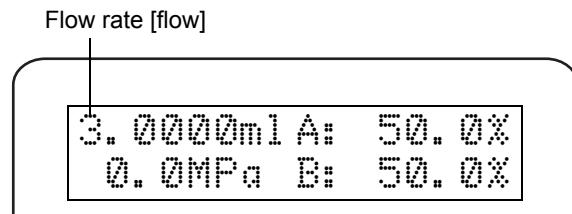


Fig. 4.2

### ⚠ CAUTION

- As a rough guide, replace the rinse solution with distilled water once a day.
- If the volume of rinse solution increases during pumping, it is because of leakage from a plunger seal. Remove the rinsing kit, identify whether the leakage is from the left or right plunger seal, and replace the seal that is leaking in accordance with the procedure "[8.2 Replacement of Plunger Seal](#)" P. 8-5.
- If the volume of rinse solution decreases during pumping, it is because of leakage from a diaphragm. Confirm the leakage from the bottom of the head holder, and replace the diaphragm in accordance with the procedure "[8.3 Cleaning and Inspection \(Replacement\) of Plungers and Diaphragms](#)" P. 8-10.

### 4.3.2 Operation Method for Manual Rinsing


It is possible to manually rinse seals and plungers, without using the optional automatic rinsing kit. The following are examples of manual rinsing cycles.

- Phosphoric acid buffer solution (low concentration): Several times a day
- Boric acid buffer solution (low concentration): Frequently during the day
- Use an automatic rinsing kit for ammonium sulfate (high concentration).

#### ■ Connection

The following explanation applies to pump A. Connect the plumbing for pump B in the same way before performing rinsing.

- Cut the rinse tubing ASSY and the transparent tubing (both provided as accessories) to appropriate lengths. (Cut the rinse tubing into pieces ①, ②, and ③, as shown in the diagram on the right.)
- Insert rinse tubing S (pieces ① and ③; provided as accessory) into the left and right rinse-solution outlets.

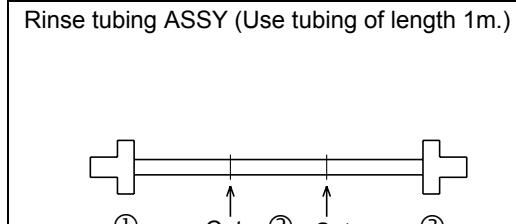

- Connect rinse tubing S on the left and right using piece ② of the rinse tubing and the transparent tubing.
- Connect piece ① of the rinse tubing cut off in step 1 to the left rinse-tubing inlet and connect the disposable syringe (accessory).  
\* Attach a syringe needle to the tip of the disposable syringe before use.

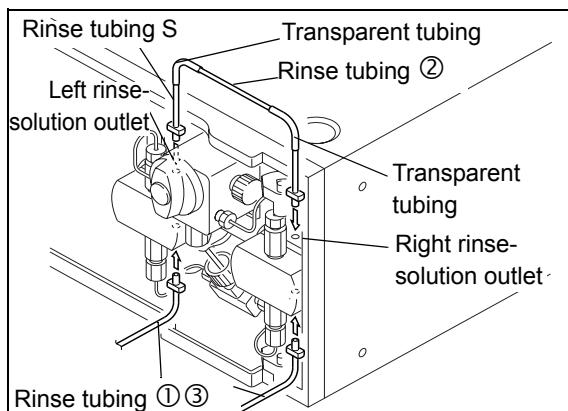


Fig. 4.4

- 5** Connect piece ③ of the rinse tubing to the right rinse-tubing inlet and insert the end of the tubing into a beaker.

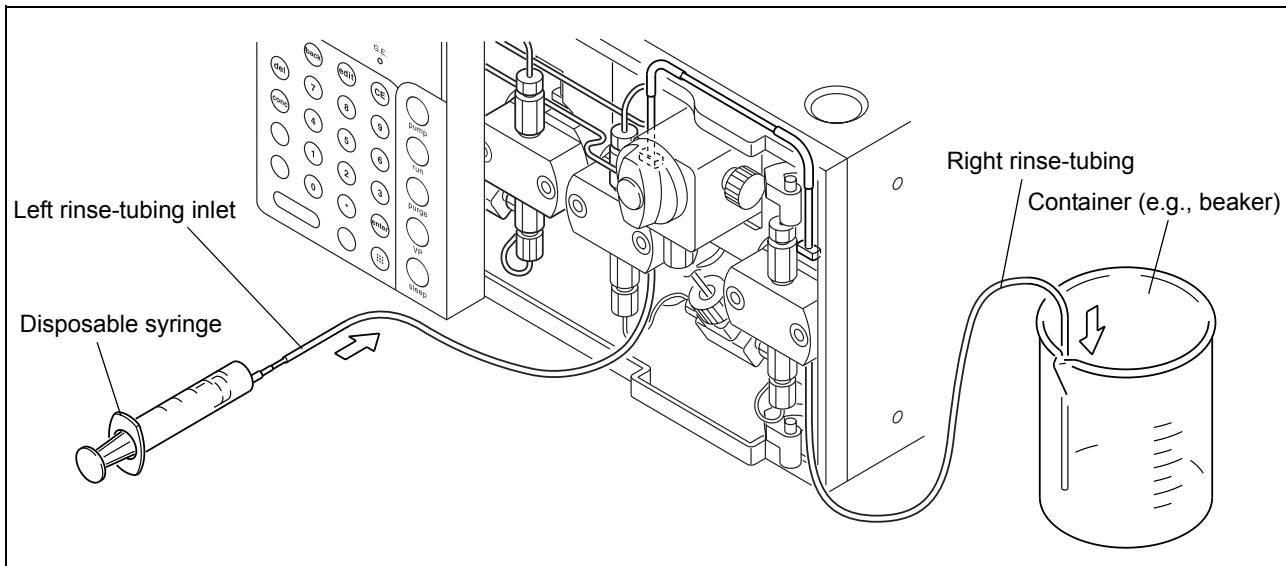


Fig. 4.5

### ■ Operation

- 1** Remove the disposable syringe from the PTFE tubing.
- 2** Draw rinse solution into the disposable syringe and reconnect it to the PTFE tubing.
- 3** Inject rinse solution into the rinse flow line using the disposable syringe.  
\* Manual rinsing is possible whether the pumps are running or not.

## 4.4 Replacing the Mobile Phase

The procedure for replacing the mobile phase varies depending on whether the new mobile phase is miscible with the old one, or whether a buffer solution is used for the mobile phase. Replace properly according to the appropriate procedure below. When the column is to be replaced also, remove the column first.

### 4.4.1 When New Mobile Phase is Miscible with the Old Mobile Phase

- 1** Pour about 100mL of the new mobile phase into a 200mL beaker.
- 2** Remove the suction filter from the reservoir and put the filter into the beaker filled with the new mobile phase by step 1 above.
- 3** Shake the filter slightly to mix the mobile phases.
- 4** Put new mobile phase into the reservoir. Then remove the suction filter from the beaker and put it into the reservoir.
- 5** Turn the drain valve knob 180° counterclockwise to open the drain valve.

**NOTE**

If the drain valve knob is turned more than 180°, any mobile phase that drains out may contain air bubbles. This is normal.

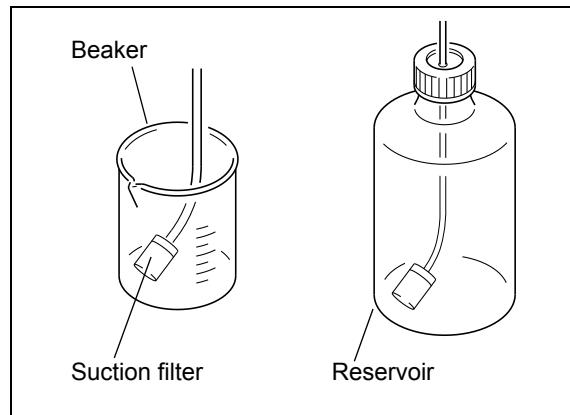


Fig. 4.6


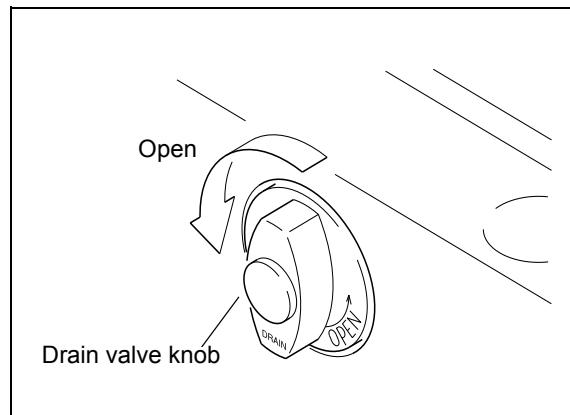


Fig. 4.7

- 6** Set [bconc] (the concentration of mobile phase B) so that the concentration on the side for replacement of the mobile phase is 100%.
  - When replacing mobile phase A, set [bconc] to 0.0%.
  - When replacing mobile phase B, set [bconc] to 100.0%.

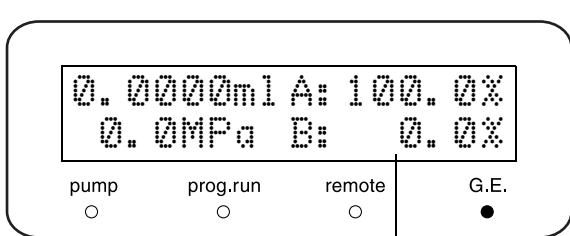

Concentration of mobile phase B [bconc]

**7** Press **purge**.

The old mobile phase will be completely expelled from the flow lines through the drain tubing.

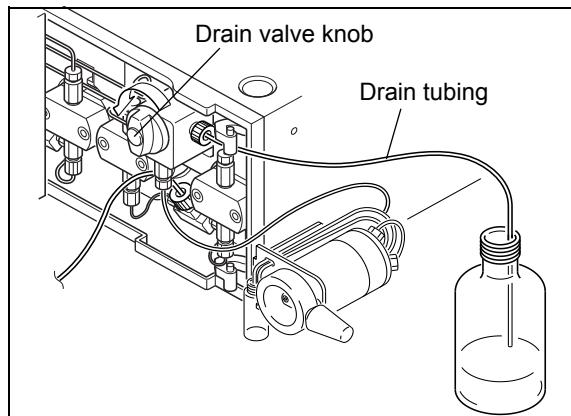


Fig. 4.8


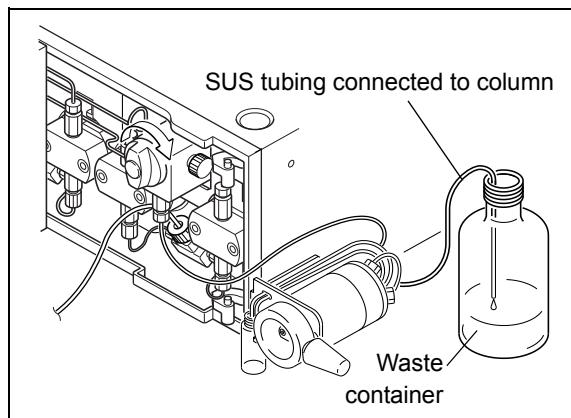
**8** Disconnect the tubing. Connecting the manual injector outlet to the column, and put the tubing into the reservoir.**9** Close the drain valve. Turn the drain valve knob clockwise as far as it will go.

Fig. 4.9

**10** Set the flow rate [flow] to about 1-3mL/min.**11** Press **pump**.

Pumping starts, and the pump indicator illuminates.

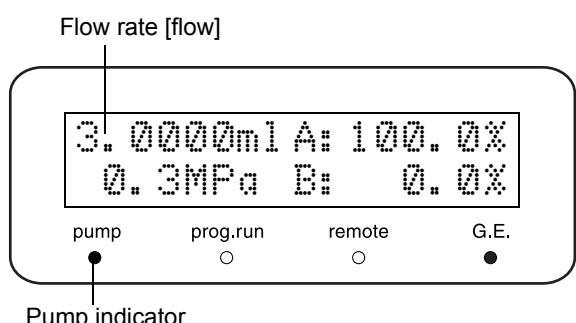

Pump indicator

**12** Press **pump**.

Pumping stops, and the pump indicator goes out.

**13** Reconnect the tubing that was disconnected in step 7 to the manual injector outlet.**14** Press **pump** again to restart pumping.

The mobile phase in the flow line downstream of the manual injector will be replaced.

- \* The flow rate should be set so that the pressure will be lower than the maximum column pressure.

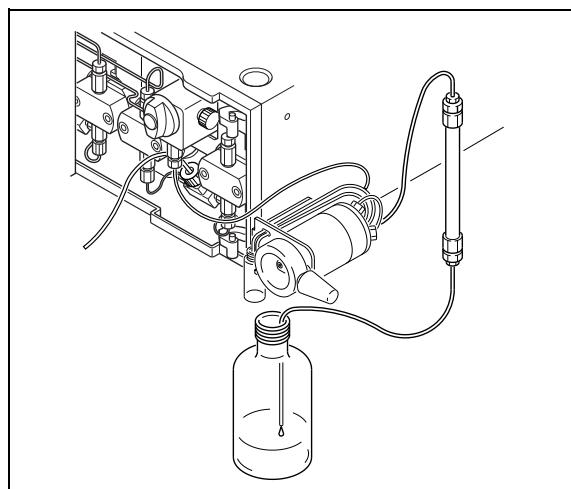


Fig. 4.10

## 4. Basic Operation

---

### 4.4.2 When New Mobile Phase is not Miscible with the Old Mobile Phase

---

- 1** Prepare an intermediate rinse solution (2-propanol or similar) that is miscible with both the old and new mobile phases.
- 2** Replace the old mobile phase with the intermediate rinse solution.  
 ["4.4.1 When New Mobile Phase is Miscible with the Old Mobile Phase" P. 4-10](#), steps 1-11
- 3** Replace the intermediate rinse solution with the new mobile phase.  
 ["4.4.1 When New Mobile Phase is Miscible with the Old Mobile Phase" P. 4-10](#), steps 1-11

### 4.4.3 When Buffer Solution is Used as Mobile Phase

---

If a buffer solution is used as the mobile phase, it deposits crystals in the flow line when it evaporates.

 **CAUTION**

Distilled or de-ionized water should be used for purging.  
Use of organic solvents such as 2-propanol may cause crystals.

- 1** Prepare distilled water or de-ionized water.
- 2** Pump at least 200mL of the water prepared in step 1 through the flow line.  
 ["4.4.1 When New Mobile Phase is Miscible with the Old Mobile Phase" P. 4-10](#), steps 1-11
- 3** Replace the water with the new mobile phase.  
 ["4.4.1 When New Mobile Phase is Miscible with the Old Mobile Phase" P. 4-10](#), steps 1-11

### 4.4.4 Rinse When Buffer Solution is Used

---

When a buffer solution is used as the mobile phase, it deposits crystals in the flow line when it evaporates. Crystals on the plungers or plunger seals could damage them and shorten their service life, so when a buffer solution is used it is important to rinse the seal inner surfaces and plunger surfaces frequently with distilled water in order to protect them and prolong their service life.

 ["4.3 Plunger Rinsing When Buffer Solution is Used as Mobile Phase" P. 4-6](#)

 **CAUTION**

When the instrument is to remain inactive following operation with a buffer solution, be sure to replace the buffer solution in the flow lines with distilled or de-ionized water to prevent deposition of buffer solution crystals.

# 5

---

## Application Operation

### Contents

5.1	Display Panel .....	5-2
5.2	Parameter in Auxiliary Functions .....	5-12
5.3	VP Functions.....	5-27
5.4	Creating Time Program.....	5-44
5.5	Control by CBM-20A or CBM-20Alite System Controller .....	5-54
5.6	Control by SCL-10Avp or SCL-10A System Controller .....	5-55
5.7	Connection to External Input/Output Terminals .....	5-56

# 5.1 Display Panel

## 5.1.1 Types of Screens

Turn the power ON, the initial screen appears.

By pushing the keys **func**, **VP** and **edit**, the screen can be switched from the initial screen to one of the three screens described below.

- Basic setting screens and auxiliary function screens
- VP function screen
- Time program edit screen

Initial screen

0.0000ml A: 100.0%
0.0MPa B: 0.0%

**func**

Basic setting screen and auxiliary function setting screens

P.5-3

■.0000ml A: 100.0%
0.0MPa B: 0.0%

Basic settings

- Flow rate
- Concentration of mobile phase B

Auxiliary settings

- Parameter
- File operation
- Control
- System
- Monitor

**VP**

VP function screen P.5-8

PRODUCT INFO
Press func or VP

VP function settings

- Mobile phase monitor
- Product information
- Maintenance information
- Validation support
- Calibration support

**edit**

Time program edit screen P.5-44

USED	LEFT
0	320

Time program editing


### 5.1.2 Basic Setting Screen and Auxiliary Function Setting Screen


In this section, basic setting screens and auxiliary function setting screens are shown in the following flow diagrams.


On each screen, press **func** to show the next screen, and press **back** to return.


On auxiliary function group screens, press **enter** to enter each group.


Press **CE** to return the initial screen.

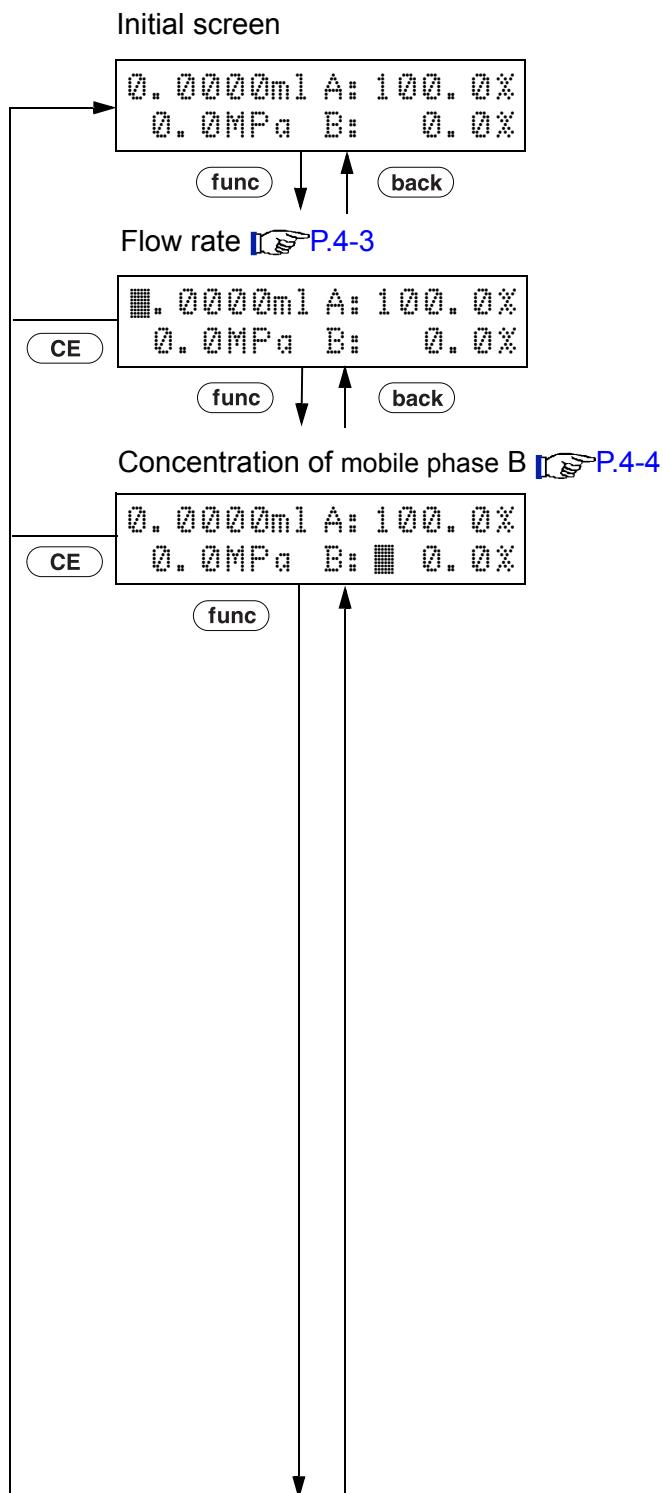

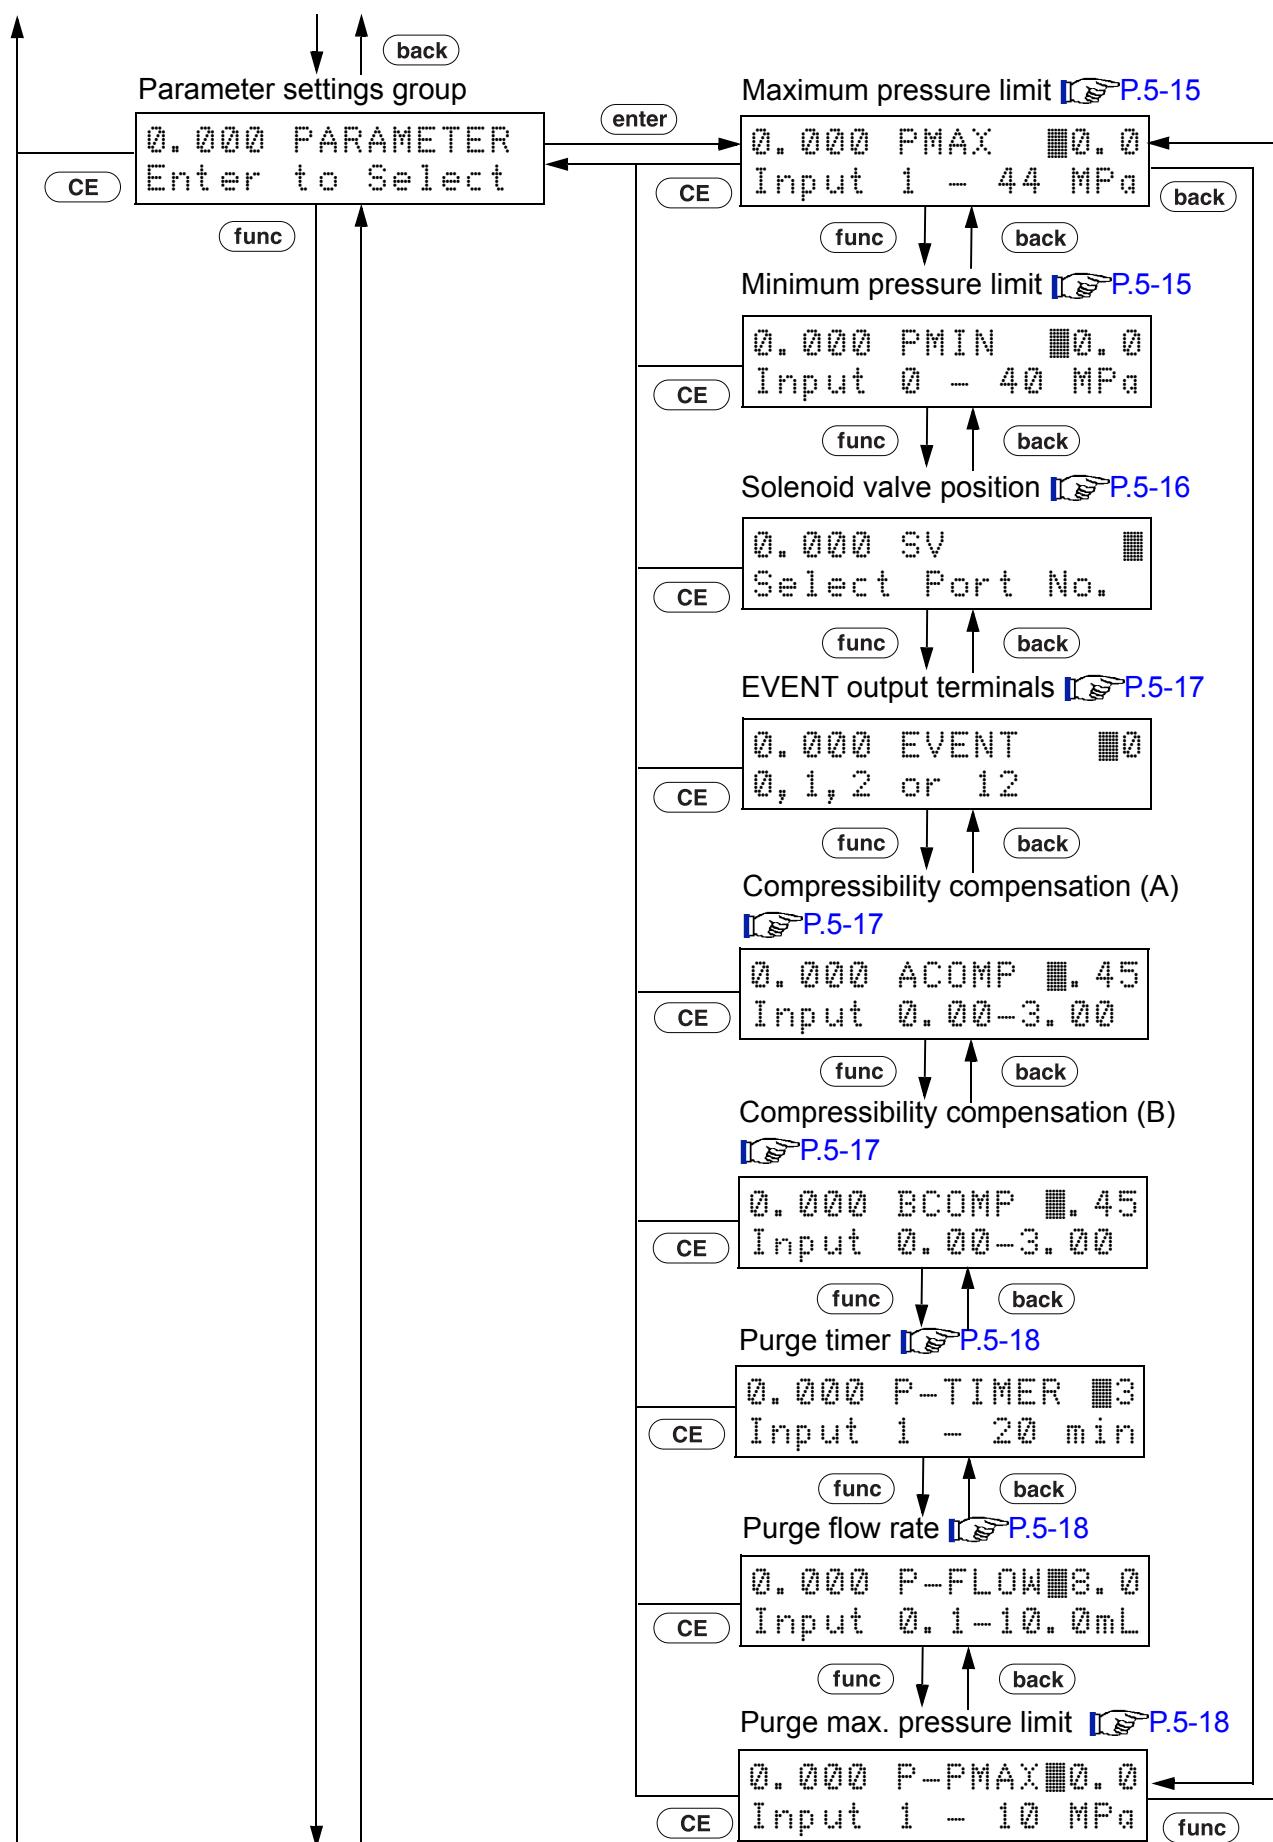

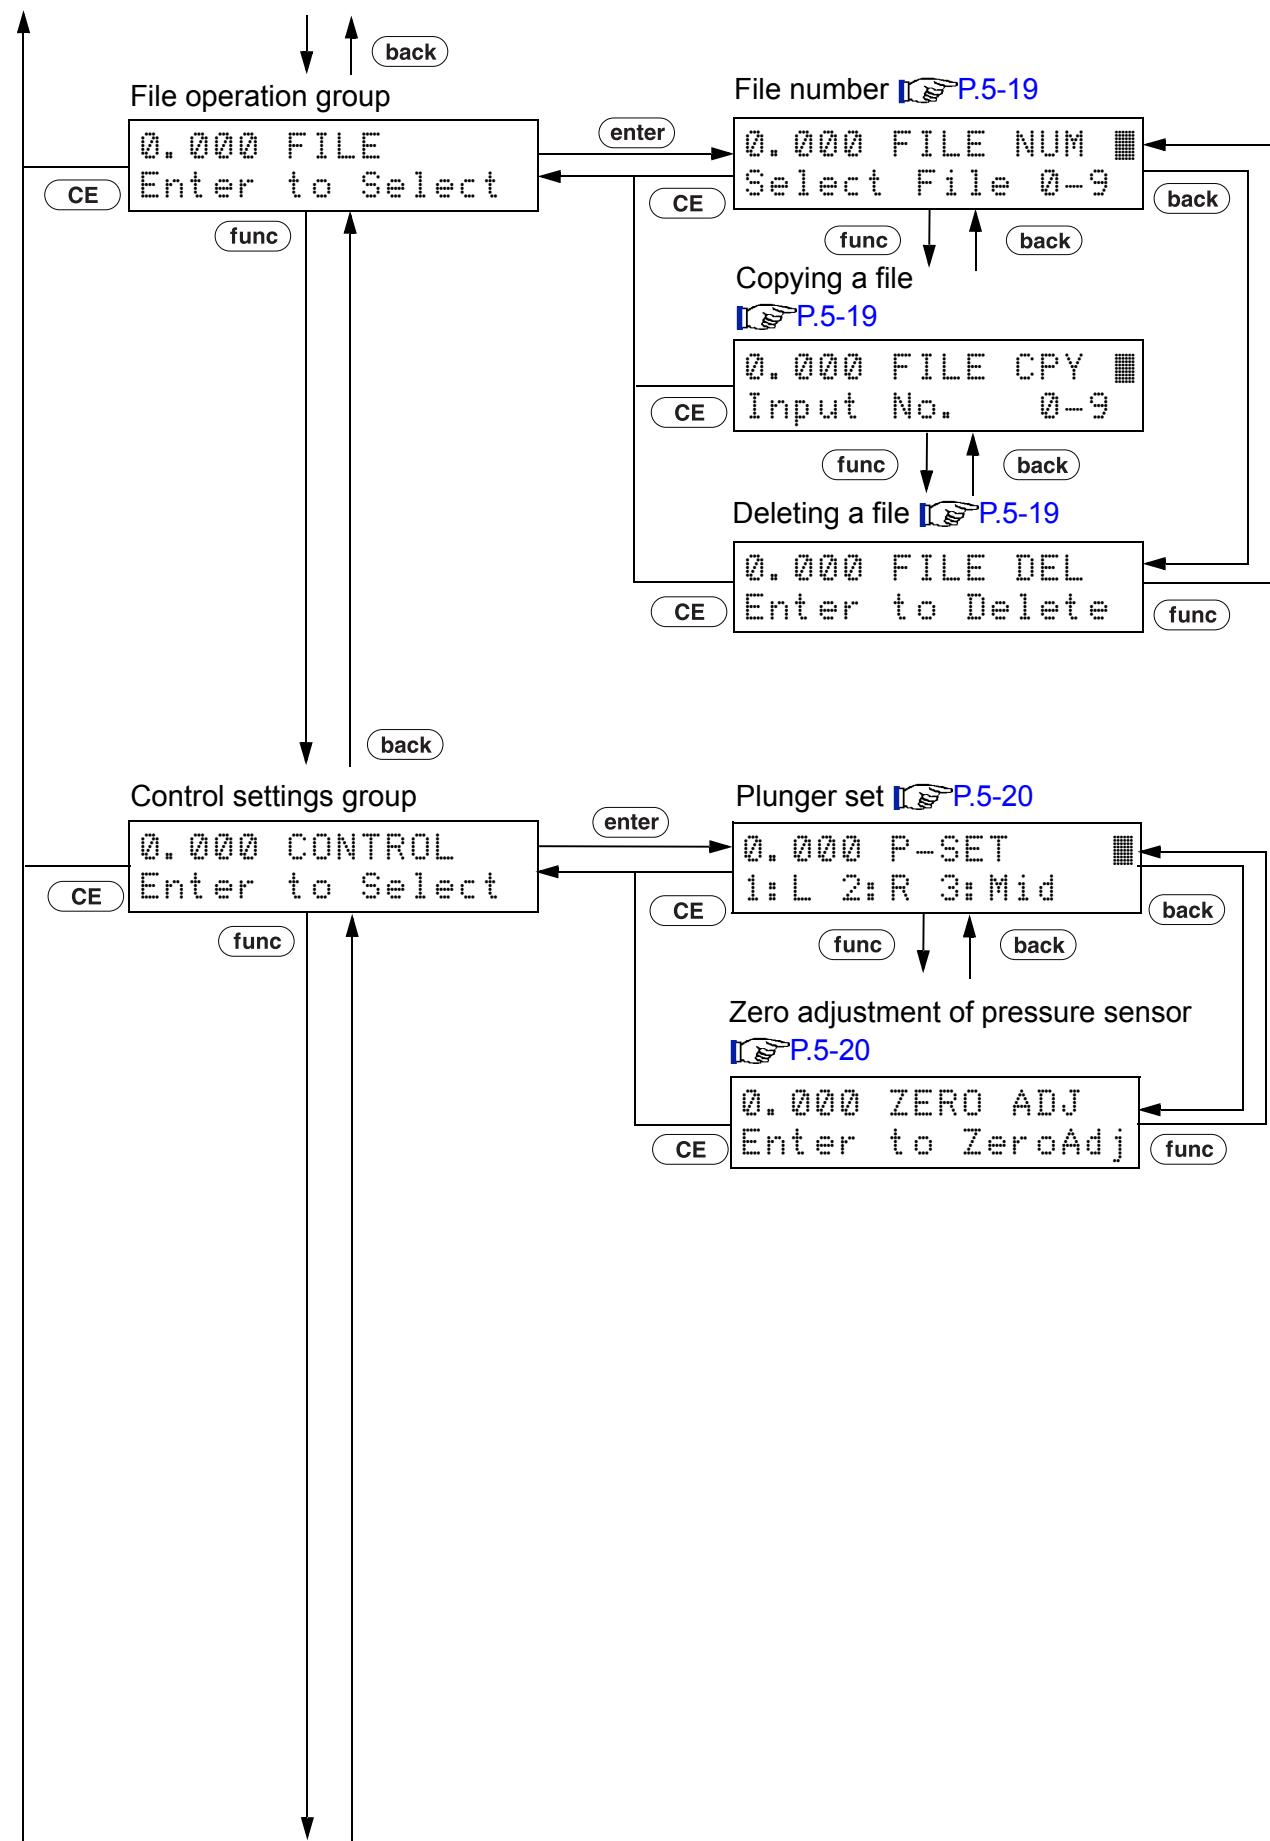

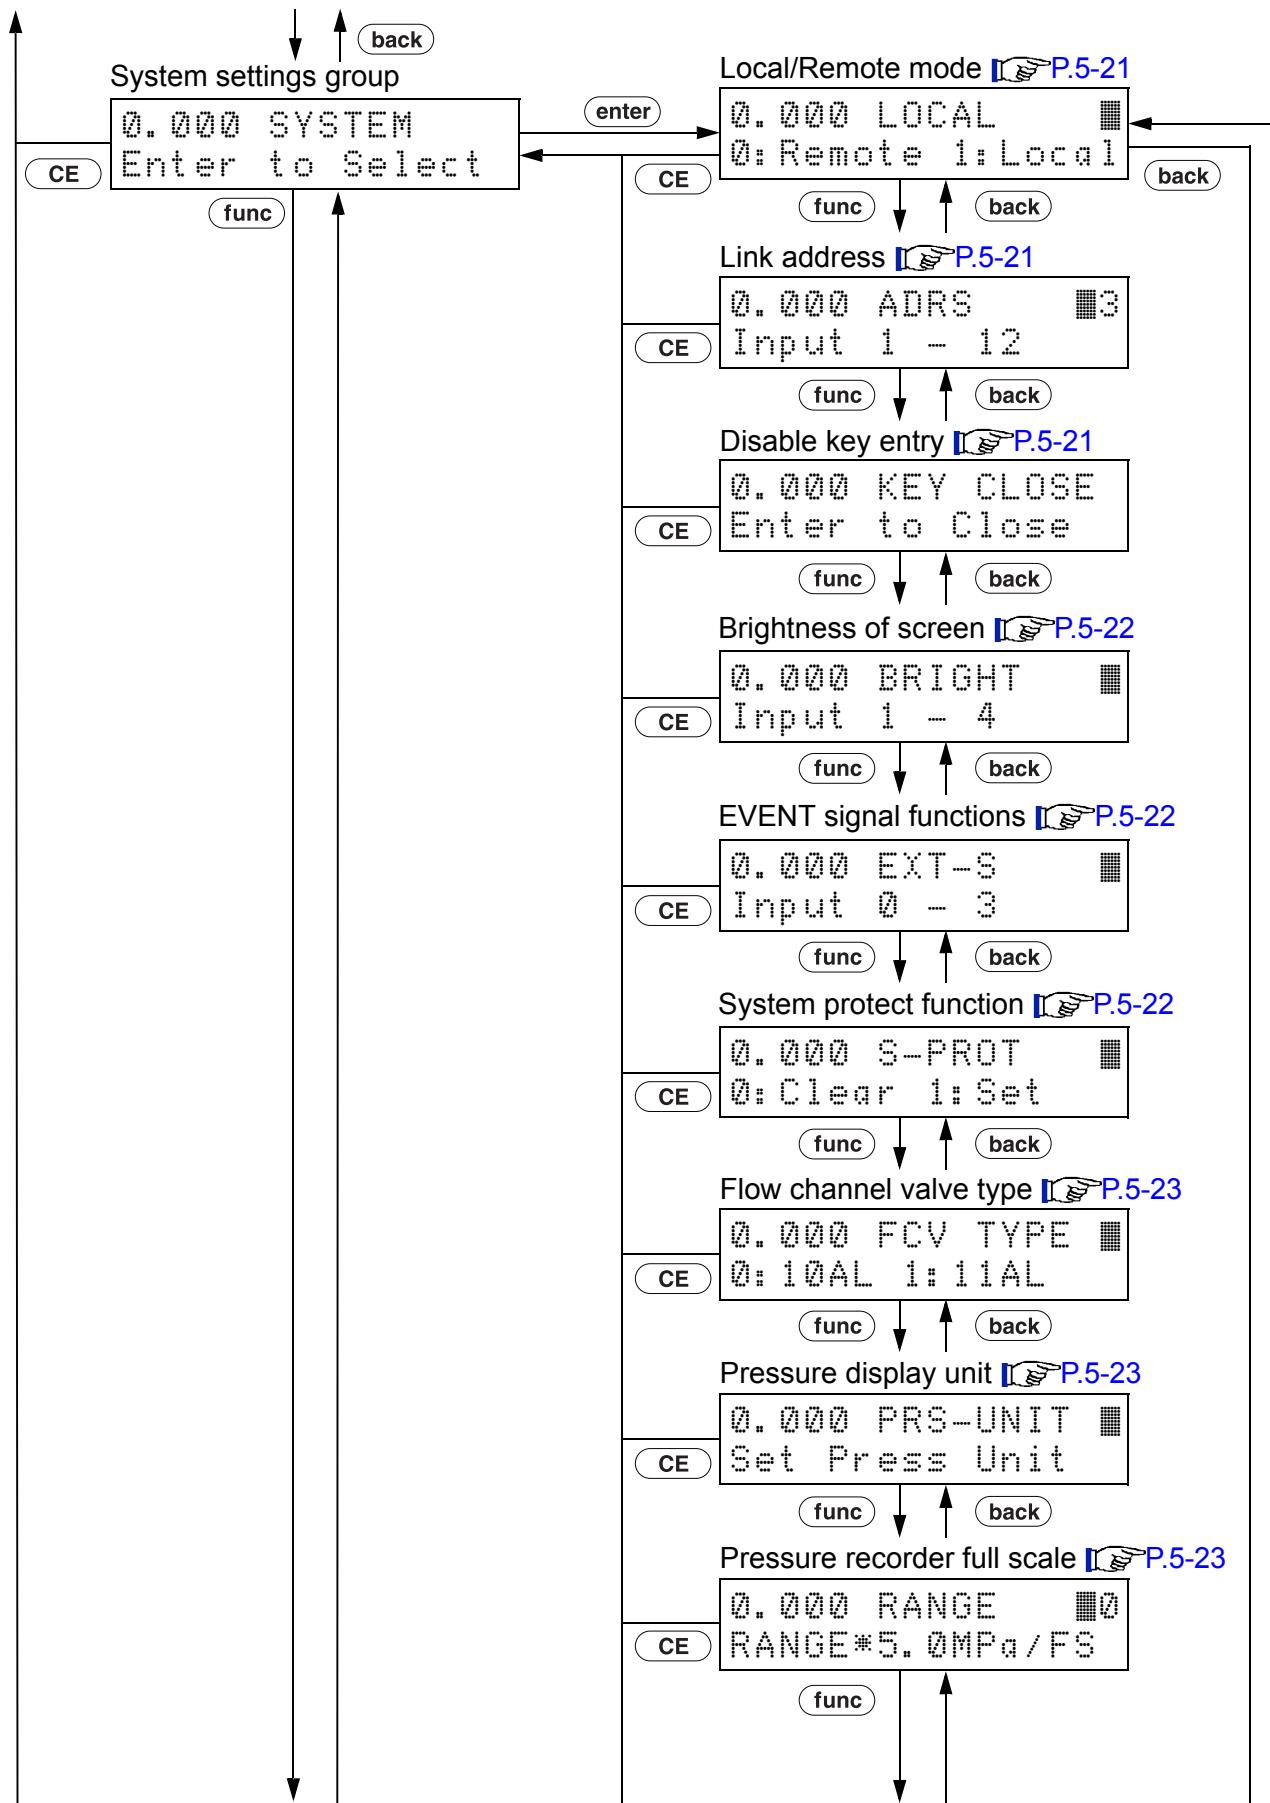

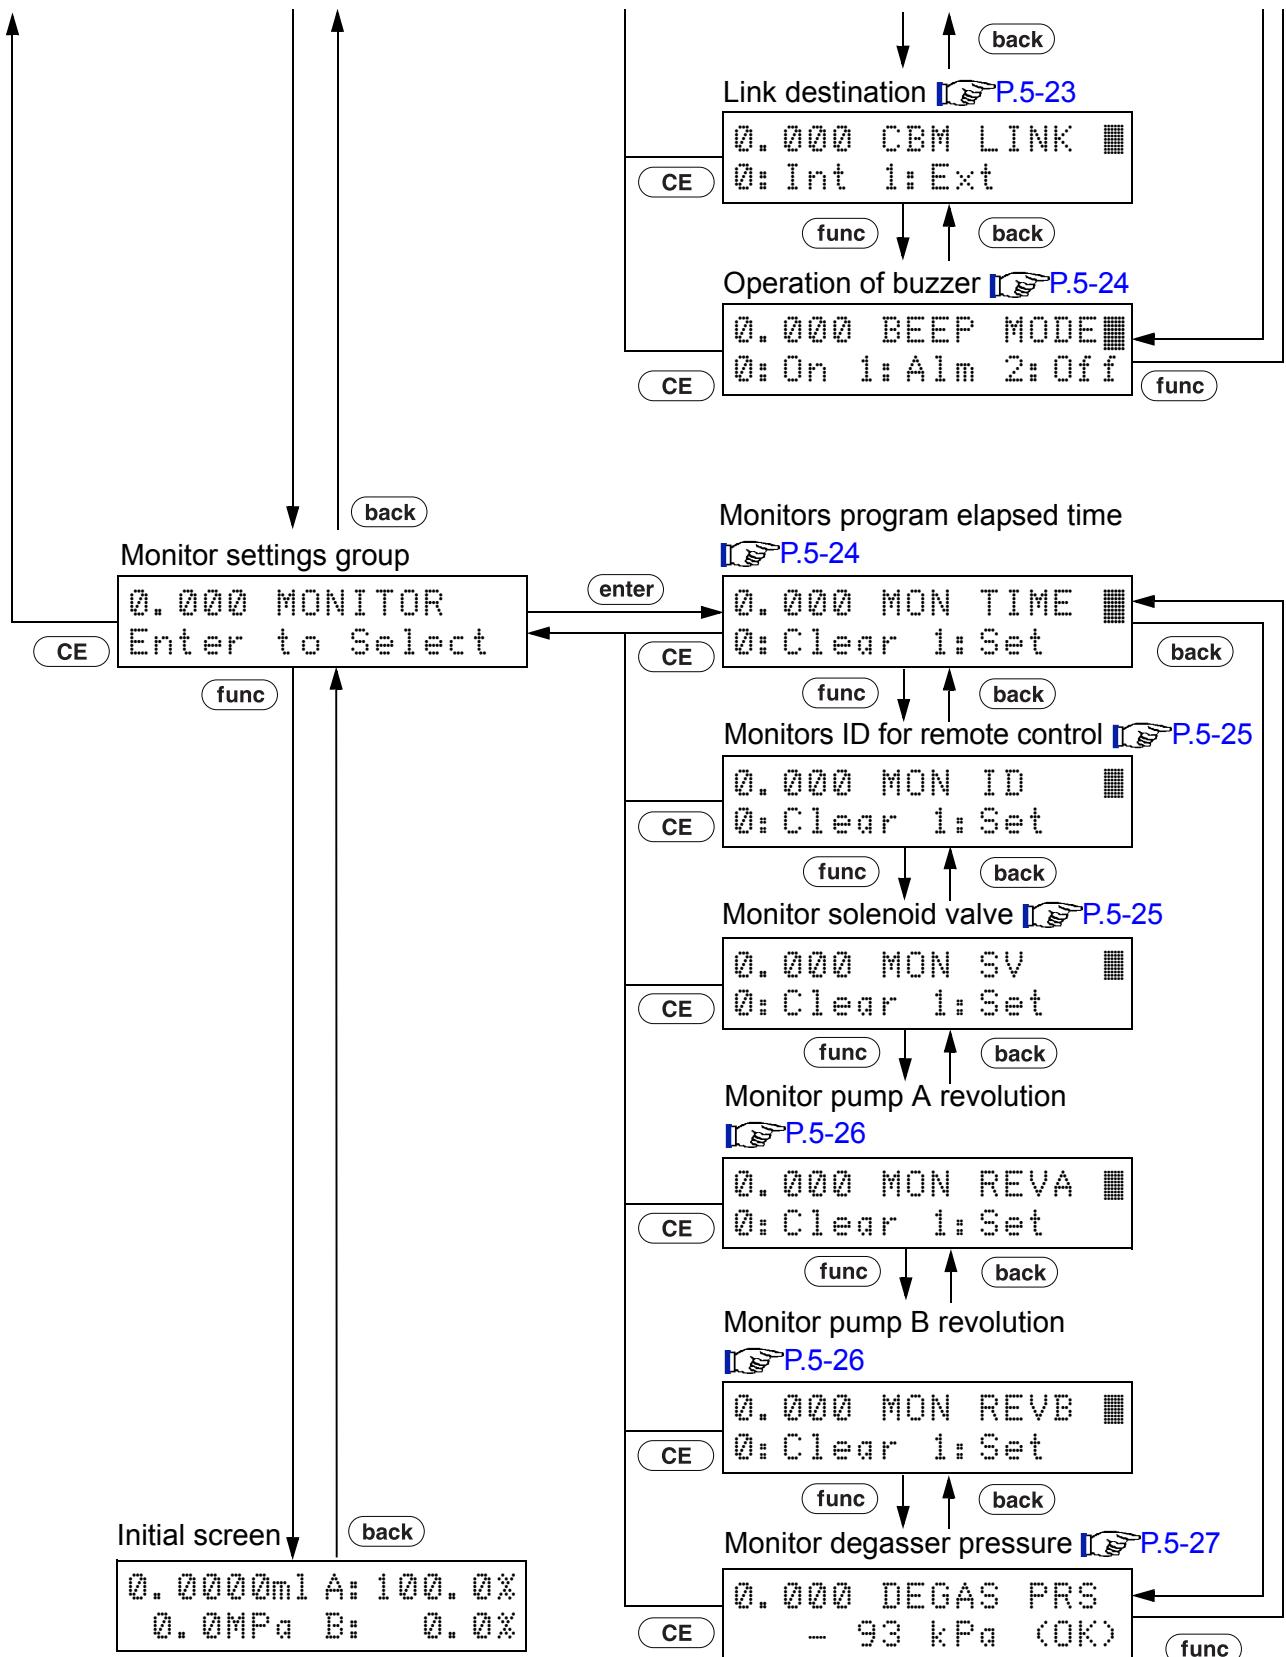

## 5. Application Operation

### 5.1.3 VP Function Screen


In this section VP function screens are shown in the following flow diagrams.


Press **VP** on initial screen to show each group screen.

Press **CE** to return to the initial screen.


Press **func** or **back** to switch the setting screen within the groups selected by **VP**.


Press **CE** to return to the initial screen in the group.

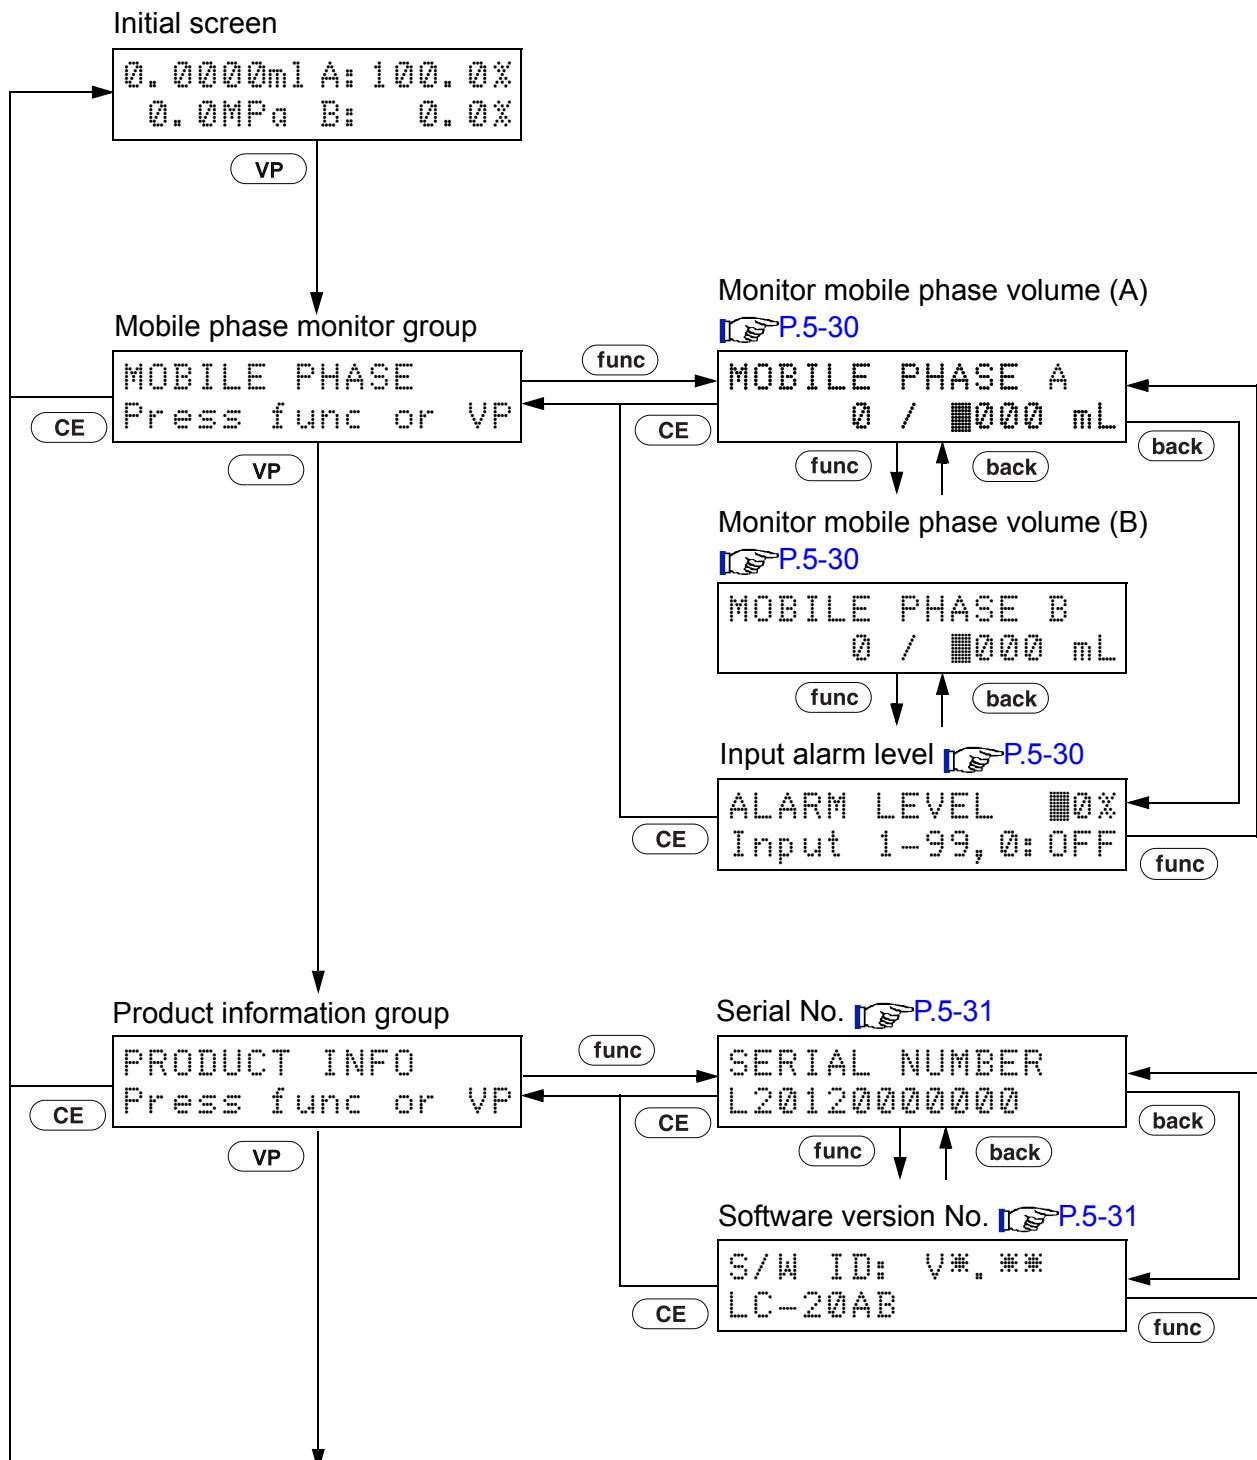

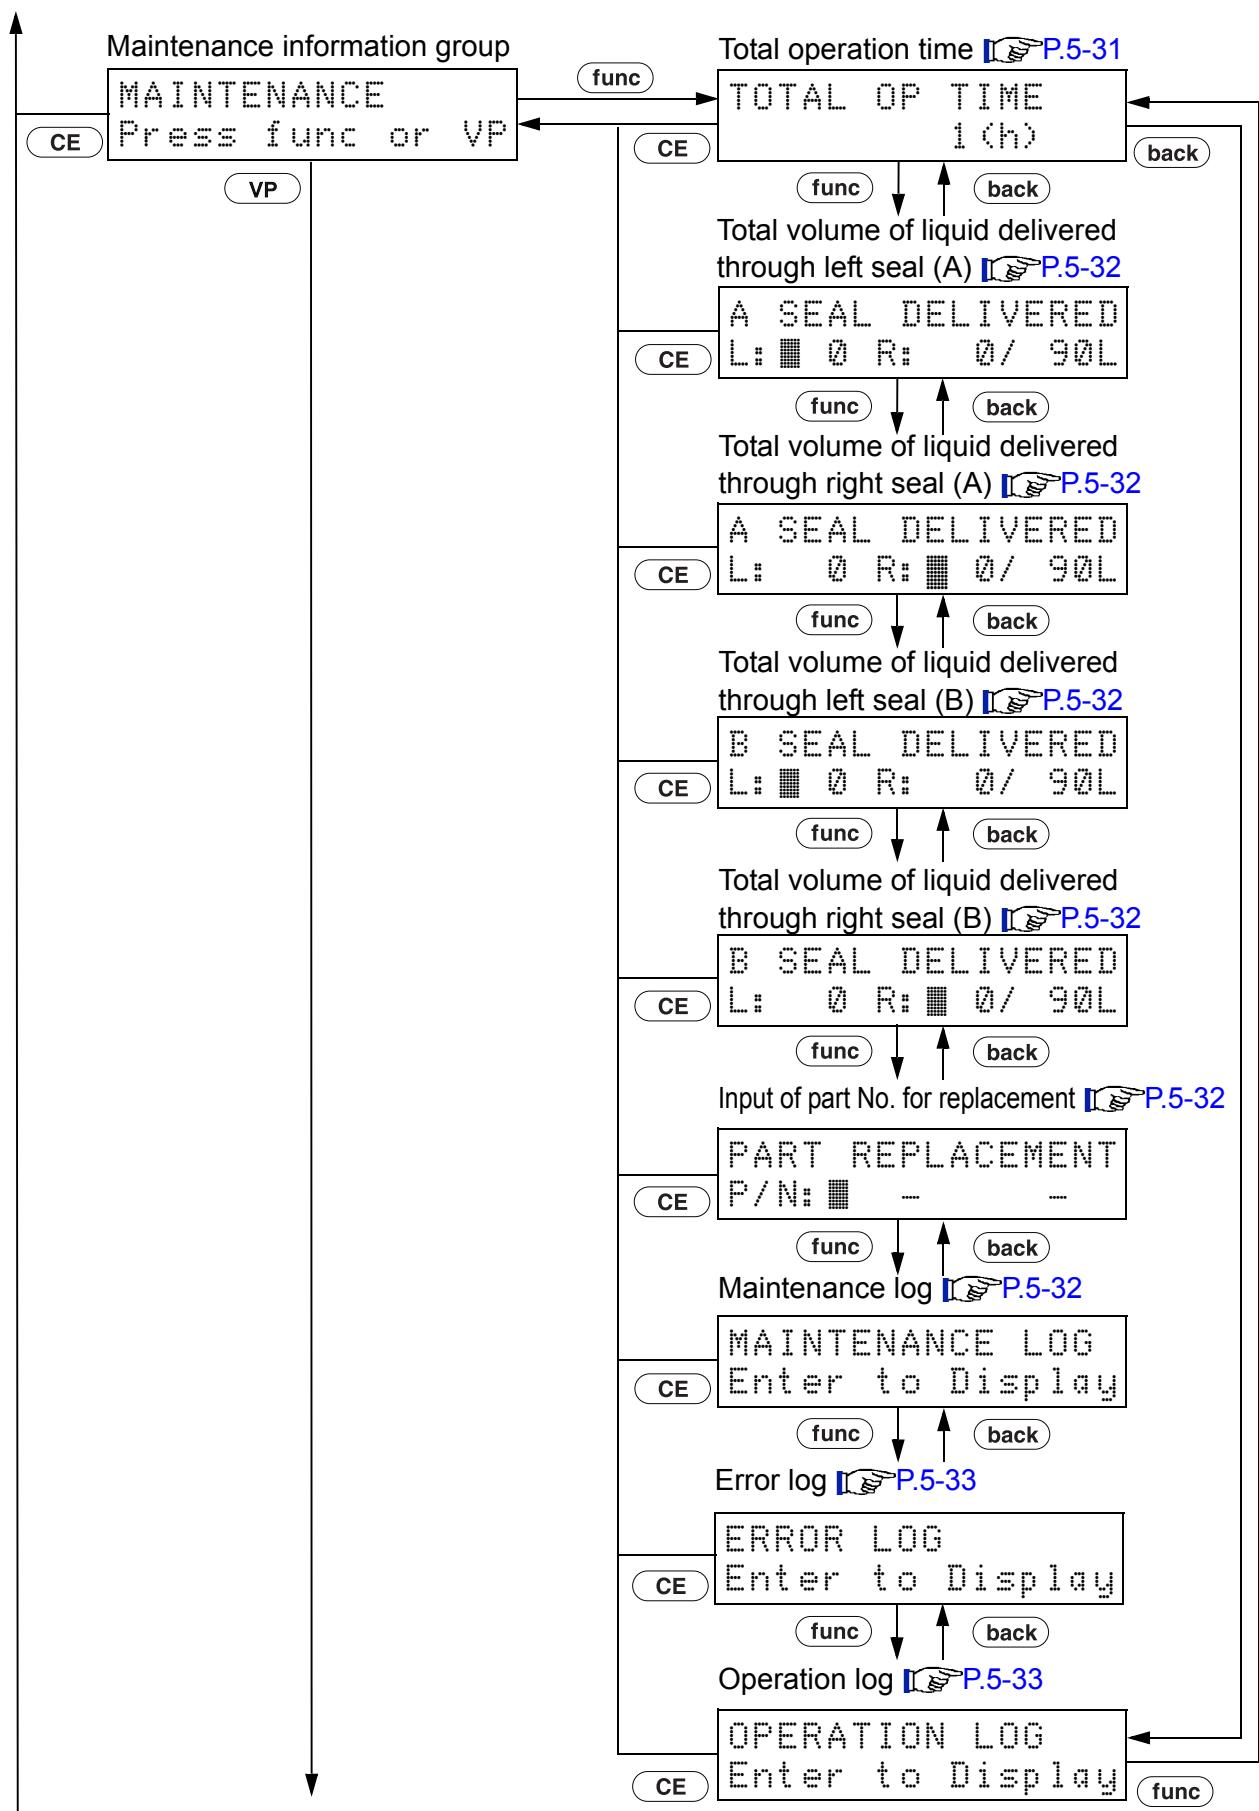

## 5. Application Operation

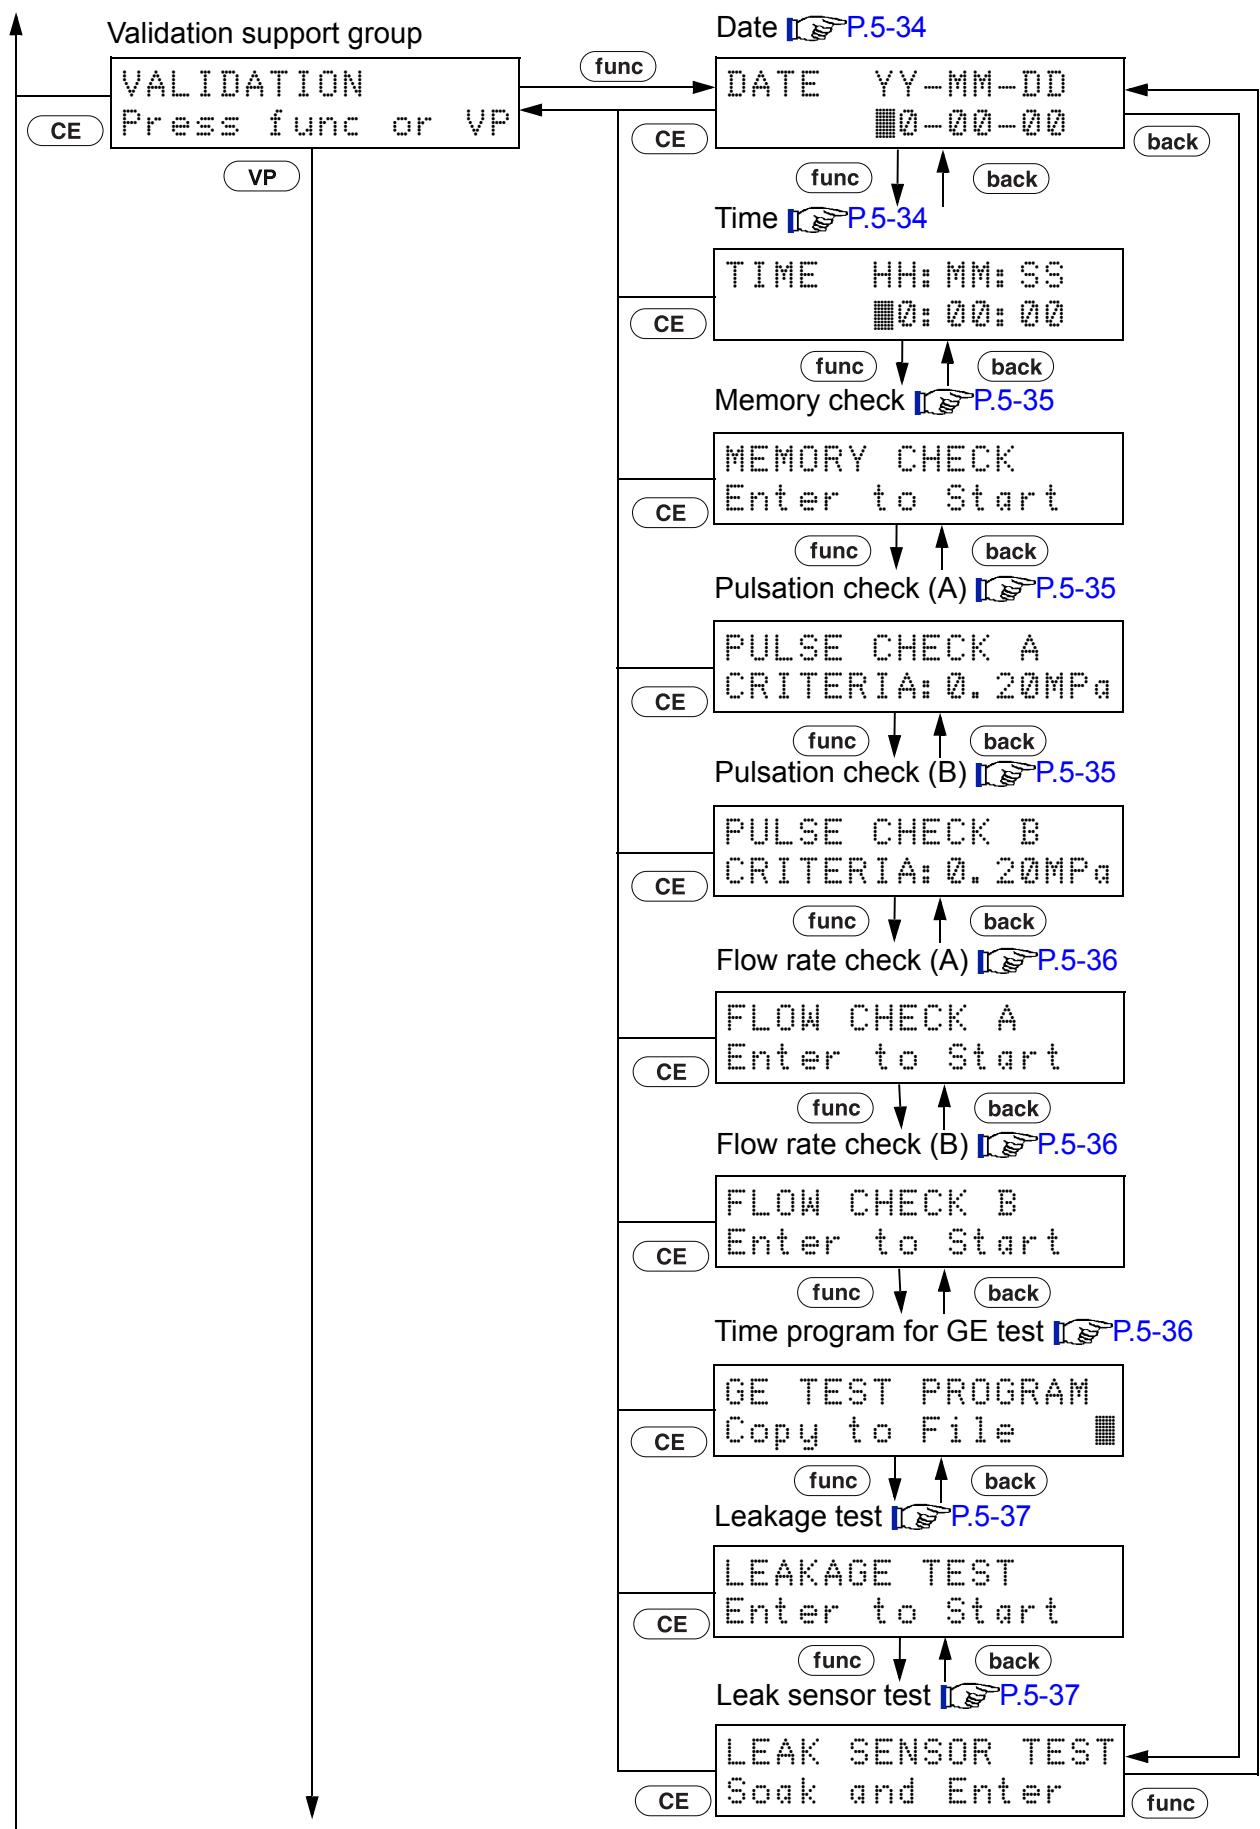

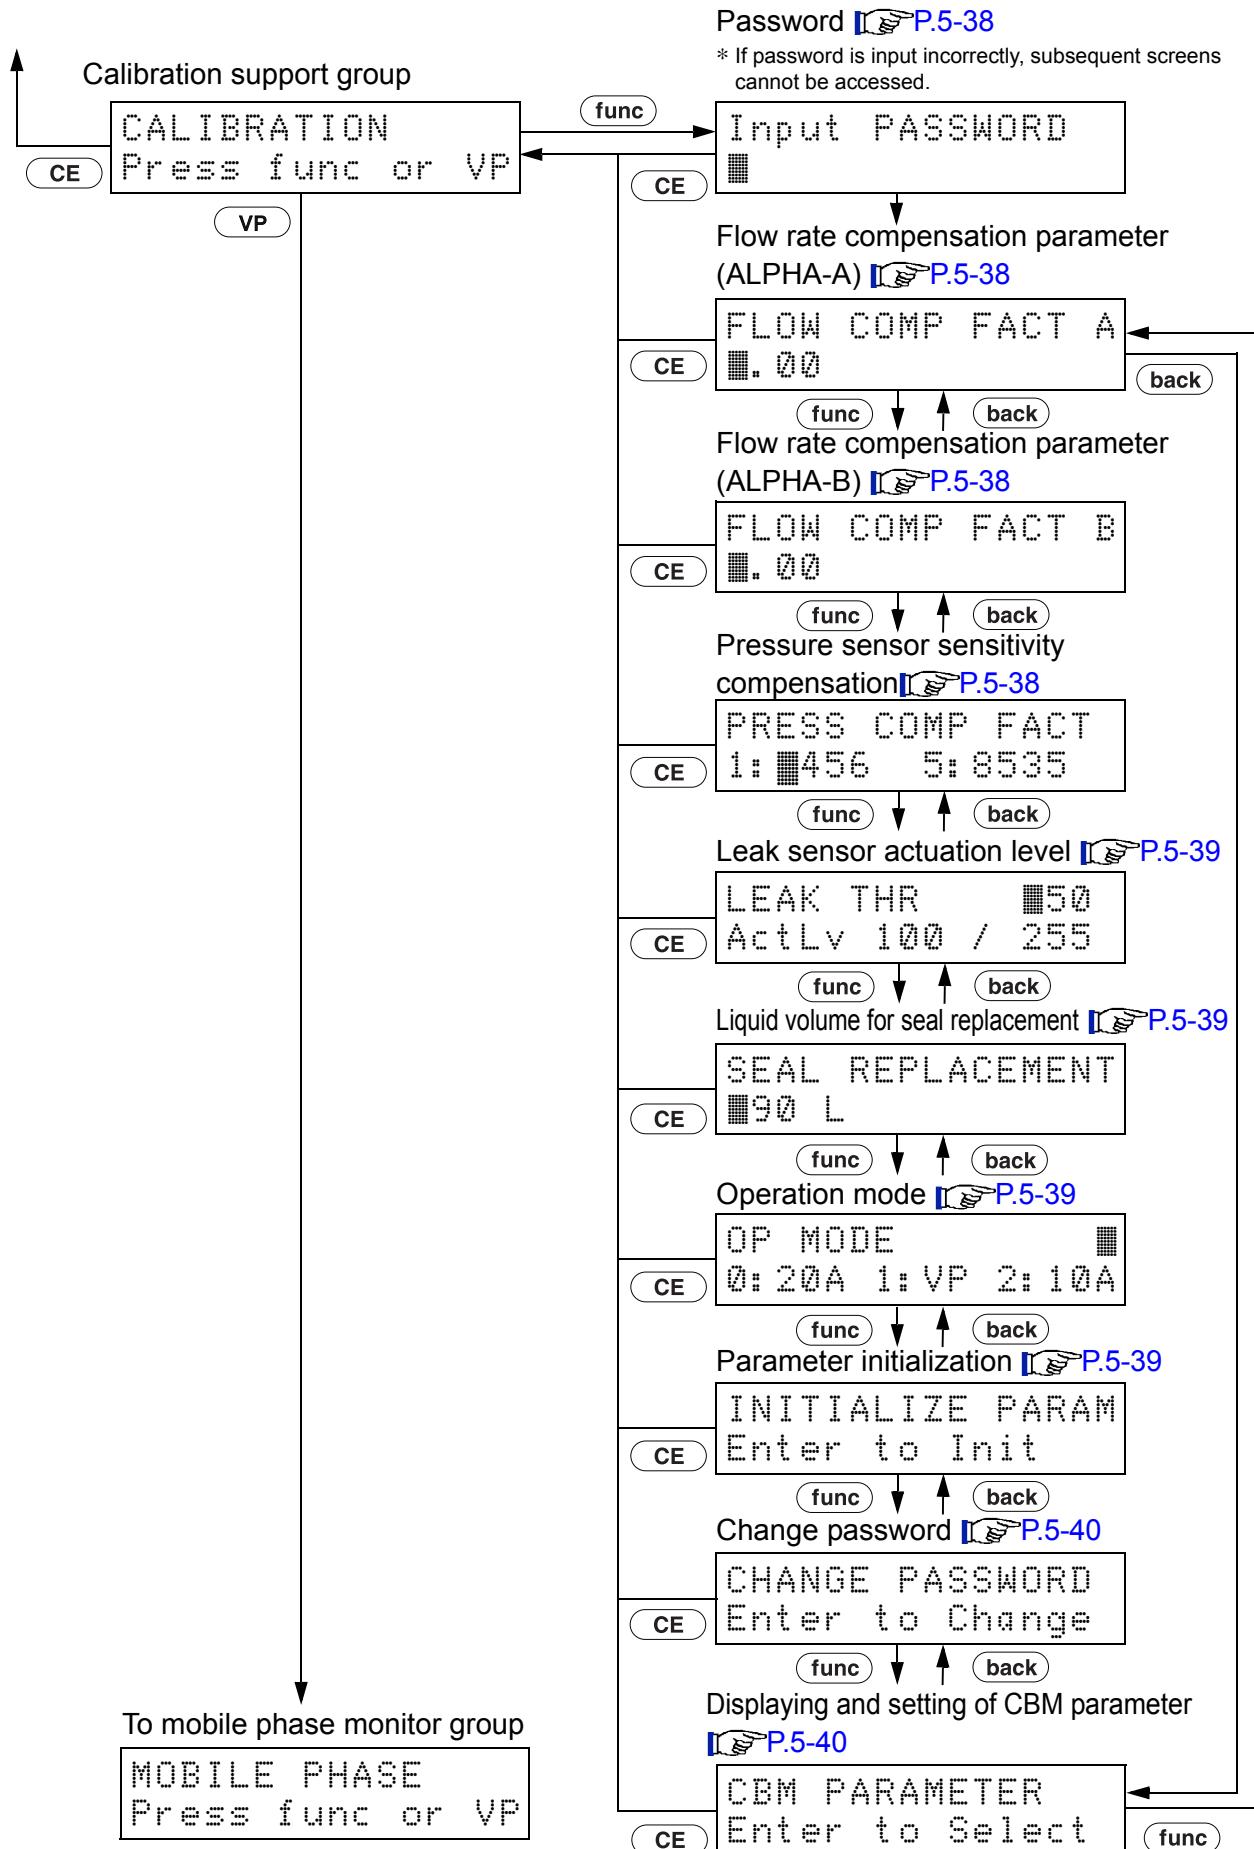

# 5.2 Parameter in Auxiliary Functions

There are five groups for auxiliary functions:

Parameter Setting, File Operation, Control Setting, System Setting and Monitor Setting.

## 5.2.1 List of Auxiliary Functions

The auxiliary functions are listed in the tables below.

 "5.1.2 Basic Setting Screen and Auxiliary Function Setting Screen" P. 5-3

### ■ Parameter Settings Group

Command	Operation	Description	Default value	Page
PMAX	Numeric keypad	To set the maximum pressure limit.	10.0	P.5-15
PMIN	Numeric keypad	To set the minimum pressure limit.	0.0	P.5-15
SV	Numeric keypad	To switch the solenoid valve to select mobile phase in optional FCV-10ALvp or FCV-11AL.	1	P.5-16
EVENT	Numeric keypad	To control output relays.	0	P.5-17
ACOMP	Numeric keypad	To perform fine adjustment of compressibility compensation for pump A.	0.45	P.5-17
BCOMP	Numeric keypad	To perform fine adjustment of compressibility compensation for pump B.	0.45	P.5-17
P-TIMER	Numeric keypad	To set a purge execution time.	3	P.5-18
P-FLOW	Numeric keypad	To set a purge flow rate.	8.0	P.5-18
P-PMAX	Numeric keypad	To set a maximum pressure limit at purging.	10.0	P.5-18

### ■ File Operation Group

Command	Operation	Description	Default value	Page
FILE NUM	Numeric keypad	To select a program file No.	0	P.5-19
FILE CPY	Numeric keypad	To copy a file. (including initial conditions and time program)	-	P.5-19
FILE DEL		To delete a time program from a file.	-	P.5-19

#### About files:

The instrument can store up to 10 files of flow rate and other parameter values, and time programs in memory.

File No. 0 to 9 are assigned to each file. The auxiliary functions other than [SV] and [EVENT] are common functions.

Each value can be switched by [FILE NUM] in the File Operation Group.

\* Operation in the table head shows the types of operation described below.

Display : Check the monitor.

 : Press  to activate the function.

Numeric keypad : Press  -  to enter a value and press  to determine the value.

## ■ Control Settings Group

Command	Operation	Description	Default value	Page
P-SET	Numeric keypad	To replace the plunger and plunger seal.	-	P.5-20
ZERO ADJ	(enter)	To perform zero adjustment of pressure screen.	-	P.5-20

## ■ System Settings Group

Command	Operation	Description	Default value	Page
LOCAL	Numeric keypad	To select independent operation or control via system controller.	0	P.5-21
ADRS	Numeric keypad	To set address of the instrument for control via system controller.	3	P.5-21
KEY CLOSE	(enter)	To lock the keypad, preventing unexpected entries.	-	P.5-21
BRIGHT	Numeric keypad	To set brightness of display screen.	3	P.5-22
EXT-S	Numeric keypad	To close [EVENT1] output terminal at the start of time program, and [EVENT2] output terminal on detection of pump error.	0	P.5-22
S-PROT	Numeric keypad	To reduce the flow rate without stopping the pumping when the pressure exceeds the p.max value.	0	P.5-22
FCV TYPE	Numeric keypad	To set a type of flow channel valve connected to the [SOL.V] connector on the back of the instrument.	0	P.5-23
PRS-UNIT	Numeric keypad	To set a unit of pressure.	0	P.5-23
RANGE	Numeric keypad	To set a full range for pressure signals for the recorder output.	10	P.5-23
CBM LINK	Numeric keypad	To set a link destination of system controller.	1	P.5-23
BEEP MODE	Numeric keypad	To set the operation of buzzer.	0	P.5-24

## ■ Monitor Settings Group

Command	Operation	Description	Default value	Page
MON TIME	Numeric keypad	To monitor the elapsed time when running a time program.	0	P.5-24
MON ID	Numeric keypad	To monitor the pump ID.	0	P.5-25
MON SV	Numeric keypad	To monitor the flow line of solenoid valve unit.	0	P.5-25
MON REVA	Numeric keypad	To monitor pump A's revolution counter.	0	P.5-26
MON REV B	Numeric keypad	To monitor pump B's revolution counter.	0	P.5-26
DEGAS PRS	Display	To monitor the vacuum pressure in degasser unit.	-	P.5-26

\* Operation in the table head shows the types of operation described below.

Display : Check the monitor.

(enter) : Press (enter) to activate the function.


Numeric keypad : Press ( - ) - ( 9 ) to enter a value and press (enter) to determine the value.

## 5. Application Operation

### 5.2.2 Showing the Auxiliary Function Screen

1 Press **CE**.


Initial screen appears.

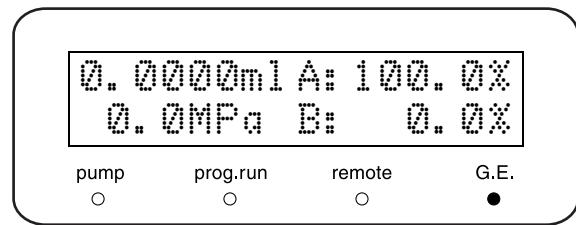


2 Press **func** three times to show parameter setting group, the first group of the auxiliary function.

Pressing more than three times shows the other groups of the auxiliary function.

\* Press **back** to return the previous screen.

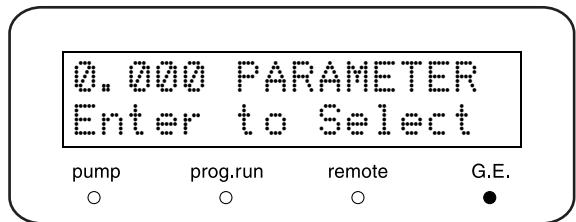

3 Select the desired group and press **enter**.

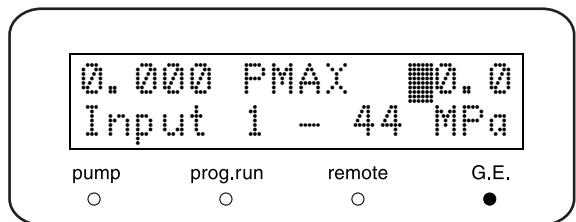

4 Press **func** and select the desired parameter.


5 Press **func** or **back** to move to the other functions.

6 Press **CE** to show the group screen.

Press **CE** to return to the initial screen.

### 5.2.3 Parameter Settings Group

This setting group is for pumping parameters.

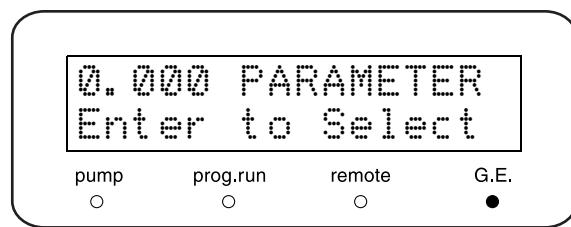

#### ■ Setting Maximum Pressure Limit [PMAX]


Sets the maximum pressure limit in order to protect the column and other parts in the flow line.

Enter a set value (pressure) and press **enter**.


Set range	Steps
1.0 ~ 44.0 MPa	0.1 MPa
10 ~ 440 kgf/cm <sup>2</sup>	1 kgf/cm <sup>2</sup>
10 ~ 440 bar	1 bar
140 ~ 6200 psi	1 psi

\* If the flow rate is set to 5.0001ml/min or a higher value, the maximum possible setting for the pressure is 22.0MPa.

$$1\text{kgf}/\text{cm}^2 = 0.098\text{MPa} = 0.98\text{bar} = 14.2\text{psi}$$




If the pressure exceeds the set maximum limit, solvent delivery is automatically stopped, an alarm sounds, and an error message shown on the right is displayed.

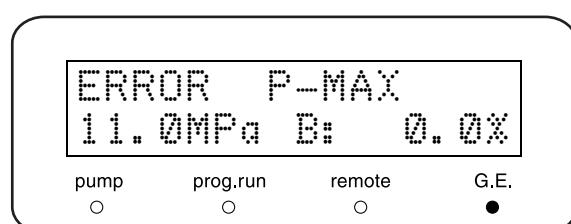

#### ■ Setting Minimum Pressure Limit [PMIN]

Sets the minimum pressure limit in order to prevent drops in pressure, which may occur in the following situations.

- When the mobile phase in the reservoir bottle is depleted and air is delivered into the flow line.
- When a leakage occurs in the flow line.



## 5. Application Operation

Enter a set value (pressure) and press **enter**.

Set range	Steps
0.0 ~ 44.0 MPa	0.1 MPa
0 ~ 440 kgf/cm <sup>2</sup>	1 kgf/cm <sup>2</sup>
0 ~ 440 bar	1 bar
0 ~ 6200 psi	1 psi


\* If the flow rate is set to 5.0001ml/min or a higher value, the maximum possible setting for the pressure is 22.0MPa.

$$1\text{kgf/cm}^2 = 0.098\text{MPa} = 0.98\text{bar} = 14.2\text{psi}$$

If the pressure is below the set minimum limit for one minute after starting solvent delivery, solvent delivery is automatically stopped, an alarm sounds, and an error message shown on the right is displayed.

### NOTE


When [0] is set as [PMIN], pumping will not stop automatically and alarm will not sound when the pressure drops.

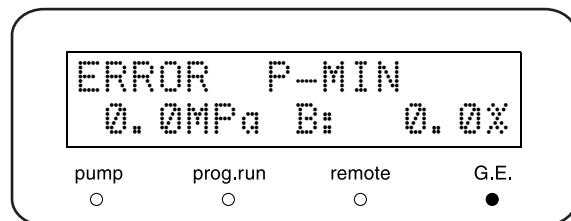

### ■ Setting Solenoid Valve Position [SV]

Selects the mobile phase to be fed when using the optional reservoir switching valve (FCV-10ALvp and FCV-11AL).

Enter the following value corresponding to the selected mobile phase and press **enter**.



Solenoid valve type	Set value	Selected mobile phase
FCV-10ALvp	1	Solvent A
	2	Solvent B
	3	Solvent C
	4	Solvent D

Solenoid valve type	Set value	Selected mobile phase
FCV-11AL	0	All channels are set to the A side.
	1	Channel 1 is set to the B side.
	2	Channel 2 is set to the B side.
	3	Channel 3 is set to the B side.

The above settings can be combined in use.

Example: Set [SV] 123 to set all 1, 2 and 3 channels to B side.

**NOTE**


Before setting [SV], select a solenoid valve unit by [FCV TYPE].

 "Selecting Flow Channel Valve Type [FCV TYPE]"  
P. 5-23

### ■ Setting EVENT Output Terminals [EVENT]

Sets the relays ON (close) / OFF (open) accessed by the EVENT output terminals on the back of the instrument. Enter the value and press **enter**.

Set value	[EVENT1] output	[EVENT2] output
0	Relay 1 OFF	Relay 2 OFF
1	Relay 1 ON	Relay 2 OFF
2	Relay 1 OFF	Relay 2 ON
12	Relay 1 ON	Relay 2 ON

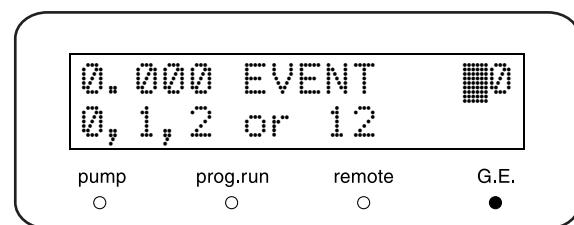



### ■ Setting Fine Adjustment of Compressibility Compensation [ACOMP] [BCOMP]

This instrument performs compressibility compensation to minimize pulsation due to mobile phase compressibility. The value set for this parameter is the compressibility of the mobile phase used. This value is utilized to fine-tune the compensation.

For low-pressure pumping, there is no particular need to alter this parameter, but when a high-compressibility mobile phase such as hexane or methanol is delivered at high pressure of 20MPa or more, alter this parameter to the compressibility of the mobile phase used.

[ACOMP] and [BCOMP] are the compressibility settings for pump A and pump B respectively, and can be set independently.

The setting units are  $(\text{GPa})^{-1}$ . Enter the value using numeric keypad, and press **enter**. The initial setting is 0.45.

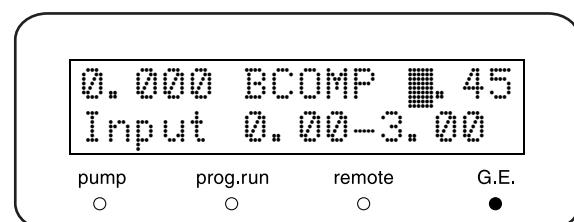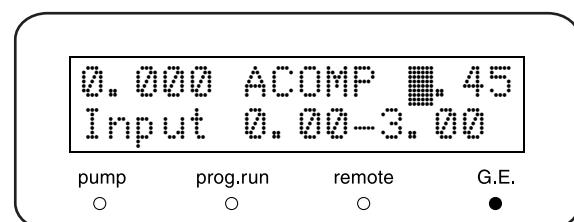


Mobile phase	Compressibility ( $\text{GPa}^{-1}$ )
Water	0.45
Acetonitrile	1.20
Methanol	1.25
Hexane	1.60

### ■ Setting Purge Time [P-TIMER]

Sets purge time.

Enter a time using the numeric keypad and press **enter**.

Setting range is 1-20 (minutes) with 1 minutes step as setting unit.

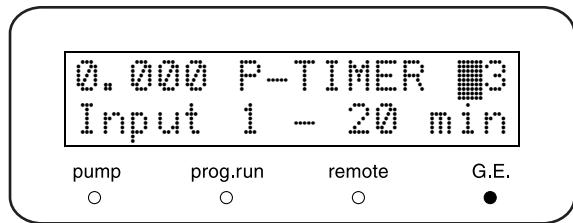


### ■ Setting Purge Flow Rate [P-FLOW]

Sets the flow rate during purging.

It is available to both purging by **purge** and auto-purging by system controller.

Enter a flow rate using the numeric keypad and press **enter**.

Setting range is 0.1-10.0 (mL/min) with 0.1mL/min step as setting unit.

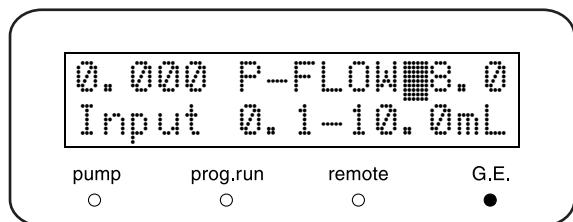


### ■ Setting Maximum Pressure Limit during Purging [P-PMAX]

Sets the maximum pressure limit during auto-purging by system controller.

During purging by **purge**, the maximum pressure limit is 2.0MPa.

Enter a maximum pressure limit using the numeric keypad and press **enter**.

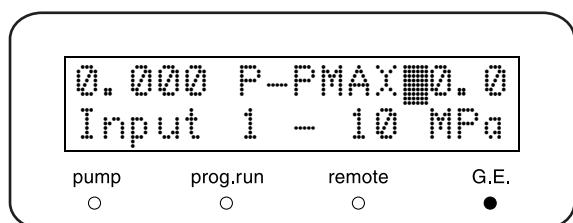


Set range	Steps
1.0 ~ 10.0 MPa	0.1 MPa
10 ~ 102 kgf/cm <sup>2</sup>	1 kgf/cm <sup>2</sup>
10 ~ 100 bar	1 bar
140 ~ 1400 psi	1 psi

1kgf/cm<sup>2</sup> = 0.098MPa = 0.98bar = 14.2psi

### 5.2.4 File Operation Group

This is the group for file operation.

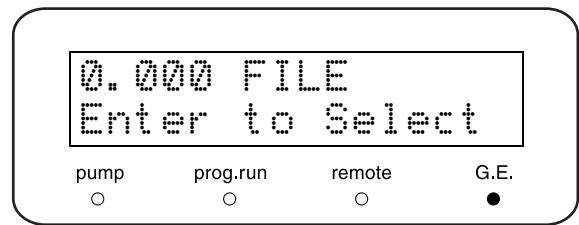


#### ■ File Number [FILE NUM]

This function selects a file.

Up to 10 files of time program can be created and stored in memory.


Enter the desired file number using the numeric keypad [0-9] and press **enter**.

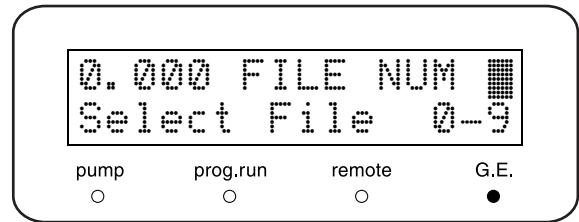

#### ■ Copying a File [FILE CPY]

The contents of the file currently selected by [FILE NUM] are copied to the selected file number.


Enter the file number and press **enter**.

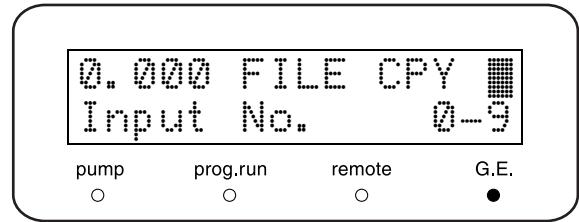

#### ■ Deleting a Time Program [FILE DEL]

The contents of the time program of the currently selected file are deleted.


Press **enter**.

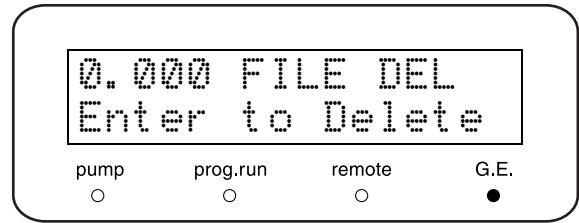

## 5. Application Operation

### 5.2.5 Control Settings Group

This is the group for control.

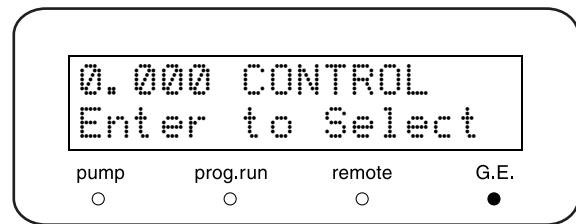


#### ■ Plunger Set [P-SET]

Manually moves the plungers to a safe position for seal replacement or removal of pump heads.

Enter the desired value and press **enter**.

The pump indicator illuminates and the plungers for pumps A and B move.


Set value	Function
1	The left plungers are retracted. In this state, remove the left pump heads.
2	The right plungers are retracted. In this state, remove the right pump heads.
3	The plungers move to an intermediate position.

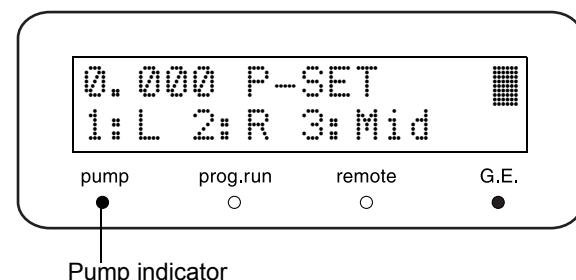

#### ■ Zero Adjustment of Pressure Sensor [ZERO ADJ]


Clears the value of the pressure sensor to zero in atmospheric pressure.

- 1 Open the drain valve.  
Pressure sensor is released from the pressure.
- 2 Press **enter**.

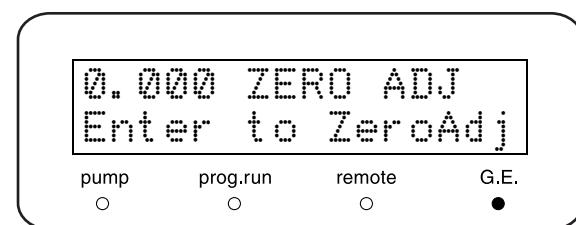

### 5.2.6 System Settings Group

This is the group for system settings.

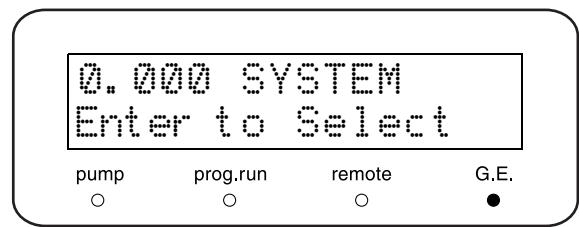


#### ■ Selecting Local/Remote Mode [LOCAL]

Sets whether this instrument is operated by system controller or the instrument operates independently when system controller is connected.

Enter the desired value, and press **enter**.

Set value	Mode	Function
0	Remote	Operate via system controller (initial setting)
1	Local	Operate independently (in local mode)

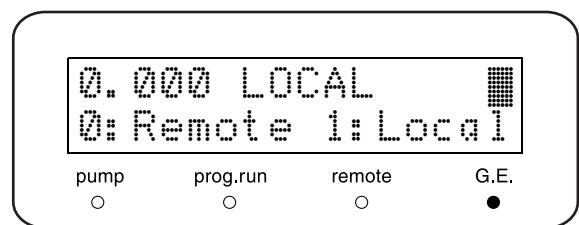


#### ■ Setting Link Address [ADRS]

Sets the address (channel number) when this instrument is connected to system controller.

Enter the address number, and press **enter**.

Address	Function
1-12	Channel numbers when this instrument is connected to system controller.

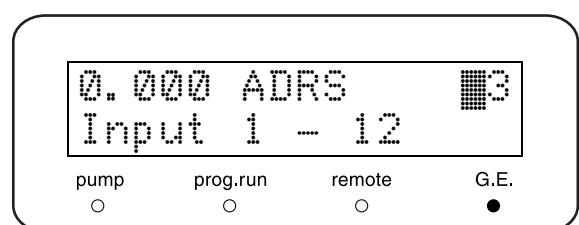


#### ■ Disables Key Entry [KEY CLOSE]

Press **enter** to prohibit the key entry.

After this, key operation is not available.

\* To release this function, press **del** while pressing **CE**.

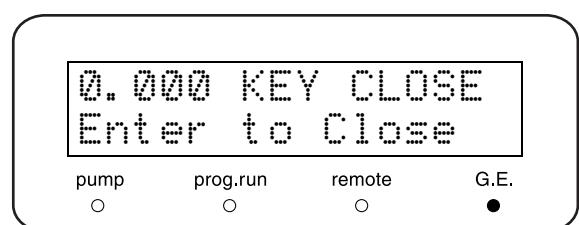


## 5. Application Operation

### ■ Setting Brightness of Display Screen [BRIGHT]

Sets the brightness of display screen.

Enter the set value and press **enter**.

Value range is 1 to 4 and 4 is the brightest.

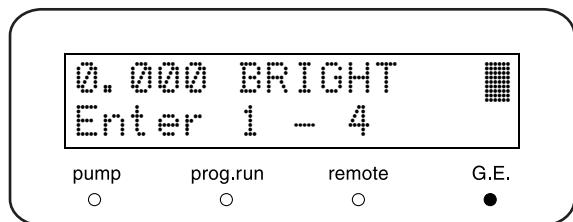


### ■ External Signal Functions for EVENT Output Terminals [EXT-S]

This feature is typically used to control external devices through the EVENT outputs (relays 1 and 2).

Enter the desired value and press **enter**.

Set value	Function
0	Relay contact points are controlled by the [EVENT] set value.
1	Relay 1 ([EVENT1] terminals) closes at the start of a time program.
2	Relay 2 ([EVENT2] terminals) closes on detection of an error.
3	Both functions of above 1 and 2 are enabled.

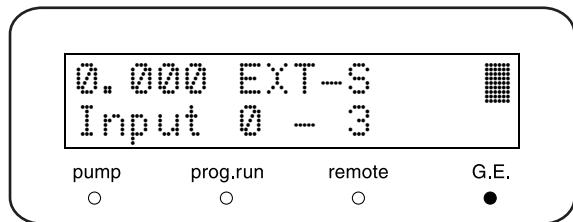

#### NOTE


The corresponding [EVENT] parameter will not be available when [EXT-S] function is activated.

### ■ Setting System Protection [S-PROT]

Halves the flow rate repeatedly until pressure does not exceed [P.MAX].

Enter the desired value and press **enter**.

Set value	Function
0	Cancels system protection.
1	Set system protection.

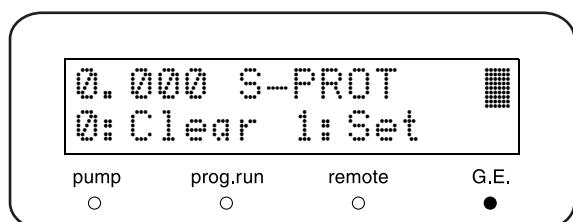


\* To clear [ERROR P.MAX], press **CE**. It turns the alarm off, and the flow rate will be increased as before.

### ■ Selecting Flow Channel Valve Type [FCV TYPE]

Selects the type of flow control valve connected to the [SOL.V] connector on the back of the instrument.

Enter the desired value and press **enter**.

Set value	Valve unit
0	FCV-10ALvp
1	FCV-11AL

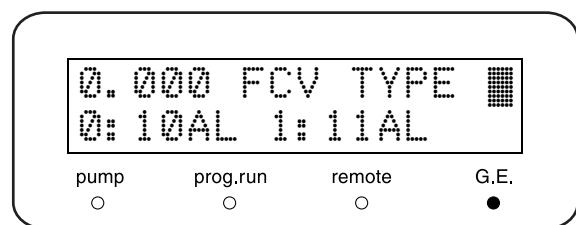


### ■ Selecting a Unit of Pressure [PRS-UNIT]

Sets the units by which the pressure is displayed.

Enter a set value and press **enter**.

Set value	Unit
0	MPa
1	kgf/cm <sup>2</sup>
2	bar
3	psi

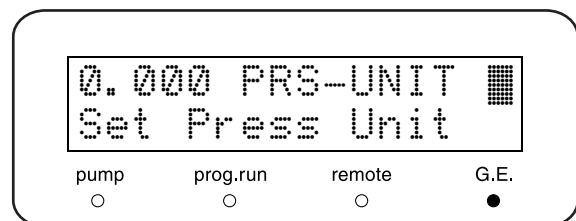


$1\text{kgf}/\text{cm}^2 = 0.098\text{MPa} = 0.98\text{bar} = 14.2\text{psi}$

### ■ Setting Pressure Recorder Range [RANGE]

Sets the full scale of the pressure recorder output.

Enter the desired value and press **enter**.

Full scale = (Set value) × 5.0MPaFS
-------------------------------------

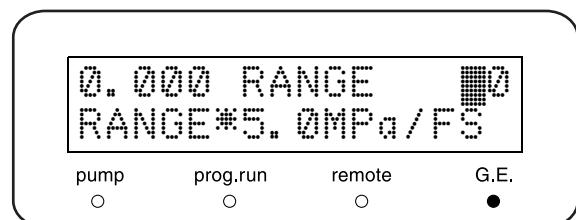

Examples:


- When set value is 1, the full scale is 5.0MPaFS.
- When set value is 10, the full scale is 50.0MPaFS.

### ■ Switching Remote Connector internal/external [CBM LINK]

Sets the link destination of system controller.

Enter the desired value and press **enter**.

Set value	Function
0	Link with CBM-20Alite (option) inside of the instrument.
1	Link with external system controller by optical cable connected to [REMOTE] connector.

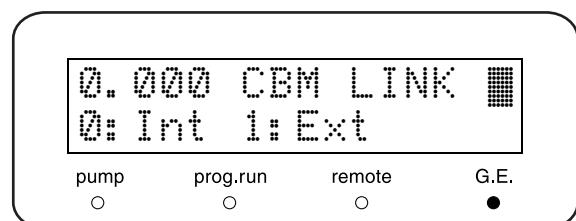


## 5. Application Operation

### ■ Setting Operation of Buzzer [BEEP MODE]

Sets the operation of buzzer.


Enter a set value and press **enter**.

Set value	Function
0	Alarm sound when error occurs and key entry sound are enabled. (default)
1	Only alarm sound when error occurs is enabled. Key entry sound is disabled.
2	All sounds are disabled.

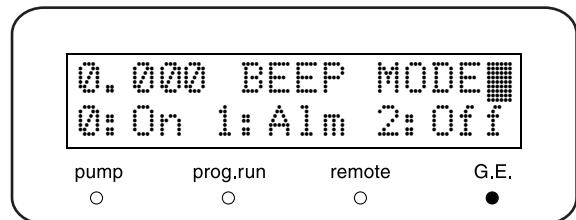

### 5.2.7 Monitor Settings Group

This is the group for monitor setting.

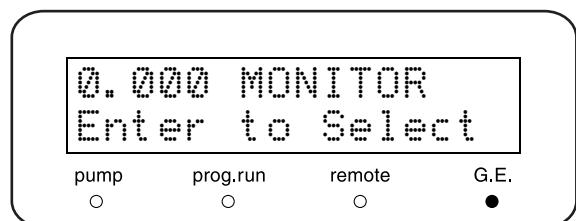


### ■ Monitoring Program Elapsed Time [MON TIME]


Monitors the time elapsed from the start of the time program.

Enter a set value and press **enter**.

Set value	Function
0	Clear this function
1	Set this function

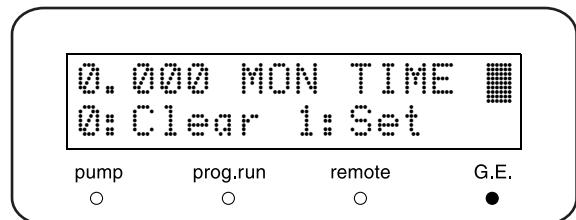

If [1] is set, the initial screen will be as shown on the right while the program is running. However, if other monitor functions are set, this screen may not be displayed.

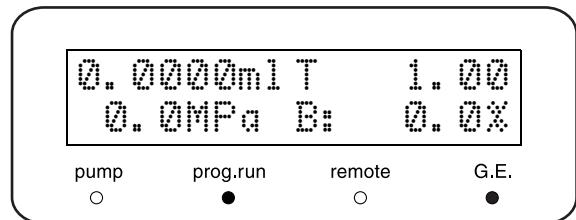


### ■ Monitoring ID for Remote Control [MON ID]

Monitors the ID (A, B, C or D) connected to a system controller.



Enter a set value and press **enter**.

Set value	Function
0	Clear this function
1	Set this function

If the ID is [A], the initial screen will be as shown on the right.

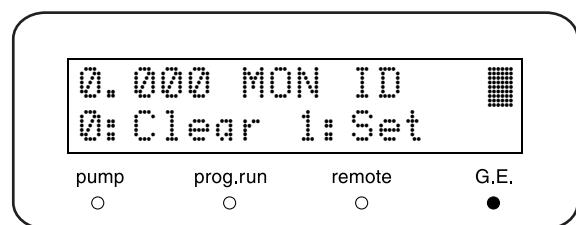

If the instrument is not connected to a system controller, the initial screen will be as shown on the right.

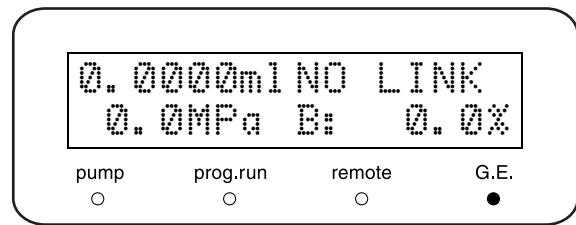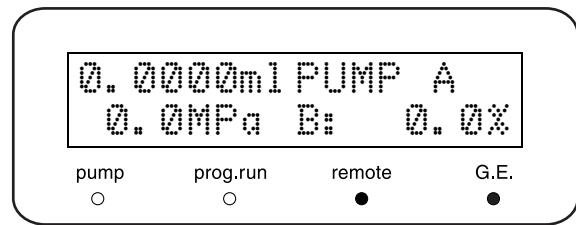



### ■ Monitoring Flow Line of Solenoid Valve Unit [MON SV]

Monitors the flow line of the solenoid valve unit.

Enter the set value and press **enter**.

Set value	Function
0	Clear this function
1	Set this function

If [1] is set, the initial screen will be as shown on the right.

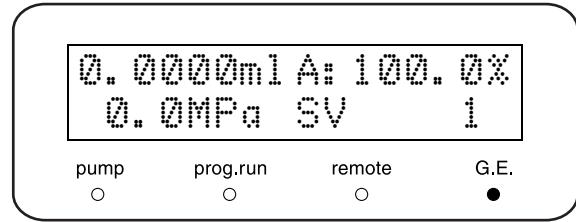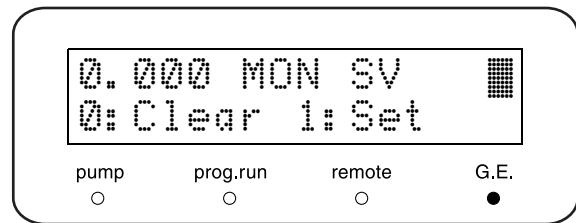


## 5. Application Operation

### ■ Monitoring Pump Revolution Counter [MON REVA] [MON REVB]

Monitors the pump revolution counters for pumps A and B.

Enter a set value and press **enter**.


Set value	Function
0	Clear this function
1	Set this function

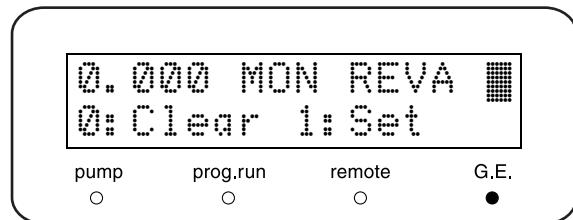

Monitoring the pump revolution counter provides an indication of the timing to replace seals.

Approx. 4,500,000 times of revolution (approx. 1,500 hours by 1mL/min) by running at 10MPa (102kgf/cm<sup>2</sup>) with 2-propanol is the aim to replace seals.


If [1] is set for [MON REVA], the initial screen will be as shown on the right. If [1] is set for [MON REVB], [B] will be displayed in the top line instead of [A]. However, if other monitor functions are set, this screen may not be displayed.

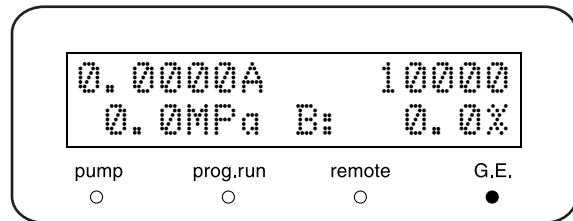

### ■ Monitoring Vacuum Pressure in Degasser Unit [DEGAS PRS]

Monitors the pressure in the DGU-20A degasser unit.

- When the pressure value is standard, [(OK)] is displayed.
- When the pressure value is not standard, [(NG)] is displayed.
- When the DGU-20A degasser unit is not connected, [(NOT CONNECTED)] is displayed.

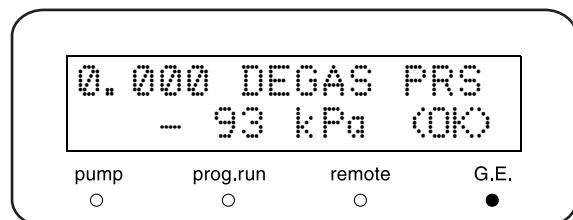

# 5.3 VP Functions

VP functions support the validation of the instrument by check functions or displaying the instrument information. There are five groups for VP functions: Mobile Phase Monitor, Product Information, Maintenance Information, Validation Support, and Calibration Support.

## 5.3.1 List of VP Functions

The VP functions are listed in the tables below.

 "5.1.3 VP Function Screen" P. 5-8

### ■ Mobile Phase Monitor Group

Command	Operation	Function	Page
MOBILE PHASE A	Display/ Numeric keypad	To monitor the remaining volume and set volume of pump A's mobile phase	P.5-30
MOBILE PHASE B	Display/ Numeric keypad	To monitor the remaining volume and set volume of pump B's mobile phase	P.5-30
ALARM LEVEL	Numeric keypad	To set the alarm level of remaining mobile phase	P.5-30

### ■ Product Information Group

Command	Operation	Function	Page
SERIAL NUMBER	Display	To show the serial number of the instrument	P.5-31
S/W ID	Display	To show the version number of software	P.5-31

### ■ Maintenance Information Group

Command	Operation	Function	Page
TOTAL OP TIME	Display	To show the total cumulative operating time of the instrument	P.5-31
A SEAL DELIVERED	Display/ <input type="button" value="enter"/>	To show the total volume of flow rate through seal (pump A), and volume at a timing to replace a seal	P.5-32
B SEAL DELIVERED	Display/ <input type="button" value="enter"/>	To show the total volume of flow rate through seal (pump B), and volume at a timing to replace a seal	P.5-32
PART REPLACEMENT	Numeric keypad	To record the replaced parts number	P.5-32
MAINTENANCE LOG	Display/ <input type="button" value="enter"/>	To show maintenance log	P.5-32
ERROR LOG	Display/ <input type="button" value="enter"/>	To show error log	P.5-33
OPERATION LOG	Display/ <input type="button" value="enter"/>	To show operation log	P.5-33

\* Operation in the table head shows the types of operation described below.

Display : Check the monitor.

: Press  to activate the function.

Numeric keypad : Press  -  to enter a value and press  to determine the value.

## 5. Application Operation

---

### ■ Validation Support Group

Command	Operation	Function	Page
DATE	Display/ Numeric keypad	To show/set the date	P.5-34
TIME	Display/ Numeric keypad	To show/set the time	P.5-34
MEMORY CHECK	(enter)	To run the memory check	P.5-35
PULSE CHECK A/B	Numeric keypad/ (enter)	To run the pulsation check	P.5-35
FLOW CHECK A/B	(enter)	To run the flow rate check	P.5-36
GE TEST PROGRAM	Numeric keypad	To set the time program to check concentration accuracy by gradient mode	P.5-36
LEAKAGE TEST	(enter)	To run the leakage check	P.5-37
LEAK SENSOR TEST	(enter)	To run the leak sensor check	P.5-37

### ■ Calibration Support Group

Command	Operation	Function	Page
Input PASSWORD* <sup>1</sup>	Numeric keypad	To input password	P.5-38
FLOW COMP FACT A/B	Numeric keypad	To enter the flow rate compensation factor (ALPHA)	P.5-38
PRESS COMP FACT	Numeric keypad	To enter pressure sensor sensitivity compensation factor	P.5-38
LEAK THR	Numeric keypad	To enter leak sensor operation level	P.5-39
SEAL REPLACEMENT	Numeric keypad	To set the volume at which seals are replaced	P.5-39
OP MODE	Numeric keypad	To select the operation mode	P.5-39
INITIALIZE PARAM	(enter)	To initialize parameters	P.5-39
CHANGE PASSWORD	Numeric keypad	To change password	P.5-40
CBM PARAMETER	(enter)	To show/set CBM-20A(lite) parameters	P.5-40

\*1 If the password is not input correctly, the functions after [FLOW COMP FACT A] in the Calibration Support Group cannot be accessed, even (func) is pressed.

\* Operation in the table head shows the types of operation described below.

Display : Check the monitor.


(enter) : Press (enter) to activate the function.

Numeric keypad : Press ( - ) - ( 9 ) to enter a value and press (enter) to determine the value.


### 5.3.2 Displaying the VP Functions

**1** Press **CE**.

The initial screen appears.

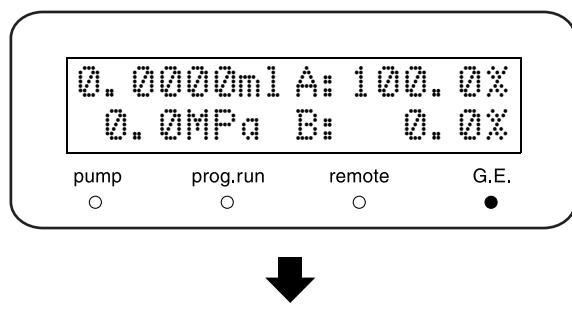


**2** Press **VP** to select the desired Group.

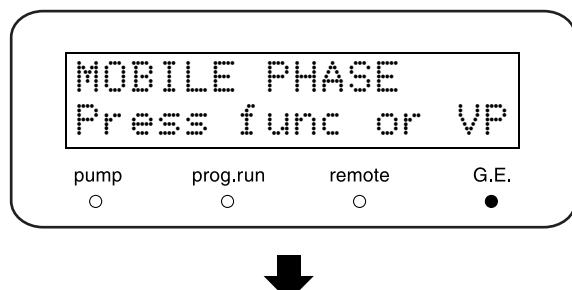

**3** Press **func** until the desired function appears.

\* To return to the previous screen, press **back**.

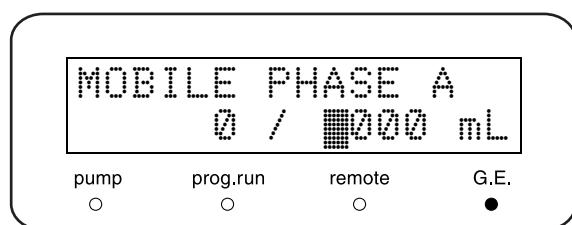

**4** Follow the further instructions of the selected function.


**5** To select a different VP Function Group, press **VP** repeatedly.

To select the desired function, press **func** or **back**.

**6** To return to the initial screen, press **CE**.

### 5.3.3 Mobile Phase Monitor Group

This is the group for mobile phase monitor function.




#### ■ Showing/Setting Mobile Phase Volume [MOBILE PHASE A/B]


Shows the current remaining volume (①) and set volume (②) of mobile phase.

Enter the mobile phase set volume in mL and press **enter**.

Remaining volume is automatically calculated by pumping.

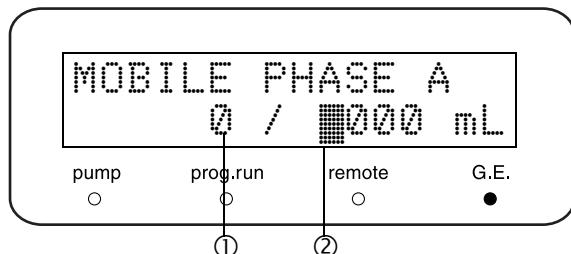


This instrument supports a function for monitoring the remaining volume of pump A's mobile phase A and pump B's mobile phase B. Select the required mobile phase by pressing **func** or **back**.



#### ■ Setting Alarm Level of Remaining Mobile Phase [ALARM LEVEL]

Shows the warning indication when the remaining volume of mobile phase is decreased less than the setting value (%).


The pumping will continue.

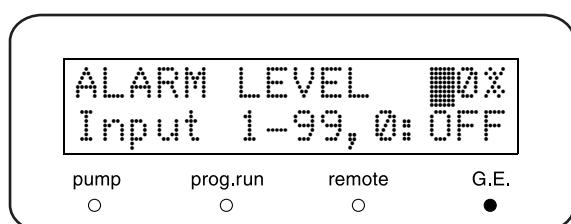

Input the value, and press **enter**.


When 0% is registered, this function will be deactivated.

Warning screen




### 5.3.4 Product Information Group

This group provides the information about the instrument.




#### ■ Showing Serial Number [SERIAL NUMBER]

Shows the serial number of this instrument.

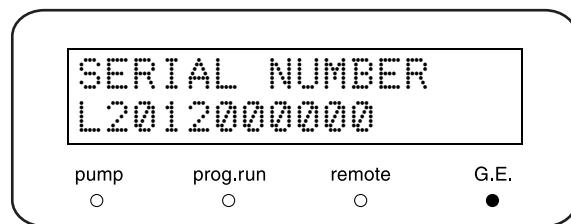


#### ■ Showing S/W Version No. [S/W ID]

Shows the name of software (same as the model name) and version.




### 5.3.5 Maintenance Information Group

This group provides the maintenance-related information.



#### ■ Showing Total Operating Time [TOTAL OP TIME]

Shows the total operating time of this instrument.




### ■ Showing Timing to Replace Plunger Seal [A/B SEAL DELIVERED]

Shows the volume of mobile phase delivered through the left plunger seal currently being used (①), the volume of mobile phase delivered through the right plunger seal currently being used (②), and the volume at which the plunger seal should be replaced (③). (Unit:L)


Press **func** to move the cursor (and switch display) through the items in the following order: pump A's left plunger seal ([L]), pump A's right plunger seal ([R]), pump B's left plunger seal ([L]), and pump B's right plunger seal ([R]). Press **back** to move the cursor in the opposite direction.

After a seal is replaced, move the cursor to the position corresponding to the replaced plunger seal by pressing **func** or **back**, and press **enter**. The value is reset to [0] and the date is recorded in the maintenance log.

Pump A: left

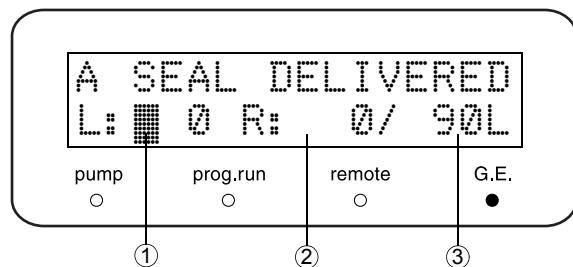


Pump B: right

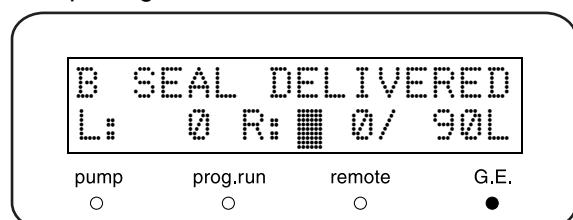

### ■ Entering Replaced Part No. [PART REPLACEMENT]

Enters the replaced part No.

The part No. is recorded in the maintenance log.

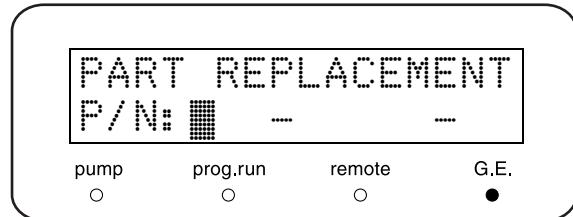

### ■ Showing Maintenance Log [MAINTENANCE LOG]




Shows the maintenance log, which contains the most recent parts replacement records (part No. and date) (up to 10).

Press **enter** repeatedly to show Log1 to Log10 in sequence, and return to the title screen.

In the example on the right, Log1 indicates that part No. 228-30000-91 was replaced on May 12, 2003.

If less than 10 logs are recorded, the screen displays the message as shown on the right.

Press **CE** to return to the title screen.

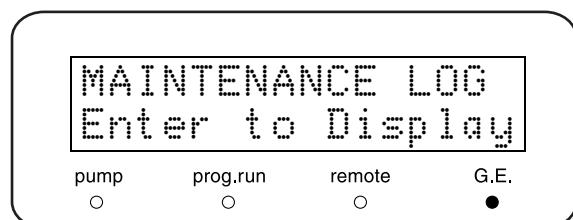

## ■ Showing Error Log [ERROR LOG]


Shows the error log, which contains the most recent errors (up to 10) with their dates.

Press **enter** repeatedly to show Log1 to Log10 in sequence, and return to the title screen.

In the example on the right, Log1 indicates that error on maximum pressure limit occurred on May 12, 2003.

If less than 10 logs are recorded, the screen displays the message as shown on the right.

Press **CE** to return to the title screen.

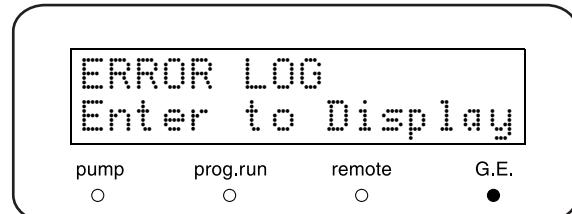

LOG 1	03-05-12
ERROR	P-MAX

⋮

No more Logs
--------------

5

## ■ Showing Operation Log [OPERATION LOG]


Shows the operation log, which contains the most recent password settings, parameter initialization, etc. (up to 10).

Press **enter** repeatedly to show Log1 to Log10 in sequence, and return to the title screen.

In the example on the right, Log1 indicates that password was changed on May 12, 2003.

If less than 10 logs are recorded, the screen displays the message as shown on the right.

Press **CE** to return to the title screen.

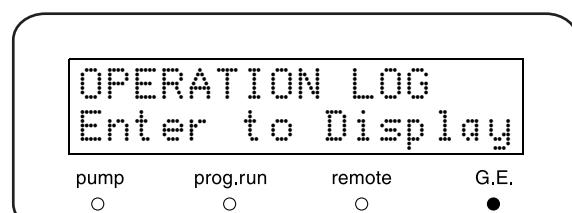

LOG 1	03-05-12
CHANGE	PASSWORD


⋮

No more Logs
--------------

## 5. Application Operation

### 5.3.6 Validation Support Group

This group checks whether the instrument is running correctly.

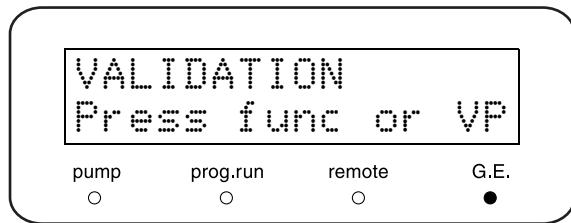

#### ■ Entering Date [DATE]


Shows/enters the date.

However, the value returns to the initial value [00-00-00] after turning the power OFF.

When the instrument is controlled by a system controller, the date is transmitted in connecting.

Example: Set January 2, 2003.

Date

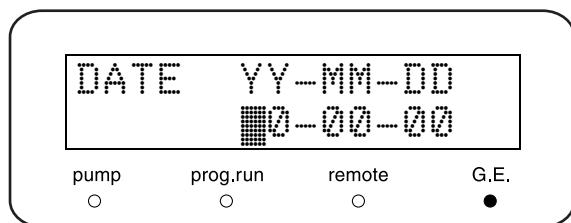

1 Enter year, month and day in 2 digits.

2 Press **enter**.

#### ■ Entering Time [TIME]


Shows/enters the time.

However, the value returns to the initial value [00:00:00] after turning the power OFF.

When the instrument is controlled by a system controller, the time is transmitted in connecting.

Example: Setting 5:30:55 p.m.

Time

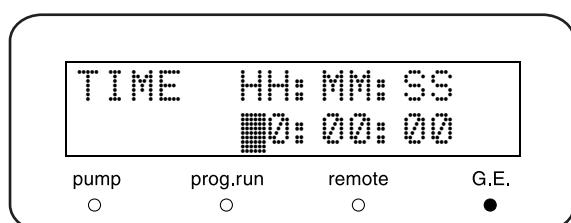

1 Enter hour, minute and second in 2 digits.  
The display uses the 24-hour clock.

2 Press **enter**.

Entered




## ■ Checking Memory [MEMORY CHECK]

Runs the memory check on ROM and RAM.

Press **enter** to start.

Results are shown when checking is completed.

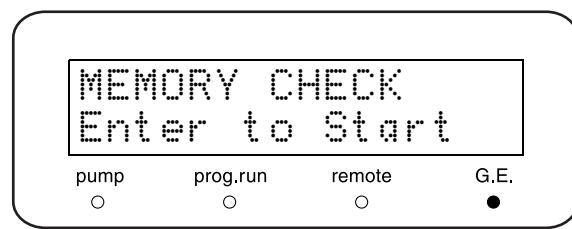

Result







## ■ Checking Pulsation [PULSE CHECK A/B]

- 1 Select either pump A or pump B by pressing **func** or **back**, and set the criterion of pressure fluctuation width (pulse). (Unit: MPa)

- 2 Press **enter** to start.  
Pumping starts at 1mL/min and measuring starts in ten minutes.  
During measuring, set flow rate (or pressure value), actual pressure value, pressure fluctuation width and remaining time.  
Results are shown when measuring is complete.

- 3 Press **enter**.  
The date and results are recorded.

5

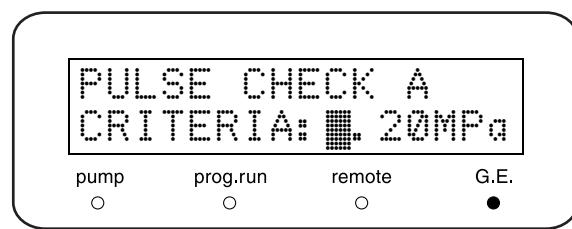

### NOTE

When measuring, ensure that parameters for solvent compressibility compensation are set correctly.

"Setting Fine Adjustment of Compressibility Compensation [ACOMP] [BCOMP]" P. 5-17


### ■ Checking Flow Rate [FLOW CHECK A/B]

- 1** Select either pump A or pump B by pressing **func** or **back**, and press **enter**. Pumping starts at 1mL/min. Prepare for measuring.
- 2** When the preparation for measuring is done, press **enter** again to measure the required time for flowing liquid to fill 5mL of measuring flask.
- 3** Enter the measured time in seconds. Flow rate accuracy (%) and the check result are shown. The criterion is within  $\pm 2\%$ .

#### NOTE

At the measuring, ensure that the parameter for solvent compressibility compensation are set correctly.


 "Setting Fine Adjustment of Compressibility Compensation [ACOMP] [BCOMP]" P. 5-17

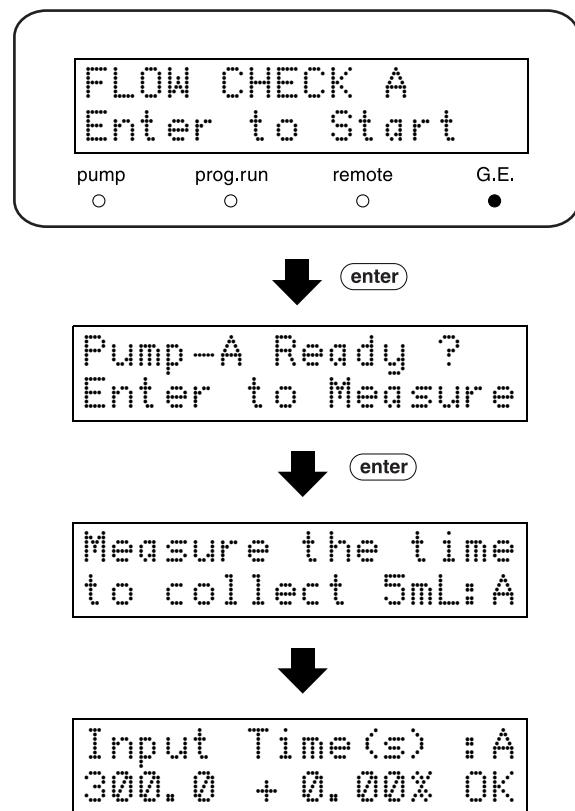

### ■ Setting Time Program to Check Concentration Accuracy of Gradient Mode [GE TEST PROGRAM]


Enter a file number 0-9 of time program in which the default gradient test program is to be copied. This file is automatically loaded for execution.

\* The test program is the gradient time program described in [P.7-21](#).

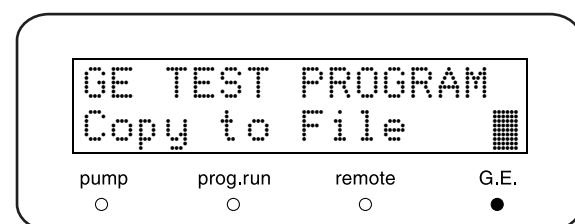

### ■ Checking Leakage [LEAKAGE TEST]

- 1 Insert a plug into the pump outlet.
- 2 Press **enter** during the pump stopped.
- 3 The pump will run, and stop when the pressure reaches about 30MPa. Then, pressure fluctuations will be monitored.  
\* If the pressure drops, there could be a leakage; inspect the entire flow line.

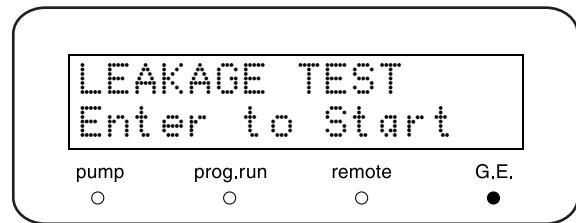

### ■ Checking Leak Sensor [LEAK SENSOR TEST]

Carries on the operation test for leak sensor.

- 1 Use a syringe filled with water to wet the thermosensor at the bottom of the leak sensor.
- 2 Wait about 10 seconds. Then, press **enter**. If the sensor detects a leakage, [GOOD] will be shown. If not, [NO GOOD] will be shown.



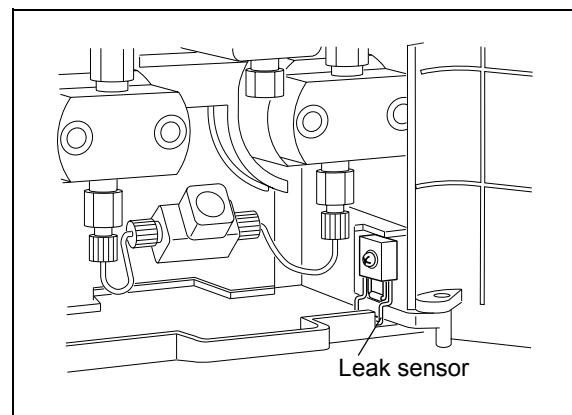


Fig. 5.1

- 3 Press **CE** to clear the result. If the result is [NO GOOD], adjust the detection level with [LEAK THR] function in the Calibration Support Group.  
 "Setting Operation Level of Leak Sensor [LEAK THR]" P. 5-39

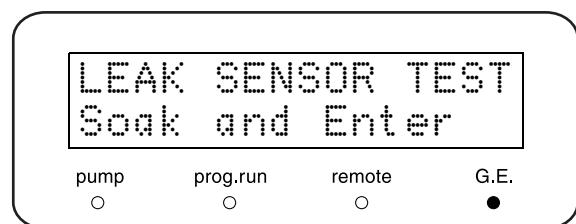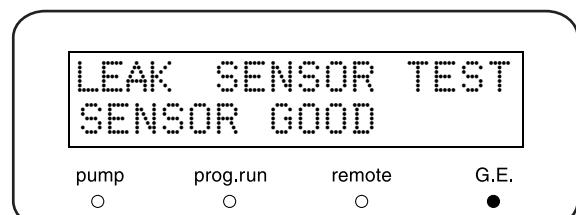

#### NOTE

After wetting and testing the leak sensor, wipe away the water on the leak tray completely.

 "8.10 Wiping of Leak Tray" P. 8-25


## 5. Application Operation

### 5.3.7 Calibration Support Group

This group calibrates the instrument.

#### NOTE

The instrument is adjusted before leaving the factory. Do not change values unnecessarily.

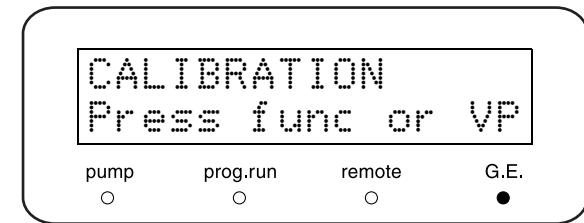


#### ■ Inputting Password [Input PASSWORD]

Password should be registered by a system manager.  
Input five numbers and press **enter**.

\* Be sure to input five numbers. The default password is [00000].

If the password is input correctly, [FLOW COMP FACT A] function (subsequent function) appears.

If the password is not input correctly, [FLOW COMP FACT A] cannot be accessed.

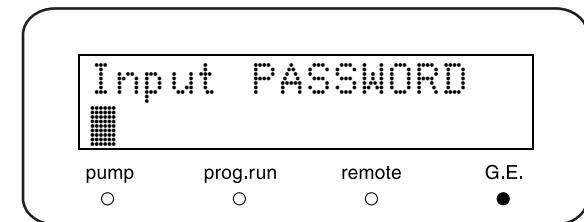


#### ■ Setting Flow Rate Compensation Parameter (ALPHA) [FLOW COMP FACT A/B]

Select either pump A or pump B by pressing **func** or **back**, enter the value, and press **enter**.

Reset if the flow rate is not accurate.

To increase the flow rate, enter the surplus value (additional flow rate to the original flow rate). To decrease the flow rate, enter the value of which should be decreased from the original value.

For example, to increase the parameter by 1.45% (because the current flow rate is 1.45% lower than the set rate) when the current setting value of the parameter is 5, enter  $5 + 1.45 = 6.45$ . This will increase the flow rate by 1.45%.

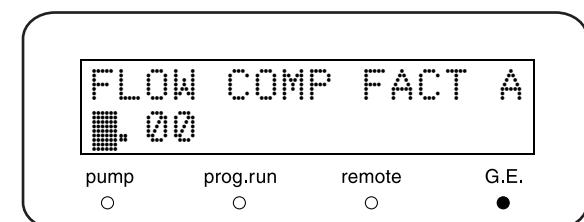


#### ■ Setting Pressure Sensor Sensitivity Compensation Factor [PRESS COMP FACT]

Enter the value and press **enter**.

Reset when the pressure sensor is replaced.

Enter the value as a multiple of 100 for PRS-1 (in [1:]) and PRS-5 (in [5:]) [XX.XX] shown in the data label of the pressure sensor.

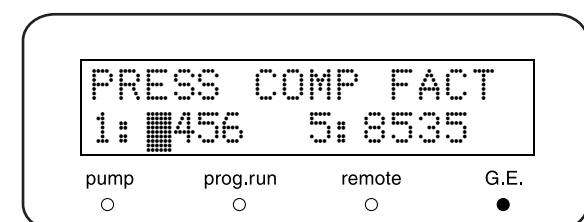


### ■ Setting Operation Level of Leak Sensor [LEAK THR]

Sets the level at which the leak sensor is actuated.

Enter the level and press **enter**.


Use this function to reset the level when the sensor fails  
[LEAK SENSOR TEST].

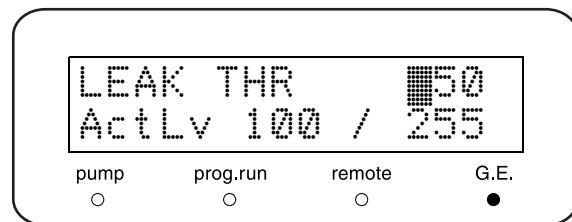

### ■ Setting Timing to replace Plunger Seal [SEAL REPLACEMENT]

Sets the timing to replace the plunger seal. (Unit:L)

Enter the set value by numeric keypad and press **enter**. It is recommended to replace seals after pumping 90L (equivalent to 1,500 hours at 1mL/min).

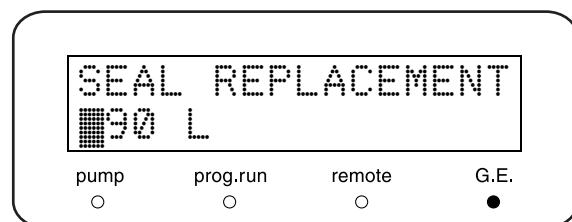


### ■ Selecting Operation Mode [OP MODE]

Select the operation mode according to the type of connected system controller.

Enter the number and press **enter**.


Set value	System controller
0	CBM-20A/20Alite
1	SCL-10Avp
2	SCL-10A

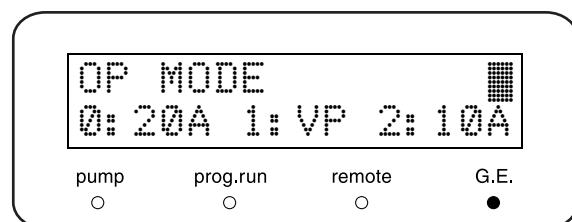

### ■ Initializing Parameters [INITIALIZE PARAM]

Initializes the parameters and deletes the time programs.


Press **enter** to return to the default value and to delete the time programs.

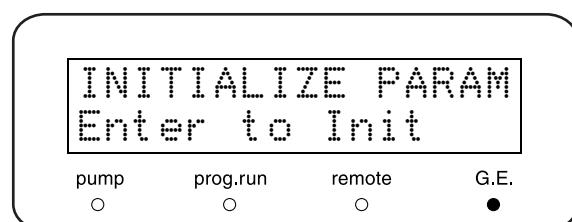

### ■ Changing Passwords [CHANGE PASSWORD]

1 Press **enter**.

Input screen appears.

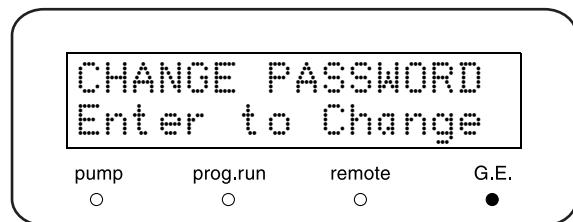

2 Input a new password and press **enter**.

The password must consist of five digits.




3 To confirm, input the same password again.



4 When the new password is registered,  
[PASSWORD CHANGED] appears.



If not, [PASSWORD WRONG] appears. In this case, the password newly entered is not registered.

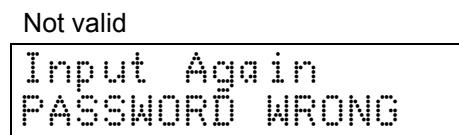

5 Press **enter** to return to the title screen.


### ■ Showing/Setting CBM Parameter [CBM PARAMETER]

Shows/sets parameters of CBM-20A/20Alite which controls the instrument.

Press **enter** to move to the CBM parameter setting screen.

To select the desired function, press **func** or **back** repeatedly.

To return to the title screen on the right, press **CE**.

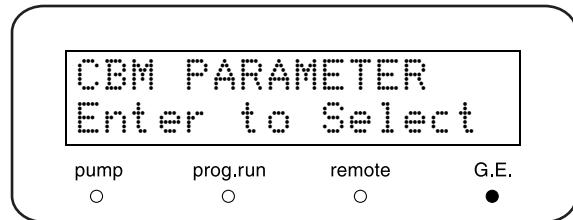

#### NOTE

When the instrument is not connected with CBM-20A/20Alite, or is set to local mode, the CBM parameter setting screen will not appear, even **enter** is pressed.

## List of CBM Parameters

SERIAL NUMBER	To show the serial No. of CBM
S/W ID	To show the program version No. of CBM
INTERFACE	To set the transmitting protocol to data processing unit
ETHERNET SPEED	To set the transmitting speed of ethernet *1
USE GATEWAY	To set usage of default gateway *1
IP ADDRESS	To set IP address of CBM *1
SUBNET MASK	To set subnet mask *1
DEFAULT GATEWAY	To set default gateway *1*2
TRS MODE	To select the communication destination when connecting to a LC workstation or a Chromatopac

\*1 Available only to show, when not allowed to change on CBM-20A/20Alite side.

\*2 Not available when [Default gateway] is not used.


### NOTE

Each parameter is activated after CBM is restarted.

Refer to CBM-20A/20Alite instruction manual for details of each parameter.


### Showing Serial No. [SERIAL NUMBER]

Shows the serial No. of CBM which controls the instrument.

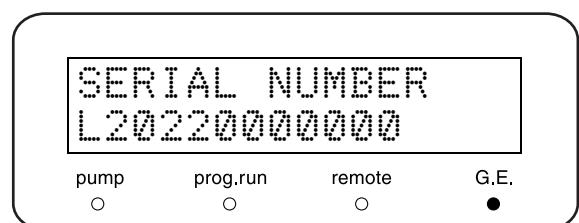

### Showing S/W Version No. [S/W ID]

Shows the name of software and version No. of CBM which controls the instrument.

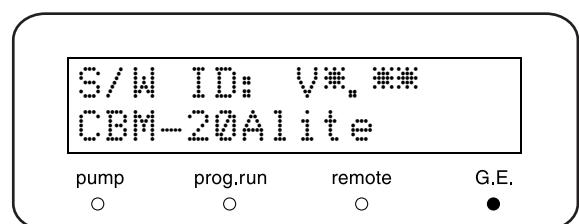


## 5. Application Operation

### Setting Transmitting Protocol to Data Processing Unit [INTERFACE]

Sets the transmitting protocol from CBM which controls the instrument to data processing unit.

Enter the value by numeric keypad and press **enter**.

Set Value	Transmitting Protocol
0	To connect with optical cable
1	To connect with serial transmission (RS-232C)
2	To connect with ethernet




### Setting Transmitting Speed of Ethernet [ETHERNET SPEED]

Sets transmitting speed of CBM ethernet which controls the instrument.

Enter the value by numeric keypad and press **enter**.

Set Value	Transmitting Speed
0	Auto Detect
1	10Mbps, Half Duplex
2	10Mbps, Full Duplex
3	100Mbps, Half Duplex
4	100Mbps, Full Duplex

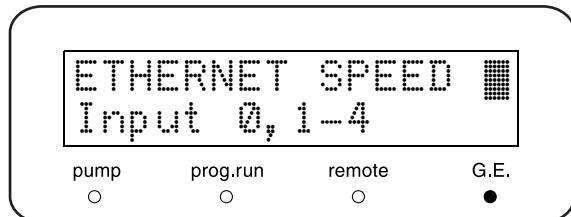


### Setting Usage of Default Gateway [USE GATEWAY]

Sets usage of default gateway of CBM which controls the instrument.

Enter the value and press **enter**.


Set Value	Default Gateway
0	Use
1	Not use

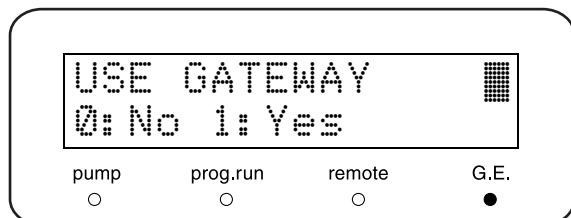

### Setting IP Address [IP ADDRESS]


Sets IP address of CBM which controls the instrument.

Enter the value and press **enter**.

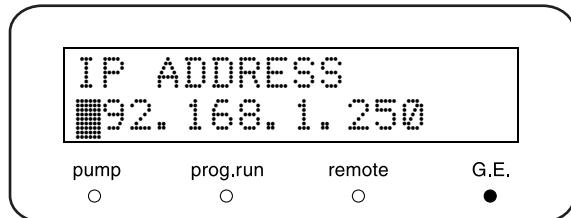


### Setting Subnet Mask [SUBNET MASK]

Sets subnet mask of CBM which controls the instrument.  
Enter the value by numeric keypad and press **enter**.




### Setting Default Gateway [DEFAULT GATEWAY]

Sets default gateway of CBM which controls the instrument.  
Enter the value by numeric keypad and press **enter**.

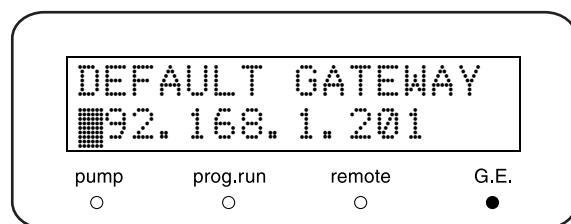

### Setting Serial Transmission [TRS MODE]

Selects the communication destination when CBM is connected to a LC workstation or a Chromatpac.  
Enter the value by numeric keypad and press **enter**.



Set Value	Remark
0	To connect in manual setting at CBM
2	To connect to CLASS-VP
3	To connect to LCsolution
11	To connect to C-R8A
12	To connect to C-R7A/C-R5A
13	To connect to C-R4A
14	To connect to C-R6A (without extended ROM board)
15	To connect to C-R6A (with extended ROM board)

#### NOTE

Value other than above are invalid.

# 5.4 Creating Time Program

Time programs can be used to execute commands (for flow rate, etc.) automatically at specified times during operation. Time programs are stored under file numbers (there are 10 files available). Before writing a program, check the file numbers already used. File numbers can be checked and specified using the [FILE NUM] auxiliary function in "File Number [FILE NUM]" P. 5-19.

## 5.4.1 Time Program Command

The commands for the time program are listed below.

Command	Description	Setting Range	Remark	Page
FLOW	To set flow rate	0 - 10.0000mL/min	Minimum setting unit: 0.0001mL/min	P.4-3
BCNC	To specify concentration of mobile phase B	0 - 100%	Minimum setting units: 0.1%	P.4-4
SV	To set opening/closing of the solenoid valves of FCV-10ALvp or FCV-11AL (S) (Optional)	0, 1, 2, 3, 4 0 - 123 *1	Refer to *1	P.5-16
EVENT	To set ON/OFF for EVENT output (of relay contacts at back of the instrument)	0, 1, 2, 12	One of 4 values (For details, <a href="#">P.5-17</a> .)	P.5-17
LOOP	To repeat program	0 - 255 Setting 0 will repeat the program 256 times.	Minimum setting units: 1	P.5-52
STOP	To stop program	N/A		P.5-52
GOTO	To switch to other programs (up to 10)	0 - 9		P.5-53

\*1:If FCV-10ALvp is set for the [FCV TYPE] parameter, the setting range is 1, 2, 3, 4. If FCV-11AL (S) is set, the range is 0-123, using combinations of 0, 1, 2 & 3.


 "Selecting Flow Channel Valve Type [FCV TYPE]" P. 5-23

### 5.4.2 Description of Time Program Screen

To create a time program, access the edit screen as described below.

**1** Press **CE**.

Initial screen appears.

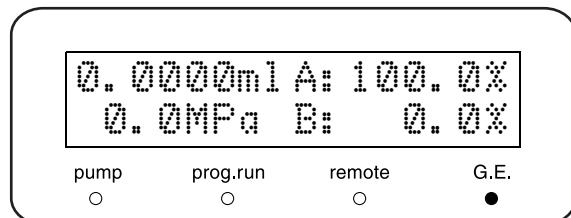


**2** Press **edit**.

The screen appears as shown on the right.

- ① Number of steps already created
- ② Number of remaining steps

This example shows that 10 steps of time program have been set, and that 310 steps remain.

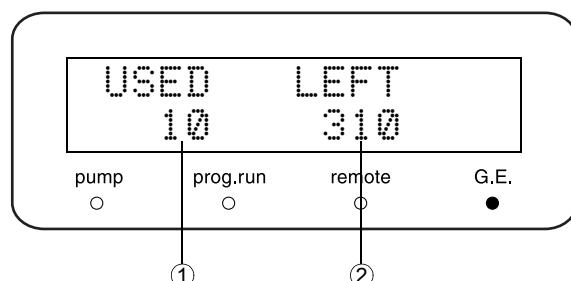


**3** Press **enter**.

Editing screen appears.

- ① Elapsed time from program start (minutes)
- ② Command
- ③ Set value

For the following programming procedure, refer to the "5.4.3 Time Program Creating Flow" P. 5-46.

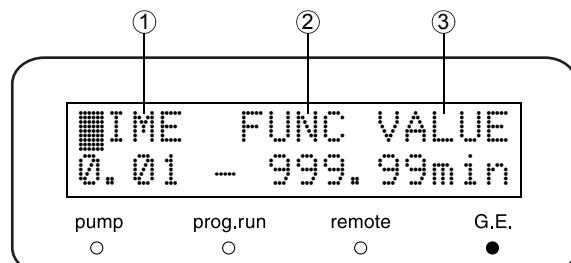

### 5.4.3 Time Program Creating Flow

In this section, the creating procedure of time programs are shown in the following flow diagrams.

Initial screen

0.0000ml A: 100.0%  
0.0MPa B: 0.0%

**edit** ↓ ↑ **CE**

USED	LEFT
0	320

**enter**

Input the time

TIME FUNC VALUE  
0.01 - 999.99min

**CE**

**enter**

Press **func** to select the command.

5.00 FLOW  
0.0 - 10.0000 mL

**CE**

**enter**

Input the Value (except for STOP)

5.00 FLOW VALUE  
0.0 - 10.0000 mL

**CE**

**enter**

Input Stored

5.00 FLOW4.0000  
0.01 - 999.99min

**CE**

Make settings for the next one.

\* The displayed screen is the one set previously.

\* To return to the previous step, press **back**.

#### 5.4.4 Creating Time Program

The following example gives the steps to create a time program to change the flow rate automatically as shown on the right. (initial flow rate : 1mL/min)

Step	TIME (min)	FUNC	VALUE (mL/min)
1	15.00	FLOW	2.0000
2	20.00	FLOW	5.0000
3	30.00	STOP	



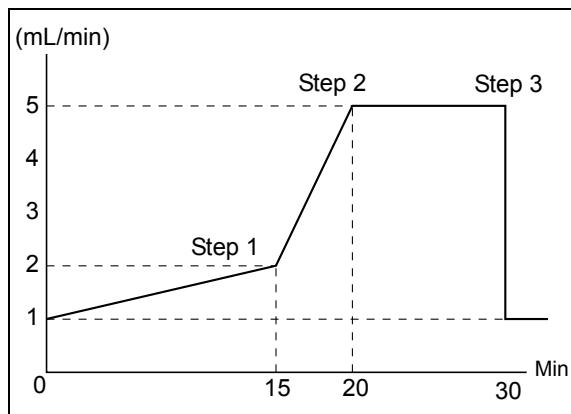


Fig. 5.2


- 1 Press **CE**.  
Initial screen appears.

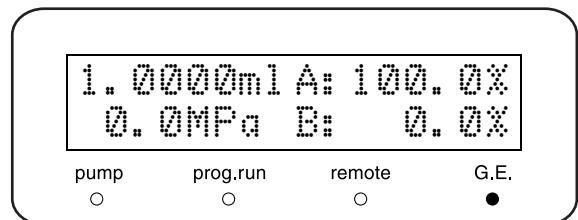

- 2 Press **edit**.  
The number of steps already created and remaining steps appear.

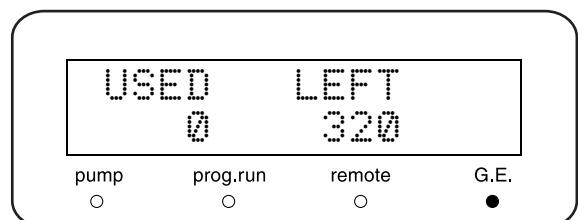

- 3 Press **enter**.  
The setting screen appears.

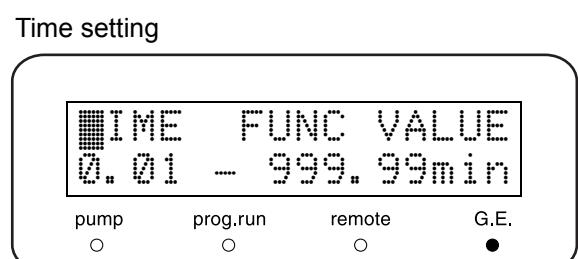


## 5. Application Operation

### Step 1


- 4 Press **1**, **5** and **enter**.

Select of command

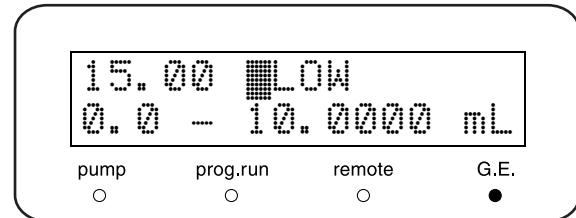


- 5 Press **func** repeatedly until [FLOW] appears.

Input the value of the command (Flow rate)

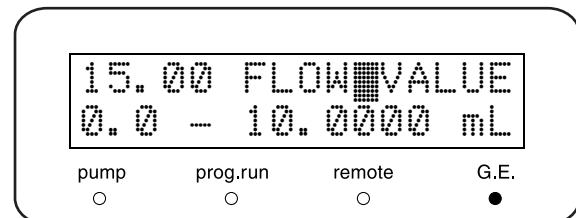

- 6 Press **enter**.


Determination of step 1

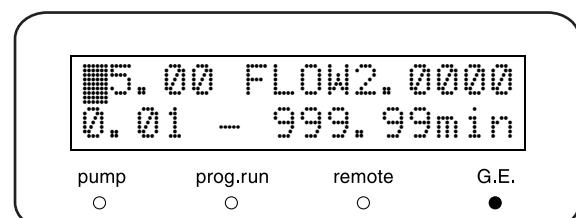

### Step 2

- 8 Press **2**, **0** and **enter** to enter the time.  
Press **enter** to select [FLOW].  
Press **5** and **enter** to enter the flow rate.


Determination of step 2

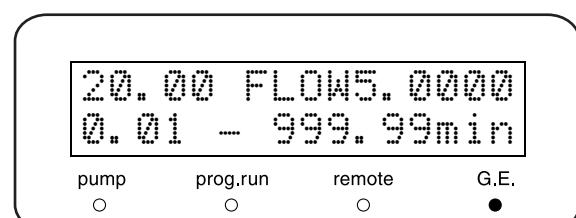

### Step 3

- 9 Press **3**, **0** and **enter**.

Select of command

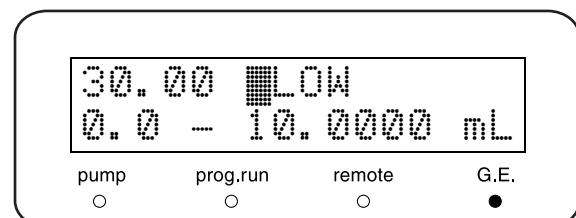


**10** Press **func** repeatedly until [STOP] appears.

Determination of step 3



**11** Press **enter**.



**12** Press **CE** to complete creating program.  
3-step time program has created.

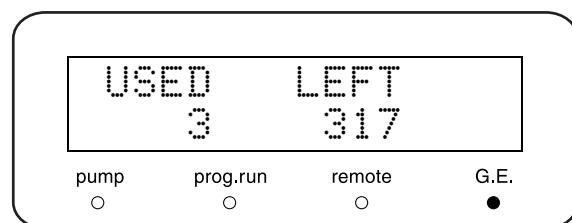

**13** Press **CE** to save the time program.  
Initial screen of step 1 appears.

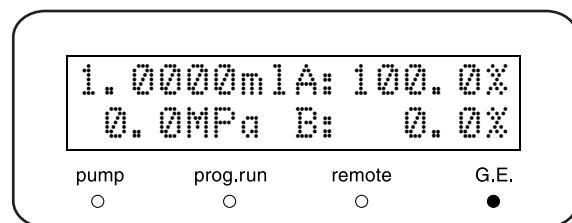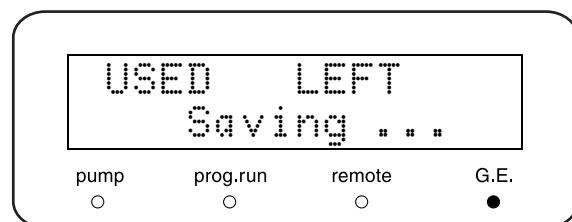

**NOTE**

When setting several steps, they are ordered automatically in sequence.

## 5. Application Operation

### 5.4.5 Creating High-Pressure Gradient Programs


[BCNC] command of time programs can be used to specify particular concentration of mobile phase B (and thereby concentration of mobile phase A also) at particular times during operation. Concentration of mobile phase A is determined relative to Concentration of mobile phase B as follows:

$$\text{Concentration of mobile phase A (\%)} = 100 (\%) - \text{Concentration of mobile phase B [BCNC] (\%)}$$

The value of [BCNC] command can be set to any concentration between 0 and 100%.

Minimum setting unit is 0.1%.

- 1 Enter the time program edit mode.  
 "5.4 Creating Time Program" P. 5-44
- 2 Enter the time.
- 3 Press **func** repeatedly until [BCNC] appears.
- 4 Enter the concentration and press **enter**.

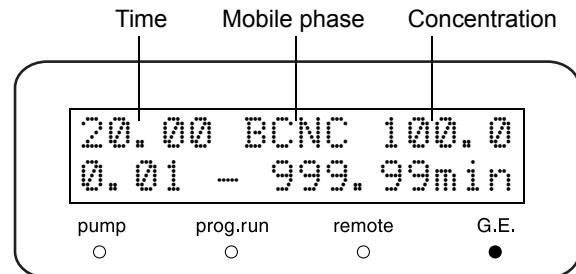

As an example of creating a high-pressure gradient program, changing the concentration of mobile phase B is shown at right. (The initial value is 0.0%.)

Step	TIME (min)	FUNC	VALUE (%)
①	20.00	BCNC	100.0
②	30.00	BCNC	100.0
③	30.01	BCNC	0.0
④	40.00	STOP	

 "5.4.4 Creating Time Program" P. 5-47

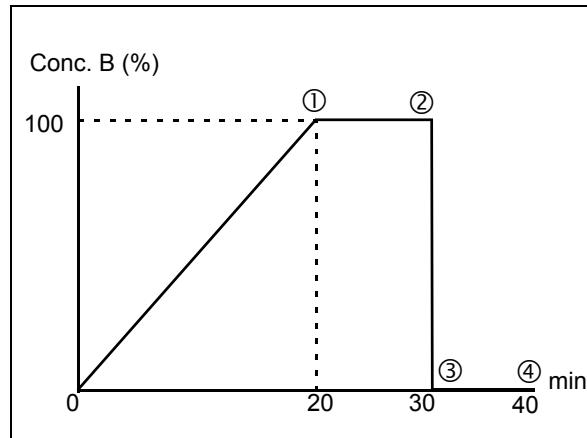


Fig. 5.3

### 5.4.6 Deleting Steps


Call up the steps and press **del**.

An example to delete the step 1 of the program set in "5.4.4 Creating Time Program" P. 5-47 is shown as follows:

**1** Show the step to be deleted.


To display the step, follow the same procedure as creating the programs.

- \* To delete a subsequent step, press **enter** repeatedly until the step appears.

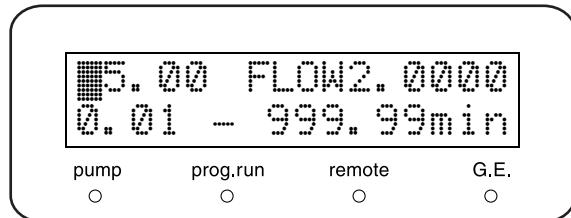

**2** Press **del**.

Step 1 will be deleted, and the subsequent step appears.

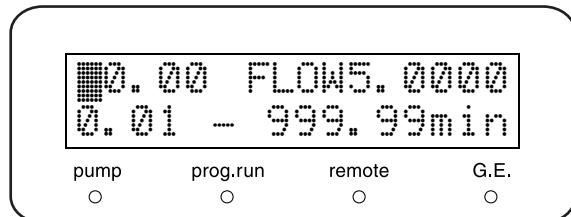

### 5.4.7 Starting and Stopping a Time Program

#### ■ Starting a Time Program

To start a time program, proceed as follows:

Press **run** to start the time program.


[prog.run] indicator illuminates.

#### ■ Stopping a Time Program

There are two ways to stop the time program:

- Press **run** to stop the running program forcefully.  
The [prog.run] indicator goes out.
- Insert [STOP] command of the program.

☞ "5.4.8 Commands Used Only For Time Program" P. 5-52

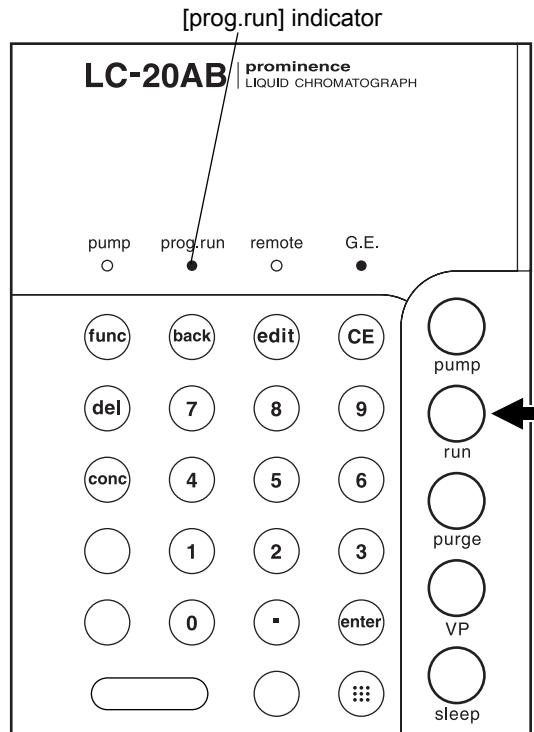


### 5.4.8 Commands Used Only For Time Program

This section describes the commands used only for the time program.

#### ■ Setting Stop Command of Time Program [STOP]

Sets the time when the time program will stop. Enter the time in the last step of time program, and press **func** until [STOP] appears. Enter **enter**, [STOP] command will be set.

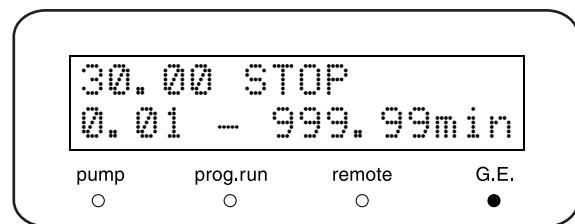

#### NOTE


In the following cases, do not set [STOP] command at the end of the program.

- ① Operating a time program endlessly.
- ② Coupling on program files by the [GOTO] command.

 "Switching File [GOTO]" P. 5-53

#### ■ Setting Loop Count of Time Program [LOOP]

[LOOP] function can register the loop count of time program.

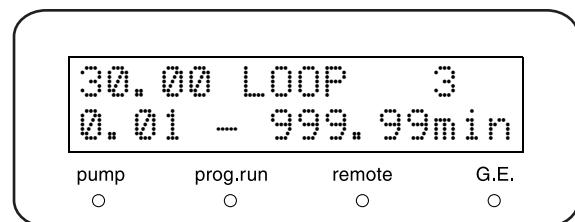

Set as right table for example. Step ① and ② will be repeated three times in 30 minutes interval.

Step	TIME (min)	FUNC	VALUE (mL/min)
①	15.00	FLOW	2.0000
②	20.00	FLOW	5.0000
③	30.00	LOOP	3

#### NOTE

- After the time program is repeated as set for [LOOP], how the time program will automatically stop depends on whether [GOTO] command following [LOOP] has been entered or not as follows.

##### With [GOTO] command:

Until the time set for [GOTO] command is reached, time program maintain the setting values when [LOOP] is ended, and then the next time program starts.

##### Without [GOTO] command:

The time program will stop when [LOOP] has finished.


- Steps set after [LOOP] command will deactivate except for [GOTO] command.
- Value of [LOOP] command can be set to 255. When [0] is set, time program will be repeated 256 times.

## ■ Switching File [GOTO]

[GOTO] command switches the specified file.

When [GOTO] command switches the file, the initial screen of the file newly called up appears, and the instrument waits in standby. However, the program can set to start automatically after [GOTO] command is completed. Follow steps 1 to 6 to set [GOTO] command to start automatically.

Enter the program No. to be switched to.

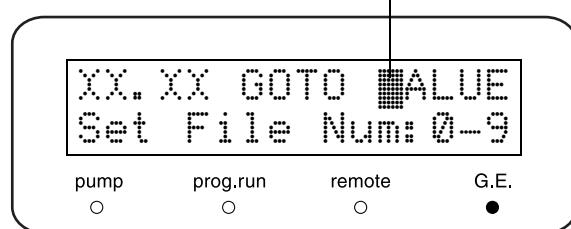

- 1 Insert the event cable into the external input/output terminal.

"5.7.2 Connection of Event Cable" P. 5-57


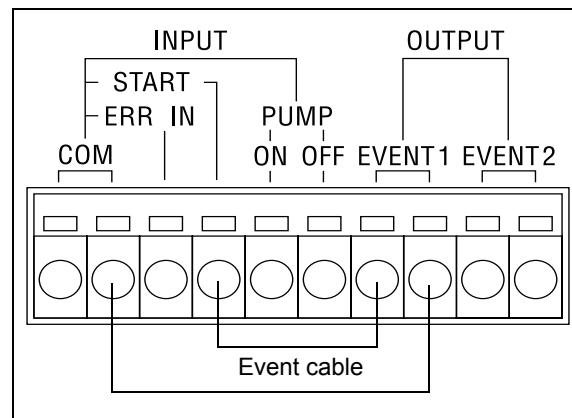


Fig. 5.4

- 2 Add the following step to the original time program.


- ① Set a time earlier than [GOTO] command.
- ② Show [EVENT].
- ③ Set [0].

- 3 Press **CE** to complete the time program.

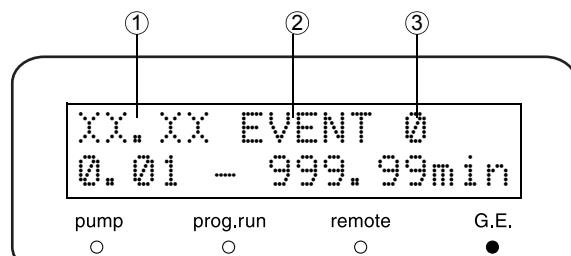


- 4 Change the file number into the one newly called up.

"File Number [FILE NUM]" P. 5-19



- 5 Set the EVENT output terminal of the newly called up file specified in step 4 as [1].

"Setting EVENT Output Terminals [EVENT]" P. 5-17

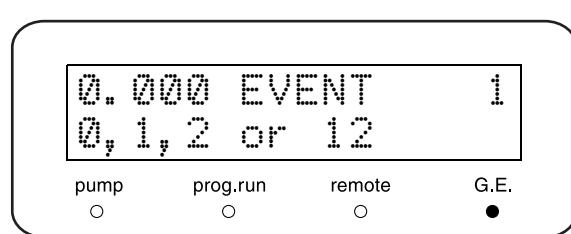

- 6 Set the file number back to the original file number.

"File Number [FILE NUM]" P. 5-19

# 5.5 Control by CBM-20A or CBM-20Alite System Controller

## 5.5.1 Preparation

To control the instrument by the CBM-20A or CBM-20Alite system controller, set the parameters as follows:

Command	Set Value	References
LOCAL	0 : Remote	 "Selecting Local/Remote Mode [LOCAL]" P. 5-21
ADRS	Link address	 "Setting Link Address [ADRS]" P. 5-21
OP MODE	0 : 20A	 "Selecting Operation Mode [OP MODE]" P. 5-39

## 5.5.2 Basic Parameters

A max. of four pump units can be connected to a CBM-20A/20Alite. CBM-20A/20Alite can set flow rate, concentration of mobile phase B, maximum pressure limit, minimum pressure limit, solenoid valves, pumping ON/OFF, time program, etc. and control binary high-pressure gradient. Also by combining the SIL-20A autosampler, auto purging function is available. Refer to the CBM-20A/20Alite instruction manual.

# 5.6 Control by SCL-10Avp or SCL-10A System Controller

## 5.6.1 Preparation

To control the instrument by the SCL-10Avp or SCL-10A system controller, set the parameters as follows:

Command	Set Value	References
LOCAL	0 : Remote	 "Selecting Local/Remote Mode [LOCAL]" P. 5-21
ADRS	Link address	 "Setting Link Address [ADRS]" P. 5-21
OP MODE	1 : VP * <sup>1</sup> 2 : 10A* <sup>2</sup>	 "Selecting Operation Mode [OP MODE]" P. 5-39

\*1 To connect to SCL-10Avp : the instrument is recognized as LC-10ADvp.

\*2 To connect to SCL-10A : the instrument is recognized as LC-10AD.

5

## 5.6.2 Basic Parameters

A max.of three pump units can be connected to a SCL-10Avp or SCL-10A. SCL-10Avp/SCL-10A can set flow rate, maximum pressure limit, minimum pressure limit, solenoid valves, pumping ON/OFF, time program, etc. and control binary high-pressure gradient. Refer to the SCL-10Avp/SCL-10A instruction manual.

## 5.6.3 Attention

When the instrument is connected to a SCL-10Avp or SCL-10A, the instrument will work in compatibility mode for LC-10ADvp or LC-10AD. In this case, the following applies.

- 1) Maximum limit of flow rate is 9.999mL/min and is set in steps of 0.001mL/min.
- 2) Maximum value of [p.max] is 43.2MPa.
- 3) Constant-pressure delivery is not supported.
- 4) Delivery modes:

Connect the instrument as [PUMP.A] and set the system controller's delivery mode to quaternary low-pressure gradient ([LP.GE]). The instrument's binary high-pressure gradient function can be controlled from the system controller by setting the flow rate [T.FLOW] and the concentration of mobile phase B [B.CONC] respectively.

For connecting the instrument to a system controller and setting parameters, refer to the System Controller' instruction manual.

### NOTE

- Set the concentration of mobile phase C and D ([C.CONC] and [D.CONC]) to 0.0%.
- If the instrument is not connected as [PUMP.A], or if the system controller's delivery mode is not set to [LP.GE] (i.e., set to [ISO.], [B.GE], or [T.GE]), the concentration of the mobile phase B at the instrument will not be controlled from the system controller. A mixture of the two liquids will be delivered at the concentration of mobile phase B set directly at the instrument.

# 5.7 Connection to External Input/Output Terminals

The external input/output terminals are connected to a event output device or other external devices with a provided event cable.

Details of the terminal and wiring are described as follows.

## ⚠ WARNING

- Before connecting the cable, turn off the power and unplug the instrument.
- Use only the specified cable.
- Connect as specified.

Otherwise, fire, electric shock or malfunction may occur.

### 5.7.1 External Input/Output Terminals

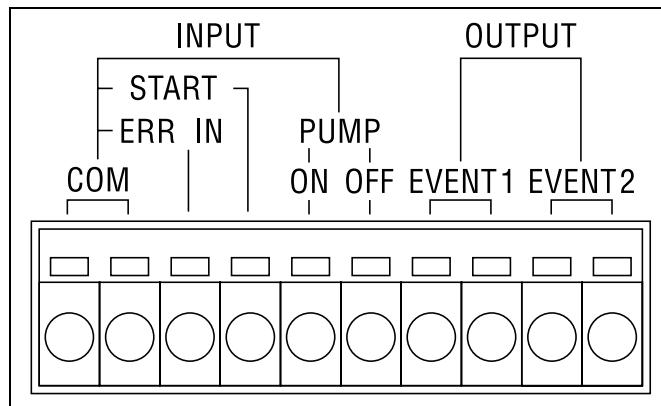


Fig. 5.5

Signals	Description	Remark
EVENT1	[Event1/2] output terminals. To connect to relay and be turned ON/OFF according to a time program or the [EVENT] value of auxiliary function.	Contact rating: 30VDC/1A
PUMP ON	[PUMP ON] input terminal. To start pumping.	These signals are implemented by shorting the appropriate wire pair between the input command terminal and the common terminal. Duration of shorting (tc) should be as follows. 0.5 sec < tc < 10 sec.
PUMP OFF	[PUMP OFF] input terminal. To stop pumping.	
START	[START] input terminal. To start the time program. When a start signal is received while program is running, time program is restarted from time [0].	
ERR IN	Error input terminal. To detect error.	
COM	Common terminal for [PUMP ON], [PUMP OFF], [START], and [ERR IN].	

### 5.7.2 Connection of Event Cable

**1** Peel the cable about 10mm.

It is not necessary for provided event cable.

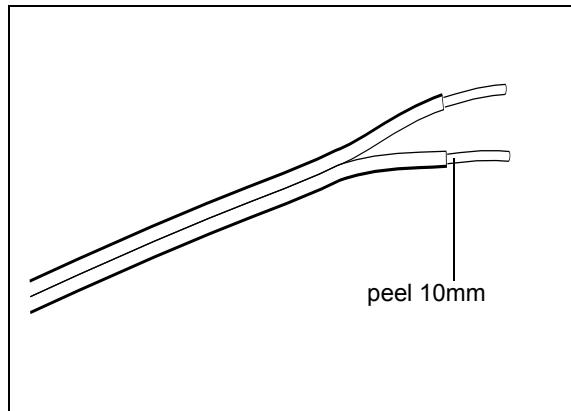


Fig. 5.6

**2** Insert the cable.

When the cable has the single core wire, just insert the cable.

When the cable has the stranded wires, strand the wires enough and insert with pressing the button of the terminal.

When removing the cable, remove the cable by pressing the button of the terminal.

#### NOTE

The instrument provides one event cable. When more than 2 cables are required, use the following cables.

- Cable with single wire :  $\phi$  0.4 to  $\phi$  1.2 (AWG26 to 16)
- Cable with stranded wire :  $0.3\text{mm}^2$  to  $1.25\text{mm}^2$  (AWG22 to 16), diameter of single wire thicker than  $\phi$  0.18.



The cable with stranded wire is suitable to prevent disconnection.

#### NOTE

If [EVENT1] or [EVENT2] signal is used, set [EVENT] and [EXT-S] parameters.

"Setting EVENT Output Terminals [EVENT]" P. 5-17

"External Signal Functions for EVENT Output Terminals [EXT-S]" P. 5-22

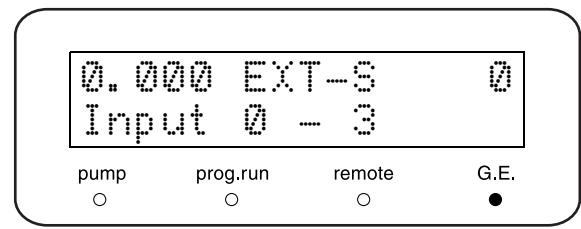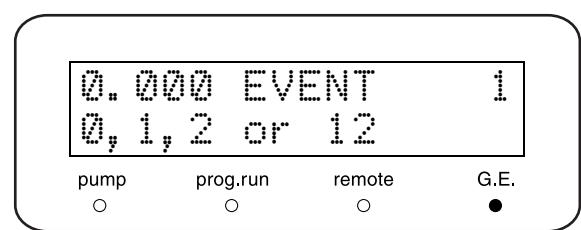

This page is intentionally left blank.

# 6

---

## Troubleshooting

### Contents

6.1	Troubleshooting and Corrective Action .....	6-2
6.2	Error Message.....	6-5

# 6.1 Troubleshooting and Corrective Action

This section describes the probable causes of problems that can arise, and the corrective action to be taken to eliminate the causes. For more detailed procedures, refer to the indicated page.

If the problem cannot be resolved even after taking the indicated measures, or if there are problems not included in the following tables, contact your Shimadzu representative.

Symptom	Probable Cause	Corrective Action	Page
Power does not turn ON even after switching ON power.	Power plug is disconnected.	<ul style="list-style-type: none"> <li>Connect plug correctly.</li> </ul>	P.9-5
	Power cord internal wires are cut.	<ul style="list-style-type: none"> <li>Replace with a new cord of the same type.</li> </ul>	P.1-3
	Power supply does not meet specifications for this instrument.	<ul style="list-style-type: none"> <li>Use power supply that meets specifications for this instrument.</li> </ul>	P.9-4
	Fuse is blown.	<ul style="list-style-type: none"> <li>Replace the fuse.</li> </ul>	P.8-24
Key operation is not possible.	( was not pressed.)	<ul style="list-style-type: none"> <li>Press ().</li> </ul> <p>Operation keys are shown to operate.</p>	P.2-8
No liquid is pumped. (The instrument does not run.)	was not pressed. (Pump indicator does not illuminate.)	<ul style="list-style-type: none"> <li>Press ().</li> </ul> <p>The pump indicator will illuminate.</p>	P.4-5
		<ul style="list-style-type: none"> <li>Have the system controller send a signal to start pumping.</li> </ul>	*1
	Flow rate is set to [0].	<ul style="list-style-type: none"> <li>Set a flow rate other than 0.</li> </ul>	P.4-3
		<ul style="list-style-type: none"> <li>Have the system controller set a flow rate.</li> </ul>	*1
	Error message (P.MAX, P.MIN etc.) appears.	<ul style="list-style-type: none"> <li>Press () to clear the message and make corrective action for errors.</li> </ul>	P.6-5
The instrument is running, but no liquid is pumped.	Air bubbles are generated inside pump head.	<ul style="list-style-type: none"> <li>Press () to purge out the bubbles.</li> <li>Insert the disposable syringe into the drain tubing outlet and draw out the bubbles.</li> </ul>	P.3-7
	Air bubbles are produced through suction filter and pump inlet.	<ul style="list-style-type: none"> <li>Make sure that the filter bushing is tightly fitted.</li> </ul>	P.9-13
	Check valve is not working properly.	<ul style="list-style-type: none"> <li>Push in 2-propanol etc. from the Inlet check valve.*2</li> </ul>	

\*1:Refer to the system controller instruction manual for details.

\*2:How to push in solvent

Unplug the PTFE tubing connected to the Inlet check valve. Attach the provided stop joint D to this unplugged PTFE tubing. Connect the provided syringe tubing D to the Inlet check valve and push in 2-propanol etc.

\*3:How to check clogging of filter

Take off the filter part of the suction filter and record a pressure waveform.

If the pressure waveform becomes ideal by taking off the filter, that suction filter is clogged.

Symptom	Probable Cause	Corrective Action	Page
Pumping is unstable, with large pump pulsation.	Air bubbles are generated inside pump head.	<ul style="list-style-type: none"> <li>Press <b>(purge)</b> to purge out the bubbles.</li> <li>Insert the disposable syringe into the drain tubing outlet and draw out the bubbles.</li> </ul>	P.3-7
	Previous mobile phase is still remaining inside pump head.	<ul style="list-style-type: none"> <li>Press <b>(purge)</b>, and thoroughly purge the old mobile phase.</li> </ul>	
	Air bubbles are generated in filter tubing.	<ul style="list-style-type: none"> <li>Press <b>(purge)</b>, and thoroughly purge the old mobile phase.</li> <li>Shake the suction filter to drive out the bubbles.</li> </ul>	
		<ul style="list-style-type: none"> <li>If the suction filter is clogged, clean it in an ultrasonic bath, Otherwise, replace it.*3</li> </ul>	P.8-21
		<ul style="list-style-type: none"> <li>Degas the mobile phase.</li> </ul>	P.1-5
	Check valve is not working properly.	<ul style="list-style-type: none"> <li>Push in 2-propanol etc. from the Inlet check valve.*2</li> <li>Pump 2-propanol to clean check valve.</li> </ul>	P.8-15
		<ul style="list-style-type: none"> <li>If cleaning check valve is not effective, clean the valve in an ultrasonic bath or replace it.</li> </ul>	P.8-16
	Liquid is leaking from gap between pump head and head holder, or from rinse flow lines.	<ul style="list-style-type: none"> <li>Replace the plunger seal.</li> <li>Replace the plunger seal. Otherwise, replace the plunger.</li> </ul>	P.8-5 P.8-10
	Liquid is leaking from flow line connection.	<ul style="list-style-type: none"> <li>Retighten the male nuts.</li> <li>Retighten the male nuts. Otherwise, replace the nuts and ferrules.</li> </ul>	P.9-6
	Flow line is (partially) clogged.	<ul style="list-style-type: none"> <li>Clean the line filter in an ultrasonic bath or replace it.</li> <li>Identify the clogged parts and replace it.</li> </ul>	P.8-19
	Plunger seals wear out too quickly.	<ul style="list-style-type: none"> <li>Replace plunger.</li> </ul>	P.8-10
Pumping is unstable, with large pump pulsation at low flow rate of 50µl/min or less.	Check valve is not working properly.*4	<ul style="list-style-type: none"> <li>Pump 2-propanol to clean check valve.</li> <li>If cleaning check valve is not effective, clean the valve in an ultrasonic bath or replace it.</li> </ul>	P.8-15 P.8-16

\*4:NOTE (Pumping at low flow rate of 50µl/min or less)

Take care not to pump at high flow rate and high pressure (approx. 3ml/min (20MPa) or more) before pumping at low flow rate of 50µl/min or less.

(Pumping may be unstable because of the seal wearing.)

## 6. Troubleshooting

---

Symptom	Probable Cause	Corrective Action	Page
Flow rate is below set value.	Check valve does not work properly.	<ul style="list-style-type: none"> <li>Pump 2-propanol to clean check valve.</li> </ul>	P.8-15
		<ul style="list-style-type: none"> <li>Pump 2-propanol to clean check valve. Otherwise, clean the valve in an ultrasonic bath or replace it.</li> </ul>	P.8-16
	Suction filter is clogged.*3	<ul style="list-style-type: none"> <li>Clean Suction filter in an ultrasonic bath. Otherwise, replace it.</li> </ul>	P.8-21
Retention time cannot be reproduced.	Check valve does not work properly.	<ul style="list-style-type: none"> <li>Pump 2-propanol to clean check valve.</li> </ul>	P.8-15
		<ul style="list-style-type: none"> <li>If cleaning check valve is not effective, replace the valve or clean it in an ultrasonic bath.</li> </ul>	P.8-16
Pressure does not rise.	Drain valve open.	<ul style="list-style-type: none"> <li>Close drain valve.</li> </ul>	P.2-2
	Liquid is leaking from flow line connections.	<ul style="list-style-type: none"> <li>Retighten the male nuts. Otherwise, replace the nuts and ferrules.</li> </ul>	P.9-8
Pressure rises too much. (Remove the column to check.)	Line filter is clogged.	<ul style="list-style-type: none"> <li>Clean the line filter in an ultrasonic bath or replace it.</li> </ul>	P.8-19
	Flow lines are clogged.	<ul style="list-style-type: none"> <li>Identify the clogged parts and replace them.</li> </ul>	
	Inner diameter of tubings is too small.	<ul style="list-style-type: none"> <li>Use tubings with the specified inner diameter.</li> </ul>	
The volume of the automatic rinsing kit's rinse solution increases.	Liquid is leaking from the gap between a pump head and a head holder, or from a rinse-solution outlet.	<ul style="list-style-type: none"> <li>Replace the plunger seal.</li> <li>If liquid is still leaking after replacing the plunger seal, replace the plunger.</li> </ul>	P.8-5
The volume of the automatic rinsing kit's rinse solution decreases.	Liquid is leaking from the gap between a pump head and a head holder, or from a rinse-solution outlet.	<ul style="list-style-type: none"> <li>Inspect (or replace) the diaphragm.</li> </ul>	P.8-10

\*3:How to check clogging of filter

Take off the filter part of the suction filter and record a pressure waveform.

If the pressure waveform improves by taking off the filter, that suction filter is clogged.

# 6.2 Error Message

The instrument has several diagnostic functions. Upon detection of a problem, an alarm sounds and an error message appears on the display panel.

The following list describes the error messages along with the causes and corrective actions.

**NOTE**


Each message is classified into the following three types.

The type is indicated under the type column.

Fatal: The instrument stops operation.  
Pressing **CE** will not clear the error message.

Alarm: The instrument stops operation.  
Press **CE** to clear the error message.

Warning: The instrument does not stop operation.  
Press **CE** to clear the error message.

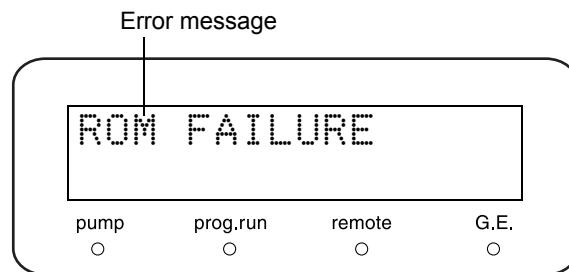

6

Error Message	Type	Cause and Action
MAIN ROM FAILURE	Fatal	Cause: ROM error (electric failure) Action: Turn power OFF and contact your Shimadzu representative.
SUB ROM FAILURE (ROM error)	Fatal	Cause: RAM error (electric failure) Action: Turn power OFF and contact your Shimadzu representative.
RAM FAILURE (RAM error)	Fatal	Cause: Interior temperature has risen to an abnormal level. Action: Check to be sure that the internal fan can move, and that the rear exhaust vent is not blocked. If this message still appears, turn the power OFF and contact your Shimadzu representative.
A-B TRANS ERROR (A-B transmission error)	Fatal	Cause: A transmission error has occurred between pumps A and B. Action: Turn power OFF and contact your Shimadzu representative.

## 6. Troubleshooting

---

Error Message	Type	Cause and Action
<b>OUT OF MAXSTEPS</b> (Max. number of steps exceeded)	Alarm	<p>Cause: More than 320 steps of time program have been set.</p> <p>Action: Delete unnecessary programs.</p> <p> <a href="#">"5.4 Creating Time Program" P. 5-44</a></p>
<b>ERROR P-MAX</b> (Max. pressure limit error)	Alarm	<p>Cause: Pump discharge pressure has exceeded the set max. pressure limit, [P.MAX]. Pumping will automatically stop, unless [S-PROT] function has been activated, in which case pumping will continue at half flow rate.</p> <p> <a href="#">"Setting System Protection [S-PROT]" P. 5-22</a></p> <p>Action: Inspect the clogging in the flow line. If no clogging is found, set the appropriate [P.MAX] value.</p> <p> <a href="#">"Setting Maximum Pressure Limit [P.MAX]" P. 5-15</a></p>
<b>ERROR P-MIN</b> (Min. pressure limit error)	Alarm	<p>Cause: Pump discharge pressure has fallen below the set min. pressure limit, [P.MIN]. Pumping will automatically stop.</p> <p>Action: Inspect the leakage in the flow line. If no leakage is found, set the appropriate P.MIN value. Note that [P.MIN] function is not activated for first one minute of pumping.</p> <p> <a href="#">"Setting Minimum Pressure Limit [P.MIN]" P. 5-15</a></p>
<b>ERROR A-HOME POS</b>	Alarm	<p>Cause: Pump A's (or pump B's) motor home position cannot be detected, the motor does not run, or the motor is slipping.</p>
<b>ERROR B-HOME POS</b> (Home position error)		<p>Action: Turn the power OFF and ON again, and press <b>pump</b>. If this message still appears, turn the power OFF and contact your Shimadzu representative.</p>
<b>OPEN DRAIN VALVE</b> (Purge error)	Alarm	<p>Cause: Pump discharge pressure has exceeded [P-PMAX] during purging.</p> <p>Action: Open the drain valve before pressing <b>purge</b>. If an error message appears during auto-purging by system controller, inspect the clogging in the flow line. If no clogging is found, set the appropriate [P-FLOW] and [P-PMAX] value.</p> <p> <a href="#">"Setting Purge Flow Rate [P-FLOW]" P. 5-18</a></p> <p> <a href="#">"Setting Maximum Pressure Limit during Purging [P-PMAX]" P. 5-18</a></p> <p> <a href="#">"5.5 Control by CBM-20A or CBM-20Alite System Controller" P. 5-54</a></p>

Error Message	Type	Cause and Action
<b>ERROR LEAK</b> (Leak error)	Alarm	Cause: Leak sensor has detected leakage. Action: Inspect the leakage in the flow line. Wipe away any liquid around the leak sensor.
<b>ERROR EXTERNAL</b> (External equipment error)	Alarm	Cause: An error signal was sent from the external device connected to the external input/output terminal [ERR IN]. Action: Inspect the external device, and eliminate the cause of the error.
<b>WARN : M. PHASE-A</b>	Warning	Cause: The remaining volume of pump A's (or pump B's) mobile phase is less than the alarm level. Action: Replace pump A's (or pump B's) mobile phase and reset the amount.  "Showing/Setting Mobile Phase Volume [MOBILE PHASE A/B]" P. 5-30
<b>WARN : M. PHASE-B</b> (Mobile phase alarm)		
<b>WARN : DEGAS PRS</b> (Degasser vacuum pressure error)	Warning	Cause: Vacuum pressure of degasser (DGU-20A) connected to this instrument has been abnormal for a certain time. Action: Check the vacuum pressure of degasser. If the vacuum pressure is [NG], turn the power OFF once and turn it ON again. If the vacuum pressure is [OK], it is of no matter, for the degasser is returning to run automatically.  "Monitoring Vacuum Pressure in Degasser Unit [DEGAS PRS]" P. 5-26

## 6. Troubleshooting

---

This page is intentionally left blank.

# 7

---

## Hardware Validation

This chapter provides instruction on hardware validation, which verifies the performance of individual components and the instrument as a whole.

### Contents

7.1	Overview of Hardware Validation.....	7-2
7.2	Implementation of Hardware Validation .....	7-3
7.3	Validation Precautions .....	7-4
7.4	Equipment Required for Validation .....	7-5
7.5	Validation: Pump .....	7-7
7.6	Validation: Gradient Pump System .....	7-19
7.7	System Validation .....	7-23
7.8	If Validation Fails.....	7-31

# 7.1 Overview of Hardware Validation

---

## 7.1.1 Hardware Validation

---


Hardware validation examines whether the LC system runs correctly and the instrument is suitable for the intended analysis. Validation is performed through LC system Installation, Operation and Performance Qualifications followed by periodic inspections. The performance of the LC system deteriorates with age, reflecting the wear of consumable parts. Hardware validation must therefore be performed periodically from the time of installation until the system is retired. Although validation aspects related to analysis, such as method validation and system suitability tests should also be performed, hardware validation is a prerequisite for these items.

---

## 7.1.2 Types of Hardware Validation

---

A High Performance Liquid Chromatograph consists of several LC components such as pump(s), autosampler, column oven, and detector(s). For this reason, hardware validation is divided into the inspection of individual components and system validation as a whole.

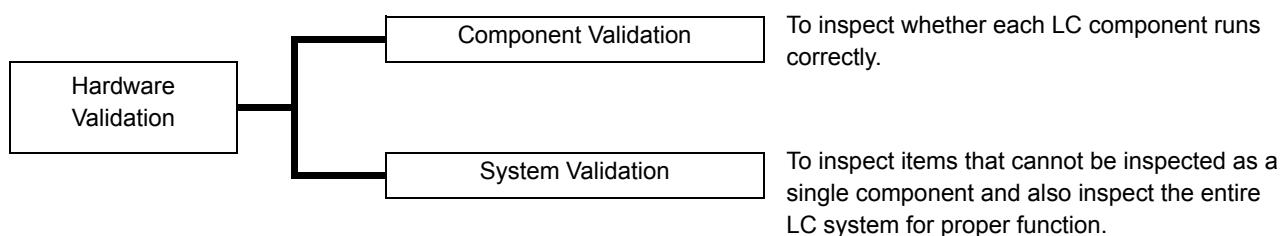

The operational protocol and criteria for this component and the HPLC system are described in this chapter to assist the user in conducting validation. Refer to each the instruction manual for each component for operational protocol of that specific component.

# 7.2 Implementation of Hardware Validation

## 7.2.1 Periodic Validation

Component and system validation must be performed at installation and every 6-12 months, as the performance of an LC instrument changes with age. It is also important to perform maintenance such as replacement of consumables in advance of hardware validation.

## 7.2.2 Daily Inspection

Daily inspection of the components and HPLC system examine the condition of maintenance parts to ensure a high level of analysis data reliability.

Items such as column deterioration and mobile phase adjustment are examined during system suitability tests.

## 7.2.3 Validation After Maintenance

After any maintenance, component performance must be re-validated. The type of validation depends on the actual work done.

If the maintenance inspection cannot be performed solely by the specific component validation, system validation is required.

**NOTE**

Maintenance information and results of hardware validation must be recorded and kept for future reference.

## 7.3 Validation Precautions

### 7.3.1 Environment

---

Instrument performance may be affected by abrupt changes in ambient temperature such as drafts from heating and air conditioning vents.

The equipment should be installed in a room with minimal (< 2°C) temperature fluctuation and away from sources of drafts and air currents.

### 7.3.2 Installation Site

---

The installation site is very important for ensuring correct validation. The site should satisfy the following conditions:

#### **WARNING**

- Provide ample ventilation with no fire sources in vicinity  
When flammable or toxic solvents are used as the mobile phase, the room must be properly ventilated.  
When flammable solvents are used, open flame or other fire sources must be strictly prohibited.

#### **CAUTION**

- Avoid dust or corrosive gas  
Avoid installing the instrument in places subject to excessive dust or corrosive gas since service life and performance levels may be affected.
- Keep away from strong magnetic fields  
Do not install the instrument near equipment that generates strong magnetic fields. If the power supply line is subject to high electrical noise, use a commercially-available power surge protector.
- Provide adequate installation surface and space  
The weight of LC-20AB is 13kg. During installation, consider the entire weight combined with other LC components.  
The lab table on which this instrument is installed should be strong enough to support the total weight of the LC system. It should be level, stable and have depth of at least 600mm.  
If these precautions are not followed, the instrument could tip over or fall off the table.  
When components are installed side by side, maintain a keep space of at least 30 mm between the components.
- Regulate room temperature and humidity  
The room temperature should be between 4 and 35°C, with minimal temperature variations throughout the course of a day. Humidity should be kept within 20-85%.
- Position instrument properly in the room  
Install the instrument in a location that is free from vibration and away from sunlight, and heat/air conditioning drafts.

# 7.4 Equipment Required for Validation

The equipment and samples listed below are required for hardware validation. Prepare necessary equipment and samples depending on the system configuration of the instrument.

## ■ Testing Equipment

A list of testing equipment required for hardware validation is shown below. A certificate ensuring traceability or inspection results should accompany each item of testing equipment that is used.

Equipment	Description
Thermo recorder	For inspection of the temperature setting accuracy for the column oven and the autosampler's sample cooler. The thermo recorder must be certified as having an accuracy rating of $\pm 1.0^{\circ}\text{C}$ for the required temperature range ( $0^{\circ}\text{C}$ to $50^{\circ}\text{C}$ ) at the time of inspection.
Resistance thermometer	For inspection of the temperature accuracy for the column oven. The resistance thermometer must have a testing accuracy of $\pm 0.5^{\circ}\text{C}$ for the required temperature range ( $0^{\circ}\text{C}$ to $50^{\circ}\text{C}$ ) at the time of inspection.
Thermocouple	For inspection of the temperature accuracy for the column oven and autosampler's sample cooler. The thermocouple must have a testing accuracy of $\pm 0.6^{\circ}\text{C}$ for the required temperature range ( $0^{\circ}\text{C}$ to $50^{\circ}\text{C}$ ) at the time of inspection.
DC voltage/current generator	For the hardware validation of the chromatopac. The DC voltage/current generator must be certified as having an accuracy rating of $\pm 0.15\%$ at the time of testing.
Stopwatch	For inspection of the flow rate accuracy for the solvent delivery module. The stopwatch must be certified at $5'30'' \pm 0.3\text{sec}$ at the time of inspection.
Measuring flask	For inspection of the flow rate accuracy for the solvent delivery module. Obtain a 5mL-measuring flask.
Electronic balance	For inspection of the injection volume accuracy for the autosampler. The balance must be calibrated and able to perform measurement with a 0.001g precision at the time of inspection.

## 7. Hardware Validation

---

### ■ Standard Reagents for Validation

A list of standard reagents required for validation is shown below. The customer should prepare standard reagents to the stated specifications.

Standard sample	Part No.	Description
Caffeine set (5 concentrations)	228-45725-91	For inspection of the absorbance linearity for the UV-VIS spectrophotometric and photodiode array detectors. For also inspection of system reproducibility for a system equipped with a UV-VIS spectrophotometric or photodiode array detector.
Caffeine (250mg/L)	228-45725-06	For inspection of system reproducibility for a system equipped with a refractive index detector, inspection of autosampler carry-over, and inspection of the gradient concentration accuracy for gradient systems.
Naphthalene (60mg/L)	228-32996-01	For inspection of system reproducibility for a system equipped with a spectrofluorometric detector.
Glycerol (0.872mg/L)	228-32996-05	For inspection of the span for the refractive index detector.

### ■ Hardware Testing Supplies

A list of supplies required for hardware validation is shown below. Note that items such as autosampler vials or mobile phase solutions may be required in addition to the items listed.

Implement	Part No.	Description
Resistor tube	228-45726-91	I.D. 0.13mm × 2m + I.D. 0.8mm × 2m For inspection of flow rate and gradient concentration accuracy for solvent delivery module, etc.
Syringe	046-00001 or 046-00038-01	For inspection of the absorbance linearity for the UV-VIS spectrophotometric and photodiode array detectors. For also inspection of the span for the refractive index detector. This item is provided with detectors as a standard accessory.
Syringe adapter	228-15672-91	Same as above.
Coupling 1.6C	228-16004-13	For each kind of inspection and in plumbing the detector. This item is provided with each component as a standard accessory.
Male nut, PEEK	228-18565	Same as above.
Plug	228-16006	For inspection of the drift/noise for the refractive index detector.
Low-pressure Hg (Mercury) lamp set	200-38423	For inspection of the wavelength accuracy for the UV-VIS photodiode array detector and the spectrofluorometric detector.
Hg (Mercury) lamp holder	228-34170-91	For inspection of the wavelength accuracy for the UV-VIS photodiode array detector.
	228-34478-91	For inspection of the wavelength accuracy for the spectrofluorometric detector.
PTFE block assembly	228-34319-91	For inspection of the wavelength accuracy for the spectrofluorometric detector.
Column Shim-pack VP-ODS or LUNA C18(2)	228-34937-91 or 00F-4252-E0	Particle size: 5µm Column Dimension: I.D. 4.6mm × length 150mm (An equivalent ODS column may also be used.) For the system validation.

# 7.5 Validation: Pump

## 7.5.1 Check Terms

Check terms for the pump validation are listed below.

	Check Term	Description
7.5.2	ROM, RAM Self Diagnosis	Checks whether the memory (ROM, RAM) functions correctly.
7.5.3	Firmware Version Check	Checks the version of firmware.
7.5.4	Display, LED Test	Checks the operation of display and LEDs.
7.5.5	Flow Rate's Control Parameter	Checks parameters to control the flow rate.
7.5.6	Pumping Stability Test	Checks that pump A's and pump B's pressure fluctuation width does not exceed the rated value.
7.5.7	Pressure Limiter Test	Checks the operation of pressure limiter.
7.5.8	Leak Sensor Test	Checks the operation of leak sensor.
7.5.9	Flow Rate Accuracy Test	Checks pump A's and pump B's flow rate accuracy by using a measuring flask.

## 7.5.2 ROM, RAM Self Diagnosis

7


### ■ Objective

To check whether the memory (ROM, RAM) functions correctly.

### ■ Check Procedure

- 1 Turn the power switch ON.
- 2 Press **VP** four times to display [VALIDATION].
- 3 Press **func** three times to display [MEMORY CHECK].
- 4 Press **enter**.  

"Checking Memory [MEMORY CHECK]" P.  
5-35

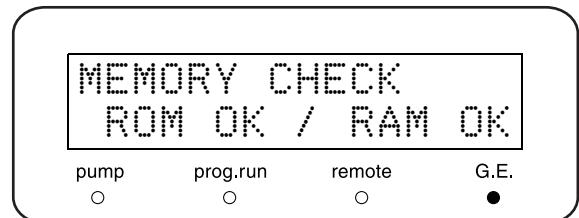

**CHECK CRITERIA : [ROM OK / RAM OK] is displayed on the screen.**

## 7. Hardware Validation


### 7.5.3 Firmware Version Check

#### ■ Objective

To check the version of firmware.

#### ■ Check Procedure

- 1 Press **VP** two times on the initial screen.  
[PRODUCT INFO] appears.
- 2 Press **func** two times to display the version number.  
 "Showing S/W Version No. [S/W ID]" P. 5-31

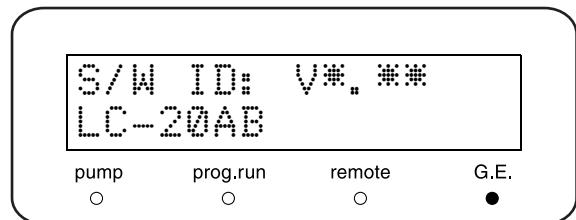

**CHECK CRITERIA : Version number appears.  
The number is same as the administrated one.**


### 7.5.4 Display, LED Test

#### ■ Objective

To check the operation of display and LEDs.

#### ■ Check Procedure

- 1 Turn the power switch ON.
- 2 Check that all the dots on the screen and LEDs on the keypanel illuminate right after turning ON the power.

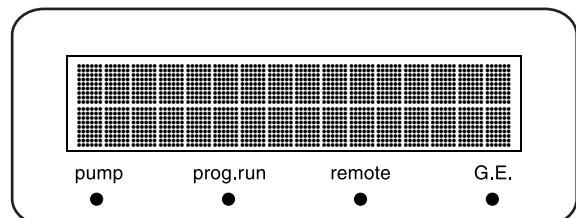

**CHECK CRITERIA : All the dots and LEDs on the screen illuminate.**




### 7.5.5 Flow Rate's Control Parameter

#### ■ Objective

To check parameters to control the flow rate.

#### ■ Check Procedure

- 1** Press **VP** five times on the initial screen.  
[CALIBRATION] appears.
- 2** Press **func** once to display [Input PASSWORD].
- 3** Enter the password as 5 digits and press **enter**.  
☞ "Inputting Password [Input PASSWORD]" P. 5-38  
[FLOW COMP FACT A] appears.
- 4** Make a note of the displayed value of [FLOW COMP FACT A] (ALPHA-A).
- 5** Press **func** once.  
Make a note of the displayed value of [FLOW COMP FACT B] (ALPHA-B).  
☞ "Setting Flow Rate Compensation Parameter (ALPHA) [FLOW COMP FACT A/B]" P. 5-38
- 6** Press **func** once.  
Make a note of the displayed two values (1: [PRS-1] and 5: [PRS-5]) of [PRESS COMP FACT].  
☞ "Setting Pressure Sensor Sensitivity Compensation Factor [PRESS COMP FACT]" P. 5-38

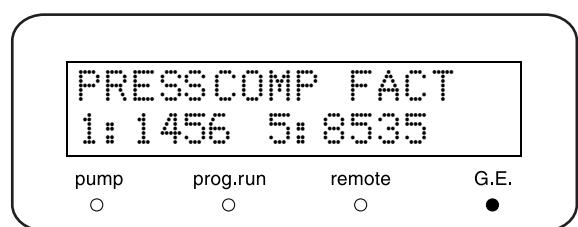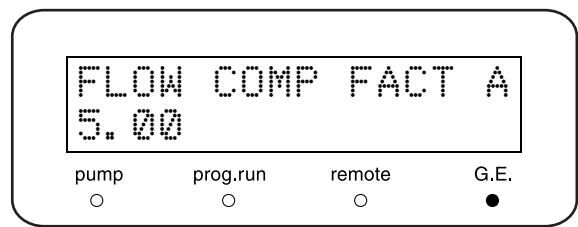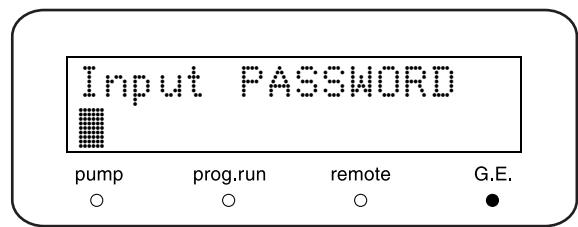

**CHECK CRITERIA : Parameters appear.**

## 7. Hardware Validation

### 7.5.6 Pumping Stability Test

#### ■ Objective

To check that the pressure fluctuation width does not exceed the rated value.

Perform this check for both pump A and pump B.

#### ■ Items Required for Check

Item	Description
Distilled water	Degas thoroughly using ultrasonic waves or an aspirator.
Resistor tube	

#### ■ Check Procedure

**1** Connect the resistor tube to the pump outlet instead of HPLC column.

**2** Fill the reservoir with distilled water to replace the mobile phase in the flow line.

**3** Press **func** repeatedly until [PARAMETER] appears and press **enter**.

**4** Press **func** or **back** repeatedly until [ACOMP] appears.  
Make a note of the current value.

Make note of this value.

1.000 ACOMP 1.20  
Input 0.00-3.00

pump      prog.run      remote      G.E.  
                  ●

**5** Press **0** · **.** · **4** · **5** · **enter** to set the value as [0.45].

1.000 ACOMP 0.45  
Input 0.00-3.00

pump      prog.run      remote      G.E.  
                  ●


**6** Press **func** once.  
Make a note of the current value of [BCOMP] (compressibility compensation) and set it to [0.45] in the way described above.

1.000 BCOMP 0.45  
Input 0.00-3.00

pump      prog.run      remote      G.E.  
                  ●

**7** Press **CE** two times to return to the initial screen.

- 8** Press **VP** four times to display [VALIDATION].
- 9** Press **func** four times to display [PULSE CHECK A].
- 10** Press **0** · **■** · **2** · **enter** to set [CRITERIA] as [0.20MPa].




- 11** Press **enter**.  
Pump A operates at 1mL/min and measurement starts one minute later. The set flow rate, the pump name, the measured pressure, the pressure fluctuation width, and the remaining time are displayed during measurement. After measurement, the measured value and the pass/fail status for the pressure fluctuation width are displayed.
- "Checking Pulsation [PULSE CHECK A/B]"  
P. 5-35

1.000 5.0 0.05  
(A) 0.98min left

PLS: A 0.07MPa OK  
Enter to Memory

- 12** Press **enter**.  
The result and date having measured will be stored at the instrument memory.
- 13** Press **func** one time to display [PULSE CHECK B].
- 14** Repeat steps 10 to 12 to measure the pressure fluctuation width for pump B.



**CHECK CRITERIA:** The measurement results for the pressure fluctuation width for pump A and pump B do not exceed 0.20MPa.

## 7. Hardware Validation

### ■ Resetting after Check

- 1 Press **func** repeatedly until [PARAMETER] appears, and press **enter**.
- 2 Press **func** or **back** repeatedly until [ACOMP] or [BCOMP] appears.
- 3 Return the value to the one recorded in step 3, 6.

### 7.5.7 Pressure Limiter Test

#### ■ Objective


To check that the pressure limiter operates properly at the upper and lower limits.

#### ■ Items Required for Check


Item	Description
Distilled water	Must be thoroughly degassed using ultrasonic waves or an aspirator.
Resistor tube	

#### ■ Check Procedure


- 1 Connect the resistor tube to the pump outlet instead of HPLC column.
- 2 Fill the reservoir with distilled water to replace the mobile phase in the flow line.
- 3 Turn the power switch ON.  
Initial screen appears.
- 4 Press **func** to activate setting of the flow rate.
- 5 Press **1** and **enter** to set the flow rate to [1mL/min].

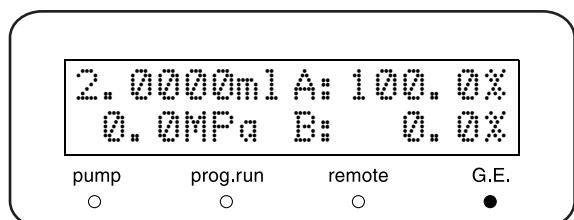


Cursor (positioned to prompt input)

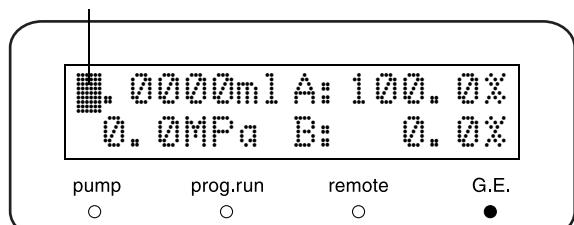

- 6** Press **func** three time to activate input of [P.MAX].  
When [PARAMETER] is displayed, press **enter**.

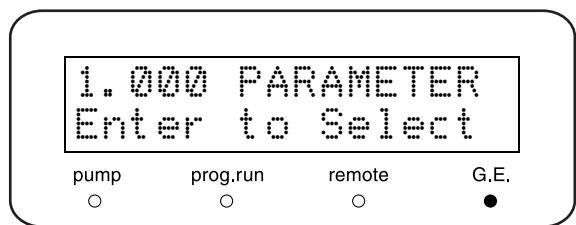


- 7** Press **2**, **0** and **enter** to set [20.0MPa] as [P.MAX].

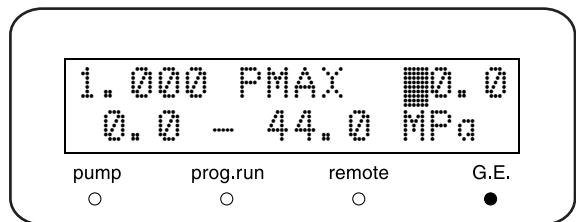


- 8** Press **func** one time to activate input of [P.MIN].

- 9** Press **0** and **enter** to set [0.0MPa] as [P.MIN].

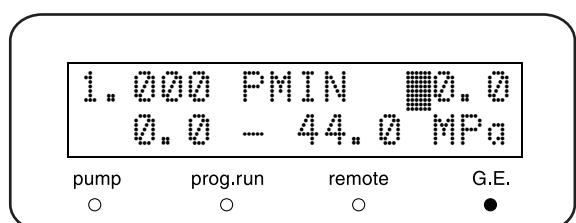


- 10** Press **CE** two times to return to the initial screen.

- 11** Press **pump** to start pumping for 3 minutes.  
 \* The pump indicator will illuminate while pumping.  
 \* At this time, neither [ERROR P-MAX] nor [ERROR P-MIN] should appear on the screen. Observe the screen and verify that neither appears.

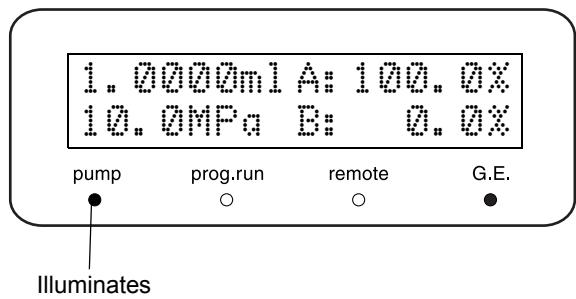

- 12** While pumping, change [P.MAX] and [P.MIN] as follows:  
 [P.MAX] = actual pressure + 1.0MPa.  
 [P.MIN] = actual pressure - 1.0MPa.  
 \* For example, when the actual pressure value is [10.0MPa], set [11.0MPa] as [P.MAX] and [9.0MPa] as [P.MIN].

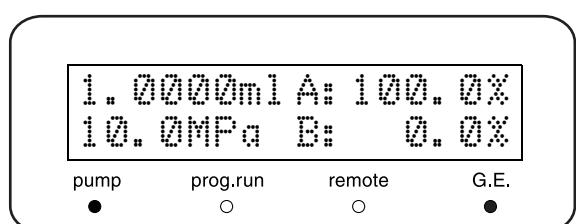


## 7. Hardware Validation


**13** Change the flow rate to 1.5mL/min, and observe the pressure.

When the actual pressure exceeds the [P.MAX] value set by step 12, [ERROR P-MAX] should appear.

**14** Press **CE** to clear [ERROR P-MAX].




**15** Reset the flow rate to [1mL/min], and press **pump** again to restart pumping.




**16** When the pressure has stabilized, change the flow rate to [0.5mL/min].

The actual pressure should fall below the [P.MIN] value set by step 12, and in several seconds, [ERROR P-MIN] should appear.



**17** Press **CE** to clear [ERROR P-MIN].



**CHECK CRITERIA : [ERROR P-MAX] and [ERROR P-MIN] appear.**


### 7.5.8 Leak Sensor Test

#### ■ Objective

To check the operation of leak sensor.

#### ■ Check Procedure

- 1** Press **VP** four times on the initial screen.  
[VALIDATION] appears.
- 2** Press **back** once to display [LEAK SENSOR TEST].  
 "Checking Leak Sensor [LEAK SENSOR TEST]" P. 5-37

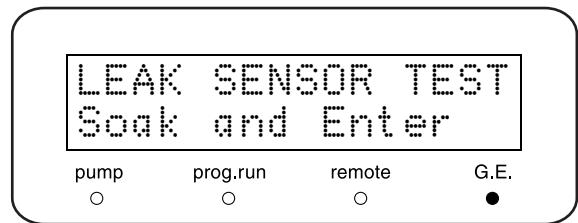

- 3** Using a syringe filled with water, wet the thermosensor at the bottom of the leak sensor.


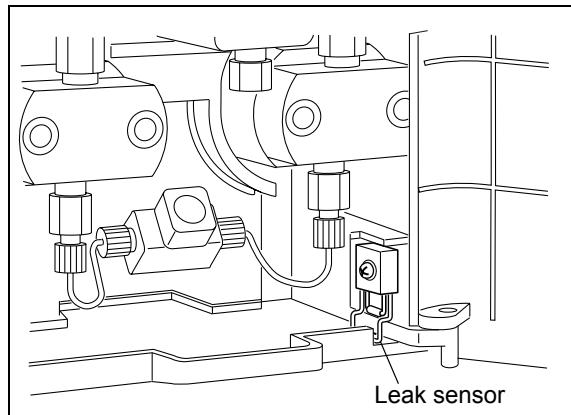


Fig. 7.1

- 4** In about 10 seconds, press **enter** to display the test result.

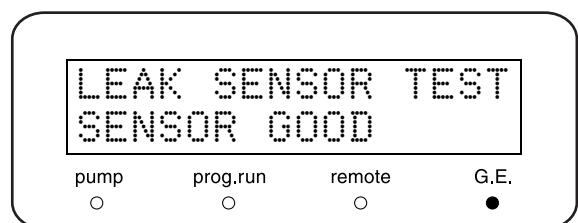

**CHECK CRITERIA : [SENSOR GOOD] appears on the screen.**

#### NOTE

After wetting and testing the leak sensor, wipe away the water on the leak tray completely.

"8.10 Wiping of Leak Tray" P. 8-25

## 7. Hardware Validation

### 7.5.9 Flow Rate Accuracy Test

#### ■ Objective

To check the flow rate accuracy by using a measuring flask.

Perform this check for both pump A and pump B.

#### ■ Items Required for Check


Item	Description
Distilled water	Degas thoroughly using ultrasonic waves or an aspirator.
Resistor tube	
Measuring flask (capacity 5mL), or measuring cylinder (capacity 10mL)	Flask/cylinder must have been validated.
Stopwatch	

#### ■ Check Procedure


- 1 Connect the resistor tube to the pump outlet instead of HPLC column.
- 2 Fill the reservoir with distilled water to replace the mobile phase in the flow line.
- 3 Press **func** repeatedly until [PARAMETER] appears, and press **enter**.

Make note of this value


- 4 Press **func** or **back** repeatedly until [ACOMP] appears.  
Make a note of the current value.

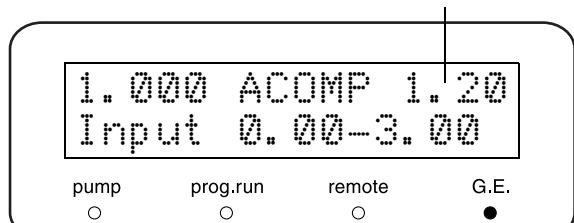



- 5 Press **0** · **•** · **4** · **5** and **enter** to set [0.45] as [ACOMP].

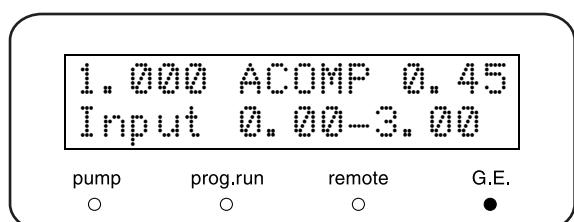

- 6 Press **func** once.  
Make a note of the current value of [BCOMP] (compressibility compensation) and set it to [0.45] in the way described above.

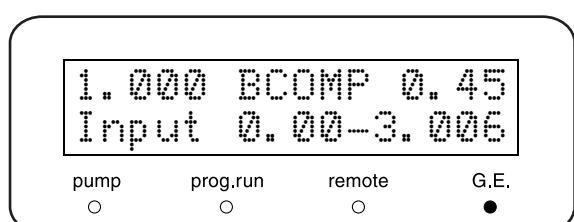

- 7** Press **CE** two times to return to the initial screen.
- 8** Press **VP** four times on the initial screen. [VALIDATION] appears.
- 9** Press **func** six times until [FLOW CHECK A] appears and press **enter**.
- 10** Pump A starts operating. Pumping continues for over 5 minutes and is stabilized.
- 11** Press **enter** again when it is ready to measure.

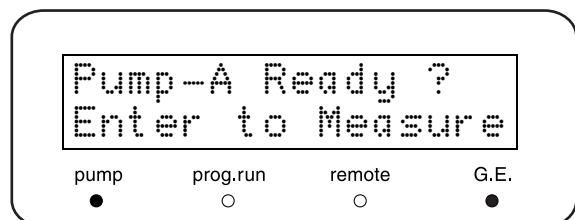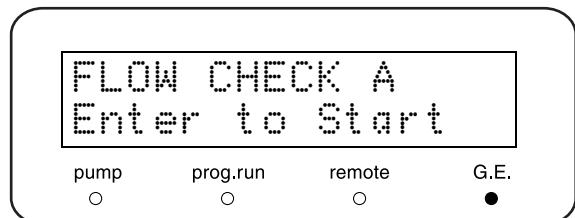

- 12** Place the end of the tubing into the flask or cylinder. Then start measuring.  
<For a measuring flask>  
The inside of the flask must be completely dry.  
1) Start the stopwatch as soon as the first drop of water emerges from the end of the tubing into the flask.  
2) Stop the stopwatch when the water is pooled 5mL.

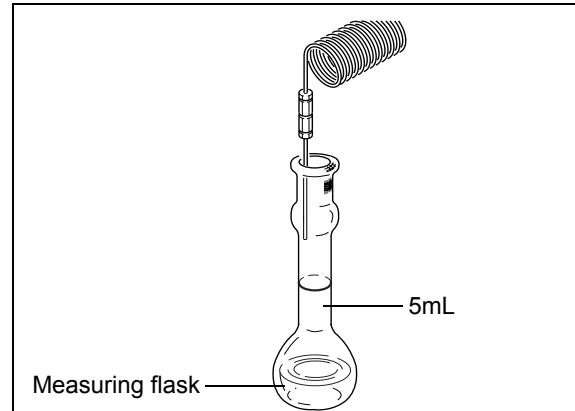


Fig. 7.2

- < For a measuring cylinder>
- 1) Bring the end of the tubing into contact with the cylinder wall.  
2) Determine a suitable water level inside the cylinder at which to start measurement. Start the stopwatch when the water reaches the determined start level.  
3) Stop the stopwatch when the water is pooled 5mL.

**NOTE**

Make sure that the end of the tubing remains above the water in the measuring cylinder throughout the measurement.


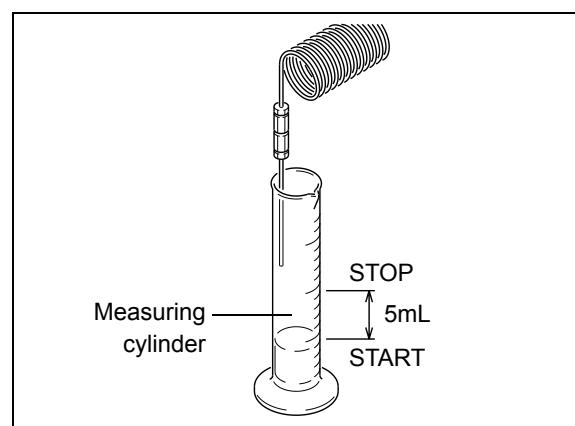



Fig. 7.3

## 7. Hardware Validation

- 13** Enter the time having measured with the numeric keypad and press **enter**.  
The flow rate accuracy (%) and the pass/fail status are displayed.

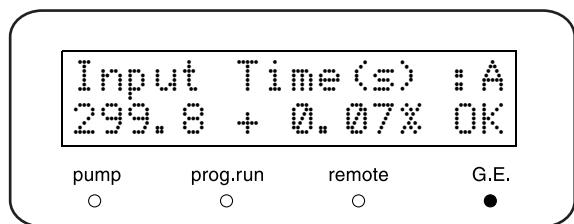

- 14** Press **func** once to display [FLOW CHECK B].
- 15** Check the flow rate for pump B in the way described above.

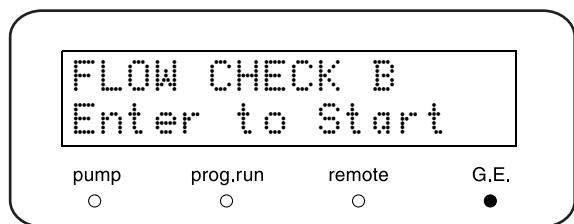

**CHECK CRITERIA : The flow rate accuracy for both pump A and pump B is within ± 2.00%.**

### ■ Resetting after Check

- 1** Press **func** repeatedly until [PARAMETER] appears. Then, press **enter**.
- 2** Press **func** or **back** repeatedly until [ACOMP] or [BCOMP] appears.
- 3** Return the value to the recorded value by step 4, 6.

# 7.6 Validation: Gradient Pump System

## ■ Objective

To check the gradient concentration accuracy for high-pressure gradient system.

## ■ Items Required for Check

Item	Description
High-pressure gradient system	Gradient mixer
UV detector	SPD-10A, 10Avp, 20A series
Data processor	Chromatopac, LC workstation or similar
Resistor tube	
Mobile phase* 500mL for each	<p>Distilled water</p> <p>(How to prepare) &lt;When using Shimadzu's standard reagents for validation&gt; Weigh 20mg of caffeine (250mg/L, Part No. 228-45725-06) and bring it to 500mL volume with water. &lt;In case of preparation by customer&gt; Weigh 20mg of anhydrous caffeine, transfer them to a 100mL measuring flask and bring it to 100mL volume with water. Then take 25mL of the solution, and add water to bring it to 500mL volume.</p>

\* Both mobile phases must be degassed using helium degasser or degasser unit.

7


## ■ Check Procedure

- 1 Connect the resistor tube between mixer outlet (1.7mL) and detector.
- 2 As mobile phase, prepare distilled water for mobile phase A, and caffeine solution for mobile phase B (500mL each).
- 3 Degas the mobile phases.
- 4 Open the drain valve and press **purge** to replace the flow lines.


## 7. Hardware Validation

- 5 Set the pumping condition as follows and press **pump** to start pumping until the baseline of detector stabilizes.

Total flow rate = 3mL/min  
Concentration of mobile phase B = 50.0%



- 6 Set the parameters of the control device as follows and pump until the baseline stabilizes.

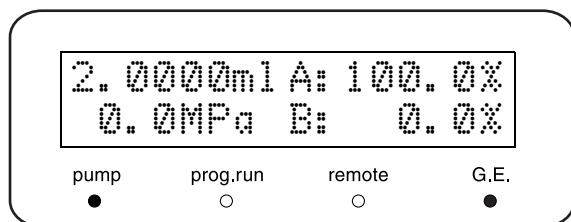

• Pumping system	Pumping mode	Binary Pump
	Flow rate	2.0mL/min
	Concentration of mobile phase B	0.0%
• UV detector	Wavelength	272nm
	RESPONSE	3 (0.5sec)
	AUX RANGE	2 (1.0AU/V)
• Data processor	1,024 mAU full scale (for Chromatopac, ATTEN=10) (With LCsolution, the intensity axis is set automatically.)	Chart speed 5mm/min (for Chromatopac, SPEED=5)

- 7 Enter the time program given in the table below, which will produce the operation pattern shown on the right.
- If a system controller or LC workstation is used, select time program from each menu, and create the program.
  - If control is local, create the time program on pump.

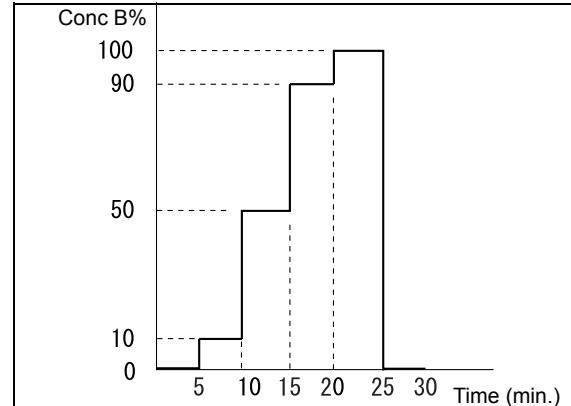


Fig. 7.4

- \* The [GE TEST PROGRAM] of VP function can copy the time program to a specified file automatically.

 "Setting Time Program to Check Concentration Accuracy of Gradient Mode [GE TEST PROGRAM]" P. 5-36

Time Program

TIME	FUNC	VALUE
5.00	B.CONC	0.0
5.01	B.CONC	10.0
10.00	B.CONC	10.0
10.01	B.CONC	50.0
15.00	B.CONC	50.0
15.01	B.CONC	90.0
20.00	B.CONC	90.0
20.01	B.CONC	100.0
25.00	B.CONC	100.0
25.01	B.CONC	0.0
30.00	STOP	

- 8** If a Chromatopac is used as the data processor, create the BASIC programs given on the right, which print the signal level at every 30 seconds (according to the model).

For C-R8A/R7A/R4A

LINE	PROGRAM
10	LPRINT LEVEL(1);
20	WAIT 30
30	GOTO 10
40	END

For C-R3A/R6A

LINE	PROGRAM
10	PRINT LEVEL;
20	WAIT 30
30	GOTO 10
40	END

For C-R5A

LINE	PROGRAM
10	LPRINT LEVEL;
20	WAIT 30
30	GOTO 10
40	END

- 9** Zero the baseline, start plotting on the data processor and continue with the gradient time program.  
If the Chromatopac is used as data processor, run the BASIC program.

## 7. Hardware Validation

---

- 10** Record the absorbance levels at the following concentrations, and use the data to calculate the actual concentrations.

**NOTE**

Measure a signal level when the baseline stabilizes.

<Calculation method>

$$\text{Actual concentration of 10\%} = \frac{\frac{(\text{Absorbance level at set concentration of 10\%})}{(\text{Absorbance level at set concentration of 100\%})} - 1}{\frac{(\text{Absorbance level at set concentration of 0\%})}{(\text{Absorbance level at set concentration of 0\%})}} \times 100$$
$$\text{Actual concentration of 50\%} = \frac{\frac{(\text{Absorbance level at set concentration of 50\%})}{(\text{Absorbance level at set concentration of 100\%})} - 1}{\frac{(\text{Absorbance level at set concentration of 0\%})}{(\text{Absorbance level at set concentration of 0\%})}} \times 100$$
$$\text{Actual concentration of 90\%} = \frac{\frac{(\text{Absorbance level at set concentration of 90\%})}{(\text{Absorbance level at set concentration of 100\%})} - 1}{\frac{(\text{Absorbance level at set concentration of 0\%})}{(\text{Absorbance level at set concentration of 0\%})}} \times 100$$

**CHECK CRITERIA : Within  $\pm 1.0\%$  of set value**

# 7.7 System Validation

- The LC system is comprised of many individual components. System validation is used to confirm the function of each component as well as the performance of the entire system.
- The standard system validation procedure described in this section is used to determine whether the LC system is functioning normally. This procedure constitutes the basis of the LC system capability inspection.
- System validation is performed at installation, and periodically thereafter. If a problem occurs during operation, system validation may be performed to determine whether the problem is in the LC system or in the analysis method.
- If the LC system passes the system validation, it can be assumed that the LC system is normal and that the problem lies in the particular analysis method or conditions being used.
- If the LC system does not pass the system validation, it may be assumed that there is an abnormality in the system, and component validation must be performed to identify the malfunctioning component(s).

## 7.7.1 Validation of Isocratic LC system

### ■ Objective

An analysis is performed and the retention time and peak area are obtained for each peak. The data is then examined to check for reproducibility. Reproducible data validates the system.

Generally, the system being validated consists of a minimum of the following components: pump, column oven, autosampler, detector, system controller and data processor.

7

### ■ Items Required for Validation

Item	Description
Mobile phase	Mixture of water and methanol (3/2, v/v) * Both the water (distilled) and the methanol should be HPLC grade.
Column	Shim-pack VP-ODS (Part No. 228-34937-91), LUNA C18 (2) (Part No. 00F-4252-E0) or equivalent ODS column (Particle size 5µm, Column Dimension : I.D. 4.6mm × length 150mm)
Sample	20mg/L caffeine solution (included in Caffeine set (5 concentrations) Part No. 228-45725-91) <Preparation> Weigh 20mg of anhydrous caffeine, transfer to a 100mL volumetric flask and dilute to volume with water. Transfer 1mL of the solution to a 10mL volumetric flask, and dilute to volume with water.
Water	HPLC grade, or equivalent
2-propanol	HPLC grade, or equivalent

### ■ Checking and Preparing the LC system

- 1** Check all the wiring connections in the LC system.  
Refer to individual component instruction manuals for details. If a Chromatopac is used, it should be connected to the detector with the signal cable connector provided with the Chromatopac, and the signal cable should then be connected to the integrator terminal of the detector.  
\* If the system normally uses Chromatopac or LC workstation, the connections used for regular analysis will be satisfactory.

- 2** Check the LC system plumbing.  
Ensure that the tubing between (a) the autosampler outlet and the column inlet, (b) the column outlet and the detector inlet, has an I.D. of less than 0.3mm, and is shorter than 300mm.  
Keep the liquid volume that is not in the column as low as possible.

- 3** Clean the system flow lines using one of the procedures described below.  
Before cleaning the flow lines, remove the column from the system, and connect the column inlet to the column outlet with a coupling 1.6C ("Fig. 7.5").

**< For a new system >**

Clean the flow lines first with 2-propanol, then with water. In each case, pass the liquid through the flow lines for 10 minutes, at a rate of 2mL/min.

**< For a system in use that uses a mobile phase with a low dielectric constant, such as hexane>**

The procedure is the same as that of a new system, given above.

**< For a system that has been using a mixture of a water solution and an organic solvent as mobile phase, or water plus an organic solvent miscible with water (methanol, acetonitrile, etc.) >**

Clean the flow lines with water. Pass water through the flow lines for 10 minutes, at a rate of 2mL/min.

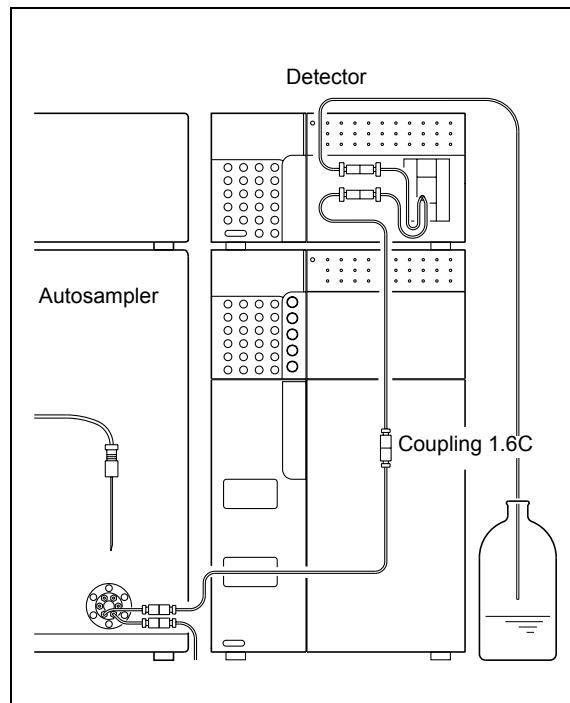


Fig. 7.5

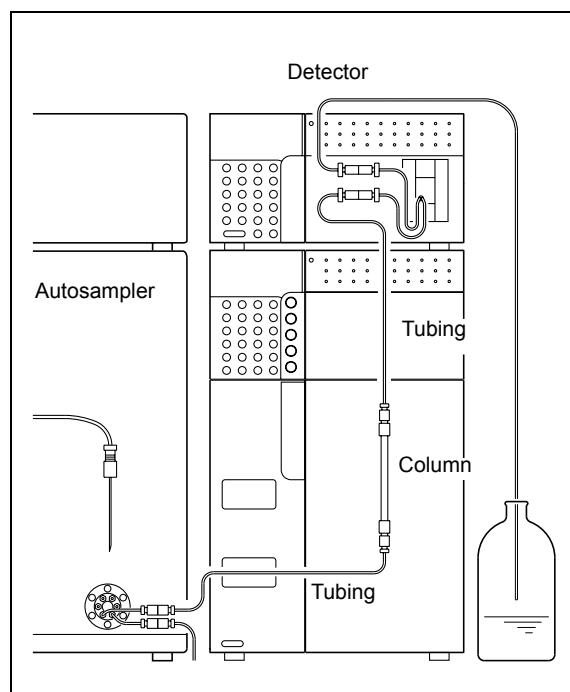



Fig. 7.6

- 4** When cleaning is finished, pour mobile phase (mixture of water and methanol (3/2, (v/v)) into the reservoir, and reconnect the column with the LC system ("Fig. 7.6").

### ■ Validation Procedure


- 1** Set the pumping flow rate to 1mL/min.  
See the pump's instruction manual for setting procedures.

Pump's display screen

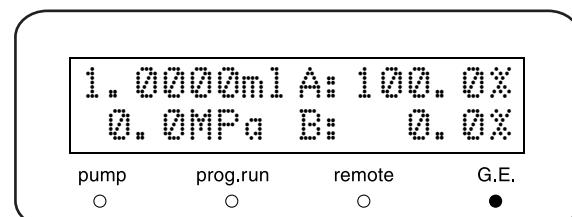

- 2** Set the column oven temperature to 40°C.  
See the column oven's instruction manual for setting procedures.


Column oven's display screen

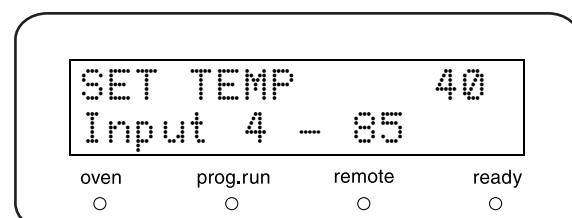

- 3** Press **pump** on the pump keypad, and **oven** on the column oven keypad. Pumping and temperature regulation will start.  
Verify that liquid flows through the detector outlet tubing, and that there are no leaks from any of the connections.

- 4** Set the detector parameters.  
 "Parameter Settings for Isocratic System Validation" P. 7-26  
See the detector's instruction manual for setting procedures.

Detector's display screen

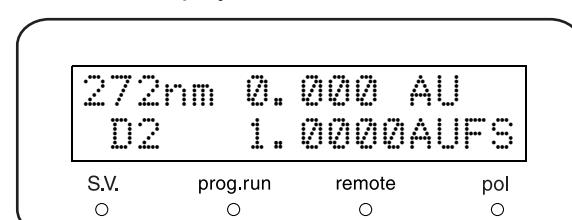

- 5** Set the autosampler parameters.  
 "Parameter Settings for Isocratic System Validation" P. 7-26

See the autosampler's instruction manual for setting procedures.

- 6** Set the data processor parameters.  
 "Parameter Settings for Isocratic System Validation" P. 7-26  
See the data processor's instruction manual for setting procedures.

## 7. Hardware Validation

7 Monitor the baseline.

When the baseline has stabilized, press the detector **zero** key, then inject 10 $\mu$ L of mobile phase, and verify that no peaks are observed.

8 Inject 10 $\mu$ L of the test standard six times, and analyze the data obtained.

9 From the peak data obtained from the six analyses, derive the relative standard deviation (coefficient of variation (C.V.)) for: retention time and peak area ("Fig. 7.7").

$$RSD(C.V.) = (SD/\bar{X}) \times 100$$

$$SD = \sqrt{\frac{\sum_{i=1}^n (X_i - \bar{X})^2}{n-1}}$$

$$\bar{X} = (X_1 + X_2 + \dots + X_n)/n$$

n : Number of analyses

X<sub>1</sub>...X<sub>n</sub> : Retention time (or areas) of each peak

$\bar{X}$  : Average

SD : Standard deviation

RSD : Relative standard deviation

C.V. : Coefficient of variation

Fig. 7.7

### ■ Parameter Settings for Isocratic System Validation

The parameters to be set for the various devices when validation analysis of an isocratic system is performed are given below.

• Pump .....	Flow rate	: 1mL/min
	P.Max	: 20.0MPa
• Column oven .....	Oven temperature	: 40°C
• Time program .....	5.00 STOP	
• Autosampler .....	RINSE VOLUME	: 200 $\mu$ L
	RINSE SPEED	: 35 $\mu$ L/s
	SAMPLING SPEED	: 15 $\mu$ L/s
	RINSE MODE	: 0 (No needle rinsing)
• Detector .....	Wavelength	: 272nm
	AUX RNG	: 2 (1AU/V)
	RESPONSE	: 3 (0.5s)
• Data processor .....	WIDTH	: 5
	DRIFT	: 0
	T.DBL	: 1000
	ATTEN	: 10 (1,024mAUFs)
	SLOPE	: 1000
	MIN.AREA	: 100000
	STOP.TM	: 5

### CHECK CRITERIA

The RSD (C.V.)'s obtained must satisfy the following criteria:

Retention time RSD must not exceed 0.5%.

Peak area RSD must not exceed 1.0%.

## 7.7.2 Validation of Gradient LC System

### ■ Objective

An analysis is performed and the retention time and peak area are obtained for each peak. The data is then examined to check for repeatability. Reproducible data validates the system.

Generally, the system being validated consists of a minimum of the following components: pump, column oven, autosampler, detector, system controller and data processor.

### ■ Items Required for Validation

Item	Description
Mobile phases	A: Distilled water B: Methanol A /B =60%/40% * Both the water (distilled) and the methanol should be HPLC grade.
Column	Shim-pack VP-ODS (Part No. 228-34937-91), LUNA C18 (2) (Part No. 00F-4252-E0) or equivalent ODS column (Particle size 5µm, Column Dimension : I.D. 4.6mm × length 150mm)
Sample	20mg/L caffeine solution (included in Caffeine set (5 concentrations) Part No. 228-45725-91) < Preparation > Weigh 20mg of anhydrous caffeine, transfer to a 100mL volumetric flask and dilute to volume with water. Transfer 1mL of the solution to a 10mL volumetric flask, and dilute to volume with water.
Water	HPLC grade, or equivalent
2-propanol	HPLC grade, or equivalent

### ■ Checking and Preparing the LC System

- 1 Check all the wiring connections in the LC system. Refer to individual component instruction manuals for details. If a Chromatopac is used, it should be connected to the detector with the signal cable connector provided with the Chromatopac, and the signal cable should then be connected to the integrator terminal of the detector.  
\* If the system normally uses Chromatopac or LC workstation, the connections used for regular analysis will be satisfactory.

- 2 Check the LC system plumbing. Ensure that the tubing between (a) the autosampler outlet and the column inlet, (b) the column outlet and the detector inlet, has an I.D. of less than 0.3mm, and is shorter than 300mm. Keep the liquid volume that is not in the column as low as possible.

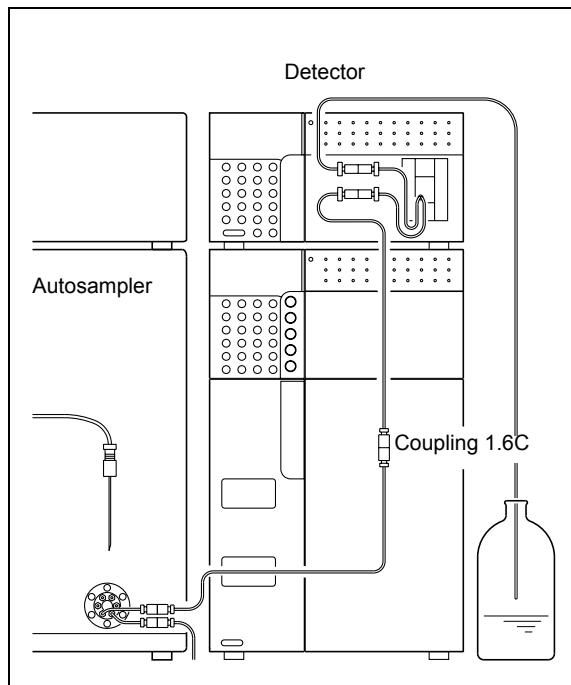


Fig. 7.8

## 7. Hardware Validation

- 3** Clean the system flow lines using one of the procedures described below.

Before cleaning the flow lines, remove the column from the system, and connect the column inlet to the column outlet with a coupling 1.6C ("Fig. 7.8").

**< For a new system >**

Clean the flow lines first with 2-propanol, then with water. In each case, pass the liquid through the flow lines for 10 minutes, at a rate of 2mL/min.

**< For a system in use that uses a mobile phase with a low dielectric constant, such as hexane>**

The procedure is the same as that of a new system, given above.

**< For a system that has been using a mixture of a water solution and an organic solvent as mobile phase, or water plus an organic solvent miscible with water (methanol, acetonitrile, etc.) >**

Clean the flow lines with water. Pass water through the flow lines for 10 minutes, at a rate of 2mL/min.

- 4** When cleaning is finished, pour mobile phase (A: water, B: methanol) into the reservoir, and reconnect the column with the LC system ("Fig. 7.9").

### ■ Validation Procedure

- 1** Set the pumping flow rate to 1mL/min, and set the concentration of mobile phase B parameter to 40%. See the pump's instruction manual for setting procedures.


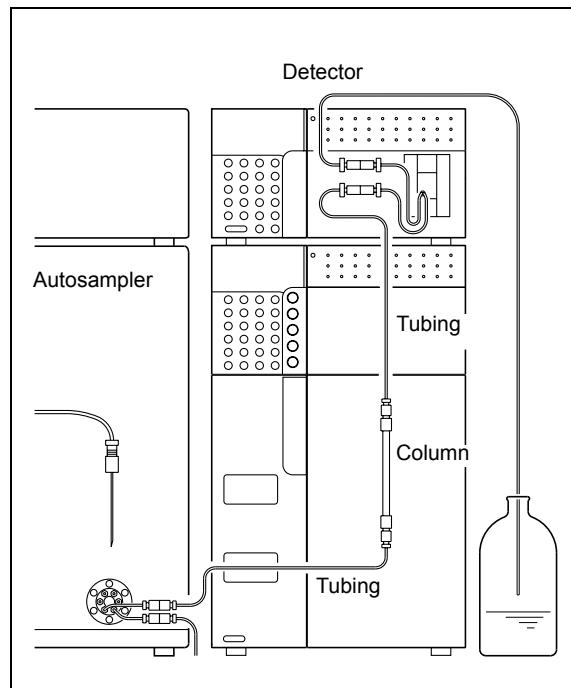



Fig. 7.9

Pump's display screen

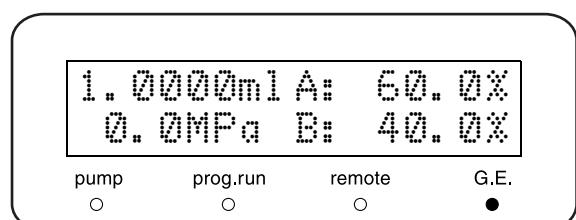


- 2** Set the column oven temperature to 40°C.  
See the column oven's instruction manual for setting procedures.
- 3** Press **pump** on the pump panel, and **oven** on the column oven panel. Pumping and temperature regulation will start.  
Verify that liquid flows through the detector outlet tubing, and that there are no leaks from any of the connections.
- 4** Set the detector parameters.  
 "Parameter Settings for Gradient System Validation" P. 7-30  
See the detector's instruction manual for setting procedures.
- 5** Set the autosampler parameters.  
 "Parameter Settings for Isocratic System Validation" P. 7-26  
See the autosampler 's instruction manual for setting procedures.
- 6** Set the data processor parameters.  
 "Parameter Settings for Gradient System Validation" P. 7-30  
See the data processor's instruction manual for setting procedures.
- 7** Monitor the baseline.  
When the baseline has stabilized, press the detector **zero** key. Then inject 10µL of mobile phase and verify that no peaks are observed the second time.

Column oven's display screen

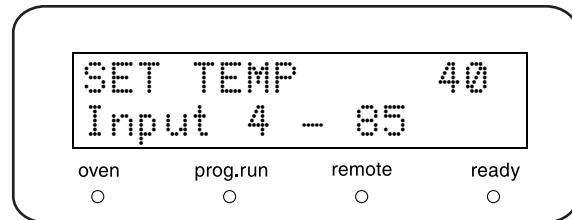

Detector's display screen

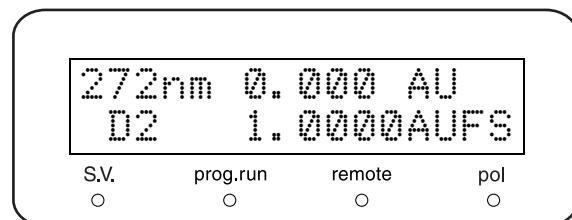

## 7. Hardware Validation

- 8 Inject 10 $\mu$ L of the test sample six times, and analyze the data obtained.
- 9 From the peak data obtained from the six analyses, derive the relative standard deviation (coefficient of variation (C.V.)) for: retention time and peak area ("Fig. 7.10").

$$RSD(C.V.) = (SD/\bar{X}) \times 100$$

$$SD = \sqrt{\frac{\sum_{i=1}^n (Xi - \bar{X})^2}{n-1}}$$

$$\bar{X} = (X_1 + X_2 + \dots + X_n) / n$$

n : Number of analyses

X<sub>1</sub>...X<sub>n</sub> : Retention time (or areas) of each peak

$\bar{X}$  : Average

SD : Standard deviation

RSD : Relative standard deviation

C.V. : Coefficient of variation

Fig. 7.10

### ■ Parameter Settings for Gradient System Validation

The parameters to be set for the various devices when validation analysis of a gradient system is performed are given below.

• Pump .....	Flow rate	: 1mL/min
	B.CONC	: 40%
	P.Max	: 20.0MPa
• Column oven .....	Oven temperature	: 40°C
• Time program .....	5.00 STOP	
• Autosampler .....	RINSE VOLUME	: 200 $\mu$ L
	RINSE SPEED	: 35 $\mu$ L/s
	SAMPLING SPEED	: 15 $\mu$ L/s
	RINSE MODE	: 0 (No needle rinsing)
• Detector .....	Wavelength	: 272nm
	AUX RNG	: 2 (1AU/V)
	RESPONSE	: 3 (0.5s)
• Data processor.....	WIDTH	: 5
	DRIFT	: 0
	T.DBL	: 1000
	ATTEN	: 10 (1,024mAUFs)
	SLOPE	: 1000
	MIN.AREA	: 100000
	STOP.TM	: 5

### CHECK CRITERIA

The RSD (C.V.)'s obtained must satisfy the following criteria:

Retention time RSD must not exceed 0.5%.

Peak area RSD must not exceed 1.0%.

## 7.8 If Validation Fails

Should the system fail to satisfy any of the system validation check criteria, or should a component fail to satisfy any of the component validation check criteria, proceed as follows.

- Check whether any consumable items have reached the end of their service life:  
The cause of failure to satisfy check criteria could be a consumable part that is no longer usable. Check consumable parts and replace them if necessary.
- Perform troubleshooting:  
It is possible that some minor problem (such as air bubbles) has caused the system to fail the criteria. Perform troubleshooting to check for such problems, and take action to eliminate any problems found. For troubleshooting procedures for individual system components, see the applicable instruction manuals.
- If a cause cannot be determined, contact your Shimadzu representative:  
If you are unable to determine the cause of the failure, or if you are unclear about troubleshooting or corrective action procedures, contact your Shimadzu representative.

## 7. Hardware Validation

---

This page is intentionally left blank.

# 8

---

## Maintenance

### Contents

8.1	Periodic Inspection and Maintenance .....	8-2
8.2	Replacement of Plunger Seal .....	8-5
8.3	Cleaning and Inspection (Replacement) of Plungers and Diaphragms .....	8-10
8.4	Cleaning of Check Valves .....	8-15
8.5	Inspection (Replacement) and Ultrasonic Bath Cleaning of Check Valves....	8-16
8.6	Inspection (Replacement) and Ultrasonic Bath Cleaning of Line Filter.....	8-19
8.7	Inspection (Replacement) and Ultrasonic Bath Cleaning of Suction Filter.....	8-21
8.8	Replacement of Drain Valve ASSY.....	8-22
8.9	Replacement of Fuse .....	8-24
8.10	Wiping of Leak Tray .....	8-25
8.11	Exterior Cleaning.....	8-26

## 8.1 Periodic Inspection and Maintenance

It is necessary to perform periodic inspections of this instrument to ensure its safe use.

It is possible to have these periodic inspections performed by Shimadzu service representatives on a contractual basis.

For information regarding the maintenance inspection contract, contact your Shimadzu representative.

### **WARNING**

- Unless the instructions here specified, turn off the power always and unplug the instrument prior to performing inspections and maintenance. Otherwise, fire, electric shock or malfunction may occur.

### **CAUTION**

- When replacing parts, use only the parts listed in "[1.3 Component Parts](#)" and "[9.3 Maintenance Parts](#)". If any other parts are used, injury or malfunction may occur.
- Never remove the main cover. Otherwise, injury or malfunction may occur.  
Contact your Shimadzu representative to remove the main cover.

---

### 8.1.1 Prior to Inspection and Maintenance

---

- Replace the mobile phase in the flow lines with water.
- Wipe away any dirt from the front panel and the main cover.
- Wipe away any dirt from the keypad with tissue paper or a soft cloth moistened with water.

## 8.1.2 List of Periodic Inspection and Maintenance

**⚠ CAUTION**

The replacement and maintenance periods listed in this table are presented only as guidelines. These are not guarantee periods. These will vary depending on usage conditions.

Inspection/Maintenance Item	6 months	1 year	2 years	3 years	Remark	Page
Replacement of Plunger seal		×			<ul style="list-style-type: none"> <li>Sealing efficiency decreases when seals are worn.</li> <li>Replace when the plunger is replaced.</li> <li>As a guideline, seals should be replaced after delivery of 90L when 2-propanol is pumped at pressure of 10MPa (102kgf/cm<sup>2</sup>). (VP function, [A(B) SEAL DELIVERED], shows the cumulative pumping volume.)</li> </ul>	P.8-5
Cleaning and inspection (replacement) of Plunger		×				P.8-10
Inspection (replacement) of diaphragm			×		<ul style="list-style-type: none"> <li>Replace when the plunger is replaced.</li> </ul>	P.8-12
Inspection (replacement) and ultrasonic bath cleaning of outlet check valve		×				P.8-16
Inspection (replacement) and ultrasonic bath cleaning of inlet check valve		×				
Inspection (replacement) and cleaning of line filter	×				<ul style="list-style-type: none"> <li>Particulates in mobile phase clog the filter in prolonged use.</li> </ul>	P.8-19
Inspection (replacement) and cleaning of suction filter			×		<ul style="list-style-type: none"> <li>Particulates in mobile phase clog the filter in prolonged use.</li> </ul>	P.8-21
Replacement of Drain valve				×	<ul style="list-style-type: none"> <li>Sealing efficiency decreases when the drain valves are worn.</li> </ul>	P.8-22
Pump ASSY lubrication				×	<ul style="list-style-type: none"> <li>Contact your Shimadzu representative.</li> </ul>	-
Fuse replacement				×		P.8-24

## 8. Maintenance

---

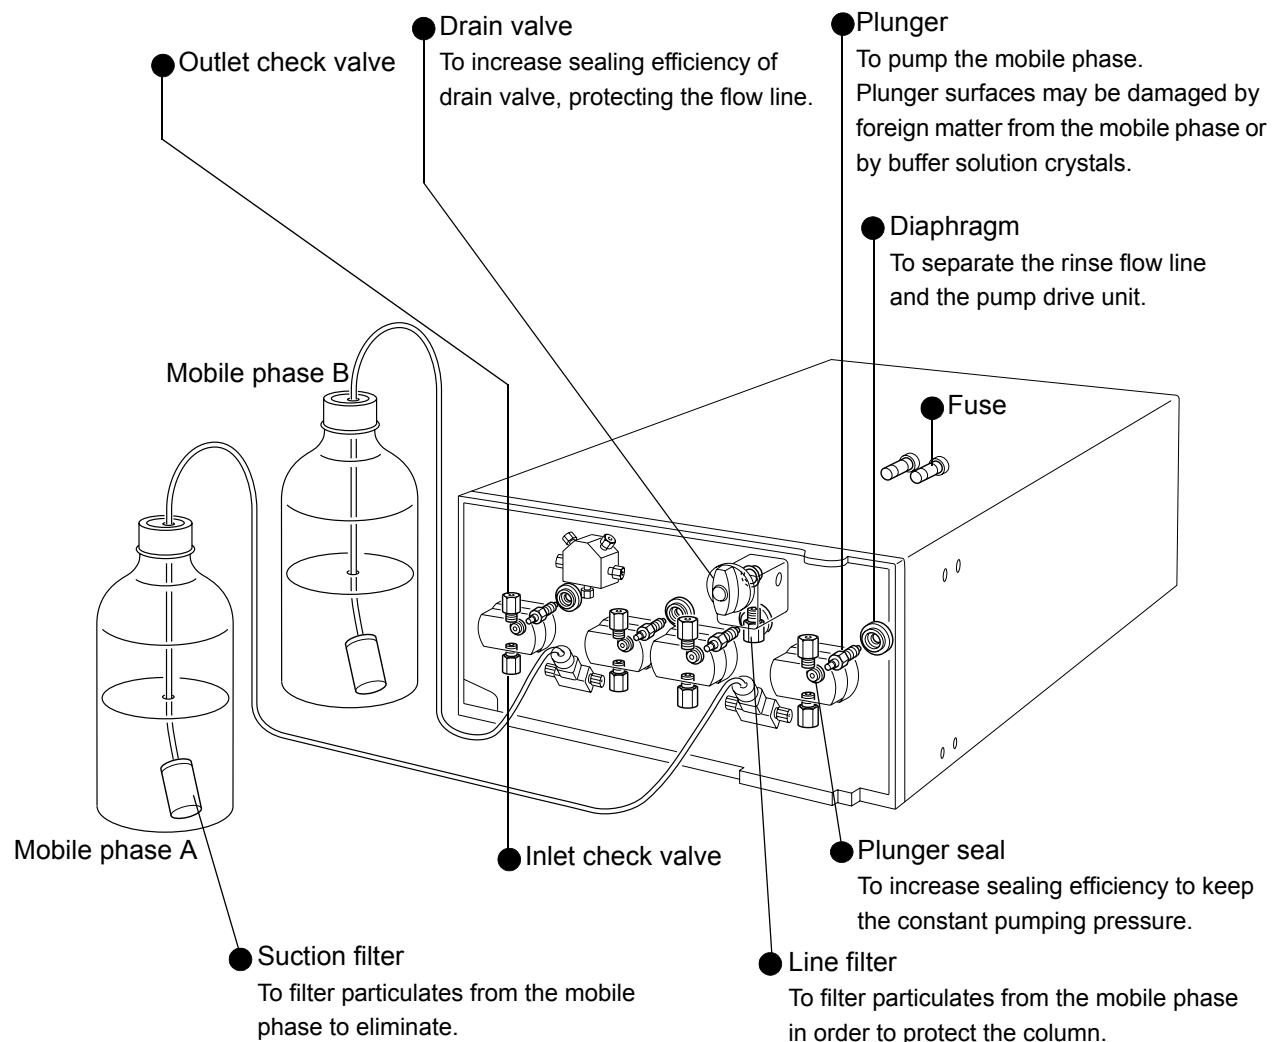


Fig. 8.1

---

### 8.1.3 Check after Inspection and Maintenance

---

After inspection and maintenance, check any leakage during pumping.

"6.1 Troubleshooting and Corrective Action" P. 6-2

# 8.2 Replacement of Plunger Seal

Plunger seals are mounted inside both the right and left pump heads of both pumps A and B. The procedure given below is for replacement of the seal inside pump A's right pump head (as viewed from the front of the instrument).

## Necessary parts


Part	Type	Part No.
Plunger seal	Consumable part	228-35146

### 8.2.1 Before Removing Pump Head

To prevent bending the plunger, follow the procedure below to retract the plunger completely.


- 1** Turn the power switch ON.  
Initial screen appears.

Initial screen




- 2** Press **func** repeatedly until [CONTROL] appears, and press **enter**.  
[P-SET] appears on the screen and the cursor blinks in the [P-SET] input field, prompting input.

[P-SET] display

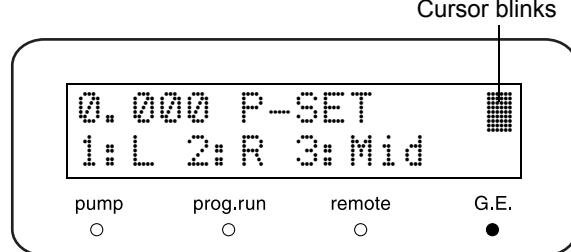

- 3** Press **2** and **enter**.  
(When replacing the left plunger seal, press **1** and **enter**.)  
The pump indicator illuminates for a short while, then goes out. The right plungers for both pumps A and B are retracted as far as possible.

"Plunger Set [P-SET]" P. 5-20

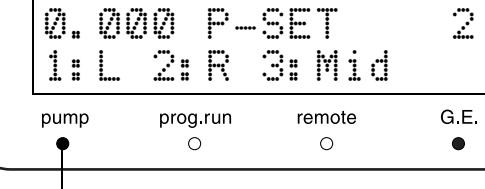

Pump indicator illuminates.

- 4** Press **CE** two times.  
Initial screen appears.

## 8. Maintenance

- 5** Use one of the following measures to ensure that the mobile phase does not flow out of the end of the tubing when plumbing is removed.
- Place the reservoir lower than the pump inlet.
  - Empty the reservoir and suction tubing of all mobile phase, and unscrew and remove the filter bushing from the pump inlet.

### 8.2.2 Removing Pump Head

- 1** Hold the outlet check valve using the provided wrench.
- 2** Loosen the male nuts at both ends of SUS tubing with the other wrench and remove SUS tubing.
- 3** Loosen male nut PEEK on the inlet-side tubing and remove it from inlet check valve.

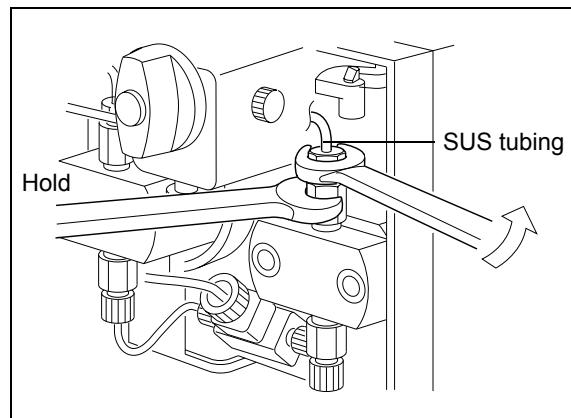


Fig. 8.2

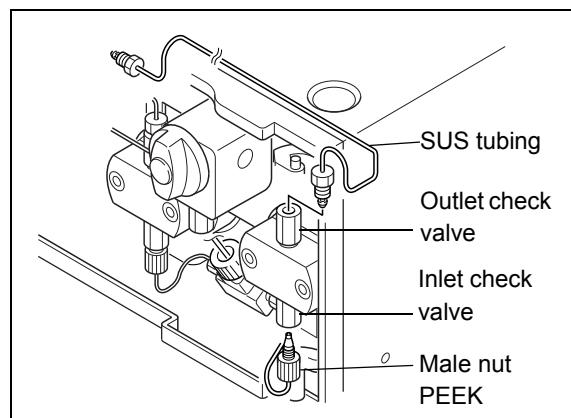


Fig. 8.3

- 4** Using the provided Allen wrench, alternately loosen the two hex socket head bolts in the pump head and remove.

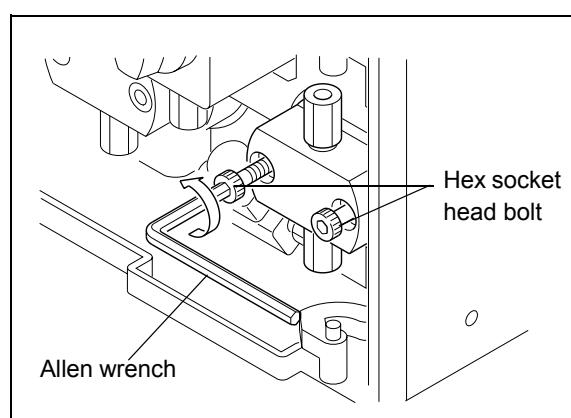


Fig. 8.4

- 5** Remove the pump head.

**⚠ CAUTION**

Ease the pump head out gently, keeping it aligned with the plunger at all times. If it is pulled out forcefully, the plunger could be bent.

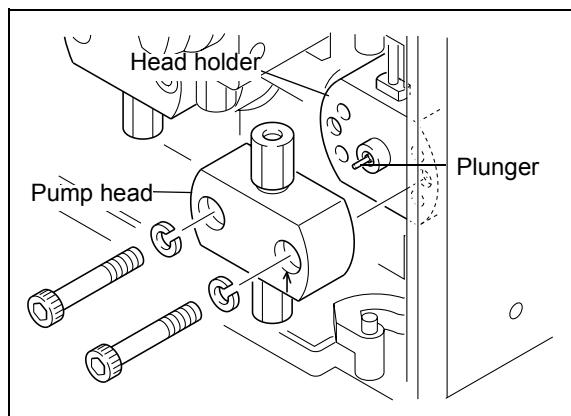


Fig. 8.5

### 8.2.3 Replacing Plunger Seal

Plunger seals are mounted inside the pump head. To remove the plunger seal, use the provided seal installer/remover.

- 1** Insert the seal installer/remover (flanged end) into the plunger seal.

#### Inside of pump head

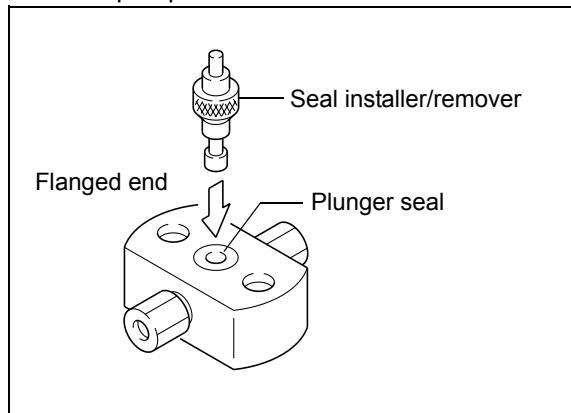


Fig. 8.6

- 2** Pull on the seal installer/remover. The plunger seal will be removed from the pump head.

**⚠ CAUTION**

After removing the seal, wipe the plunger head inner side and plunger seal outlet with clean gauze soaked in 2-propanol. If seal material adheres to these surfaces, the sealing efficiency of the plunger cannot be maintained.

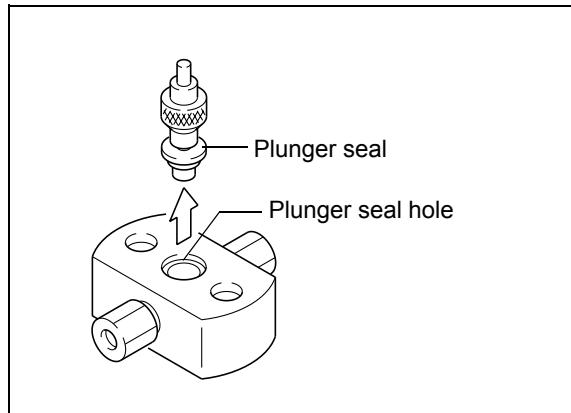


Fig. 8.7

## 8. Maintenance

- 3** Insert the seal installer/remover (straight end) into the new plunger seal.
- 4** Insert the new plunger seal vertically into the pump head. Then pull the installer/remover out of the seal.

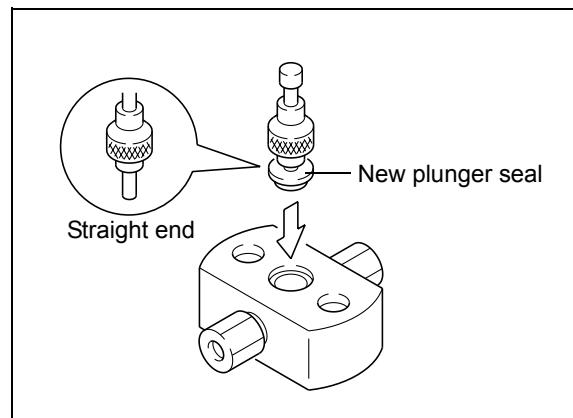


Fig. 8.8

### 8.2.4 Installing Pump Head

- 1** Mount the pump head onto the head holder so that the arrow on the pump head is pointing upward.

#### **CAUTION**

Ease the pump head in gently, keeping it aligned with the plunger at all times. If it is pushed in forcefully, the plunger could be bent.

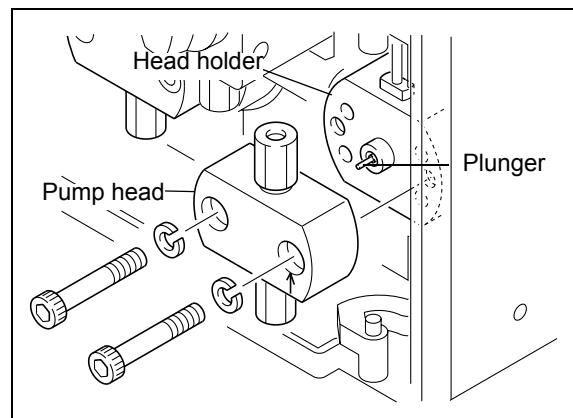


Fig. 8.9

- 2** Place the two hex socket head bolts into the holes in the pump head, and screw them in alternately and uniformly with provided Allen wrench.

#### **NOTE**

Screw the bolts in alternately 90°. At the end, tighten the bolts securely with the Allen wrench.

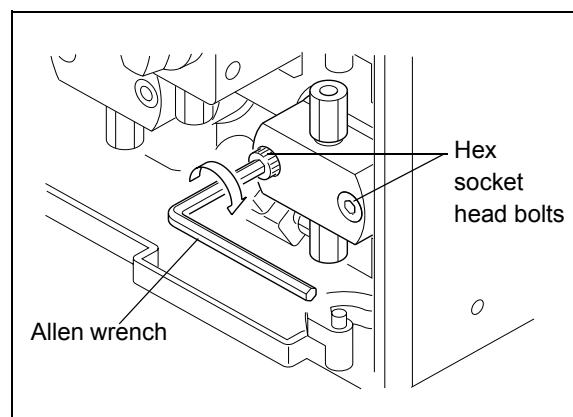


Fig. 8.10

- 3 Screw the male nuts on the both ends of the SUS tubing into outlet check valve and the converging block.
- 4 Screw the male nut PEEK on the inlet-side tubing into inlet check valve.
- 5 Return the reservoir or the suction filter bushing to its original position.

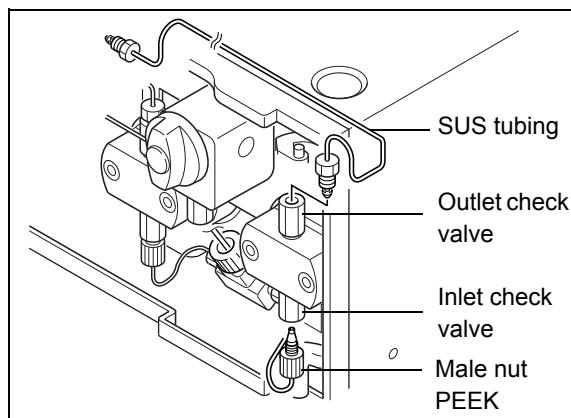


Fig. 8.11

#### 8.2.5 Check after Replacement

After replacing a plunger seal, check the following:

- Pumping (pressure value) is stable.
- There is no leakage from the gap between the pump head and the head holder.
- There is no leakage from the rinse flow line.

**NOTE**

When the phenomena above happen even after replacement of the plunger seals, the surfaces of the plunger may be scratched or nicked, in which case the plunger must be replaced.

 "8.3 Cleaning and Inspection (Replacement) of Plungers and Diaphragms" P. 8-10

## 8.3 Cleaning and Inspection (Replacement) of Plungers and Diaphragms

Plungers and diaphragms are mounted to the pump bodies on the left and right of both pumps A and B. The procedure for cleaning, inspecting, and replacing the plunger and diaphragm on the right of pump A is described below. When replacing a plunger, be sure to replace the plunger seal and the diaphragm.

### Necessary parts

Part	Type	Part No.
Plunger holder ASSY	Consumable part	228-35281-95
diaphragm	Consumable part	228-32784-91

### 8.3.1 Removing Pump Head and Head Holder ASSY

- 1 Remove the pump head.  
 "8.2.1 Before Removing Pump Head" P. 8-5,  
 "8.2.2 Removing Pump Head" P. 8-6

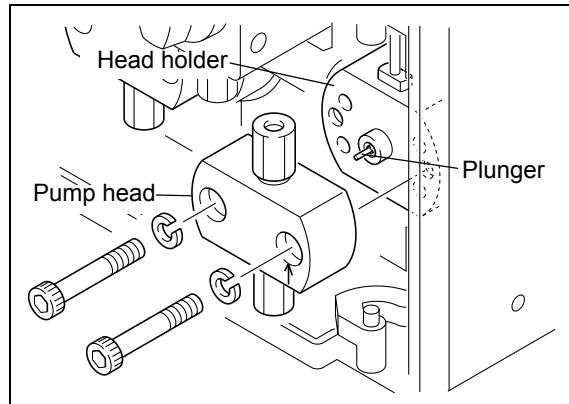


Fig. 8.12

- 2 Using the provided Allen wrench, alternately loosen the two hex socket head bolts in the pump head and remove.

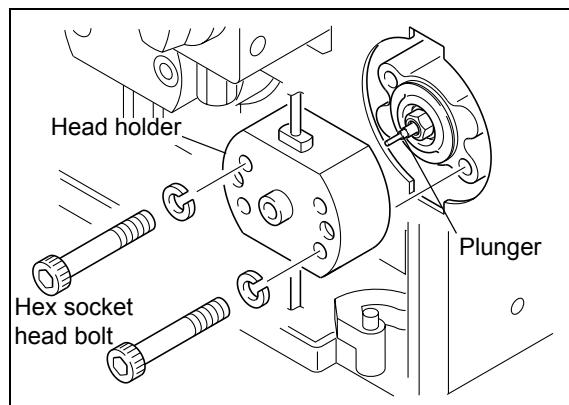


Fig. 8.13



#### CAUTION

Ease the head holder out gently, keeping it aligned with the plunger at all times. If it is pulled out forcefully, the plunger could be bent.

### ■ When the Head Holder is difficult to remove

- 1** Reinsert the two hex socket head bolts into the head holder's M4 bolt holes and tighten them alternately. The force of the two hex socket head bolts pushing against the body causes the head holder to become detached.

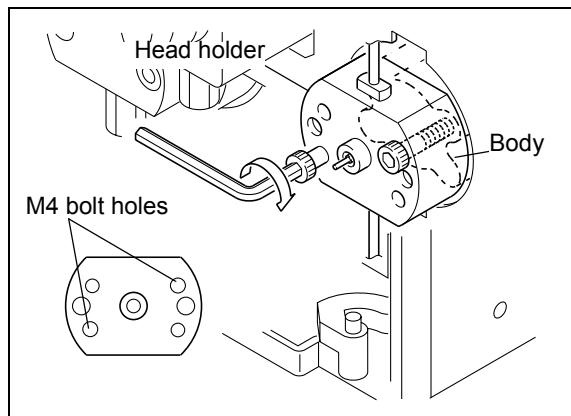


Fig. 8.14

### 8.3.2 Cleaning and Inspecting (Replacing) of Plungers

- 1** Using the provided box driver, rotate the plunger holder counterclockwise, and remove it.

#### **⚠ CAUTION**

When inserting the box driver into the plunger holder, be careful not to bend the plunger.

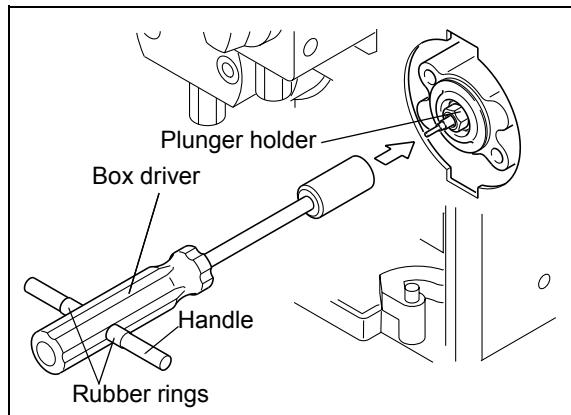


Fig. 8.15

- 2** Wipe any seal material with clean gauze soaked in 2-propanol.  
Seal material will interfere the sealing efficiency.

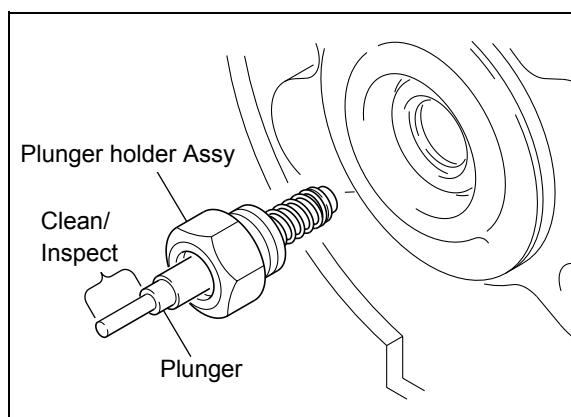


Fig. 8.16

## 8. Maintenance

- 3 Visually inspect the plunger for any scratches or nicks.  
If any scratches are found, replace the plunger.

**⚠ CAUTION**

Plunger surfaces may be damaged by foreign matter (from the mobile phase) or buffer solution crystals inside the head holder.

Components of Plunger Holder  
Plunger holder Assy  
(Part No.228-35281-95)

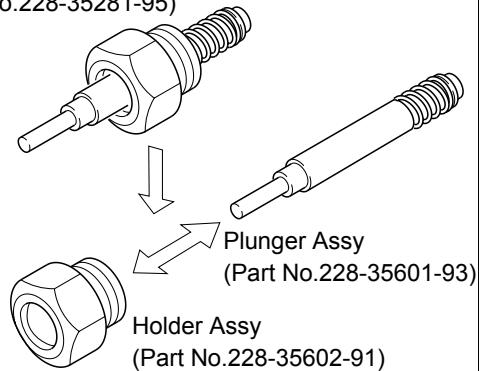


Fig. 8.17

### 8.3.3 Inspection (Replacement) of Diaphragms

When replacing a plunger, be sure to replace the diaphragm.

- 1 Remove the diaphragm.
- 2 Inspect the diaphragm for scratches or deformation.  
If any scratches or deformation is found, replace the diaphragm.

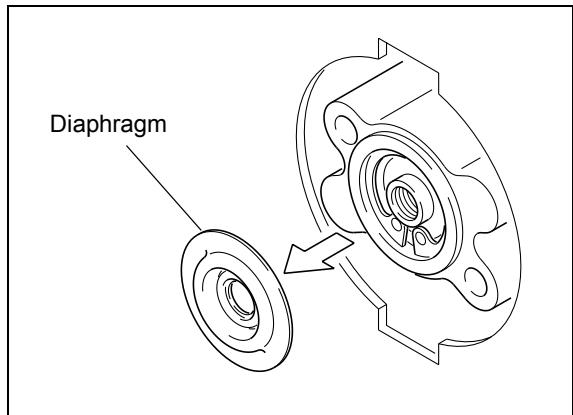


Fig. 8.18

### 8.3.4 Re-Installing after Inspection

- 1 Mount the diaphragm to the body.

**NOTE**

Be sure to mount the diaphragm with the correct orientation, as shown on the "Fig. 8.19".

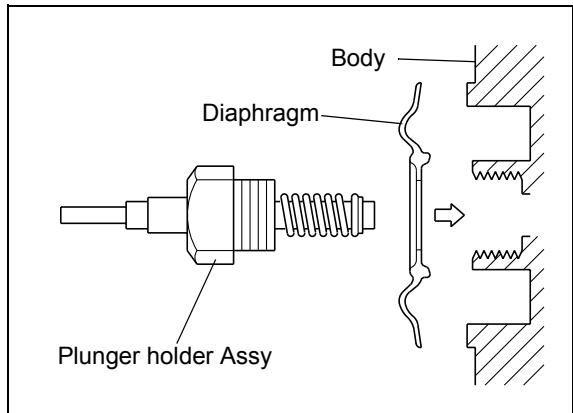


Fig. 8.19

- 2** Holding the plunger by finger, insert it into the pump chamber.

**NOTE**

Check that the diaphragm is centered properly.

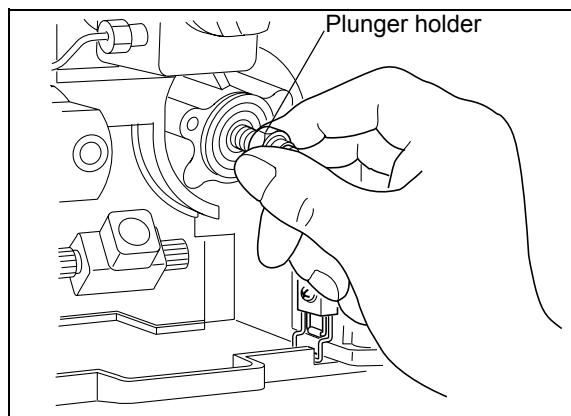


Fig. 8.20

- 3** Use the box driver to tighten the plunger holder.

- 4** Insert the head holder into the body.

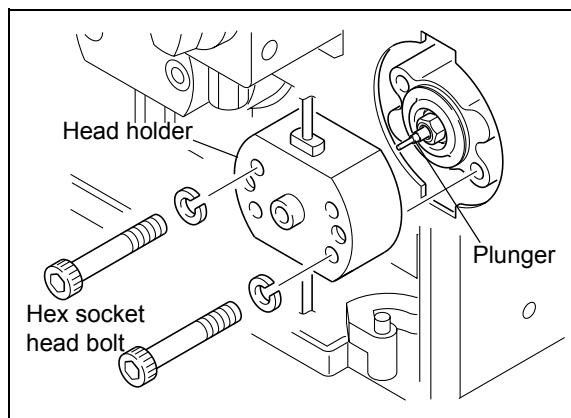


Fig. 8.21

**CAUTION**

Ease the head holder out gently, keeping it aligned with the plunger at all times. If it is pulled out forcefully, the plunger could be bent.

- 5** Insert the two hex socket head bolts in the head holder, and tighten them with the Allen wrench.

**NOTE**

Tighten the hex socket head bolts alternately, in 90° increments. At the end, tighten the bolts securely with the Allen wrench, holding the long part of the wrench like a handle.

## 8. Maintenance

- 6** Reinstall the pump head and the plumbing to the original state.

 "8.2.4 Installing Pump Head" P. 8-8

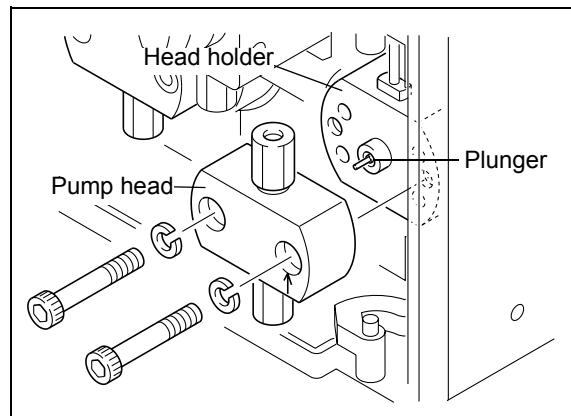


Fig. 8.22

### 8.3.5 Check after Cleaning and Inspection (Replacement)

After cleaning and inspecting (replacing) a plunger and/or a diaphragm, use the following procedure to check the diaphragm.

- 1** Insert a syringe needle into the tip of the disposable syringe (accessory).
- 2** Attach rinse tubing S (accessory) to the tip of the syringe needle and insert it in the rinse-solution outlet at the top of the head holder.
- 3** Block the rinse-solution inlet at the bottom of the head holder with your finger.
- 4** Push in the disposable syringe's plunger and release it at an appropriate position. If no air is leaked, the plunger will return to its original position.

#### ■ If Air Is Leaked

Check the connection between the rinse tubing and the head holder and, if there are no irregularities, disassemble the components and check that the diaphragm is mounted properly.

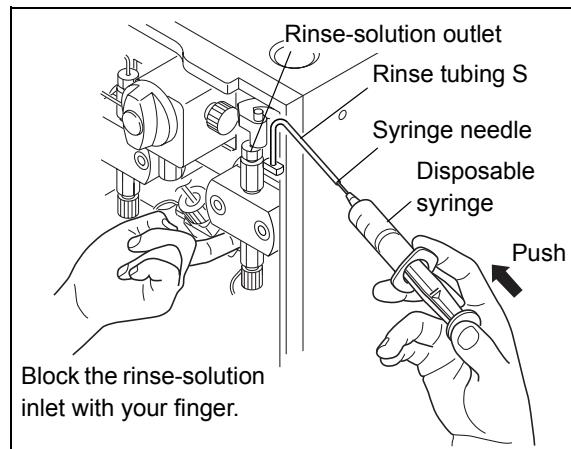


Fig. 8.23

# 8.4 Cleaning of Check Valves

The check valves are cleaned by pumping 2-propanol through the flow lines.

The procedure is described below.

- 1** Replace the mobile phase in the reservoir with 2-propanol.
- 2** Put the suction filter into the reservoir filled with the 2-propanol.
- 3** Unscrew the male nuts from both ends of the column, and remove the column from the flow line.
- 4** Screw the male nuts from the column into the ends of a resistor tube (0.1mm I.D. × 2m length).
- 5** Turn the power switch ON.  
Initial screen will appear.


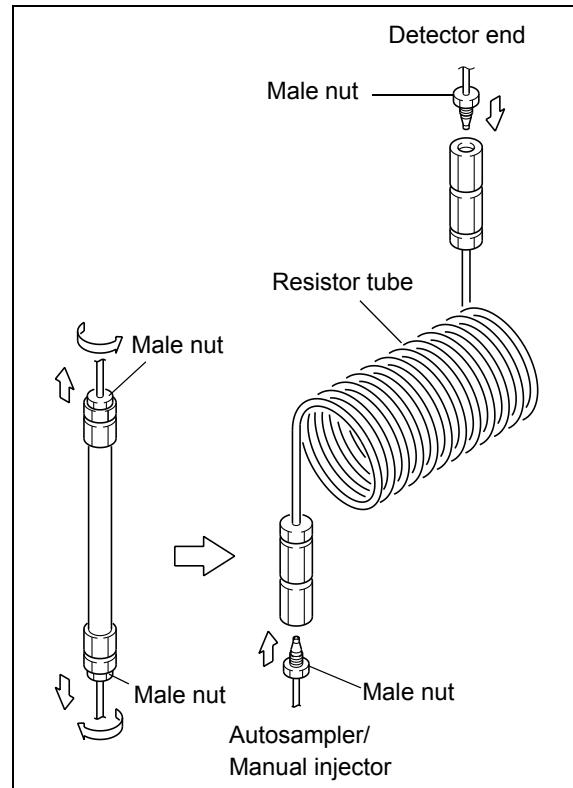


Fig. 8.24

- 6** Set the flow rate to 2mL/min. Set the concentration of mobile phase B to 0% when cleaning pump A's check valves and set the concentration of mobile phase B to 100% when cleaning pump B's check valves.  
☞ "4.1.2 Setting Flow Rate" P. 4-3  
☞ "4.1.3 Setting the Concentration of Mobile Phase B" P. 4-4

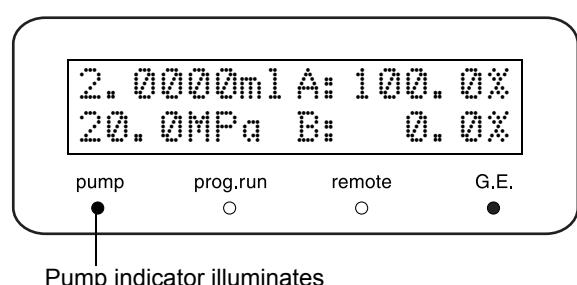

Pump indicator illuminates

- 7** Press **pump**.  
Pumping of 2-propanol will begin at a rate of 2mL/min, and the pump indicator will illuminate.  
Pump for at least 1 hour.

## 8.5 Inspection (Replacement) and Ultrasonic Bath Cleaning of Check Valves

Inlet and outlet check valves are mounted to the pump heads on the left and right of both pumps A and B. The procedure for removing, ultrasonic bath cleaning, inspecting, and replacing inlet and outlet check valves on the right of pump A is described below.

### Necessary parts

Part	Type	Part No.
Inlet check valve ASSY	Replacement part	228-45704-91
Outlet check valve ASSY	Replacement part	228-45705-91

### NOTE

Use one of the following measures to ensure that the mobile phase does not flow out of the end of the inlet-side tubing when the inlet-side tubing's male nut PEEK is removed.

- Place the reservoir lower than the pump inlet.
- Empty the reservoir and tubing of all mobile phase, and unscrew and remove the filter bushing from the pump inlet.

**1** Hold the outlet check valve using the provided wrench

**2** Loosen the male nuts at both ends of SUS tubing using the other wrench and remove SUS tubing.

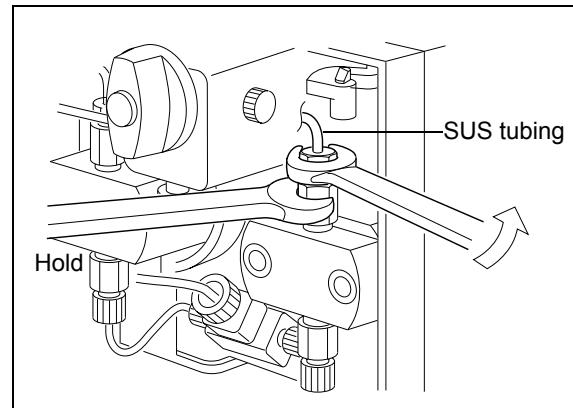


Fig. 8.25

- 3** Loosen male nut PEEK on the inlet-side tubing and remove it from inlet check valve.

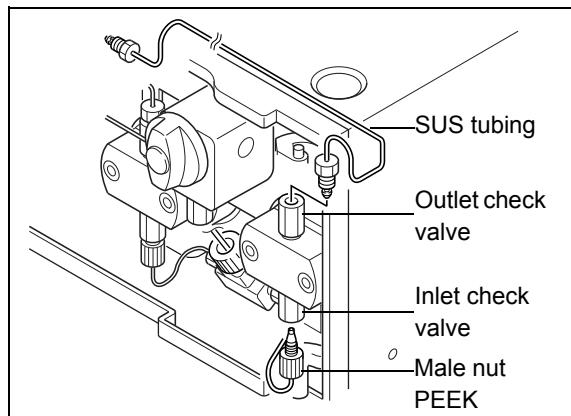


Fig. 8.26

- 4** Use the provided wrench to unscrew and remove the inlet and outlet check valves.

**⚠ CAUTION**

Do not disassemble the check valves for any reason. If they are disassembled, their performance may be affected.

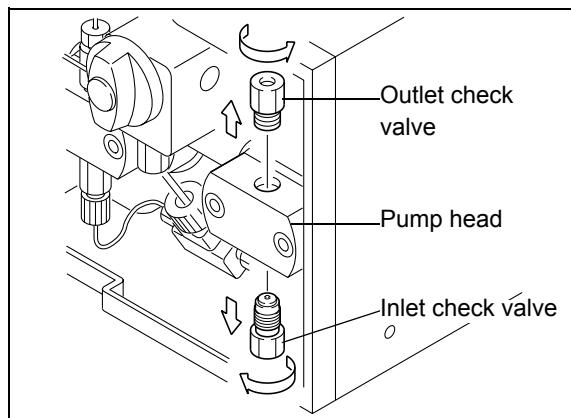


Fig. 8.27

- 5** Put the inlet and outlet check valves in a 2-propanol bath, and clean in an ultrasonic bath for 5 minutes.

- 6** Screw the inlet and outlet check valves back into the pump head, and tighten with the wrench.

- 7** Return SUS tubing, the inlet-side tubing, the suction filters, and the reservoir bottle to their original states.

## 8. Maintenance

8 Plug the instrument and turn the power switch ON.  
Initial screen appears.

9 To open the drain valve, turn the drain valve knob 180° counterclockwise.

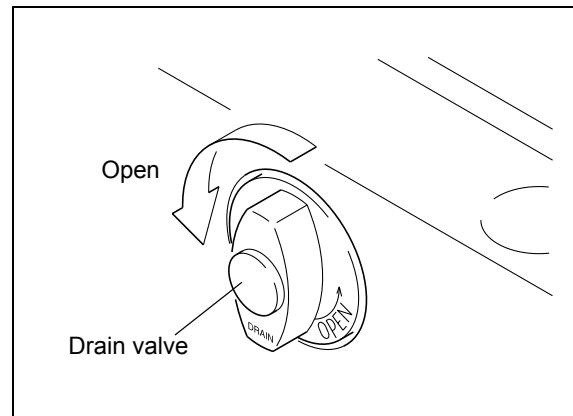



Fig. 8.28

10 Set the flow rate to 2mL/min.

"4.1.2 Setting Flow Rate" P. 4-3

11 Set the concentration of mobile phase B to 0% when cleaning check valves of pump A and set the concentration of mobile phase B to 100% when cleaning check valves of pump B.

"4.1.3 Setting the Concentration of Mobile Phase B" P. 4-4

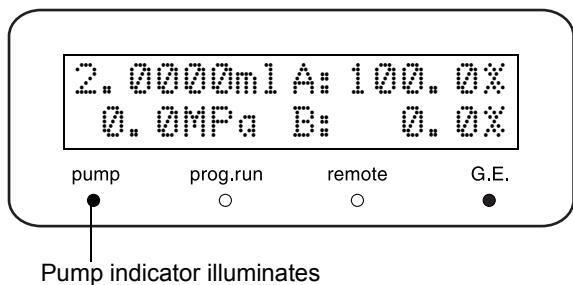

12 Press **pump**.

The pump indicator illuminates, and liquid flows from the drain tubing.

If liquid flows continuously, the check valves are functioning normally.

If the liquid does not flow continuously from the drain tubing, the check valves must be replaced.

# 8.6 Inspection (Replacement) and Ultrasonic Bath Cleaning of Line Filter

Necessary parts

Part	Type	Part No.
Frit	Consumable part	228-32744

- 1 Hold the line filter by the provided wrench.

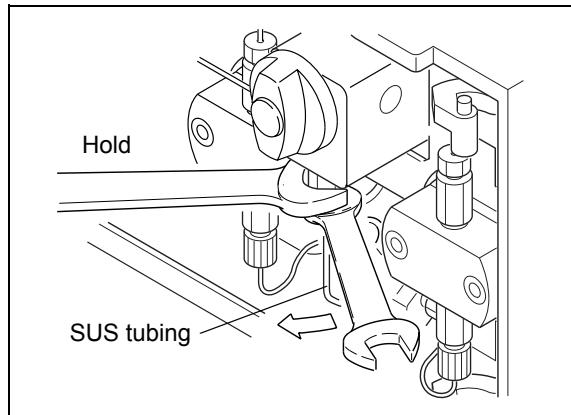


Fig. 8.29

- 2 Unscrew the male nuts on the end of the SUS tubing using another wrench, and remove the SUS tubing.

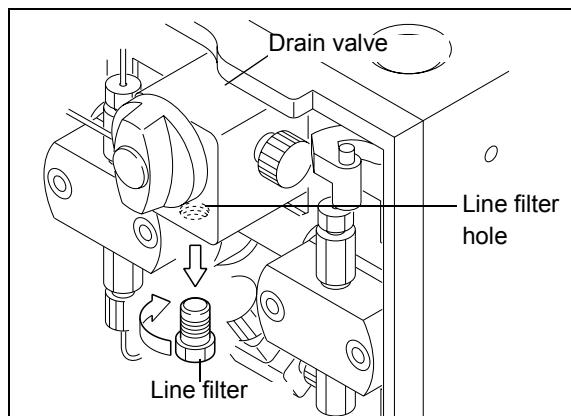


Fig. 8.30

- 3 Using the wrench, unscrew and remove the line filter.

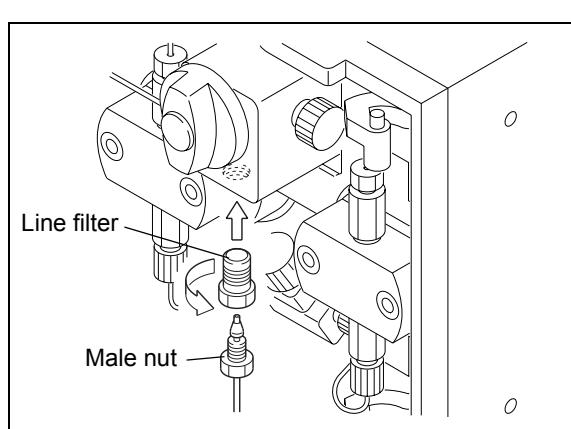


Fig. 8.31

- 4 Wipe any dirt from the line filter hole with a cotton swab.

- 5 Put the line filter in a bath of 2-propanol, and clean with an ultrasonic bath for 5 minutes.

- 6 Screw the line filter back into the line filter opening, and tighten it with the open-ended wrench.


- 7 Screw the male nut on the SUS tubing back into the line filter, and tighten the nut with the open-ended wrench.

## 8. Maintenance

**8** Turn the power switch ON.  
Initial screen appears.

**9** In a no load state, pump water at a rate of 1mL/min.

- If the pressure displayed does not exceed 0.3MPa, the line filter is functioning normally.
- If the pressure displayed exceeds 0.3MPa, the frit must be replaced.

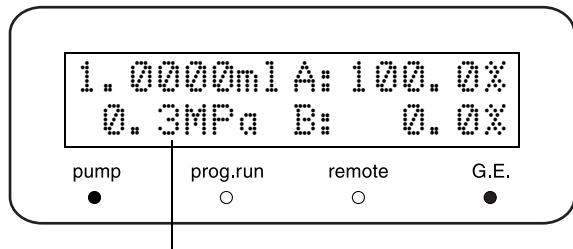

Filter is normal if this value is 0.3MPa or under.

### ■ Replacing Frit

- 1 Remove the line filter.  
☞ Perform steps 1 through 3 of the procedure in P.8-19.
- 2 Remove the frit on the end of the line filter body using nippers.

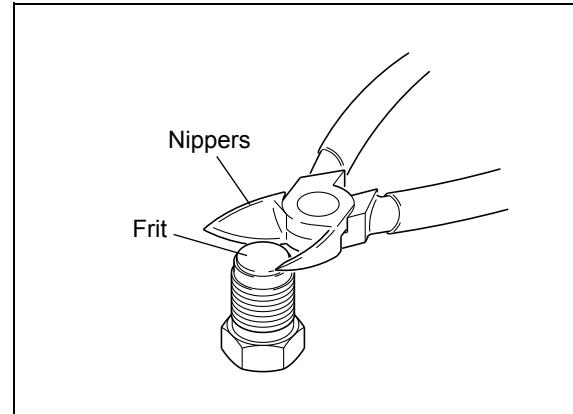


Fig. 8.32

- 3 Put a new frit into the line filter body.
- 4 Reinstall the line filter.  
☞ Perform steps 6 through 7 of the procedure in P.8-19.

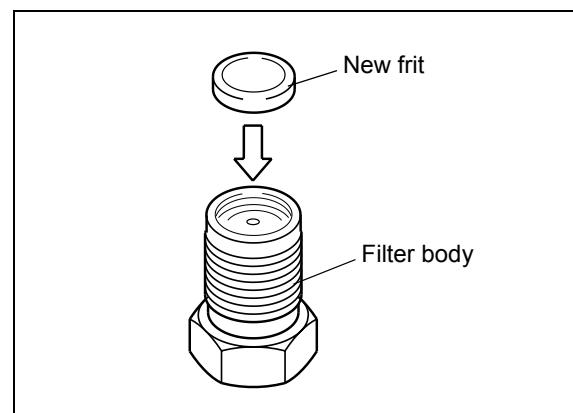


Fig. 8.33

## 8.7 Inspection (Replacement) and Ultrasonic Bath Cleaning of Suction Filter

Necessary parts

Part	Type	Part No.
Suction filter	Consumable part	228-43342-91

- 1 Pull the suction filter out of the suction tubing.
- 2 Clean the suction filter in a bath of 2-propanol, in an ultrasonic cleaning device for 5 minutes.

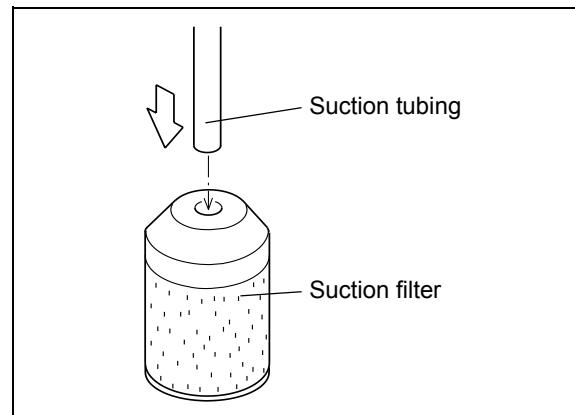


Fig. 8.34

- 3 Insert the suction tubing into the suction filter.
- 4 Turn the power switch ON.  
The initial screen appears on the display.
- 5 Pump water at 1mL/min for 10 minutes.
- 6 Check that air bubbles do not accumulate inside the solvent tubing.  
If they do, the tubing must be replaced.

## 8.8 Replacement of Drain Valve ASSY

Necessary parts

Part	Type	Part No.
Drain valve ASSY	Replacement part	228-45574-91

- 1** Unscrew the drain valve ASSY by turning counterclockwise. And pull it in straight line.

**NOTE**

Confirm that there are no alien substance in the hole.

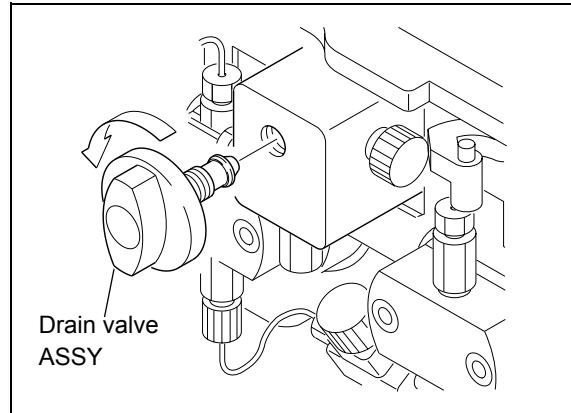


Fig. 8.35

- 2** Wet the seal of the new drain valve ASSY by using the 2-propanol, and insert it into the hole of the housing in a straight line.

**NOTE**

If the drain valve assy is inserted slantwise and forcefully, the seal can deform. As a result, the sealing of the seal cannot be maintained.

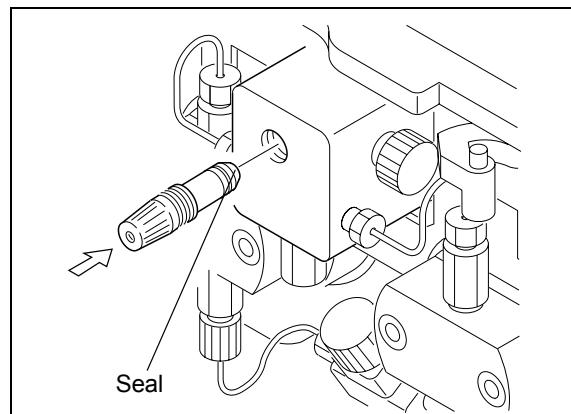


Fig. 8.36

- 3** Screw the new drain valve ASSY as far as it will go to close.

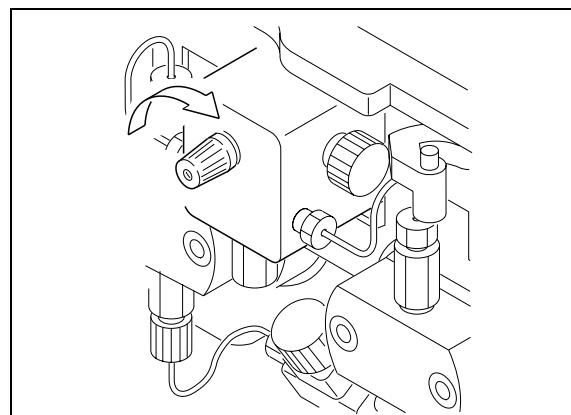


Fig. 8.37

- 4** Screw the knob to the drain valve ASSY and insert the cap into the knob, while the knob position is vertical.

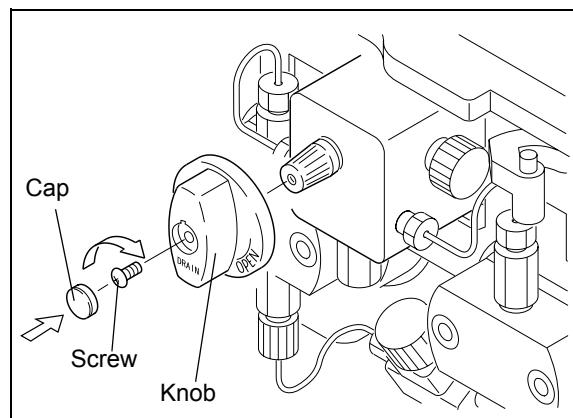


Fig. 8.38

## 8.9 Replacement of Fuse

### **⚠ WARNING**

- Before replacing fuses, turn off the power and unplug the instrument.
  - For replacement, only use fuses of the correct type and rating.
- Failure to heed the above could result in fire, electric shock or short circuits.

The correct rating of the fuses is:

Necessary parts

Part	Type	Part No.
250V 5AT (5 × 20)	Replacement part	072-02004-23

- 1** Pull out the fuse holder by using a coin.

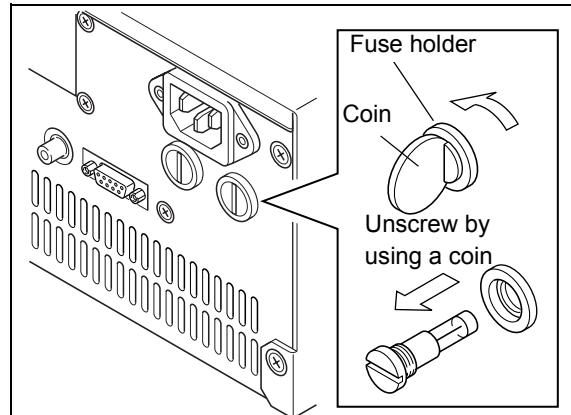


Fig. 8.39

- 2** Place new fuses into the fuse holder.

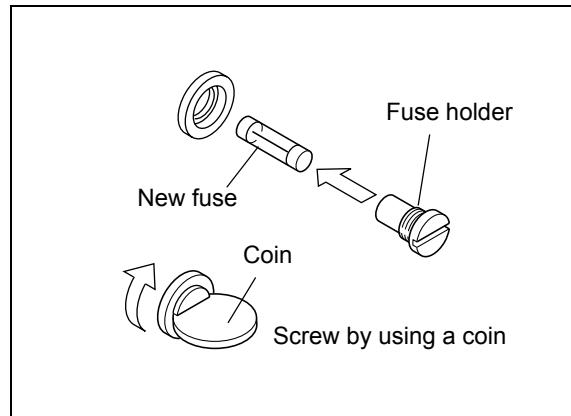


Fig. 8.40

- 3** Push the fuse holder in and fix by using a coin.

## 8.10 Wiping of Leak Tray

The protective plate is attached on the leak tray in order to protect the leak sensor and to guide the leakage to sensor and drain outlet.

Wipe away the leakage on the leak tray completely, as below.

**NOTE**

When a buffer solution is used as the mobile phase, it may deposit crystals on the leak tray when it evaporates. Wipe the dirt on the leak tray with cloth soaked in water, as below.

- 1 Rotate the protective plate, to bring the leak tray and the leak sensor into sight.

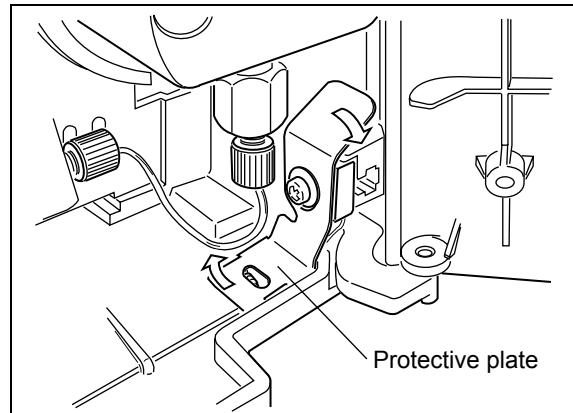


Fig. 8.41

- 2 Wipe away the leakage around the leak sensor and on the leak tray completely.

**NOTE**

- Don't twist and pull the leak sensor.
- Wipe the dirt on the leak tray with cloth soaked in water.

- 3 Re-rotate the protective plate.

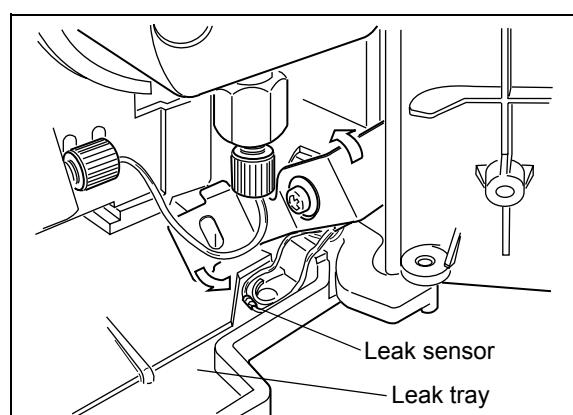


Fig. 8.42

**⚠ CAUTION**

- Make sure to re-rotate the protective plate after the wiping.  
Leak sensor may not detect leakage without the protective plate.

## 8.11 Exterior Cleaning

If the instrument cover or front panel becomes dirty, wipe it clean with a soft dry cloth or tissue paper. For persistent stains, clean the exterior using the following procedure.

- 1** Dip a piece of cloth in a dilute neutral detergent and twist firmly to remove excess liquid. Use this cloth to scrub the soiled area of the exterior surface of the instrument.
- 2** Dip a piece of cloth into water and twist firmly to remove excess liquid. Use this cloth to wipe away all the remaining detergent. Use a dry cloth to remove all moisture from the exterior surface of the instrument.

**NOTE**

Do not allow spilled water to remain on the instrument surface, and do not use alcohol or thinner-type solvents to clean the surfaces. These can cause rusting and discoloration.

# 9

---

## Technical Information

### Contents

9.1	Installation .....	9-2
9.2	Specifications .....	9-37
9.3	Maintenance Parts .....	9-39
9.4	Introduction to HPLC System.....	9-41
9.5	Mobile Phase Characteristics.....	9-44

# 9.1 Installation

---

## 9.1.1 Installation Site

---

### ■ Suitable Sites and Preparation

To ensure safe operation, install the instrument in a suitable location that satisfies the following conditions.

#### **WARNING**

- Ample ventilation

The solvents used with the HPLC system are often flammable and toxic.

Therefore, the room where the instrument is installed must be well-ventilated.

- No fire sources used near the instrument

The solvents used with the HPLC are often flammable. Therefore, the use of open flame where the instrument is installed must be strictly prohibited. Also, do not install in the same room with equipment that emits or could potentially emit sparks.

- Fire extinguishers permanently available

Have fire extinguishers permanently available in case of fire.

- Protective equipment provided near the instrument

If solvent gets into the eyes or onto the skin, it must be flushed away immediately.

Provide equipment, such as eye wash stations and safety showers, as close to the instrument as possible.

#### **CAUTION**

- Avoid dust or corrosive gas

To ensure a long service life of the instrument and preserve its performance levels, avoid installing it in places subject to large amounts of dust or corrosive gas.

- Keep away from equipment generating strong magnetic fields

To ensure proper operation, do not install the instrument in places subject to strong magnetic fields.

If the power supply line is subject to high electrical noise, install a surge protector.

- Install the instrument in the location that satisfies the following conditions to preserve the performance:

- room temperature is between 4 and 35°C, with minimal temperature variation through a day.
- air currents from heating or air conditioning equipment are not directed on the instrument.
- sunlight does not shine directly on the instrument.
- there is no vibration.
- humidity stays within 20 - 85%.
- place without condensation

## ■ Required Installation Space

### **CAUTION**

- The weight of this instrument is 13kg. During installation, consider the entire weight combined with other LC components.  
The lab table on which this instrument is installed should be strong enough to support the total weight of the LC system. It should be level, stable and have depth of at least 600mm.  
If these precautions are not followed, the instrument could tip over or fall off the table.
- Keep at least 100mm between the rear of the instrument and the wall.  
This allows for sufficient air circulation to provide cooling and prevent the instrument from overheating and impairing the performance.

Typical system configurations and required installation spaces are shown in the figures below.

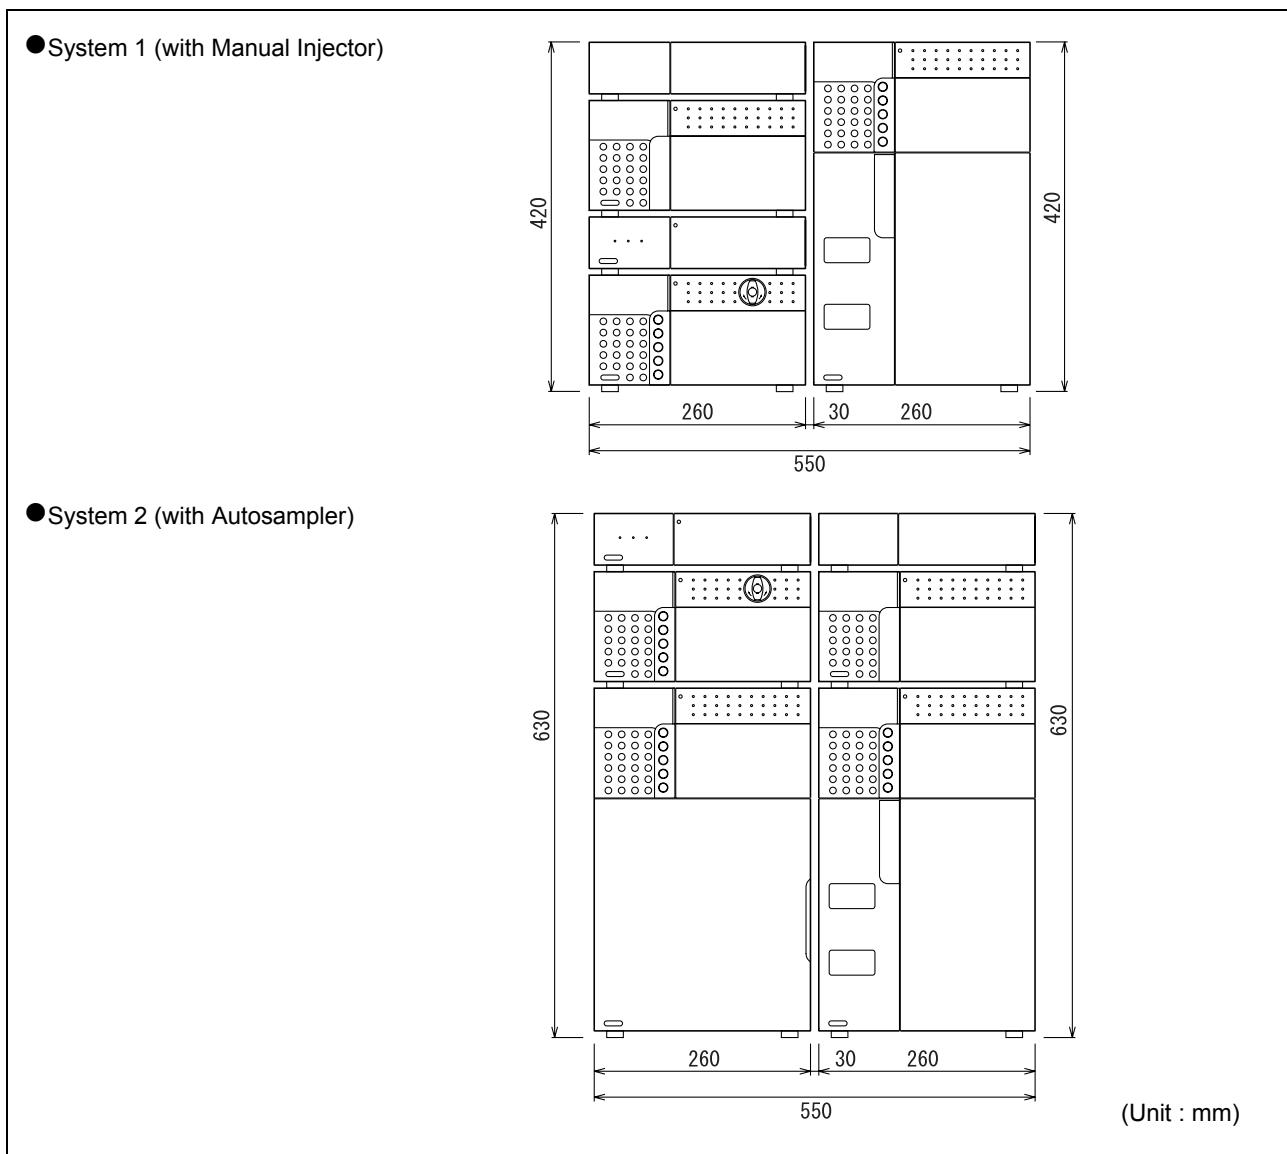


Fig. 9.1

## 9. Technical Information

### 9.1.2 Installation

#### ■ Remove the Shipping Screws

In order to prevent shock during transportation, the instrument is fixed with the shipping screws. Remove these screws prior to installation.

**NOTE**

When the instrument is used without removing the shipping screws, system makes noise because of vibration.

- 1** Loose and remove the shipping screws (with washer).

 "2.3 Right Side and Base Panel" P. 2-5

#### ■ Installation

The instrument is designed for stacking with other Shimadzu HPLC components.

 "9.4 Introduction to HPLC System" P. 9-41

 **CAUTION**

When the LC-20A series components are stacked on each other, the clearance between the components is only 5 mm.

Use caution to avoid pinching your fingers between the components.



Fig. 9.2

#### ■ Stacking Brackets

The use of commercially available stacking brackets is recommended. These brackets limit the possibility of the instrument falling off the lab table during an earthquake or the like. Various grades of stacking brackets are available.

Fasten the instrument firmly in place by attaching stacking brackets to both the right and left sides. For more details, contact your Shimadzu representative.

An example of stacking bracket placement is shown in "Fig. 9.3".

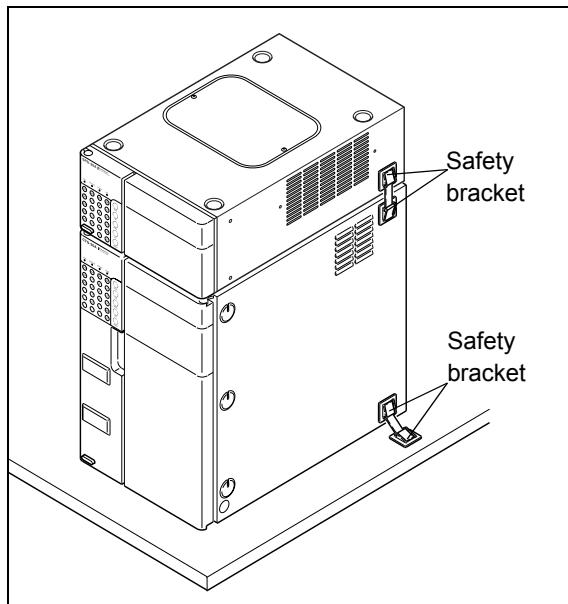


Fig. 9.3

### 9.1.3 Power Supply Connection

The following table shows the electrical voltage, power consumption, and frequency.

Part No.	Power Supply Voltage (indicated on the instrument)	Consumption	Frequency
228-45002-31	AC100-120V(100-120V~)	180VA	50/60Hz
228-45002-32	AC100-120V(100-120V~)		
228-45002-38	AC220-240V(220-240V~)		

Verify that the power outlet to be used for connection has sufficient capacity. If capacity is insufficient, a power outage or voltage drop can occur, affecting not only this instrument, but other instruments connected to the same power supply.

#### ■ Connection to Power Outlet

##### **⚠ WARNING**

Handle the power cord with care, and observe the following precautions to avoid cord damage, fire, electric shock or instrument malfunction.

- Do not place heavy objects on the cord.
- Keep hot items away from the cord.
- Do not modify the cord.
- Do not bend the cord excessively or pull on it.
- To unplug the instrument, pull the plug itself, NOT the cord.

If the cord is damaged, replace it immediately.

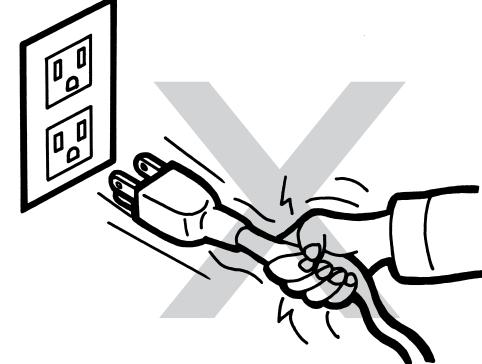


Fig. 9.4

##### **⚠ CAUTION**

Before plugging in the instrument, make sure that the power switch is OFF.

- 1 Insert the connector side of the power cord into the power cord connector at the back of the instrument.
- 2 Insert the plug side of the power cord into the power supply outlet.

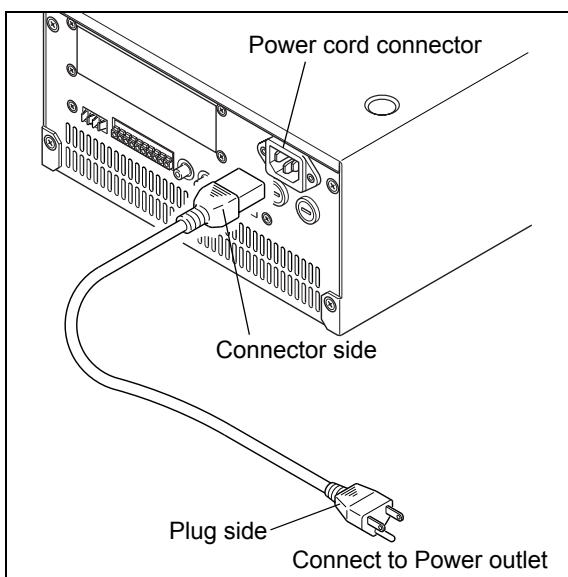


Fig. 9.5

### ■ Grounding

#### ⚠ WARNING

The three-line type power cable provided as an accessory includes the grounding wire. Be sure to ground through this cable in order to prevent electrical shock and to ensure stable operation of the instrument.

### 9.1.4 Prior to Plumbing

Many different types of tubings and connectors are used to plumb the instrument at installation. It is necessary to cut tubings and mount connectors prior to the plumbing. In this section, instructions and precautions for these preparations are described.

### ■ Types of Tubings and Connectors

The tubing and connectors used for the plumbing are made of stainless steel (SUS) or resin as follows.

#### Stainless steel (SUS)

- Stainless steel tubing 1.6 O.D. × 0.3 I.D.
- Male nuts, 1.6 MN
- Ferrules 1.6F

#### Resin

- FEP tubing, PTFE tubing, ETFE tubing, PEEK tubing, PE tubing, etc.
- Male nut PEEK
- PEEK ferrules
- PTFE ferrules

### ■ Cutting Tubings

Cut provided tubing to the proper lengths for installation.

#### Cutting SUS Tubings

- 1 Position the provided file (for cutting SUS tubing) diagonally against the tubing, and cut up around the tubing.

#### NOTE

Cut up the tubing so that the cut surface is at a right angle.

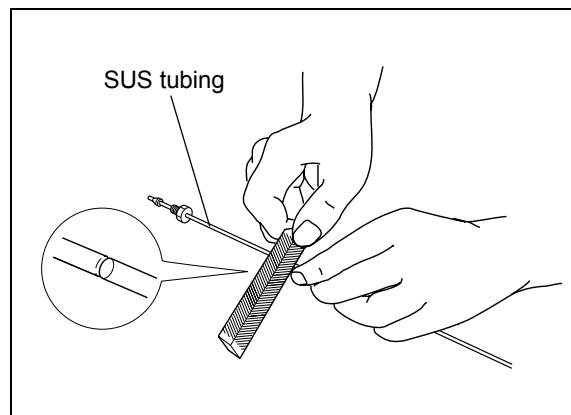


Fig. 9.6

- 2 Holding the tubing at equal distances from the cutting up line, bend it up and down and from side to side to cut off.
- 3 File the cut surface to make smooth and straight.

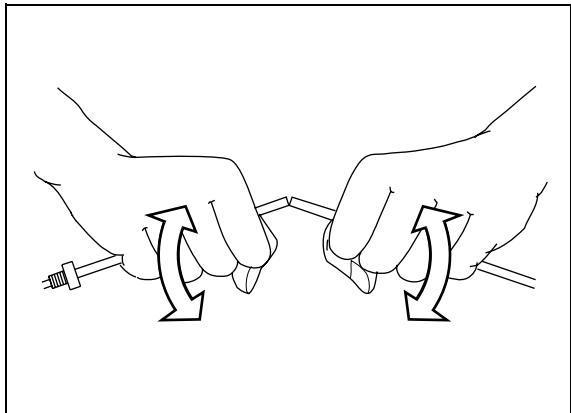


Fig. 9.7

**⚠ CAUTION**

- Make the cut surface at right angle. Otherwise, dead volume will be created and may cause chromatographic peak broadening.
- Make sure that the inner diameter of the tubing is not deformed. Otherwise, the tubing may be clogged.

### Cutting Resin Tubings

Cut off the resin tubing at a right angle using a cutter.

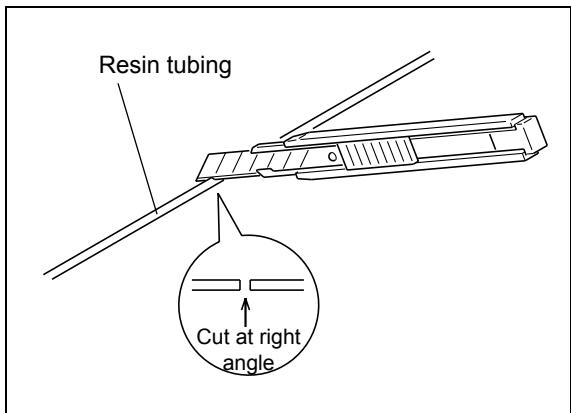


Fig. 9.8

### ■ Connecting Tubings

- 1 Mount a male nut and a ferrule to the tubing.

#### ⚠ CAUTION

Install stainless steel male nuts and ferrules on SUS tubing, and resin nuts and ferrules on resin tubing. If resin male nuts are mounted on SUS tubing, the nuts will be damaged and leakage may occur.

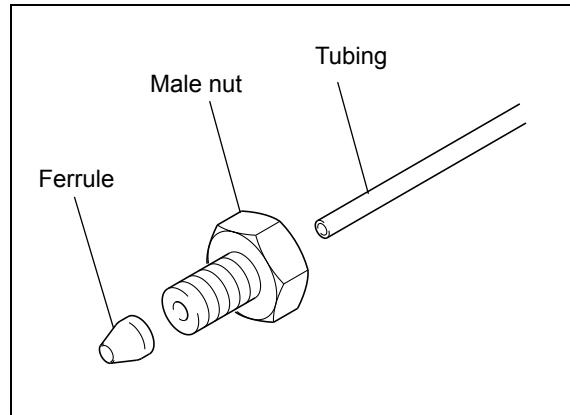


Fig. 9.9

- 2 Insert the end of the tubing, with the ferrule on it, into the appropriate opening. Then tighten the male nut.  
The ferrule will be secured on the tubing.

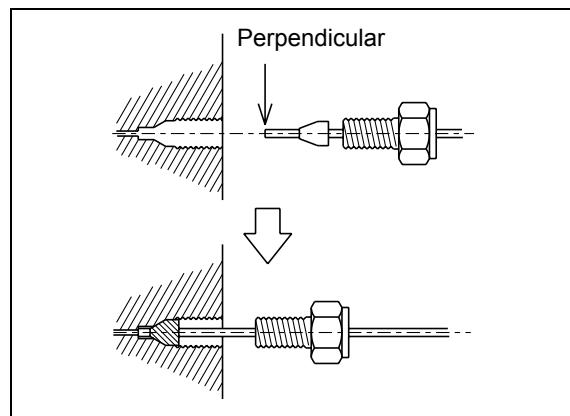


Fig. 9.10

#### ⚠ CAUTION

- Insert the tubing completely into the opening, until it butts against the end of the opening.  
Otherwise, dead volume will be created and may cause chromatographic peak broadening.
- Do not overtighten the male nut.  
Otherwise, the threads will be damaged.

#### NOTE

- For an SUS male nut:  
Use the open-end wrench (provided) to tighten and loosen the nut.  
If the nut is to be connected to a union or other part that is not secured, use a second wrench to secure the union.
- For a resin male nut:  
Tighten and loosen the nut by hand.

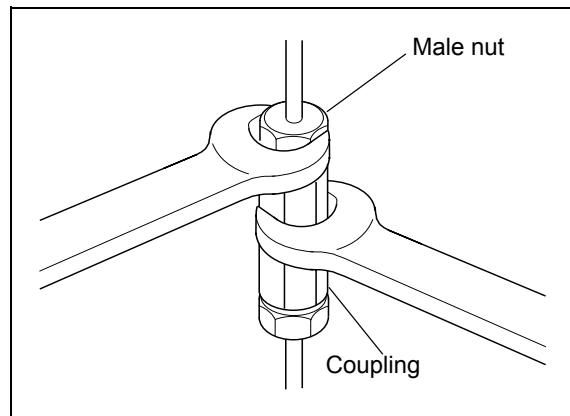


Fig. 9.11

- 3** Loosen and move the male nut slightly to verify that the ferrule is secured on the tubing.

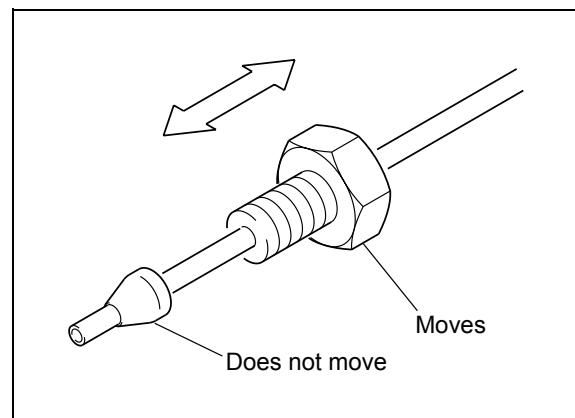


Fig. 9.12

### ■ Protective Plugs

Inlets and outlets of the instrument are fitted with protective plugs (bushings, stop plugs, caps and similar items) to keep out dirt and dust during shipment.

When the inlet and outlet are not connected to other thing, keep the protective plugs on. Otherwise, dirt and dust may cause clogging of the instrument.

Keep the plugs, and replace them when the instrument will be left not in use for a long time.

#### NOTE

- For stop plugs:  
Use the wrench provided to unscrew and screw in the plugs.
- For resin plugs:  
Remove and replace the plugs by hand.

## 9. Technical Information

### 9.1.5 Plumbing

#### ⚠ CAUTION

- Before plumbing, turn OFF the power supply to all the system components and unplug them.
- For plumbing, use the appropriate parts listed in "1.3 Component Parts".
- Connect only the tubing described in the instructions.  
Otherwise, injury or equipment failure may cause.

The necessary plumbing is as follows:

- Plumbing of suction filter . . . . . Plumbing to form the flow line from the reservoir bottles to the pump.
- Plumbing of drain tubing . . . . . Plumbing to check the performance of the instrument before operation.
- Plumbing of tubing for leakage . . . . . Plumbing to evacuate If leaks occur in any of the instrument in a stack, this tubing directs it down to the lowest device in the stack, and from there to a waste container.

#### NOTE

For details on plumbing when the optional degasser and/or reservoir switching valve is/are used, see the instruction manual(s) for these options.

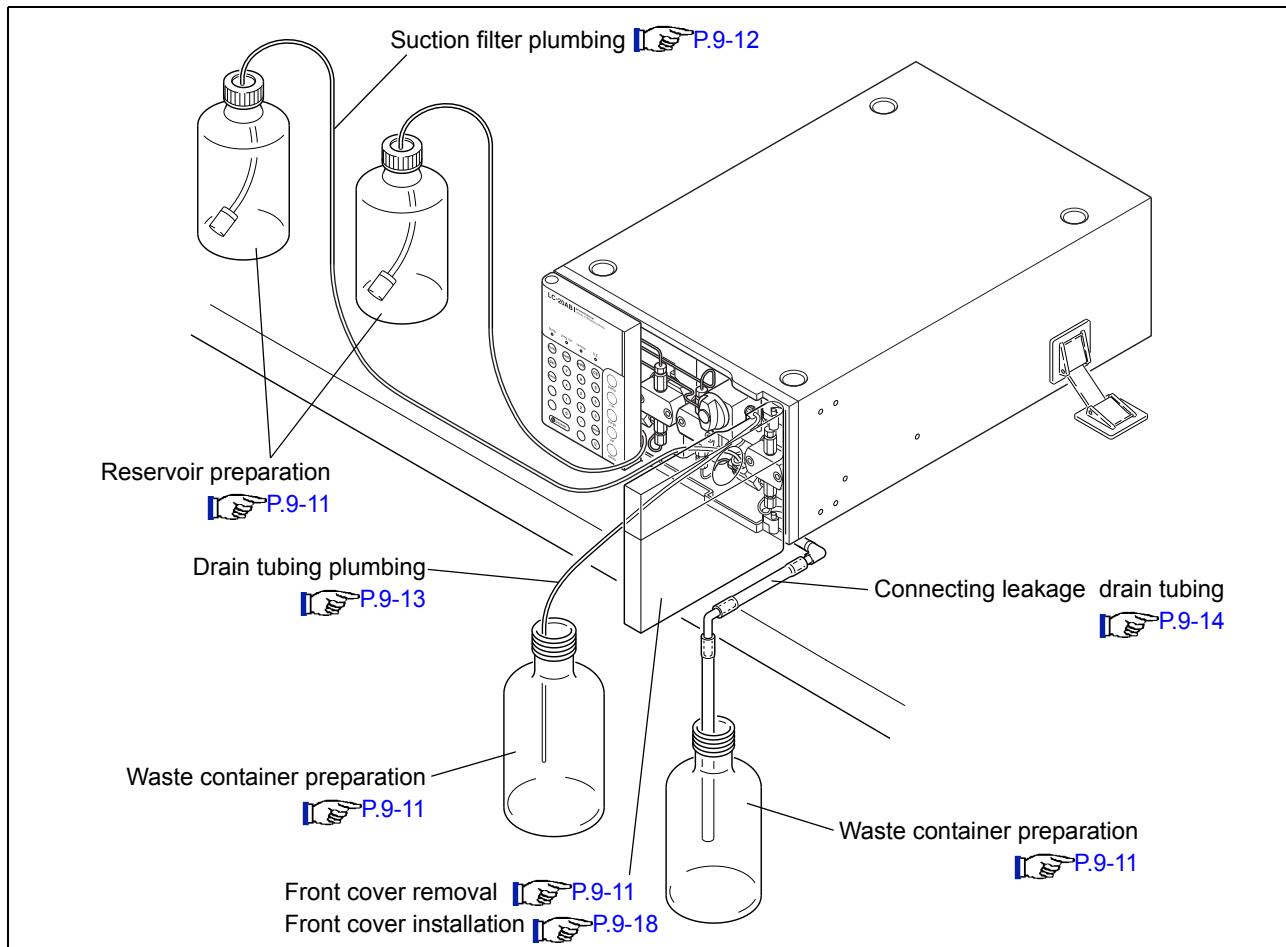


Fig. 9.13

## ■ Reservoir and Waste Container Preparation

Before connecting the plumbing, prepare (a) reservoirs and (b) waste container (to receive the mobile phase after analysis and to collect leakage).

### **⚠ WARNING**

Do not use cracked or damaged bottles.

The reservoir should be made of glass and have a capacity of at least 500mL.

### **⚠ CAUTION**

The waste container must be positioned lower than the instrument (for example, on the floor). If it is positioned higher than the instrument, liquid will not drain, and will leak from the connections.

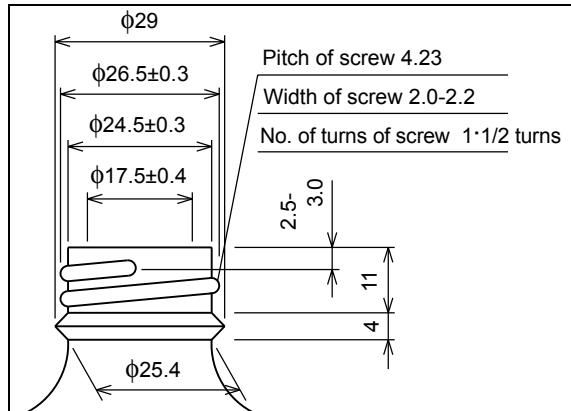


Fig. 9.14

## ■ Front Cover Removal

The front cover must be removed in order to perform the plumbing.

- 1 Press on the cover at the position indicated in the figure, and release to open the front cover.

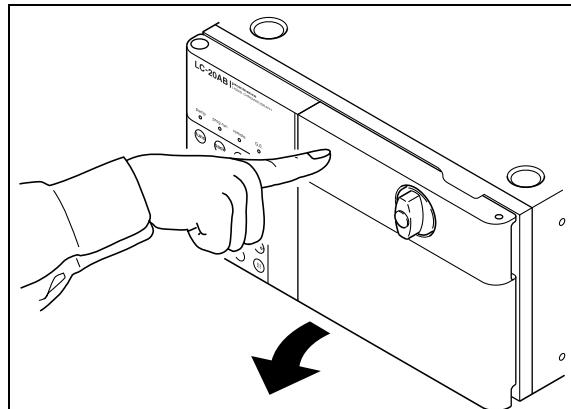


Fig. 9.15

- 2 Hold the front cover upward and remove.

### **NOTE**

The front cover can be removed at 120 degree of open angle.

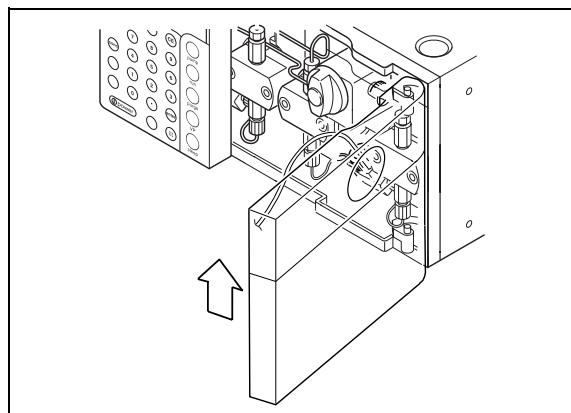


Fig. 9.16

### ■ Suction Filter (Accessory) Installation

**NOTE**

Prevent any dirt from adhering to the filter portion of the filter when installing it.

Dirt on the filter could cause clogging and flow rate fluctuations.

**NOTE**

In order to ensure stable analysis at all times, the mobile phase should be degassed.

For details of the degassers,  "1.4 Optional Parts" P. 1-5

- 1** Remove the ferrule, bushing and coil spring from the filter tubing.

- 2** Cut the tubing to a length appropriate for connecting the reservoir bottle and the pump suction port.

- 3** Pour mobile phase into the reservoir.

●Suction filter (assembly)

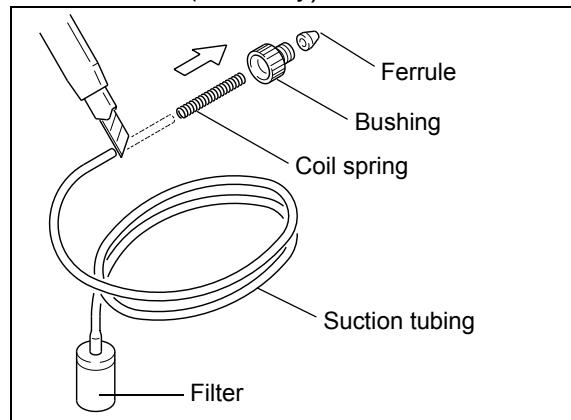


Fig. 9.17

- 4** Put the filter into the reservoir, pass the tubing through the hole in the lid and through the bolt cap, place the lid into the bottle mouth, and screw the bottle cap on.

**NOTE**

The filter should touch the bottom of the bottle.

- 5** Replace the ferrule, bushing and coil spring on the tubing.

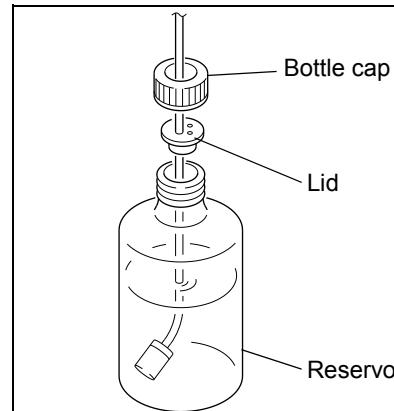


Fig. 9.18

- 6** Remove the shipping bushing from the pump A inlet.

**NOTE**

Replace it if the instrument is out of use for a long time, to prevent foreign matter from entering the inlet. Retain the shipping bushing after removal.

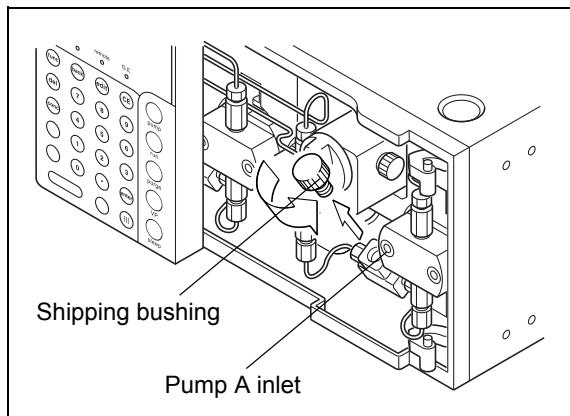


Fig. 9.19

- 7** Attach the ferrule and bushing on the end of the tubing into the pump A inlet.

**NOTE**

When arranging the tubing upwards, fix it with tubing clamp.

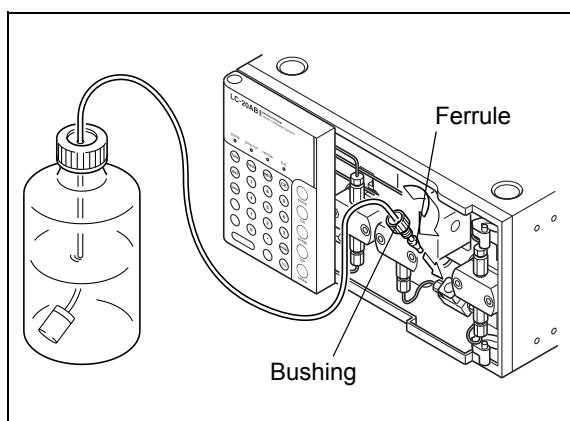


Fig. 9.20

- 8** Connect to pump B in the same way.

9

**■ Drain Tubing (Accessory) Installation**

- 1** Remove the shipping cap from the drain tubing connection port.

**NOTE**

Keep the shipping cap after removal and attach it again if the instrument will not be used for a long time to prevent foreign matter from entering the port.

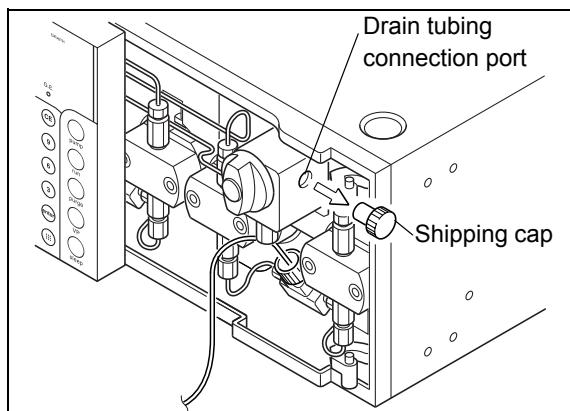


Fig. 9.21

## 9. Technical Information

**2** Screw the male nut of the drain tubing into the drain tubing connection port.

**3** Put the other end of the drain tubing into the waste container.

**NOTE**

To ensure a smooth flow of liquid, put the tubing into the bottle with its end pointing downward.

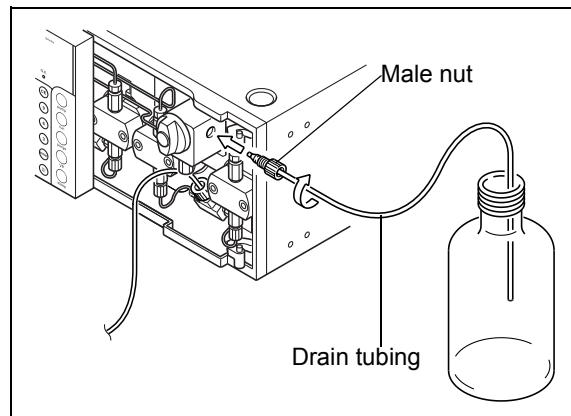


Fig. 9.22

### ■ Connecting Leakage Drain Tubing

This instrument is designed so that if leaks occur internally (except the column oven), the leaked liquid flows down to the lowest level of the instrument and is drained into the waste container.

The procedure for connecting leakage drain tubing is given below.

(Except for the waste container, all parts shown in the figure on the right are standard accessories.)

**NOTE**

- For connecting, cut a silicone tubing into the length in which both of the cut parts will not sag.
- Set the silicone tubing so that its edge does not touch the liquid surface in the waste container.

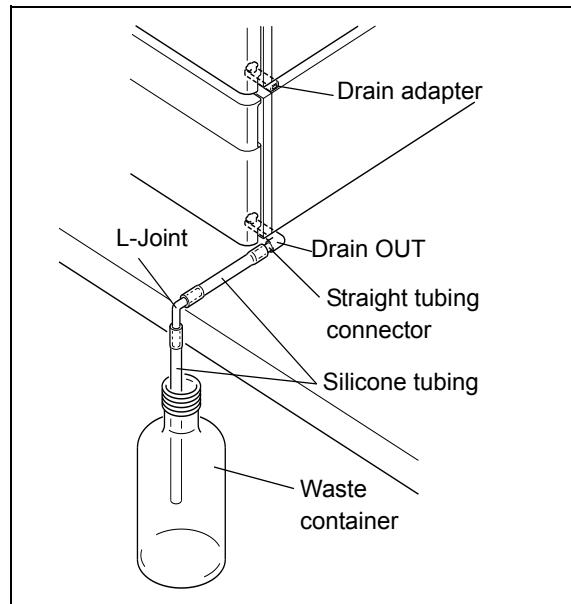


Fig. 9.23

### Bottom of Instrument

- 1** Insert the drain OUT, STD into leakage drain outlet from the front of the instrument.

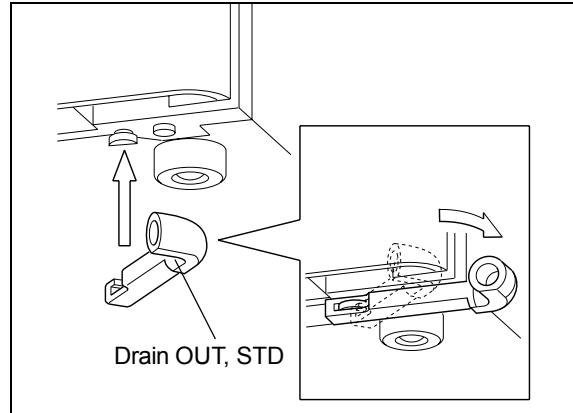


Fig. 9.24

- 2** Turn the drain OUT, STD counterclockwise 45° to secure.

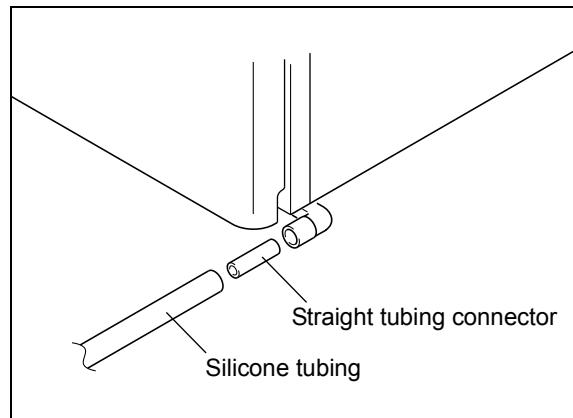


Fig. 9.25

- 3** Connect one end of the silicone tubing adapter to the drain OUT, STD with a straight tubing connector.

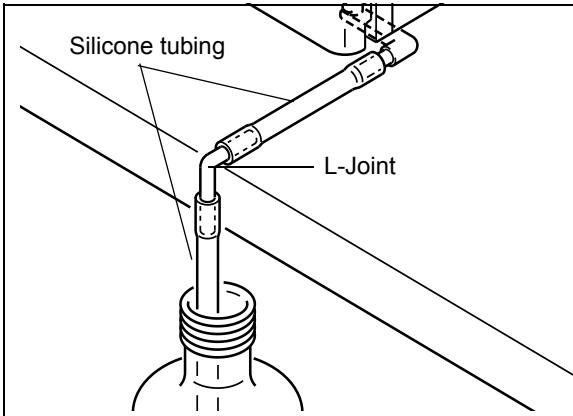


Fig. 9.26

- 4** Cut the silicone tubing at the edge of the table, and connect an L-Joint. Let the L-Joint head downward as in the right figure and connect the other cut part of the silicone tubing.

- 5** Insert the other end of the silicone tubing into the waste container.

**NOTE**

To ensure a smooth flow of liquid, insert the silicone tubing into the container with its tip pointing downward.

### Second Instrument from Bottom

#### NOTE

Leaks from the column oven are drained separately (See column oven Instruction Manual.).

If any components are installed on top of the column oven, carry out the same procedure as in "Installation on top of the column oven" on next page.

Also, when the bottom unit has no leakage hole ("Fig. 9.28"), carry out the same procedure as in "Installation on top of the column oven" on next page.

- 1** Insert the drain adapter into the position shown in the illustration, and slide it on the instrument of bottom.

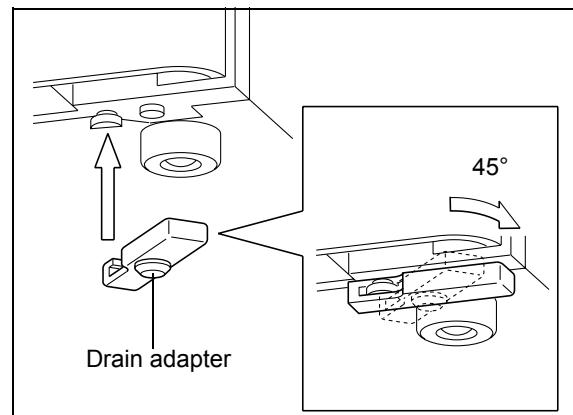


Fig. 9.27

- 2** The drain adapter connects the drain outlet to the leakage hole of the bottom unit.
- 3** Pour some water onto a spot near the drain outlet of the top unit, and verify that the water flows to the waste container.

#### ●Cross-section of connection parts

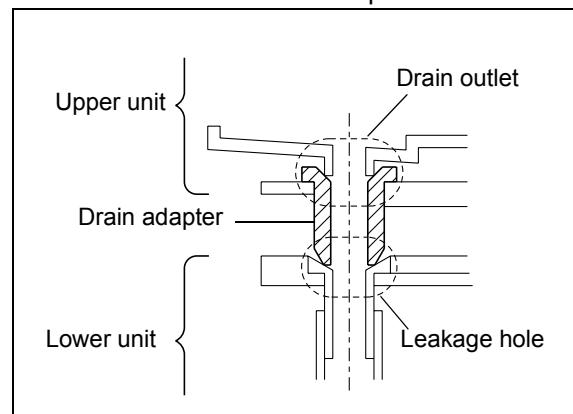


Fig. 9.28

## Installation on Top of the Column Oven

**NOTE**

When the bottom unit has no leakage hole ("Fig. 9.28"), carry out the same procedure described below.

- 1 Insert the drain OUT, CTO into leakage drain outlet from the front of the instrument.

- 2 Turn the drain OUT, CTO counterclockwise 45° to secure.

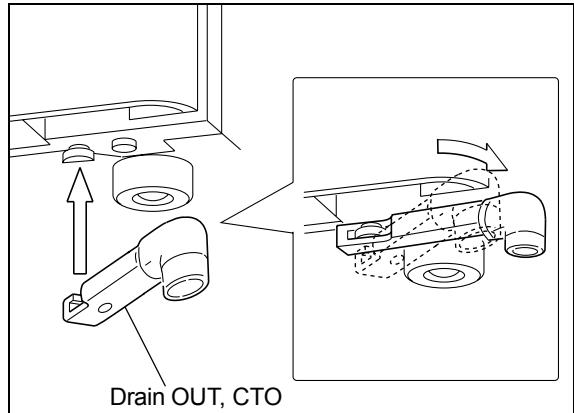


Fig. 9.29

- 3 Connect one end of the silicone tubing adapter to the drain OUT, CTO with a straight tubing connector.

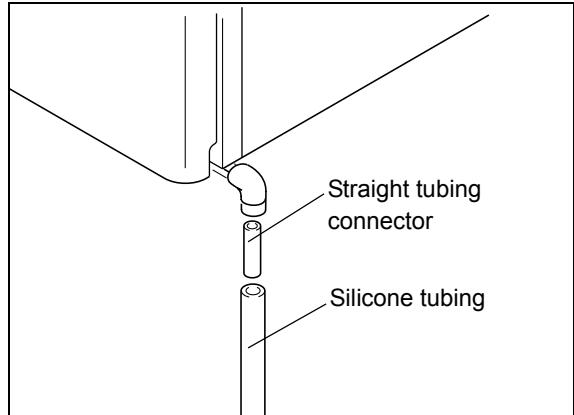


Fig. 9.30

- 4 Insert the other end of the silicone tubing into the waste container.

"Fig. 9.13"

**NOTE**

- To ensure a smooth flow of liquid, insert the silicone tubing into the container with its tip pointing downward.
- Set the silicone tubing so that its edge does not touch the liquid surface in the waste container. When the tip of tubing touches into the liquid of waste container, the drainage becomes difficult to flow.

## 9. Technical Information

### ■ Front Cover Installation

- 1** After performing the plumbing, install the front cover using the reverse of the removal procedure.
- 2** Close the front door.

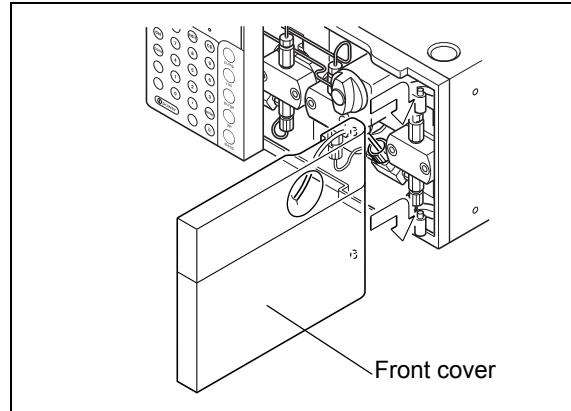


Fig. 9.31

### 9.1.6 Installation of Manual Injector and Column

The procedures in this section covers installation of the manual injector and column installation. For similar column oven installation procedures, see the column oven instruction manual.

### ■ Installation of Manual Injector

Use the manual injectors listed below.

Option name	Part No.	Features
Manual injector Type 7725	228-32210-91	Manual injector for general purpose analysis. Standard sample loop: 20µL
Manual injector Type 7725i	228-32210-93	Same as type 7725, but with a position sensing switch. Can send signals synchronized with injection of samples to system controller or Chromatopac.
Semi-micro manual injector Type 8125	228-23200-91	Manual injector for semi micro volume range. Standard sample loop: 5µL. Includes position sensing switch. Can send signals synchronized with injection of samples to system controller or Chromatopac.
Non-metallic manual injector Type 9725	228-32650-91	Has liquid-contacting parts made of non-metallic materials. Maximum use temperature: 60°C
Non-metallic manual injector Type 9725i	228-32650-93	Same as type 9725, but with a position sensing switch. Can send signals synchronized with injection of samples to system controller or Chromatopac.

- 1** Attach the injector installation plate (option) onto the instrument with accessory screws.

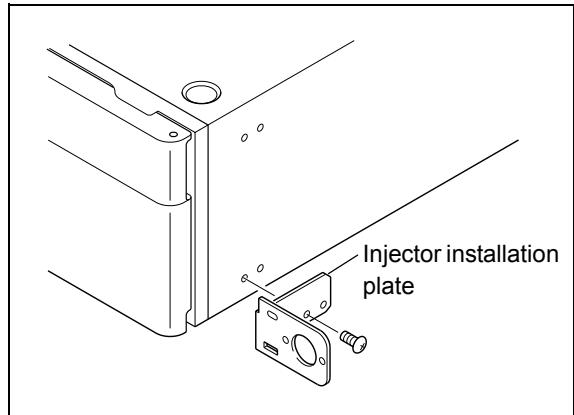


Fig. 9.32

- 2** Attach the manual injector to the installation plate with the screws attached to the injector.  
(For more detailed instructions, see the instruction manual for the used manual injector.)

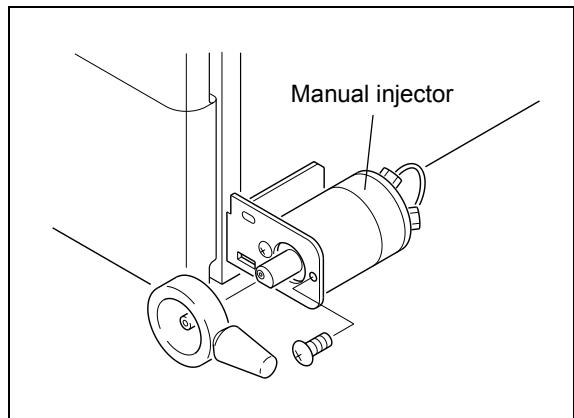


Fig. 9.33

- 3** Insert the vial holder provided with the installation plate into the vial holder opening in the plate.
- 4** Insert the vial provided with the installation plate into the vial holder.

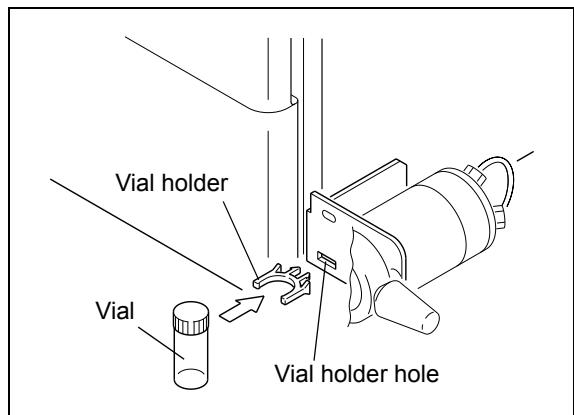


Fig. 9.34

## 9. Technical Information

### ■ Installation of Column Holder

- 1** Attach the column holder to the pump with the provided screws.

- 2** Orient the column with its outlet at the top, and attach it to the column holder.

The orientation of the column should be as shown in the figure on the right.

Verify that the column is securely clamped.

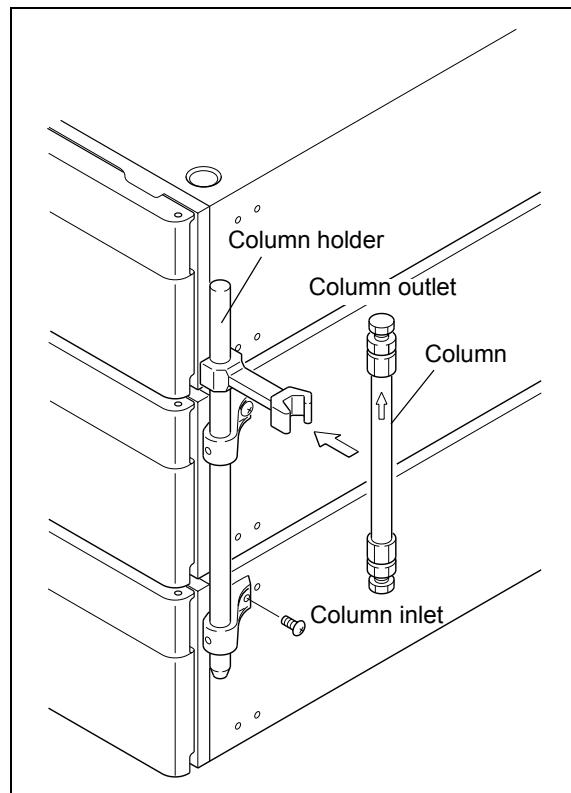


Fig. 9.35

### 9.1.7 Flow Line Plumbing

#### ■ Manual Injector Plumbing

**NOTE**

For connecting ports 1 to 6 of the manual injector, use the male nuts (with long bushing) and ferrules, provided as manual injector standard accessories.

- 1** Screw the sample loop male nuts (with long bushing) into ports 1 and 4 of the manual injector.
- 2** Install a male nut (with long bushing) and ferrule to one end of each of the two waste liquid tubing sections. Then attach the tubing and ferrules into ports 5 and 6 of the manual injector. Tighten the nuts.

● Back of manual injector

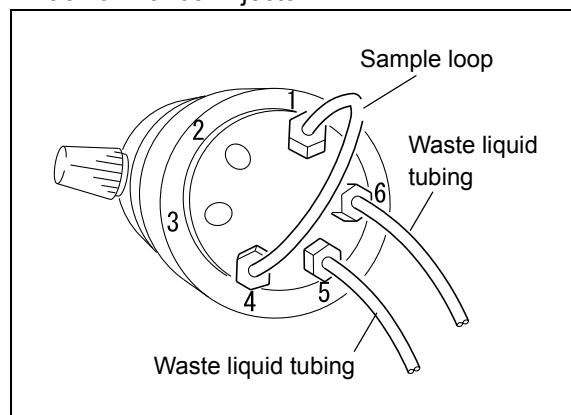


Fig. 9.36

**3** Unscrew and remove the vial cap.

**4** Route the other ends of the waste liquid tubing through the tubing opening and into the vial.

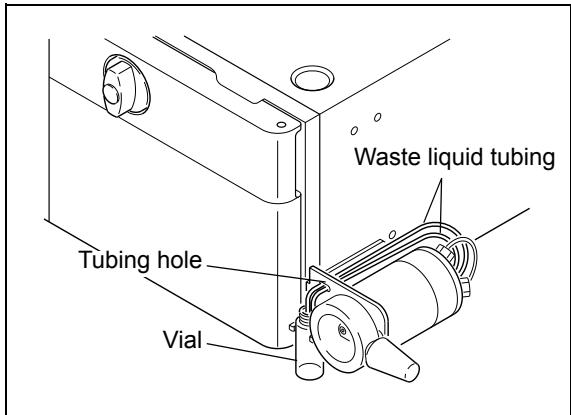


Fig. 9.37

**NOTE**

To prevent liquid from flowing out due to the siphon effect, position the ends of the waste liquid tubing level with the needle port.

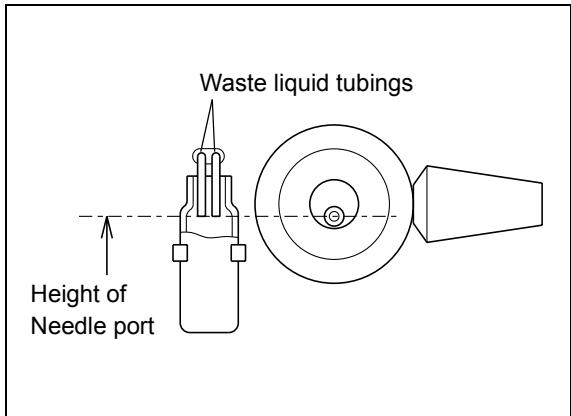


Fig. 9.38

### ■ Plumbing between Pump Unit and Manual Injector

**1** Cut the 1.6 O.D. × 0.3 I.D. SUS tubing (standard accessory of the pump) long enough to connect the pump outlet and port 2 of the manual injector.

**2** Attach male nut and ferrule to both ends of the SUS tubing.

- Pump outlet end: 1.6MN male nut and 1.6F ferrule provided as pump standard accessories.
- Manual injector end: Male nut (long bushing) and ferrule (provided as manual injector standard accessories).

**3** Insert the ends of the SUS tubing into the pump outlet and port 2 of the manual injector, and tighten the male nuts.

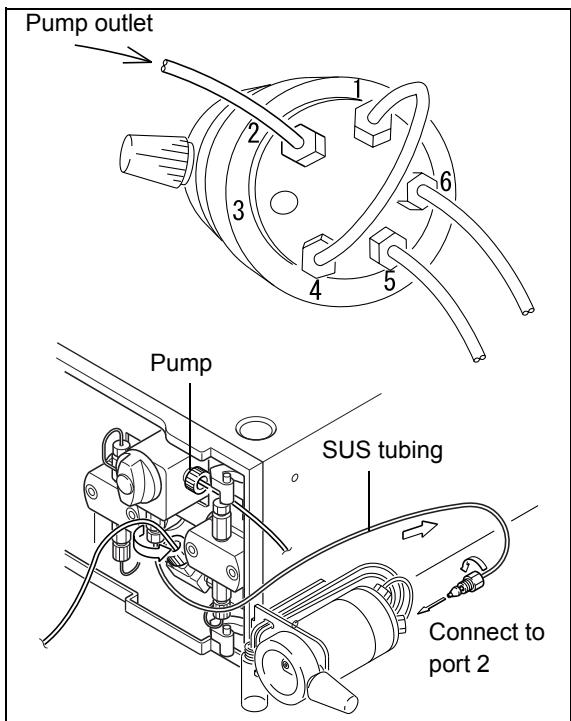


Fig. 9.39

### ■ Plumbing between Manual Injector and Column

- 1** Cut the 1.6 O.D. × 0.3 I.D. SUS tubing (standard accessory of the pump) to a length appropriate for connecting port 3 of the manual injector and the column inlet.

**NOTE**

In order to minimize peak broadening, cut the plumbing between the manual injector and the column as short as possible.

- 2** Place a male nut and ferrule on both ends of the SUS tubing.
  - Manual injector end: Male nut (long bushing) and ferrule (provided as standard accessories of the manual injector)
  - Column inlet end: Male nut and ferrule (provided as standard accessories of the pump)

- 3** Unscrew and remove the stop plug from the column inlet.

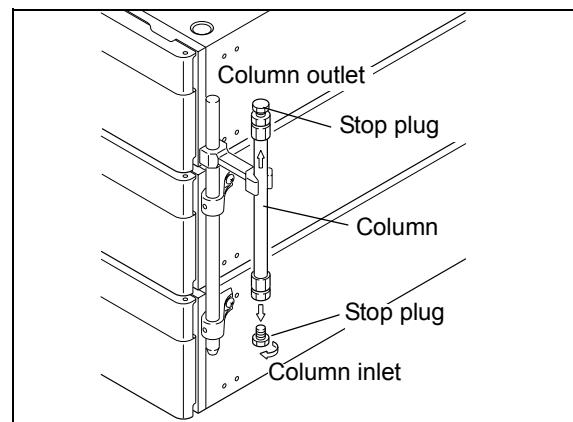


Fig. 9.40

- 4** Insert the ends of the SUS tubing into port 3 of the manual injector and the column inlet, and tighten the male nuts.

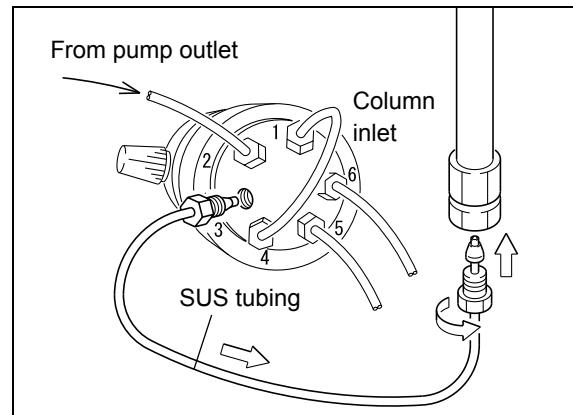


Fig. 9.41

## ■ Plumbing between Column and Detector

The figure below shows the flow line from the column outlet to the detector and the waste container. Use the accessories provided with the detector to connect this tubing. (For more detailed plumbing procedure, see the relevant sections of the detector instruction manual.)

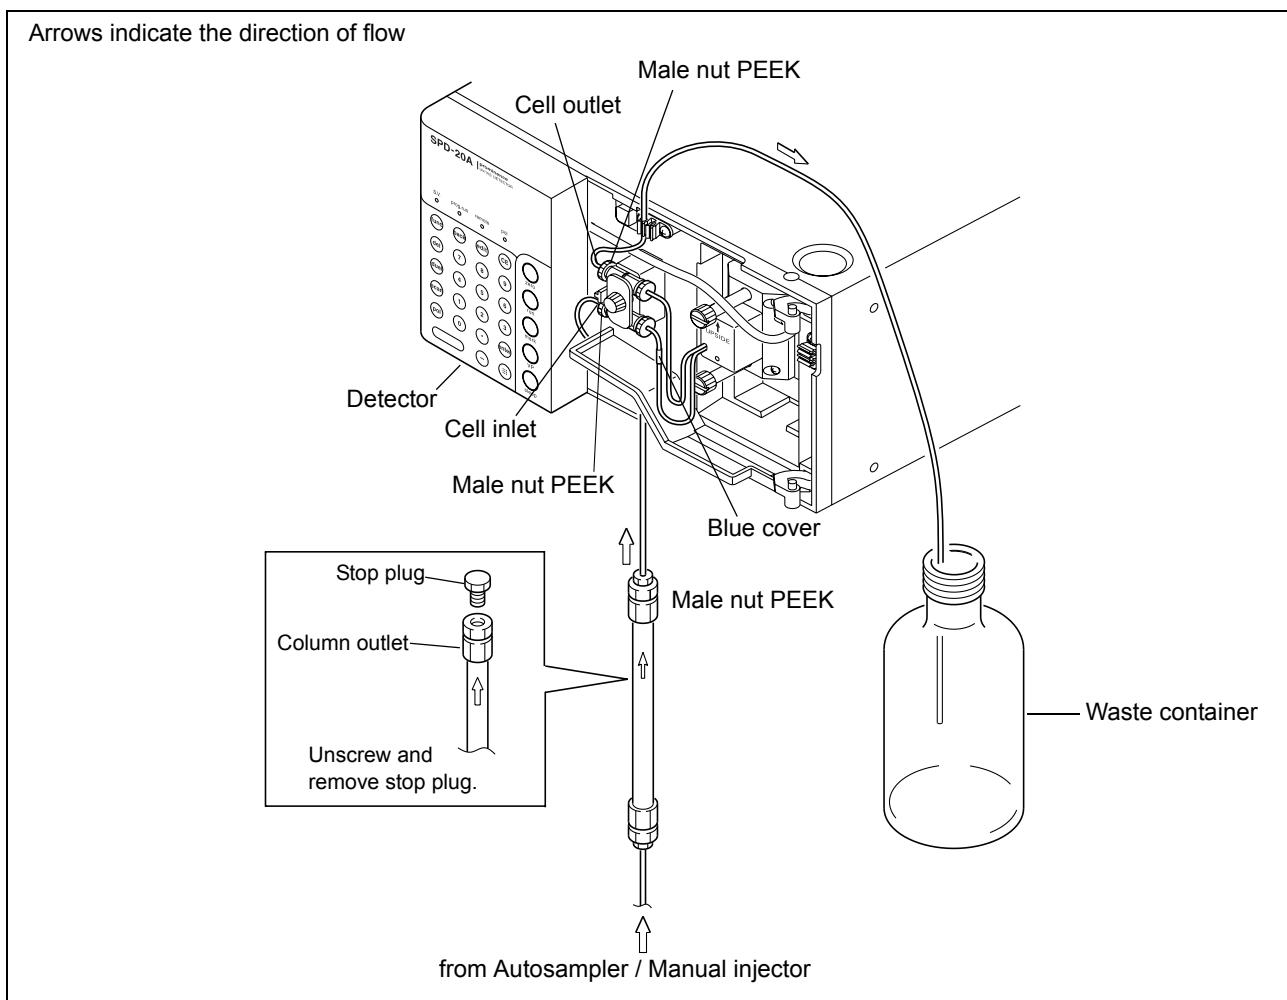


Fig. 9.42

### 9.1.8 Installation and Plumbing of Mixer (Option)

A special SUS mixer with excellent solvent mixing performance is available for use with a gradient elution system.

Procedures for installing and plumbing the mixer are given below.

#### ■ Preparation of Mixer

The mixer may be plumbed to accommodate three volumes; 0.5mL, 1.7mL and 2.6mL.

Select the appropriate capacity for the application. (The standard plumbing, installed at delivery, is for 2.6mL capacity.)

- 1 Remove the mixer cover.

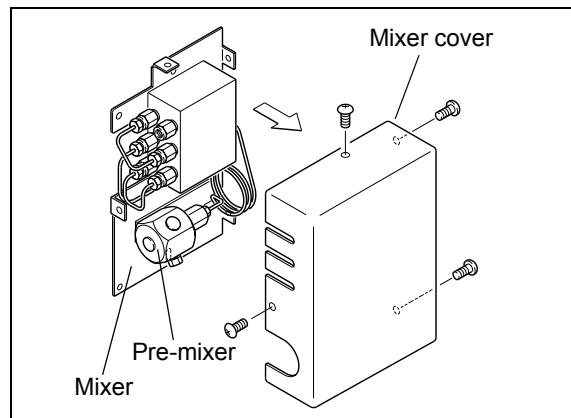


Fig. 9.43

- 2 Configure the mixer tubing using the following illustrations.

#### NOTE

Attach caps to ports which are not used, to prevent dirt or dust entering through them.

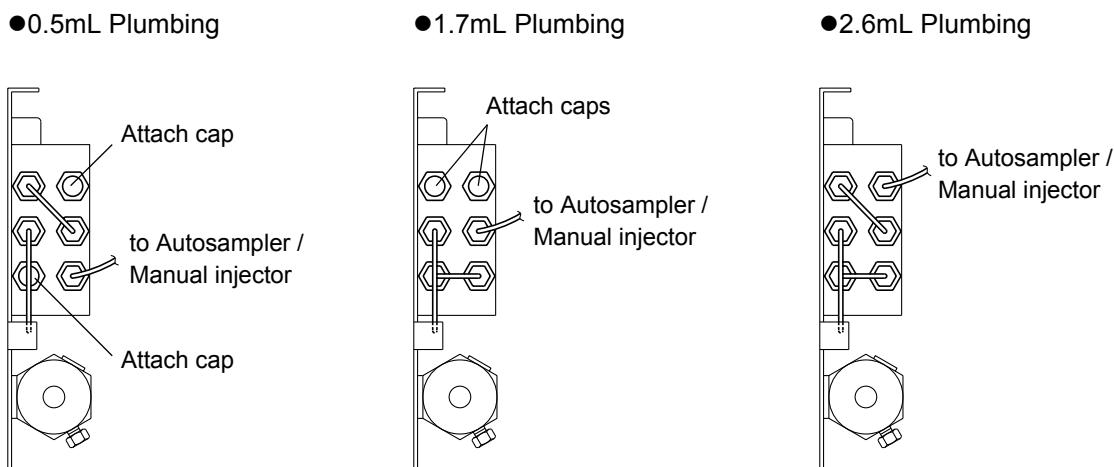


Fig. 9.44

- 3** The mixer assembly consists of two sections: a mixer section and a pre-mixer section.

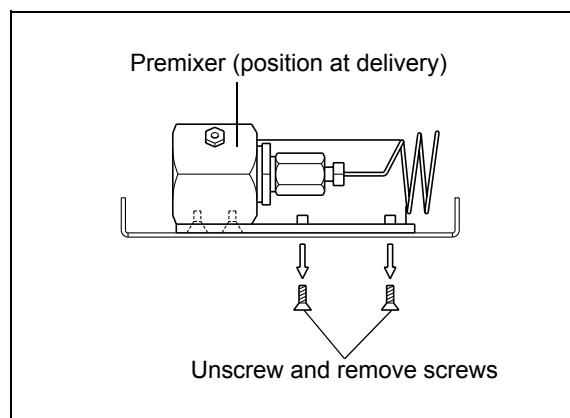


Fig. 9.45

- 4** The premixer section must be moved on the assembly base plate before installing the mixer on the instrument. Move and refasten the pre-mixer as shown in the figure.

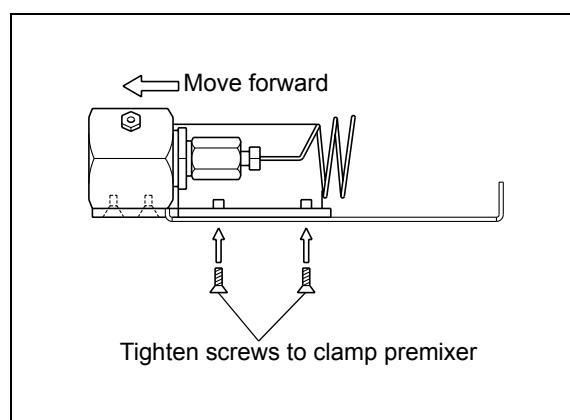


Fig. 9.46

### ■ Mounting the Mixer on the Instrument

The mixer can be installed in any of the following three positions:

- On the right side of the instrument
- Left inside of column oven
- Right inside of column oven

9

Installing the mixer on this instrument is described here.

For installing of the mixer on a column oven, see the column oven instruction manual.

- 1** Unscrew the cover installation screws attached on the right side of this instrument.

- 2** Install the mixer on this instrument using the unscrewed screws.

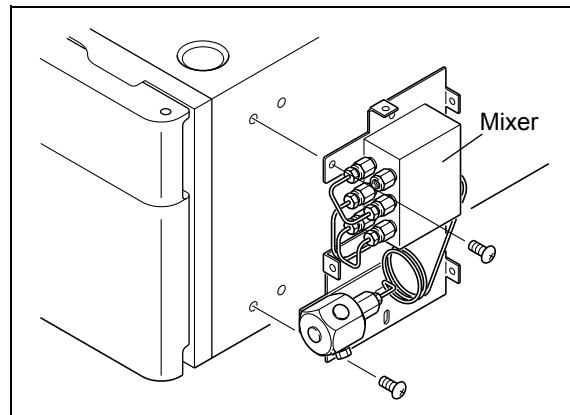


Fig. 9.47

### ■ Mixer Plumbing

- 1** Install the mixer on this instrument and remove the premixer caps from inlets A and B.

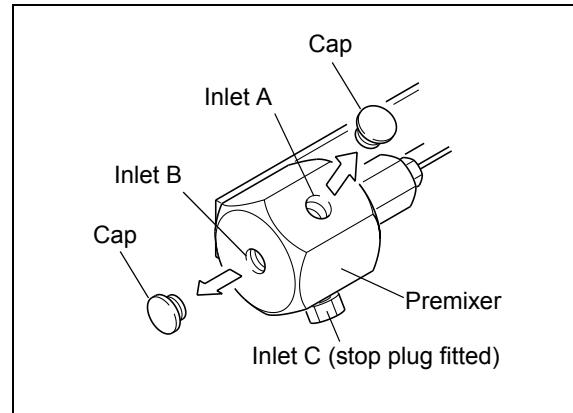


Fig. 9.48

- 2** Screw the stop plug provided with the mixer into inlet A of the premixer.

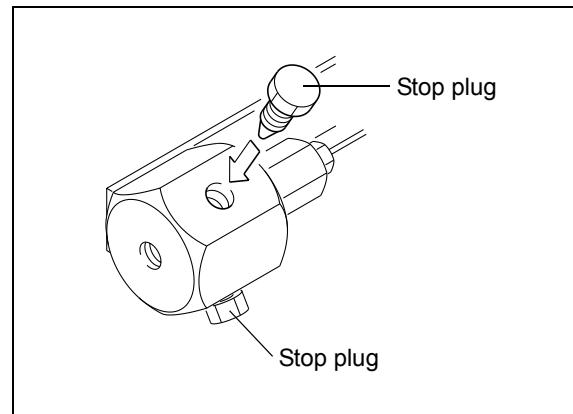


Fig. 9.49

- 3** Cut the two 1.6 O.D. × 0.3 I.D. SUS tubing sections provided with the mixer long enough to connect for the following:
- Pump outlet and premixer inlet
  - Mixer outlet and injector

- 4** Attach the 1.6MN male nuts and 1.6F ferrules provided with the mixer to both ends of each SUS tubing.

- 5** Attach the ends of one tubing section and ferrule into the pump outlet and premixer inlet B, and screw in the male nuts.

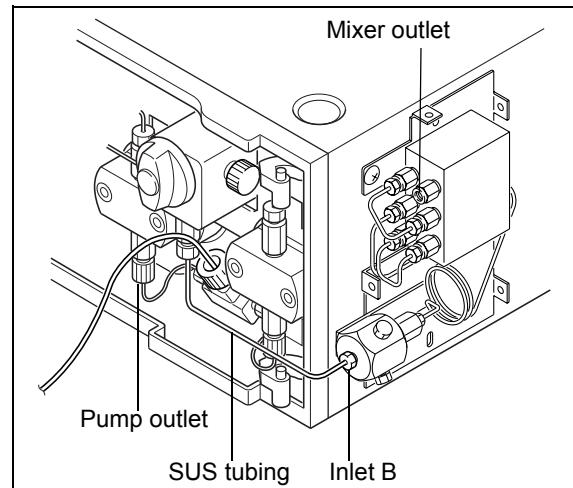


Fig. 9.50

- 6** Attach the ends of the other tubing and its ferrule into the mixer outlet and port 2 of the manual injector, and screw in the male nuts.

**NOTE**

If an autosampler is used, see its instruction manual for procedures.

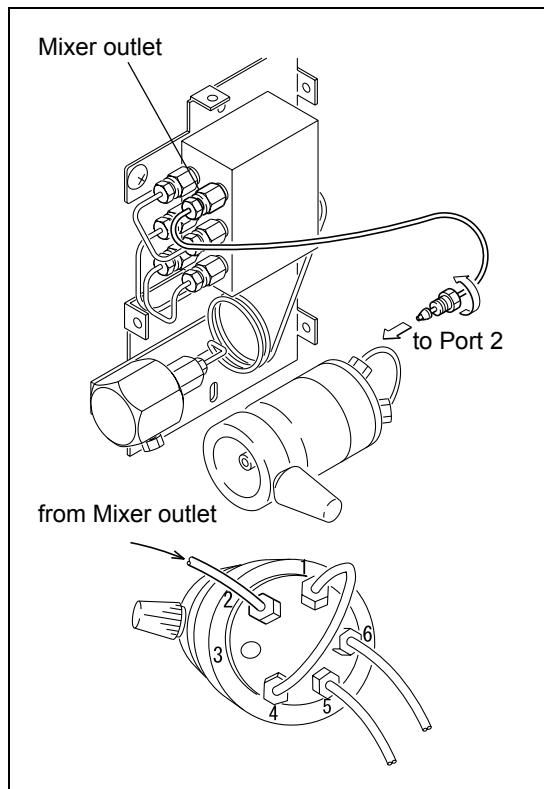


Fig. 9.51

### ■ Mixer Cover Installation

- 1** Secure the mixer cover with the screws.

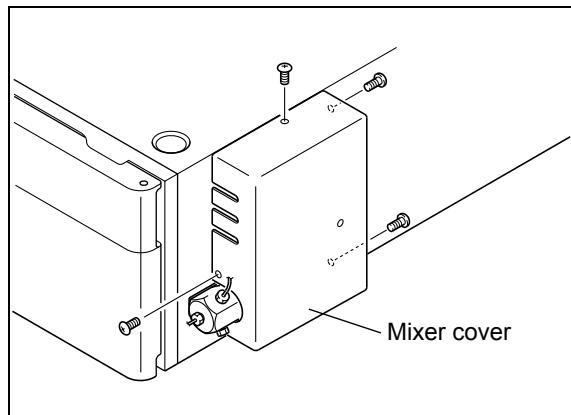


Fig. 9.52

### 9.1.9 Wiring

#### ⚠ WARNING

- Before performing wiring, turn OFF all components and unplug the power cables.
- Do not use any other than specified cables for wiring.
- Do not perform any other than the indicated wiring operations.

Failure to observe the above cautions could result in fire, electric shock or instrument malfunction.

#### ■ Connectors

- [REMOTE] connector . . . . . For connection to external system controller.  
Use to connect the instrument to a system controller.
- [DGU/SOL. V] connector . . . . . For connection of optional reservoir selection valve/degasser
- [PUMP PRESS] connector . . . . . For connection to Chromatopac (or other integrator) or recorder.  
Outputs voltage proportional to pressure.
- External input/output terminals . . . . . For connection to external equipment. For connection instructions, see "[5.7 Connection to External Input/Output Terminals](#)" P. 5-56.
- [DGU PRESS] connector. . . . . For connection to degasser to enter the pressure signal of vacuum pump inside of degasser.

Use the connectors above needed for the system. Connection instructions are provided on the following pages.

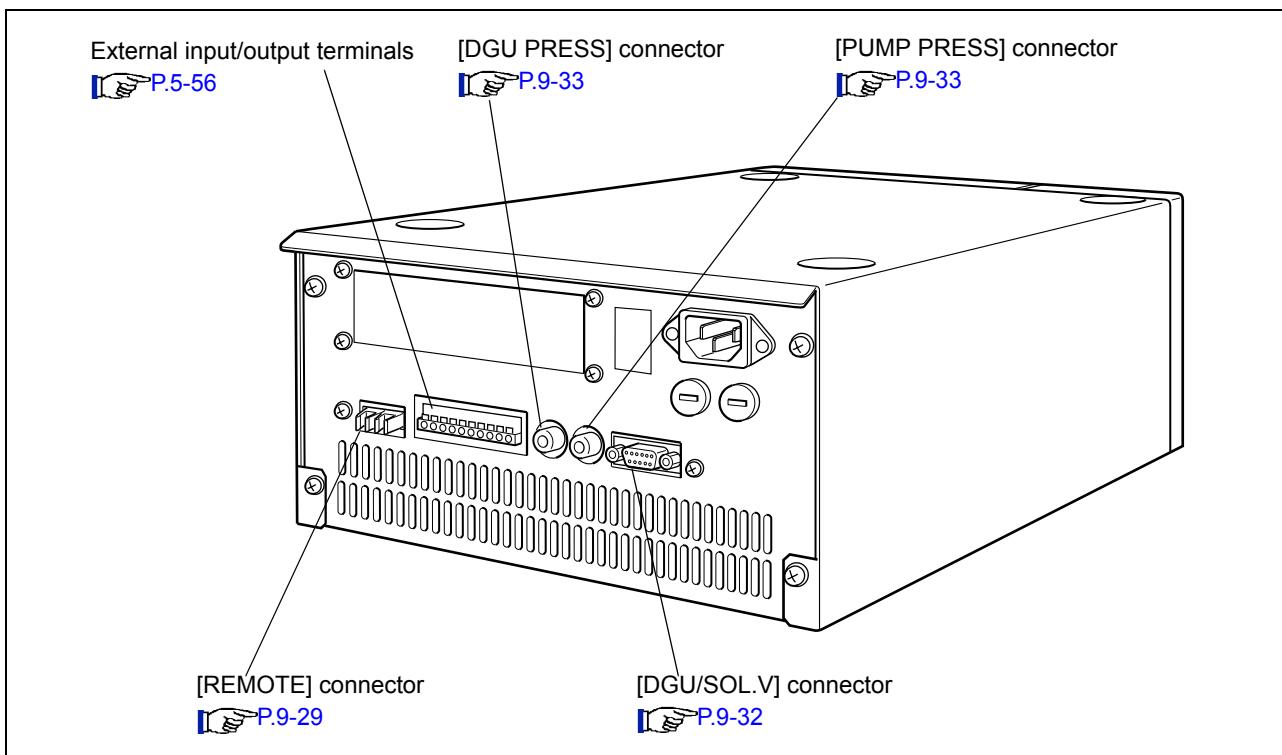


Fig. 9.53

## ■ Connecting the Optical Cable

The optical cable provided with this instrument is a two-way assembly for both transmission and reception of signals, and is connected to the [REMOTE] connector.

Instructions and precautions for connecting the optical cable are provided below.

- 1 Before connection, remove the cap from the connection channel to be used.

### **⚠ CAUTION**

The caps on the [REMOTE] connectors prevent dirt or dust from getting into the connector.

If a [REMOTE] connector is not used, leave the cap on it to prevent dirt or dust from interfering with communication.

When a cap is removed, keep it in a safe place for future use.

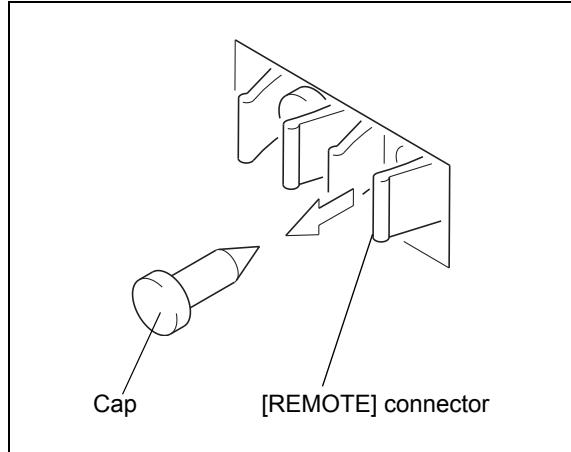


Fig. 9.54

- 2 Insert the optical cable plug into the [REMOTE] connector until it clicks into place.

### **⚠ CAUTION**

- Make sure there is no dirt or dust on the plug. Dirt or dust on the plug will get inside the [REMOTE] connector.
- Be careful not to insert the plug across two different channels.

Failure to follow these precautions above could result in malfunction or communication problems.

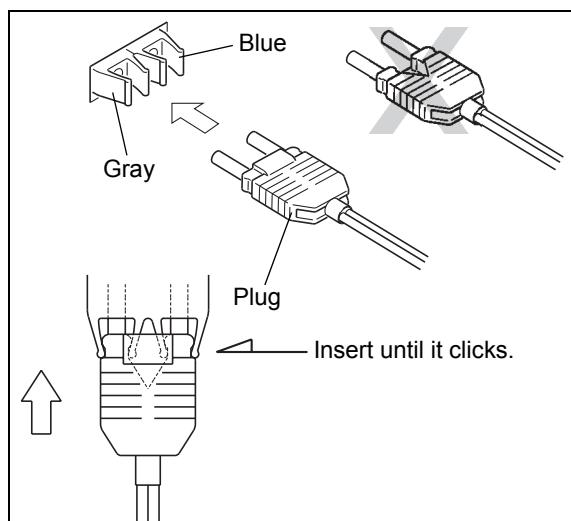


Fig. 9.55

### **⚠ CAUTION**

- Do not bend the optical cable less than 35 mm in radius.
- When inserting and removing the plug, grip the plug itself, not the cable.
- Do not bend the cable where it joins the plug.

Failure to follow these above precautions could result in damage to the plug or a broken wire in the cable.

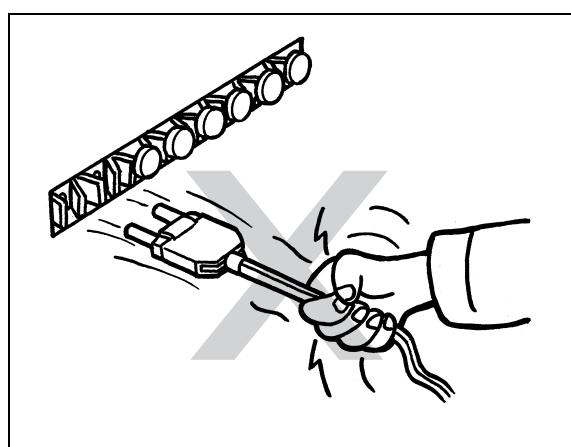


Fig. 9.56

### ■ Connection to System Controller

- 1** Referring to "Connecting the Optical Cable", connect the pump and system controller [REMOTE] connector with the optical cable.

**NOTE**

Channels between 3 and 8 of the system controller [REMOTE] connector are typically used for this purpose.

- 2** Plug in the pump, and turn the power switch on.

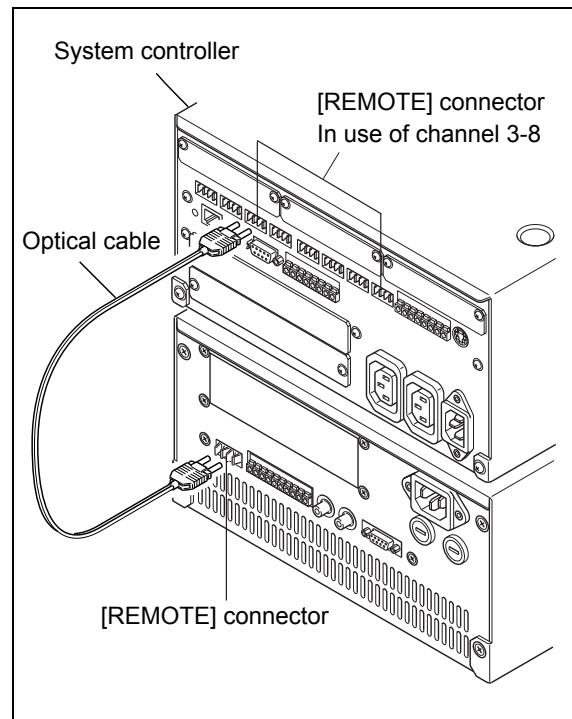


Fig. 9.57

- 3** Check the [LOCAL] and [CBM LINK] parameter and set the [ADRS] parameter.

**I** "5.2.6 System Settings Group" P. 5-21

- [LOCAL] : Check the value is [0] (initial value). (Remote mode)
- [CBM LINK]: Check the value is [1] (initial value). (External connection)
- [ADRS] : Enter the system controller's connector channel number.

0. 000 LOCAL 0  
0: Remote 1: Local  
pump prog.run remote G.E.  
○ ○ ● ●

0. 000 CBM LINK 1  
0: Int 1: Ext  
pump prog.run remote G.E.  
○ ○ ● ●

0. 000 ADRS 3  
Input 1 - 12, 85  
pump prog.run remote G.E.  
○ ○ ● ●

## ■ Connection to System Controller (in case of the installed CBM-20Alite)

The optional CBM-20Alite can control a maximum of 5 LC components (including this instrument). Since it is installed in this instrument, the system requires a smaller space.



Refer to the CBM-20Alite instruction manual.



### WARNING

- Only Shimadzu service representative is responsible for installation of CBM-20Alite.  
There is a risk of electric shock or short.
- By the installation of the instrument, remove the power plug of the instrument from the power outlet.  
There is a risk of electric shock or short.

- 1** Check the [LOCAL] parameter is [0:Remote], and set the [CBM LINK] parameter to [0:Int] (Internal Connection).
- "Selecting Local/Remote Mode [LOCAL]" P. 5-21  
 "Switching Remote Connector internal/external [CBM LINK]" P. 5-23

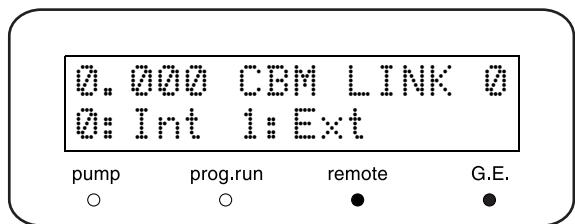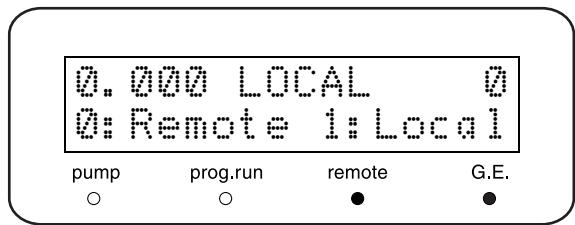


### NOTE

It is not necessary to connect the optical cable, because the instrument controlled by the internal-connected CBM-20Alite.

In case of internal connection, the link address [ADRS] is the fixed value [5].

- "Setting Link Address [ADRS]" P. 5-21

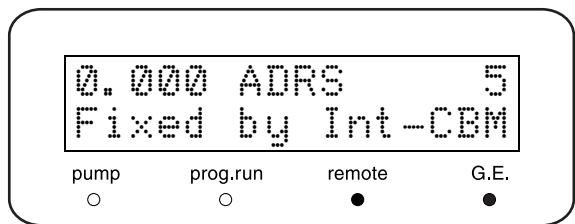

### ■ Connection of [DGU/SOL.V] Connector

[DGU/SOL.V] connector attaches the reservoir selector valve or degasser to the pump.

 "1.4 Optional Parts" P. 1-5

For detailed connection instructions, see the instruction manuals for the options.

The procedure given here is for connection of the reservoir select valve (FCV-11AL).

#### CAUTION

Make sure that the power switch of the instrument is OFF before connecting or disconnecting the special cable.

Otherwise, the instrument could be damaged.

**1** Using the accessory cable for reservoir select valve, connect the reservoir select valve to this instrument's [SOL. V] connector.

**2** Tighten the [SOL. V] connector screws with a Phillips screwdriver.  
The connector on the reservoir select valve is a flat cable connector and does not use screws.

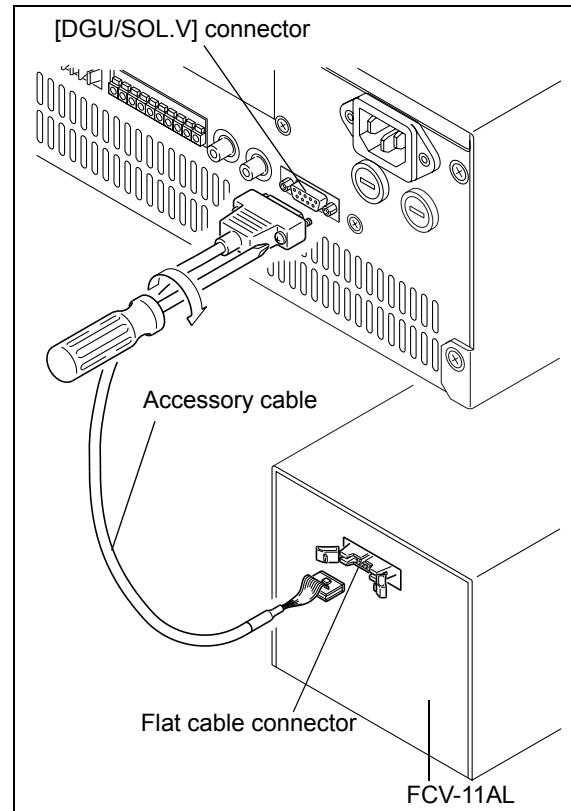


Fig. 9.58



**3** Plug in the instrument, and turn the power switches on.

**4** Set the pump [FCV TYPE] (selecting solenoid valve unit) of auxiliary function.

If necessary, also set its [SV] (opening/closing solenoid valve unit).

 "5.2 Parameter in Auxiliary Functions" P. 5-12

- [FCV TYPE] : Enter [1].
- [SV] : Set the parameter depending on a kind of selected mobile phase.

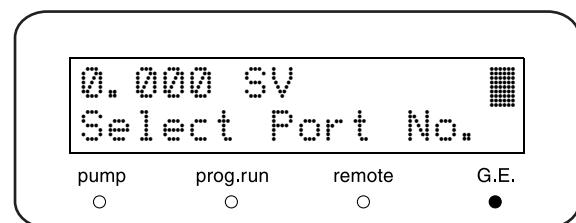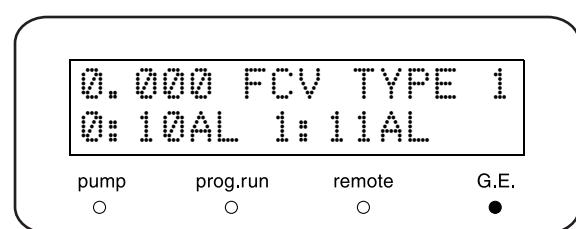

## ■ Connection of [PUMP PRESS] Connector

[PUMP PRESS] connector connects the instrument to a Chromatopac (or other integrator) or recorder. It outputs voltage proportional to pressure. The procedure given here is for a pump connected to a Chromatopac.


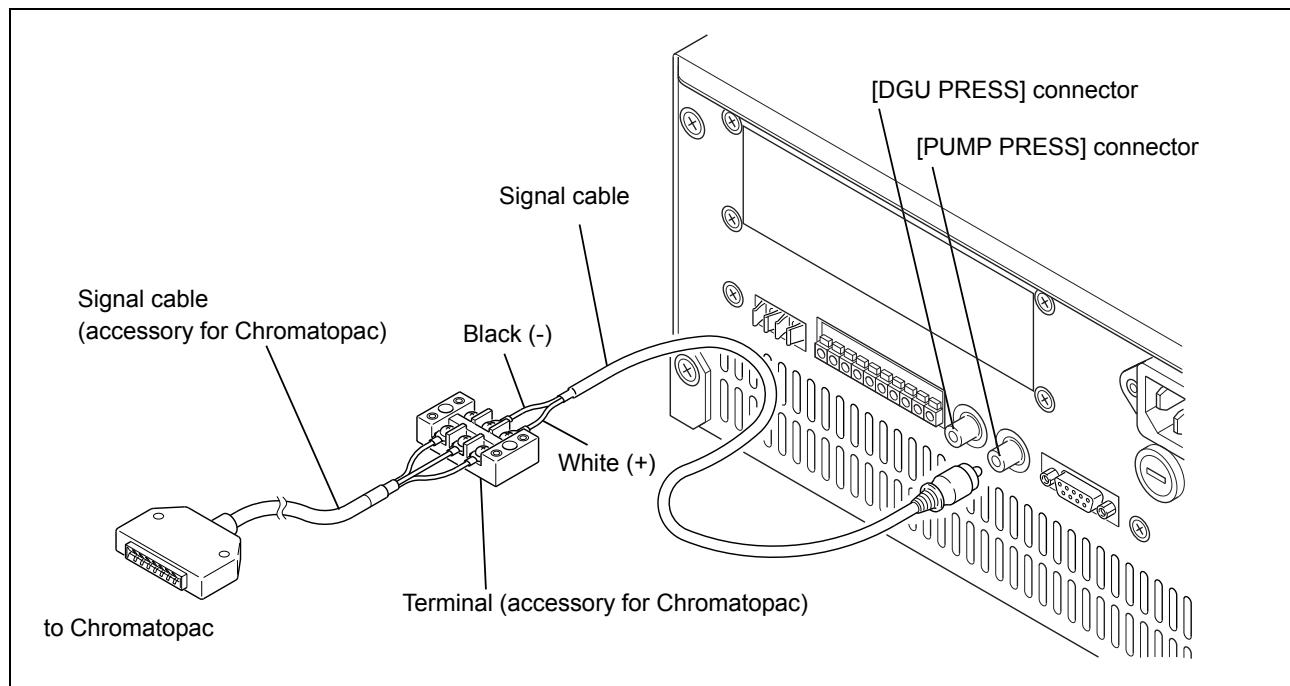


Fig. 9.59

- 1** Connect the provided signal cable to the [PUMP PRESS] connector. Then connect the instrument to the Chromatopac as shown in the figure above.
- 2** Plug the pump in and turn the power switch ON.
- 3** Set the pump [RANGE] parameter.  
☞ "Setting Pressure Recorder Range [RANGE]" P. 5-23

9

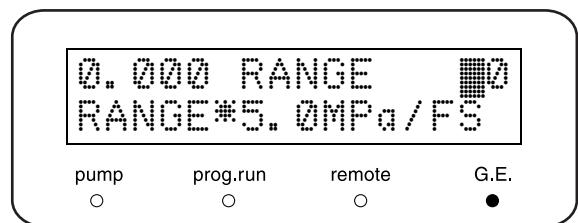

## ■ Connection of [DGU PRESS] Connector

[DGU PRESS] connector is to enter the pressure signal of vacuum pump in degasser unit. Refer to the instruction manual of degasser unit.

### 9.1.10 Installation of Automatic Rinsing Kit (Optional)

The automatic rinsing kit is an optional product for automatically and continually rinsing the plungers and the plunger seals attached to the back of the pump heads. The installation method is described below.

#### **⚠️ WARNING**

Be sure to connect the plumbing in the way described here.

Incorrect plumbing may shorten the life expectancy of the diaphragms attached to the main unit.

The arrows indicate the flow of the rinse solution.

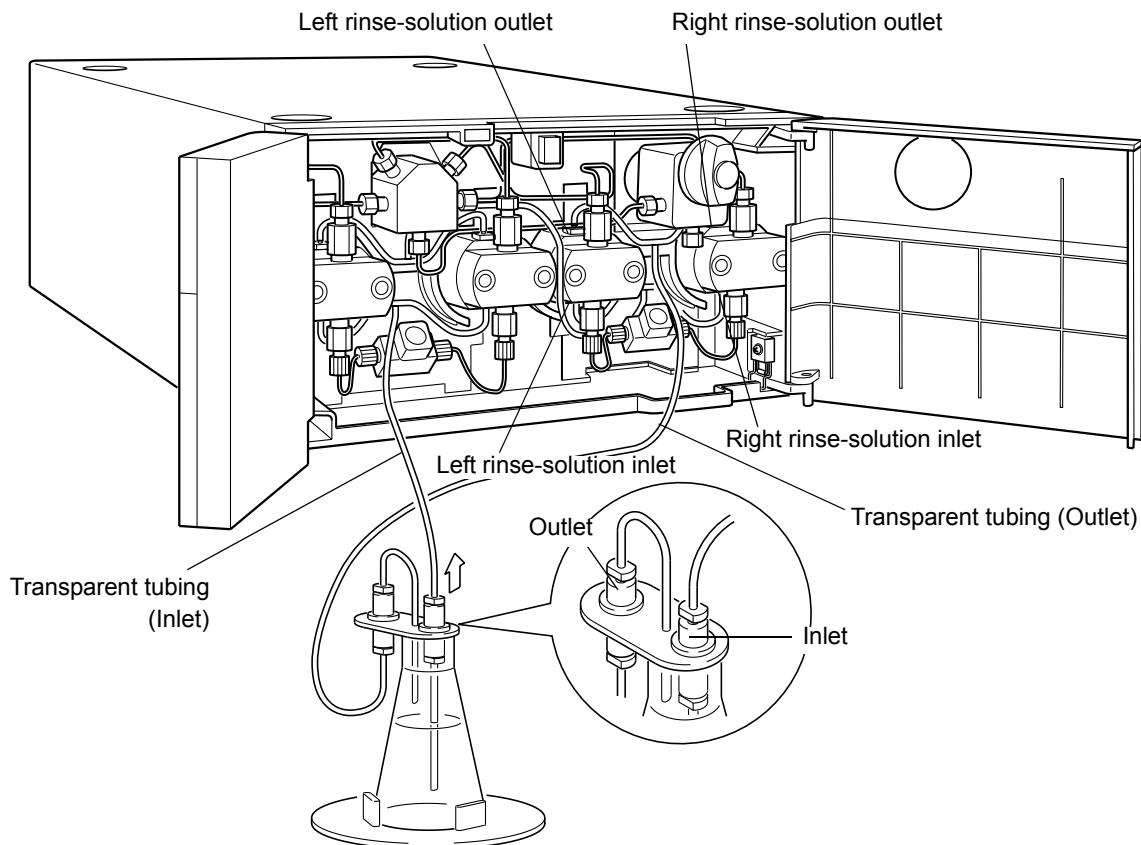


Fig. 9.60

- 1** Insert rinse tubing S (accessory) into the rinse-solution outlet above the head holder.

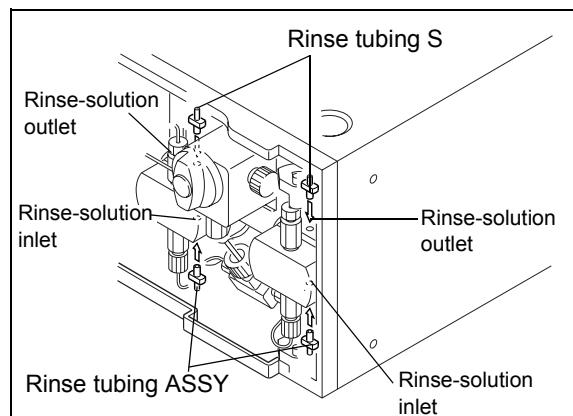


Fig. 9.61

- 2** Cut the rinse tubing assembly (accessory) in the way shown on the right with a cutter and insert it into the rinse-solution inlet below the head holder.

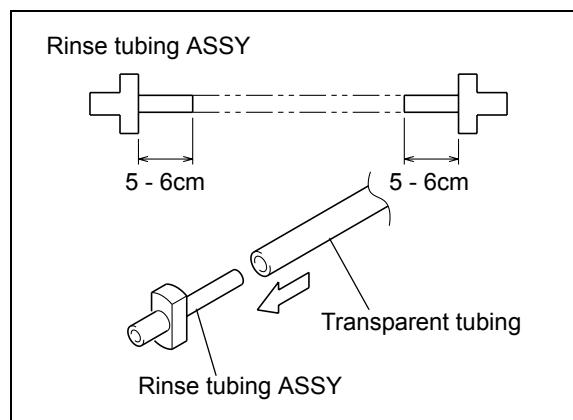


Fig. 9.62

The arrows indicate the flow of the rinse solution.

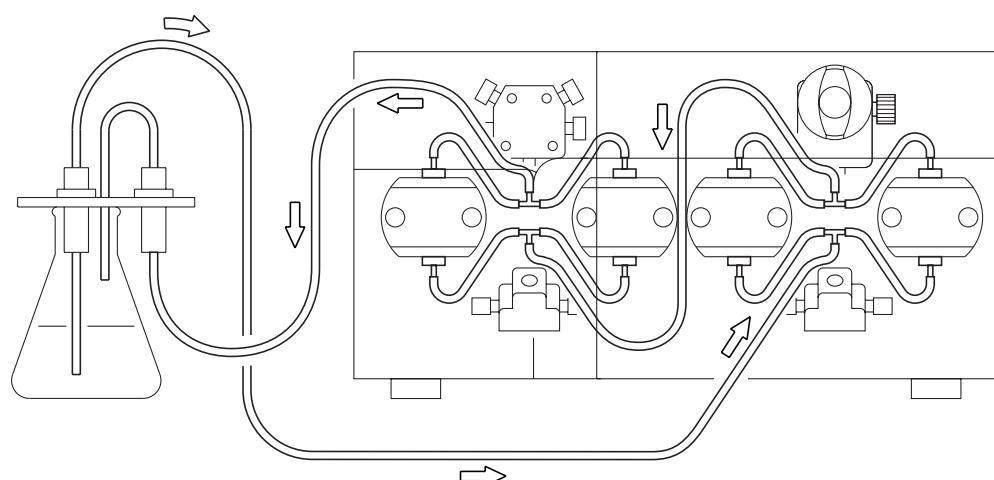


Fig. 9.63

## 9. Technical Information

---

- 4** Add distilled water to the conical flask provided with the automatic rinsing kit it is about 80% full.

- 5** Attach the automatic rinsing kit to the conical flask.

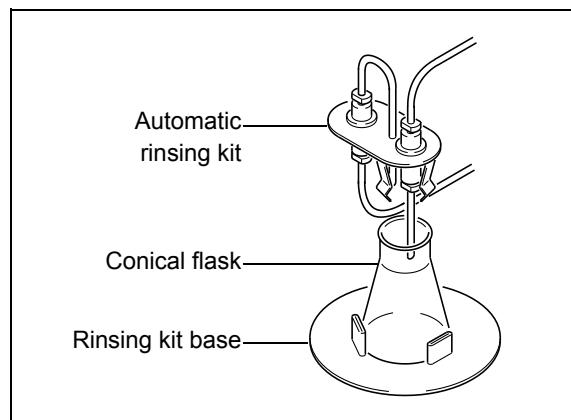


Fig. 9.64

**NOTE**

Do not pull on the rinse tubing connected to the pump heads or any of the automatic rinsing kit tubing, or you could disconnect the tubing.

# 9.2 Specifications

## 9.2.1 LC-20AB Pump Unit

Item	Specification			
Pump Type	Micro-volume double plunger pump (approx. 10µL/stroke)			
Pumping Methods	Constant flow delivery			
Flow Rate Setting Range	0.0001-5mL/min (1.0-40MPa) 5.0001-10mL/min (1.0-20MPa)			
Flow Rate Accuracy	$\pm 1\%$ or $\pm 0.5\text{mL}/\text{min}$ , whichever is the greater. (0.01-2mL/min) $\pm 2\%$ (2-5mL/min) (when water is pumped at 1-40MPa, with water and room temperature constant between 20-30 °C.)			
Flow Rate Precision	$\pm 0.3\%$ (RSD0.1% and below) (when water is pumped at 0.05-5ml/min, 1-40MPa, with water and room temperature constant between 20-30 °C.)			
Pressure limits function	Upper and lower limits			
Liquid-contacting part materials	SUS316L, PEEK, PTFE, ruby, sapphire, HastelloyC®			
Suction Filter	10µm			
Line Filter	5µm mesh, capacity 30µL			
Time Program	Commands for flow rate, concentration, [EVENT] functions, [LOOP] (for program repetition), 10 files, total 320 steps			
Pressure Display Accuracy	$\pm 2\%$ or $\pm 0.5\text{MPa}$ , whichever is the greater.			
Plunger Rinsing Line	Connecting the optional automatic rinsing kit enables automatic rinsing.			
Dimensions	W 260 × H 140 × D 420mm, excluding protruding parts			
Weight	13kg			
Operating Temperature Range	4-35 °C			
Power Supply	Part No.	Power Supply Voltage (indicated on the instrument)	Power Consumption	Frequency
	228-45002-31	AC100-120V (100-120V~)	180VA	50/60Hz
	228-45002-32	AC100-120V (100-120V~)		
	228-45002-38	AC220-240V (220-240V~)		

## 9. Technical Information

---

### 9.2.2 High-Pressure Gradient System

---

#### ■ High-Pressure Gradient System controlled by System Controller (CBM-20A)

Item	Specification
Number of solvents mixed	2
Gradient profile	Step, linear and exponential functions (only when LC workstation controls) possible at multiple levels
Maximum program steps	Max. 400 steps per program. 20 programs files
Program duration	0.01-9999.9 minutes (in 0.01 minutes steps)
Mix ratio setting range	0-100% (in 0.1% steps)
Concentration accuracy	± 0.5% (for binary gradient with water/caffeine solution, at 0.05-2mL/min, 1.0-40MPa)
Flow rates possible	0.0001-10mL/min

#### ■ High-Pressure Gradient System controlled by Pump Unit (LC-20AB)

Item	Specification
Number of solvents mixed	2
Gradient profile	Step and linear possible at multiple levels
Maximum program steps	Max. 320 steps per program. 10 program files.
Program duration	0.01-999.99 minutes (in 0.01 minutes steps)
Mix ratio setting range	0-100% (in 0.1% steps)
Concentration accuracy	± 0.5% (for binary gradient with water/caffeine solution, at 0.05-2mL/min, 1.0-40MPa)
Flow rates possible	0.0001-10mL/min

# 9.3 Maintenance Parts

## 9.3.1 Consumable Parts

Part	Part No.	Remark
Plunger seal	228-35146	For pump head
Frit	228-32744	Lines filter's frit
Suction filter	228-43342-91	Filter body only (cleaned)

## 9.3.2 Replacement Parts

### ■ Mechanical Parts

Part	Part No.	Remark
Plunger holder ASSY	228-35281-95	
Plunger ASSY	228-35601-93	
Holder ASSY	228-35602-91	
Inlet check valve ASSY	228-45704-91	
Outlet check valve ASSY	228-45705-91	
Pump head	228-34541	
Head holder	228-38022	
Diaphragm, 2 pieces	228-32784-91	
Suction filter ASSY	228-39181-95	
Bush	228-39084	For suction filter
Ferrule 3.0F-T	228-12493	For suction filter
FEP tubing 3 × 1.5	670-10321-05	For suction filter
Drain tubing ASSY	228-25495-93	
Rinse tubing ASSY	228-39184-92	
ETFE tubing 1.6 × 0.8	228-18495-01	For use between the inlet block and the check valve
Male nut 1.6MN PEEK	228-35403	For plumbing between the inlet block and the check valve
Inlet block	228-18648	Pump inlet
Pressure sensor ASSY, 20AB	228-45552-91	
Drain valve ASSY, B/D	228-45574-91	
Right panel ASSY, 20AB	228-46513-93	Front cover
Thrust	228-34469	

## 9. Technical Information

---

Part	Part No.	Remark
SUS tubing B-A-L ASSY	228-45592-91	For pump A (left head)
SUS tubing B-A-R ASSY	228-45592-92	For pump A (right head)
SUS tubing B-B-L ASSY	228-45592-93	For pump B (left head)
SUS tubing B-B-R ASSY	228-45592-94	For pump B (right head)
SUS tubing B-P ASSY	228-45592-95	For converging block
Panel 20AD	228-42208	For mounting the inlet block

### ■ Electrical Parts

Part	Part No.	Remark
Fuse 5AT, 250V	072-02004-23	
Switch ASSY	228-42287-91	
Power supply LEA100F-24	074-80427-61	
PCB LC-20AB ASSY	228-42118-92	without EEPROM
PCB sensor ASSY	228-35842-92	
Left panel 20AB ASSY	228-43200-93	Display panel and keypad assembly
Leak sensor ASSY	228-39247-92	
Fan for SPD60 LC-10A	228-25246-91	

---

### 9.3.3 Maintenance Kit

---

A set of consumable parts and plumbing parts is provided as Maintenance Kit ASSY.

### ■ Maintenance Kit for LC-20AD (Part No.228-45593-91)

Part	Part No.	Q'ty	Remark
Plunger seal	228-35146	2	
Frit	228-32744	2	
Suction filter ASSY	228-39181-95	1	
Plunger holder ASSY	228-35218-95	1	
Ferrule, 1.6F	228-16000-10	4	
Male nut, 1.6MN	228-16001	4	
Male nut, PEEK	228-18565	4	
SUS pipe 1.6mm O.D. × 0.3mm I.D.	228-36993-96	1	2m



# 9.4 Introduction to HPLC System

The Prominence LC (LC-20A) series components are for use with Shimadzu high performance liquid chromatography (HPLC) systems, which are designed to provide high accuracy and high sensitivity analyses. Example system configurations are provided below, along with descriptions of the operations of the various components.

## 9.4.1 Example of a Simple (Isocratic) System

Each component of the system is controlled locally. This is a simple system composed of the minimum number of components for stable analysis.

### ■ Solvent Flow      ■ Function of Components

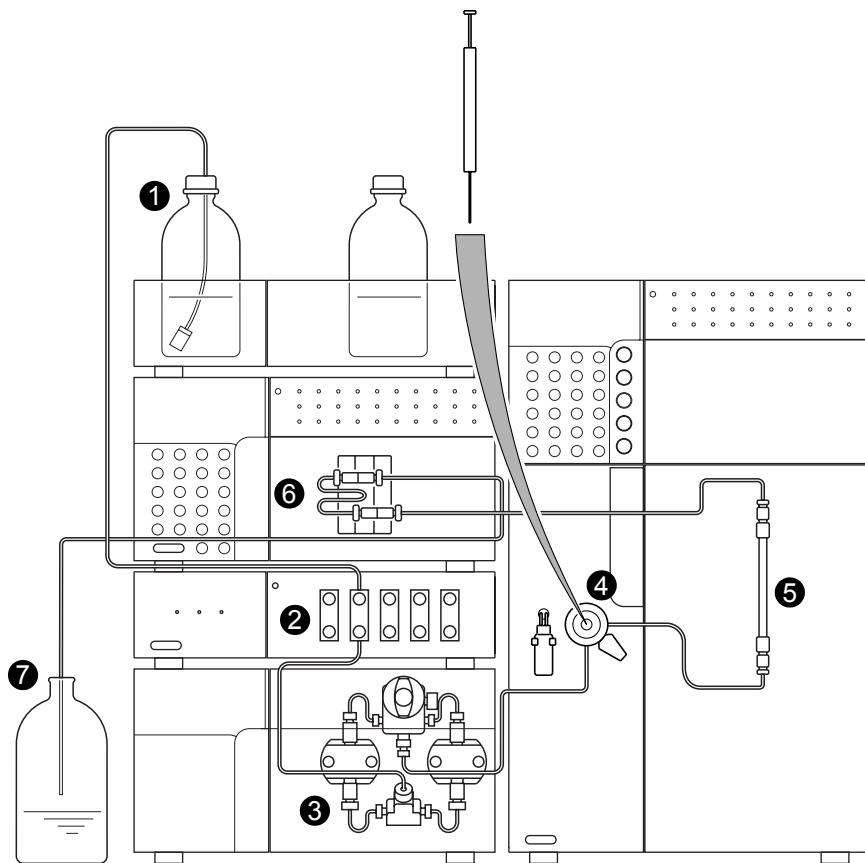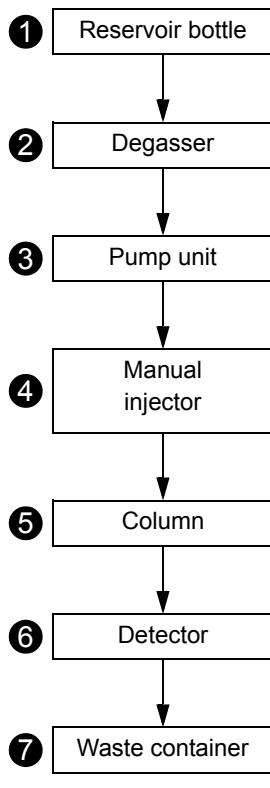


- ① Mobile phase is drawn out of the reservoir bottle and pumped through the tubing by the pump.
- ② The degasser removes dissolved air from the mobile phase, preventing air bubbles and consequent rise, drift or other baseline irregularities caused by dissolved air.
- ③ The pump sends the mobile phase through the manual injector, column and detector, in that order, and finally into the waste container.
- ④ Samples are injected into the system by the manual injector, with a syringe.
- ⑤ In the column, the components are separated by means of the mutual interactions of the mobile phase and the column packing (stationary phase).
- ⑥ The detector detects the components eluted from the column, and sends the signal data to a Chromatopac or PC.
- ⑦ Mobile phase from the detector drains into the waste container.


### 9.4.2 Example of Autosampler System (1)

Centralized control of all the components by a CBM-20Alite system controller enhances ease operation and is well suited for automated analyses. The CBM-20Alite can control a maximum of 5 LC components. Since it is installed in the pump unit or autosampler, the system requires a smaller space.

#### ■ Solvent Flow

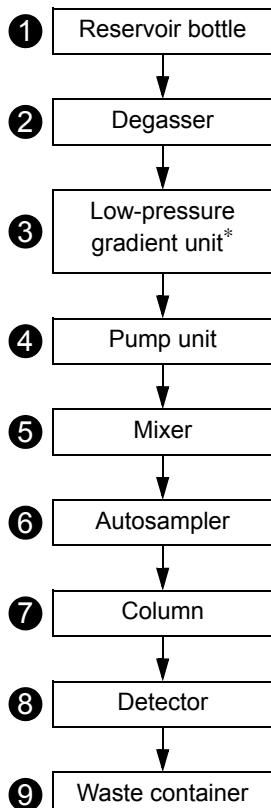

#### ■ Function of Components

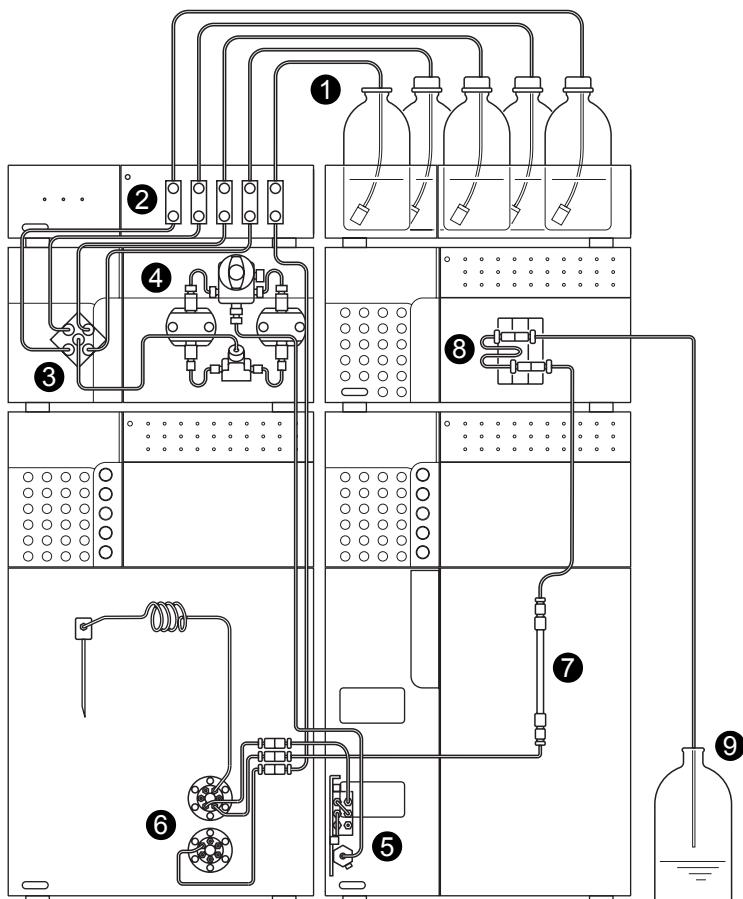

- ① Mobile phase is drawn out of the reservoir bottles and pumped through the tubing by the pump.
- ② The degasser removes dissolved air from the mobile phase, preventing air bubbles and consequent rise, drift or other baseline irregularities caused by dissolved air.
- ③ The low-pressure gradient unit mixes up to 4 mobile phases that have been degassed by the degasser.  
(\*This item is necessary for a low-pressure gradient system.)
- ④ The pump sends the mobile phase through the autosampler, column and detector, in that order, and finally into the waste container.
- ⑤ The mixer enhances the mixing efficiency of the mobile phases. This item is required for low or high-pressure gradient system.
- ⑥ The autosampler automatically injects the sample into the flow lines. By adding a rack changer, it is possible to automatically change the autosampler racks.
- ⑦ In the column, the components are separated by means of the mutual interactions of the mobile phase and the column packing (stationary phase).
- ⑧ The detector detects the components separated in the column, and sends the signal data to a Chromatopac or PC.
- ⑨ Mobile phase from the detector drains into the waste container.



### 9.4.3 Example of Autosampler System (2)

The CBM-20A system controller can control a maximum of 8 LC components (12 LC components as an option).

Use the same type of pumps for high-pressure gradient system.

#### ■ Solvent Flow

#### ■ Function of Components

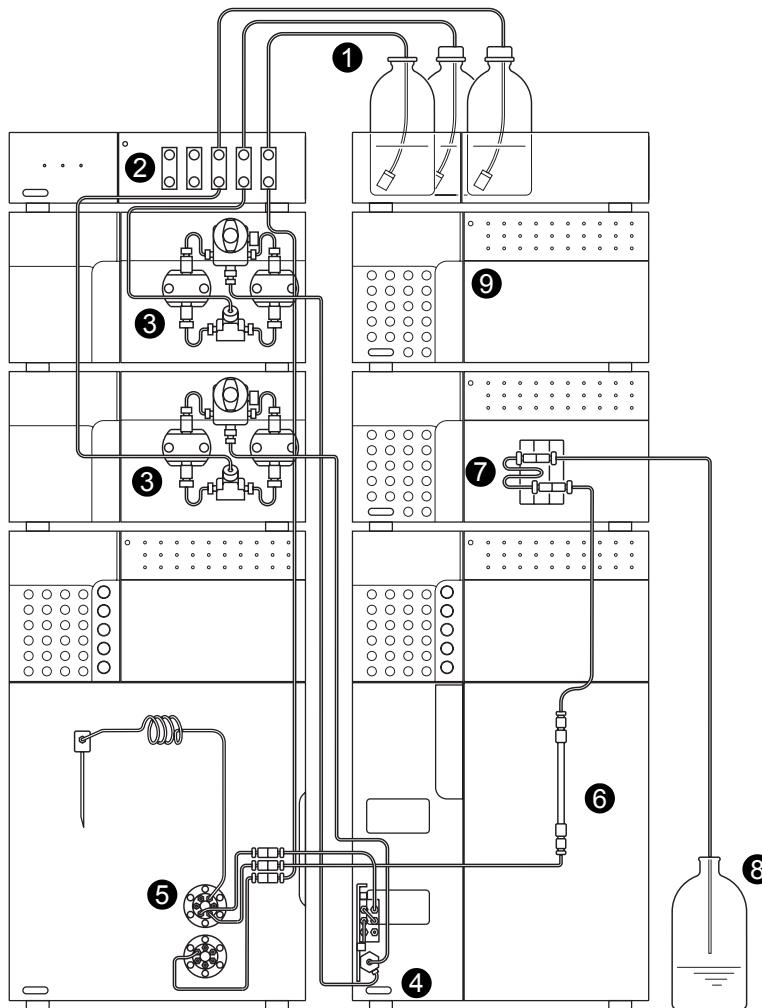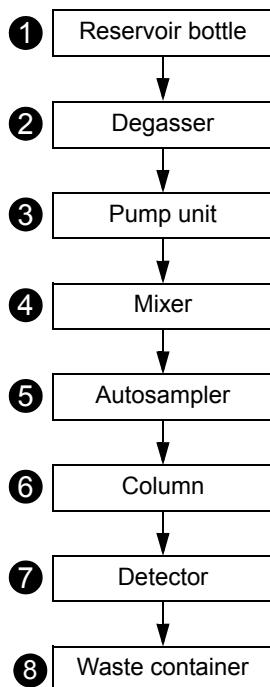

- ① Mobile phase is drawn out of the reservoir bottles and pumped through the tubing by the pump.
- ② The degasser removes dissolved air from the mobile phase, preventing air bubbles and consequent rise, drift or other baseline irregularities caused by dissolved air.
- ③ The pump sends the mobile phase through the autosampler, column and detector, in that order, and finally into the waste container.
- ④ The mixer enhances mixing efficiency of the mobile phases.
- ⑤ The autosampler automatically injects the sample into the flow lines. By adding a rack changer, it is possible to automatically change the autosampler racks.
- ⑥ In the column, the components are separated by means of the mutual interactions of the mobile phase and the column packing (stationary phase).
- ⑦ The detector detects the components eluted from the column, and send the signal data to a Chromatopac or PC.
- ⑧ Mobile phase from the detector drains into the waste container.
- ⑨ The CBM-20A system controller can control a maximum of 8 LC components (12 LC components as an option) including a maximum of 4 pump units.

# 9.5 Mobile Phase Characteristics

	(1) Solvent (*) $\eta < 5 \text{ cP}$ , $> 45^\circ\text{C}$ (**) $\eta < 5 \text{ cP}$ , $< 45^\circ\text{C}$	(2) Source	(3) UV Cutoff	(4) R.I. $25^\circ$	Boiling Point $(^\circ\text{C})$	Viscosity $(\text{cP}, 25^\circ\text{C})$	(5) $p'$	(6) $e^{\circ}\text{a}$	(7) Water Solubility $\% W_{in}^{20^\circ\text{C}}$ Solvent	(8) Dielectric Constant $\epsilon^{20}$	(9) $p' +$ $0.25e$
1	FC-78 (*) FC-75 (Fluorescent solvent) FC-43	(LC specific)	210nm 210 (opaque under 210)	1.267 1.276 1.291	50 102 174	0.4 0.8 2.6	<-2 <-2 <-2	-.25 -.25 -.25		1.88 1.86 1.9	p' and Dielect. const. (Function proportional to strength)
2	Isooctane(*)(2,2,4-tri methylpentane)	LC	197	1.389	99	0.47	0.1	0.01	0.011	1.94	0.1
3	n-Heptane(*)	LC	195	1.385	98	0.40	0.2	0.01	0.010	1.92	0.5
4	n-Hexane(*)	LC	190	1.372	69	0.30	0.1	0.01	0.010	1.88	0.5
5	n-Pentane(**)	LC	195	1.355	36	0.22	0.0	0.00	0.010	1.84	0.5
6	Cyclohexane	LC	200	1.423	81	0.90	-0.2	0.04	0.012	2.02	0.5
7	Cyclopentane(*)	LC	200	1.404	49	0.42	-0.2	0.05	0.014	1.97	0.6
8	i-Chlorobutane(*)	LC	220	1.400	78	0.42	1.0	0.26		7.4	2.8
9	Carbon disulfide	LC	380	1.624	46	0.34	0.3	0.15	0.005	2.64	1.7
10	2-Chloropropane(**)	LC	230	1.375	36	0.30	1.2	0.29		9.82	3.7
11	Carbon tetrachloride	LC	265	1.457	77	0.90	1.6	0.18	0.008	2.24	2.3
12	n-Butyl ether		220	1.397	142	0.64	2.1	0.25	0.19	2.8	2.4
13	Triethylamine			1.398	89	0.36	1.9	0.54		2.4	2.4
14	Bromoethane(*)			1.421	38	0.38	2.0	0.35		9.4	4.3
15	i-Propyl ether(*)		220	1.365	68	0.38	2.4	0.28	0.62	3.9	3.2
16	Toluene	LC	285	1.494	110	0.55	2.4	0.29	0.046	2.4	2.9
17	p-Xylene		290	1.493	138	0.60	2.5	0.26		2.3	3.0
18	Chlorobenzene			1.521	132	0.75	2.7	0.30		5.6	4.1
19	Bromobenzene			1.557	156	1.04	2.7	0.32		5.4	4.1
20	Iodobenzene						2.8	0.35			
21	Phenyl ether			1.580	258	3.3	3.4			3.7	3.7
22	Phenetole			1.505	170	1.14	3.3			4.2	4.9
23	Ethyl ether(**)	LC	218	1.350	35	0.24	2.8	0.38	1.3	4.3	4.0
24	Benzene	LC	280	1.498	80	0.60	2.7	0.32	0.058	2.3	3.6
25	Tricresy phosphate										
26	Ethyl iodide			1.510	72	0.57	2.2			7.8	4.2
27	n-Octanol		205	1.427	195	7.3	3.4	0.5	3.9	10.3	5.8
28	Fluorobenzene			1.46	85	0.55	3.1			5.4	4.6
29	Benzylether			1.538	288	4.5	4.1				
30	Methylene chloride(**)	LC	233	1.421	40	0.41	3.1	0.42	0.17	8.9	5.6
31	Anisole			1.514	154	0.9	3.8			4.3	4.6
32	i-Pentanol			1.405	130	3.5	3.7	0.61	9.2	14.7	7.3
33	1,2-Dichloroethane	LC	228	1.442	83	0.78	3.5	0.44	0.16	10.4	6.3

	(1) Solvent (*) $\eta < .5 \text{ cP}$ , $> 45^\circ\text{C}$ (**) $\eta < .5 \text{ cP}$ , $< 45^\circ\text{C}$	(2) Source	(3) UV Cutoff	(4) R.I. $25^\circ$	Boiling Point ( $^\circ\text{C}$ )	Viscosity (cP, $25^\circ\text{C}$ )	(5) $p'$	(6) $e^\circ_a$	(7) Water Solubility %W <sub>u</sub> in $20^\circ\text{C}$ Solvent	(8) Dielectric Constant $\epsilon^{20}$	(9) $p' +$ $0.25e$
34	t-Butanol			1.385	82	3.6	4.1	0.7	miscible	12.5	
35	n-Butanol	LC	210	1.397	118	2.6	3.9	0.7	20.1	17.5	8.3
36	n-Propanol	LC	240	1.385	97	1.9	4.0	0.82	miscible	20.3	
37	Tetrahydrofuran(*)	LC	212	1.405	66	0.46	4.0	0.57	miscible	7.6	
38	Propylamine(*)			1.385	48	0.35	4.2		miscible	5.3	
39	Ethylacetate(*)	LC	256	1.370	77	0.43	4.4	0.58	8.8	6.0	5.8
40	i-Propanol	LC	205	1.384	82	1.9	3.9	0.82	miscible	20.3	
41	Chloroform(*)	LC	245	1.443	61	0.53	4.1	0.40	0.072	4.8	5.6
42	Acetophenone			1.532	202	1.64	4.8			17.4	8.7
43	Methylethyl	LC	329	1.376	80	0.38	4.7	0.51	23.4	18.3	9.1
44	Cyclohexanone			1.450	156	2.0	4.7			18.3	9.1
45	Nitrobenzene			1.550	211	1.8	4.4			34.8	13.2
46	Benzonitrile			1.536	191	1.2	4.8			25.2	10.9
47	Dioxane	LC	215	1.420	101	1.2	4.8		miscible	2.2	
48	Tetramethyl urea	LC	265	1.449	175		6.0	0.56		23.0	10.7
49	Quinoline			1.625	237	3.4	5.0			9.0	7.4
50	Pyridine			1.507	115	0.88	5.3		miscible	12.4	
51	Nitroethane		380	1.390	114	0.64	5.2			0.9	
52	Acetone(*) Benzyl alcohol	LC	330	1.356 1.538	56 205	0.30 5.5	5.1 5.7	0.71	miscible	13.1	8.8
53	Tetramethyl guanidine						6.1	0.6			
54	Methoxyethanol	LC	210	1.400	125	1.60	5.5		miscible	19.9	
55	Tris(cyanoethoxy) propane	GC					6.6	0.56			
56	Propylene carbonate	LC					6.1				
57	Ethanol	LC	210	1.359	78	10.8	4.3		miscible	24.6	
58	Oxydipropionitrile	GC					6.8				
59	Aniline			1.584	184	3.77	6.3			6.9	8.1
60	Acetic acid			1.370	118	1.1	6.0		miscible	6.2	
61	Acetonitrile(*)	LC	190	1.341	82	0.34	5.8		miscible	37.5	
62	N,N-dimethylaceta-mide	LC	268	1.436	166	0.78	6.5	0.88		37.8	
63	Dimethylformamide	LC	268	1.428	153	0.80	6.4			36.7	
64	Dimethylsulfoxide	LC	268	1.477	189	2.00	7.2	0.62	miscible	4.7	
65	N-methyl-2-pyrolidone	LC	285	1.468	202	1.67	6.7			32	
66	Hexamethyl phosphoric acid triamide			1.457	233	3	7.4	0.65		30	
67	Methanol(*)	LC	205	1.326	65	0.54	5.1		miscible	32.7	
68	Nitromethane		380	1.380	101	0.61	6.0			2.1	
69	m-Cresol			1.540	202	14	7.4			11.8	10.0
70	N-methylformamide			1.447	182	1.65	6.0		miscible	182	

## 9. Technical Information

---

	(1) Solvent (*) $\eta < .5 \text{ cP}$ , $> 45^\circ\text{C}$ (**) $\eta < .5 \text{ cP}$ , $< 45^\circ\text{C}$	(2) Source	(3) UV Cutoff	(4) R.I. $25^\circ$	Boiling Point $(^\circ\text{C})$	Viscosity $(\text{cP}, 25^\circ\text{C})$	(5) $p'$	(6) $\epsilon^\circ_a$	(7) Water Solubility $\%W_{in} 20^\circ\text{C}$ Solvent	(8) Dielectric Constant $\epsilon^{20}$	(9) $p' +$ $0.25e$
71	Ethylene glycol			1.431	182	16.5	6.9		miscible	37.7	
72	Formamide			1.447	210	3.3	9.6		miscible	111	
73	Water	LC		1.333	100	0.89	10.2			80	

- (1) An asterisk (\*) indicates solvents most suitable for LC, with low boiling points ( $>45^\circ\text{C}$ ) and low viscosity ( $<0.5\text{cP}$ ).  
 Double asterisks (\*\*) indicates solvents with a very low viscosity and boiling point.
- (2) "LC" indicates that a grade of solvent specifically for LC is commercially available from companies like the following:  
 Burdick & Jackson, Baker Chemical, Mallinkrodt Chemical, Fischer Scientific, Waters Associate, Manufacturing Chemists. Inc.  
 "GC" indicates that a solvent is used as a stationary phase for gas chromatography, and can be purchased from companies selling GC columns and stationary phases. (These solvents are used as stationary phase in liquid-to-liquid LC.)
- (3) The wavelength below which the solvent becomes opaque.  
 (4) Refractive index at  $25^\circ\text{C}$ .  
 (5) Polarity parameter of solvent.  
 (6) Solvent's strength parameter in relation to liquid-to-solid adsorption in alumina.  
 (7) Water solubility (%W) at  $20^\circ\text{C}$  of solvent used in liquid-to -solid adsorption.  
 (8) Value at  $20^\circ\text{C}$ .  
 (9) Function consisting of P' (proportional to solvent strength) plus the dielectric constant, in ion chromatography.

Source: A.Krstulovic and P.R.Brown, *Reversed-Phase High-Performance Liquid Chromatography*, Wiley Interscience, 1982.

# Index

## A

A/B SEAL DELIVERED .....	5-32
Accessory Pack .....	1-4
ACOMP .....	5-17
ADRS .....	5-21
ALARM LEVEL .....	5-30
Auto Purging Function .....	5-54
Automatic Rinsing Kit .....	1-6, 4-6, 9-34
Auxiliary Function .....	5-12

## B

BCOMP .....	5-17
BEEP MODE .....	5-24
BRIGHT .....	5-22

## C

Calibration Support Group .....	5-11, 5-28, 5-38
CBM LINK .....	5-23
CBM PARAMETER .....	5-40
CHANGE PASSWORD .....	5-40
Check Valve .....	2-3, 8-16
COM .....	5-56
Component Validation .....	7-2
Consumable Parts .....	9-39, 9-40
Control Settings Group .....	5-5, 5-13
Converging Block .....	2-3
Cutting Tubings .....	9-6

## D

DATE .....	5-34
DEGAS PRS .....	5-26
DGU PRESS Connector .....	2-6, 9-33
DGU/SOL.V Connector .....	2-6, 9-32
Display Panel .....	2-2, 2-7
Drain Tubing .....	9-13
Drain Valve .....	2-3
Drain Valve Knob .....	2-2

## E

ERR IN .....	5-56
ERROR LOG .....	5-33
Error Message .....	6-5
EVENT .....	5-17
EVENT1 .....	5-56
EVENT2 .....	5-56
External Input/Output Terminals .....	2-6, 5-56
EXT-S .....	5-22

## F

FCV TYPE .....	5-23
File .....	5-12
FILE CPY .....	5-19
FILE DEL .....	5-19
FILE NUM .....	5-19
File Operation Group .....	5-5, 5-12
FLOW CHECK A/B .....	5-36
FLOW COMP FACT A/B .....	5-38
Front Cover .....	9-11
Fuse Holders .....	2-6

## G

GE TEST PROGRAM .....	5-36
GOTO .....	5-53
Grounding .....	9-6

## H

Hardware Validation .....	7-2
---------------------------	-----

## I

INITIALIZE PARAM .....	5-39
Input PASSWORD .....	5-38
Installation .....	9-2
Installation Space .....	9-3

## K

KEY CLOSE .....	5-21
-----------------	------

# Index

---

Keypad ..... 2-2, 2-8

## L

---

LEAK SENSOR TEST ..... 5-37  
LEAK THR ..... 5-39  
Leakage Drain Tubing ..... 9-14  
LEAKAGE TEST ..... 5-37  
Line Filter ..... 2-3  
LOCAL ..... 5-21  
LOOP ..... 5-52

## M

---

Maintenance Information Group .. 5-9, 5-27, 5-31  
MAINTENANCE LOG ..... 5-32  
Maintenance Parts ..... 9-39  
Maximum Pressure Limit ..... 5-15  
MEMORY CHECK ..... 5-35  
Minimum Pressure Limit ..... 5-15  
Mixer ..... 1-6, 9-24  
MOBILE PHASE A/B ..... 5-30  
Mobile Phase Monitor Group ..... 5-8, 5-27, 5-30  
MON ID ..... 5-25  
MON REVA/B ..... 5-26  
MON SV ..... 5-25  
MON TIME ..... 5-24  
Monitor Settings Group ..... 5-7, 5-13

## O

---

OP MODE ..... 5-39  
OPERATION LOG ..... 5-33  
Optional Parts ..... 1-5

## P

---

Parameter Settings Group ..... 5-4, 5-12, 5-15  
PART REPLACEMENT ..... 5-32  
Periodic Inspection and Maintenance ..... 8-2  
Periodic Validation ..... 7-3  
P-FLOW ..... 5-18  
Plumbing ..... 9-10  
Plunger Rinsing ..... 4-6  
PMAX ..... 5-15  
Power Cord Connector ..... 2-6  
Power Supply Connection ..... 9-5  
Power Switch ..... 2-2

P-PMAX ..... 5-18  
PRESS COMP FACT ..... 5-38  
Product Information Group ..... 5-8, 5-27, 5-31  
PRS-UNIT ..... 5-23  
P-SET ..... 5-20  
P-TIMER ..... 5-18  
PULSE CHECK A/B ..... 5-35  
Pump Head ..... 2-3, 8-5  
PUMP OFF ..... 5-56  
PUMP ON ..... 5-56  
PUMP PRESS Connector ..... 2-6, 9-33

## R

---

RANGE ..... 5-23  
REMOTE Connector ..... 2-6, 9-29  
Replacement of Check Valves ..... 8-16  
Replacement of Diaphragms ..... 8-12  
Replacement of Drain Valve ASSY ..... 8-22  
Replacement of Fuse ..... 8-24  
Replacement of Line Filter ..... 8-19  
Replacement of Plunger Seal ..... 8-5  
Replacement of Plungers ..... 8-10  
Replacement of Suction Filter ..... 8-21  
Replacement Parts ..... 9-39  
Replacing the Mobile Phase ..... 4-10

## S

---

S/W ID ..... 5-31  
SEAL REPLACEMENT ..... 5-39  
SERIAL NUMBER ..... 5-31  
Shipping Screw ..... 2-5, 9-4  
Specifications ..... 9-37  
S-PROT ..... 5-22  
START ..... 5-56  
STOP ..... 5-52  
SV ..... 5-16  
System Controller ..... 5-54, 9-30, 9-43  
System Settings Group ..... 5-6, 5-13, 5-21  
System Validation ..... 7-2, 7-23

## T

---

TIME ..... 5-34  
Time Program ..... 5-44  
TOTAL OP TIME ..... 5-31  
Troubleshooting and Corrective Action ..... 6-2

**V**

---

Validation Support Group ..... 5-10, 5-28, 5-34  
Validation: Pump ..... 7-7  
VP Functions ..... 5-8, 5-27

**W**

---

Wiring ..... 9-28

**Z**

---

ZERO ADJ ..... 5-20

This page is intentionally left blank.