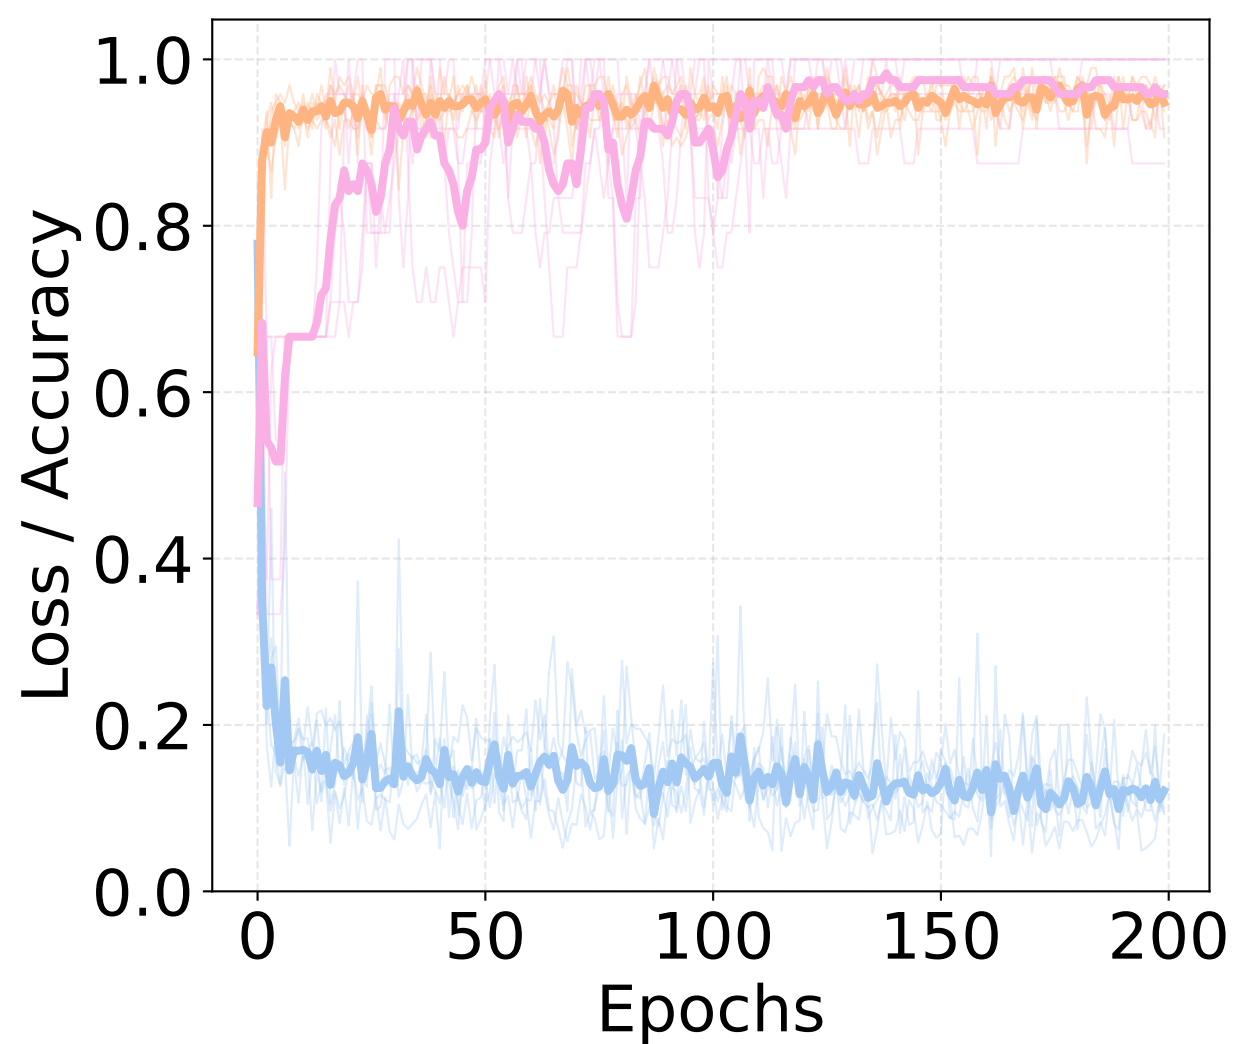
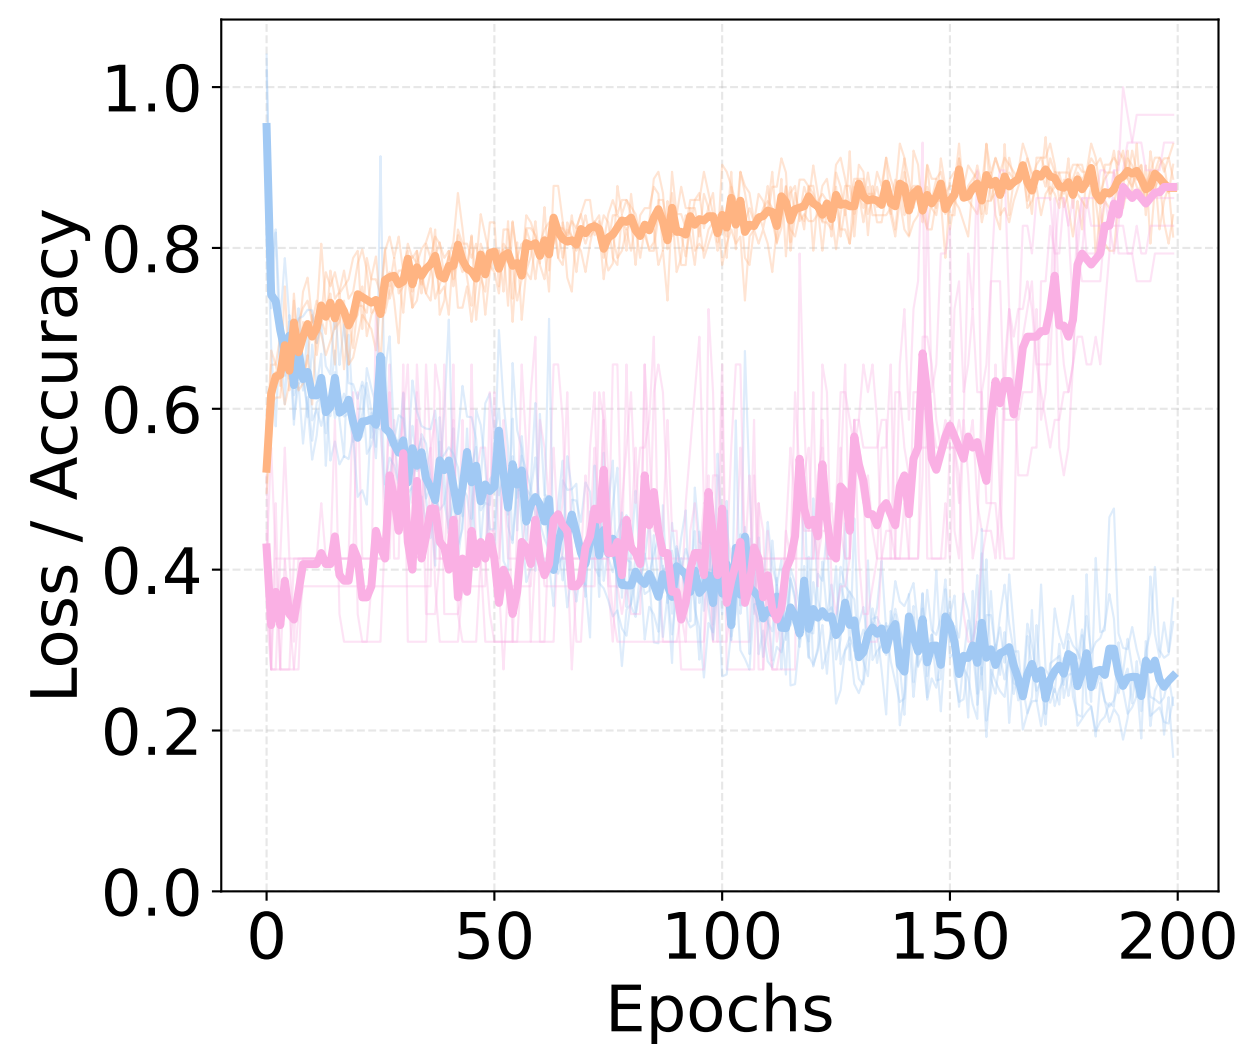


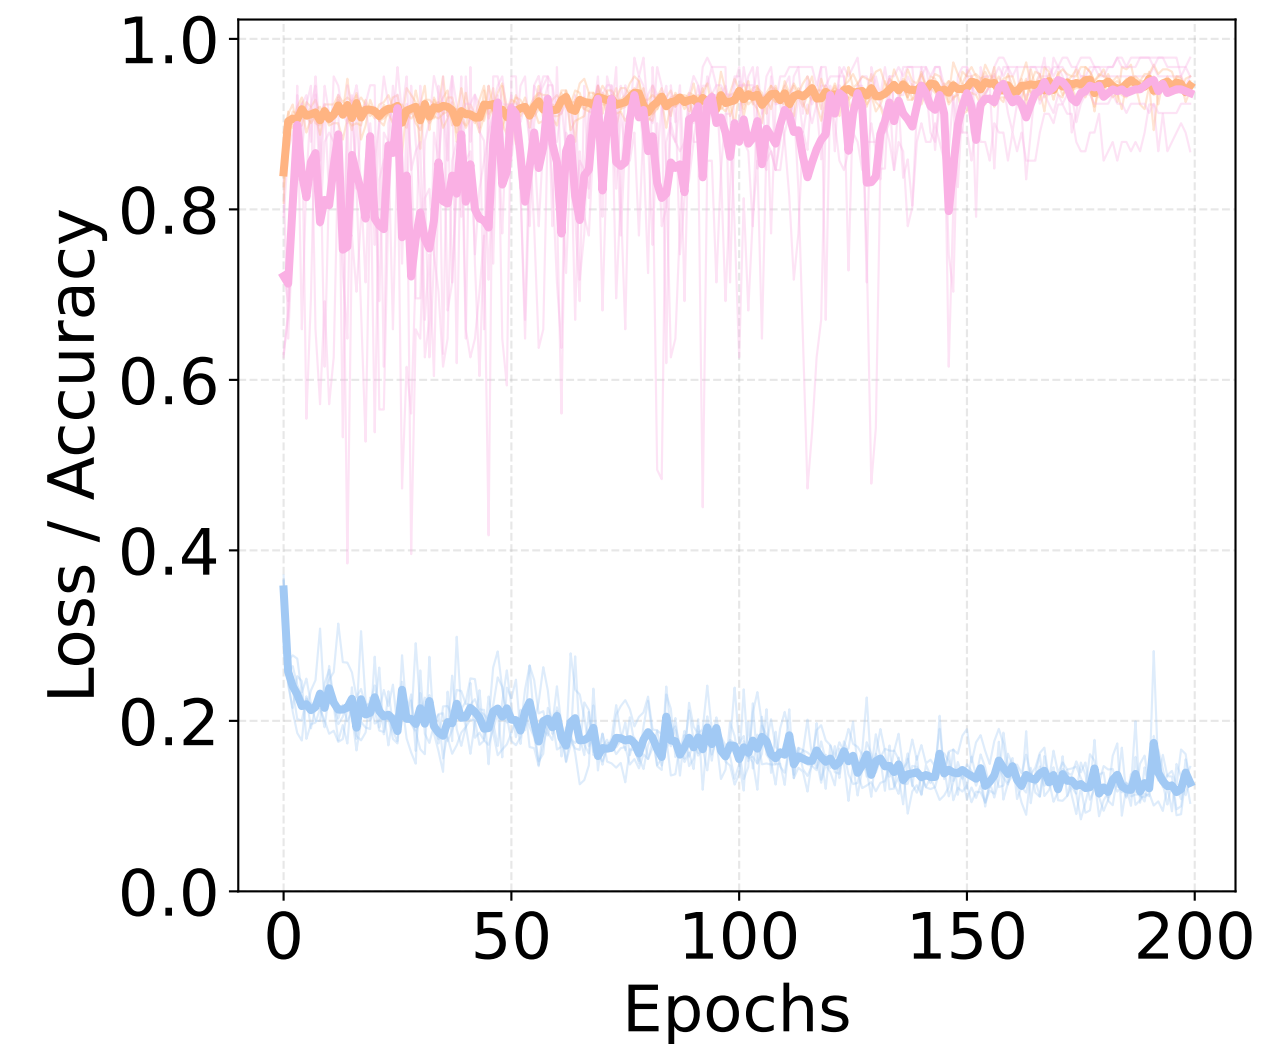
Iris

Test Acc: 0.947 ± 0.045 

Wine

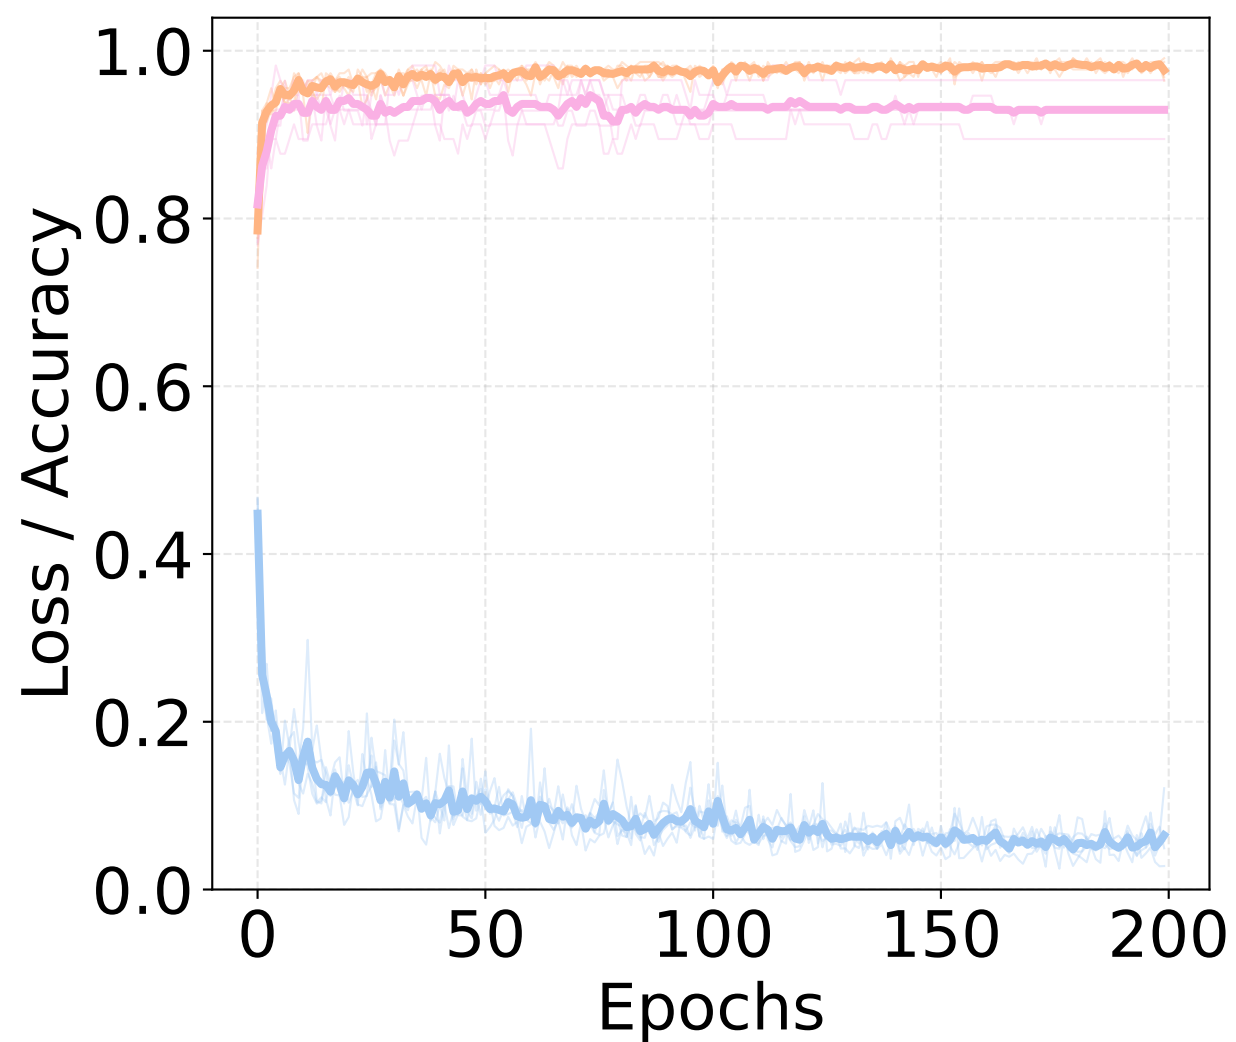
Test Acc: 0.876 ± 0.035 

Breast Cancer

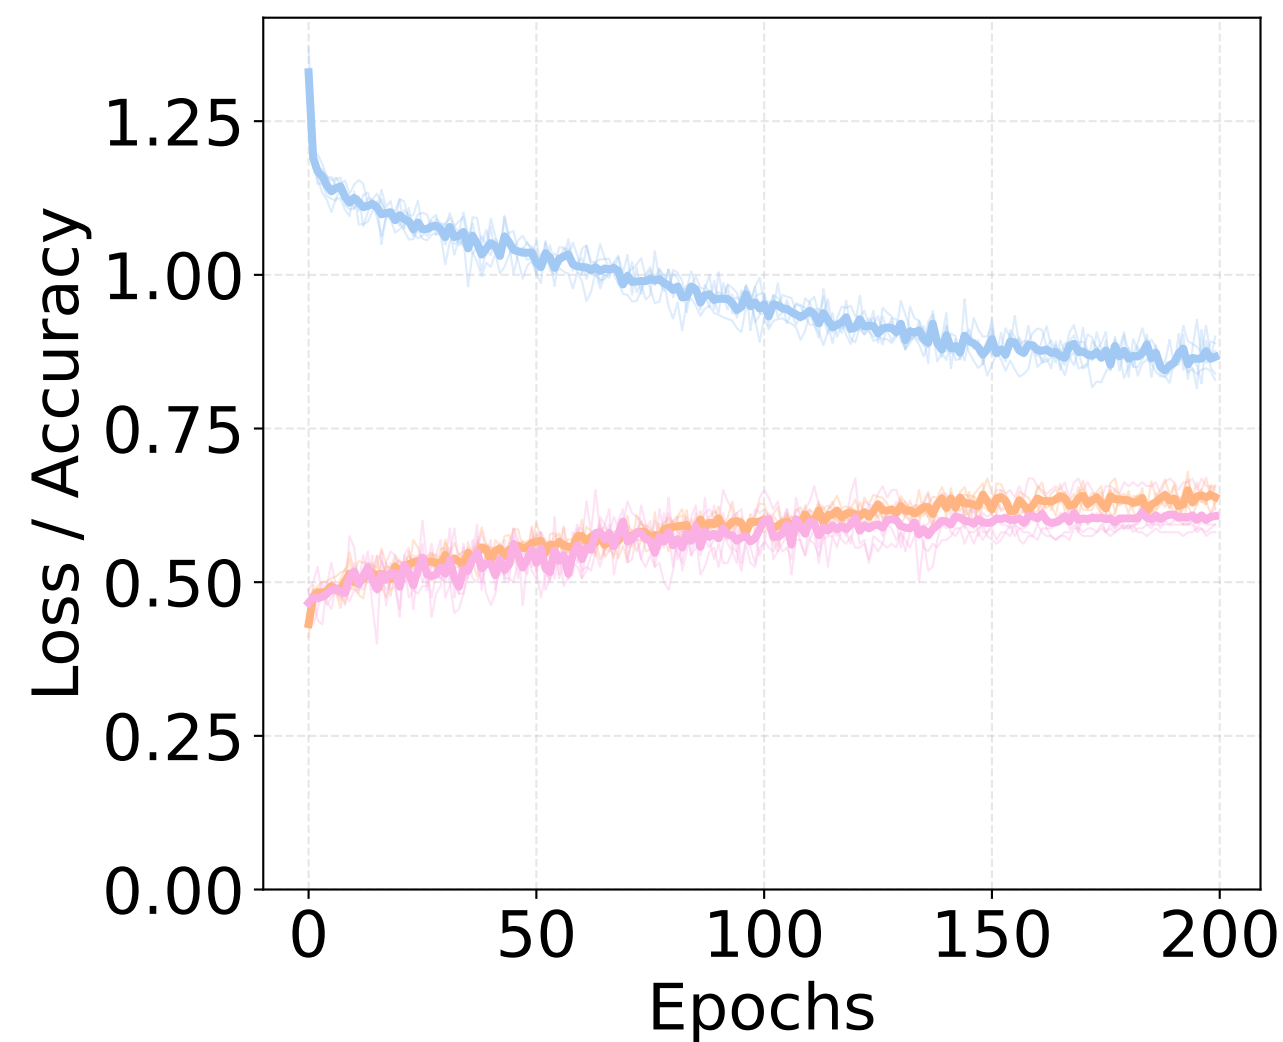
Test Acc: 0.933 ± 0.020 

— Train Loss — Train Accuracy — Validation Accuracy

Ionosphere

Test Acc: 0.920 ± 0.023 

Covtype

Test Acc: 0.604 ± 0.027 

Digits

Test Acc: 0.841 ± 0.030 