Cabinet de dermatologie Es-Senia


Triage support report — skin lesion

dermIA v2.0.0 · model ham10000-bcn20000-m5-v3 v3.0.0 (full profile)


Patient	P-2026-0421	Analysis date	01/08/2026, 13:46
Age	70 years	Requested by	Dr Karim Haddad
Sex	female	Body site	lower limb
Tracked lesion	#1 — jambe gauche	Decision thresholds	original

URGENT


Suspected melanoma
The probability of melanoma exceeds the safety threshold. Prompt dermatological assessment recommended.

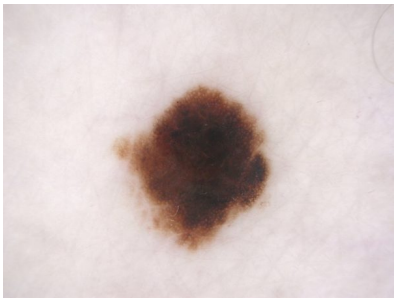

Analysed image

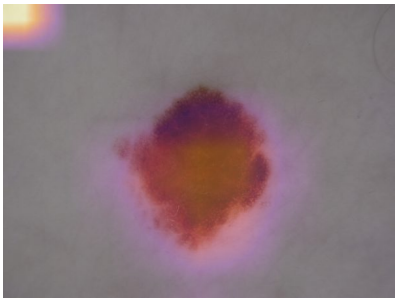

Most influential regions (Grad-CAM, “Melanoma”)

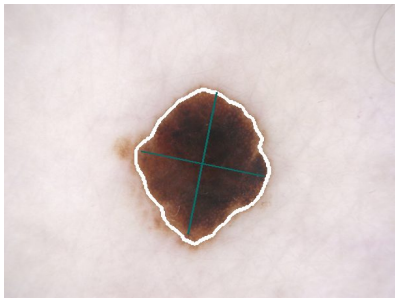

Outline and axes used for ABCD

Estimated probabilities

Diagnosis	Probability	In the guaranteed set*
Melanoma	91.7%	yes
Melanocytic nevus	8.3%	
Benign keratosis	0.0%	
Dermatofibroma	0.0%	
Vascular lesion	0.0%	
Actinic keratosis / Bowen's disease	0.0%	
Basal cell carcinoma	0.0%	

* Conformal set (Mondrian, alpha = 0.10): contains the true diagnosis with a probability of at least 90% for each class, assuming the cases resemble the calibration data. Melanoma decision if p(mel) ≥ 0.03 (cost ratio R = 10).
Original model thresholds, calibrated on its calibration set.

Automatic ABCD criteria (indicative)

Criterion	Measure	Detail
A — Asymmetry	2/2	asymmetric principal axes (shape or colours)
B — Border	1/8	sectors with an abrupt edge
C — Colours	3/6	light brown, dark brown, black
D — Diameter	6.0 mm	6 mm or less

Indicative automatic measurements: on the HAM10000 test set, each separates melanoma from nevus only modestly (AUC 0.66 to 0.73). They do not replace dermoscopic examination.

Change since the analysis of 18/04/2026 (105 days)

• Melanoma probability increased: from 44.8% to 91.7%.

Also compare the images visually: framing and magnification may differ between examinations.

Medical review

Confirmed by Dr Karim Haddad on 02/08/2026.

Final diagnosis: Melanoma

Physician's signature: _____

Disclaimer. This document is produced by a decision-support tool. It is not a diagnosis and replaces neither clinical examination nor histology. Model status: RESEARCH — non-commercial use — not a medical device. Training data: HAM10000 (Tschandl et al., Sci Data 2018, doi:10.1038/sdata.2018.161) + BCN20000 (Hernández-Pérez et al., Sci Data 2024, doi:10.1038/s41597-024-03387-w) — licence CC BY-NC 4.0 (non-commercial).