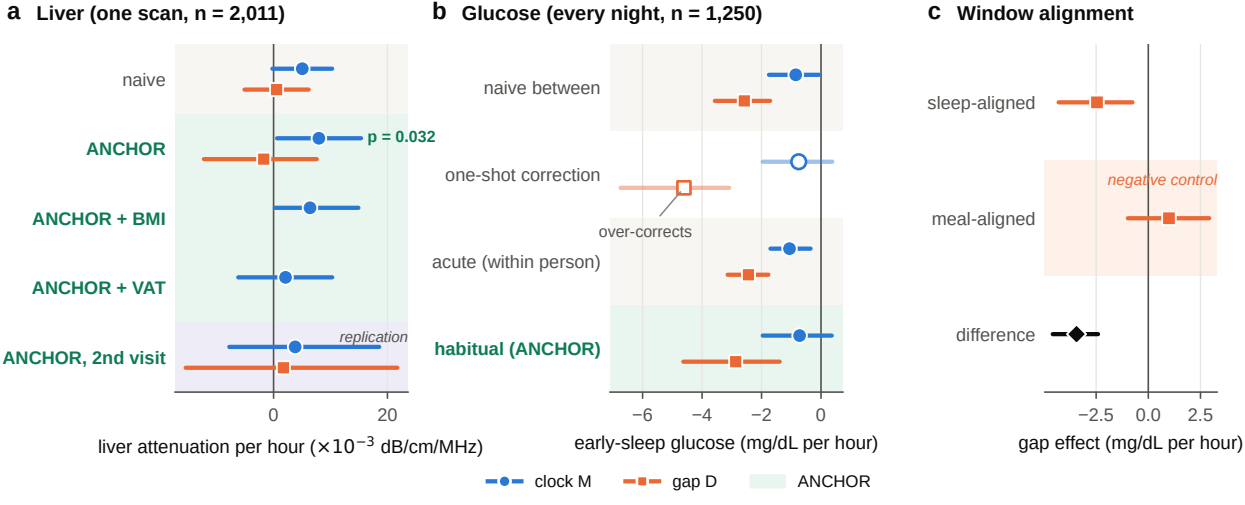
a Liver (one scan, n = 2,011)
naive
ANCHOR
p = 0.032
ANCHOR + BMI
ANCHOR + VAT
ANCHOR, 2nd visit
replication
0
20
liver attenuation per hour (×10⁻³ dB/cm/MHz)
b Glucose (every night, n = 1,250)
naive between
one-shot correction
over-corrects
acute (within person)
habitual (ANCHOR)
−6
−4
−2
0
early-sleep glucose (mg/dL per hour)
c Window alignment
sleep-aligned
negative control
meal-aligned
difference
−2.5
0.0
2.5
gap effect (mg/dL per hour)
clock M
gap D
ANCHOR