

ACCUTOME

Probe Freq: 12 MHz Max. Depth: 60 mm Gain: 57 dB

MRN: 11528696


Facility: RSUD DR. SAIFUL ANWAR

Physician: VR

Operator: DR. NADIA, SP.M(K)

OD 12--

Scan Date: 6/5/2023

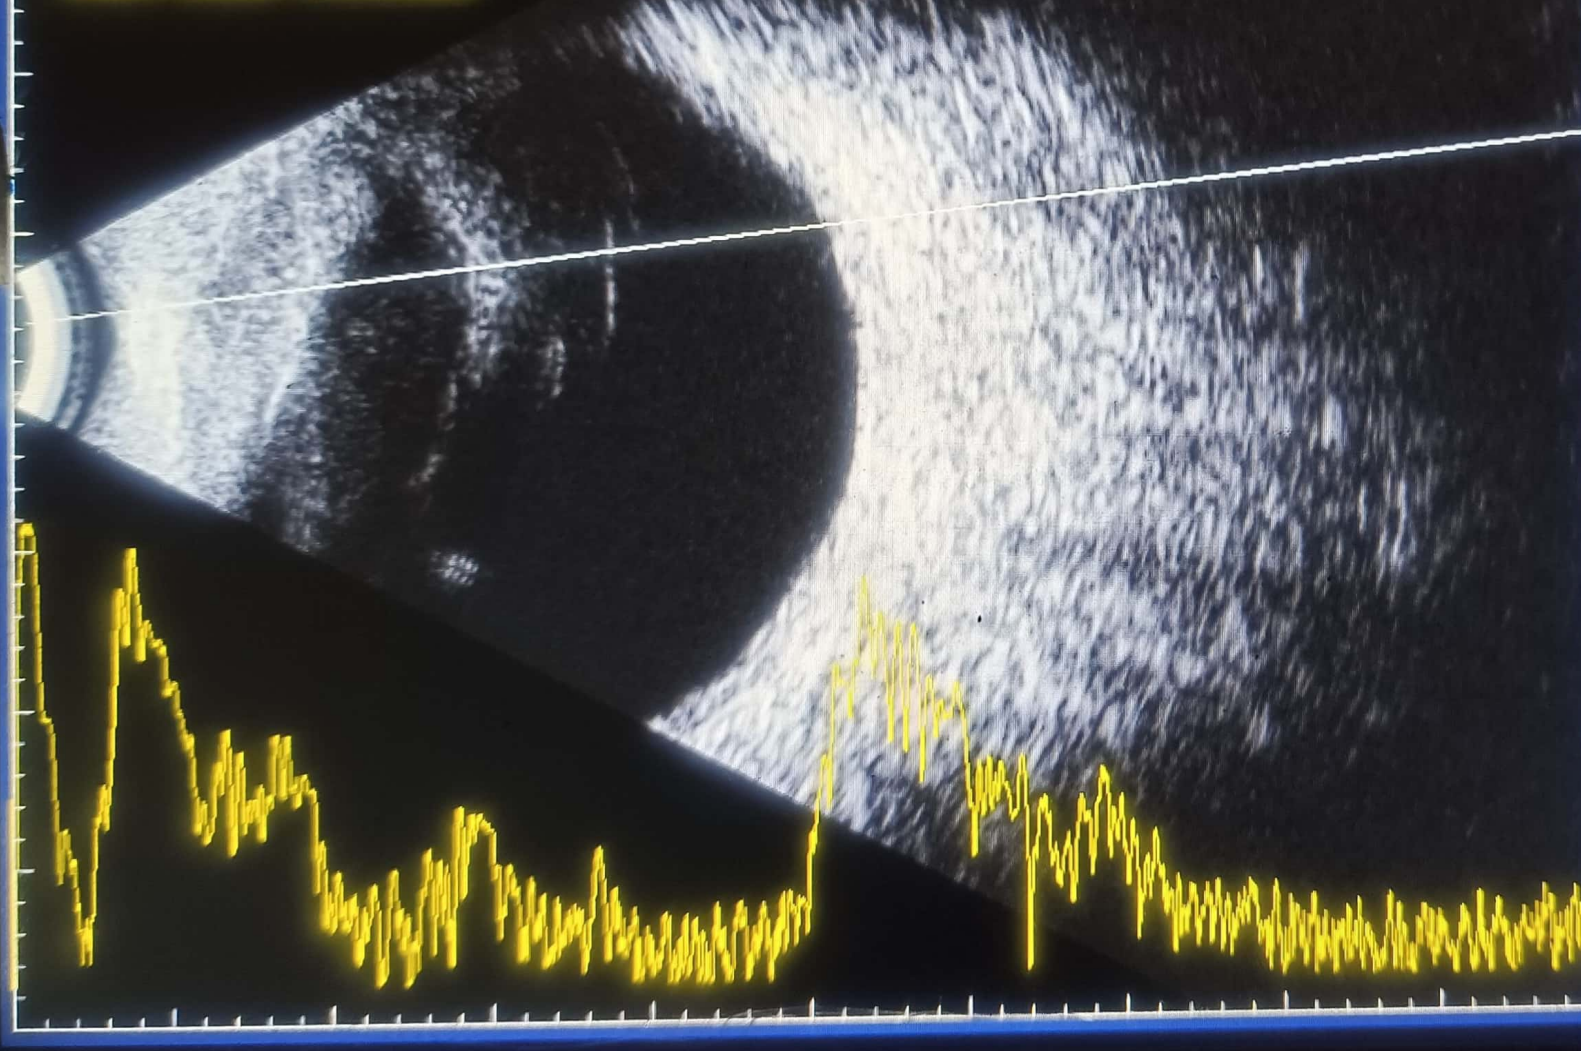

 ACCUTOME

Probe Freq: 12 MHz Max. Depth: 60 mm Gain: 55 dB

MRN: 11528696


Facility: RSUD DR. SAIFUL ANWAR

Physician: VR

Operator: DR. NADIA, SP.M(K)

OD 3AX

Scan Date: 6/5/2023

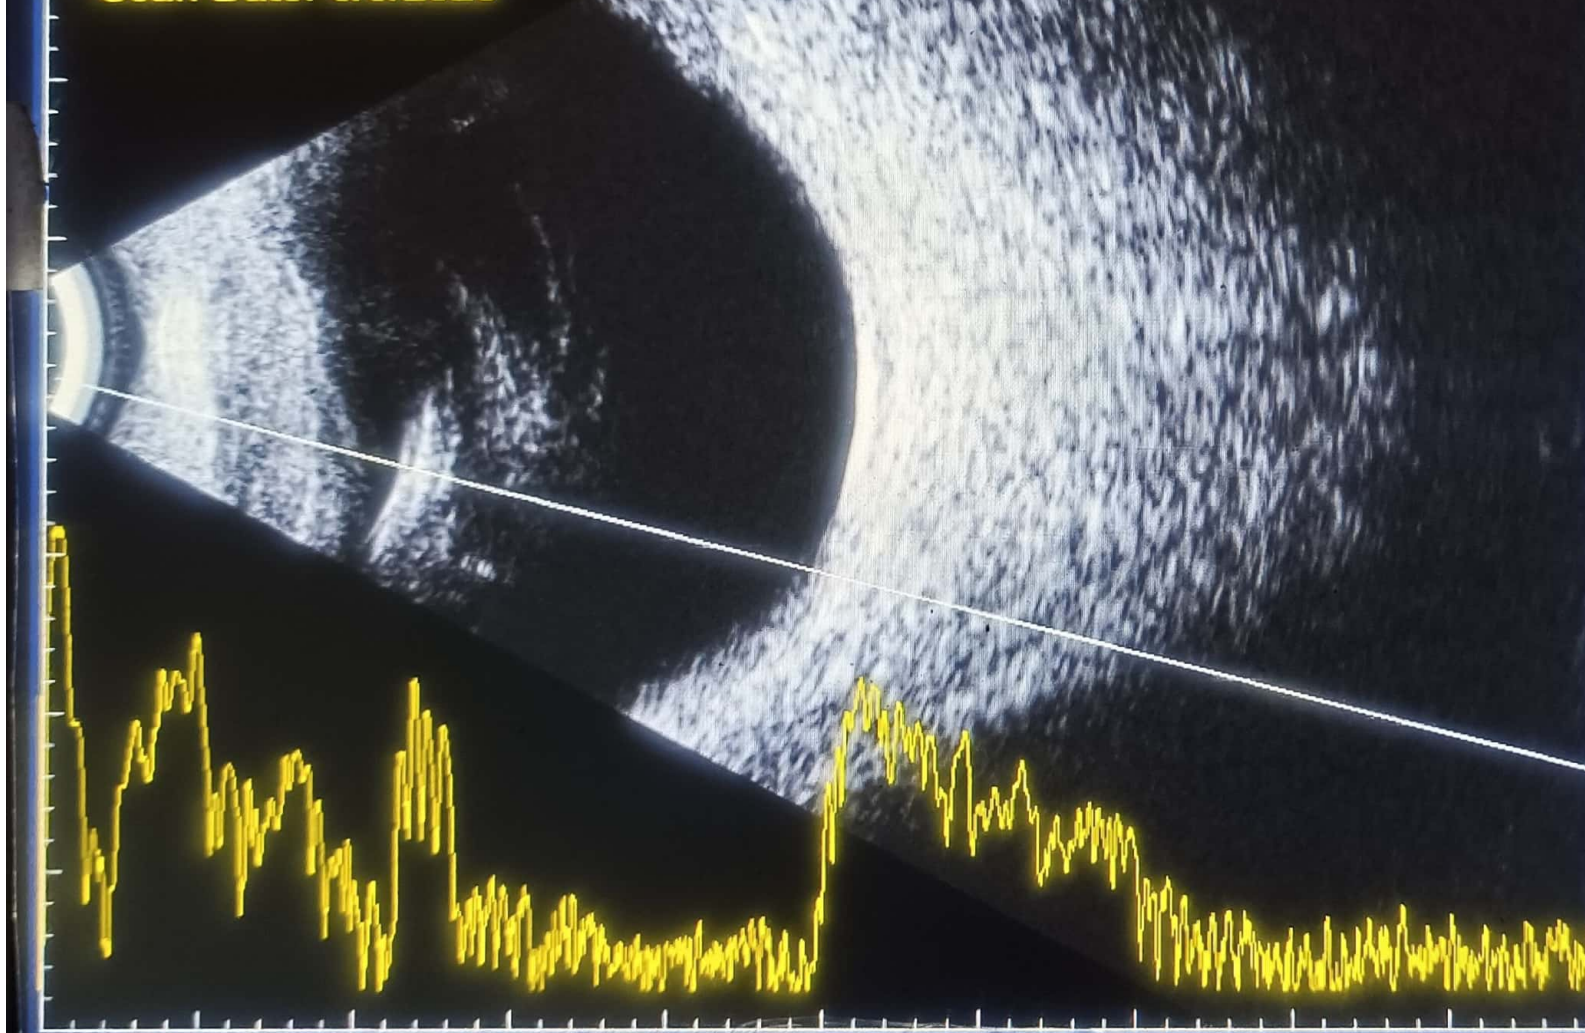



ACCUTOME

Probe Freq: 12 MHz Max. Depth: 60 mm Gain: 55 dB

MRN: 11528696

Facility: RSUD DR. SAIFUL ANWAR

Physician: VR

Operator: DR. NADIA, SP.M(K)

OD 11AX

Scan Date: 6/5/2023

