


NeuroPulseAI ECG Analysis Report


Clinical Grade BioAmp Monitoring System

Patient: Manas Tandon Age: 21 Blood Group: O+
Generated: 23-04-2026 13:47:41

I. ECG Clinical Waveform

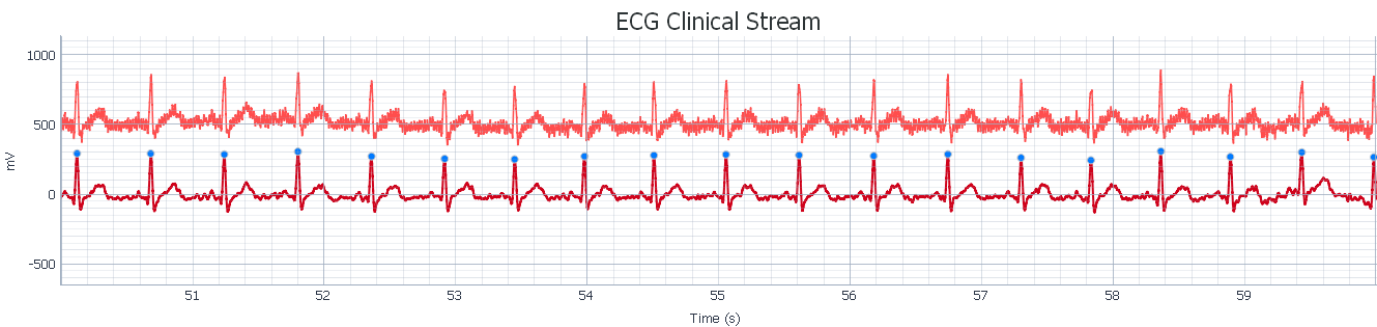

II. BPM Vital Trend

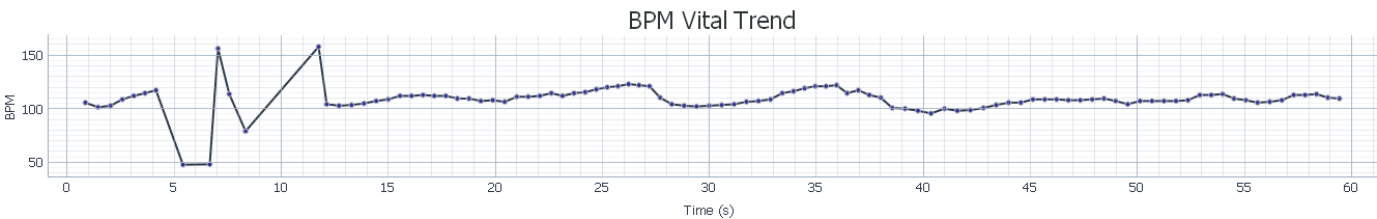

III. Analysis Metrics

Session Duration: 60.0s | Mean BPM: 108.82 | R-Peak Count: 102 | Signal Quality: Good

IV. Clinical Observations

- Recording duration 60.0 sec at approx 250.0 Hz sampling.
- Detected 102 R-peaks with signal quality marked as good.
- Average BPM 108.8, range 47.6 to 157.9.
- Estimated short-term variability (SDNN) 108.5 ms.

V. Engineering Diagnostics

- Signal morphology is stable enough for engineering-level ECG review.
- Detected heart rate is above 100 BPM in this window.
- Short-term variability appears high or peak detection may be unstable.
- These are engineering diagnostics, not a clinical diagnosis.

AI Summary Note:

Recording duration 60.0 sec at approx 250.0 Hz sampling. Detected 102 R-peaks with signal quality marked as good. Average BPM 108.8, range 47.6 to 157.9. Estimated short-term variability (SDNN) 108.5 ms. Signal morphology is stable enough for engineering-level ECG review. Detected heart rate is above 100 BPM in this window. Short-term variability appears high or peak detection may be unstable. These are engineering diagnostics, not a clinical diagnosis. AI Analyst note: this report supports engineering interpretation and is not a certified medical diagnosis.