


NeuroPulseAI ECG Analysis Report

Clinical Grade BioAmp Monitoring System


Patient: Aditya Kumar Singh Age: N/A Blood Group: N/A

Generated: 23-04-2026 15:21:20

I. ECG Clinical Waveform

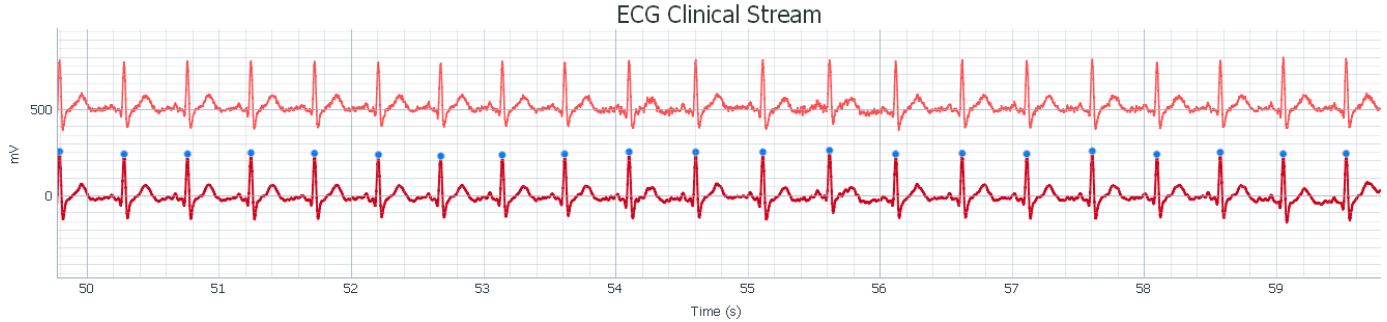

II. BPM Vital Trend

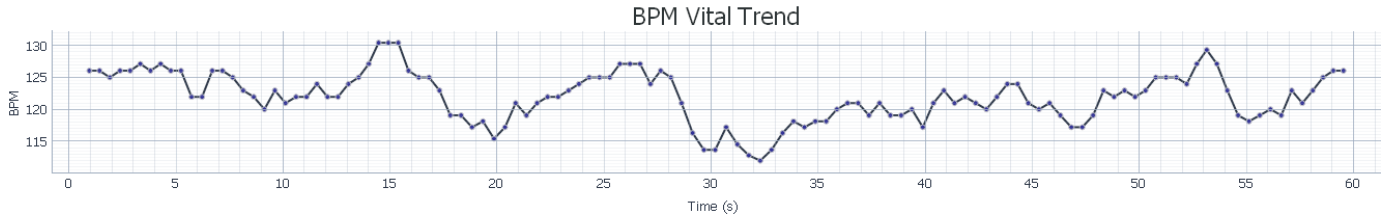

III. Analysis Metrics

Session Duration: 59.78s | Mean BPM: 122.07 | R-Peak Count: 121 | Signal Quality: Good

IV. Clinical Observations

- Recording duration 59.8 sec at approx 250.0 Hz sampling.
- Detected 121 R-peaks with signal quality marked as good.
- Average BPM 122.1, range 111.9 to 130.4.
- Estimated short-term variability (SDNN) 15.8 ms.

V. Engineering Diagnostics

- Signal morphology is stable enough for engineering-level ECG review.
- Detected heart rate is above 100 BPM in this window.
- Short-term variability appears low in this segment.
- These are engineering diagnostics, not a clinical diagnosis.

AI Summary Note:

Recording duration 59.8 sec at approx 250.0 Hz sampling. Detected 121 R-peaks with signal quality marked as good. Average BPM 122.1, range 111.9 to 130.4. Estimated short-term variability (SDNN) 15.8 ms. Signal morphology is stable enough for engineering-level ECG review. Detected heart rate is above 100 BPM in this window. Short-term variability appears low in this segment. These are engineering diagnostics, not a clinical diagnosis. AI Analyst note: this report supports engineering interpretation and is not a certified medical diagnosis.