


NeuroPulseAI ECG Analysis Report


Clinical Grade BioAmp Monitoring System

Patient: Aditya Kumar Singh Age: N/A Blood Group: N/A
Generated: 23-04-2026 15:46:58

I. ECG Clinical Waveform

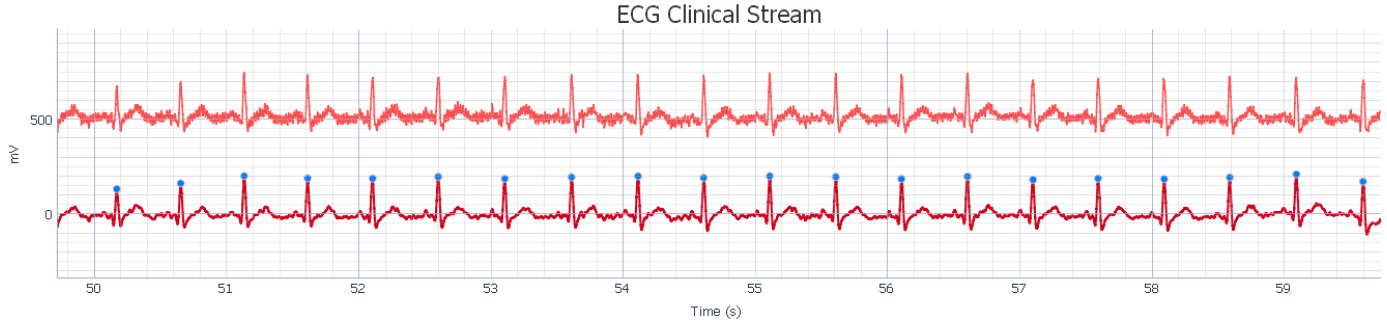

II. BPM Vital Trend

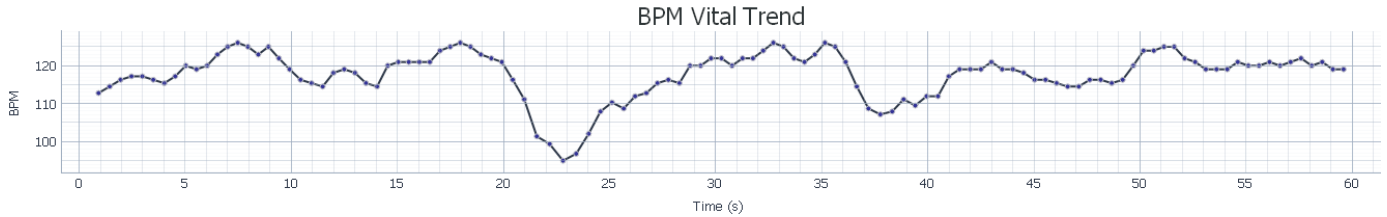

III. Analysis Metrics

Session Duration: 59.72s | Mean BPM: 117.87 | R-Peak Count: 117 | Signal Quality: Good

IV. Clinical Observations

- Recording duration 59.7 sec at approx 250.0 Hz sampling.
- Detected 117 R-peaks with signal quality marked as good.
- Average BPM 117.9, range 94.9 to 126.0.
- Estimated short-term variability (SDNN) 28.4 ms.

V. Engineering Diagnostics

- Signal morphology is stable enough for engineering-level ECG review.
- Detected heart rate is above 100 BPM in this window.
- Short-term variability appears moderate in this segment.
- These are engineering diagnostics, not a clinical diagnosis.

AI Summary Note:

Recording duration 59.7 sec at approx 250.0 Hz sampling. Detected 117 R-peaks with signal quality marked as good. Average BPM 117.9, range 94.9 to 126.0. Estimated short-term variability (SDNN) 28.4 ms. Signal morphology is stable enough for engineering-level ECG review. Detected heart rate is above 100 BPM in this window. Short-term variability appears moderate in this segment. These are engineering diagnostics, not a clinical diagnosis. AI Analyst note: this report supports engineering interpretation and is not a certified medical diagnosis.