


NeuroPulseAI ECG Analysis Report

Clinical Grade BioAmp Monitoring System


Patient: Aditya Kumar Singh Age: N/A Blood Group: N/A

Generated: 29-04-2026 18:05:35

I. ECG Clinical Waveform

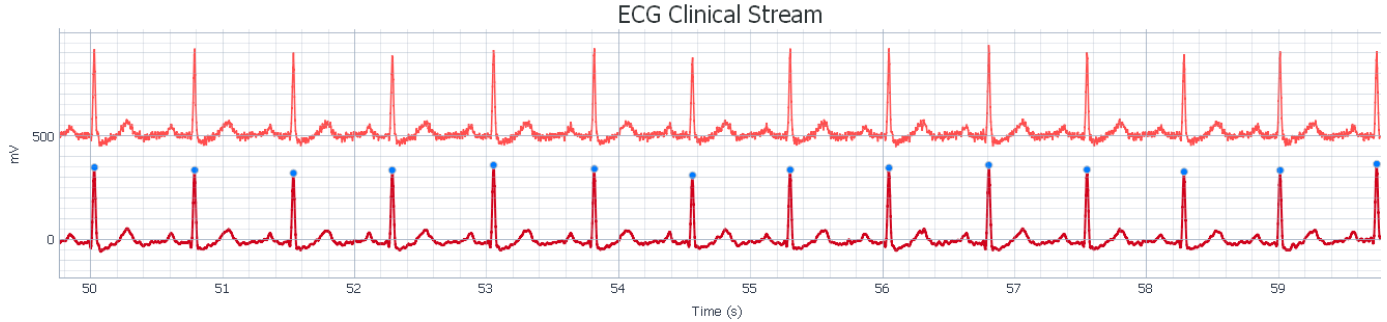

II. BPM Vital Trend

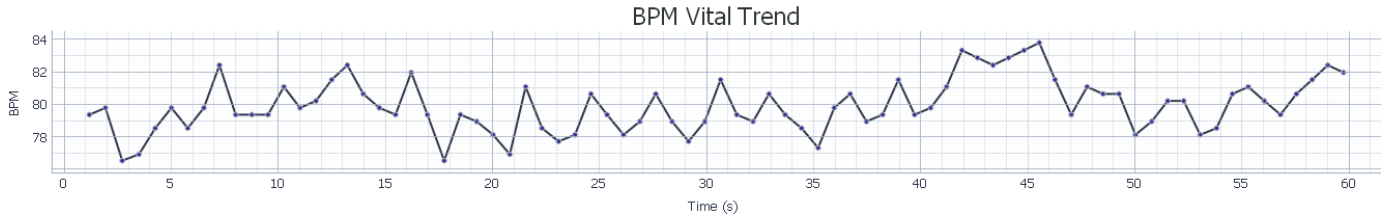

III. Analysis Metrics

Session Duration: 59.77s | Mean BPM: 79.93 | R-Peak Count: 80 | Signal Quality: Good

IV. Clinical Observations

- Recording duration 59.8 sec at approx 250.0 Hz sampling.
- Detected 80 R-peaks with signal quality marked as good.
- Average BPM 79.9, range 76.5 to 83.8.
- Estimated short-term variability (SDNN) 15.3 ms.

V. Engineering Diagnostics

- Signal morphology is stable enough for engineering-level ECG review.
- Detected heart rate lies in the common resting reference range.
- Short-term variability appears low in this segment.
- These are engineering diagnostics, not a clinical diagnosis.

AI Summary Note:

Recording duration 59.8 sec at approx 250.0 Hz sampling. Detected 80 R-peaks with signal quality marked as good. Average BPM 79.9, range 76.5 to 83.8. Estimated short-term variability (SDNN) 15.3 ms. Signal morphology is stable enough for engineering-level ECG review. Detected heart rate lies in the common resting reference range. Short-term variability appears low in this segment. These are engineering diagnostics, not a clinical diagnosis. AI Analyst note: this report supports engineering interpretation and is not a certified medical diagnosis.