


NeuroPulseAI ECG Analysis Report


Clinical Grade BioAmp Monitoring System

Patient: Aditya Kumar Singh Age: N/A Blood Group: N/A
Generated: 02-05-2026 12:28:47

I. ECG Clinical Waveform

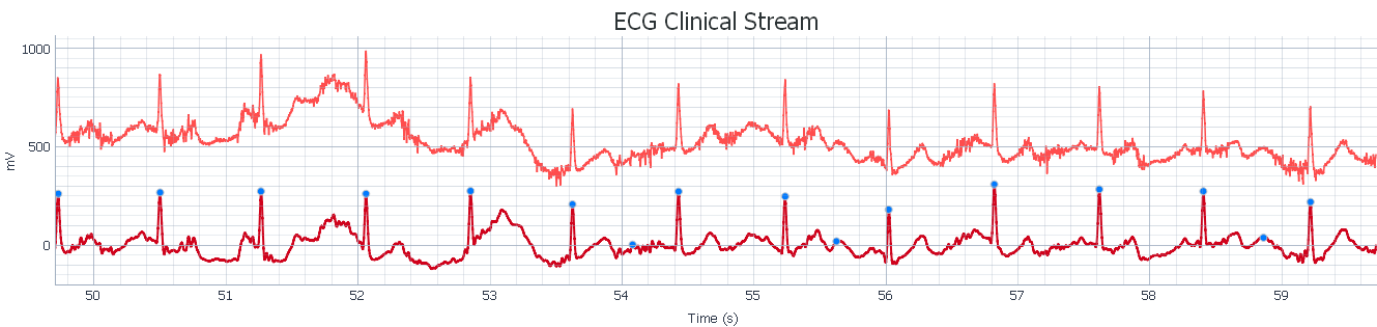

II. BPM Vital Trend

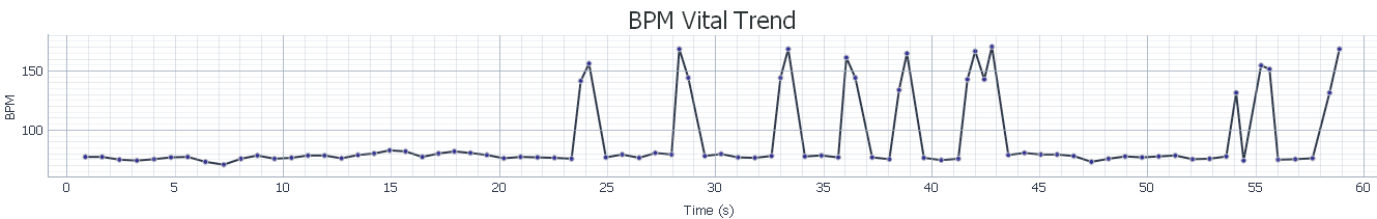

III. Analysis Metrics

Session Duration: 59.71s | Mean BPM: 94.02 | R-Peak Count: 87 | Signal Quality: Good

IV. Clinical Observations

- Recording duration 59.7 sec at approx 250.0 Hz sampling.
- Detected 87 R-peaks with signal quality marked as good.
- Average BPM 94.0, range 70.8 to 170.4.
- Estimated short-term variability (SDNN) 160.8 ms.

V. Engineering Diagnostics

- Signal morphology is stable enough for engineering-level ECG review.
- Detected heart rate lies in the common resting reference range.
- Short-term variability appears high or peak detection may be unstable.
- These are engineering diagnostics, not a clinical diagnosis.

AI Summary Note:

Recording duration 59.7 sec at approx 250.0 Hz sampling. Detected 87 R-peaks with signal quality marked as good. Average BPM 94.0, range 70.8 to 170.4. Estimated short-term variability (SDNN) 160.8 ms. Signal morphology is stable enough for engineering-level ECG review. Detected heart rate lies in the common resting reference range. Short-term variability appears high or peak detection may be unstable. These are engineering diagnostics, not a clinical diagnosis. AI Analyst note: this report supports engineering interpretation and is not a certified medical diagnosis.