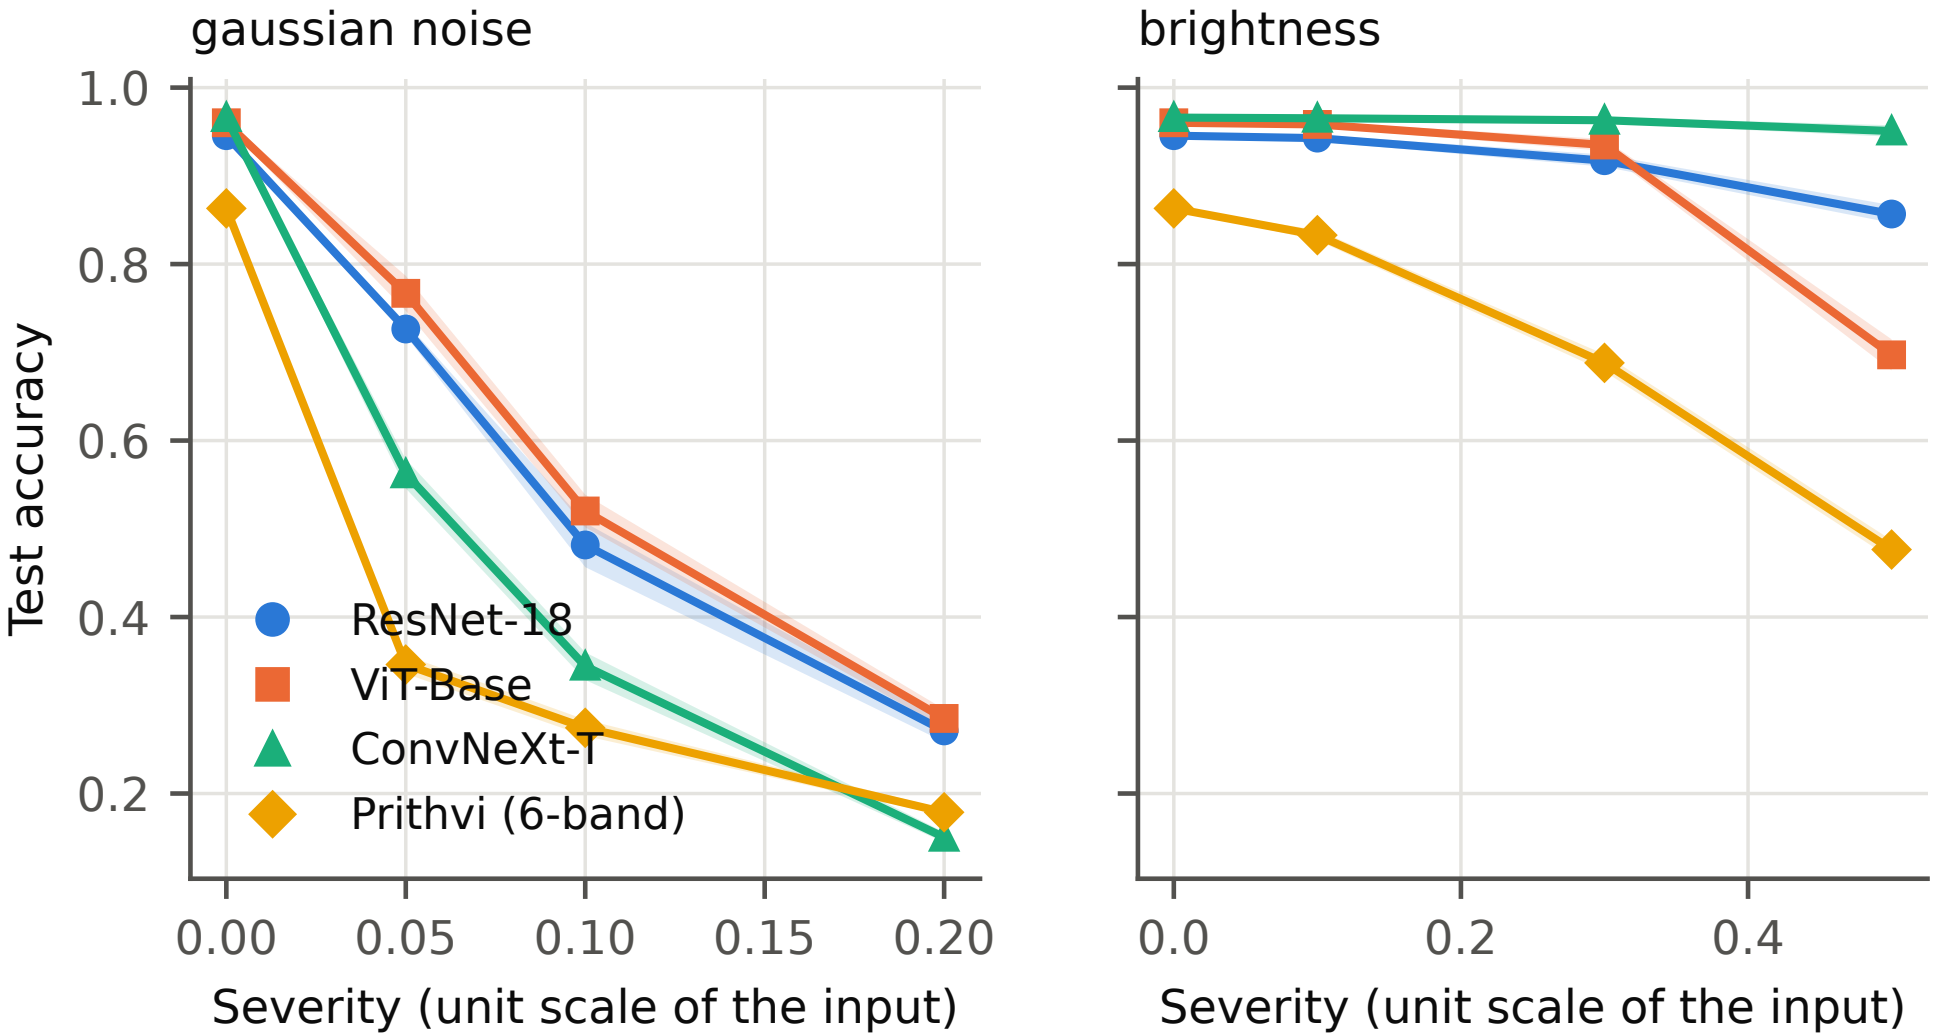
gaussian noise
brightness
Test accuracy
1.0
0.8
0.6
0.4
0.2
ResNet-18
ViT-Base
ConvNeXt-T
Prithvi (6-band)
0.00
0.05
0.10
0.15
0.20
0.0
0.2
0.4
Severity (unit scale of the input)
Severity (unit scale of the input)