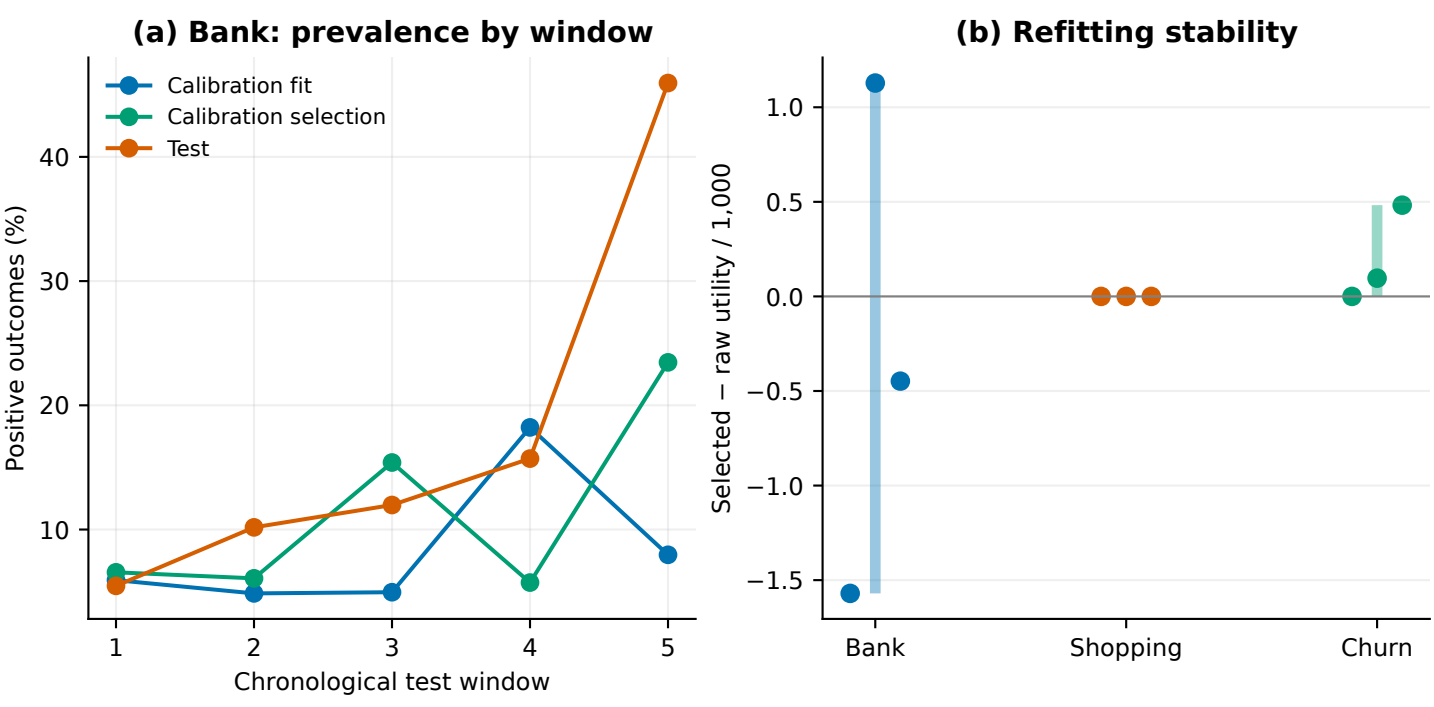
(a) Bank: prevalence by window
Calibration fit
Calibration selection
Test
Positive outcomes (%)
10
20
30
40
1
2
3
4
5
Chronological test window
(b) Refitting stability
Selected − raw utility / 1,000
1.0
0.5
0.0
−0.5
−1.0
−1.5
Bank
Shopping
Churn