


## Fiducial ROIs

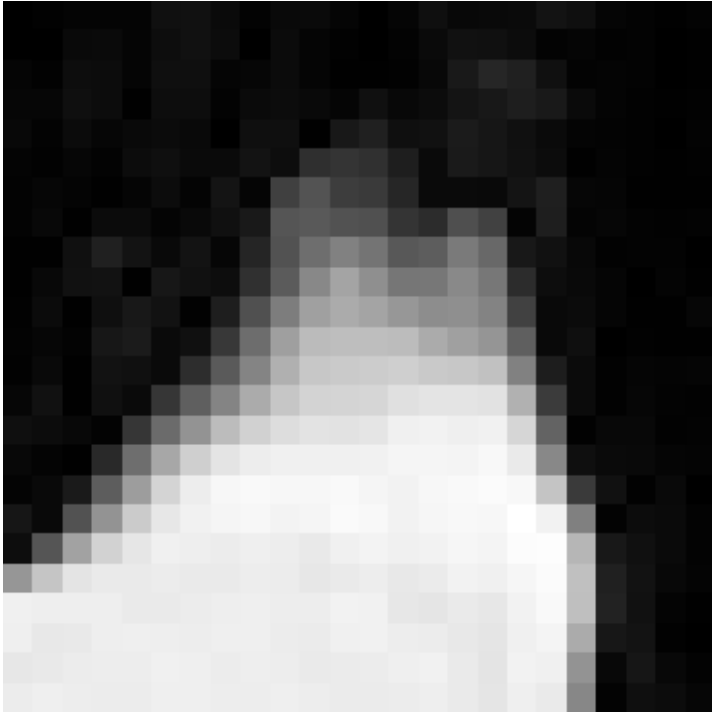


## Institution Table

Name	Johns Hopkins
Number of Licenses	12
Address	3101 Wyman Park Dr. Baltimore, MD 21211
Phone Number	555-555-5555


## Data Acquisition Table

Phantom filler $T_1$	
Phantom filler $T_2$	
Phantom filler composition	
Sequence type	GR
Pixel bandwidth	$160 \frac{\text{Hz}}{\text{px}}$
Voxel dimensions	0.977 mm x 0.977 mm x 1.0 mm
Sequence repetition time (TR)	10 ms
Echo delay time (TE)	4.76 ms
Number of signals averaged (NSA)	1
Data acquisition matrix size	256, 0, 0, 218
Image matrix size	
Field of view size	
Type of acquisition	3D
Number of slices	192
Slice orientation	1, 0, 0, 0, 1, 0
Slice position	-125.0, -102.88, 137.371
Slice thickness	1 mm
Direction of phase encoding	COL


Axial Contour Plot

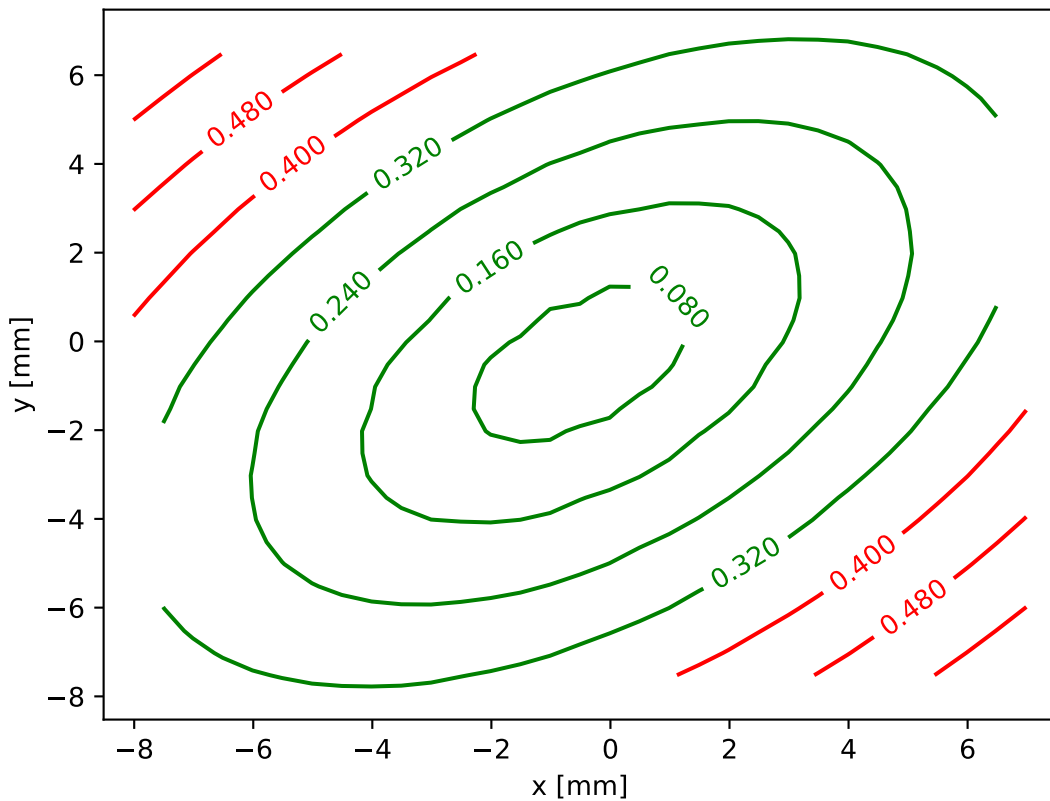


Sagittal Contour Plot

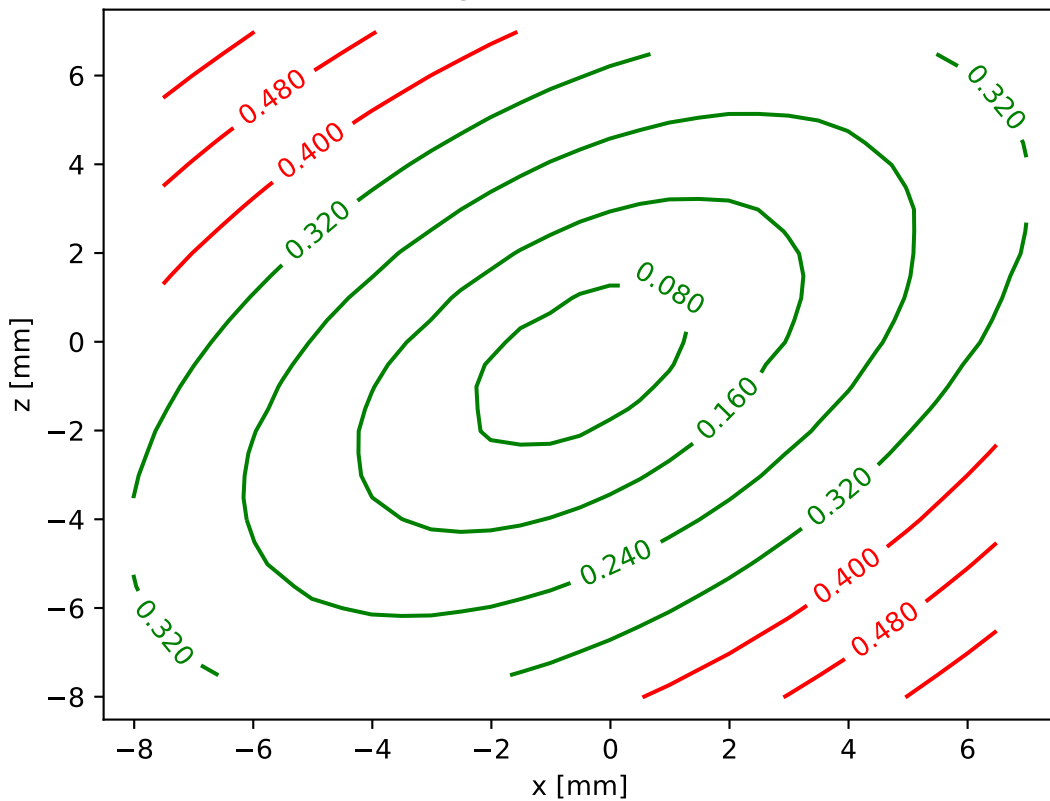


Coronal Contour Plot

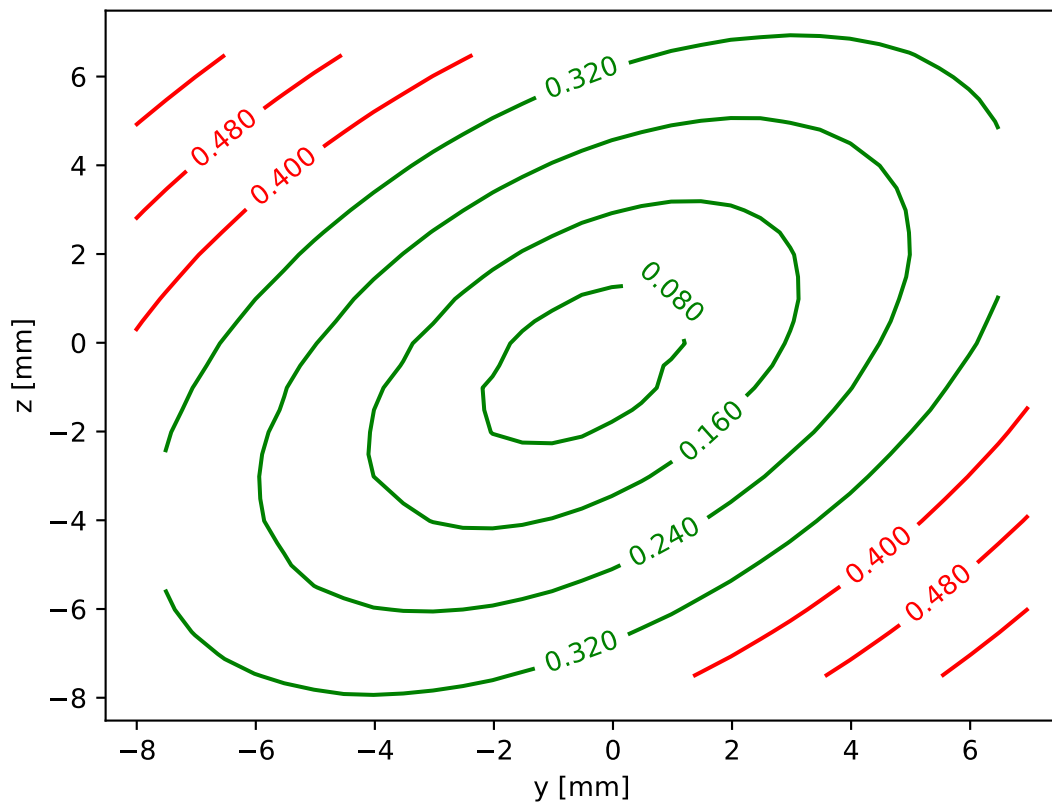

Axial Contour Plot Series ( $z = -6.514493171792839$  mm)

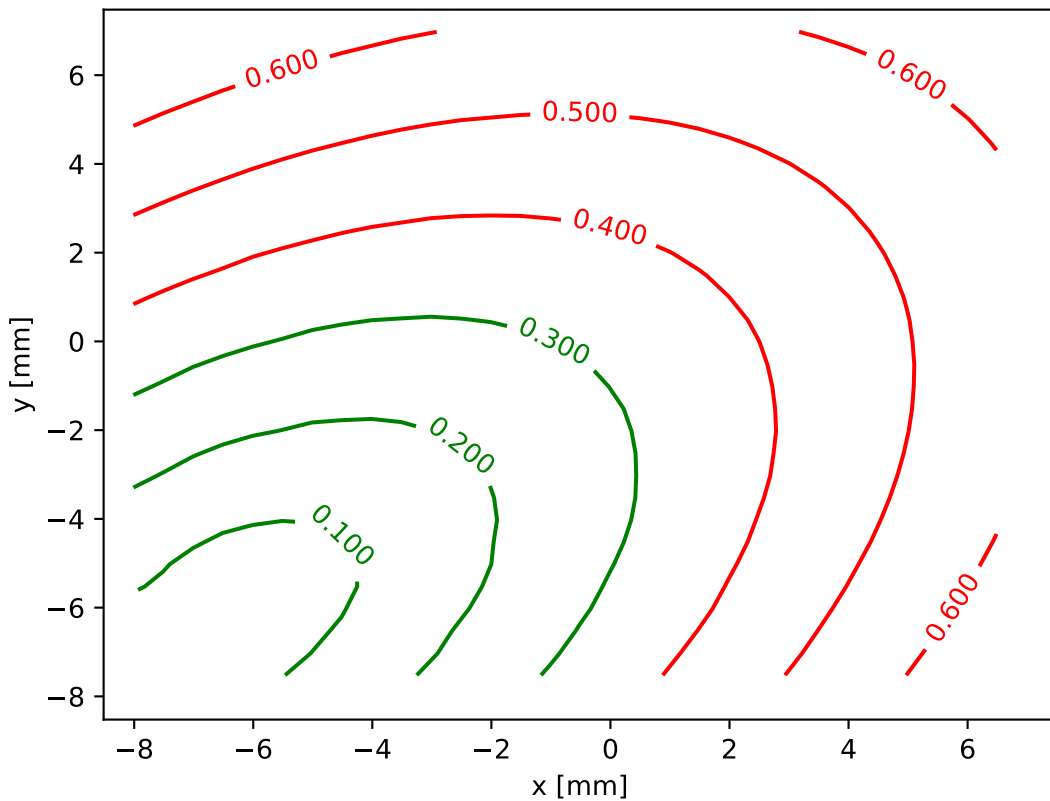


Axial Contour Plot Series ( $z = -4.514493171792839$  mm)

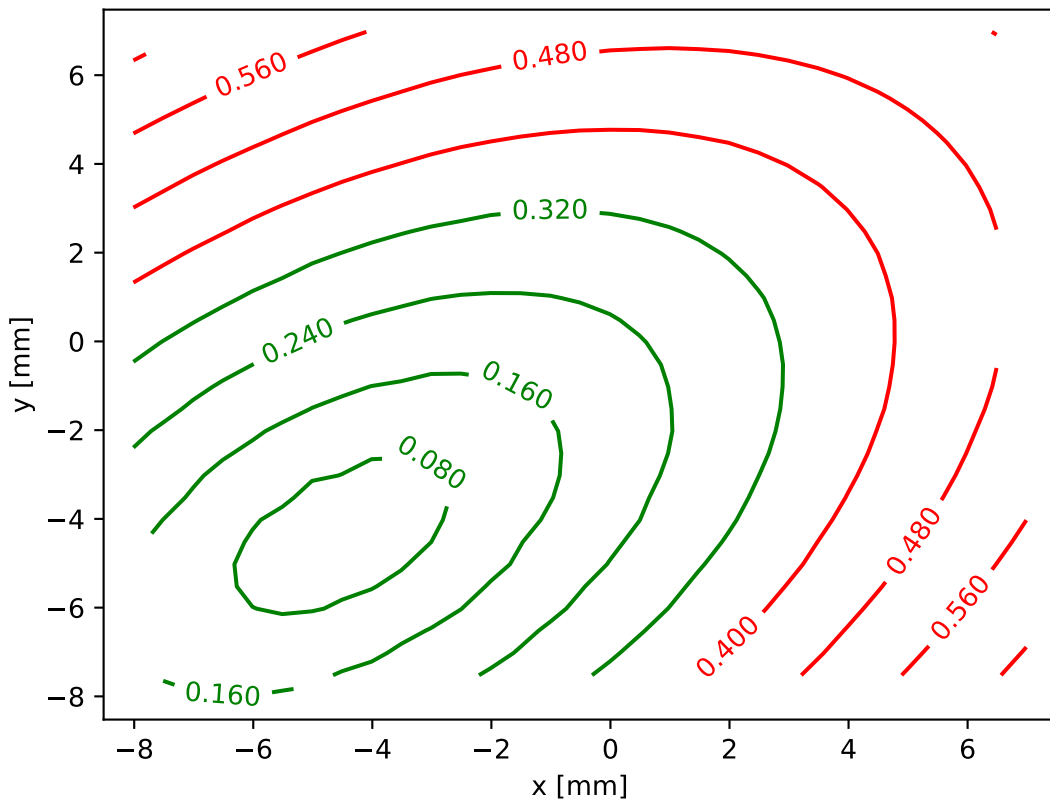





Axial Contour Plot Series ( $z = -2.5144931717928394$  mm)

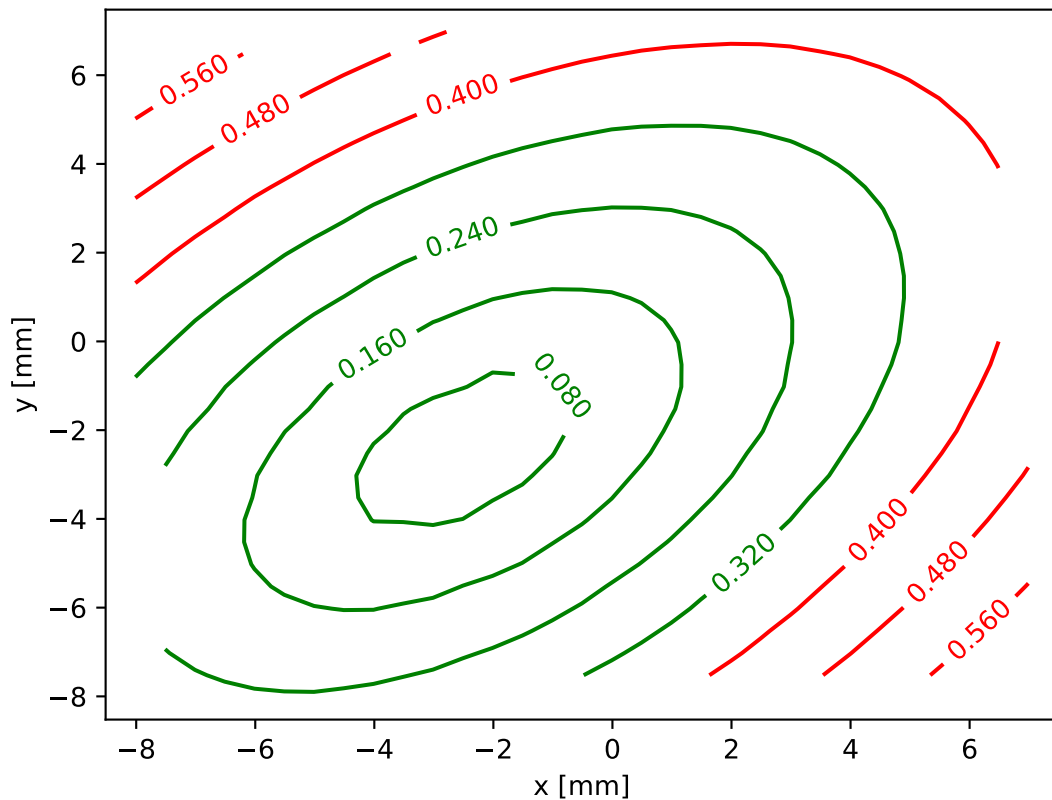


Axial Contour Plot Series ( $z = -0.5144931717928394$  mm)

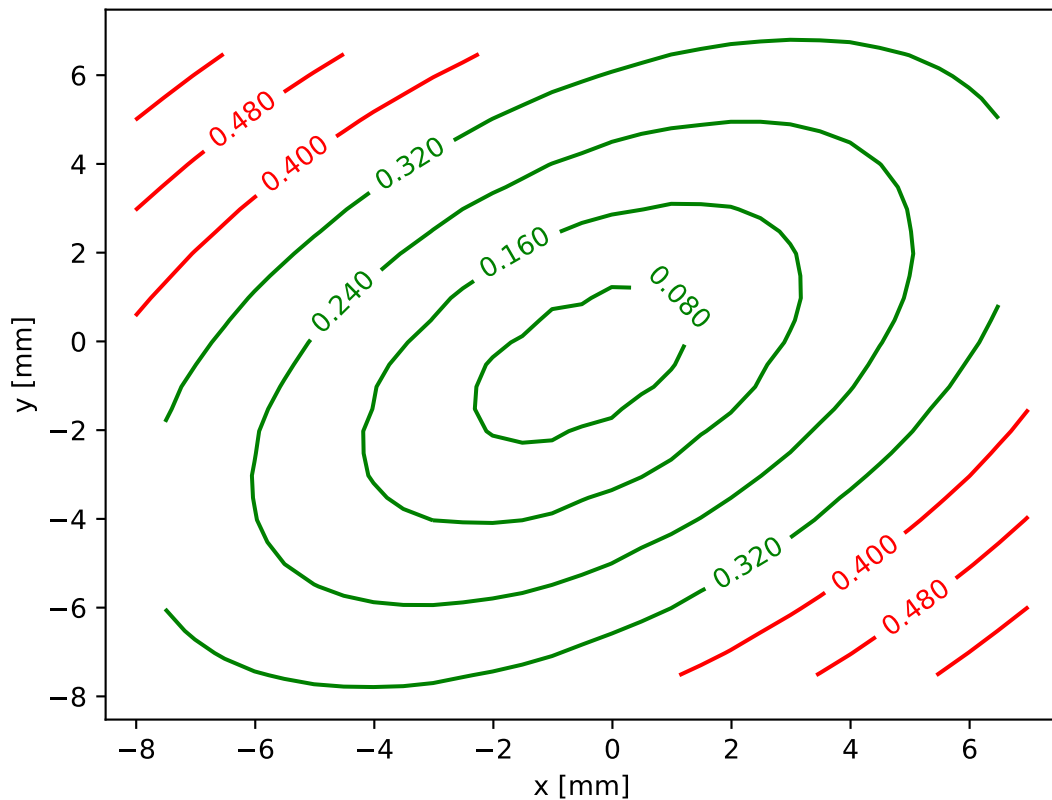


Axial Contour Plot Series ( $z = 1.4855068282071606$  mm)

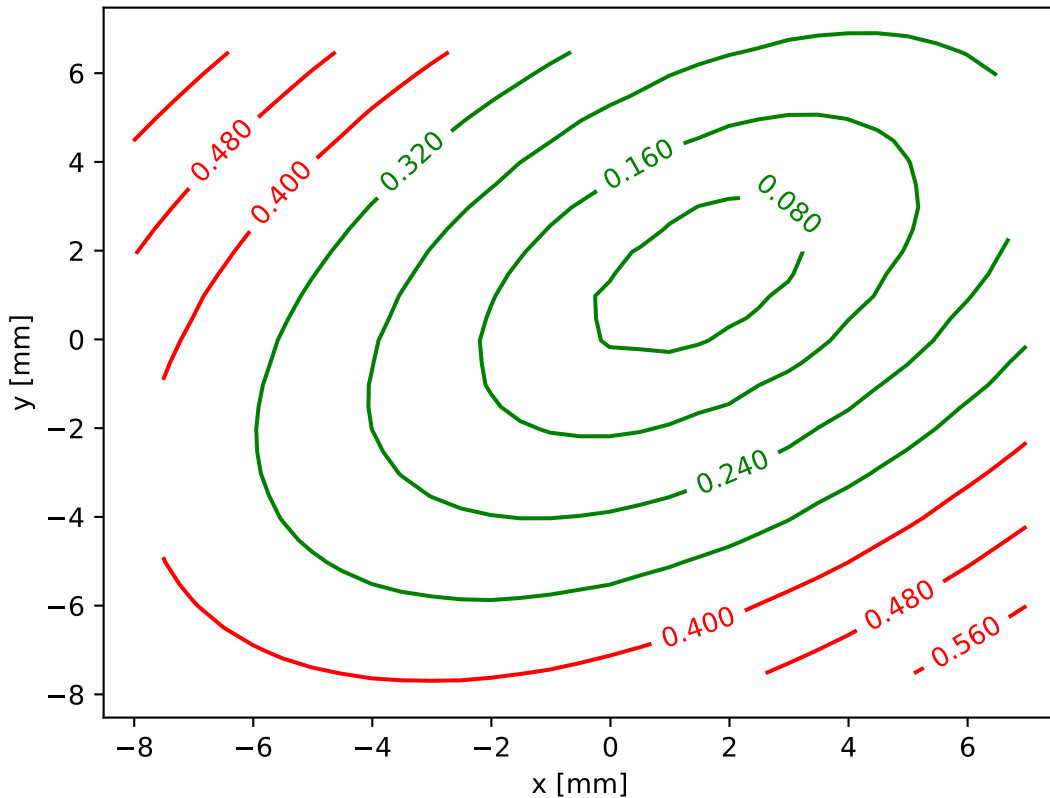


Axial Contour Plot Series ( $z = 3.4855068282071606$  mm)

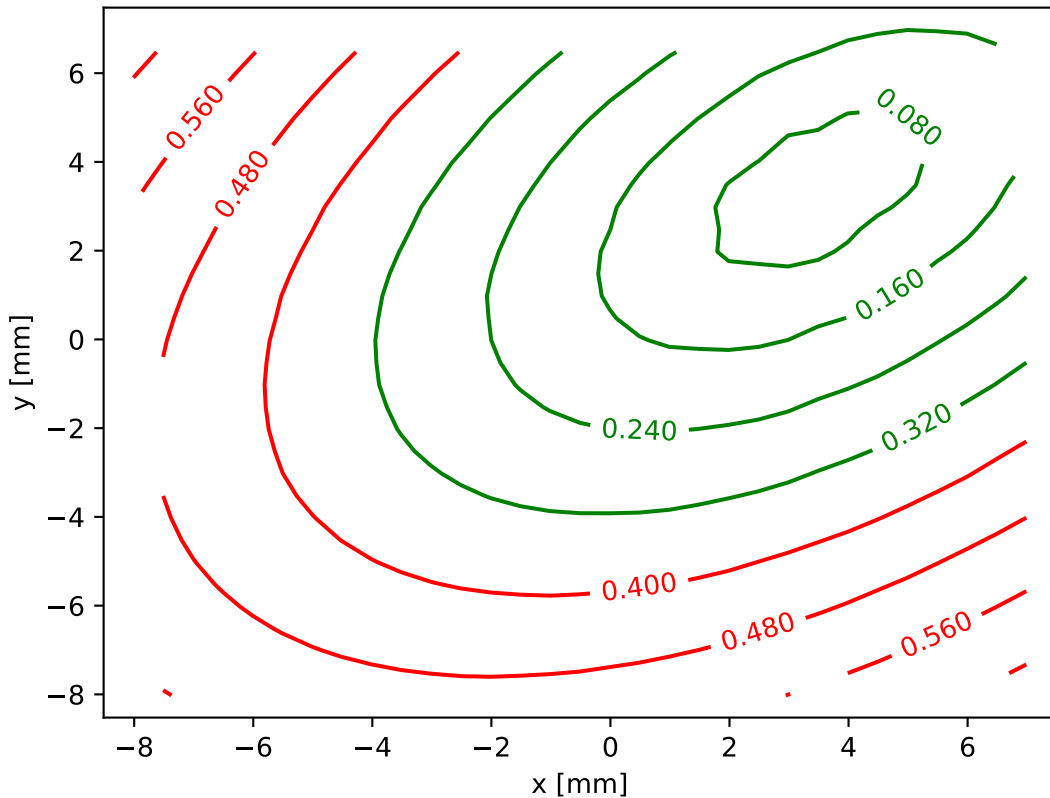

Axial Contour Plot Series ( $z = 5.485506828207161$  mm)

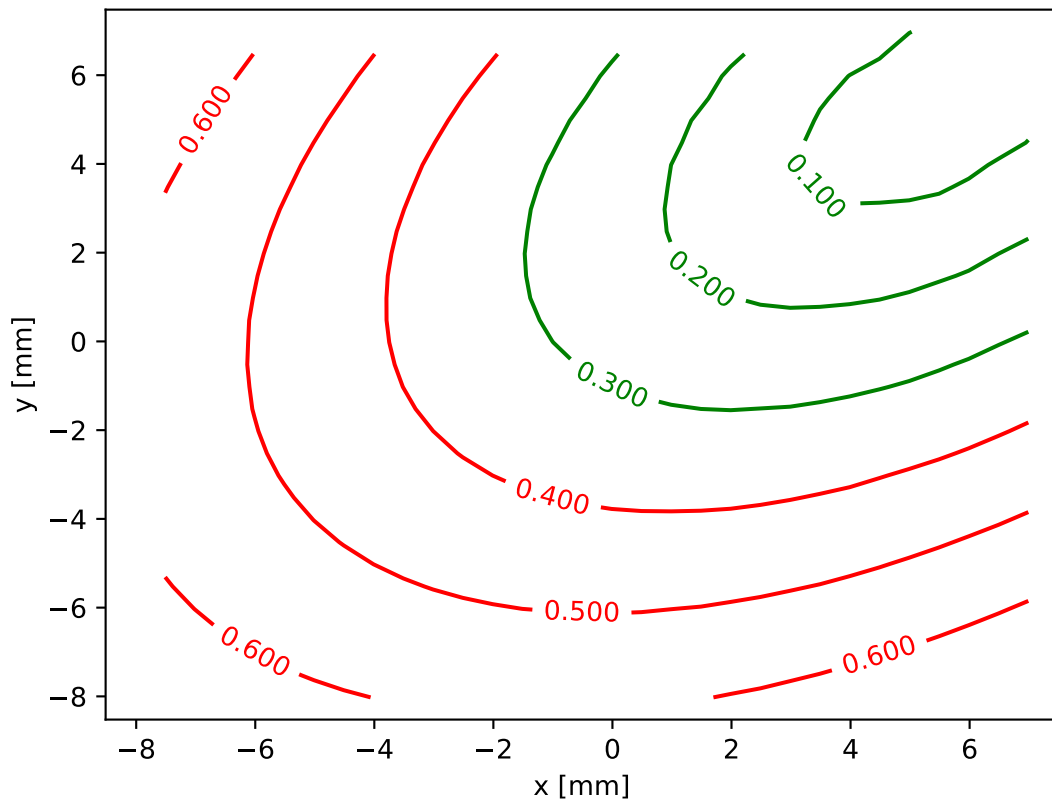

Scatter Plot of Geometric Distortion vs. Distance from Isocenter

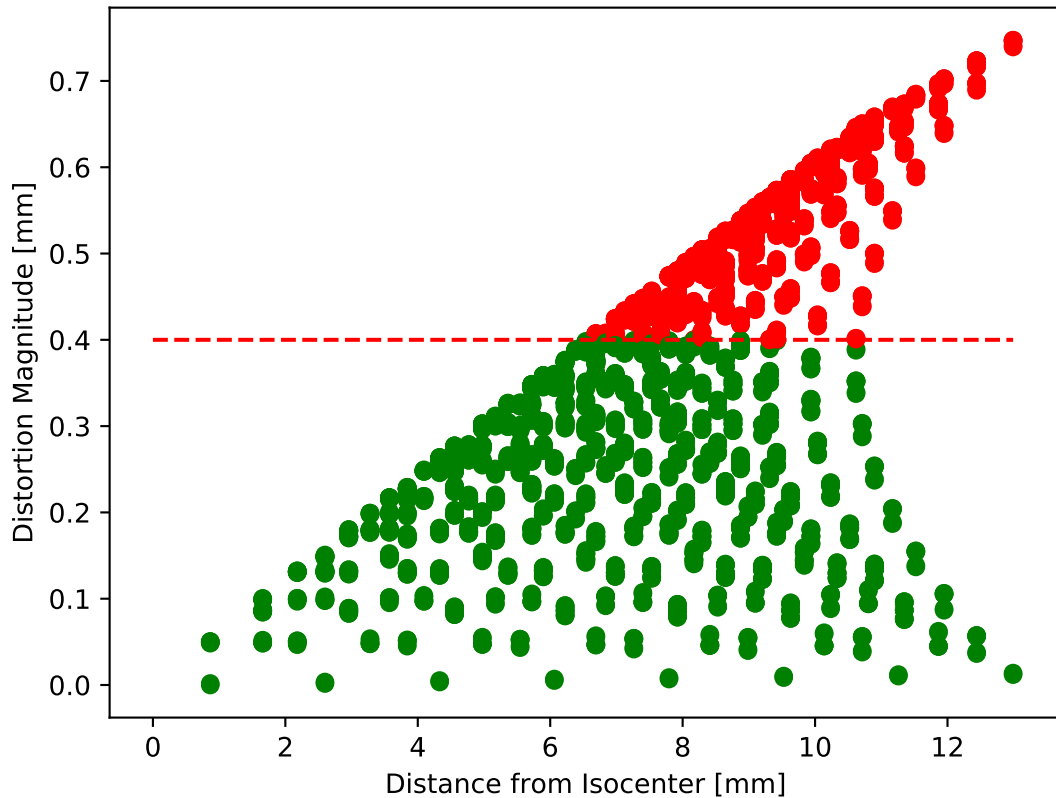

## Error Table

Distance from Isocenter [mm]	Maximum Error [mm]	Average Error [mm]
1.0	0.066	0.054
2.0	0.125	0.098
3.0	0.185	0.146
4.0	0.246	0.193
5.0	0.306	0.24
6.0	0.367	0.288
7.0	0.428	0.335

