

# Shapeless Adaptive Removal of the Transcranial Alternating Current Stimulation Artifact from the Electroencephalogram

Robert Guggenberger<sup>1,\*</sup>, Falk Schlegelmilch<sup>2</sup>, and Alireza Gharabaghi<sup>1</sup>

<sup>1</sup>Department for Translational Neurosurgery, University Hospital Tübingen

<sup>2</sup>neuroConn GmbH, Ilmenau

\*Corresponding author: robert.guggenberger@posteo.eu

April 19, 2017

## Abstract

Your abstract.

## 1 Introduction

The combination of transcranial alternating current stimulation (tACS) and electroencephalogram (EEG) has been explored in several recent studies. While the analysis of EEG before or after stimulation posits limited technical challenges, the EEG recording during stimulation is heavily affected by the stimulation artifact.

### 1.1 Matched Phase and Frequency

Computational simulations suggest that the power of endogenous oscillations would increase most if the frequency of tACS matches the targets eigenfrequency (Kutchko and Fröhlich, 2013; Zaehle et al., 2010). This has been supported by evidence from animal studies (Schmidt et al., 2014), and human studies combining tACS with transcranial magnetic stimulation (TMS) (Guerra et al., 2016), or contrasting pre and post resting state power analysis (Zaehle et al., 2010). It has also been suggested that the phase of neuronal populations would be locked to the phase of the tACS signal (Reato et al., 2013). This has been supported by evidence from studies combining tACS with motor output (Brittain et al., 2013), TMS (Raco et al., 2016; Nakazono et al., 2016) or sensory perception (Gundlach et al., 2016).

This suggests that the effect of tACS can result in neurophysiological effects which are phase- and frequency-matched to the stimulation artifact. Such frequency and phase matching between tACS and EEG recordings can render the removal of the artifact difficult or impossible, as the signal might no longer be separable from the artifact.

### 1.2 Non-Stationary Amplitude Modulation

An approach to tackle this issue is to assess the time-course of the EEG signal. Consider the assumption that the artifact is stationary and superpositioned on the physiological signal. Then, modulations in the amplitude of the recorded EEG-signal must be caused by changes in the underlying physiology. This would be the case, even if frequency and phase are matched to the stimulation signal. Approaches assuming such stationarity of the stimulation artifact have been used e.g. by Pogosyan et al. (2009).

Yet, detailed analysis of the stimulation artifact provides evidence that the artifact amplitude is actually not stationary. Instead, the amplitude is modulated by heart-beat and respiration (Noury et al., 2016). Consider furthermore that event-related responses like modulation of skin impedance can also affect the scalp conductance at stimulation electrodes. This would introduce event-related amplitude modulation of the

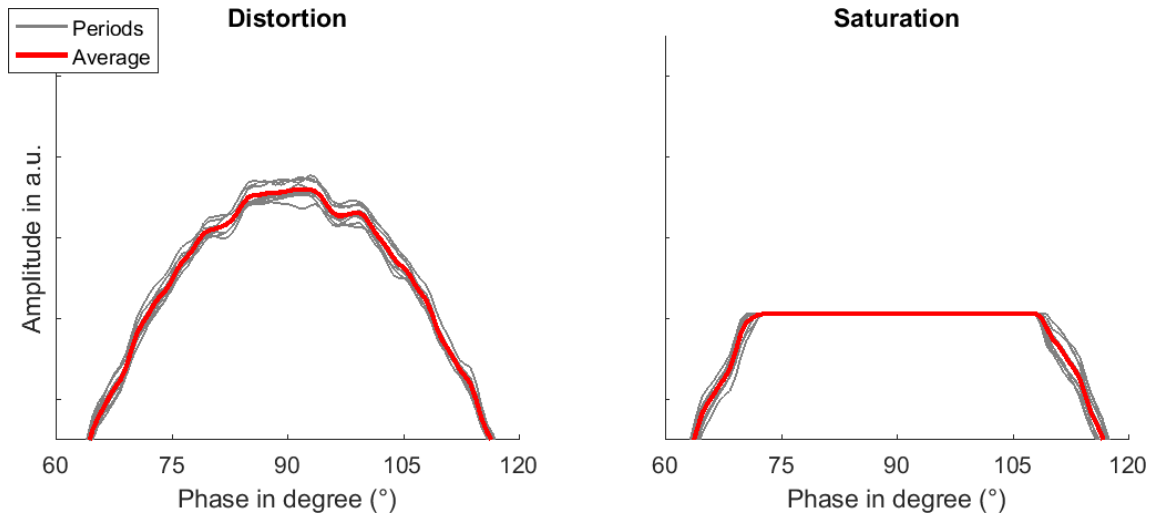


Figure 1: Non-Sinusoidality

*It shows the distortion/saturation of the sinus waveform using two exemplary trials of tACS-EEG. The gray traces indicate nine individual periods, while the red trace indicates their average. In the left figure, note the periodic, but non-sinusoidal waveform. In the right figure, note the saturation.*

stimulation artifact. In that regard, disentangling true signal from the stimulation artifact stays technically challenging.

### 1.3 Artifact Distortion

Ideally, the stimulation artifact resembles a sinusoid. Yet, practical experience suggests that the signal is usually distorted to various degrees. (see figure 1).

A major reason for distortion by amplifier saturation, i.e. the stimulation artifact exhibits an amplitude too large for the dynamic range of the amplifier, causing the signal to be cut off. Even when close to the saturation threshold, non-linearities in the amplifier slew rate can distort the shape. Additionally, the temporally and spatially uneven impedance distribution has been suggested to cause distortion, rendering the resulting waveform periodic, but non-sinusoidal.

### 1.4 Computational Demands

Methods based on adaptive template construction and temporal principal component analysis (tPCA) (Nizy et al., 2005) have been explored for removal of non-stationary and misshaped tACS artifacts (Helfrich et al., 2014). Consider that the process of template construction, the estimation of accurate weights for initial removal and the removal of residual artifacts using tPCA artifact removal is computationally cumbersome, and often requires off-line analysis supported by visual inspection. This multi-staged template-approach has therefore of limited utility for on-line artifact removal. Furthermore, a critical evaluation has suggested that the residual artifact spans several principal components, and a sufficient artifact removal is not possible with tPCA (Noury et al., 2016).

### 1.5 Rationale

We were interested in development of a computationally fast approach, feasible for online artifact removal. At the same time, the approach was required to account for the non-stationarity of the artifacts amplitude, and the possibility of non-sinusoidal distortion and saturation. Ideally, the approach should allow to estimate physiological signals at the frequency of stimulation, even if physiological oscillations were phase-locked to the stimulation signal.

## 2 Methods

## 3 Evaluation

## 4 Conclusion

## References

- Brittain, J.-S., Probert-Smith, P., Aziz, T. Z., and Brown, P. (2013). Tremor suppression by rhythmic transcranial current stimulation. *Current Biology*, 23(5):436–440, DOI: 10.1016/j.cub.2013.01.068.
- Guerra, A., Pogosyan, A., Nowak, M., Tan, H., Ferreri, F., Lazzaro, V. D., and Brown, P. (2016). Phase dependency of the human primary motor cortex and cholinergic inhibition cancelation during beta tACS. *Cerebral Cortex*, 26(10):3977–3990, DOI: 10.1093/cercor/bhw245.
- Gundlach, C., Müller, M. M., Nierhaus, T., Villringer, A., and Sehm, B. (2016). Phasic modulation of human somatosensory perception by transcranially applied oscillating currents. *Brain Stimulation*, 9(5):712–719, DOI: 10.1016/j.brs.2016.04.014.
- Helfrich, R. F., Schneider, T. R., Rach, S., Trautmann-Lengsfeld, S. A., Engel, A. K., and Herrmann, C. S. (2014). Entrainment of brain oscillations by transcranial alternating current stimulation. *Current Biology*, 24(3):333–339, DOI: 10.1016/j.cub.2013.12.041.
- Kutchko, K. M. and Fröhlich, F. (2013). Emergence of metastable state dynamics in interconnected cortical networks with propagation delays. *PLoS Computational Biology*, 9(10):e1003304, DOI: 10.1371/journal.pcbi.1003304.
- Nakazono, H., Ogata, K., Kuroda, T., and Tobimatsu, S. (2016). Phase and frequency-dependent effects of transcranial alternating current stimulation on motor cortical excitability. *PLOS ONE*, 11(9):e0162521, DOI: 10.1371/journal.pone.0162521.
- Niazy, R., Beckmann, C., Iannetti, G., Brady, J., and Smith, S. (2005). Removal of FMRI environment artifacts from EEG data using optimal basis sets. *NeuroImage*, 28(3):720–737, DOI: 10.1016/j.neuroimage.2005.06.067.
- Noury, N., Hipp, J. F., and Siegel, M. (2016). Physiological processes non-linearly affect electrophysiological recordings during transcranial electric stimulation. *NeuroImage*, 140:99–109, DOI: 10.1016/j.neuroimage.2016.03.065.
- Pogosyan, A., Gaynor, L. D., Eusebio, A., and Brown, P. (2009). Boosting cortical activity at beta-band frequencies slows movement in humans. *Current Biology*, 19(19):1637–1641, DOI: 10.1016/j.cub.2009.07.074.
- Raco, V., Bauer, R., Tharsan, S., and Gharabaghi, A. (2016). Combining TMS and tACS for closed-loop phase-dependent modulation of corticospinal excitability: A feasibility study. *Frontiers in Cellular Neuroscience*, 10, DOI: 10.3389/fncel.2016.00143.
- Reato, D., Rahman, A., Bikson, M., and Parra, L. C. (2013). Effects of weak transcranial alternating current stimulation on brain activity—a review of known mechanisms from animal studies. *Frontiers in Human Neuroscience*, 7, DOI: 10.3389/fnhum.2013.00687.
- Schmidt, S. L., Iyengar, A. K., Foulser, A. A., Boyle, M. R., and Fröhlich, F. (2014). Endogenous cortical oscillations constrain neuromodulation by weak electric fields. *Brain Stimulation*, 7(6):878–889, DOI: 10.1016/j.brs.2014.07.033.
- Zaehle, T., Rach, S., and Herrmann, C. S. (2010). Transcranial alternating current stimulation enhances individual alpha activity in human EEG. *PLoS ONE*, 5(11):e13766, DOI: 10.1371/journal.pone.0013766.