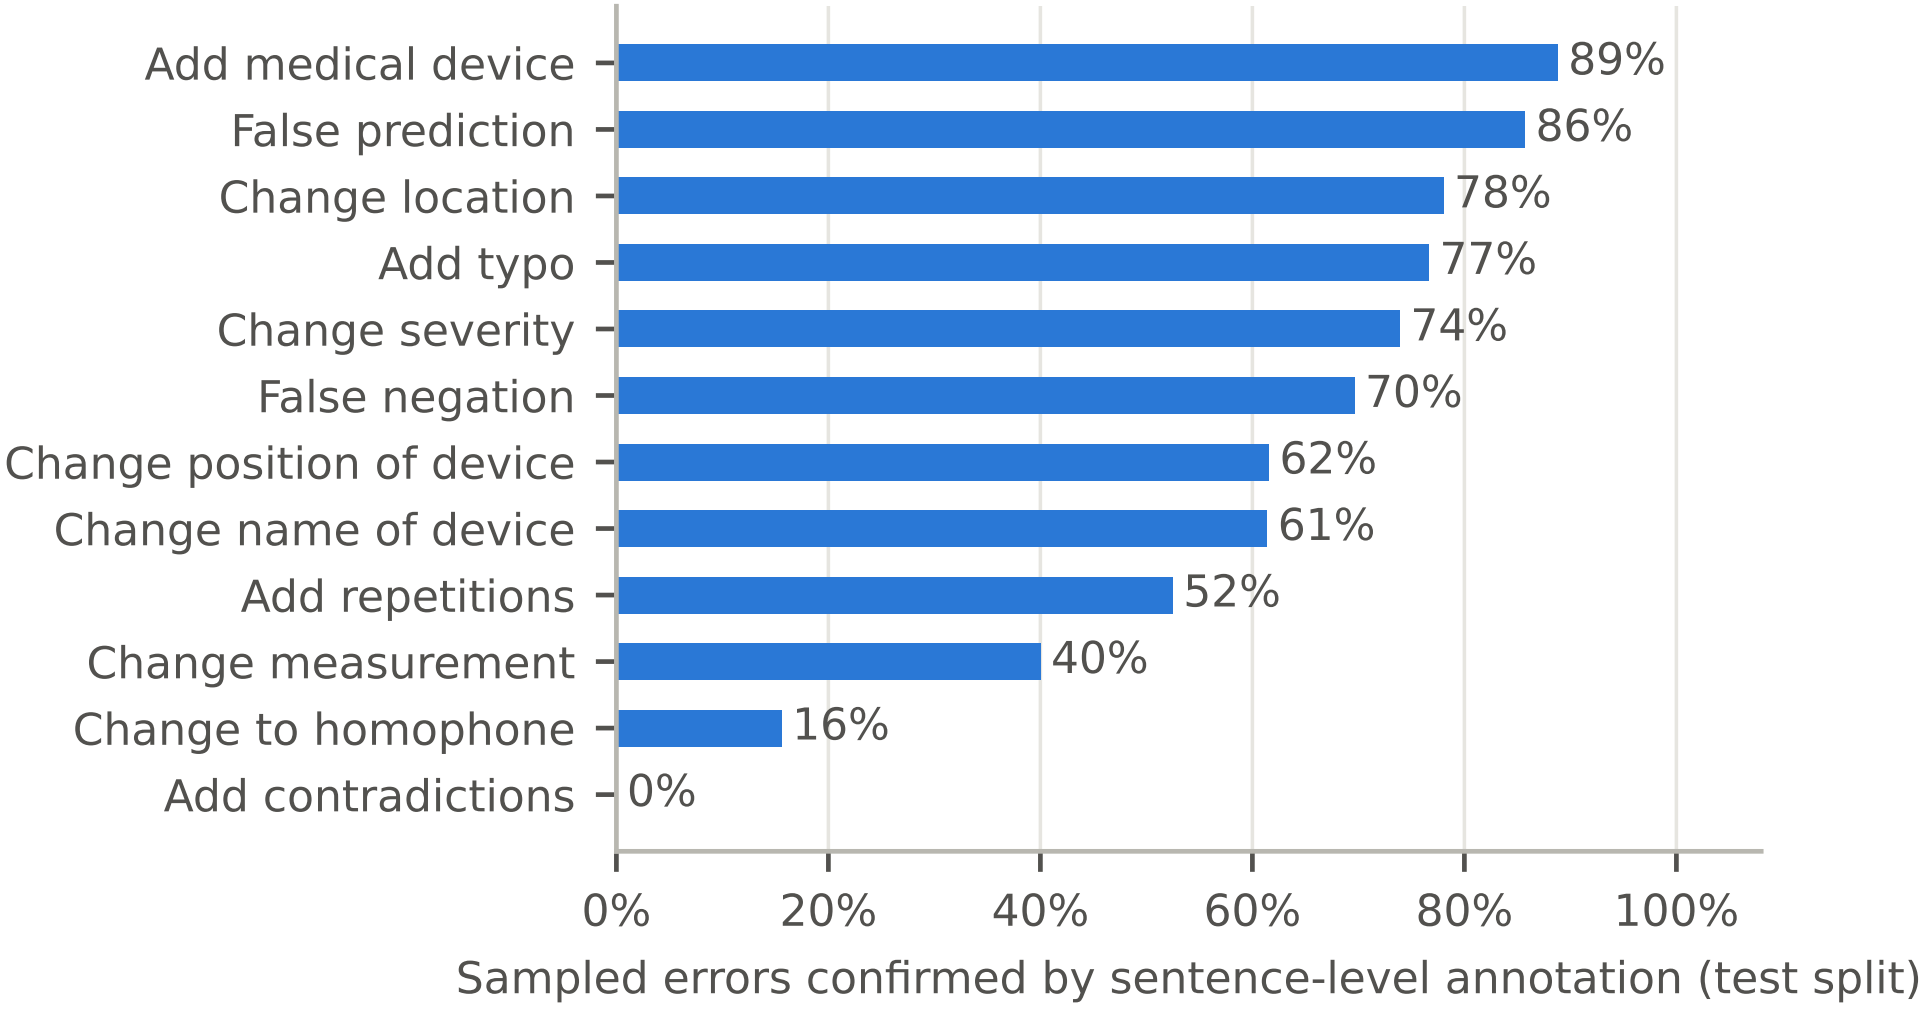
Add medical device
False prediction
Change location
Add typo
Change severity
False negation
Change position of device
Change name of device
Add repetitions
Change measurement
Change to homophone
Add contradictions
89%
86%
78%
77%
74%
70%
62%
61%
52%
40%
16%
0%
0%
20%
40%
60%
80%
100%
Sampled errors confirmed by sentence-level annotation (test split)