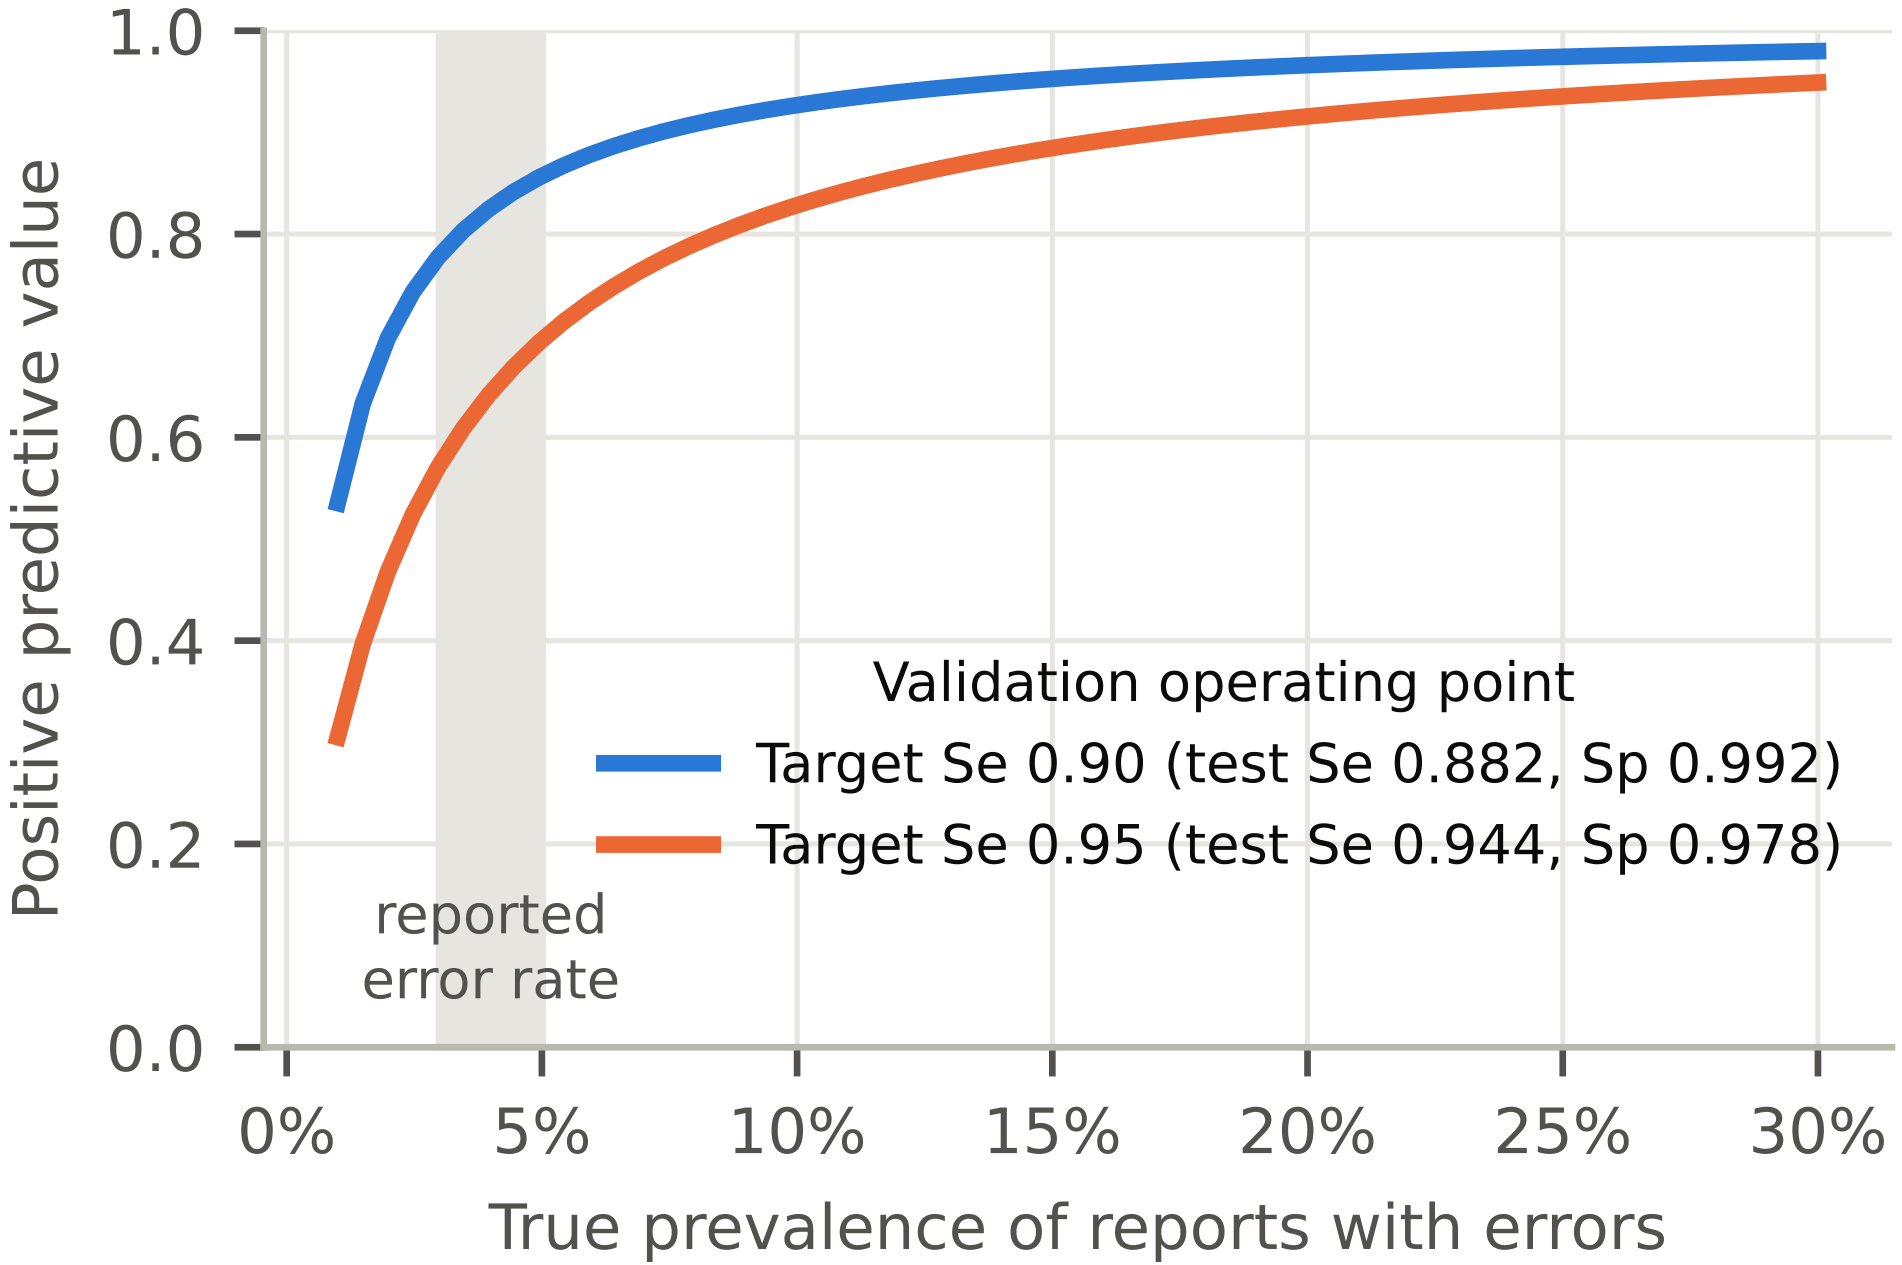
1.0
0.8
0.6
0.4
0.2
0.0
Positive predictive value
reported
error rate
Validation operating point
Target Se 0.90 (test Se 0.882, Sp 0.992)
Target Se 0.95 (test Se 0.944, Sp 0.978)
0%
5%
10%
15%
20%
25%
30%
True prevalence of reports with errors