




Calibration Certificate NO: SL61850

Model: Slimline
Serial Number: 6005
Max Pressure Rating: 10000 psi
Temperature Rating: 177 °C
Calibration Date: Jul 13, 2026

Measurements and Derived Results

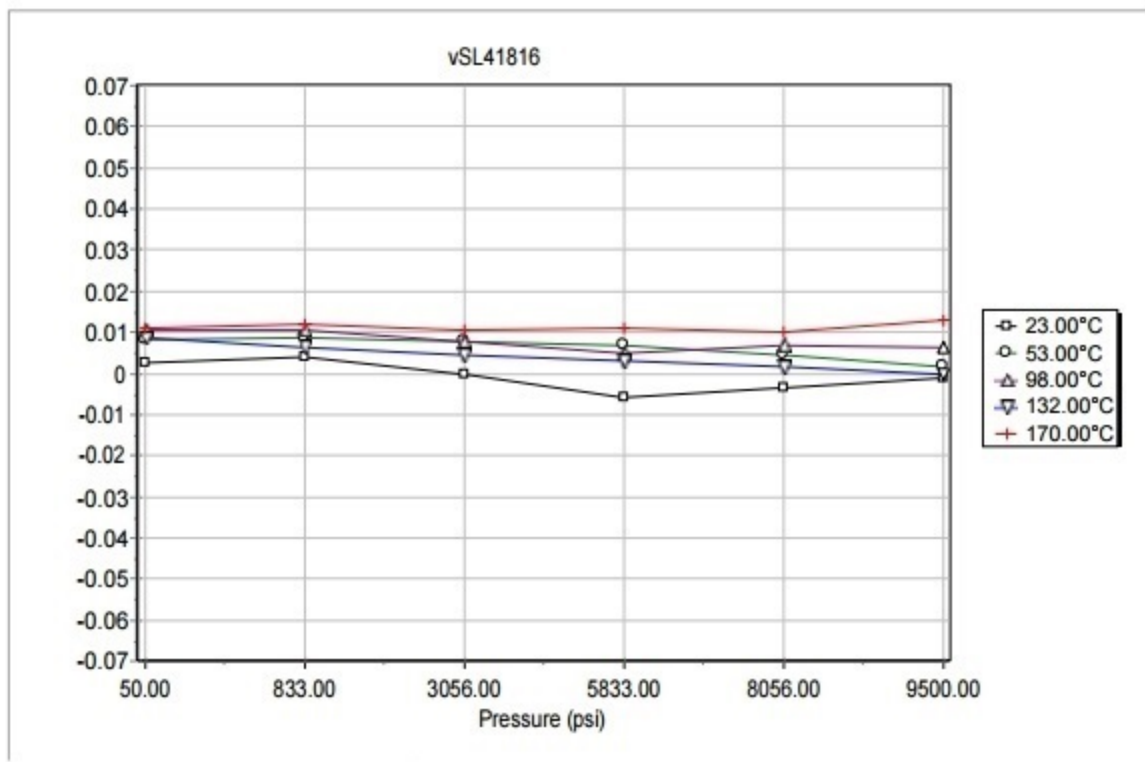

Specifications

Pressure Range:	Minimum:	50 psi	Maximum:	10000 psi
Temperature Range:	Minimum:	10 °C	Maximum:	177 °C
Pressure:	Accuracy:	± 0.05% FS		± 5.000 psi
Temperature	Accuracy:			± 1.0 °C

Summary

Pressure Accuracy (Maximum Error): + 1.95 psi 0.016% FS

Temperature Accuracy (Maximum Error): - 0.59 °C

Calibrations are verified to 95% of maximum full scale pressure.

Working Standards

- DHI Oil Operated Piston Gauge – Model PG 7302-5, SN301 – M Range 100kPa to 500MPa $\pm 0.005\%$ FS.
- DHI 40kg Mass Set MS-AMH-40, SN2266
- Hart Scientific Black Stack – Model 2560 - SN 91362.
- Hart Scientific Platinum Resistance Thermometer – Model 5614 – SN 496051 with an accuracy of $\pm 0.006\text{ }^{\circ}\text{C}$ ($\pm 0.011\text{ }^{\circ}\text{F}$).

Traceability Statement

All working standards are traceable to nationally or internationally recognized standards.

- DHI Model DHI PC-7302-5, SN301 traceability of mass is maintained through reference mass set R100 through determination by National Institute of Standards and Technology, NIST, United States.
- The traceability of mass is maintained to the fundamental unit of the kilogram [kg] through reference mass set R100 through determinations performed by National Institute of Standards and Technology, NIST, United States.
- The measured true mass values of the PG7302-5 components is as follows:
 - The Piston mass is equal to 200.0011g with an uncertainty of $\pm 3\text{ mg}$ and has an average density of 7230 kg/m³.
 - The Mass Carrying Bell is equal to 800.0044 g with an uncertainty of $\pm 8\text{ mg}$ and has an average density of 6100 kg/m³.
 - The Mass Set is made up of 10 masses of 10.1 kg or less adjusted to $\pm 20\text{ ppm}$ of their nominal true mass values and has an average density of 8000 kg/m³. The uncertainty of the masses in mg is guaranteed to be less than 5 ppm or 1 mg, whichever is greater.
- The traceability of effective area is maintained through the 2004 DHI Piston-Cylinder calibration Chain to the National Institute of Standards and Technology, NIST, United States, and the Laboratoire national d'Essais, LNE, France.
- All DH calibrations are performed in accordance with DHI laboratory Quality assurance manual, Rev C September 2003 and conform to ISO/IEC 17025, ANSI/NCSL Z540-1-1994, ISO/IEC Guide 25, ISO 9002, ISO-10012-1, MIL-STD 45662A.
- The Platinum Resistance Thermometer (PRT) Model 5614, SN496051 was calibrated at the ice point and/or by comparison to Standard Platinum Resistance Thermometers (SPRTs). These SPRTs are calibrated to the International Temperature Scale of 1990 (ITS-90) and their calibration is traceable to the National Institute of Standards and Technology (NIST).
- Omega Well Monitoring local gravity has been determined through the National Geodetic Survey of Canada.



Calibration Performed and Approved By

Omega Well Monitoring recommended recalibration interval is 1 year.
This certificate shall not be reproduced without the written approval of the laboratory.