




Beam profile at 3 cm from the collimator holder (40 kV and 30mA)

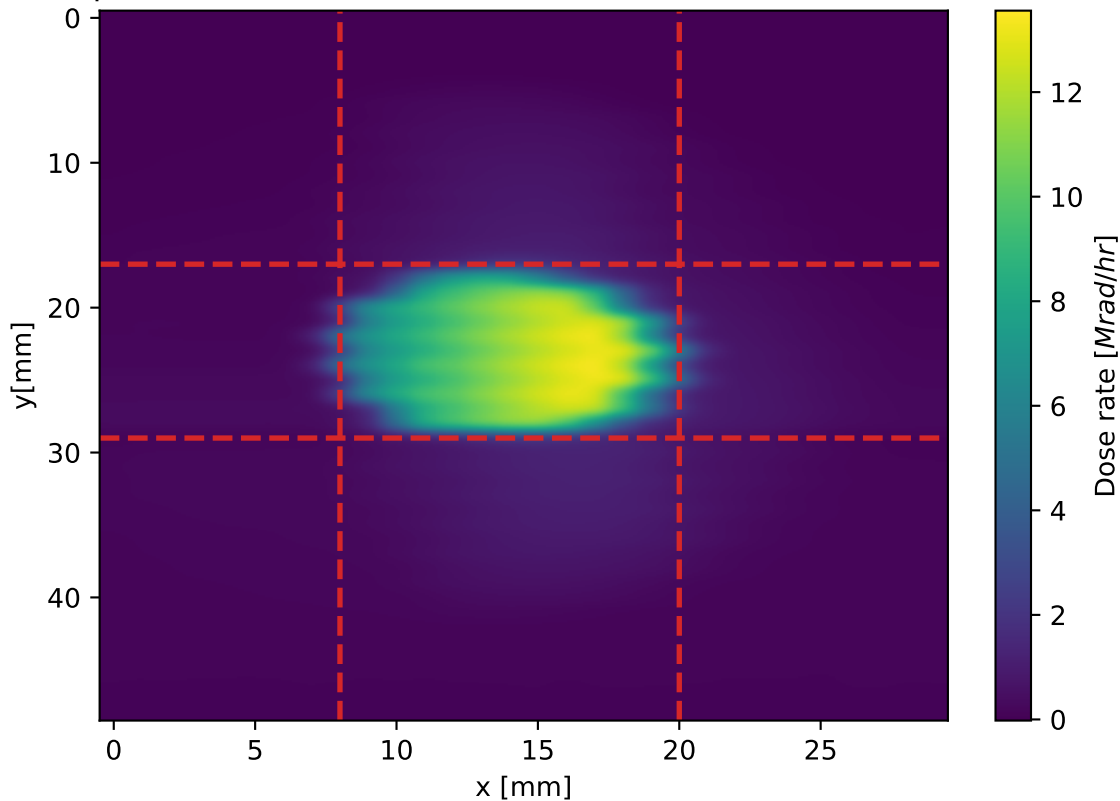


Beam profile at 3 cm without collimator support

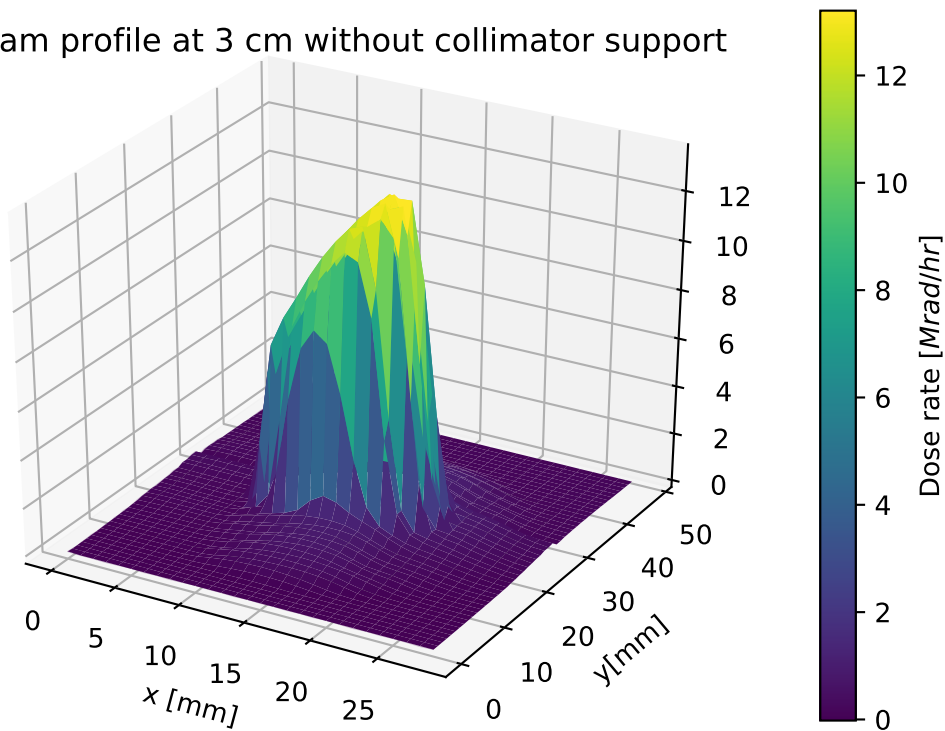


Calibration curve for 3cm

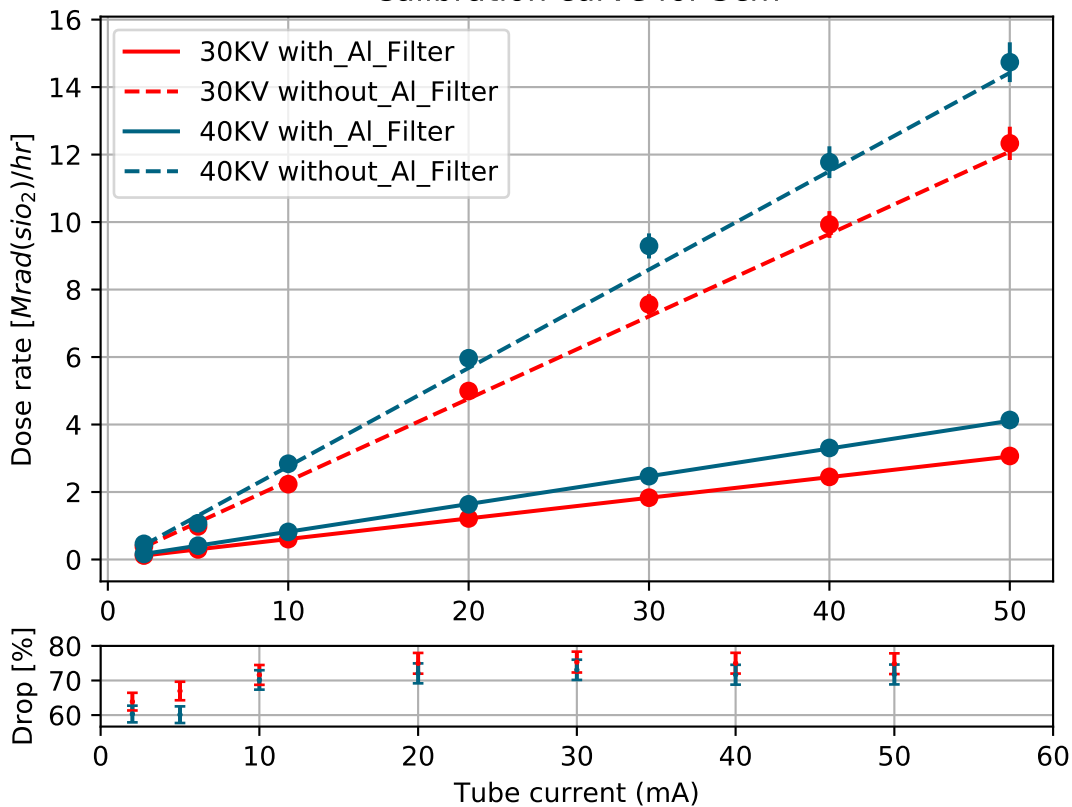


Calibration curve for 5cm

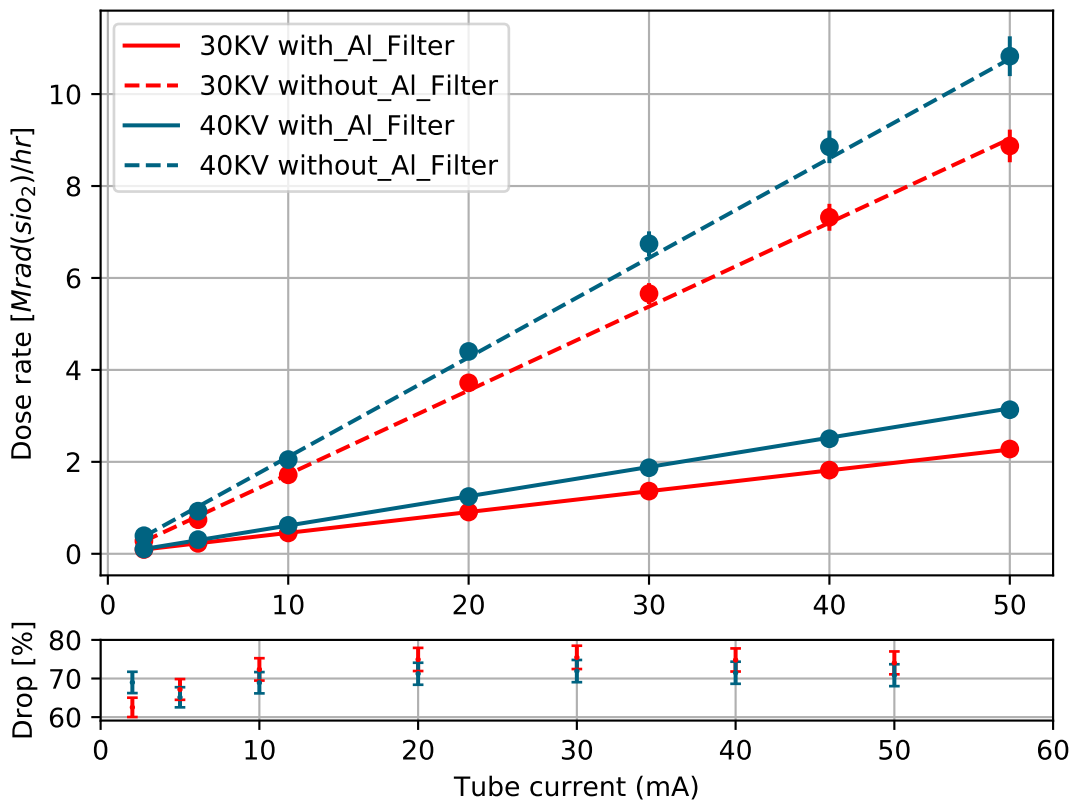


Calibration curve for 8cm

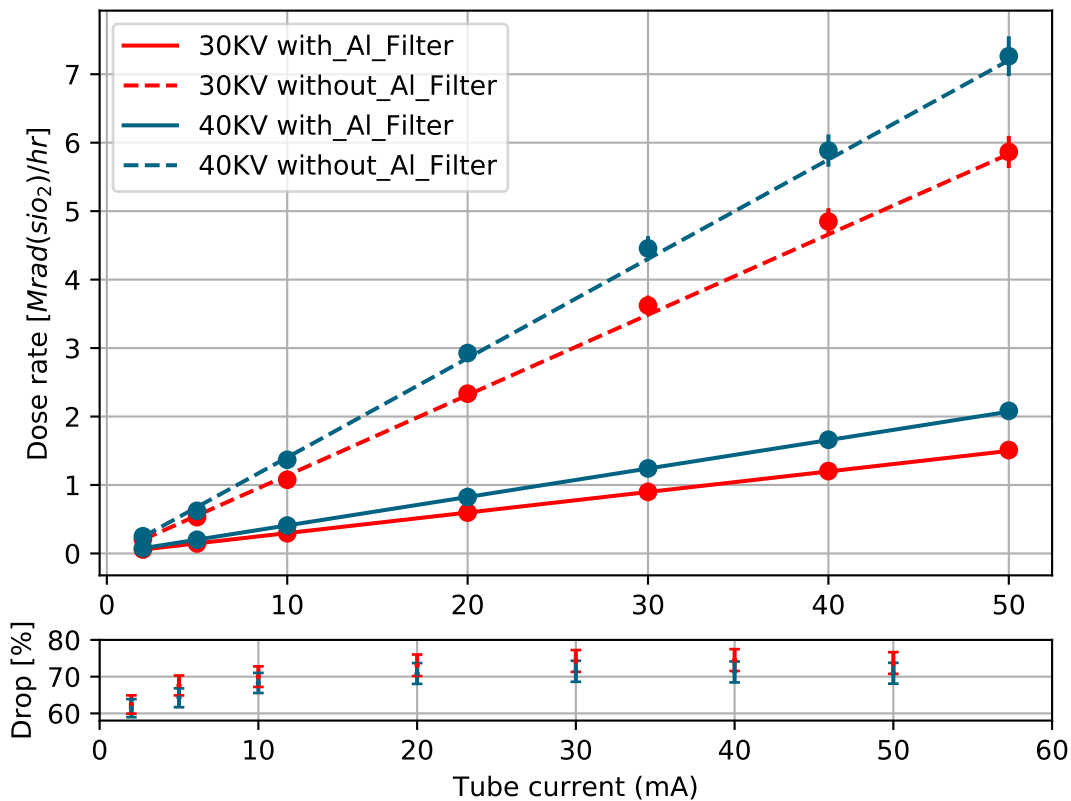


Radius covered by beam spot without_Al_Filter

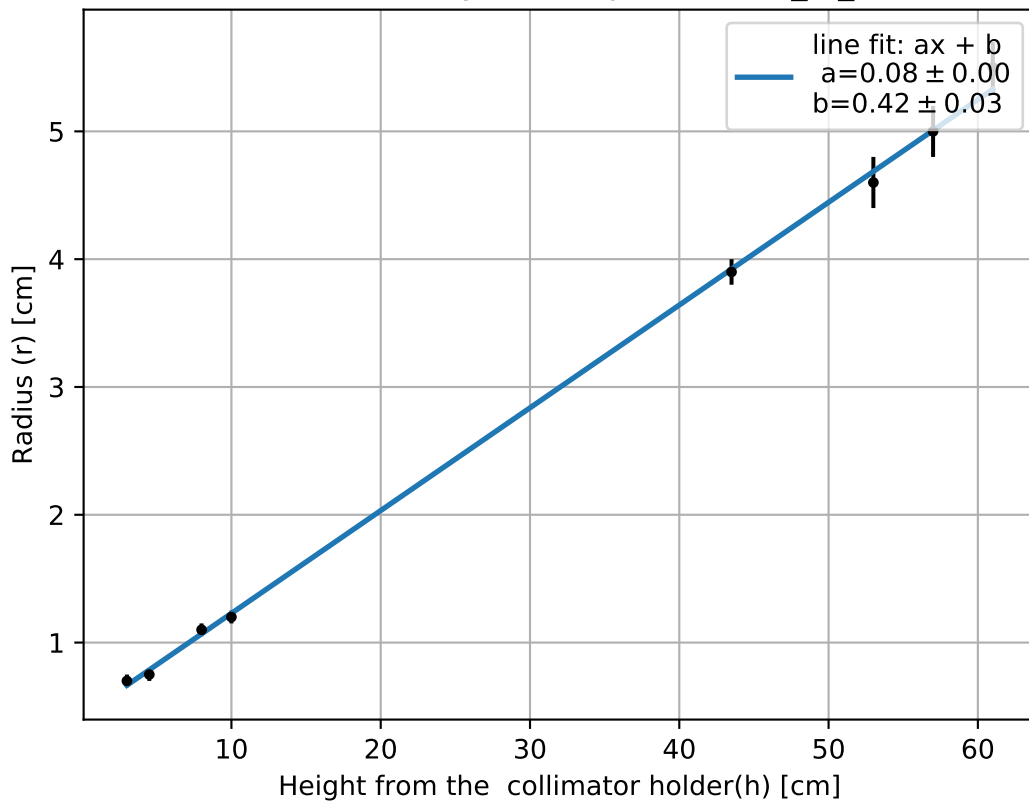


Diameter covered by beam spot without_AI_Filter

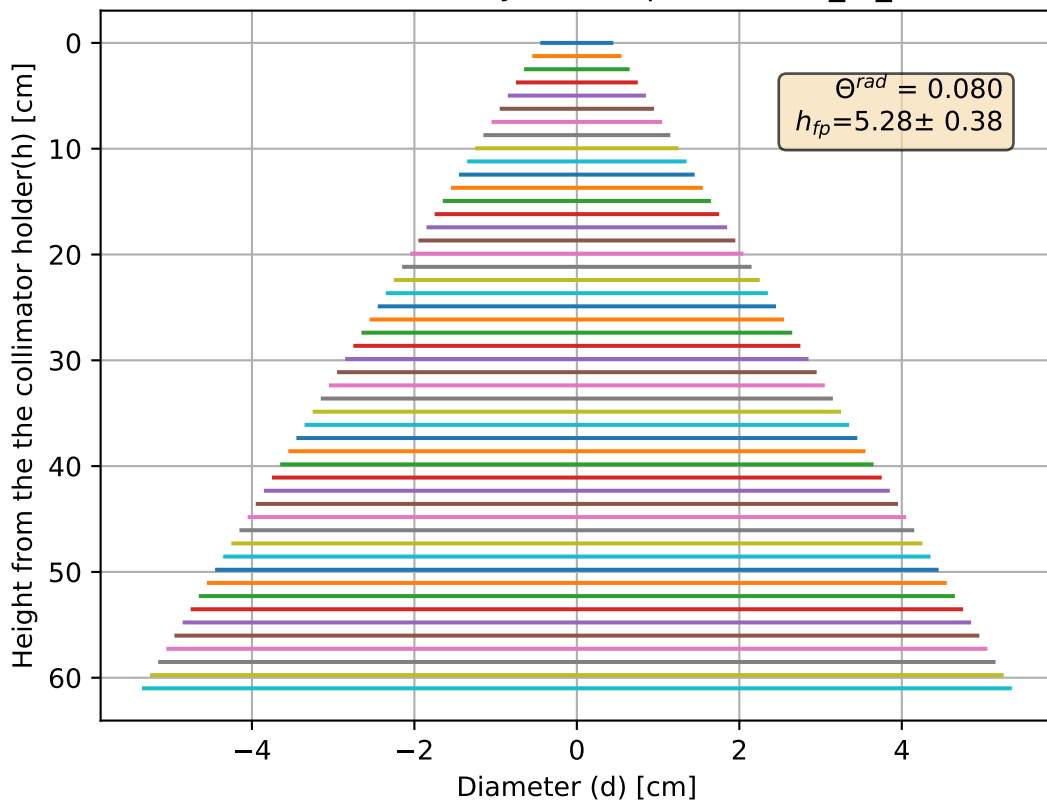


Radius covered by beam spot with _Al_Filter

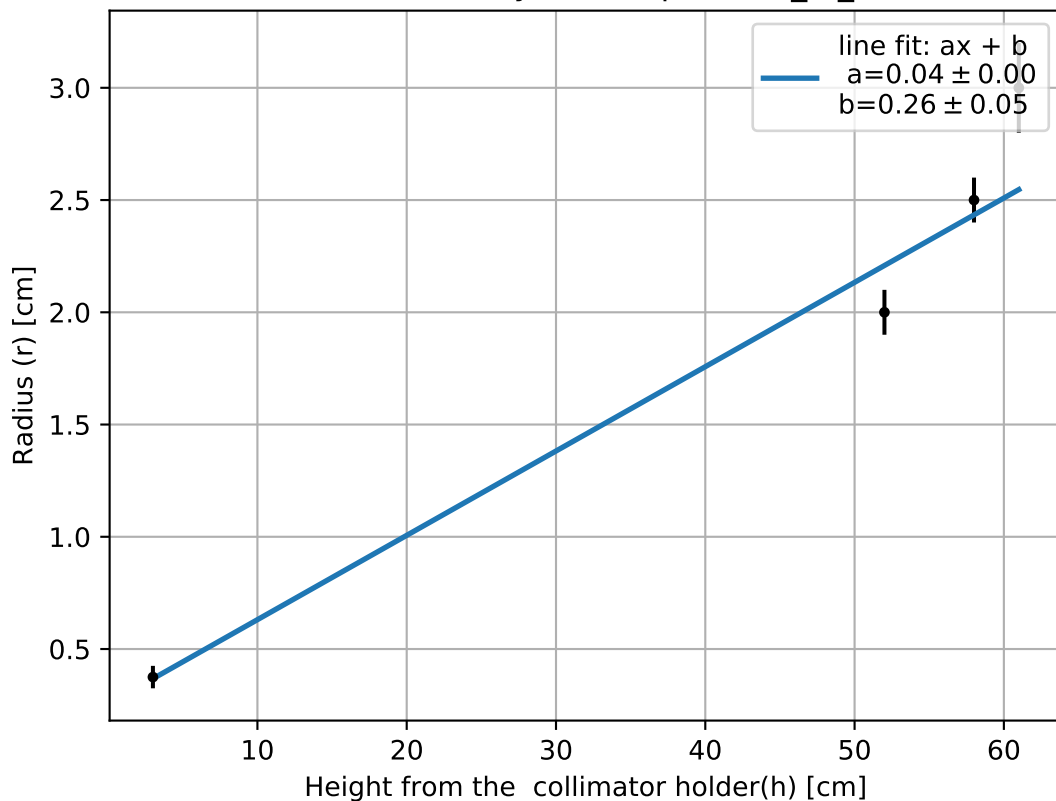


Diameter covered by beam spot with_Al_Filter

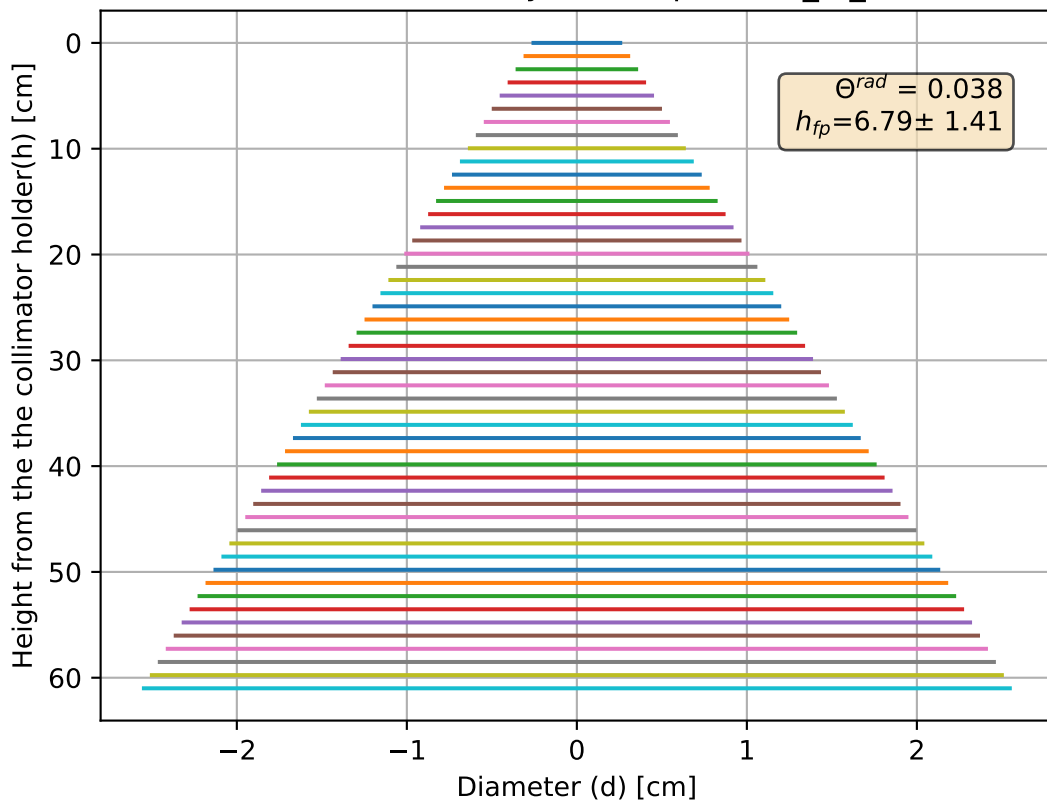


Dose rate vs distance at (40 kV and 50 mA)

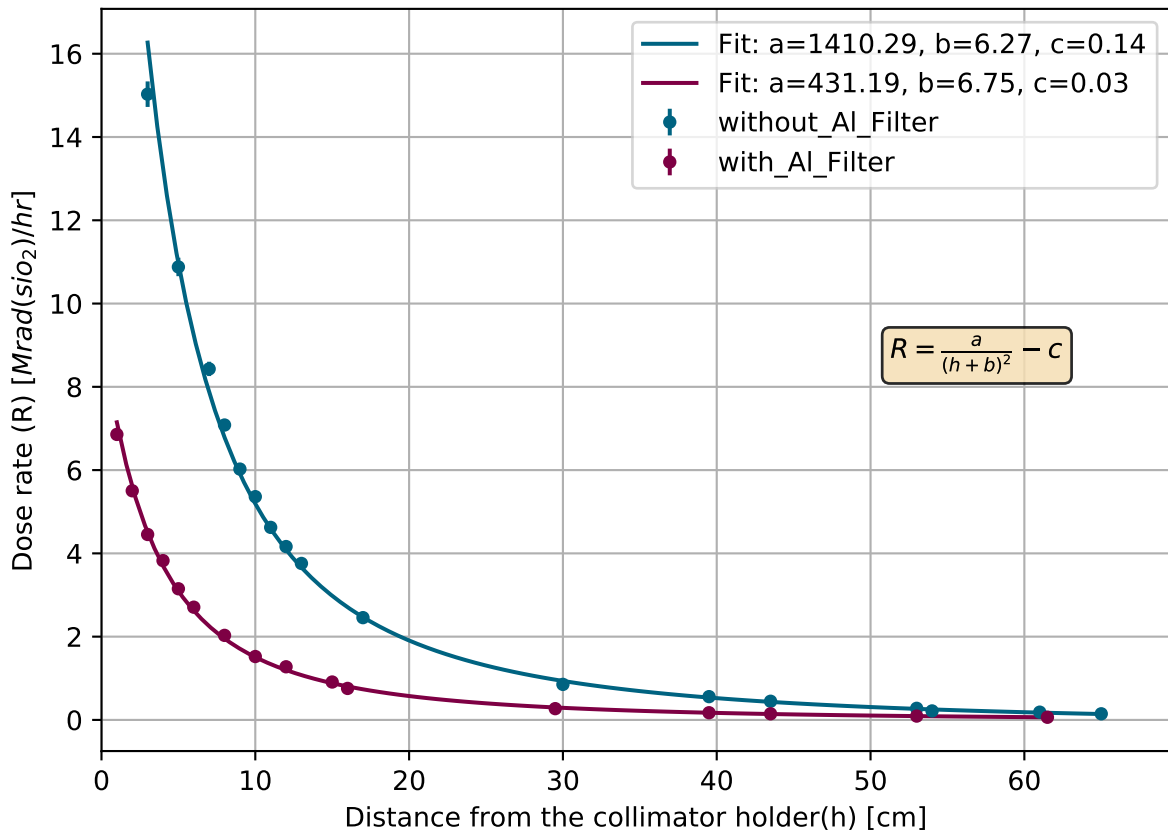

(40 kV and 50 mA)

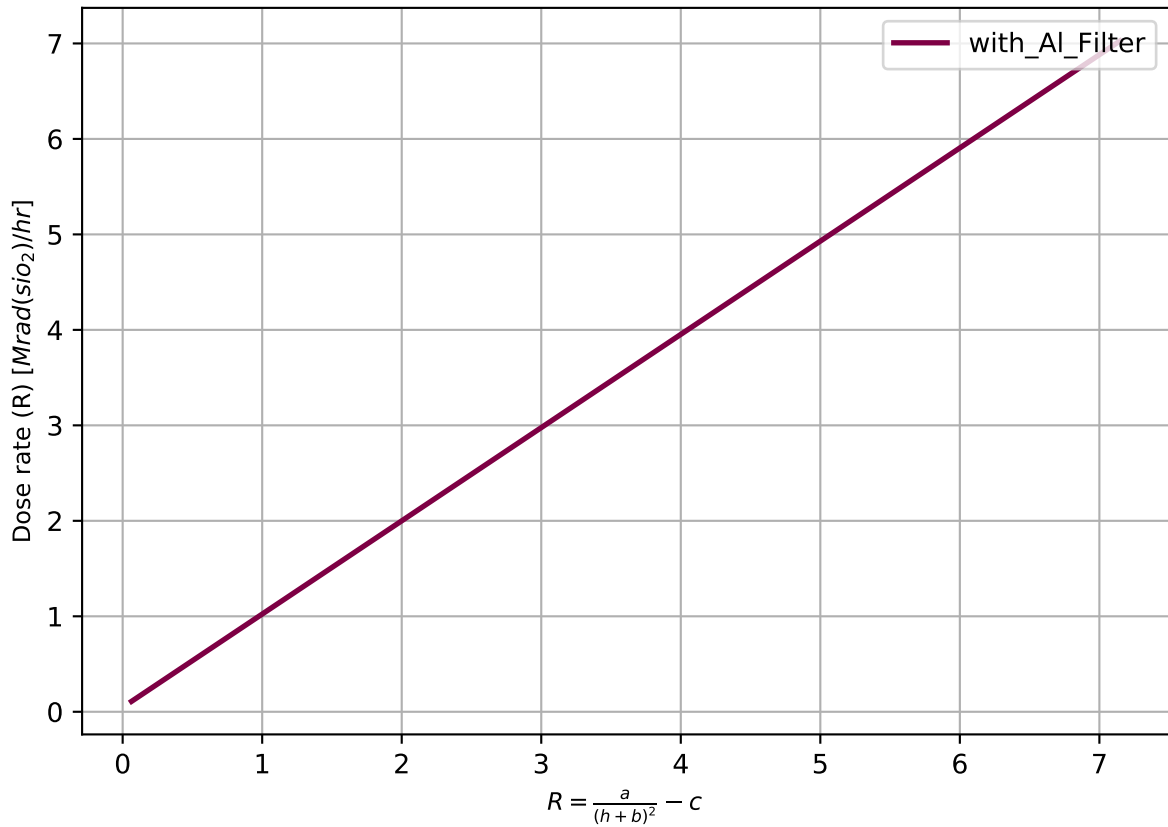

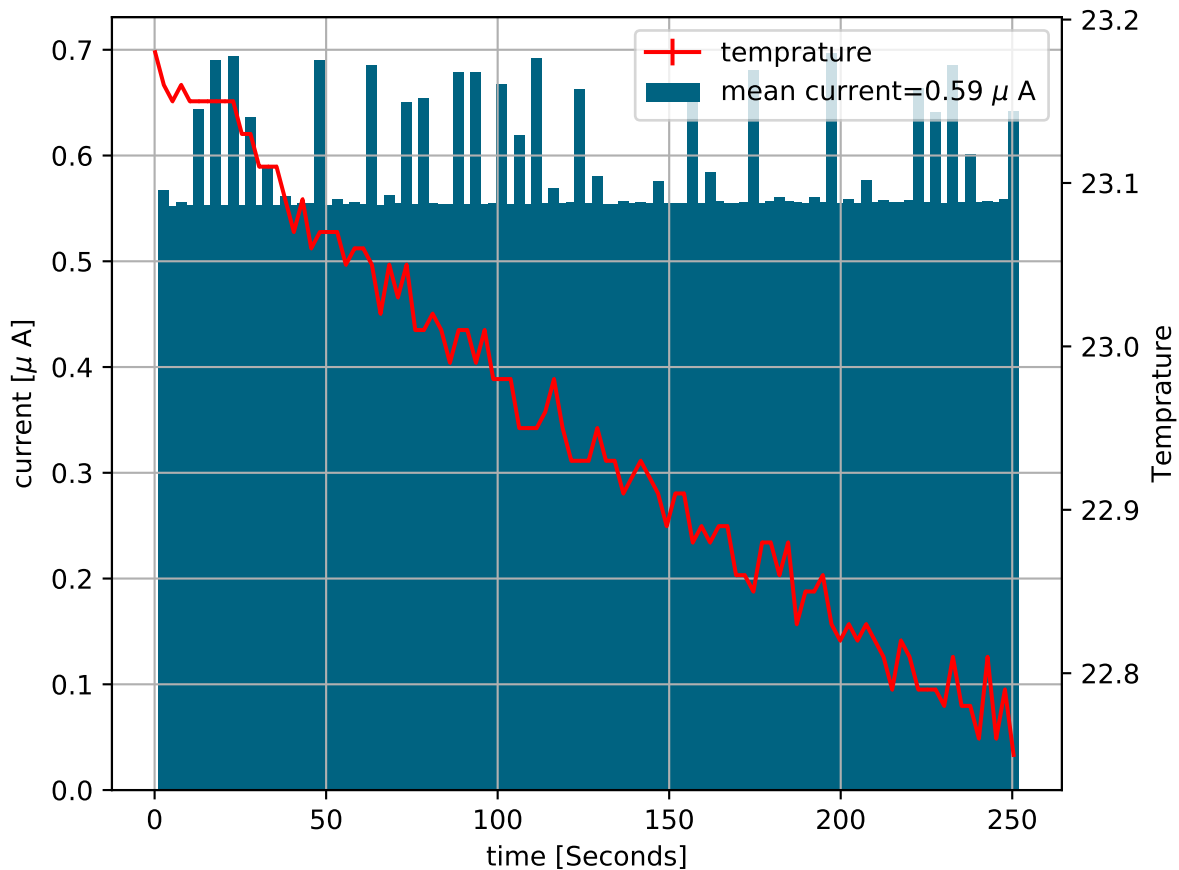

Effect of tube Voltage at 8cm without_Al_Filter

