CERTIFICATE OF ANALYSIS - POTASSIUM SORBATE

Serial No.:	UV04232A1	Material Name:	Potassium Sorbate
Batch Number:	PS20250320	Standard:	USP–NF 2024
Company Name:	Sina Pharm	Analysis Date:	07/10/2025
Analyst:	Reda Ibrahim	Lab:	PureSip Laboratory

TEST RESULTS SUMMARY

Test	Acceptance Criteria (USP-NF 2024)	Result	Status
Assay (Content of Potassium Sorbate)	98.0% - 101.0% on dried basis	98.9%	PASS
Standard %RSD (n=3)	NMT 2.0%	0.42%	PASS
Sample %RSD (n=3)	NMT 2.0%	0.21%	PASS
Limit of Aldehyde (as Formaldehyde)	NMT 0.002%	Conforms	PASS
Loss on Drying	NMT 1.0%	0.3%	PASS
Appearance	White crystalline powder	Conforms	PASS

UV-VIS CALIBRATION CURVE

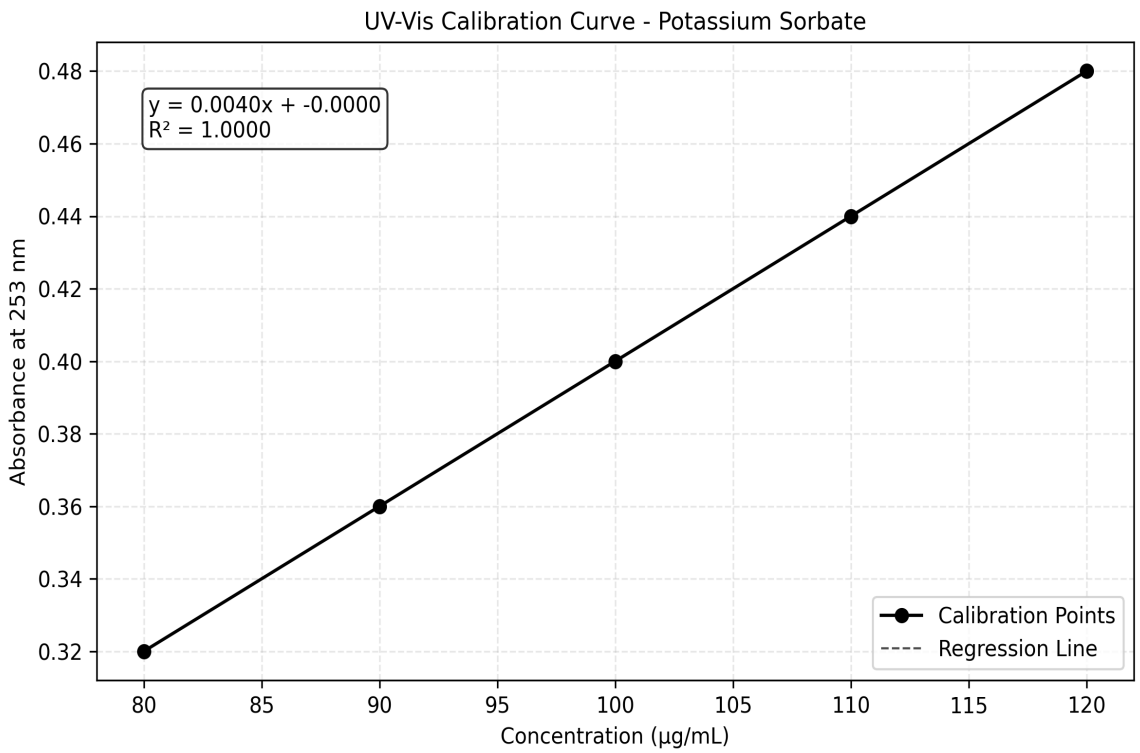

UV SPECTRA - REPLICATE READINGS

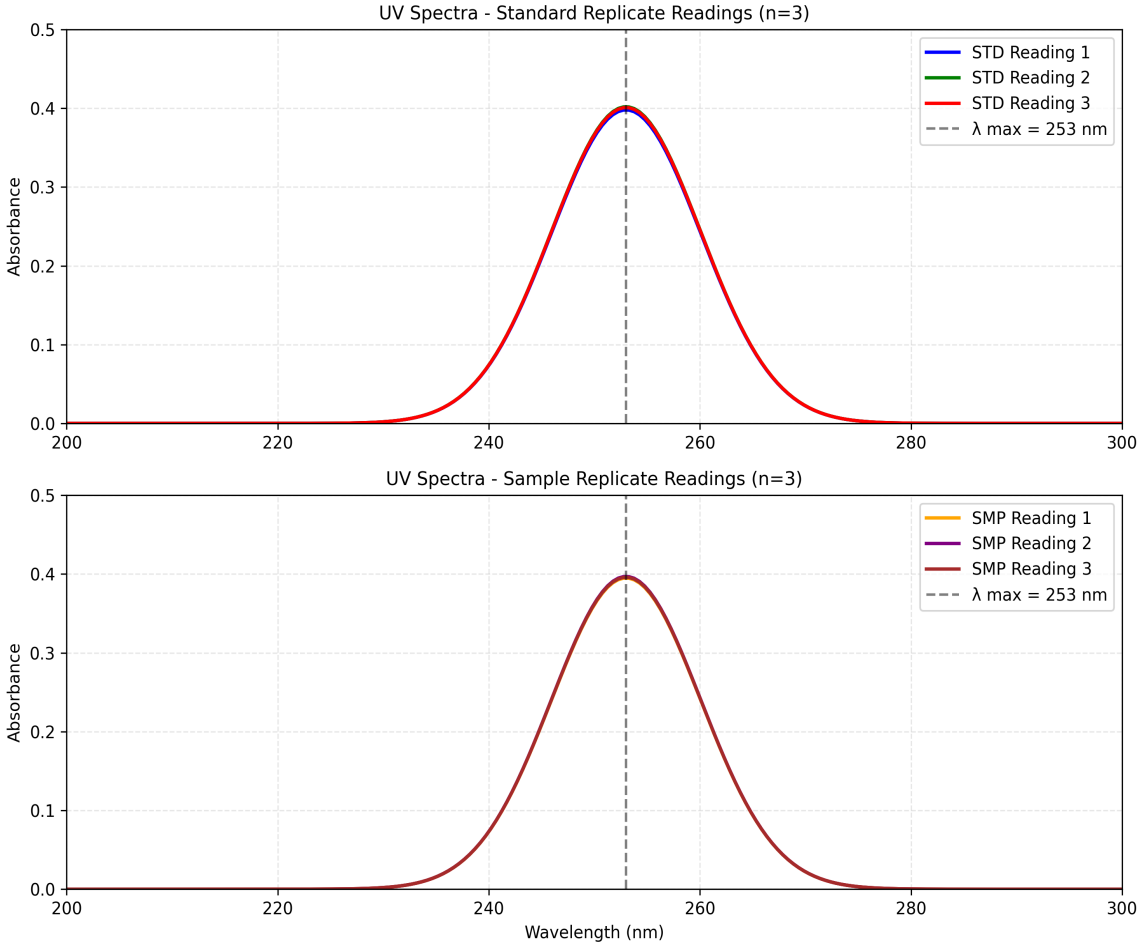

REPLICATE READINGS DATA

Reading	Type	Absorbance at 253 nm	Weight (mg)	Concentration (%)
#1	Standard	0.398	100.0	100.0
#2	Standard	0.402	100.0	100.0
#3	Standard	0.401	100.0	100.0
#1	Sample	0.395	100.2	98.7
#2	Sample	0.397	100.1	99.2
#3	Sample	0.396	100.3	98.9

REPLICATE READINGS CHART

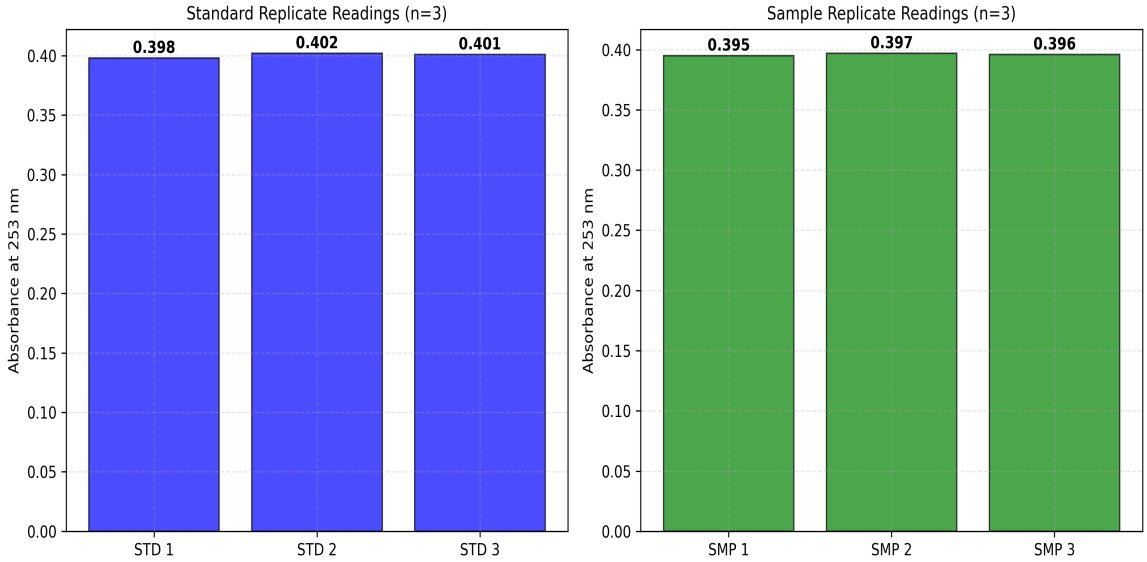

LIMIT OF ALDEHYDE TEST - VISUAL COMPARISON

CONCLUSION

The sample of Potassium Sorbate (Batch No: PS20250320) complies with USP-NF 2024 specifications. The assay result of 98.9% for Potassium Sorbate content is within the required range of 98.0% to 101.0%. The method demonstrated excellent precision with %RSD values of 0.42% for standard and 0.21% for sample readings. The Limit of Aldehyde test shows that the sample conforms to the specification (NMT 0.002% as formaldehyde).

Tested by:

Reda Ibrahim

Laboratory Analyst

Date: 07/10/2025

Quality Control PureSip SINCE 2018