Assay-system agreement is an empirical question

System-pair correlations above · selected CYP molecule extremes below

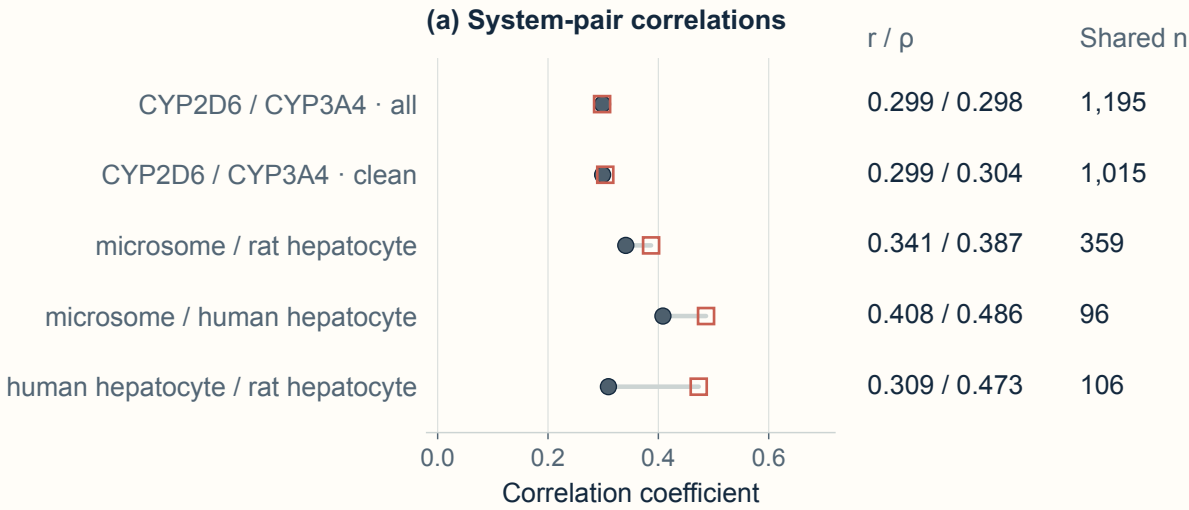

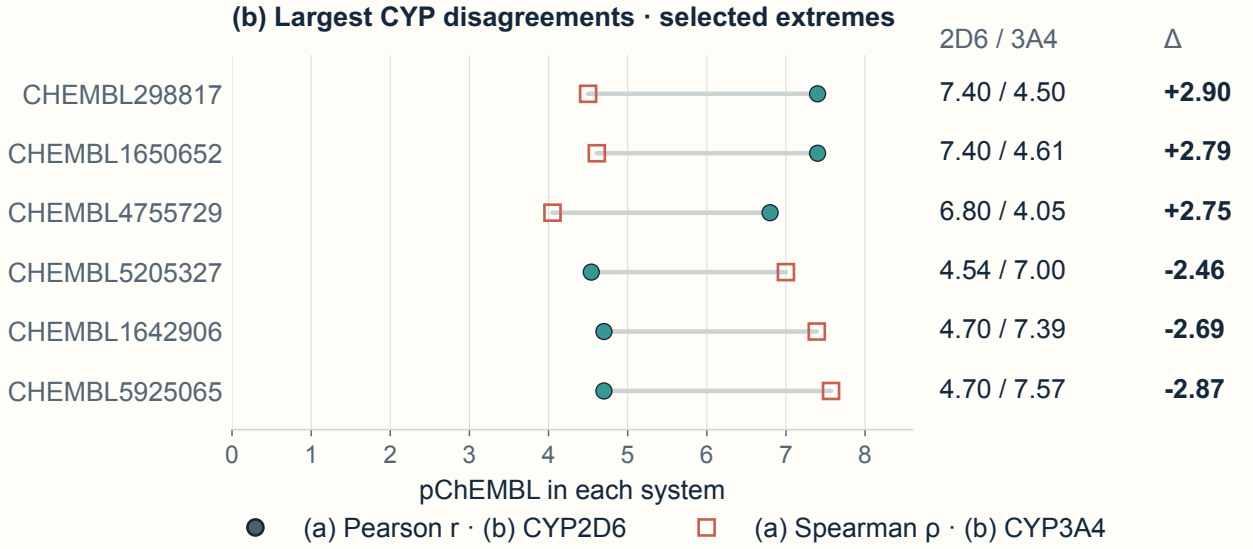

Species and matrix differ across clearance pairs. Selected extremes do not represent the distribution; neither assay system is declared wrong.