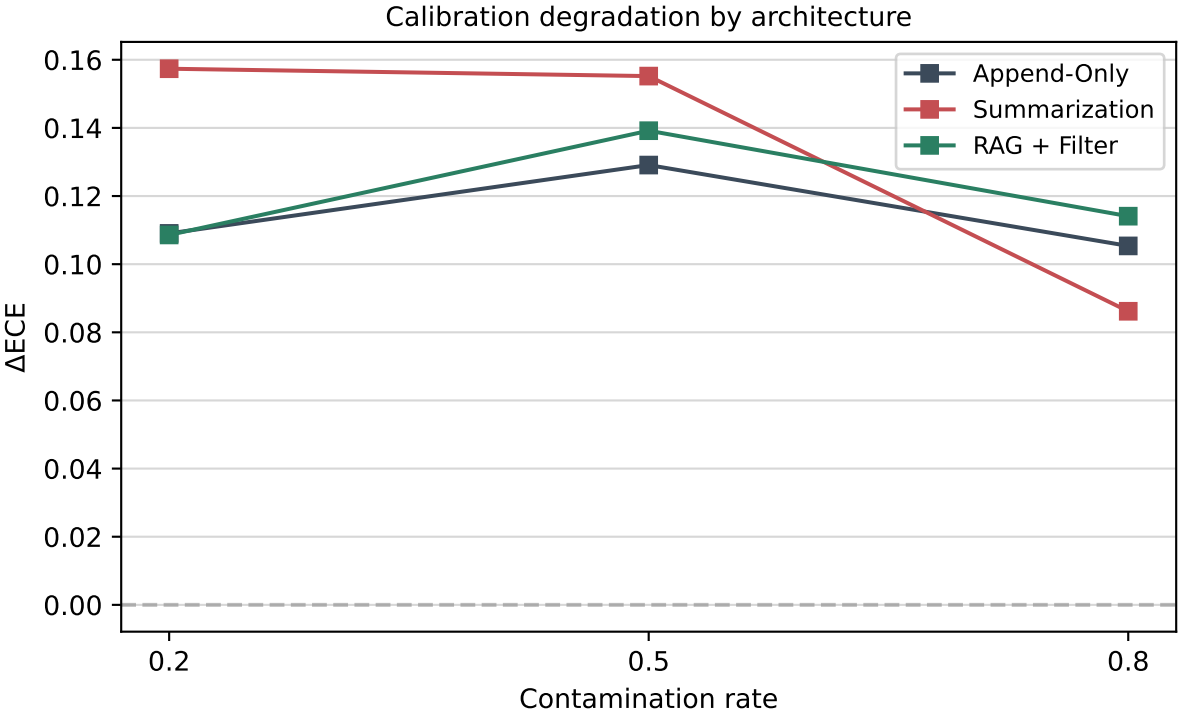
Calibration degradation by architecture
Append-Only
Summarization
RAG + Filter
ΔECE
0.16
0.14
0.12
0.10
0.08
0.06
0.04
0.02
0.00
0.2
0.5
0.8
Contamination rate