**NA Caltechnologies Co., Ltd.**

75/107 Moo 11, Klongnueng Klongluang Pathumthani 12120 Thailand
Tel: +66-2-529-2460-5
Fax: 66-2529-2466, 66-529-2133
Email: sales-cal@nacal.co.th URL: https://www.nacal.co.th

ACCREDITED ISO/IEC 17025 CALIBRATION LABORATORY AC-2658

NSC-TISI-TIS 17025 Calibration 0289

# Quotation

To : Kunlada Panman PMA DIV. Ext. 1610
NMB-MINEBEA THAI LIMITED
1 Moo 7, Phaholyothin Rd., KM.51, T. Chiangraknoi, A. Bangpa-In, Ayutthaya 13180 Thailand

Tel : 0-3536-1429-38 Ext. 1610
Fax :
Email : kunlada.p@minebea.co.th

Date : January 15, 2025
Quotation No : NA-CAL-25-01-0740
Quotation Type : CALIBRATION
Sub Type : LAB

**Your reference**
Suchaya Tiwamongkol
Mobile : 061-249-4491
Email : suchayat@nacal.co.th

| No. | DESCRIPTION | ISO/IEC 17025 | | QTY | UNIT PRICE (THB) | DISC. | AMOUNT (THB) |
|---|---|---|---|---|---|---|---|
| | | Lab | Site | | | | |
| 1 | Digimatic Caliper / 500-501-10 / Mitutoyo / 0033855<br>**Calibration Conditions :**<br>- Decision rule for statements of conformity in the calibration certificate will be referred to the attachment sheets with this quotation.<br>- Normal turn around time is 7-14 working days.<br>Note : Please do not deduct withholding Tax (ได้รับ BOI เลขที่ 66-0346-1-04-1-0) | ANAB | ANAB | 1 | 1,100.00 | 20% | 880.00 |
| | | | | | **TOTAL** | | 880.00 |
| | | | | | **VAT** 7 % | | 61.60 |
| | | | | | **GRAND TOTAL** | | 941.60 |

**Remarks :**

1. Price Validity 30 days
2. Term of Payment. 90 days after delivery.
3. Please acknowledge the conditions on the next page and sign.

**We hope that our quotation will be taken under your favorable consideration.**

Customer, I accept all above mentioned:
(Please sign, stamp and fax to 0-2529-2133)

**Authorized signature**

.....
( )
Date :

**Authorized signature, NA Caltechnology Co., Ltd.**

.....
( Mr. Yanyong Pithong )
Laboratory Manager
Date : January 15, 2025

**Conditions:**

1. The equipment submitted for calibration should be carefully packed.
2. The equipment submitted for calibration must be in good working order.
3. The laboratory reserves the right to compensate for damages. In cases where it can be proved that it was caused by the instrument or accessories has a long service life and is old/ damaged/ in a condition not available for use/ is an outdated tool/ the application has expired, the application must be updated (Calibrator model 5500A, 5502A, 5520A, 5522A, 5700A, 5720A, 5725A, 5502E, 5100B, 5025E, 3010, 3041, C-101 and 9100, Digital Multimeter model 3458A, 8508 and 4950).
4. The laboratory reserves the right to compensate for damages in the event the instrument was found to be defective during calibration. The instrument will be returned and all or part of the fee collected. This depends on the actual expenses incurred.
5. Laboratory will not be responsible for any damages. that may occur while the instrument or accessories are in the care of the laboratory. Unless it can be proven that the instrument or accessories used for calibration were damaged or lost as a result of the laboratory's actions.
6. In case of damage or defect of instrument caused by calibration of the laboratory. We reserve the right to indemnify our customers. Maximum not more than the calibration value.
7. The laboratory is not liable for any damage or defect of instrument during transportation, except for transportation by company staff.
8. The above service fee may change if the calibration items sent for calibration to the laboratory or on-site work are changed.

**เงื่อนไข**

1. เครื่องมือที่นำมาสอบเทียบ ควรมีการบรรจุอย่างระมัดระวัง
2. เครื่องมือที่นำมาสอบเทียบต้องอยู่ในสภาพสมบูรณ์
3. ห้องปฏิบัติการฯ จะไม่รับผิดชอบใดๆ กรณีพิสูจน์ได้ว่าเกิดจากเครื่องมือหรืออุปกรณ์ มีอายุการใช้งานยาวนาน และมีสภาพ เก่า/ชำรุด/อยู่ในสภาพไม่พร้อมใช้งาน/ เป็นเครื่องมือล้าสมัย/ Application หมดอายุต้องมีการ Update Application (เครื่องมือ Calibrator model 5500A, 5502A, 5520A, 5522A, 5700A, 5720A, 5725A, 5502E, 5100B, 5025E, 3010, 3041, C-101และ 9100 เครื่องมือ Digital Multimeter model 3458A, 8508, 4950).
4. ห้องปฏิบัติการฯ ขอสงวนสิทธิ์ การชดใช้ค่าเสียหายในกรณี เครื่องมือถูกพบว่ามีข้อบกพร่องระหว่างการสอบเทียบ เครื่องมือนั้นจะถูกส่งคืนและเก็บค่าธรรมเนียมทั้งหมดหรือบางส่วน ทั้งนี้ขึ้นอยู่กับค่าใช้จ่ายที่เกิดขึ้นจริง
5. ห้องปฏิบัติการฯ จะไม่รับผิดชอบต่อความเสียหายใดๆ ที่อาจเกิดขึ้นขณะที่เครื่องมือหรืออุปกรณ์เสริมอยู่ในความดูแลของห้องปฏิบัติการฯ เว้นแต่จะพิสูจน์ได้ว่าเครื่องมือหรืออุปกรณ์เสริมที่นำมาสอบเทียบเสียหายสูญหายอันเกิดจากการกระทำของห้องปฏิบัติการฯ
6. ในกรณีที่อุปกรณ์เสียหายหรือชำรุดอันเนื่องมาจากการสอบเทียบของห้องปฏิบัติการฯ เราขอสงวนสิทธิ์ในการชดใช้ค่าเสียหายให้กับลูกค้าของเราสูงสุดไม่เกินค่าสอบเทียบ
7. ห้องปฏิบัติการฯ จะไม่รับผิดชอบต่อความเสียหายหรือข้อบกพร่องใดๆ ของอุปกรณ์ในระหว่างการขนส่ง ยกเว้นการขนส่งโดยพนักงานของ ห้องปฏิบัติการฯ
8. ค่าบริการข้างต้นอาจเปลี่ยนแปลงได้ หากรายการสอบเทียบที่ส่งมาสอบเทียบยังห้องปฏิบัติการหรืองาน On-site มีการเปลี่ยนแปลง

Customer acknowledge and signed

---

(  )

Date:


**NA Caltechnologies Co., Ltd.**
75/107 Moo 11, Klongnueng, Klongluang, Pathumthani 12120, THAILAND
Tel. +662-529-2460-5, Fax. +662-529-2133, 529-2466
Email: sales-cal@nacal.co.th Website: www.nacal.co.th

# Quotation Attachment:

## Decision Rule for Statements of Conformity in the Calibration Certificate:

1. Based on ISO/IEC 17025:2017 requirements, NACAL will provide a statement of conformity to a specification or standard for the calibration results as "Pass", "Pass#", "Fail#" or "Fail" in the calibration certificates and reports.
   ** For some of calibration parameters or certificates will not be provided these statements due to smaller specifications or higher measurement uncertainty that may affect to the level of risk as false accept and false reject of the results. **

2. The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements.

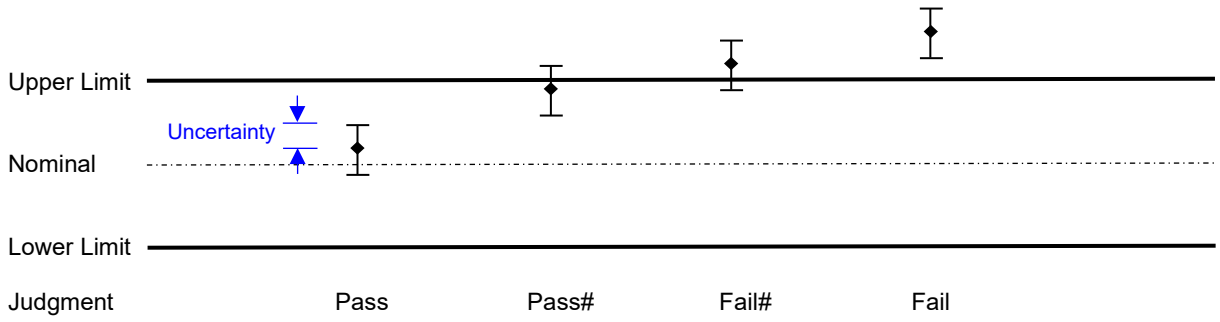


- Pass - The measurement result plus the expanded uncertainty with a 95% coverage probability were within the specification limit. Then conformity with the specification is stated.
- Pass# - The measurement result was within the specification limit, but a portion of the expanded uncertainty with a 95% coverage probability was overlapped the specification limit. It is not possible to state conformity using the 95% coverage probability for the expanded uncertainty although the measurement result was below the limit.
- Fail# - The measurement result was out of the specification limit, but a portion of the expanded uncertainty with a 95% coverage probability was in the specification. It is not possible to state non-conformity using the 95% coverage probability for the expanded uncertainty although the measurement result was out of the limit.
- Fail - The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the specification limit. Then non-conformity with the specification is stated.

3. If customer needs to prescribe own rule which the measurement uncertainty is not taken into account, or other decision rules applied, the customer can request to NACAL via the laboratory's emails for following those rules, NACAL shall include notes and explanations in the certificate in order to ensure unambiguous reporting as the customer's request.

Effective Date: March 15, 2019


Authority: Laboratory Manager
Rev.00 (January 2019)

**NA Caltechnologies Co., Ltd.**
75/107 Moo 11, Klongnueng, Klongluang, Pathumthani 12120, THAILAND
Tel. +662-529-2460-5, Fax. +662-529-2133, 529-2466
Email: sales-cal@nacal.co.th Website: www.nacal.co.th

## ใบแนบใบเสนอราคา:

## การระบุข้อความของความเป็นไป หรือ ไม่เป็นไปตามข้อกำหนด ในใบรับรองการสอบเทียบ:

1. อ้างอิงจากข้อกำหนด ISO/IEC 17025:2017 ห้องปฏิบัติการสอบเทียบ บริษัท เอ็นเอ แคลเทคโนโลยี จำกัด จะรายงานข้อความแสดงความเป็นไปหรือไม่เป็นไปตามข้อกำหนดของเครื่องมือที่ถูกสอบเทียบ ลงในใบรับรองการสอบเทียบ โดยใช้ข้อความว่า “ผ่าน” “ผ่าน#” “ไม่ผ่าน#” หรือ “ไม่ผ่าน”
   ** สำหรับการสอบเทียบเครื่องมือบางประเภท ห้องปฏิบัติการขอสงวนสิทธิ์ที่จะไม่แสดงข้อความเหล่านี้ อันเนื่องมาจากเหตุผลด้านขีดจำกัด (Specification) ของเครื่องมือมีขนาดเล็กมากเกินไป หรือ มีค่าความไม่แน่นอนจากการวัดสูงเกินไป ที่อาจมีความเสี่ยงต่อการไม่ยอมรับผลการตัดสิน **
2. กฎการตัดสินผลการสอบเทียบที่นำมาใช้ ห้องปฏิบัติการอ้างอิงจากเอกสาร ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification โดยมีเงื่อนไขและการตัดสินผลการสอบเทียบเป็นไปตามรูปภาพ ดังต่อไปนี้

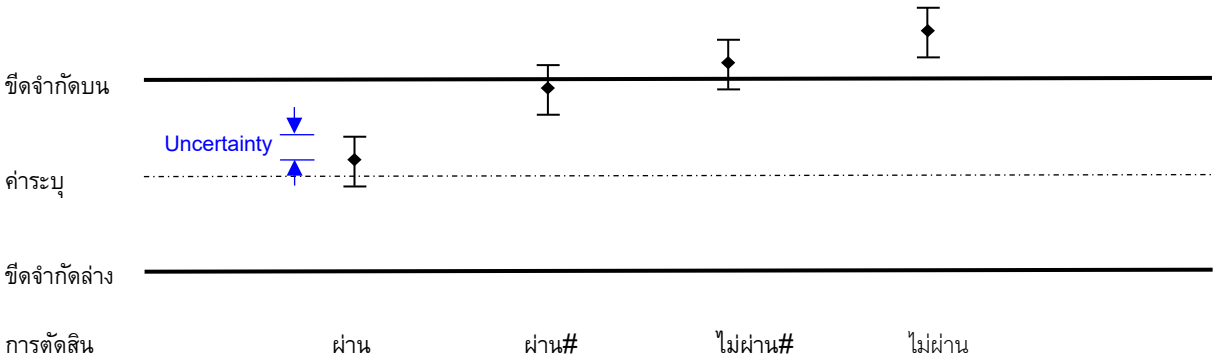


- ผ่าน - ผลการสอบเทียบเมื่อนำมารวมกับค่าความไม่แน่นอนจากการวัดที่ระดับความเชื่อมั่น 95% มีค่าอยู่ในขอบเขตของขีดจำกัดที่กำหนด สามารถระบุได้ว่า ผลการสอบเทียบ เป็นไปตาม ข้อกำหนดของเครื่องมือ
- ผ่าน# - ผลการสอบเทียบมีค่าอยู่ในขอบเขตของขีดจำกัดที่กำหนด แต่พบว่ามีบางส่วนของค่าความไม่แน่นอนจากการวัดที่ระดับความเชื่อมั่น 95% อยู่นอกขอบเขตของขีดจำกัดที่กำหนด สามารถระบุได้ว่า ผลการสอบเทียบ อาจเป็นไปตาม ข้อกำหนดของเครื่องมือ
- ไม่ผ่าน# - ผลการสอบเทียบมีค่าอยู่นอกขอบเขตของขีดจำกัดที่กำหนด แต่พบว่ามีบางส่วนของค่าความไม่แน่นอนจากการวัดที่ระดับความเชื่อมั่น 95% อยู่ในขอบเขตของขีดจำกัดที่กำหนด สามารถระบุได้ว่า ผลการสอบเทียบ อาจไม่เป็นไปตาม ข้อกำหนดของเครื่องมือ
- ไม่ผ่าน - ผลการสอบเทียบเมื่อนำมารวมกับค่าความไม่แน่นอนจากการวัดที่ระดับความเชื่อมั่น 95% มีค่าอยู่นอกขอบเขตของขีดจำกัดที่กำหนด สามารถระบุได้ว่า ผลการสอบเทียบ ไม่เป็นไปตาม ข้อกำหนดของเครื่องมือ

3. หากลูกค้ามีความประสงค์ที่จะให้ห้องปฏิบัติการใช้กฎการตัดสินผลการสอบเทียบ โดยไม่รวม ค่าความไม่แน่นอนจากการวัด หรือ ใช้กฎการตัดสินอื่นๆ ขอให้ท่านได้แจ้งความประสงค์ดังกล่าวเข้ามายังห้องปฏิบัติการผ่านช่องทาง Email ของห้องปฏิบัติการ ซึ่งท่านสามารถแจ้งความประสงค์ดังกล่าวเพียงครั้งเดียวเท่านั้น โดยห้องปฏิบัติการจะปฏิบัติตามคำร้องขอของท่านตลอดไป จนกว่าจะมีการแจ้งเปลี่ยนแปลง

มีผลตั้งแต่วันที่ 15 มีนาคม 2562 เป็นต้นไป
ผู้จัดการห้องปฏิบัติการสอบเทียบ