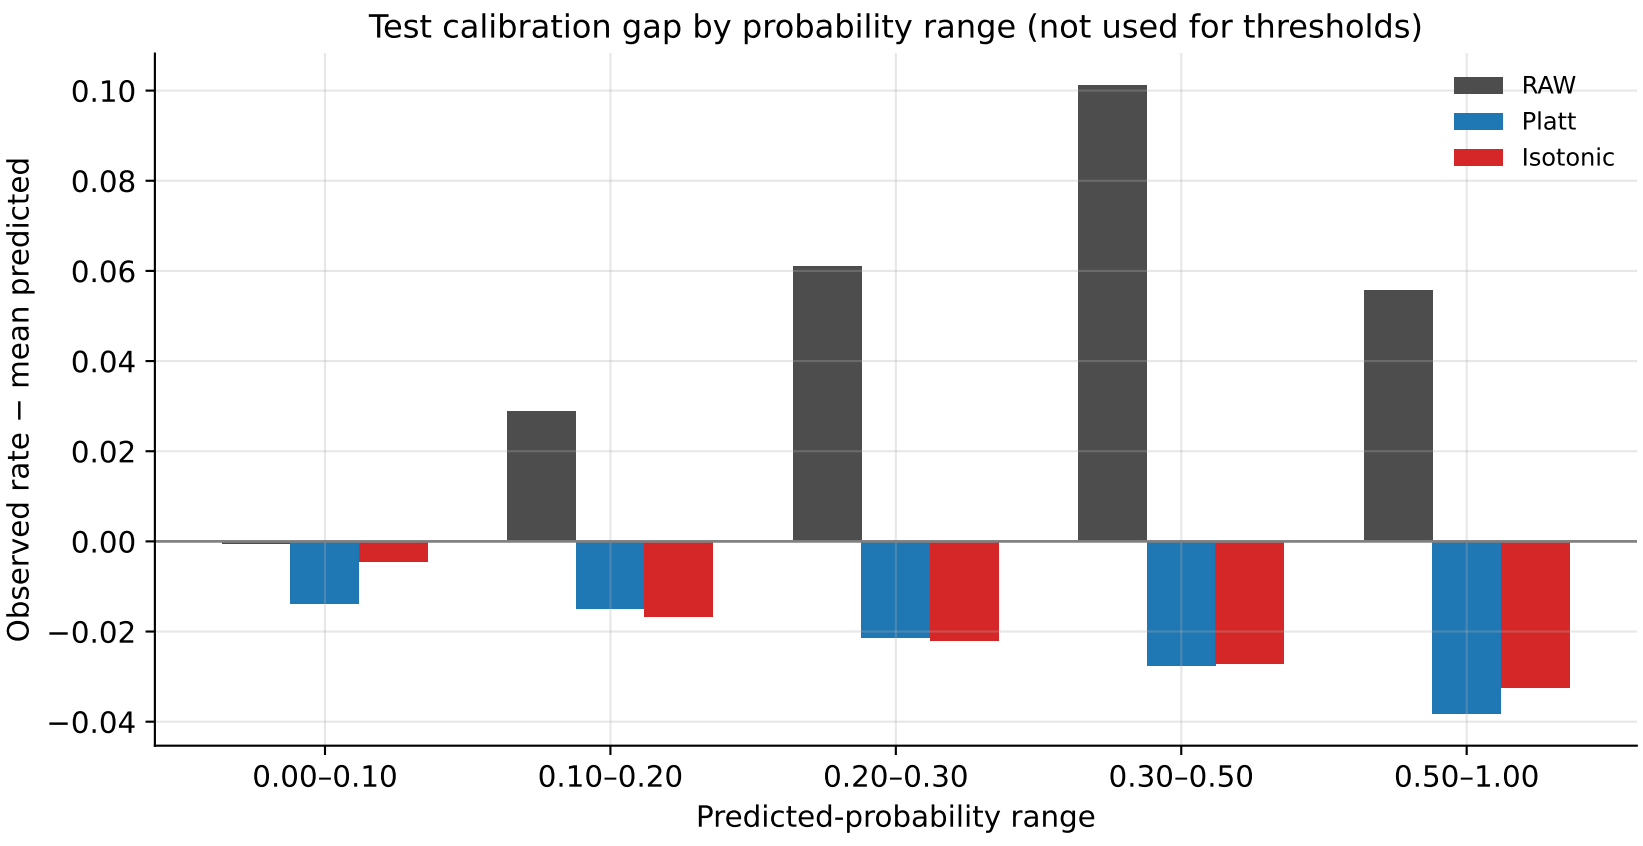
Test calibration gap by probability range (not used for thresholds)
RAW
Platt
Isotonic
Observed rate − mean predicted
0.10
0.08
0.06
0.04
0.02
0.00
−0.02
−0.04
0.00–0.10
0.10–0.20
0.20–0.30
0.30–0.50
0.50–1.00
Predicted-probability range