

RS232 Connections and configuration for MSeries ForTest equipment

The instrument is equipped with a serial port COM1 which is located in the rear of the instrument panel Through this port it is possible to send commands and receive responses from the device



Note : Only COM1 works with the serial protocol

COM2 it's for internal use or for send messages to a printer or receive data from a barcode reader



The COM1 of the device must be connected to a master controller (a PC for example) using a ForTest's serial cable. Standard RS232 cable don't work.


Pinout specification are available [here](#).

This cable now can be connected to a PC by using a integrated serial card or an USB/RS232 adapter



From the Control Panel of your operating system is it possible to see the available COM port of the PC and open a connection with the ForTest device.

From Windows : **Control Panel -> System and Security -> Device Manager**

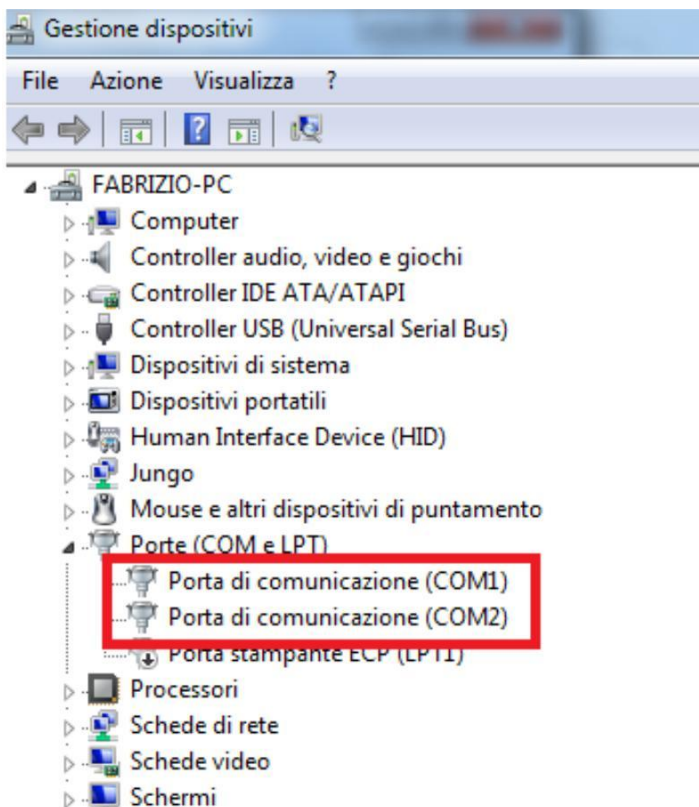



In this case for example a PC is equipped with two separated serial ports

COM1 of the PC is connected with the ForTest's cable to COM1 of the instrument




From the menu **SET** of the device please go to "**COM PORT SETTINGS**" section using the UP and DOWN keys

Please check that:

- Serial address is set to 01
- COM1 modality is set to "PC directly" (or Prot. ForTest)
- COM1 baudrate is set to 9600

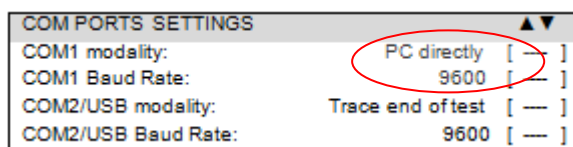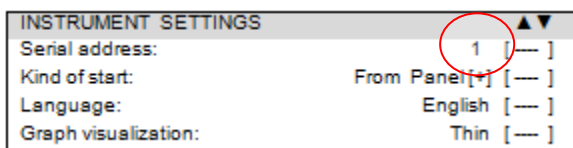


To test if the communication is working properly it is necessary to open the **COM** port from the PC connected to the equipment with a serial terminal application like Hyperterminal or [Putty](#) and send command **":0116D"** (please note that terminal will not return echo of characters). If the communication work properly a string of 101 characters will be returned

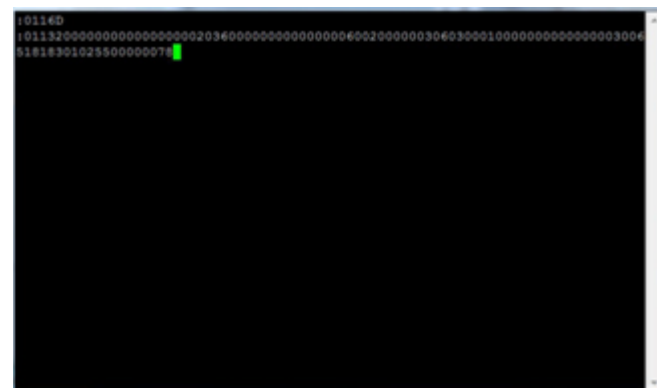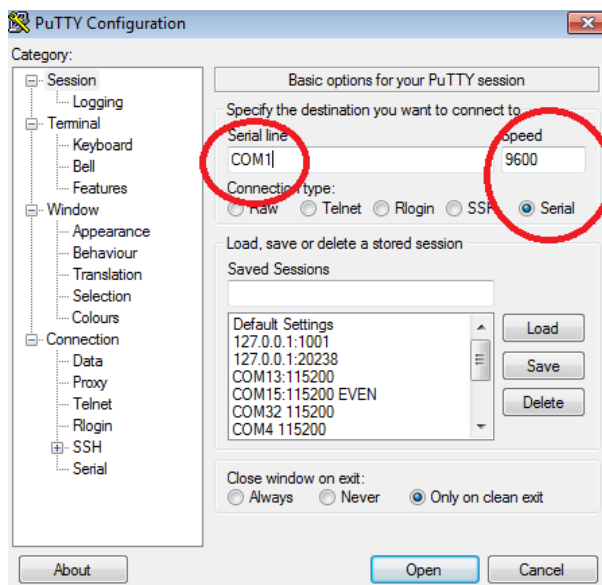

If you have a PC software ForTest the configuration is the follow:

From menu **File > Option > Connection**

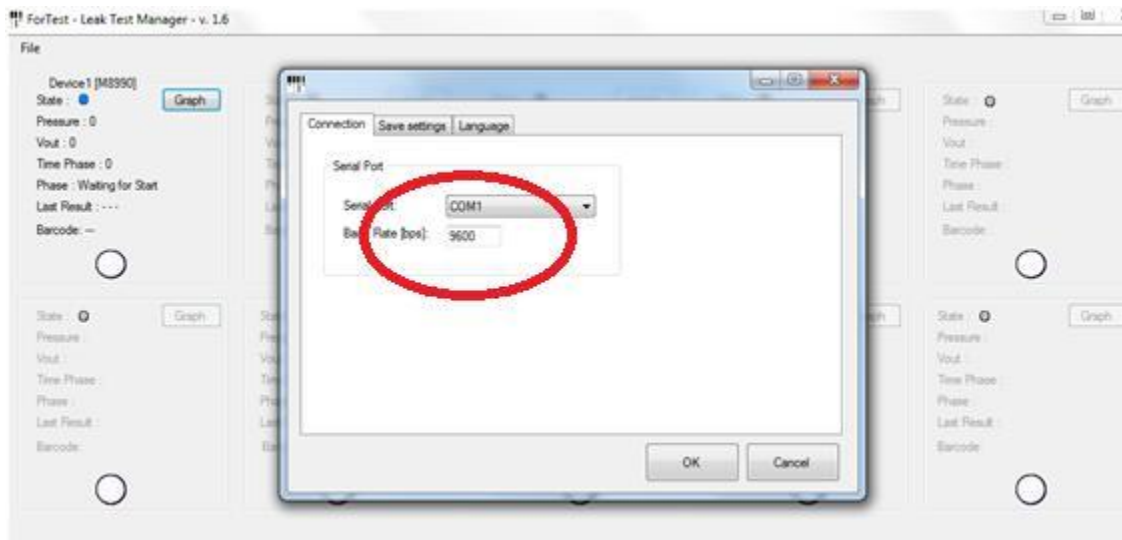

Please check that the **COM** port selected is right and the baudrate is the same set on the **SET** menu

Click "**OK**" and restart the program

Device now should be connected



ForTest Italia s.r.l.

Sede legale:
V.le Gramsci, 239/F - 41037 Mirandola (MO) - IT
Sede operativa:
Comparto Alfieri Maserati, Sez. 2A
Via Sibilla Aleramo, 7
41123 Modena (MO) - IT

P.I. / C.F. IT02934911203 REA MO-378687
Phone +39 059 557250
Fax +39 059 579022
www.fortest.com
info@fortest.com