

SCHEMATICS FOR RS485 CONNECTION TO FORTEST T-SERIES



SCHEMATICS FOR T8000 CONNECTION

Table 2. RS-232 PINOUT	
PIN #	SIGNAL
1	DCD
2	RD
3	TD
4	DTR
5	GND
6	DSR
7	RTS
8	CTS



Table 1. RS-422/485 PINOUT	
PIN #	SIGNAL
2	RD (A)-
3	TD (B) +
4	GND
6	GND
7	RD (B)+
8	TD (A)-

COM1 pin8
COM1 pin9
COM1 pin5

A "[4WSD9R](#)" RS232/RS485 converter is used

RS232 side is connected to a PC. Connection require a RS232/USB converter or a RS232 PCI Card native.

RS485 side is connected to COM1 of a T8000 at the specified pins.

For more information about RS485 pins side equipment please refer to this [link](#).

COMMUNICATION TEST USING MODBUS-RTU

On the SET menu of the instrument the necessary settings are:


- Serial Address : 01
- SER0/USB modality : Modbus RTU
- SER0/USB baud rate : 115200 bps

From the following link you can download the PC utility that allows you to test the modbus rtu communication

- <http://downloads.fortest-leak-testing.it/modpoll.zip>

Executing the command: `modpoll.exe -b 115200 -d 8 -s 1 -p none -a 1 -r 49 -c 20 -l 1000 COM1`

replacing "COM1" with the number of the port corresponding to the one connected to the instrument you should get the following response that can be decoded with the communication protocol table.

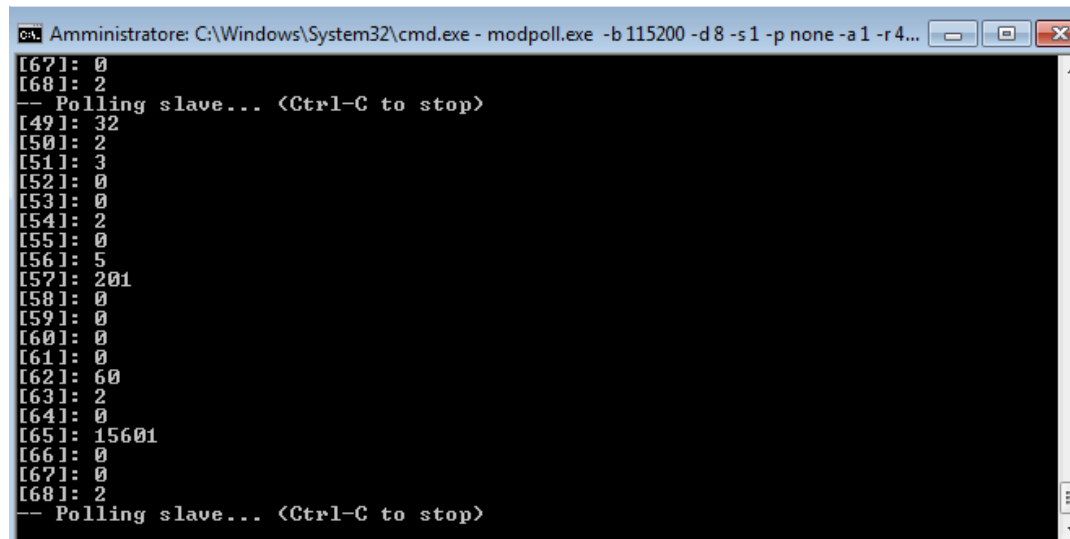

```
Administrator: C:\Windows\System32\cmd.exe - modpoll.exe -b 115200 -d 8 -s 1 -p none -a 1 -r 49...
[67]: 0
[68]: 2
-- Polling slave... (Ctrl-C to stop)
[49]: 32
[50]: 2
[51]: 3
[52]: 0
[53]: 0
[54]: 2
[55]: 0
[56]: 5
[57]: 201
[58]: 0
[59]: 0
[60]: 0
[61]: 0
[62]: 60
[63]: 2
[64]: 0
[65]: 15601
[66]: 0
[67]: 0
[68]: 2
-- Polling slave... (Ctrl-C to stop)
```