


Filename: Tapestation SAM8520.cHSRNA

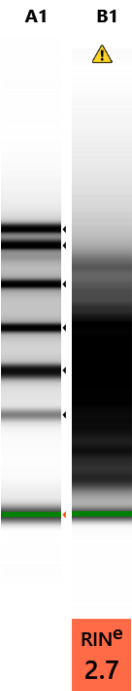


Default image (Contrast 100%)

Sample Info

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	3750	Electronic Ladder		Ladder
B1	2.7	0.4	14200	8520		Caution! Expired ScreenTape device; Sample concentration outside recommended range; The upper ribosomal fragment has degraded

A1: Electronic Ladder

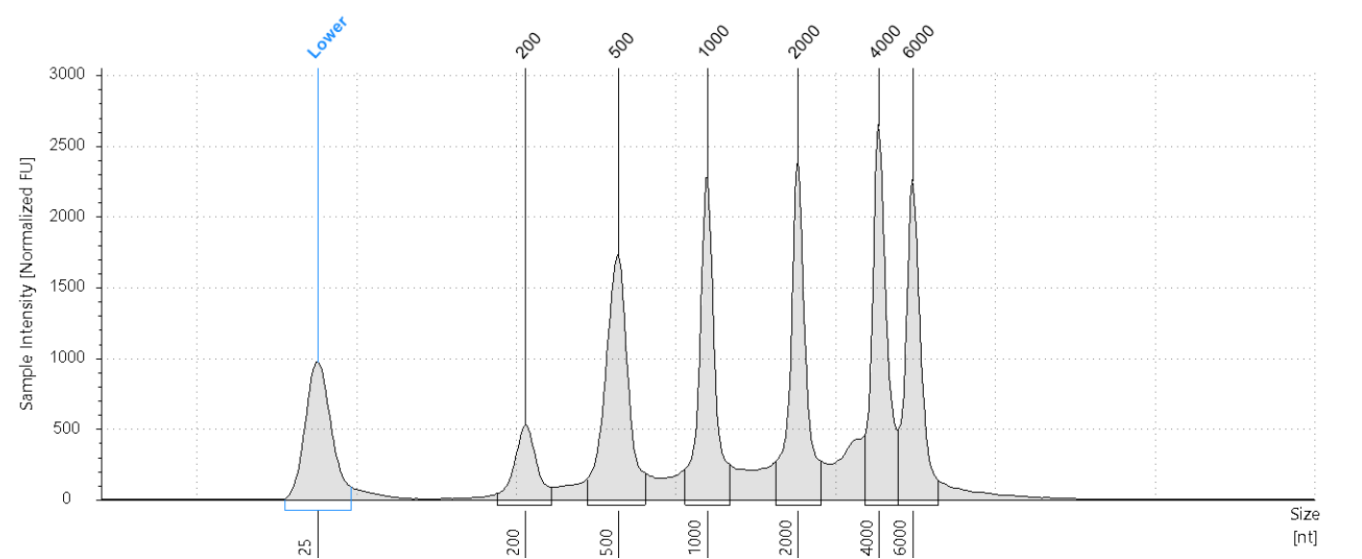


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	3750	Electronic Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
200	189	-	2770	5.98		
500	638	-	3760	20.25		
1000	557	-	1640	17.66		
2000	580	-	854	18.42		
4000	634	-	466	20.11		
6000	554	-	272	17.58		

B1: 8520

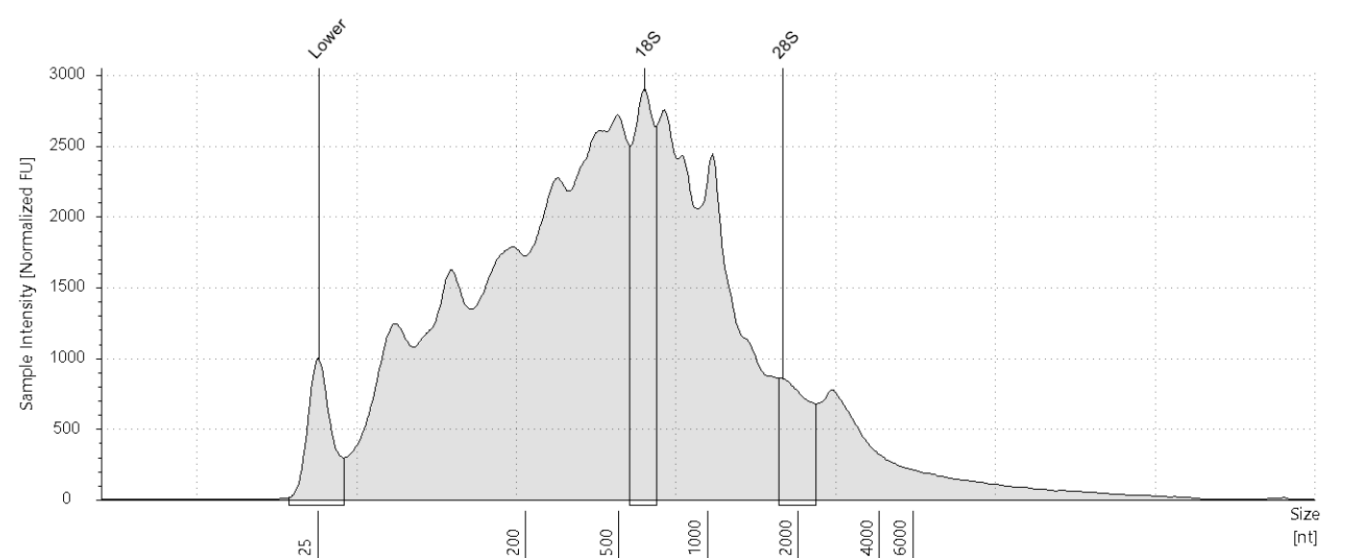


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
B1	2.7	0.4	14200	8520		Caution! Expired ScreenTape device; Sample concentration outside recommended range; The upper ribosomal fragment has degraded

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
606	1260	-	6110	71.70		18S
1756	496	-	831	28.30		28S

Filename: Tapestation SAM8521.cRNA

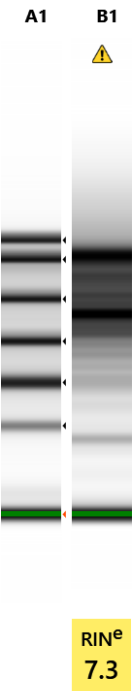


Default image (Contrast 100%)

Sample Info

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	-	70.4	Electronic Ladder		Ladder
B1	7.3	1.0	163	8521		Caution! Expired ScreenTape device (used after two weeks of first use)

A1: Electronic Ladder

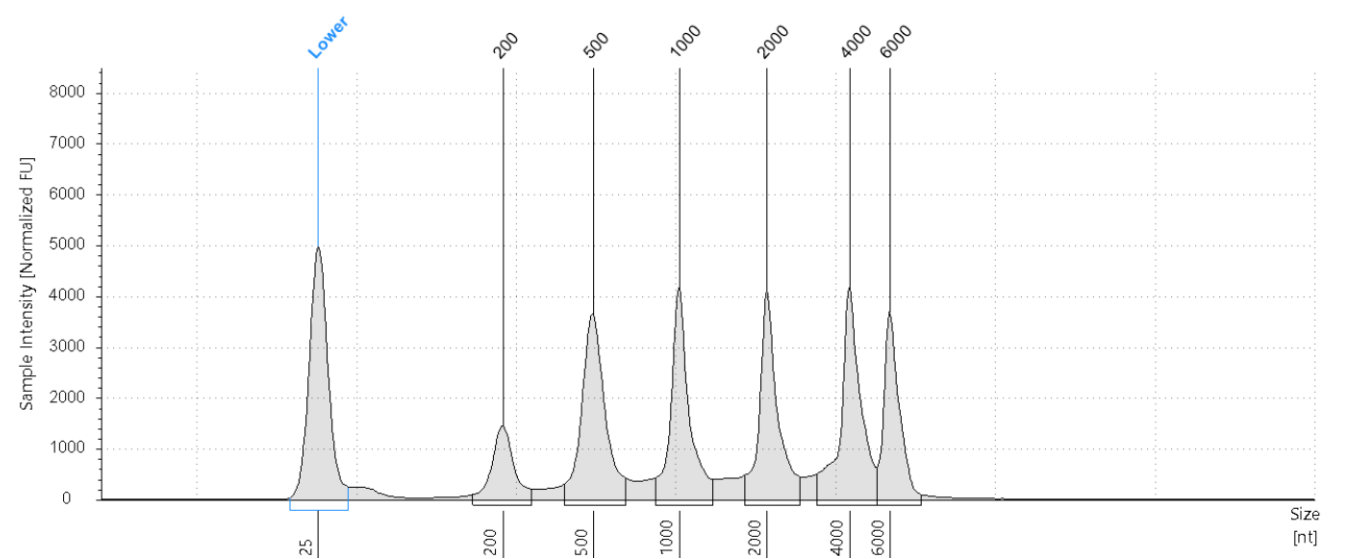


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	-	70.4	Electronic Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
200	4.92	-	72.4	7.80		
500	13.2	-	77.6	20.88		
1000	11.8	-	34.6	18.62		
2000	11.4	-	16.8	18.11		
4000	12.9	-	9.47	20.38		
6000	8.98	-	4.40	14.22		

B1: 8521

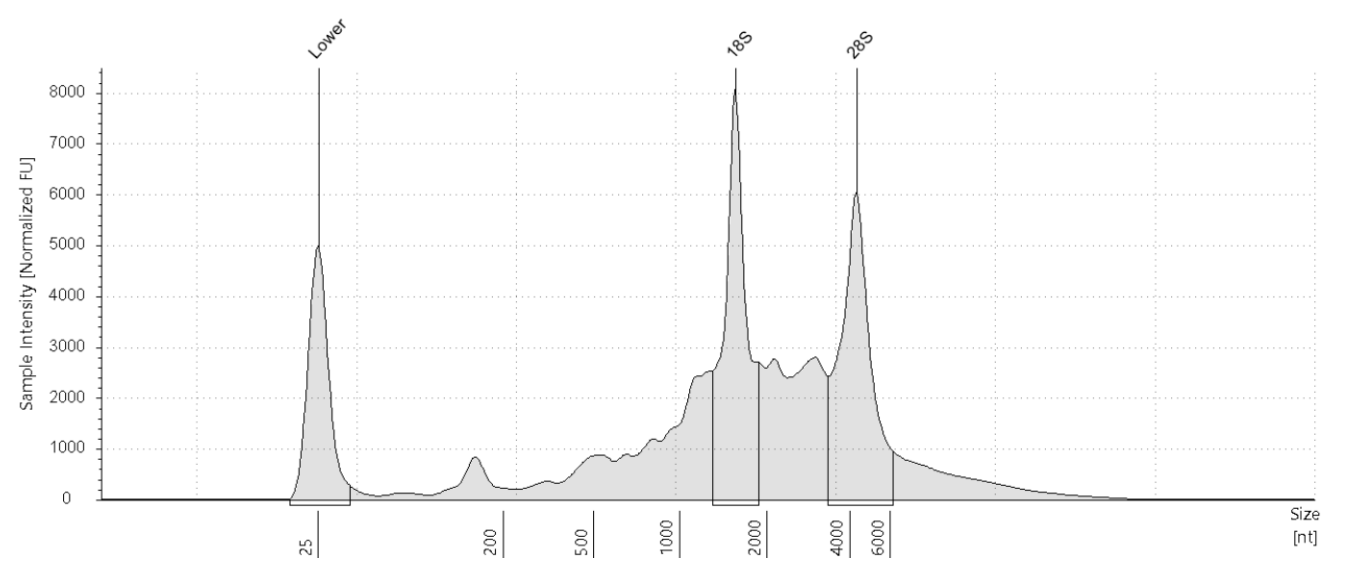

Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	7.3	1.0	163	8521		Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
1565	36.7	-	69.1	49.01		18S
4297	38.2	-	26.2	50.99		28S