



Filename: TCP_2627_011-TapeStation Sample QC report-21-05-2026.cRNA

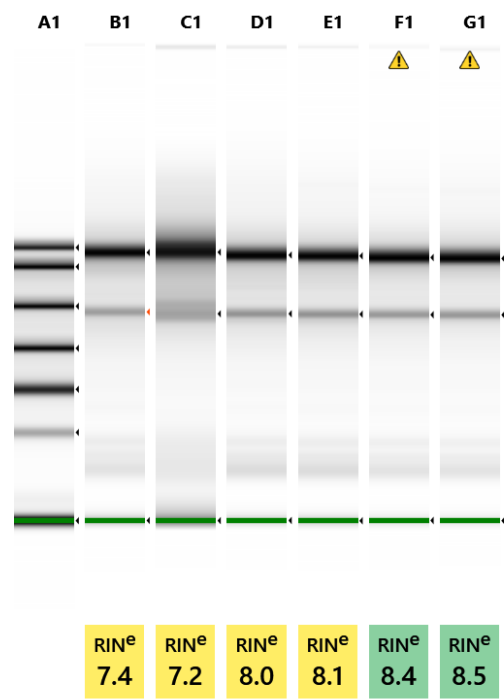

A1: Electronic Ladder

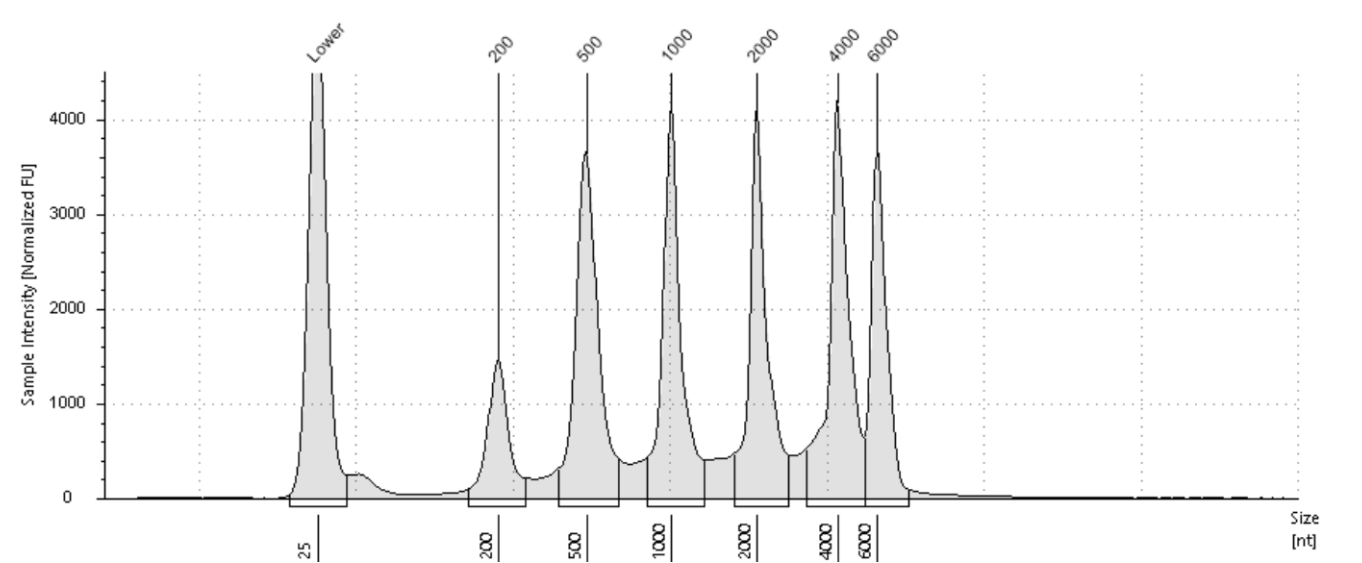


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	-	70.4	Electronic Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
200	4.92	-	72.4	7.80		
500	13.2	-	77.6	20.88		
1000	11.8	-	34.6	18.62		
2000	11.4	-	16.8	18.11		
4000	12.9	-	9.47	20.38		
6000	8.98	-	4.40	14.22		

B1: M1-SAM8545

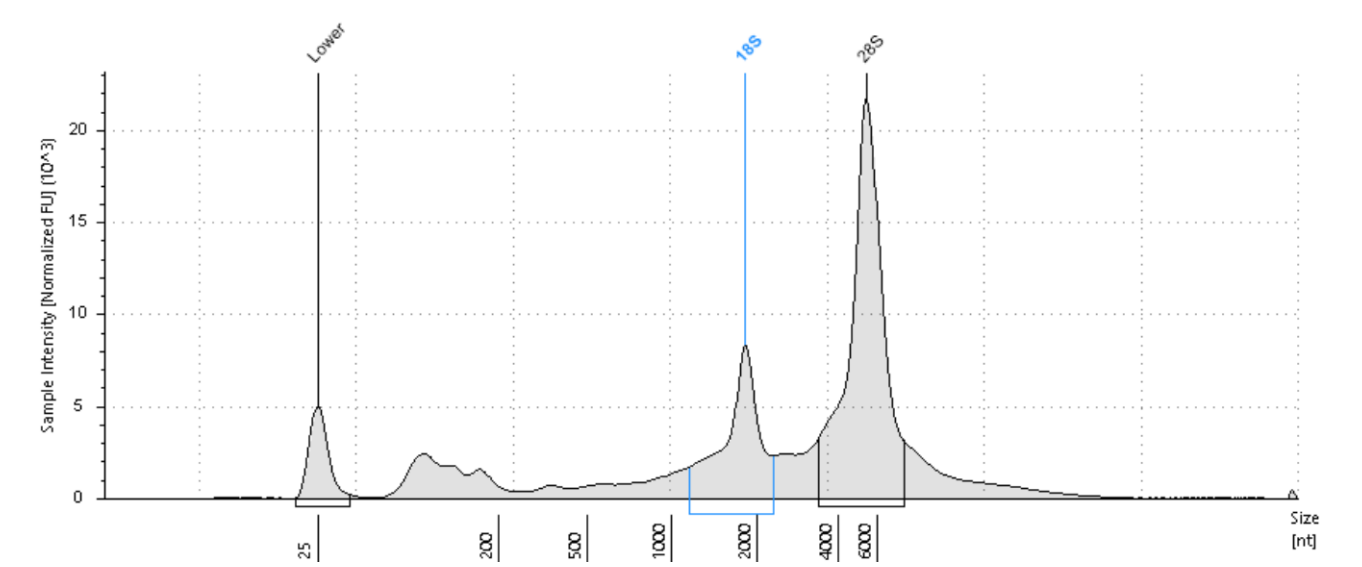


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
B1	7.4	2.6	307	M1-SAM8545		

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
1817	55.4	-	89.7	27.72		18S
5396	145	-	78.8	72.28		28S

C1: M3-SAM8546

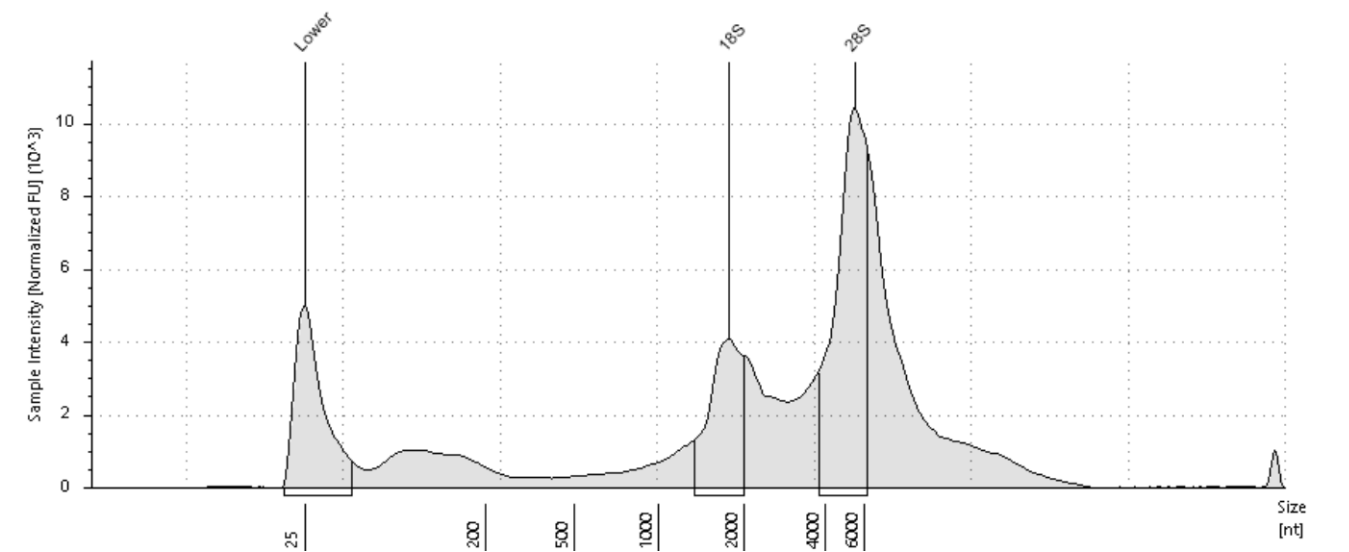


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
C1	7.2	2.4	157	M3-SAM8546		

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
1768	18.0	-	30.0	29.81		18S
5447	42.5	-	22.9	70.19		28S

D1: S2-SAM8547

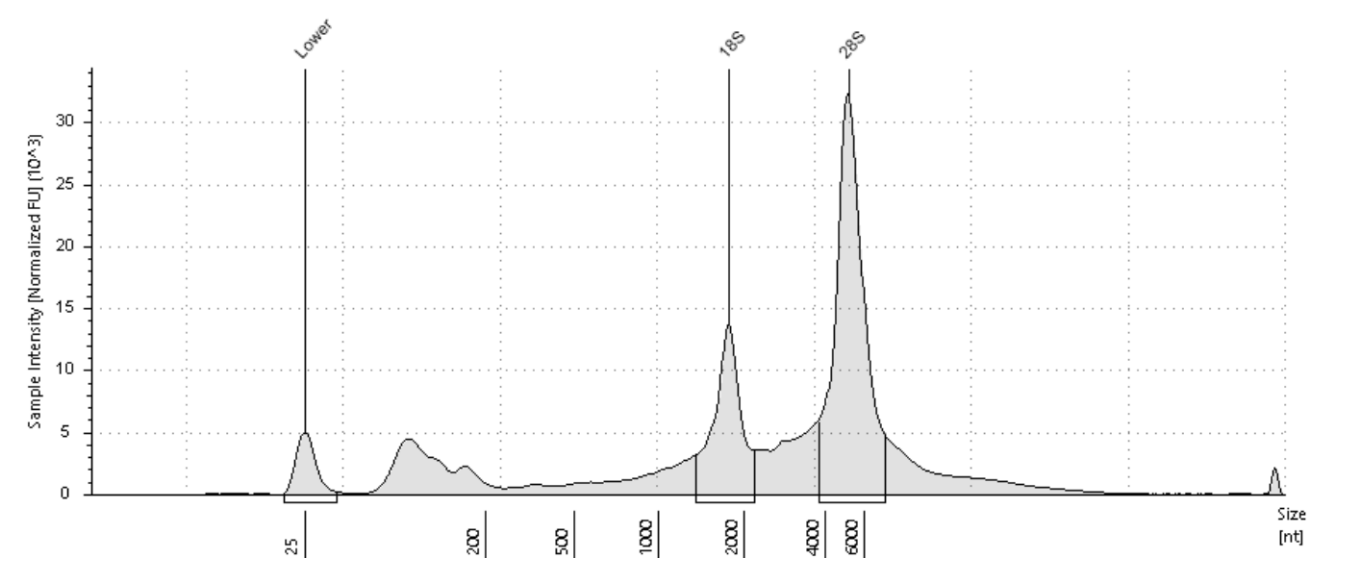


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
D1	8.0	2.6	447	S2-SAM8547		

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
1765	70.9	-	118	27.75		18S
5119	185	-	106	72.25		28S

E1: S3-SAM8548

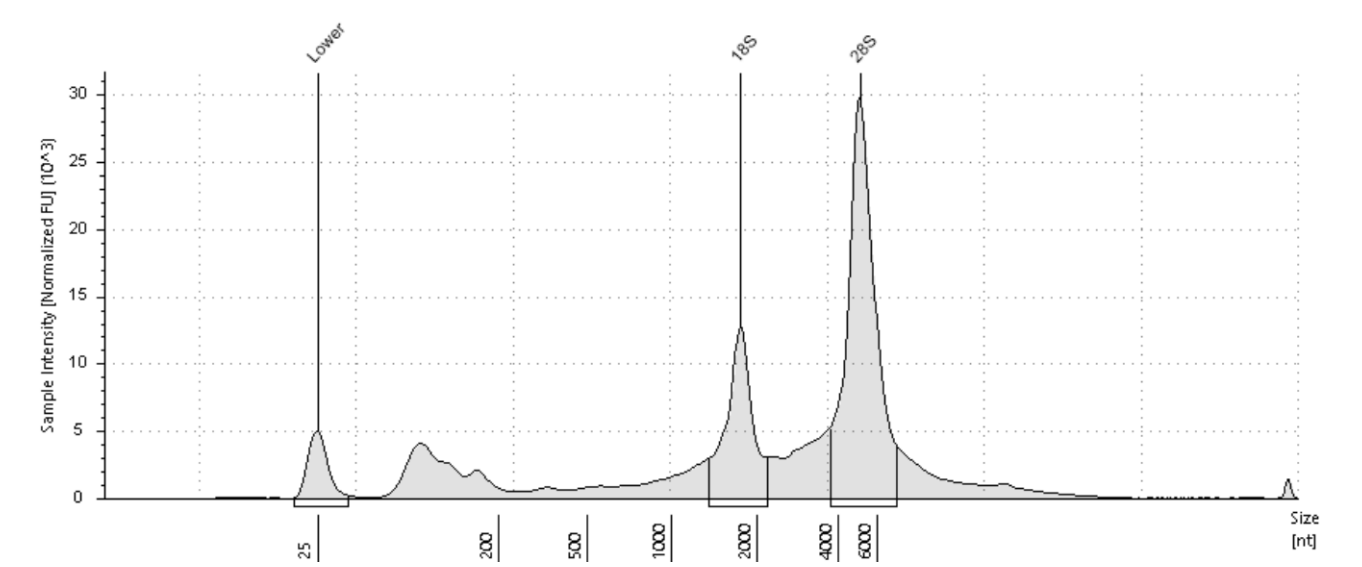


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
E1	8.1	2.5	392	S3-SAM8548		

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
1756	65.1	-	109	28.27		18S
5040	165	-	96.5	71.73		28S

F1: L1-SAM8549

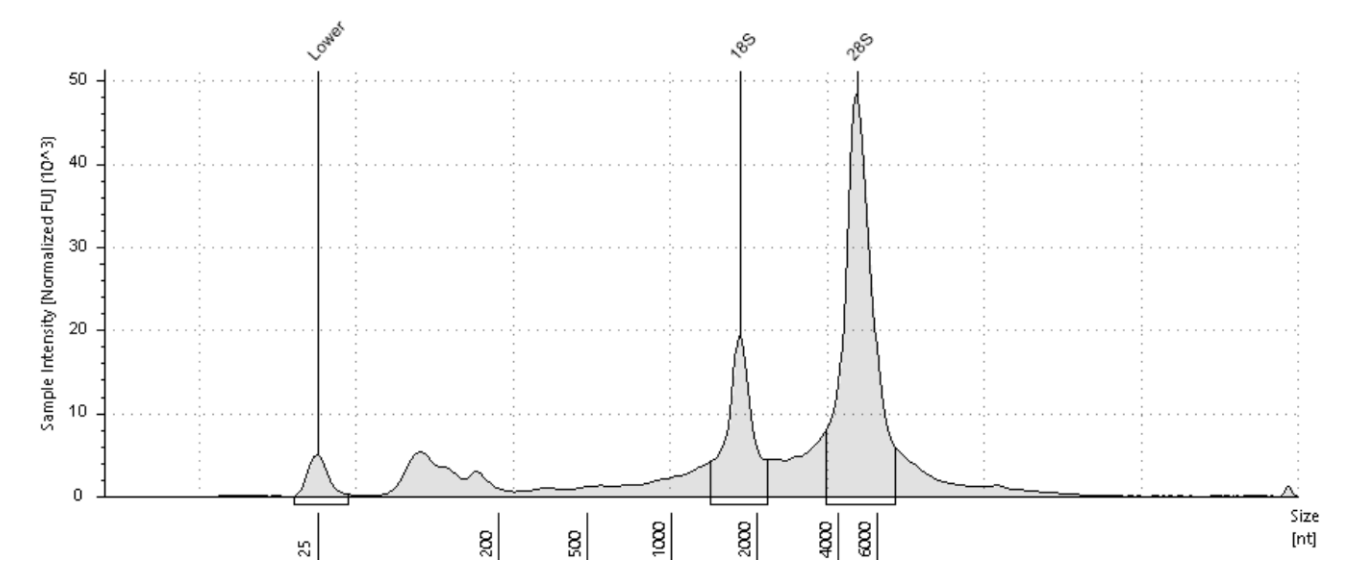


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
F1	8.4	3.0	578	L1-SAM8549		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
1736	92.0	-	156	25.18		18S
4859	273	-	166	74.82		28S

G1: L3-SAM8550

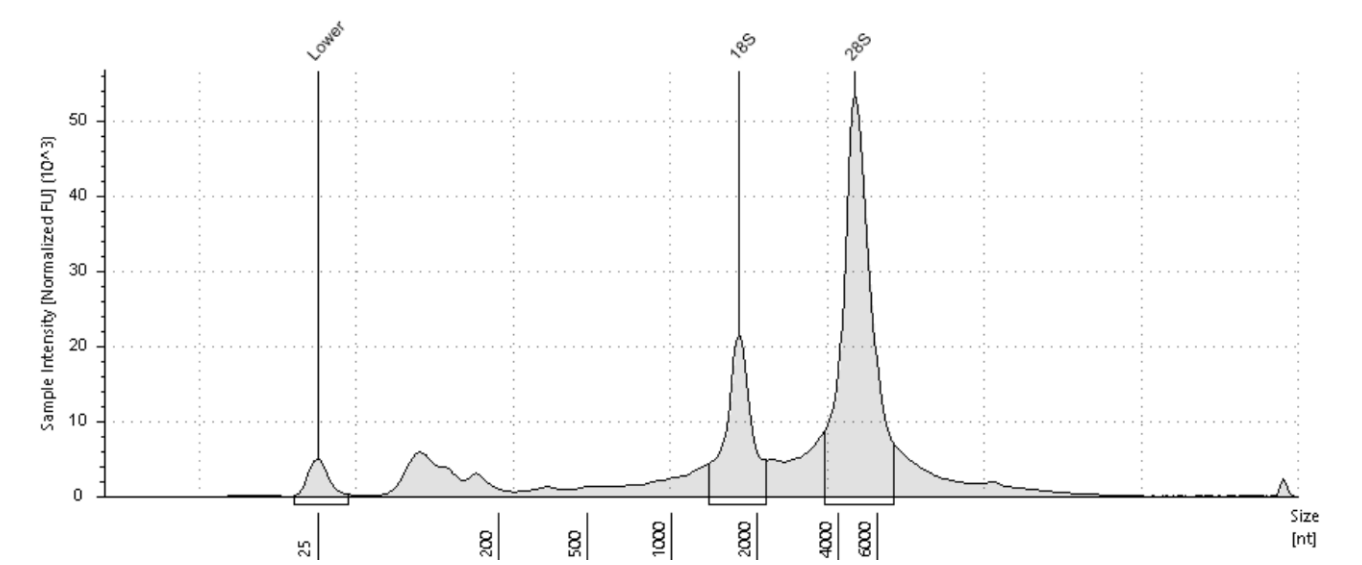

Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
G1	8.5	2.9	638	L3-SAM8550		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	36.0	36.0	4240	-		Lower Marker
1739	101	-	171	25.33		18S
4783	298	-	183	74.67		28S