Filename: T222 S308.cD1000

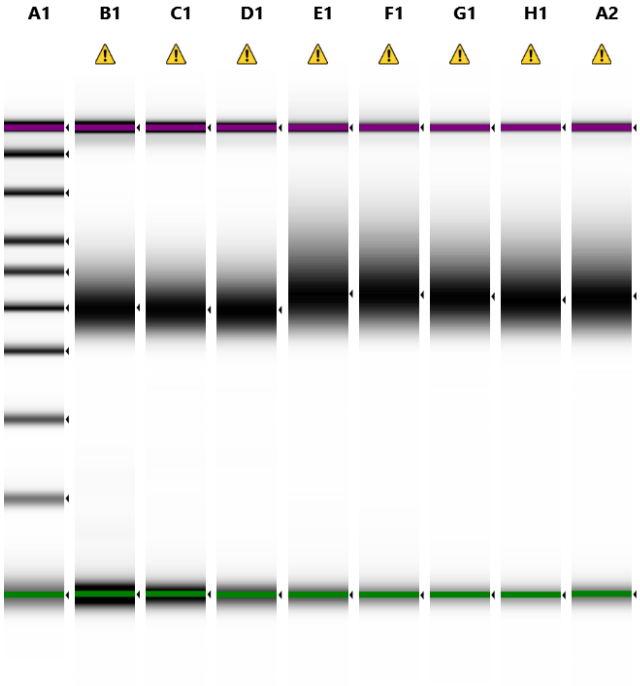

Default image (Contrast 50%), Image is Scaled to Highest Sample Peak

Sample Info

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	20.3	Electronic Ladder		Ladder
B1	8.27	VT-S1-SAM8121	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
C1	11.3	VT-S2-SAM8122	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
D1	17.2	VT-S3-SAM8123	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
E1	27.8	VT-S4-SAM8124	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
F1	33.8	VT-S5-SAM8125	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
G1	38.9	VT-S6-SAM8126	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
H1	37.6	VT-S7-SAM8127	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
A2	30.1	VT-S7-D-SAM8127D	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

© Agilent Technologies, Inc. 2023

A1: Electronic Ladder

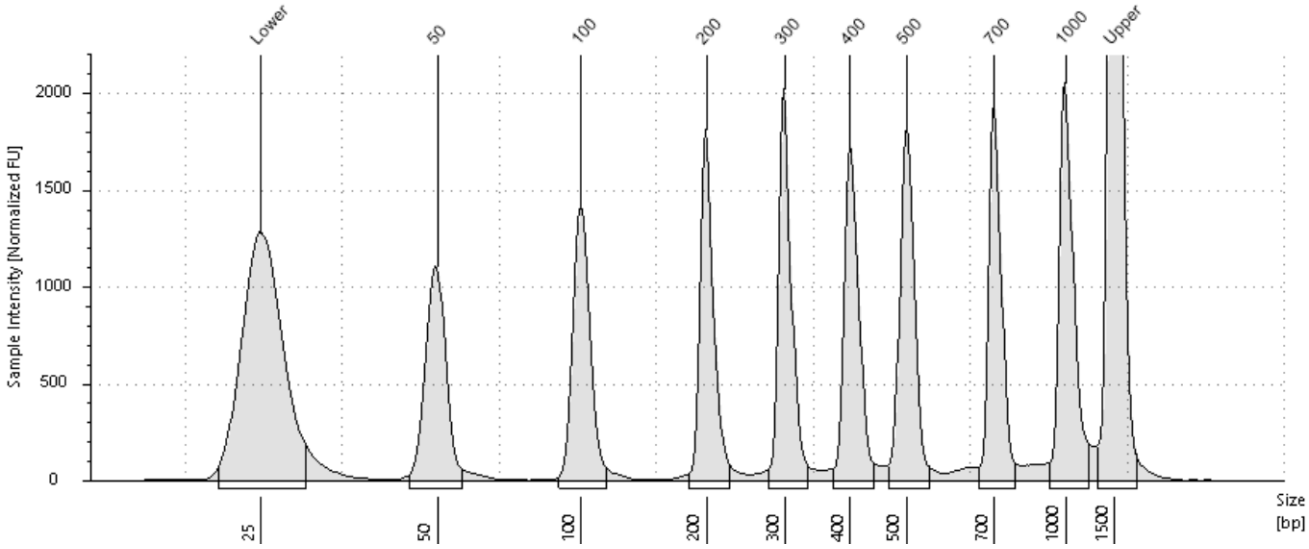

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	20.3	Electronic Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.22	-	321	-		Lower Marker
50	2.25	-	69.3	11.11		
100	2.37	-	36.5	11.71		
200	2.47	-	19.0	12.20		
300	2.55	-	13.1	12.56		
400	2.57	-	9.87	12.66		
500	2.71	-	8.33	13.36		
700	2.46	-	5.41	12.15		
1000	2.89	-	4.44	14.25		
1500	6.50	6.50	6.67	-		Upper Marker

© Agilent Technologies, Inc. 2023

B1: VT-S1-SAM8121

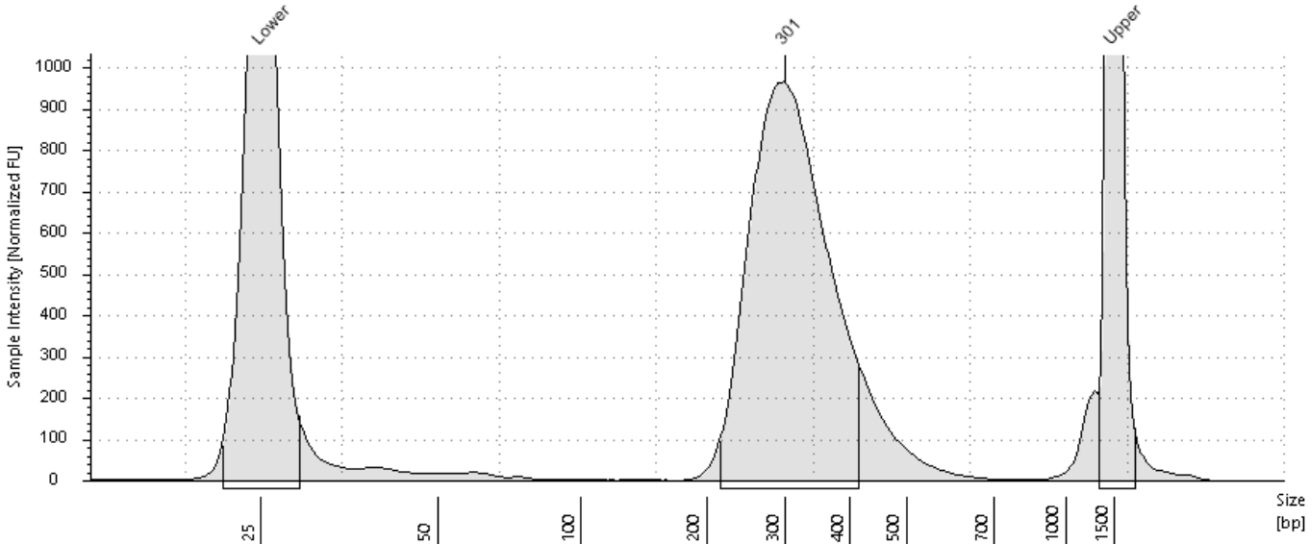

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
B1	8.27	VT-S1-SAM8121	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.95	-	366	-		Lower Marker
301	8.27	-	42.3	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

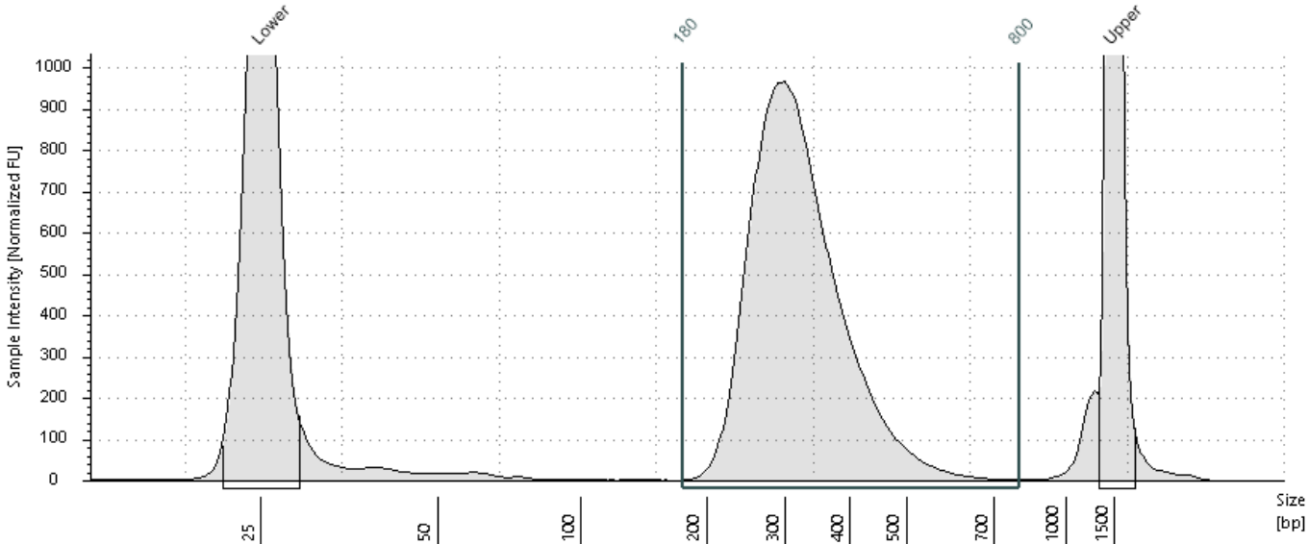

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
180	800	326	9.24	45.5	88.56		

© Agilent Technologies, Inc. 2023

C1: VT-S2-SAM8122

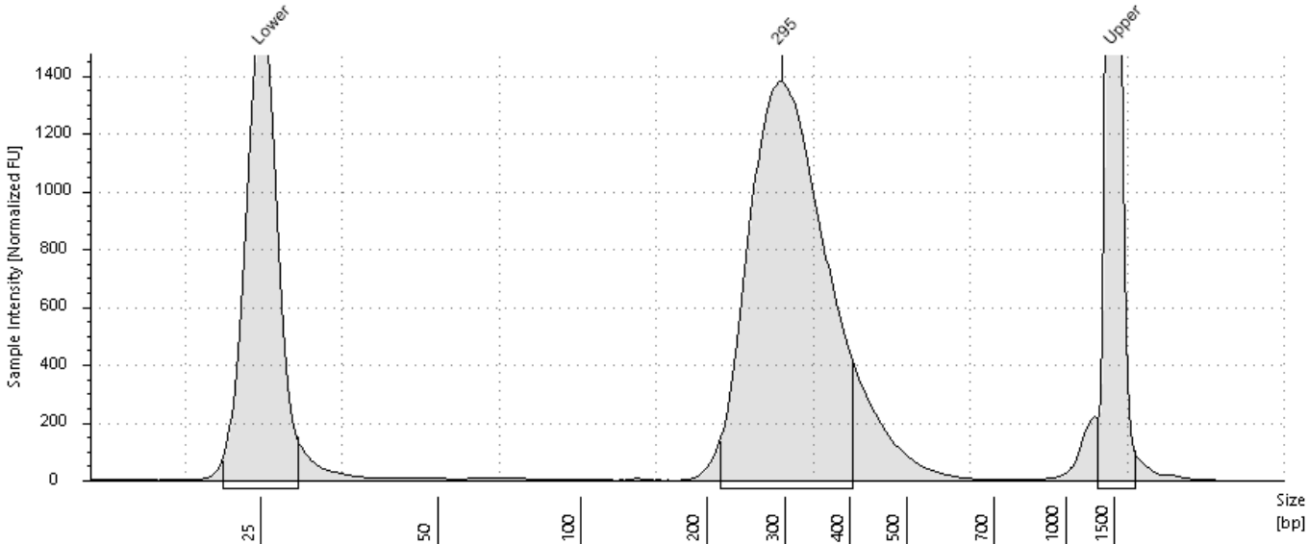

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
C1	11.3	VT-S2-SAM8122	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.62	-	346	-		Lower Marker
295	11.3	-	58.9	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

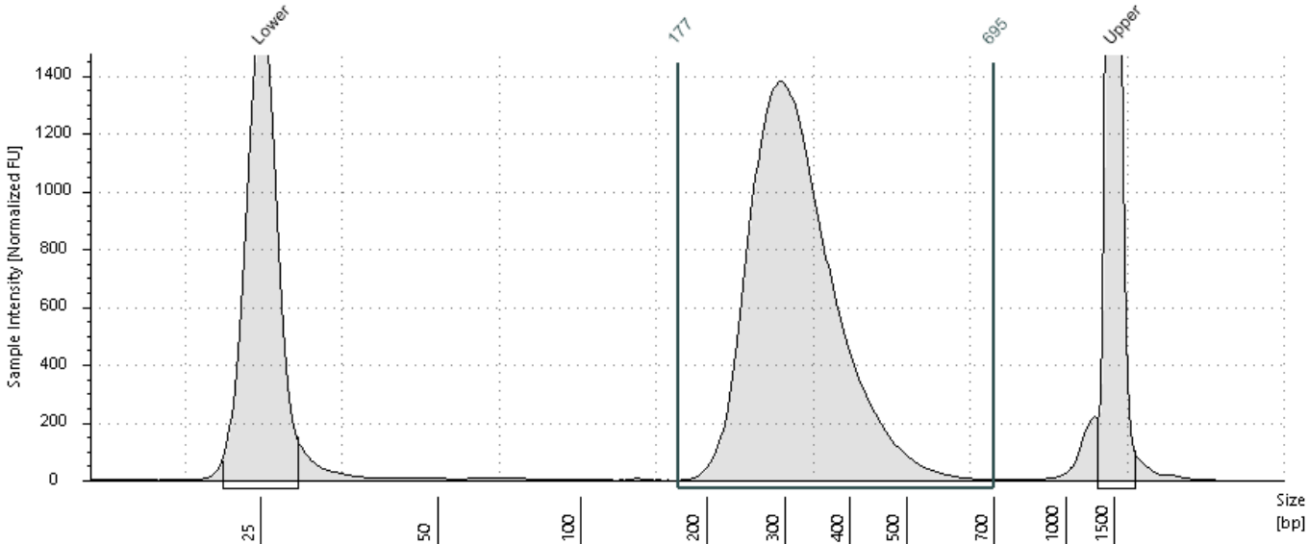

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
177	695	322	12.7	63.2	93.15		

© Agilent Technologies, Inc. 2023

D1: VT-S3-SAM8123

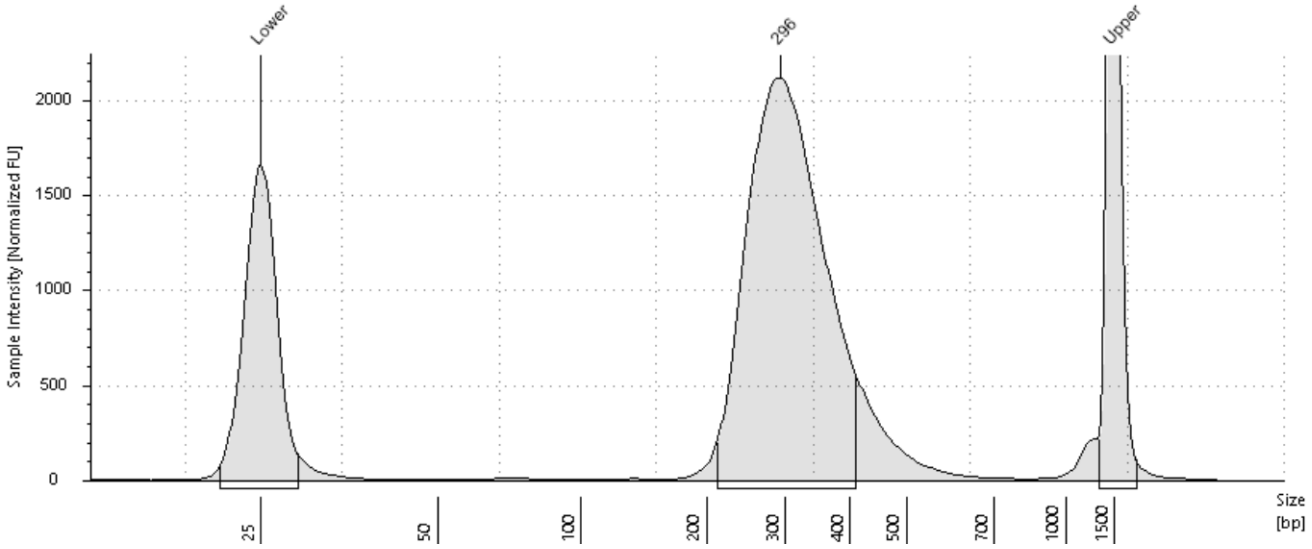

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
D1	17.2	VT-S3-SAM8123	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.78	-	356	-		Lower Marker
296	17.2	-	89.3	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

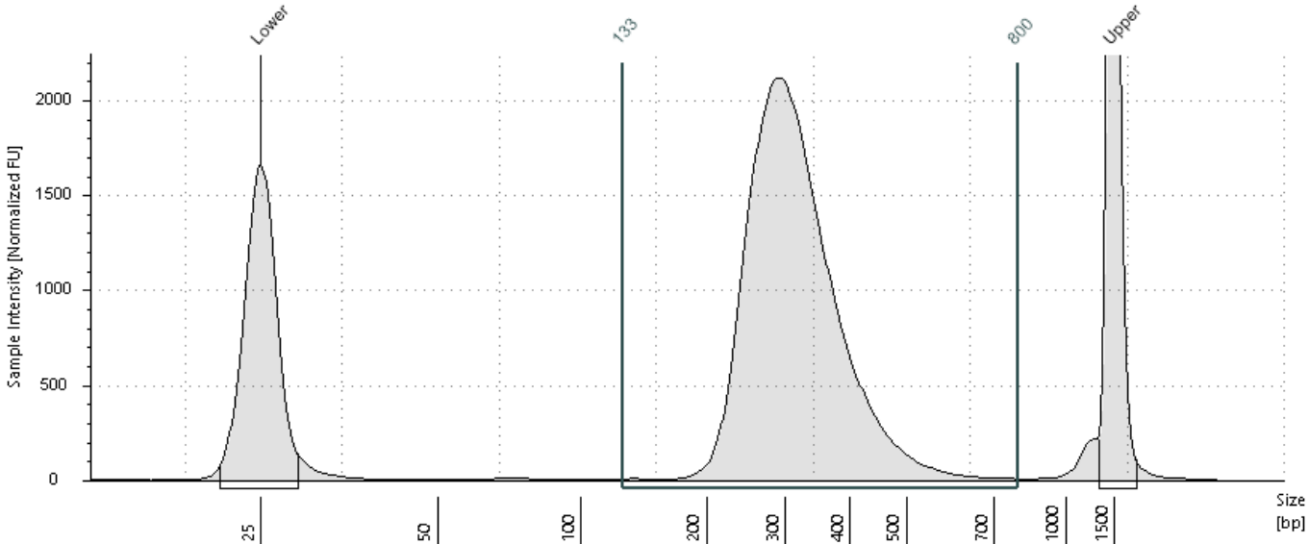

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
133	800	322	19.2	95.6	95.32		

© Agilent Technologies, Inc. 2023

E1: VT-S4-SAM8124

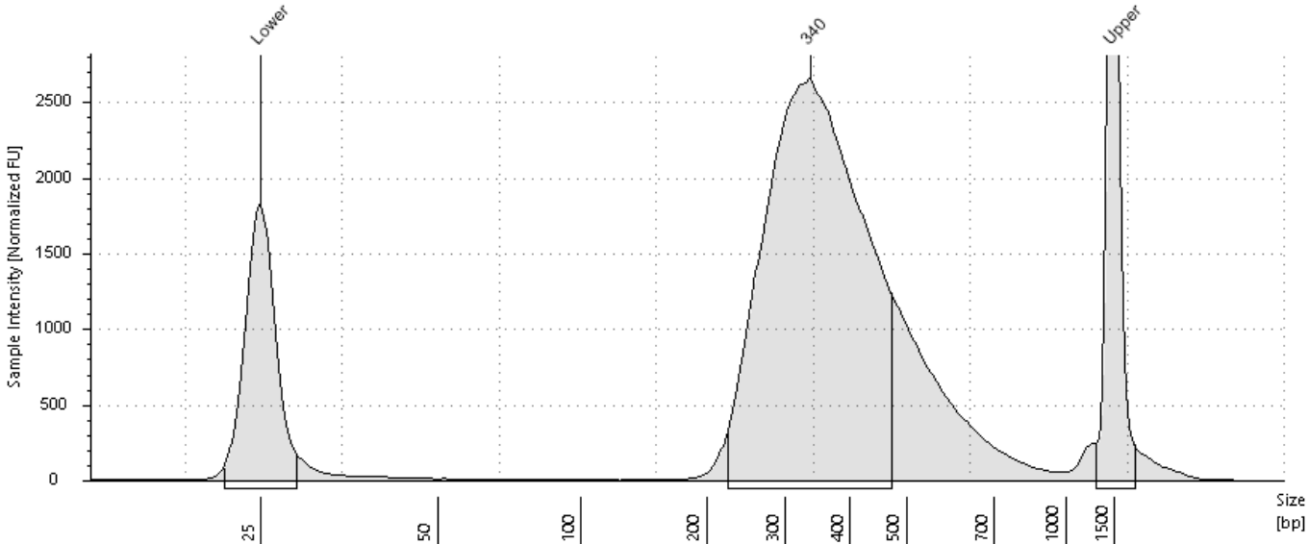

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
E1	27.8	VT-S4-SAM8124	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.88	-	362	-		Lower Marker
340	27.8	-	126	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

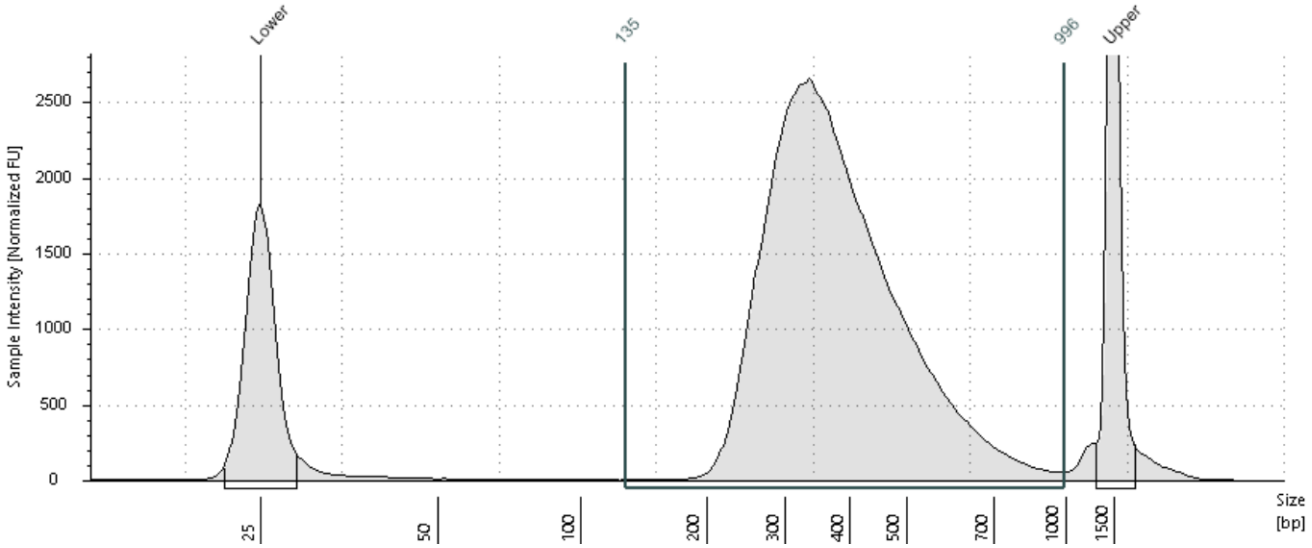

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
135	996	392	34.7	147	95.98		

© Agilent Technologies, Inc. 2023

F1: VT-S5-SAM8125

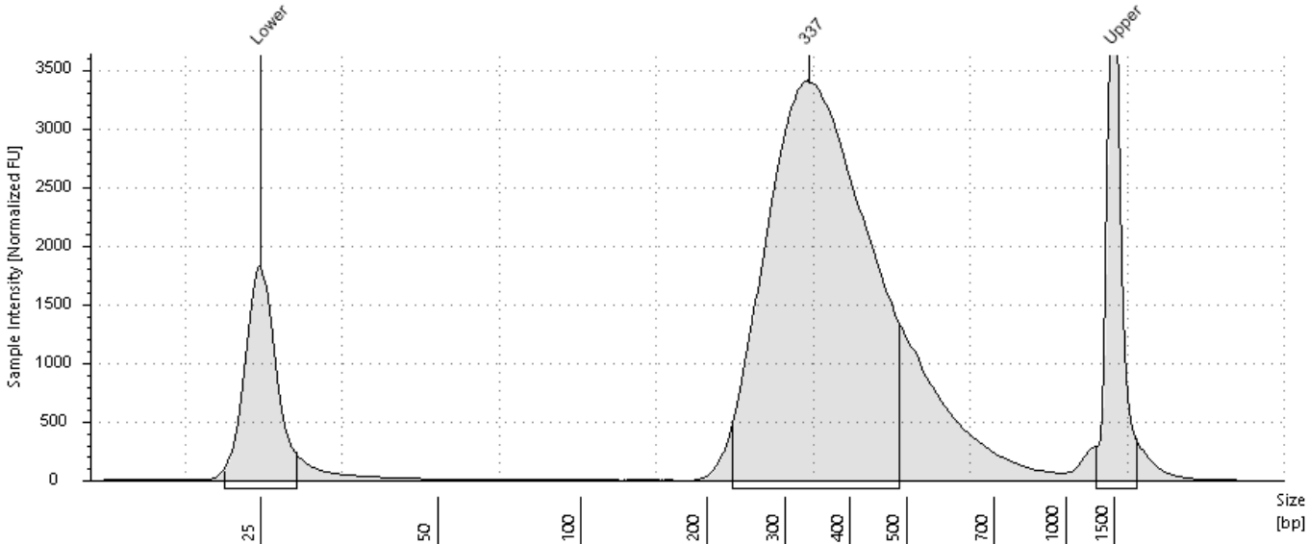

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
F1	33.8	VT-S5-SAM8125	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.60	-	344	-		Lower Marker
337	33.8	-	154	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

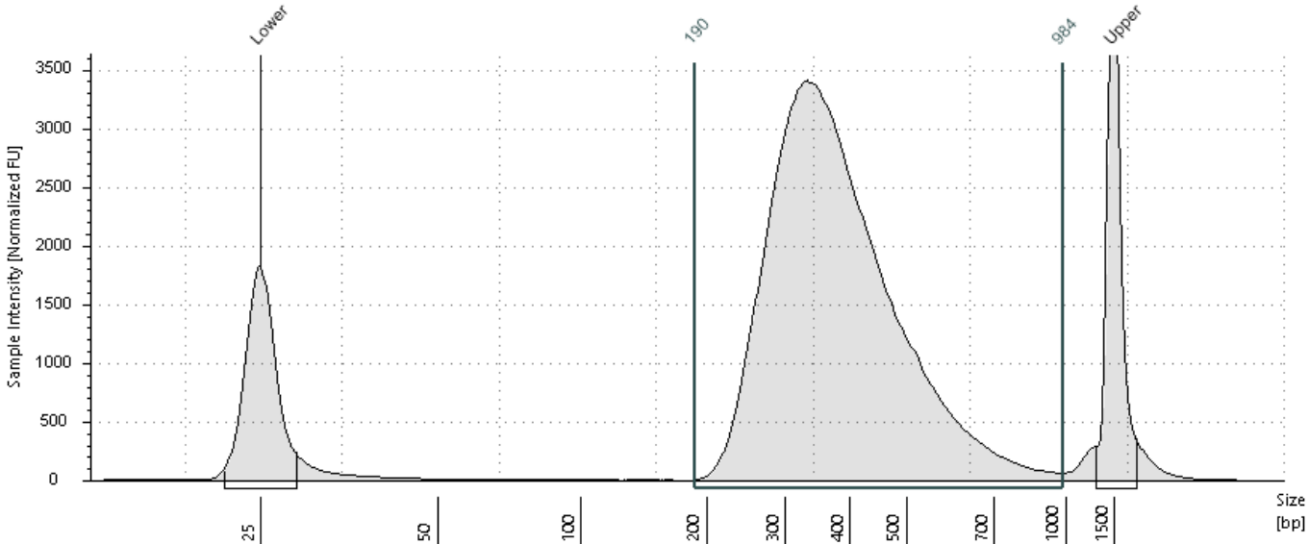

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
190	984	390	40.4	171	96.16		

© Agilent Technologies, Inc. 2023

G1: VT-S6-SAM8126

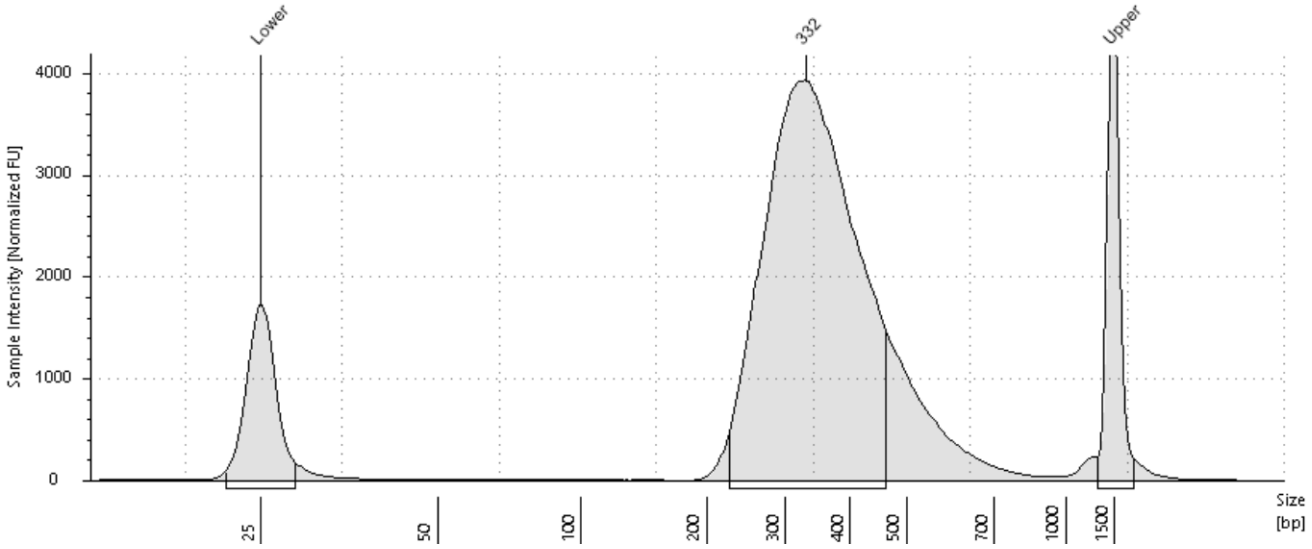

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
G1	38.9	VT-S6-SAM8126	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.52	-	340	-		Lower Marker
332	38.9	-	180	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

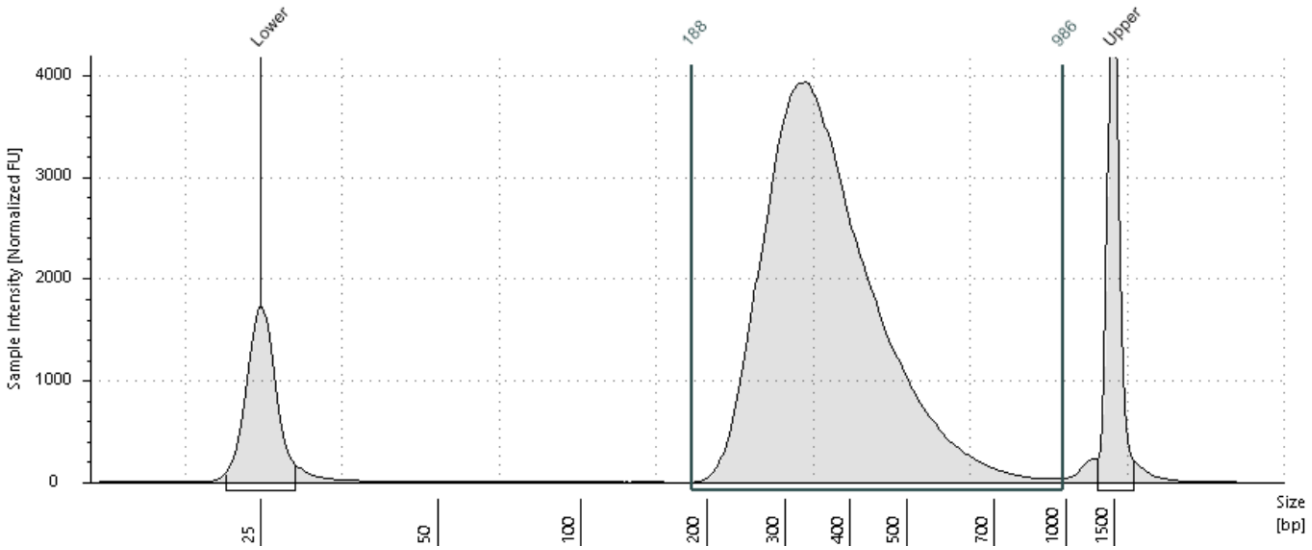

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
188	986	372	45.9	201	97.62		

© Agilent Technologies, Inc. 2023

H1: VT-S7-SAM8127

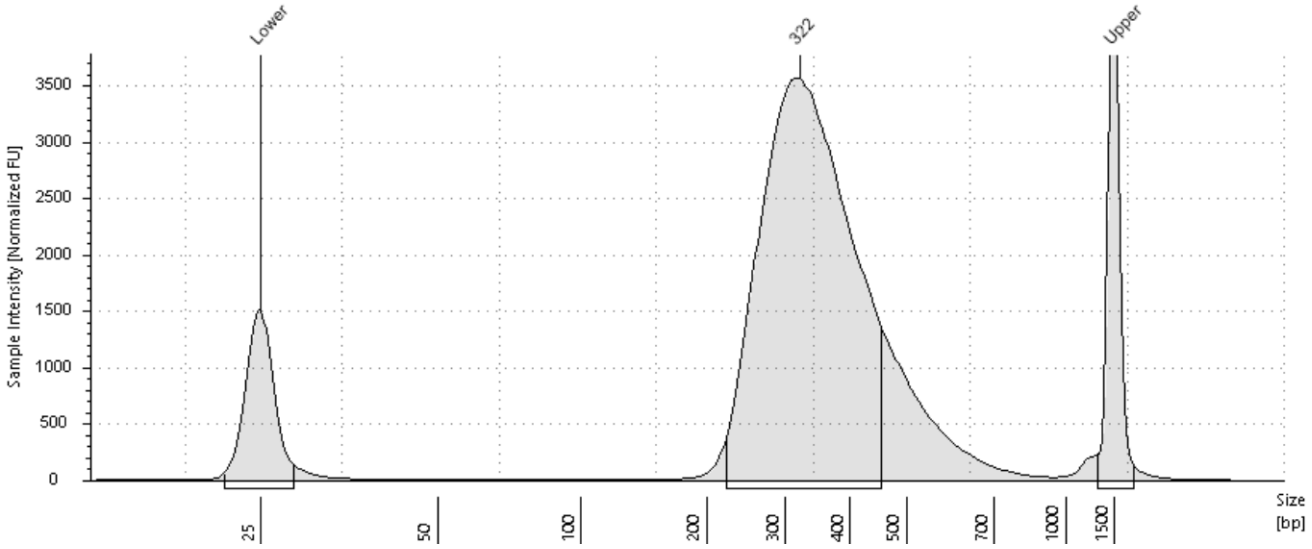

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
H1	37.6	VT-S7-SAM8127	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	4.99	-	307	-		Lower Marker
322	37.6	-	180	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

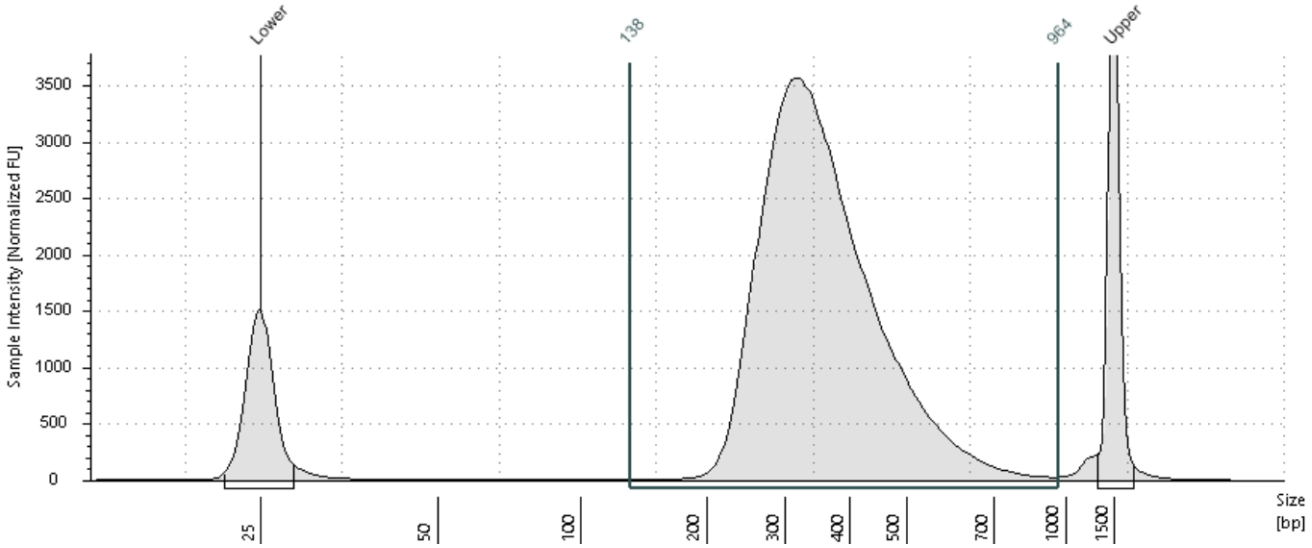

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
138	964	366	44.7	200	98.03		

© Agilent Technologies, Inc. 2023

A2: VT-S7-D-SAM8127D

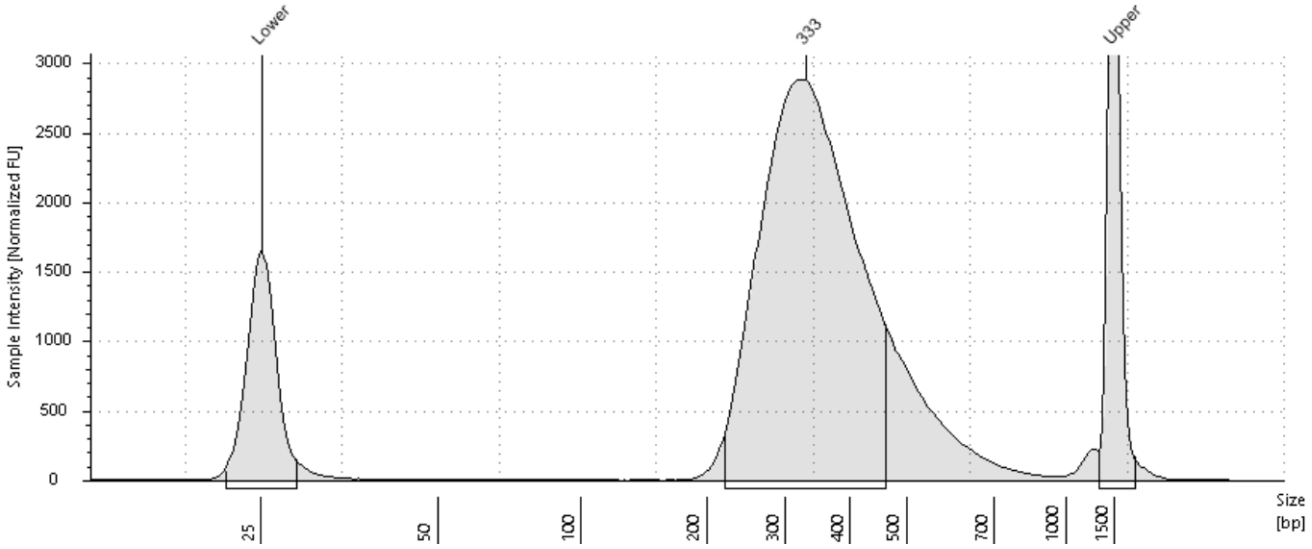

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A2	30.1	VT-S7-D-SAM8127D	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.36	-	330	-		Lower Marker
333	30.1	-	139	100.00		
1500	6.50	6.50	6.67	-		Upper Marker

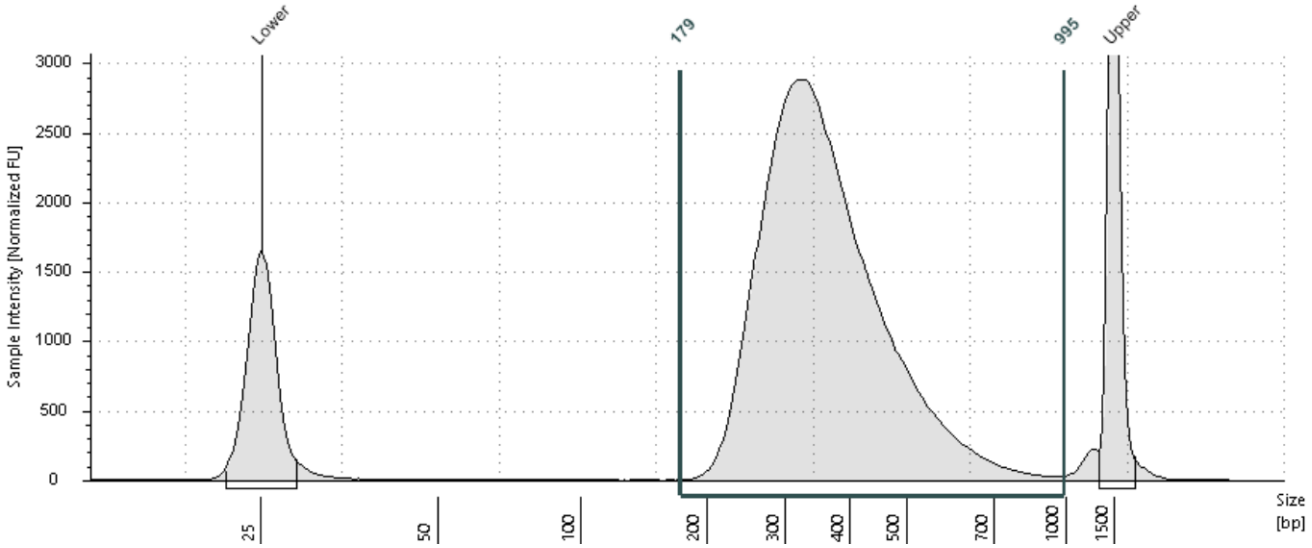

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
179	995	370	35.9	159	97.56		

© Agilent Technologies, Inc. 2023