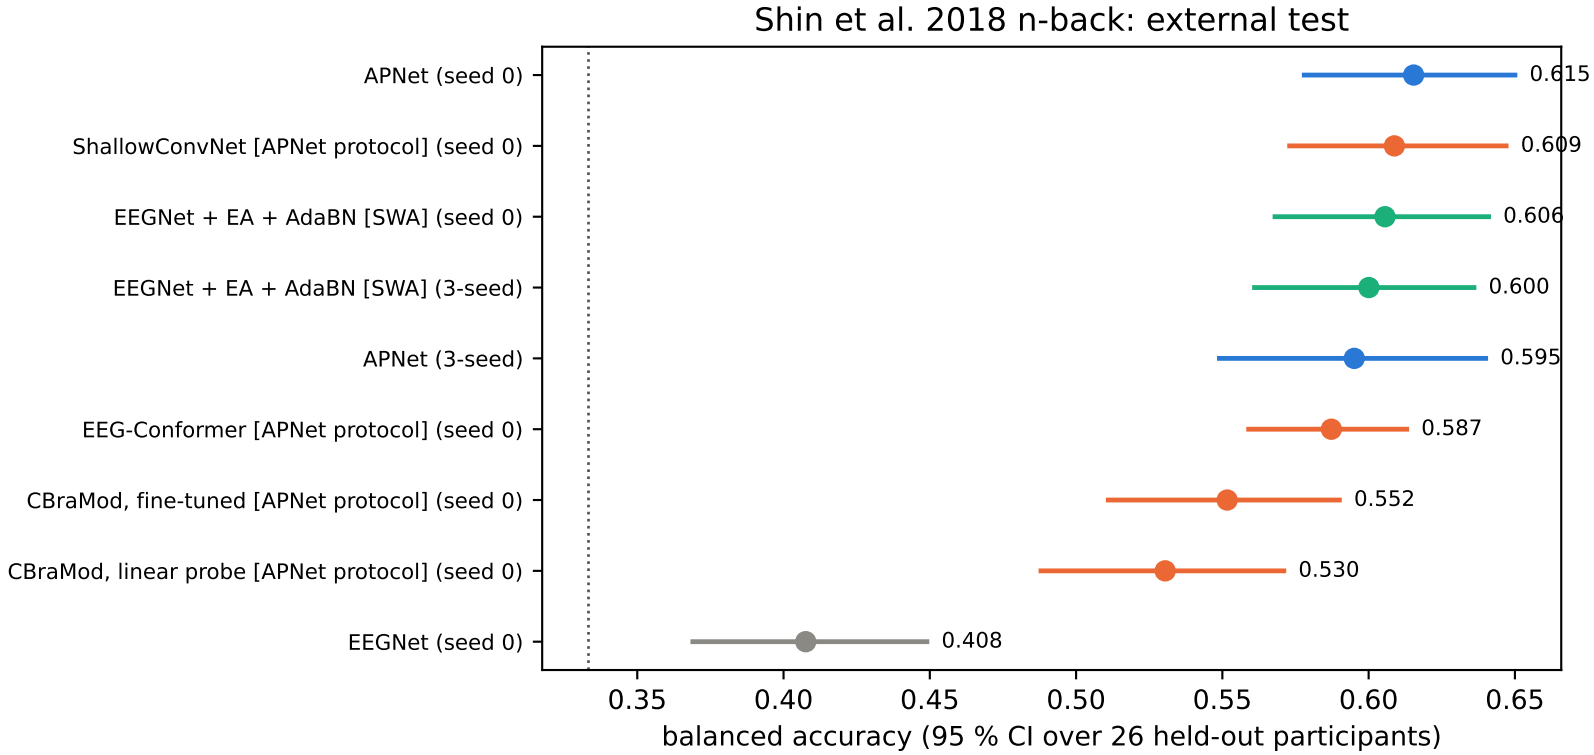
Shin et al. 2018 n-back: external test
APNet (seed 0)
ShallowConvNet [APNet protocol] (seed 0)
EEGNet + EA + AdaBN [SWA] (seed 0)
EEGNet + EA + AdaBN [SWA] (3-seed)
APNet (3-seed)
EEG-Conformer [APNet protocol] (seed 0)
CBraMod, fine-tuned [APNet protocol] (seed 0)
CBraMod, linear probe [APNet protocol] (seed 0)
EEGNet (seed 0)
0.615
0.609
0.606
0.600
0.595
0.587
0.552
0.530
0.408
0.35
0.40
0.45
0.50
0.55
0.60
0.65
balanced accuracy (95 % CI over 26 held-out participants)

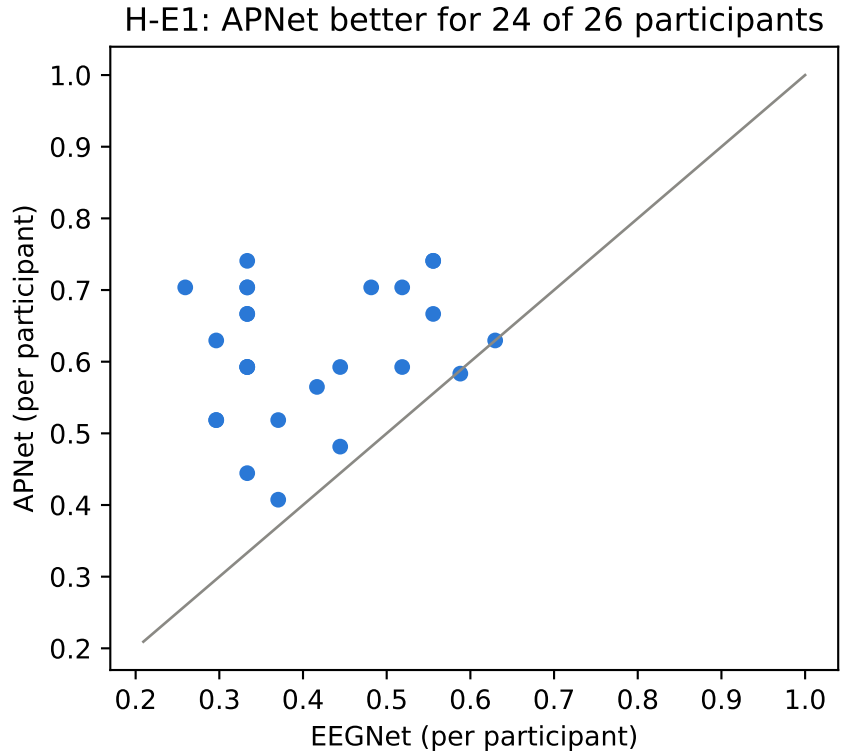
H-E1: APNet better for 24 of 26 participants
APNet (per participant)
EEGNet (per participant)
1.0
0.9
0.8
0.7
0.6
0.5
0.4
0.3
0.2
0.2
0.3
0.4
0.5
0.6
0.7
0.8
0.9
1.0