

Team 10 - Sequence Diagrams

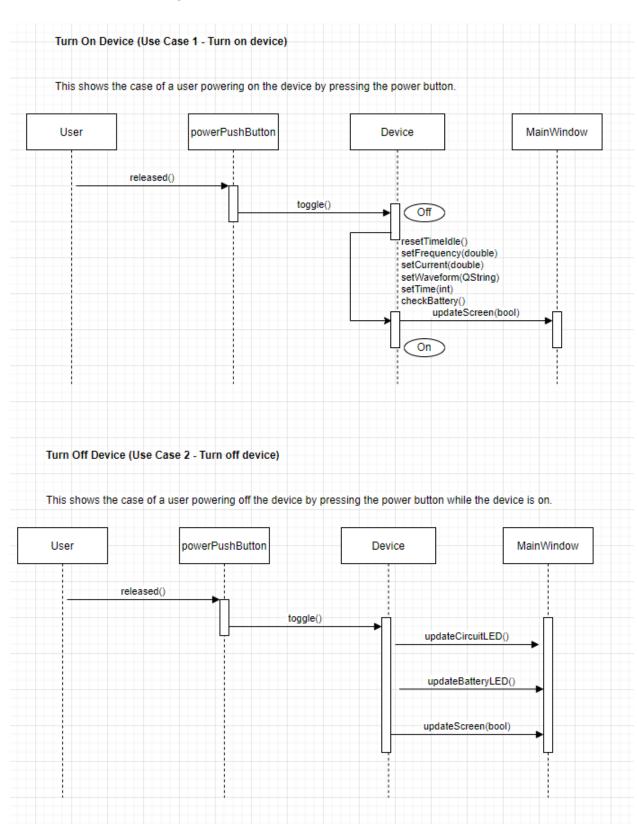


Change Current (Use Case 3 - User change current intensity)

This shows the user changing the device's current intensity/level. In this sequence diagram example, the user presses the up button twice, which incrementing the current by 50 microamperes. Then, the user presses the down button once, decrementing the current by 100 microampere.

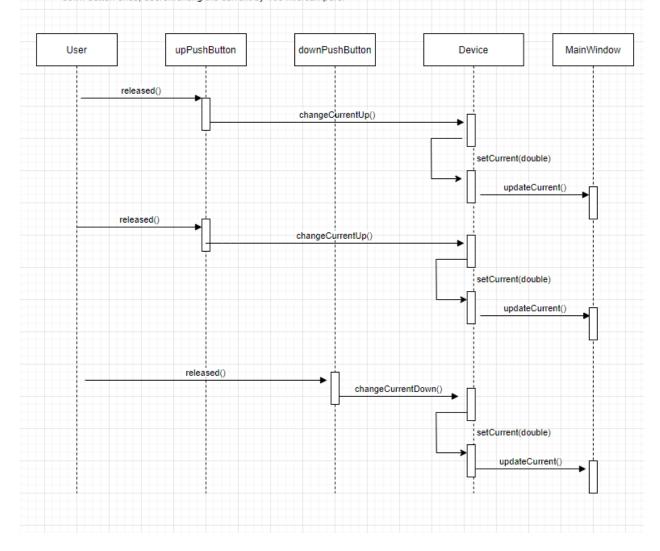


Change Frequency (Use Case 4 - User change frequency)

This shows the user changing the device's frequency level by pressing the frequency button.

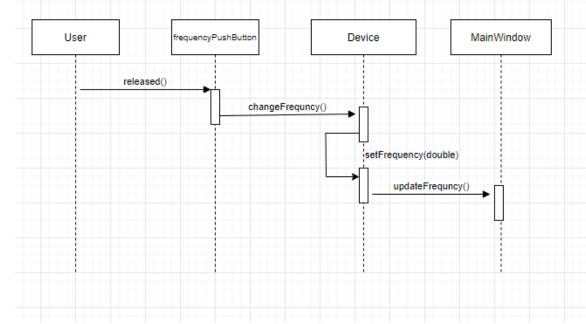


Record Session History (Use Case 5 - Record session history)


This shows a record of the treatment history be saved in memory after a treatment session is complete.

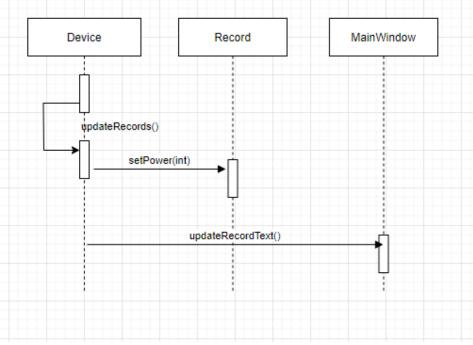


Fault Safety (Use Case 6 - Device Auto-disables itself)

This shows a case where the device exceeds a fault of 700 microamps and automatically disables itself.

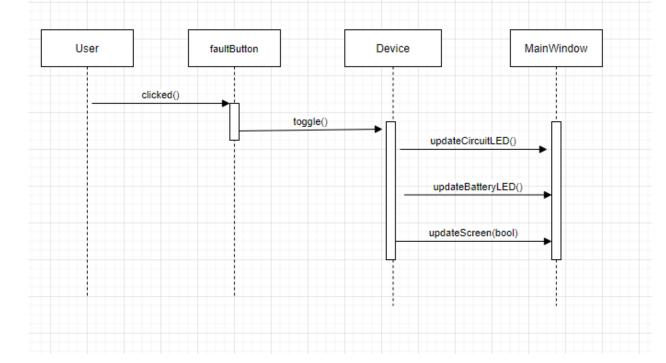

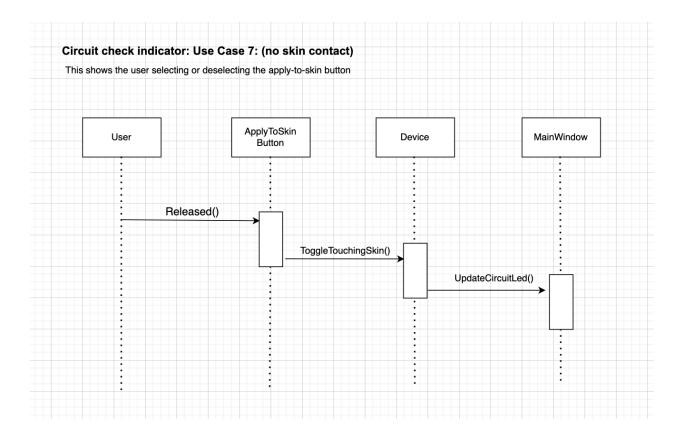

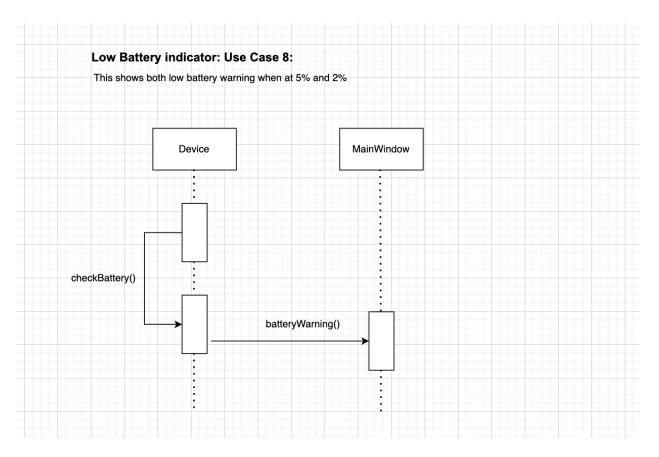

Change Timer (Use Case 10 - User change timer)

This shows the user changing the device's timer by pressing the timer button.

