Dose-volume histogram — Lung_Patient_24

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

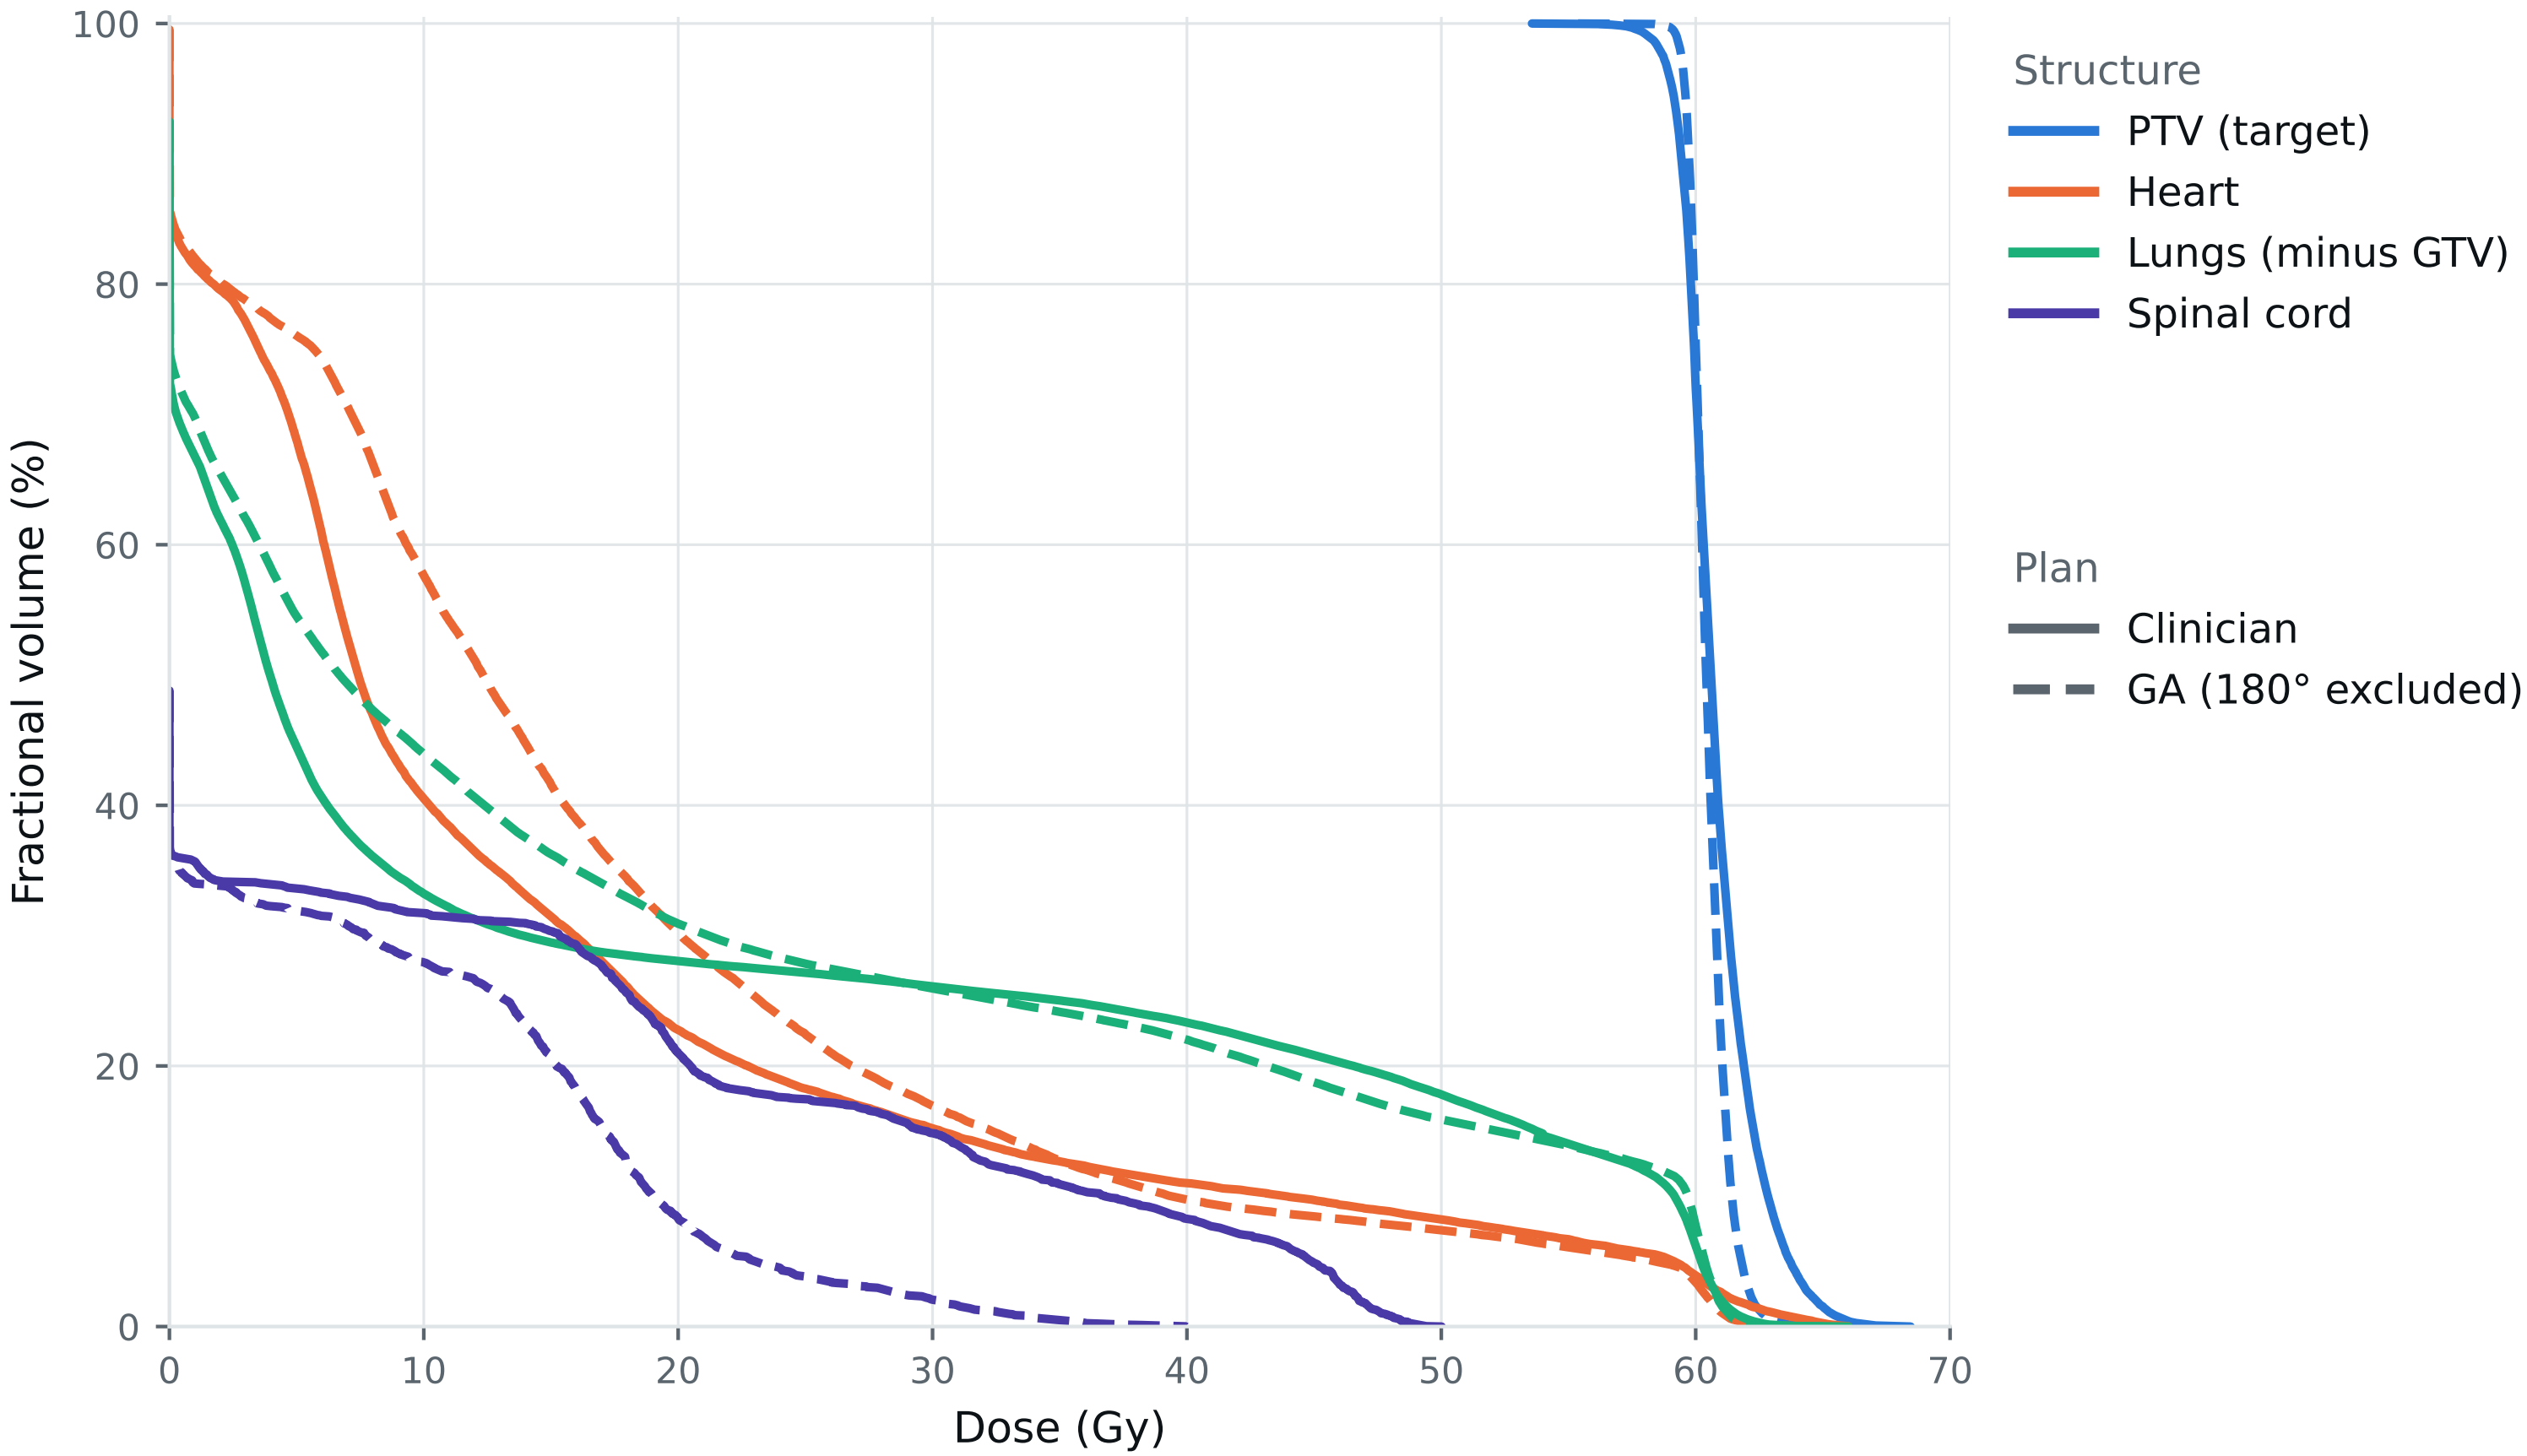

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_24

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

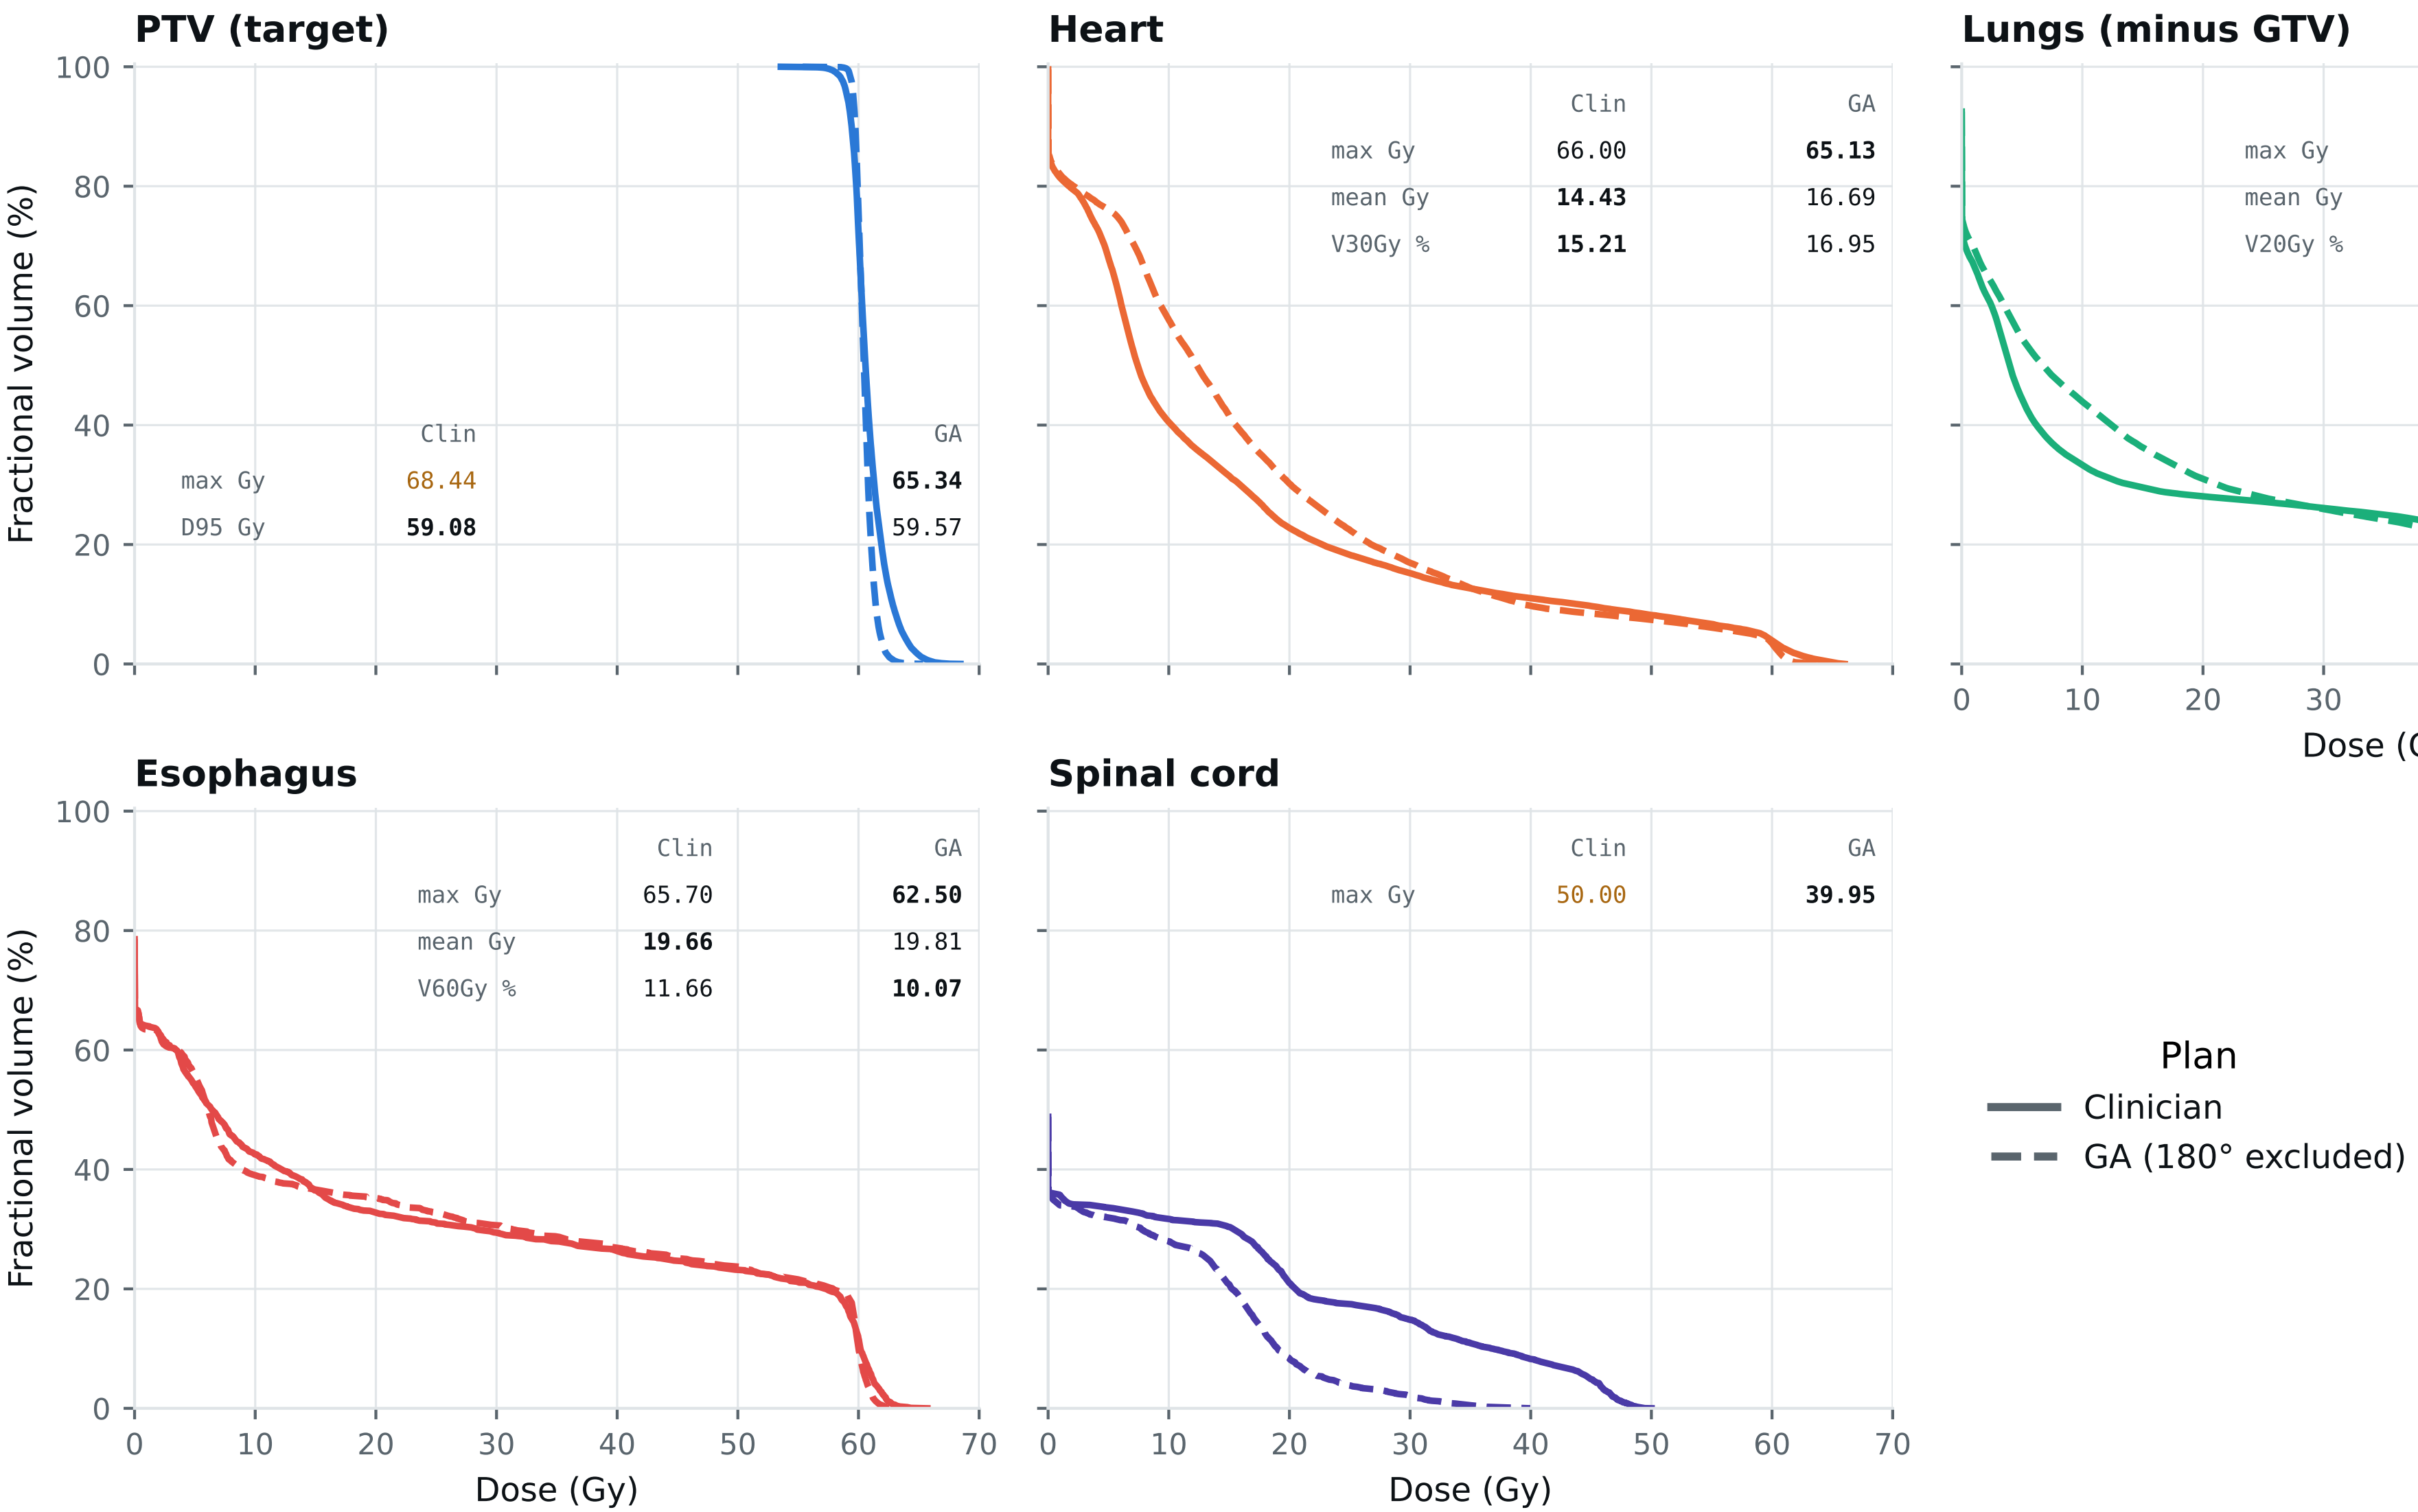

Clinical criteria — Lung_Patient_24

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	68.44	**63.90**	Gy
PTV max	69	66	68.44	**65.34**	Gy
ESOPHAGUS max	66	–	65.70	**62.50**	Gy
ESOPHAGUS mean	34	21	**19.66**	19.81	Gy
ESOPHAGUS V60Gy	17	–	11.66	**10.07**	%
HEART max	66	–	66.00	**65.13**	Gy
HEART mean	27	20	**14.43**	16.69	Gy
HEART V30Gy	50	48	**15.21**	16.95	%
LUNG_L max	66	–	**33.52**	43.85	Gy
LUNG_R max	66	–	66.00	**65.10**	Gy
CORD max	50	48	50.00	**39.95**	Gy
SKIN max	60	–	47.32	**45.79**	Gy
LUNGS_NOT_GTV max	66	–	66.00	**65.10**	Gy
LUNGS_NOT_GTV mean	21	20	**16.52**	17.81	Gy
LUNGS_NOT_GTV V20Gy	37	–	**28.07**	30.92	%
PTV D95 (target coverage)			59.08	59.57	
Objective value (search signal)			167.76	119.62	
MOSEK solve time			60 s	53 s	

Beam angles (gantry°)		
	Clinician	0°, 340°, 315°, 295°, 235°, 210°, 185°
	GA	235°, 185°, 30°, 75°, 90°, 300°, 345°

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_24_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.