Dose-volume histogram — Lung_Patient_36

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

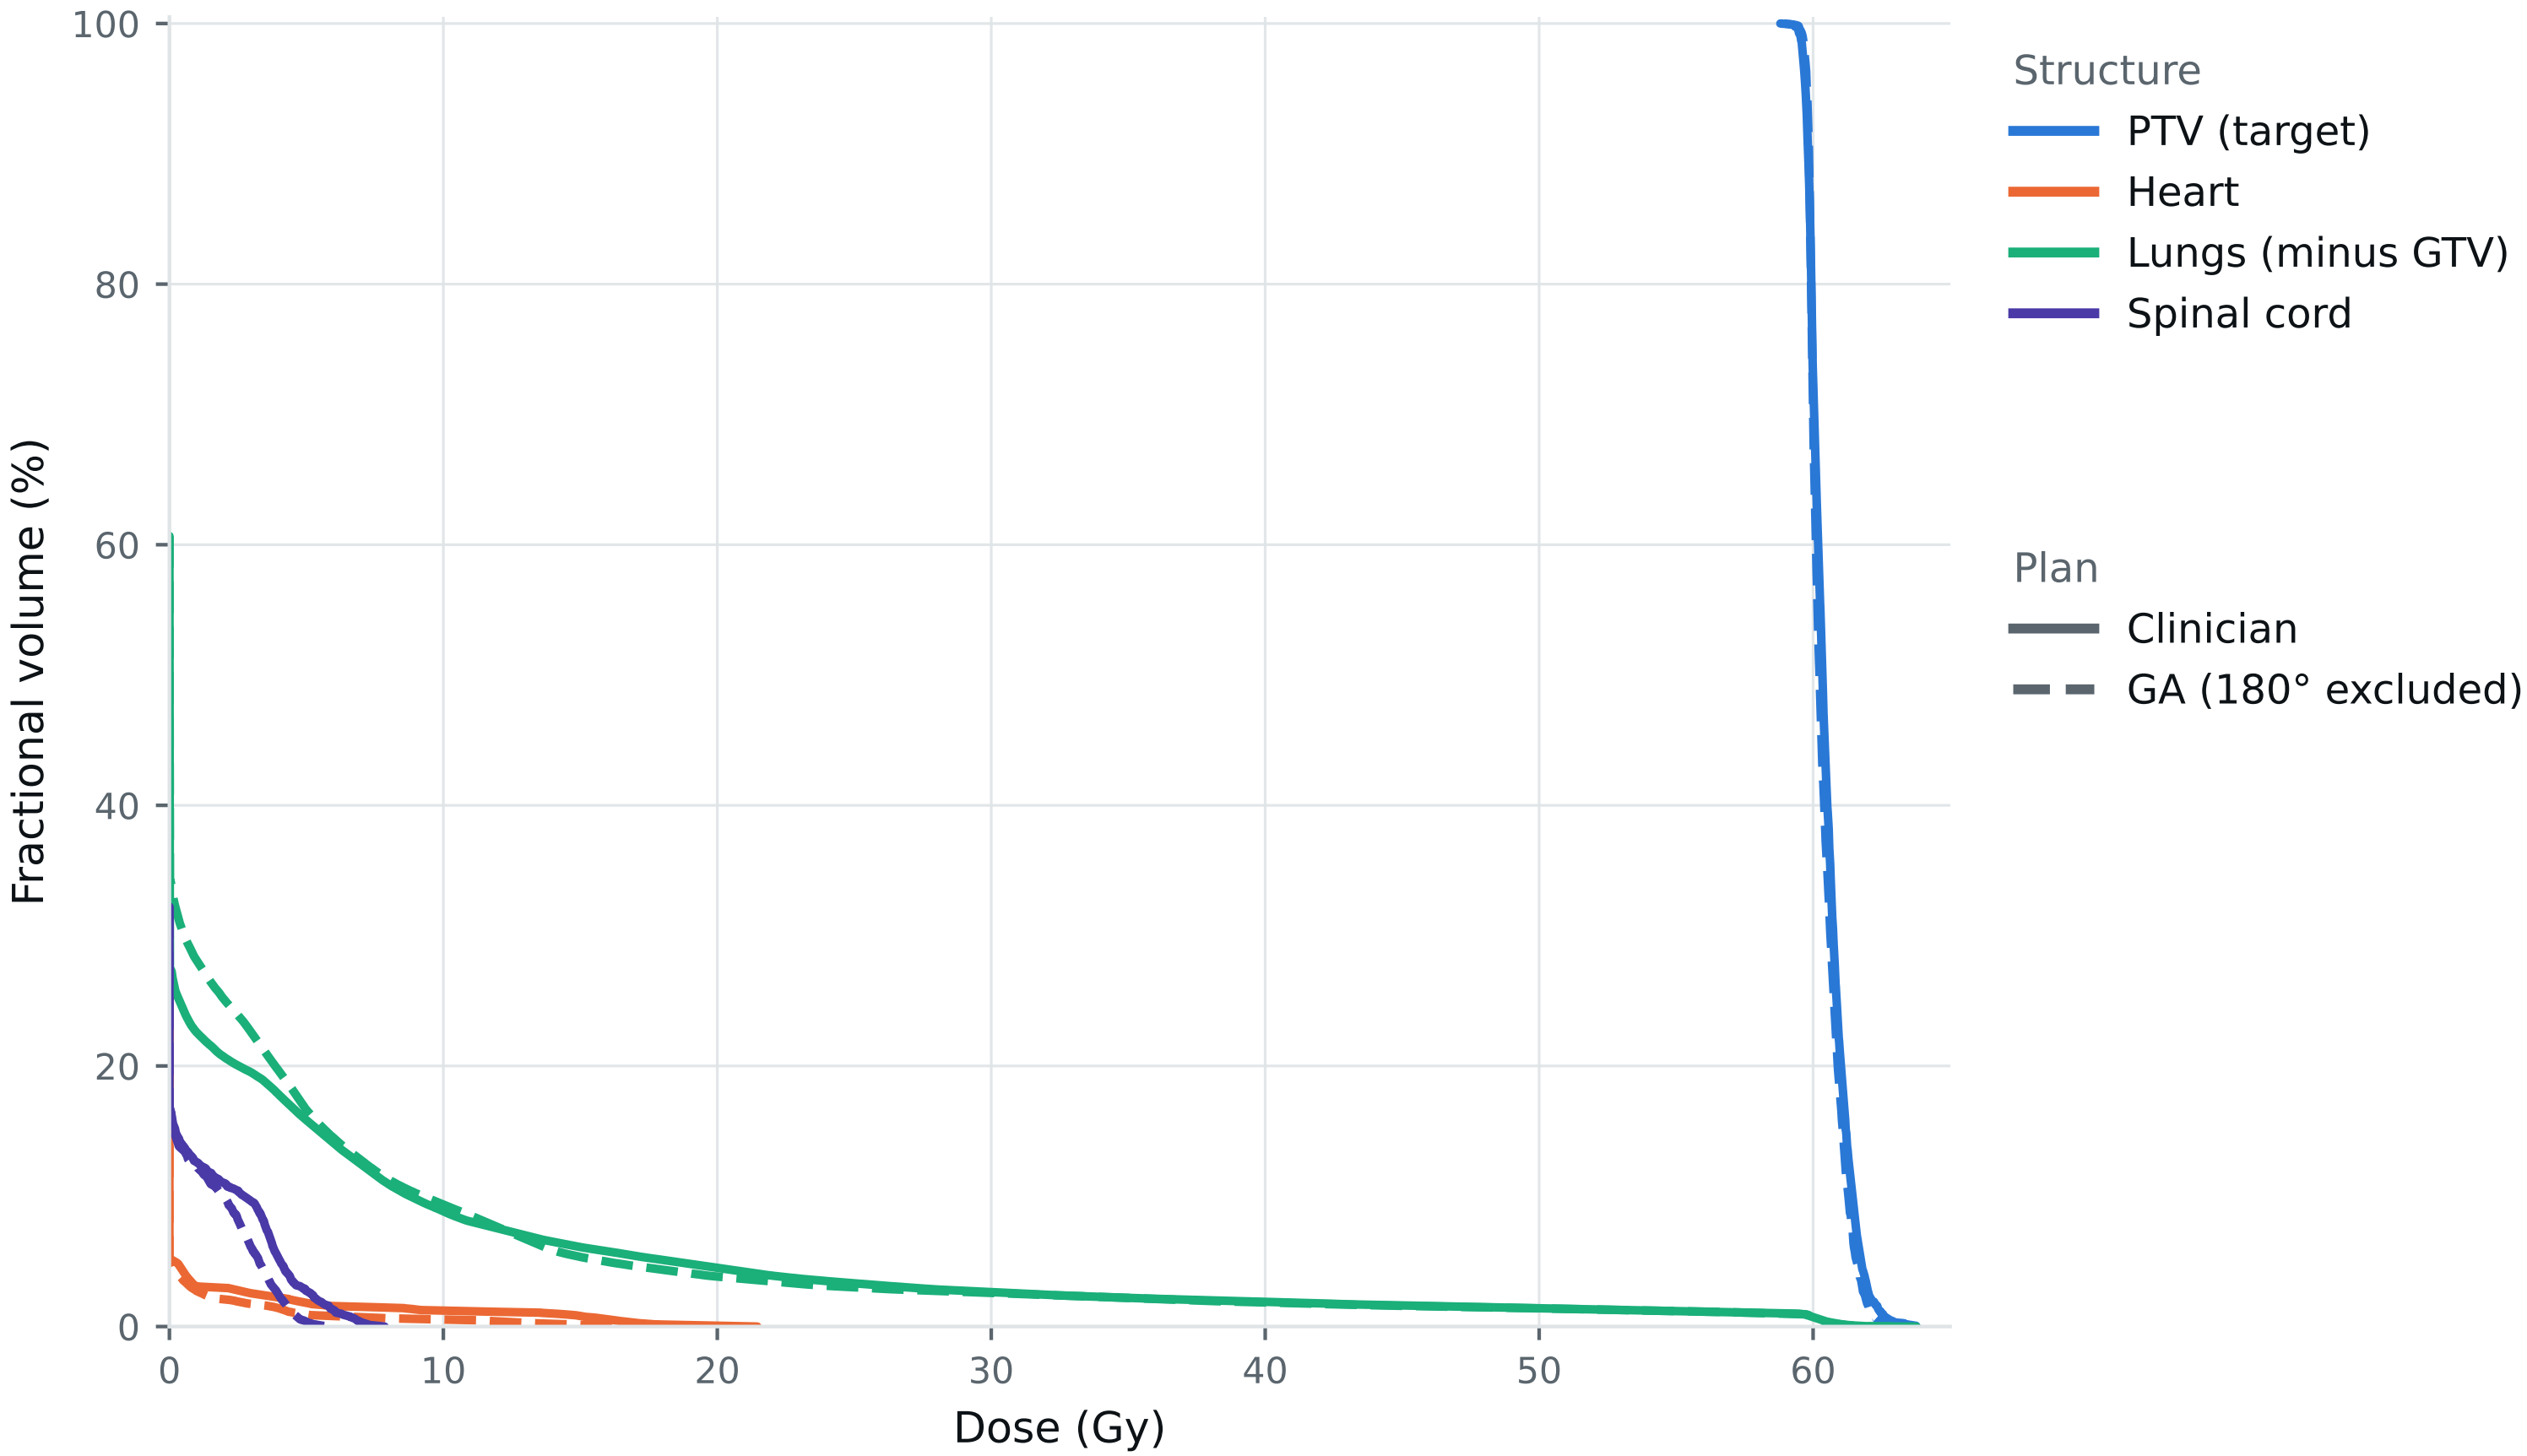

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_36

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

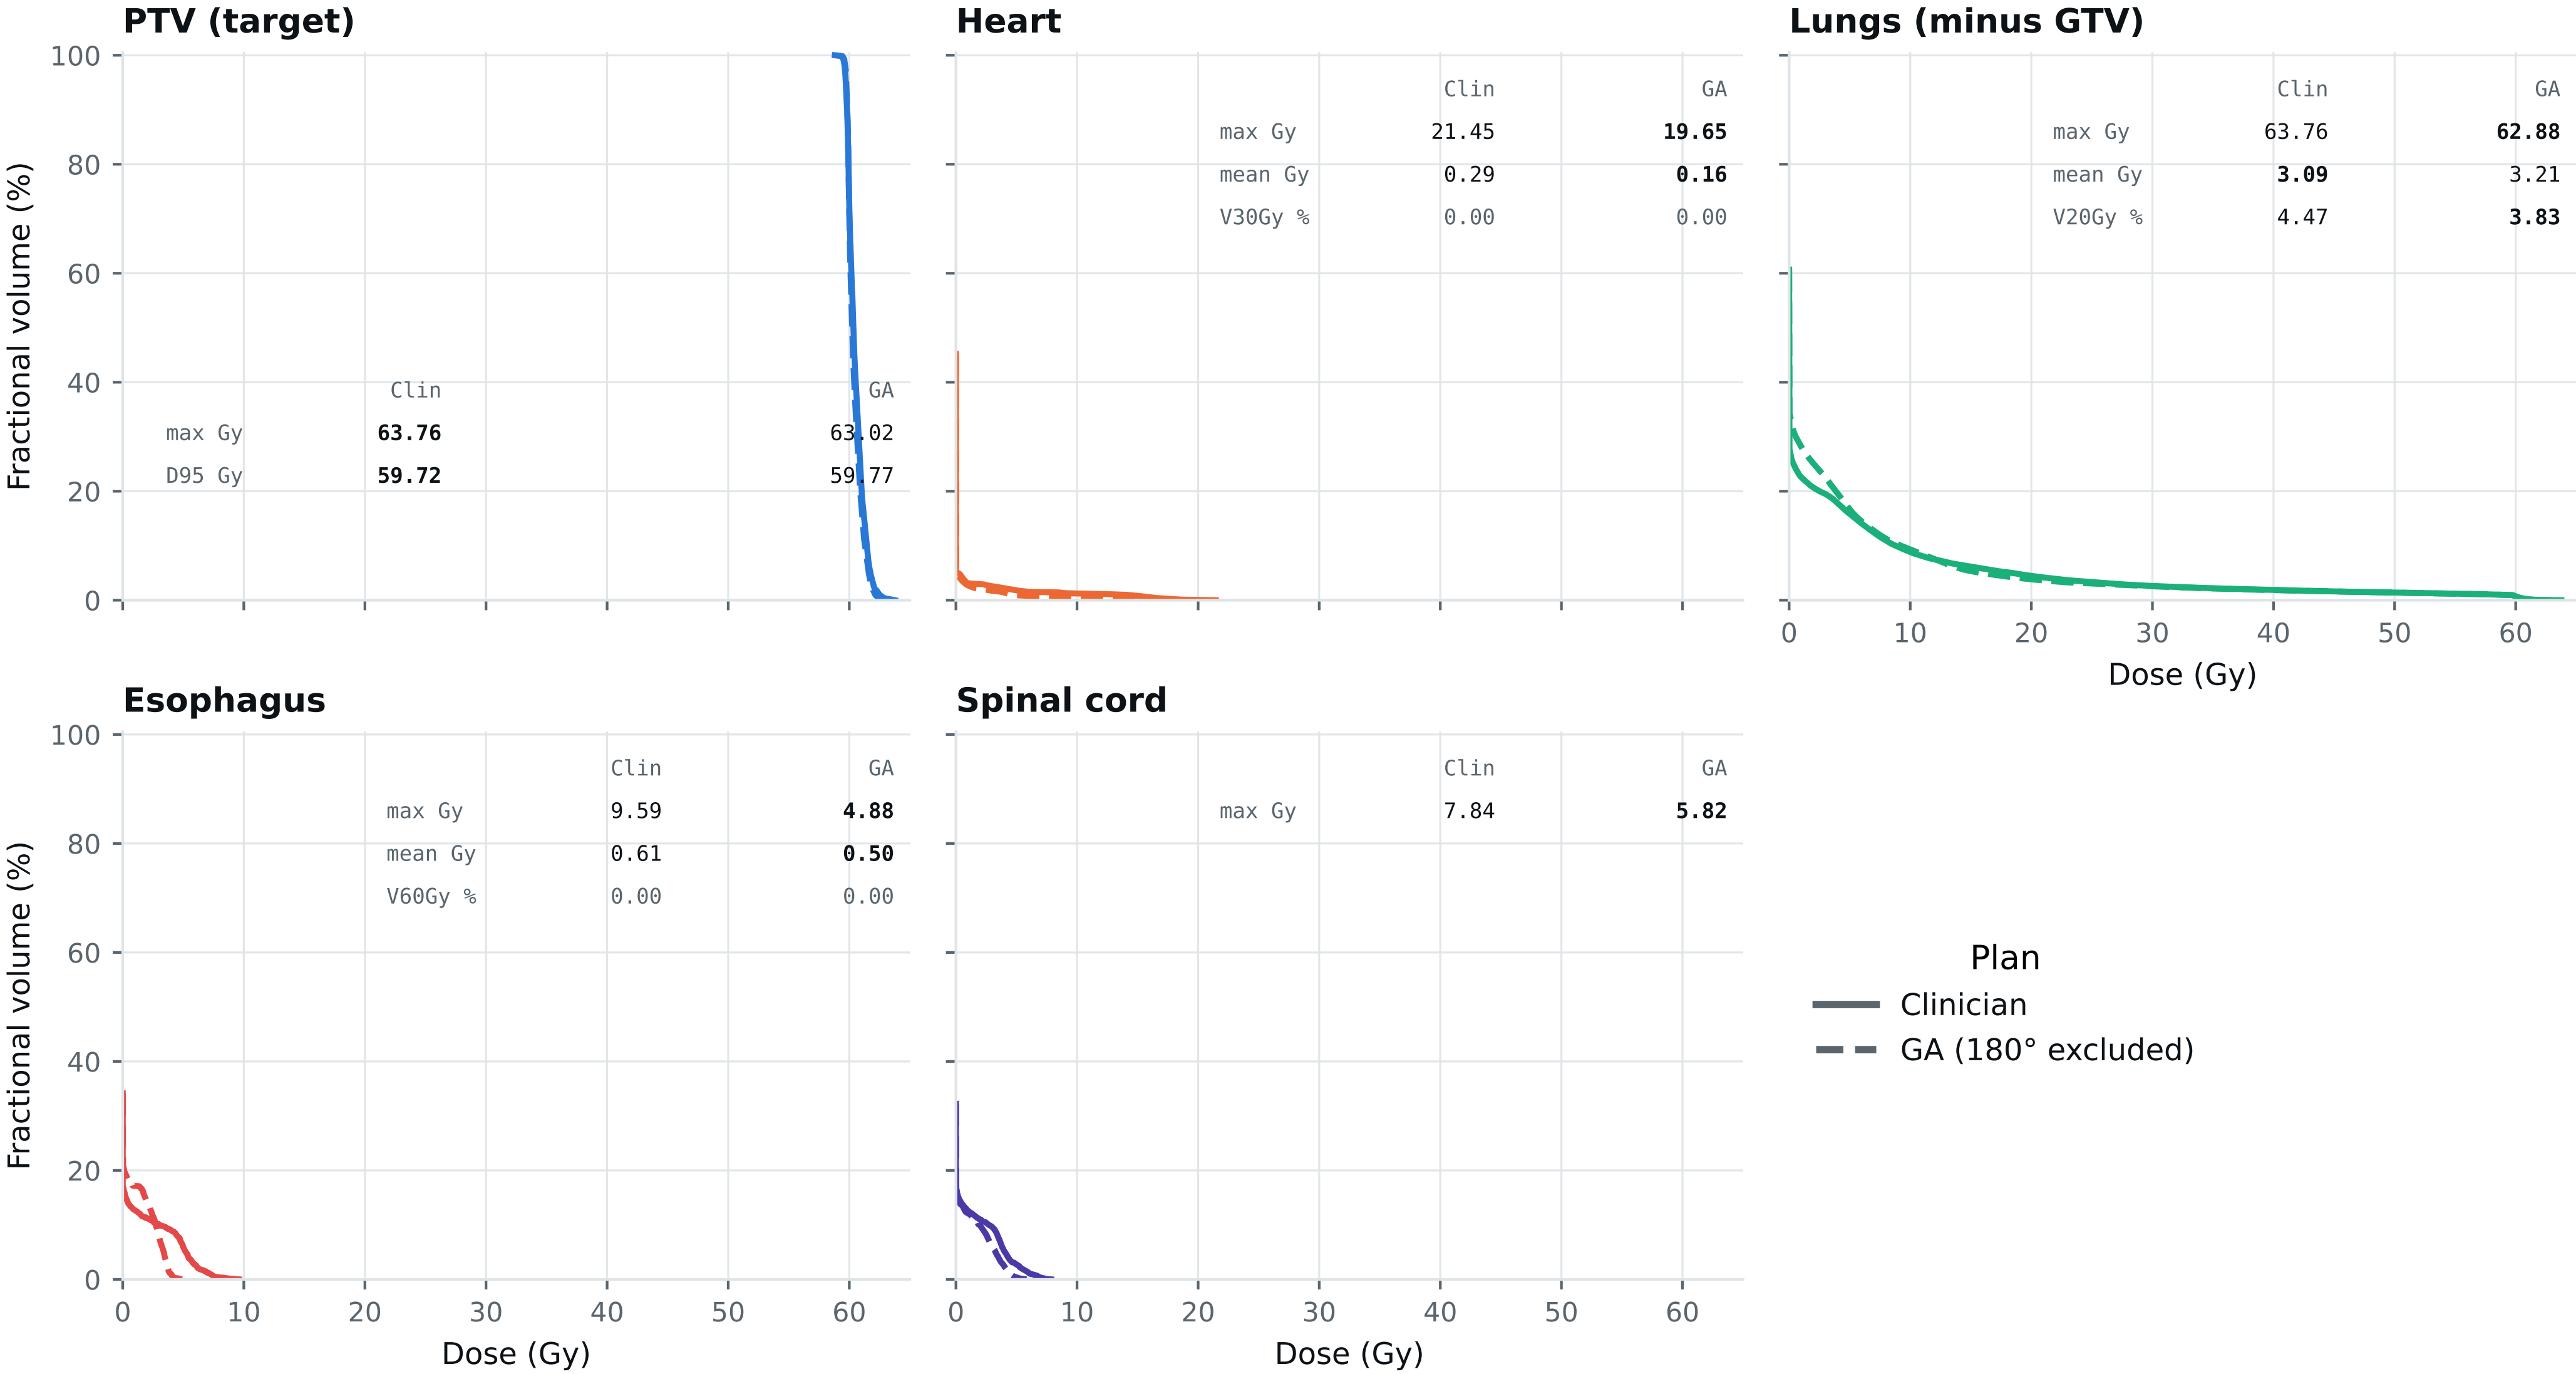

Clinical criteria — Lung_Patient_36

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	**62.76**	63.02	Gy
PTV max	69	66	**63.76**	63.02	Gy
ESOPHAGUS max	66	–	9.59	**4.88**	Gy
ESOPHAGUS mean	34	21	0.61	**0.50**	Gy
ESOPHAGUS V60Gy	17	–	0.00	0.00	%
HEART max	66	–	21.45	**19.65**	Gy
HEART mean	27	20	0.29	**0.16**	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	–	63.76	**63.02**	Gy
LUNG_R max	66	–	**15.81**	21.56	Gy
CORD max	50	48	7.84	**5.82**	Gy
SKIN max	60	–	**44.46**	46.24	Gy
LUNGS_NOT_GTV max	66	–	63.76	**62.88**	Gy
LUNGS_NOT_GTV mean	21	20	**3.09**	3.21	Gy
LUNGS_NOT_GTV V20Gy	37	–	4.47	**3.83**	%
PTV D95 (target coverage)			59.72	59.77	
Objective value (search signal)			38.98	35.49	
MOSEK solve time			7 s	9 s	

```
Beam angles (gantry°)   Clinician  175°, 120°, 60°, 30°, 0°, 330°
                        GA         120°, 330°, 15°, 45°, 75°, 90°, 195°
```

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_36_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.