Dose-volume histogram — Lung_Patient_26

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

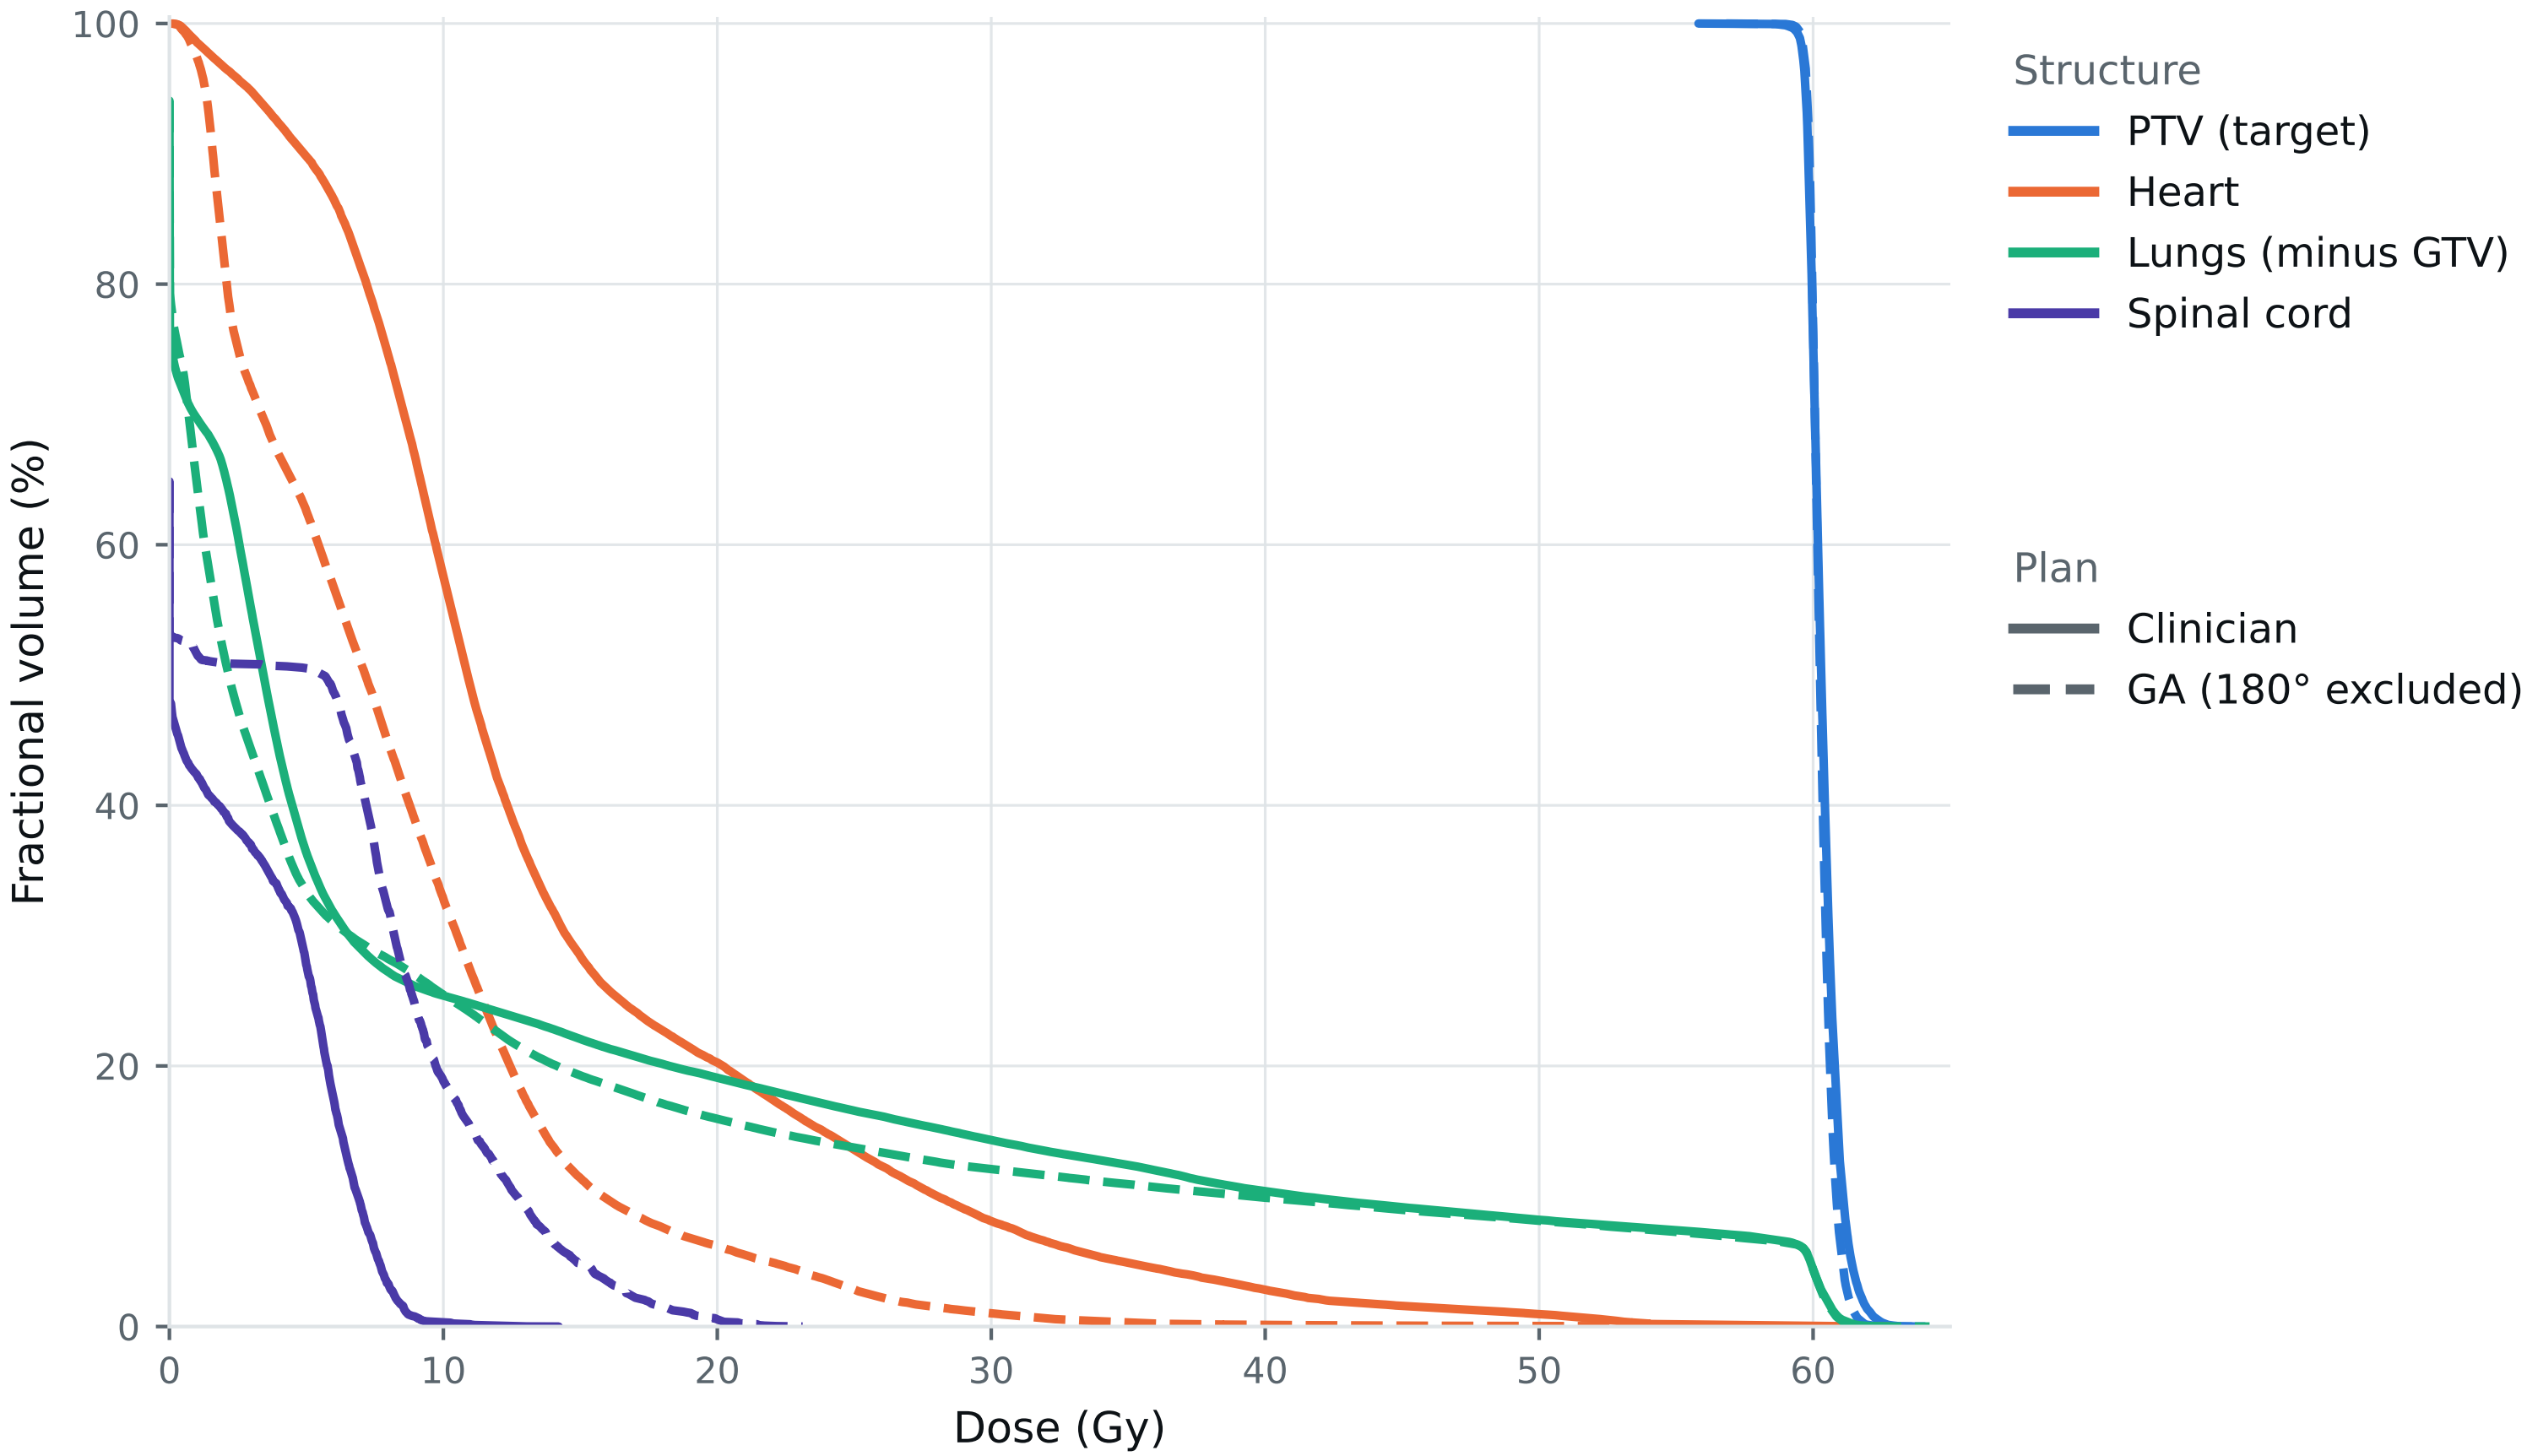

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_26

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

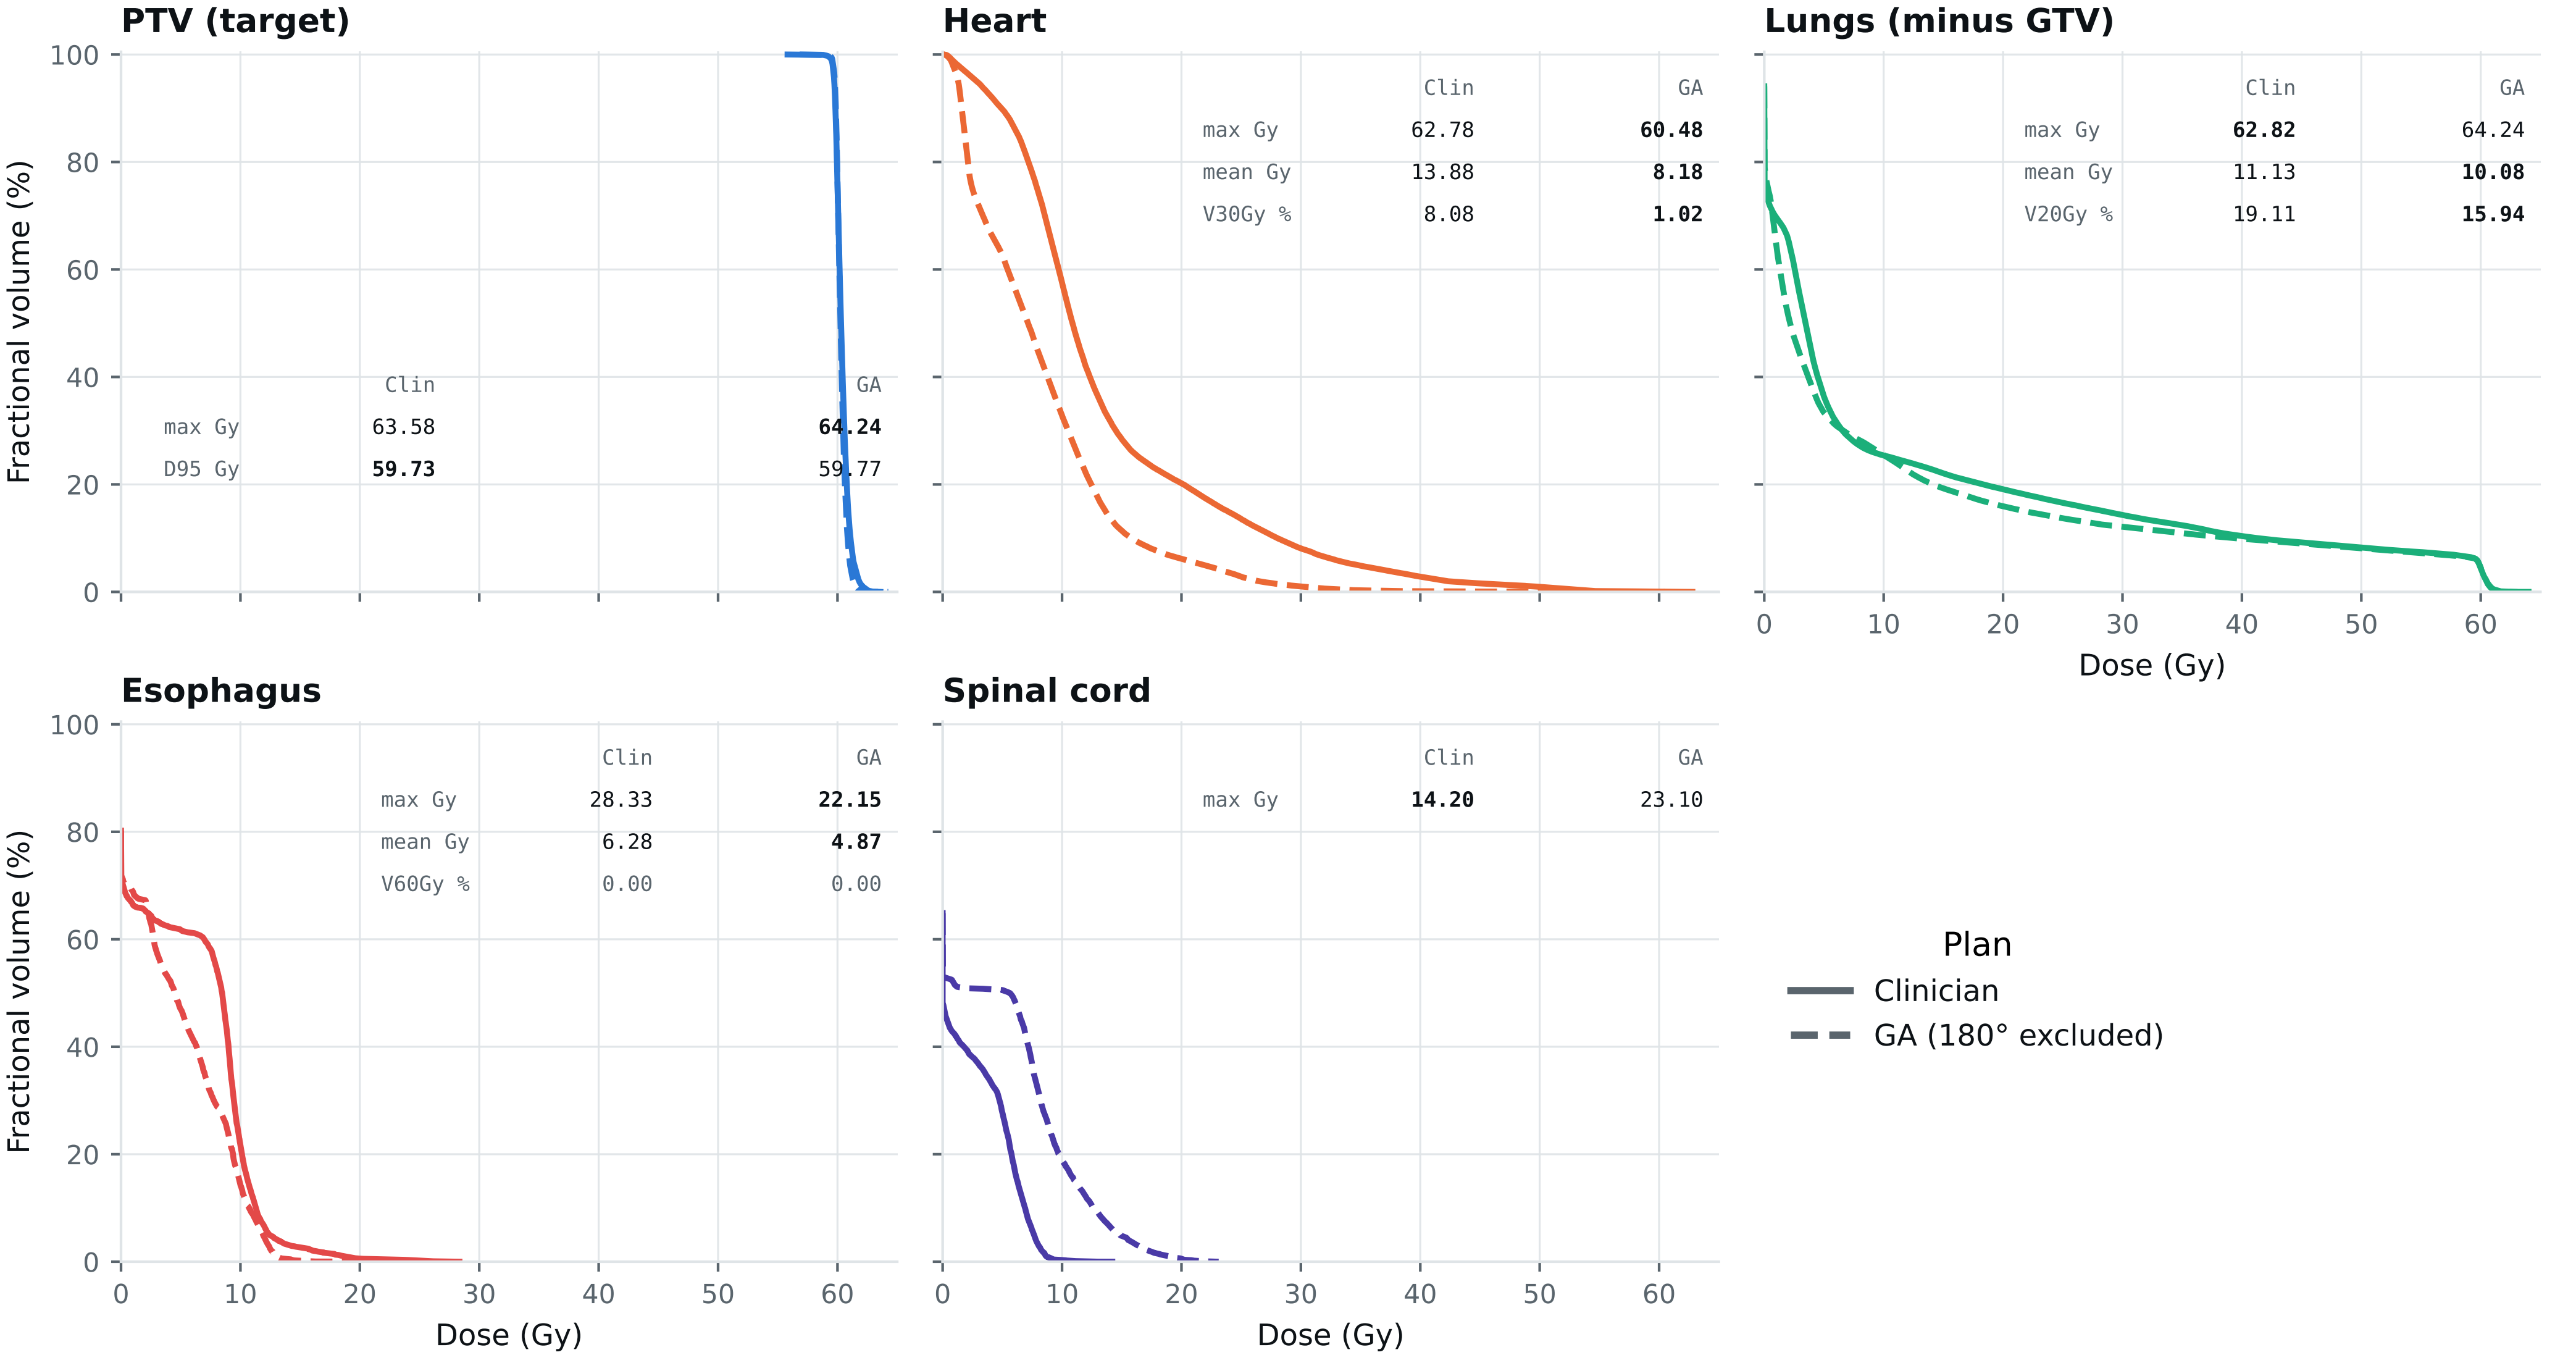

Clinical criteria — Lung_Patient_26

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	63.40	**61.89**	Gy
PTV max	69	66	63.58	**64.24**	Gy
ESOPHAGUS max	66	–	28.33	**22.15**	Gy
ESOPHAGUS mean	34	21	6.28	**4.87**	Gy
ESOPHAGUS V60Gy	17	–	0.00	0.00	%
HEART max	66	–	62.78	**60.48**	Gy
HEART mean	27	20	13.88	**8.18**	Gy
HEART V30Gy	50	48	8.08	**1.02**	%
LUNG_L max	66	–	**62.82**	64.24	Gy
LUNG_R max	66	–	**11.72**	23.34	Gy
CORD max	50	48	**14.20**	23.10	Gy
SKIN max	60	–	60.00	60.00	Gy
LUNGS_NOT_GTV max	66	–	**62.82**	64.24	Gy
LUNGS_NOT_GTV mean	21	20	11.13	**10.08**	Gy
LUNGS_NOT_GTV V20Gy	37	–	19.11	**15.94**	%
PTV D95 (target coverage)			59.73	59.77	
Objective value (search signal)			67.18	57.39	
MOSEK solve time			53 s	50 s	

```
Beam angles (gantry°)   Clinician  175°, 150°, 120°, 45°, 20°, 0°, 210°
                        GA         175°, 60°, 90°, 135°, 195°, 225°, 255°
```

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_26_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.