Dose-volume histogram — Lung_Patient_4

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

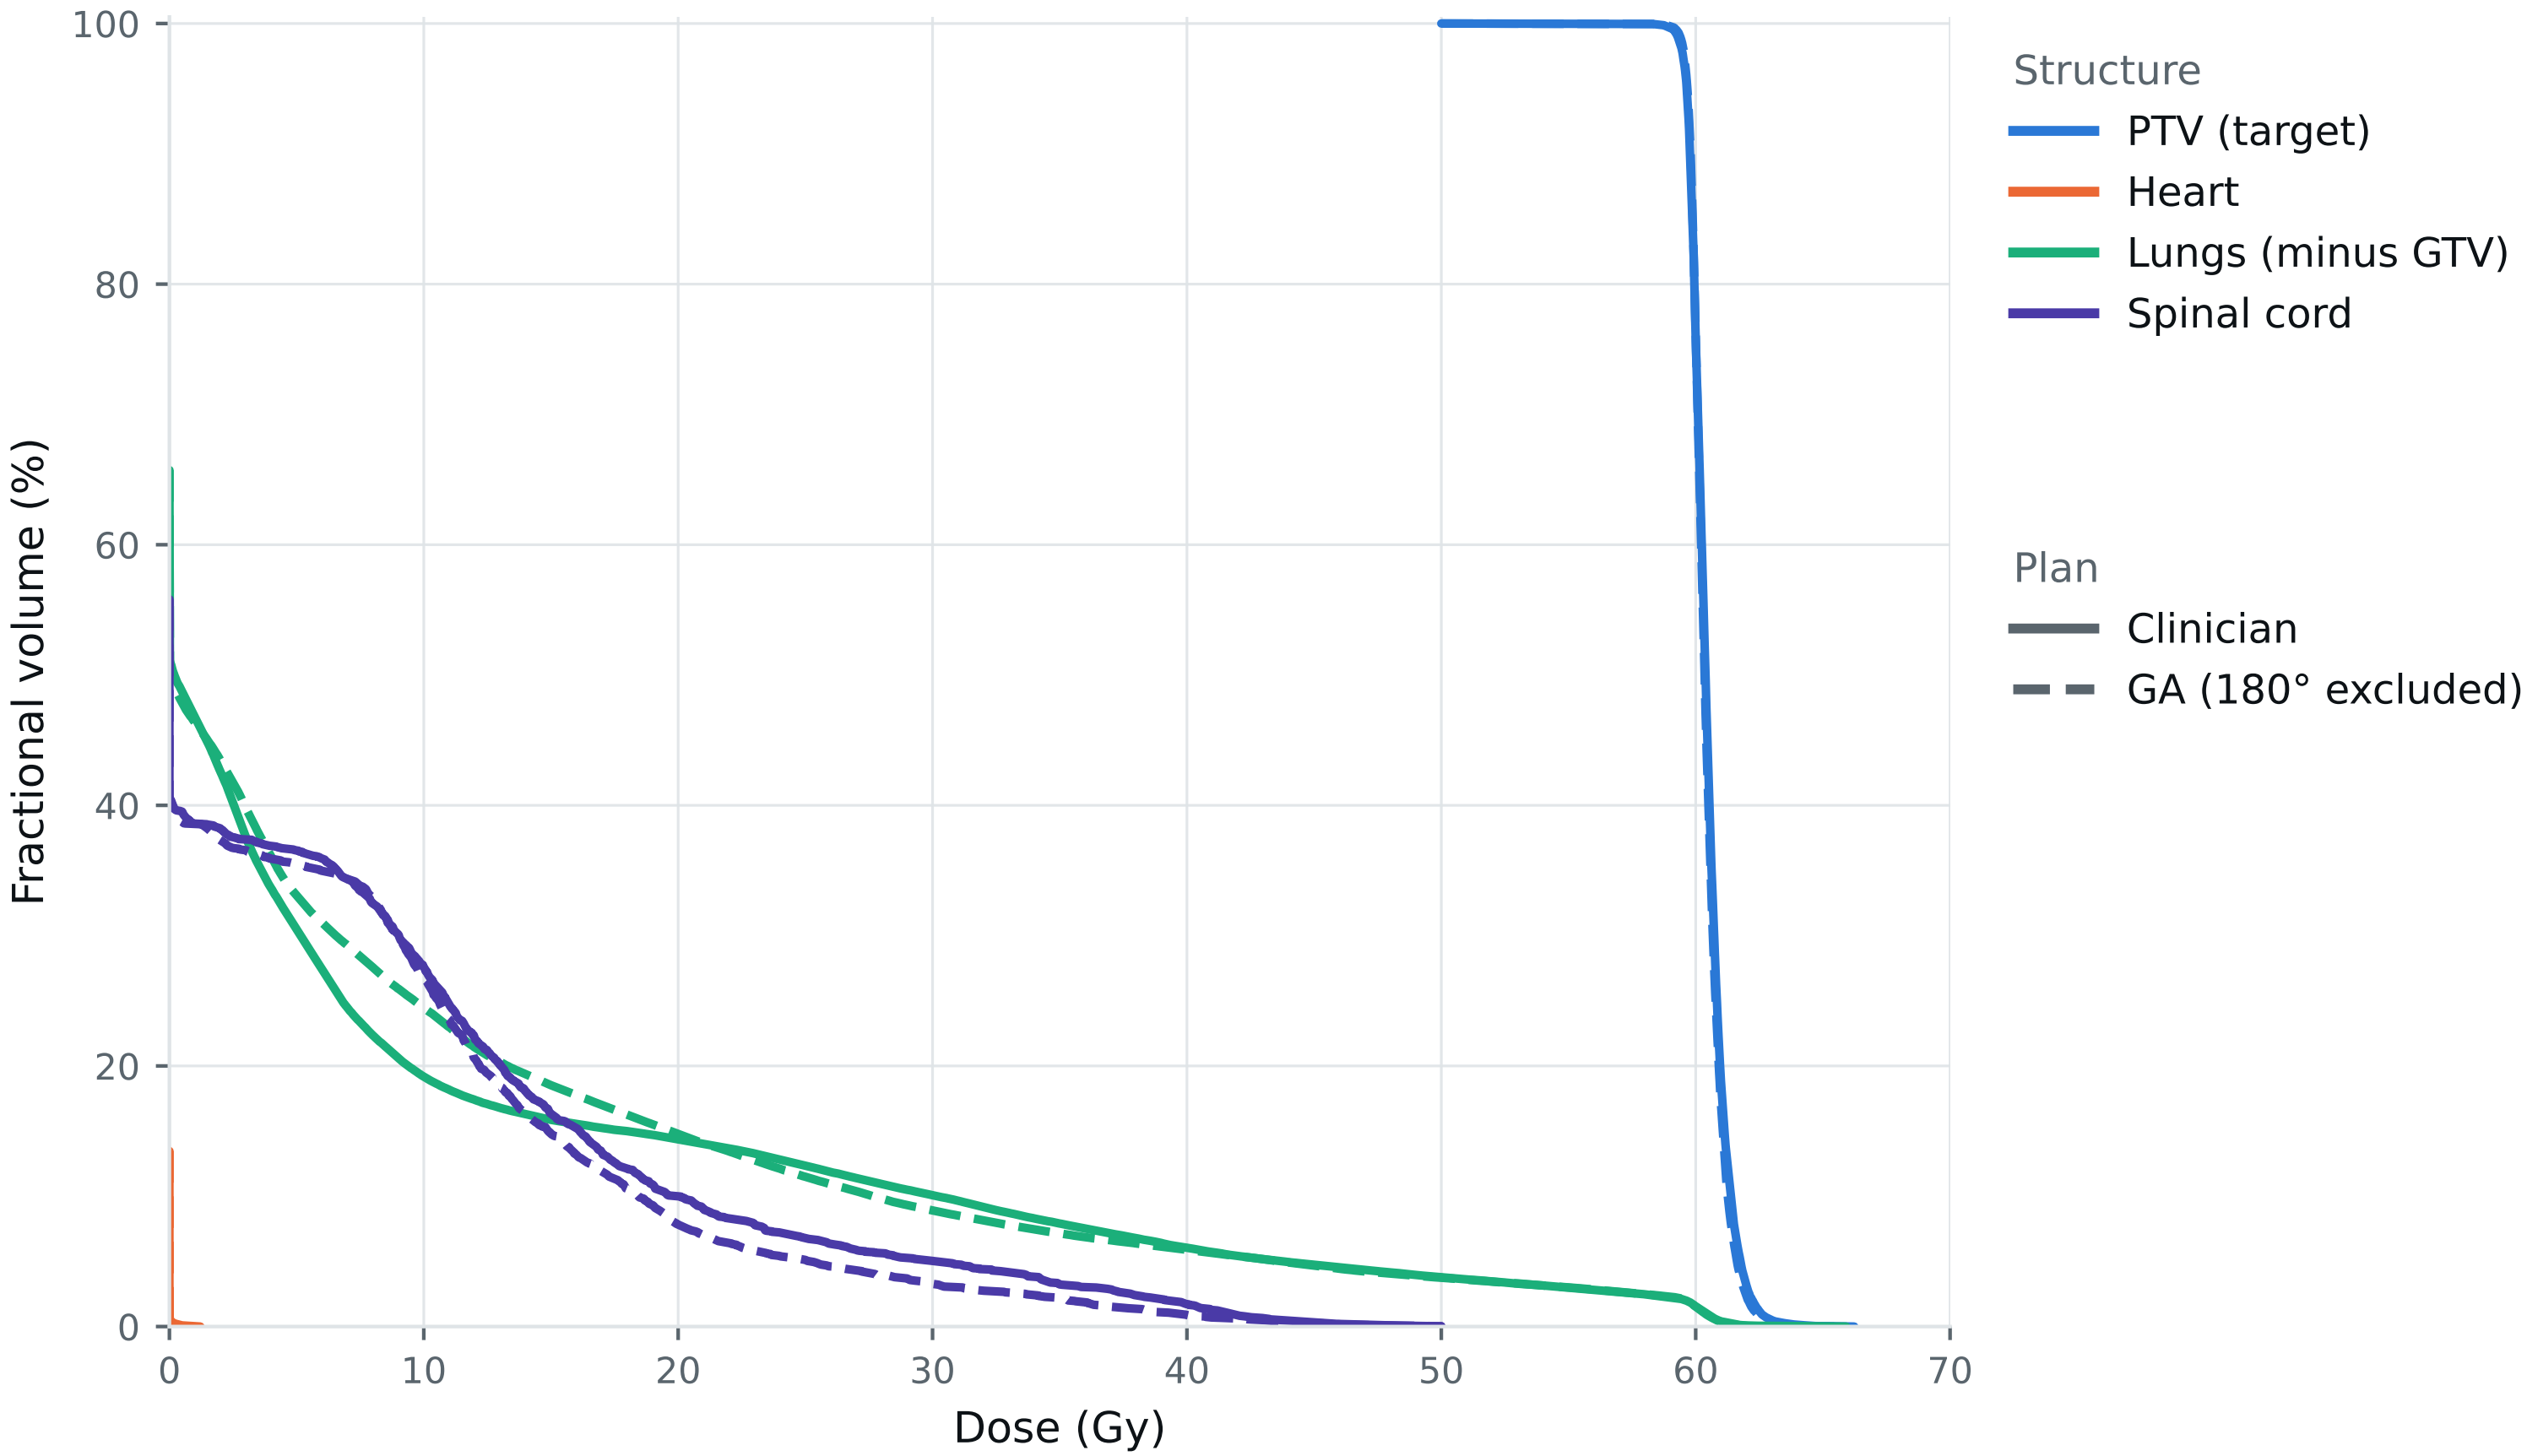

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_4

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = best plan; grey = all plans are within 0.01 of each other, so the row carries no signal. Amber misses a goal, red exceeds a limit.

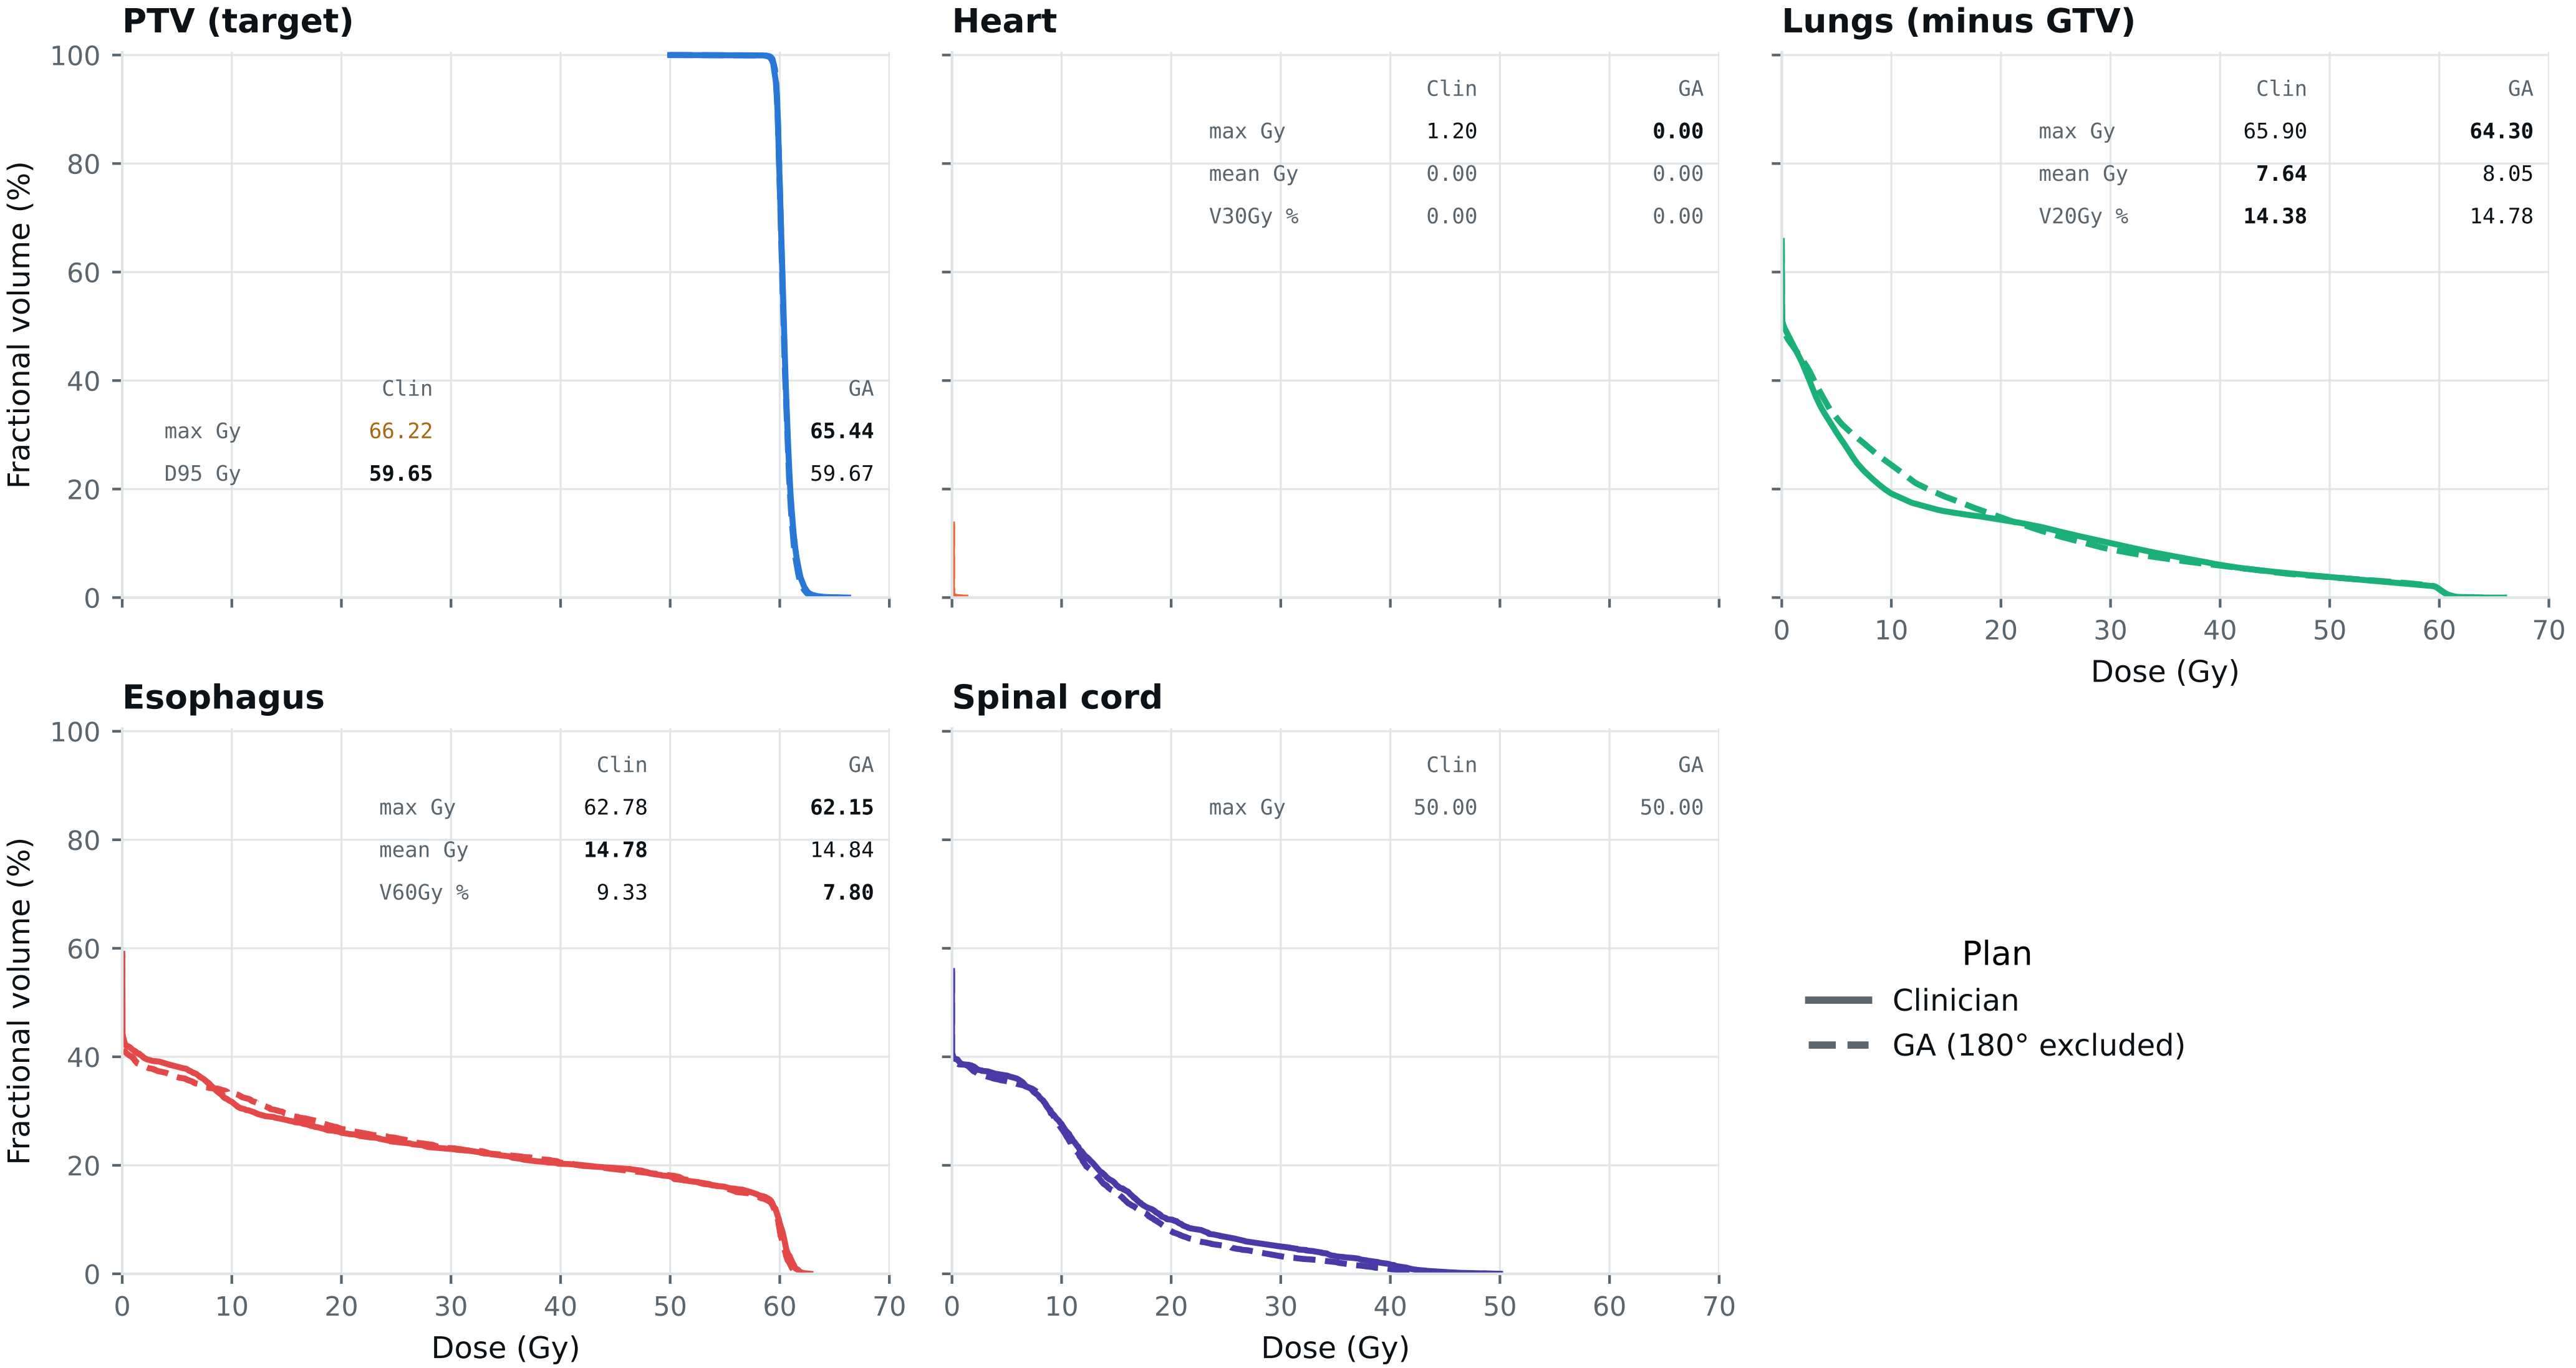

Clinical criteria — Lung_Patient_4

Lung_2Gy_30Fx protocol. Every criterion is a ceiling, so lower is better; bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	63.05	**62.80**	Gy
PTV max	69	66	66.22	**65.44**	Gy
ESOPHAGUS max	66	–	62.78	**62.15**	Gy
ESOPHAGUS mean	34	21	**14.78**	14.84	Gy
ESOPHAGUS V60Gy	17	–	9.33	**7.80**	%
HEART max	66	–	1.20	**0.00**	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	–	**24.22**	45.12	Gy
LUNG_R max	66	–	65.90	**64.30**	Gy
CORD max	50	48	50.00	50.00	Gy
SKIN max	60	–	**46.49**	47.01	Gy
LUNGS_NOT_GTV max	66	–	65.90	**64.30**	Gy
LUNGS_NOT_GTV mean	21	20	**7.64**	8.05	Gy
LUNGS_NOT_GTV V20Gy	37	–	**14.38**	14.78	%
PTV D95 (target coverage)			59.65	59.67	
Objective value (search signal)			89.90	87.65	
Solve time			42 s	39 s	

```
Beam angles (gantry°)   Clinician  0, 185, 210, 240, 270, 300, 330
                        GA         30, 60, 150, 185, 255, 300, 345
```

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.
Source: Lung_Patient_4_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.