Dose-volume histogram — Lung_Patient_31

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

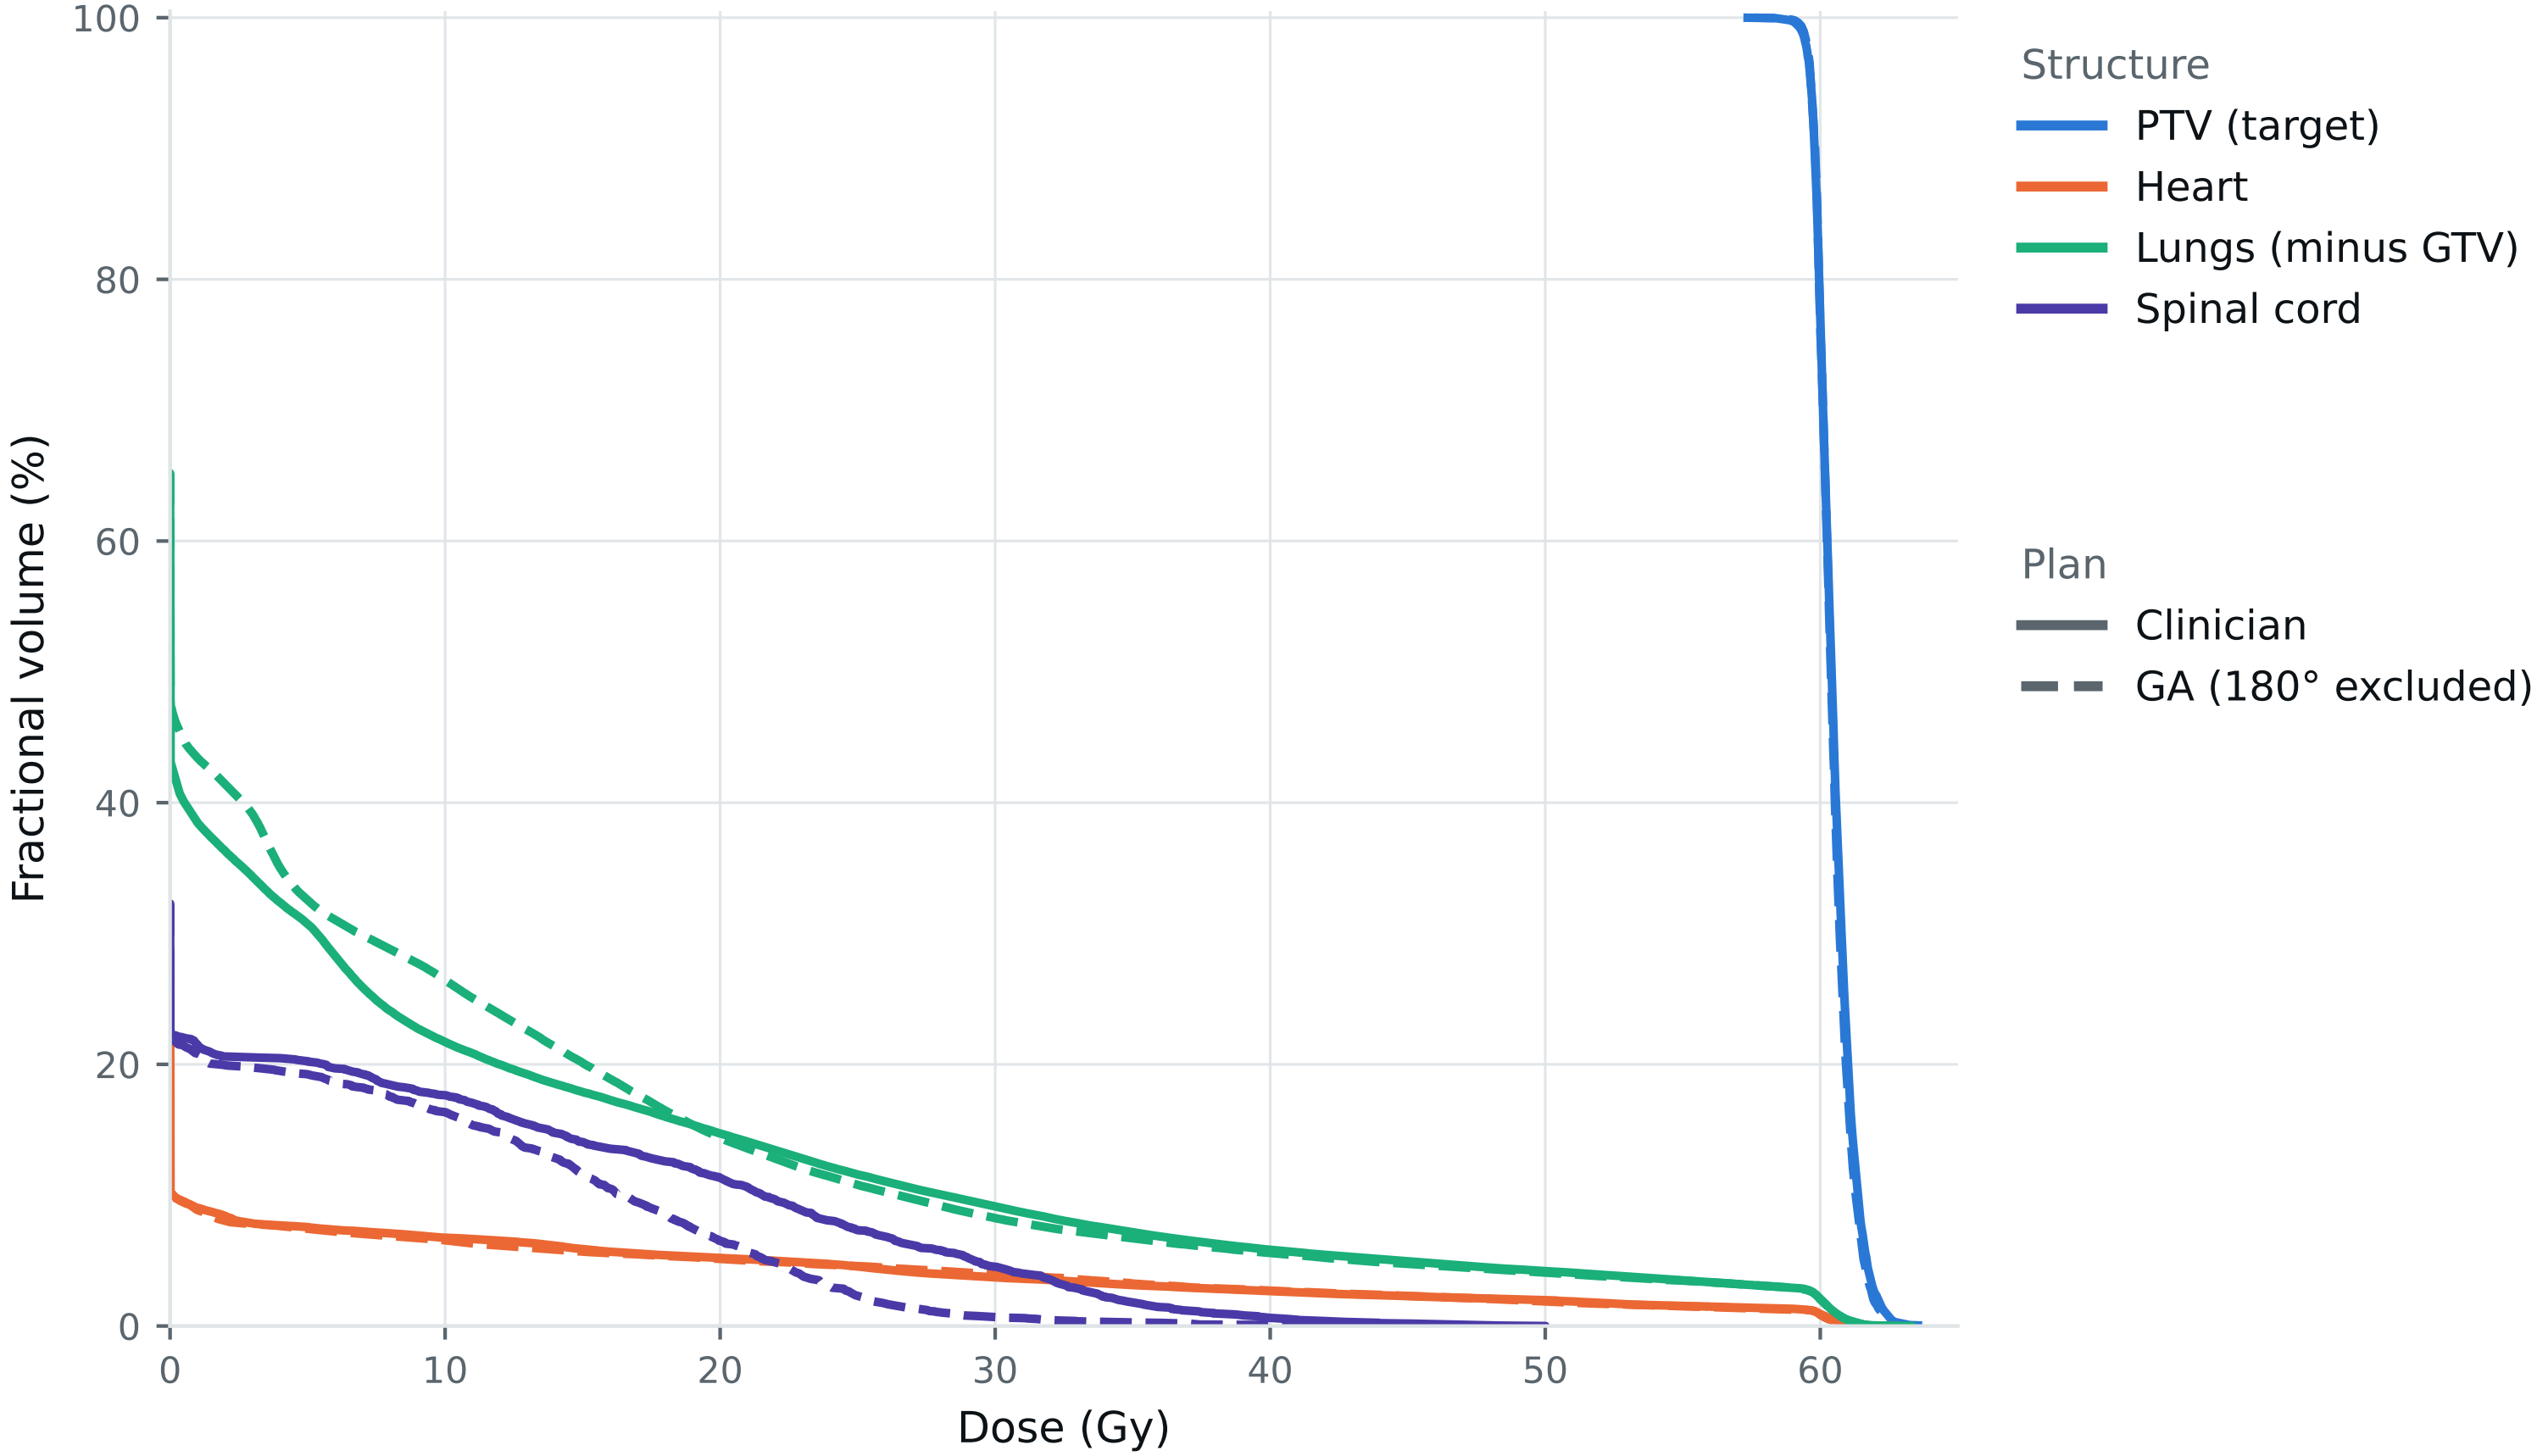

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_31

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

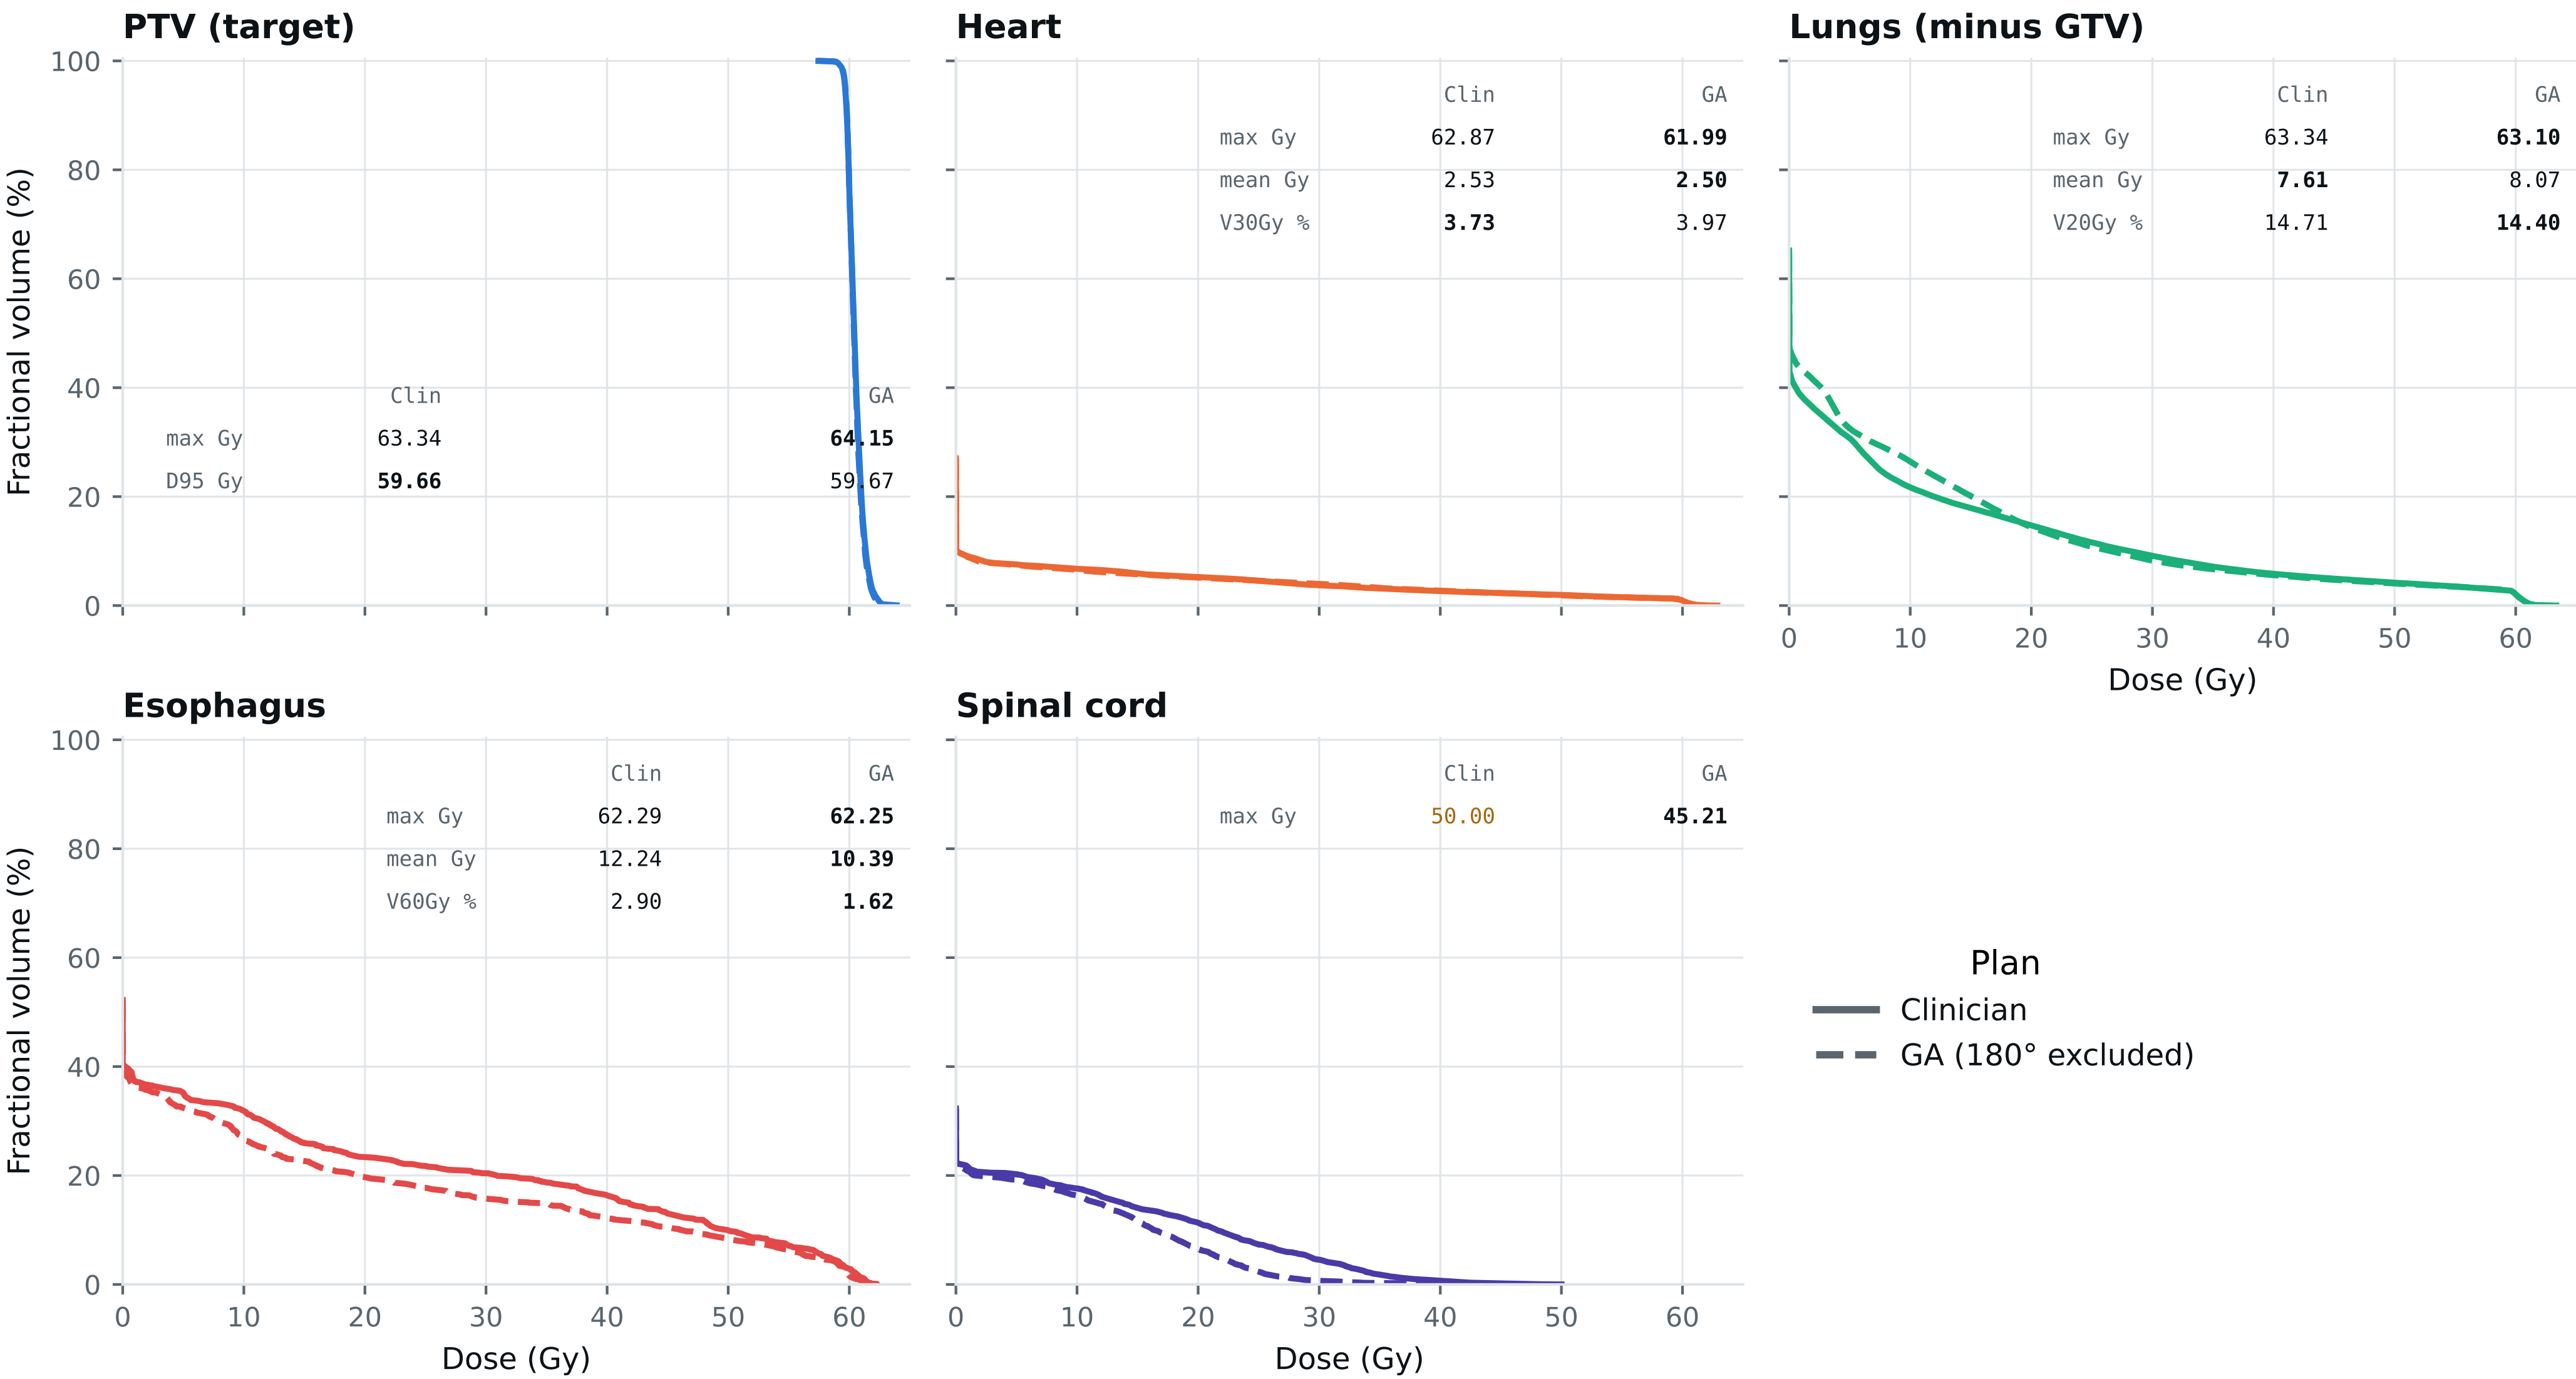

Clinical criteria — Lung_Patient_31

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	63.09	**61.93**	Gy
PTV max	69	66	63.34	**64.15**	Gy
ESOPHAGUS max	66	–	62.29	**62.25**	Gy
ESOPHAGUS mean	34	21	12.24	**10.39**	Gy
ESOPHAGUS V60Gy	17	–	2.90	**1.62**	%
HEART max	66	–	62.87	**61.99**	Gy
HEART mean	27	20	2.53	**2.50**	Gy
HEART V30Gy	50	48	**3.73**	3.97	%
LUNG_L max	66	–	38.72	**36.25**	Gy
LUNG_R max	66	–	63.34	**63.10**	Gy
CORD max	50	48	50.00	**45.21**	Gy
SKIN max	60	–	43.54	**43.23**	Gy
LUNGS_NOT_GTV max	66	–	63.34	**63.10**	Gy
LUNGS_NOT_GTV mean	21	20	**7.61**	8.07	Gy
LUNGS_NOT_GTV V20Gy	37	–	14.71	**14.40**	%
PTV D95 (target coverage)			59.66	59.67	
Objective value (search signal)			90.64	83.22	
MOSEK solve time			18 s	19 s	

Beam angles (gantry°)		
	Clinician	145°, 10°, 335°, 310°, 245°, 215°, 180°
	GA	145°, 10°, 215°, 75°, 240°, 285°, 345°

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.
Source: Lung_Patient_31_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.