Dose-volume histogram — Lung_Patient_41

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

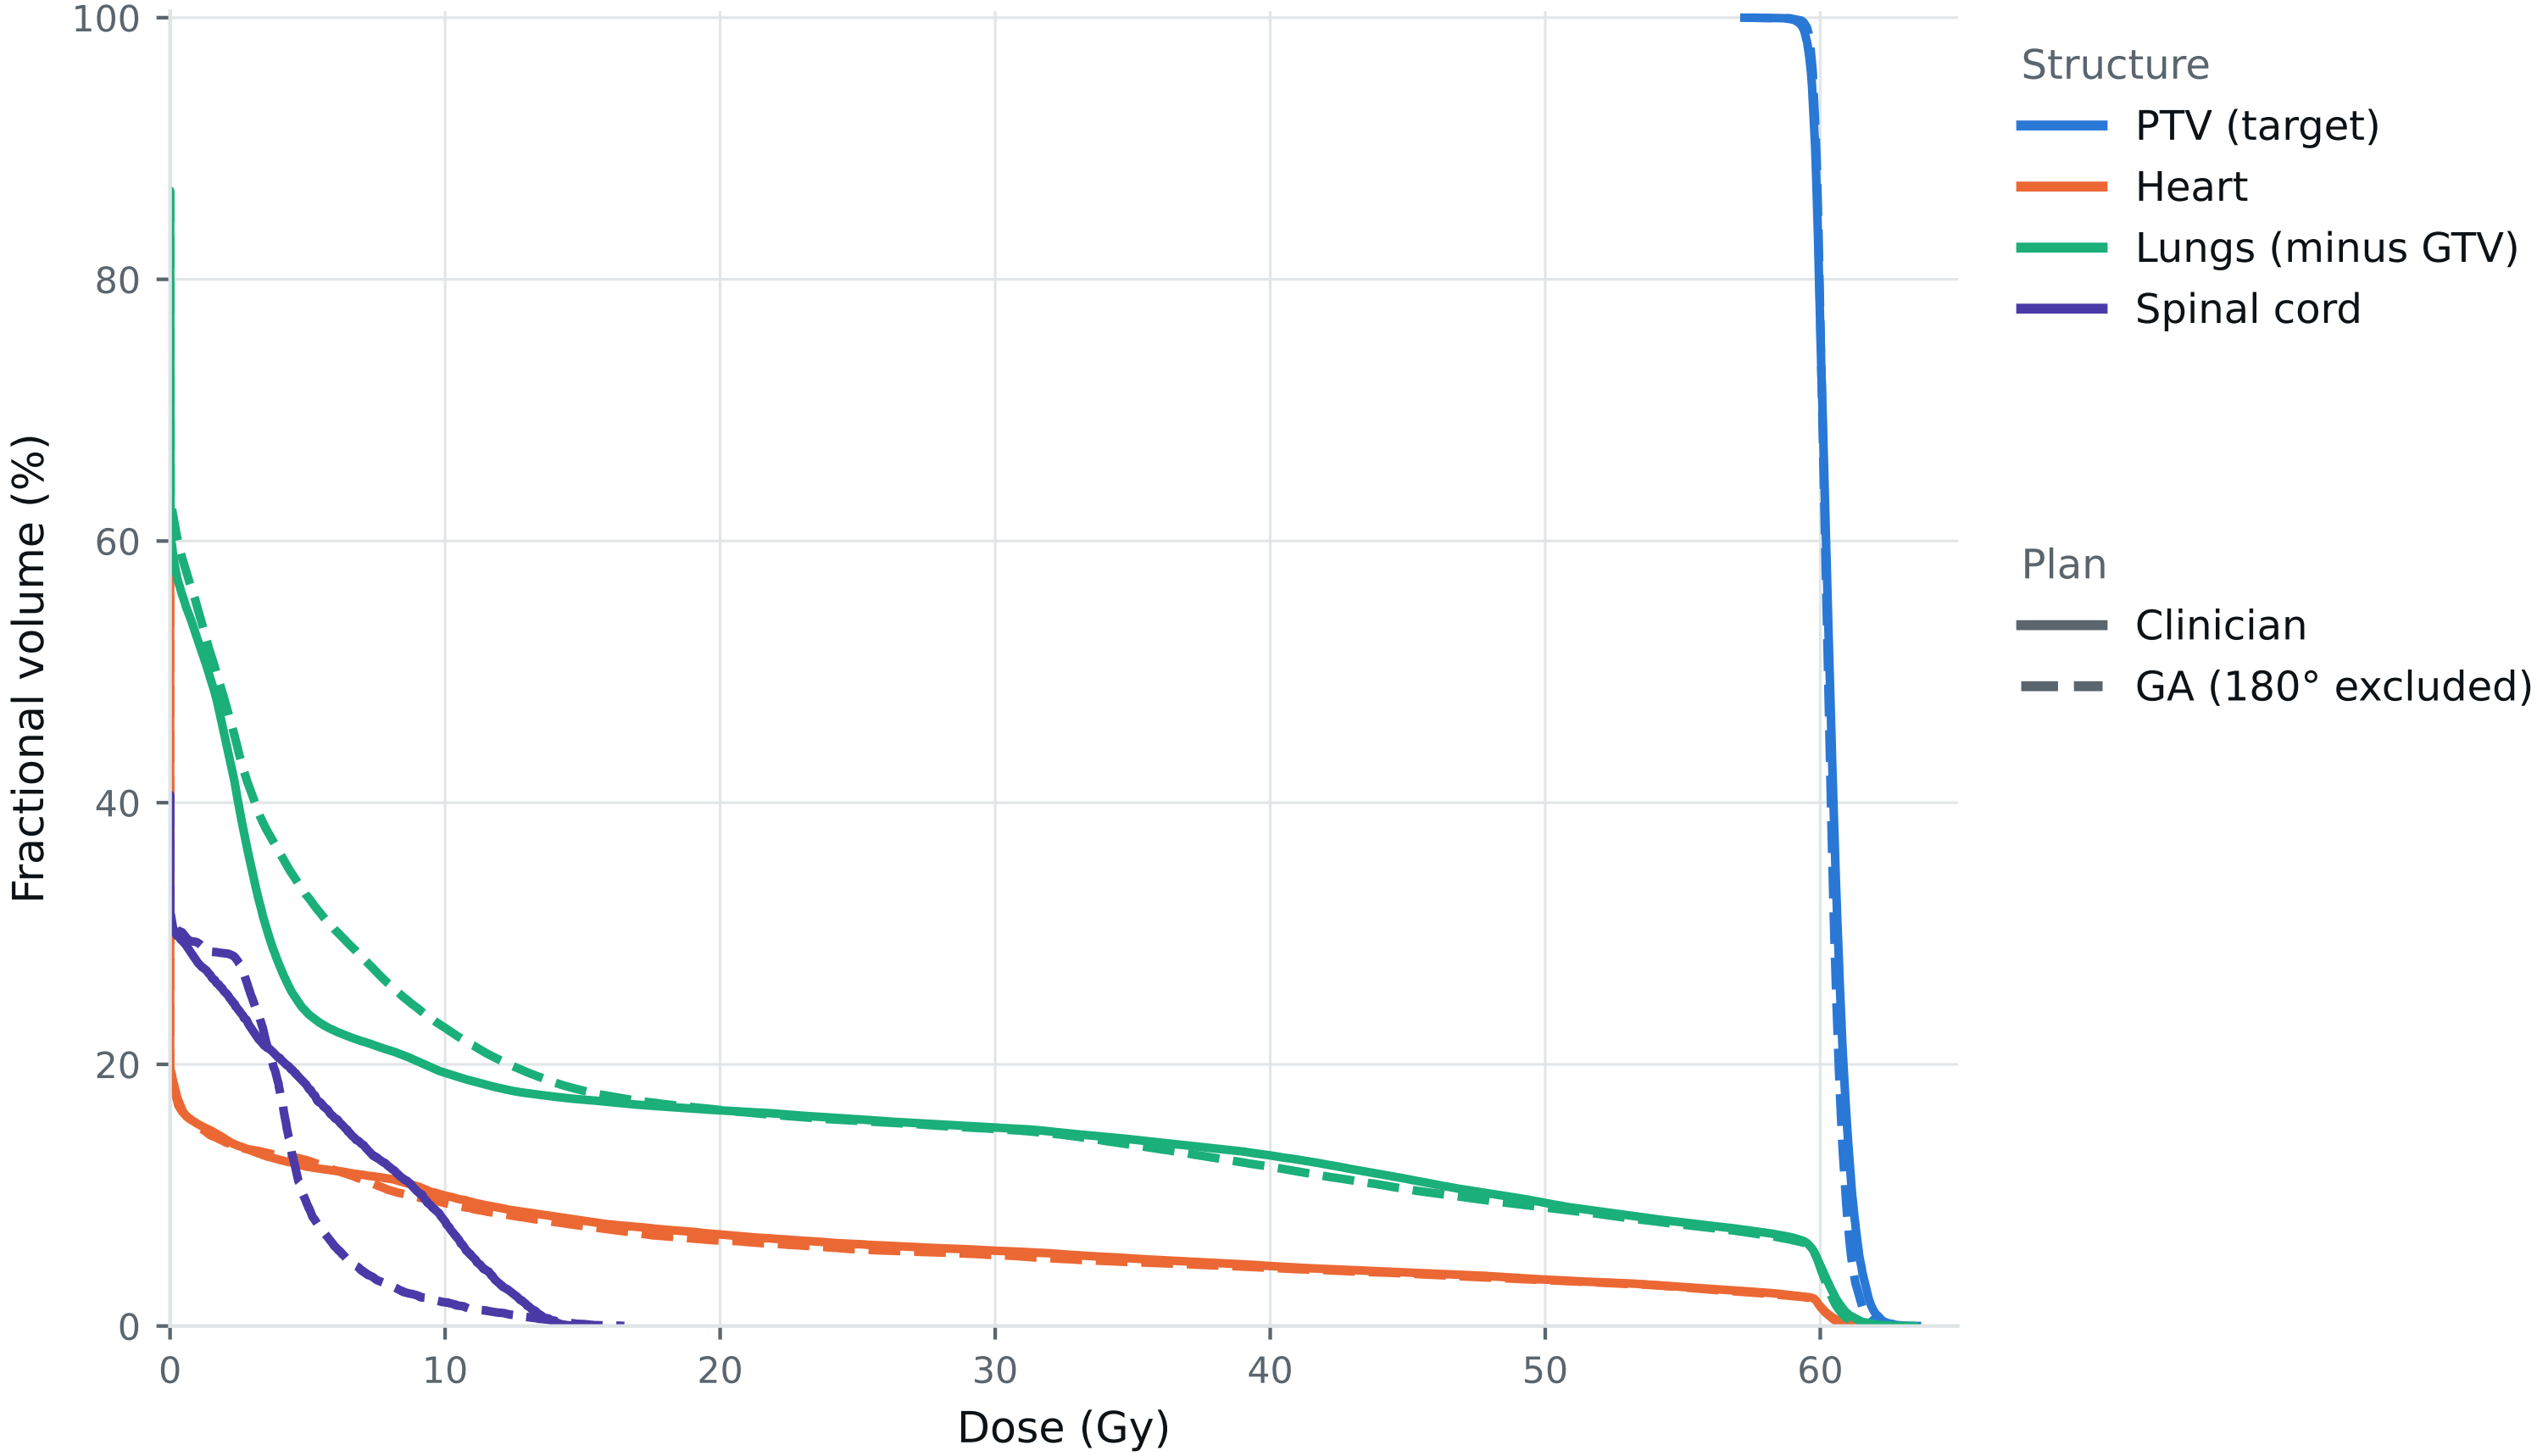

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_41

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

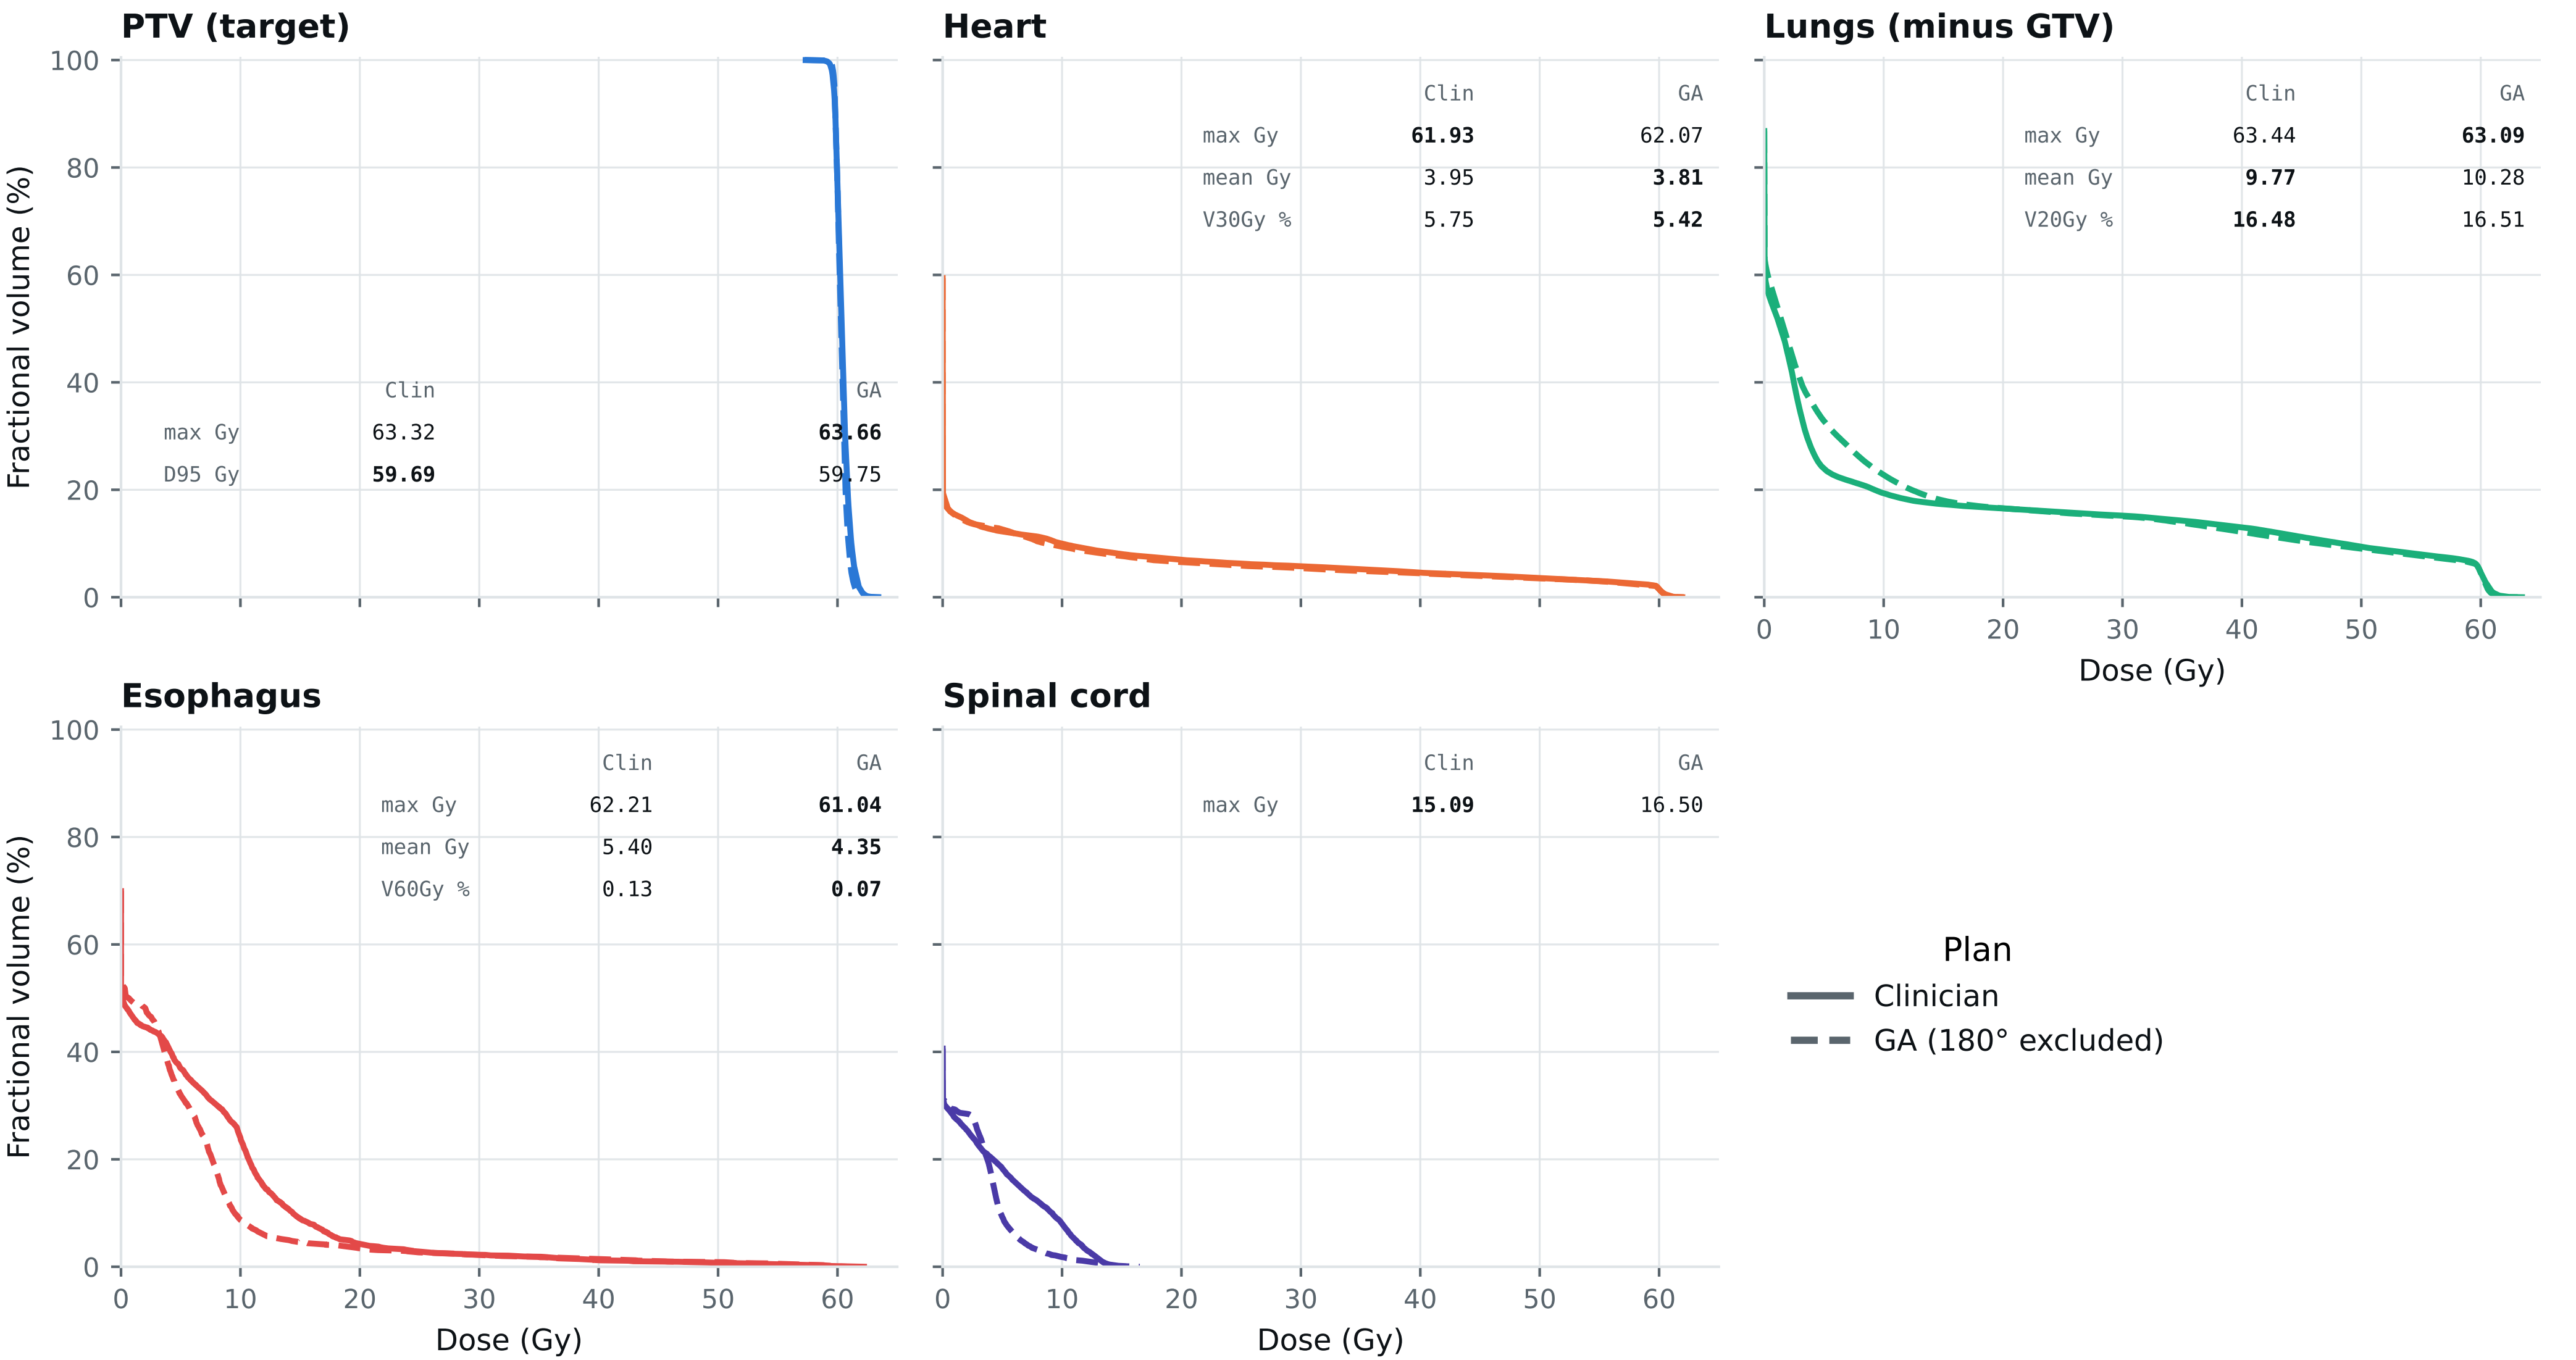

Clinical criteria — Lung_Patient_41

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	62.31	**62.13**	Gy
PTV max	69	66	63.32	**63.66**	Gy
ESOPHAGUS max	66	–	62.21	**61.04**	Gy
ESOPHAGUS mean	34	21	5.40	**4.35**	Gy
ESOPHAGUS V60Gy	17	–	0.13	**0.07**	%
HEART max	66	–	**61.93**	62.07	Gy
HEART mean	27	20	3.95	**3.81**	Gy
HEART V30Gy	50	48	5.75	**5.42**	%
LUNG_L max	66	–	63.44	**63.09**	Gy
LUNG_R max	66	–	**17.55**	43.71	Gy
CORD max	50	48	**15.09**	16.50	Gy
SKIN max	60	–	**46.60**	49.28	Gy
LUNGS_NOT_GTV max	66	–	63.44	**63.09**	Gy
LUNGS_NOT_GTV mean	21	20	**9.77**	10.28	Gy
LUNGS_NOT_GTV V20Gy	37	–	**16.48**	16.51	%
PTV D95 (target coverage)			59.69	59.75	
Objective value (search signal)			73.60	68.63	
MOSEK solve time			53 s	37 s	

```
Beam angles (gantry°)   Clinician  175°, 147°, 115°, 60°, 32°, 5°
                        GA         5°, 45°, 105°, 135°, 195°, 255°, 345°
```

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_41_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.