Dose-volume histogram — Lung_Patient_27

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

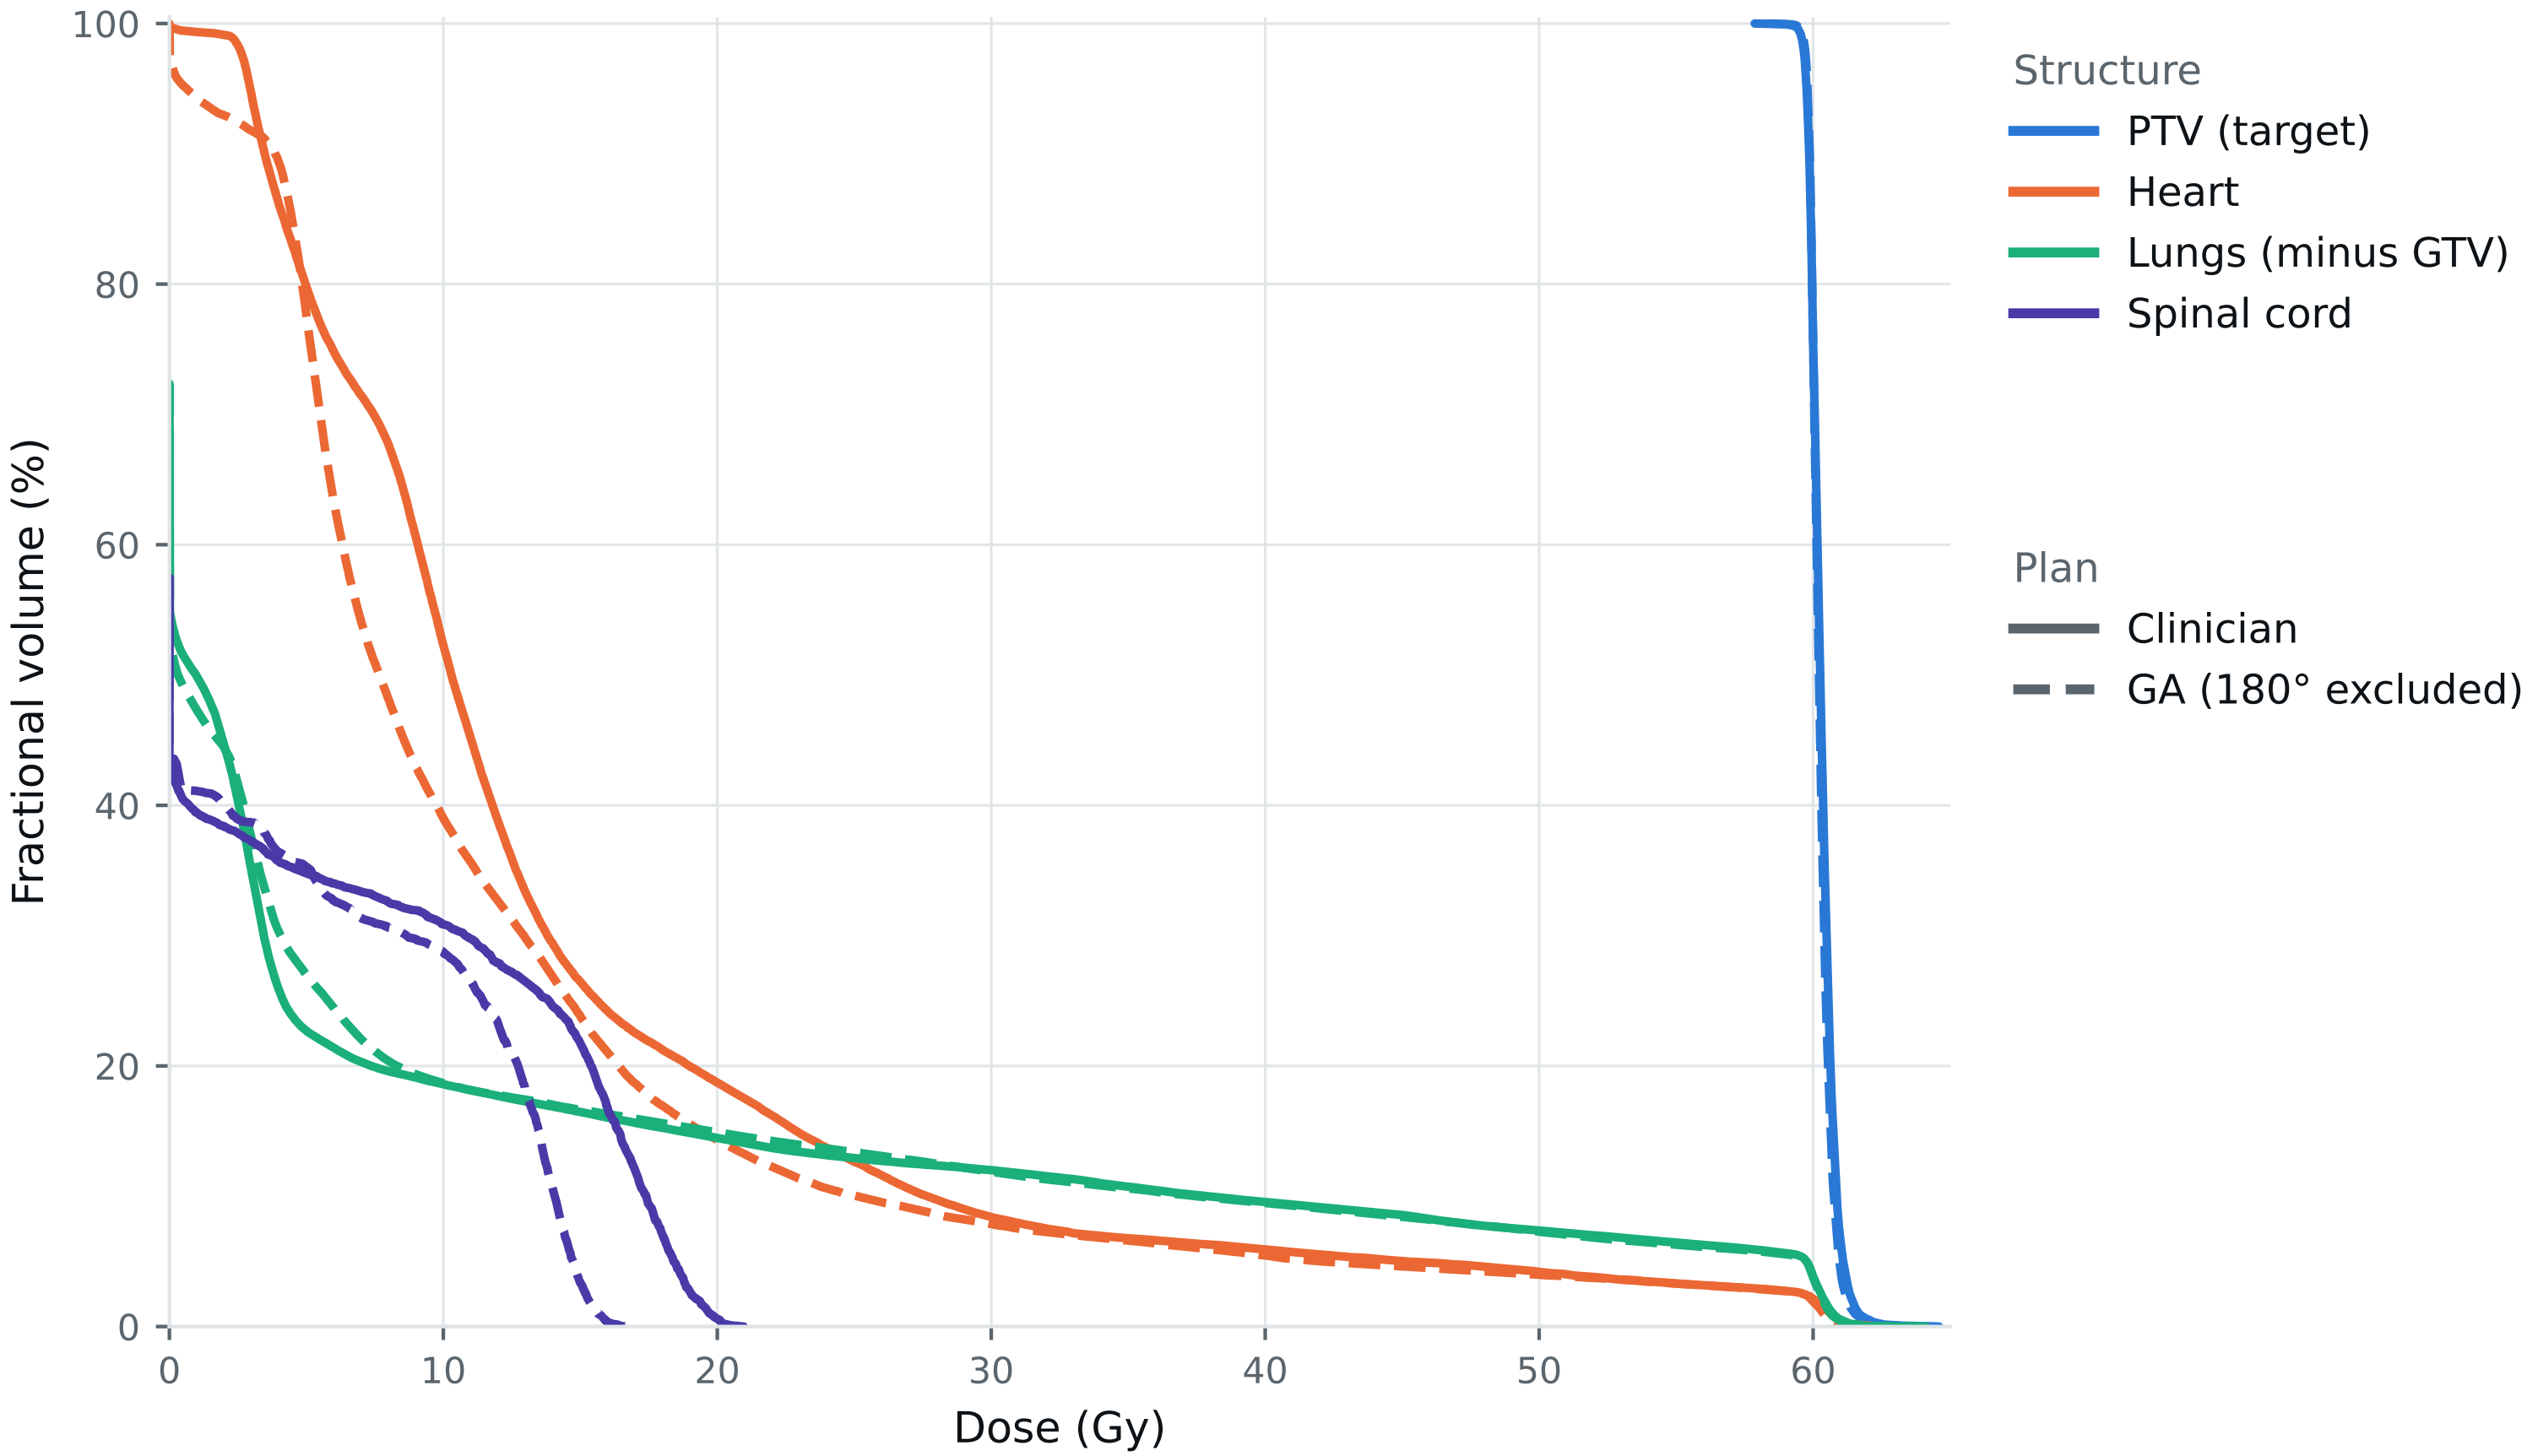

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_27

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

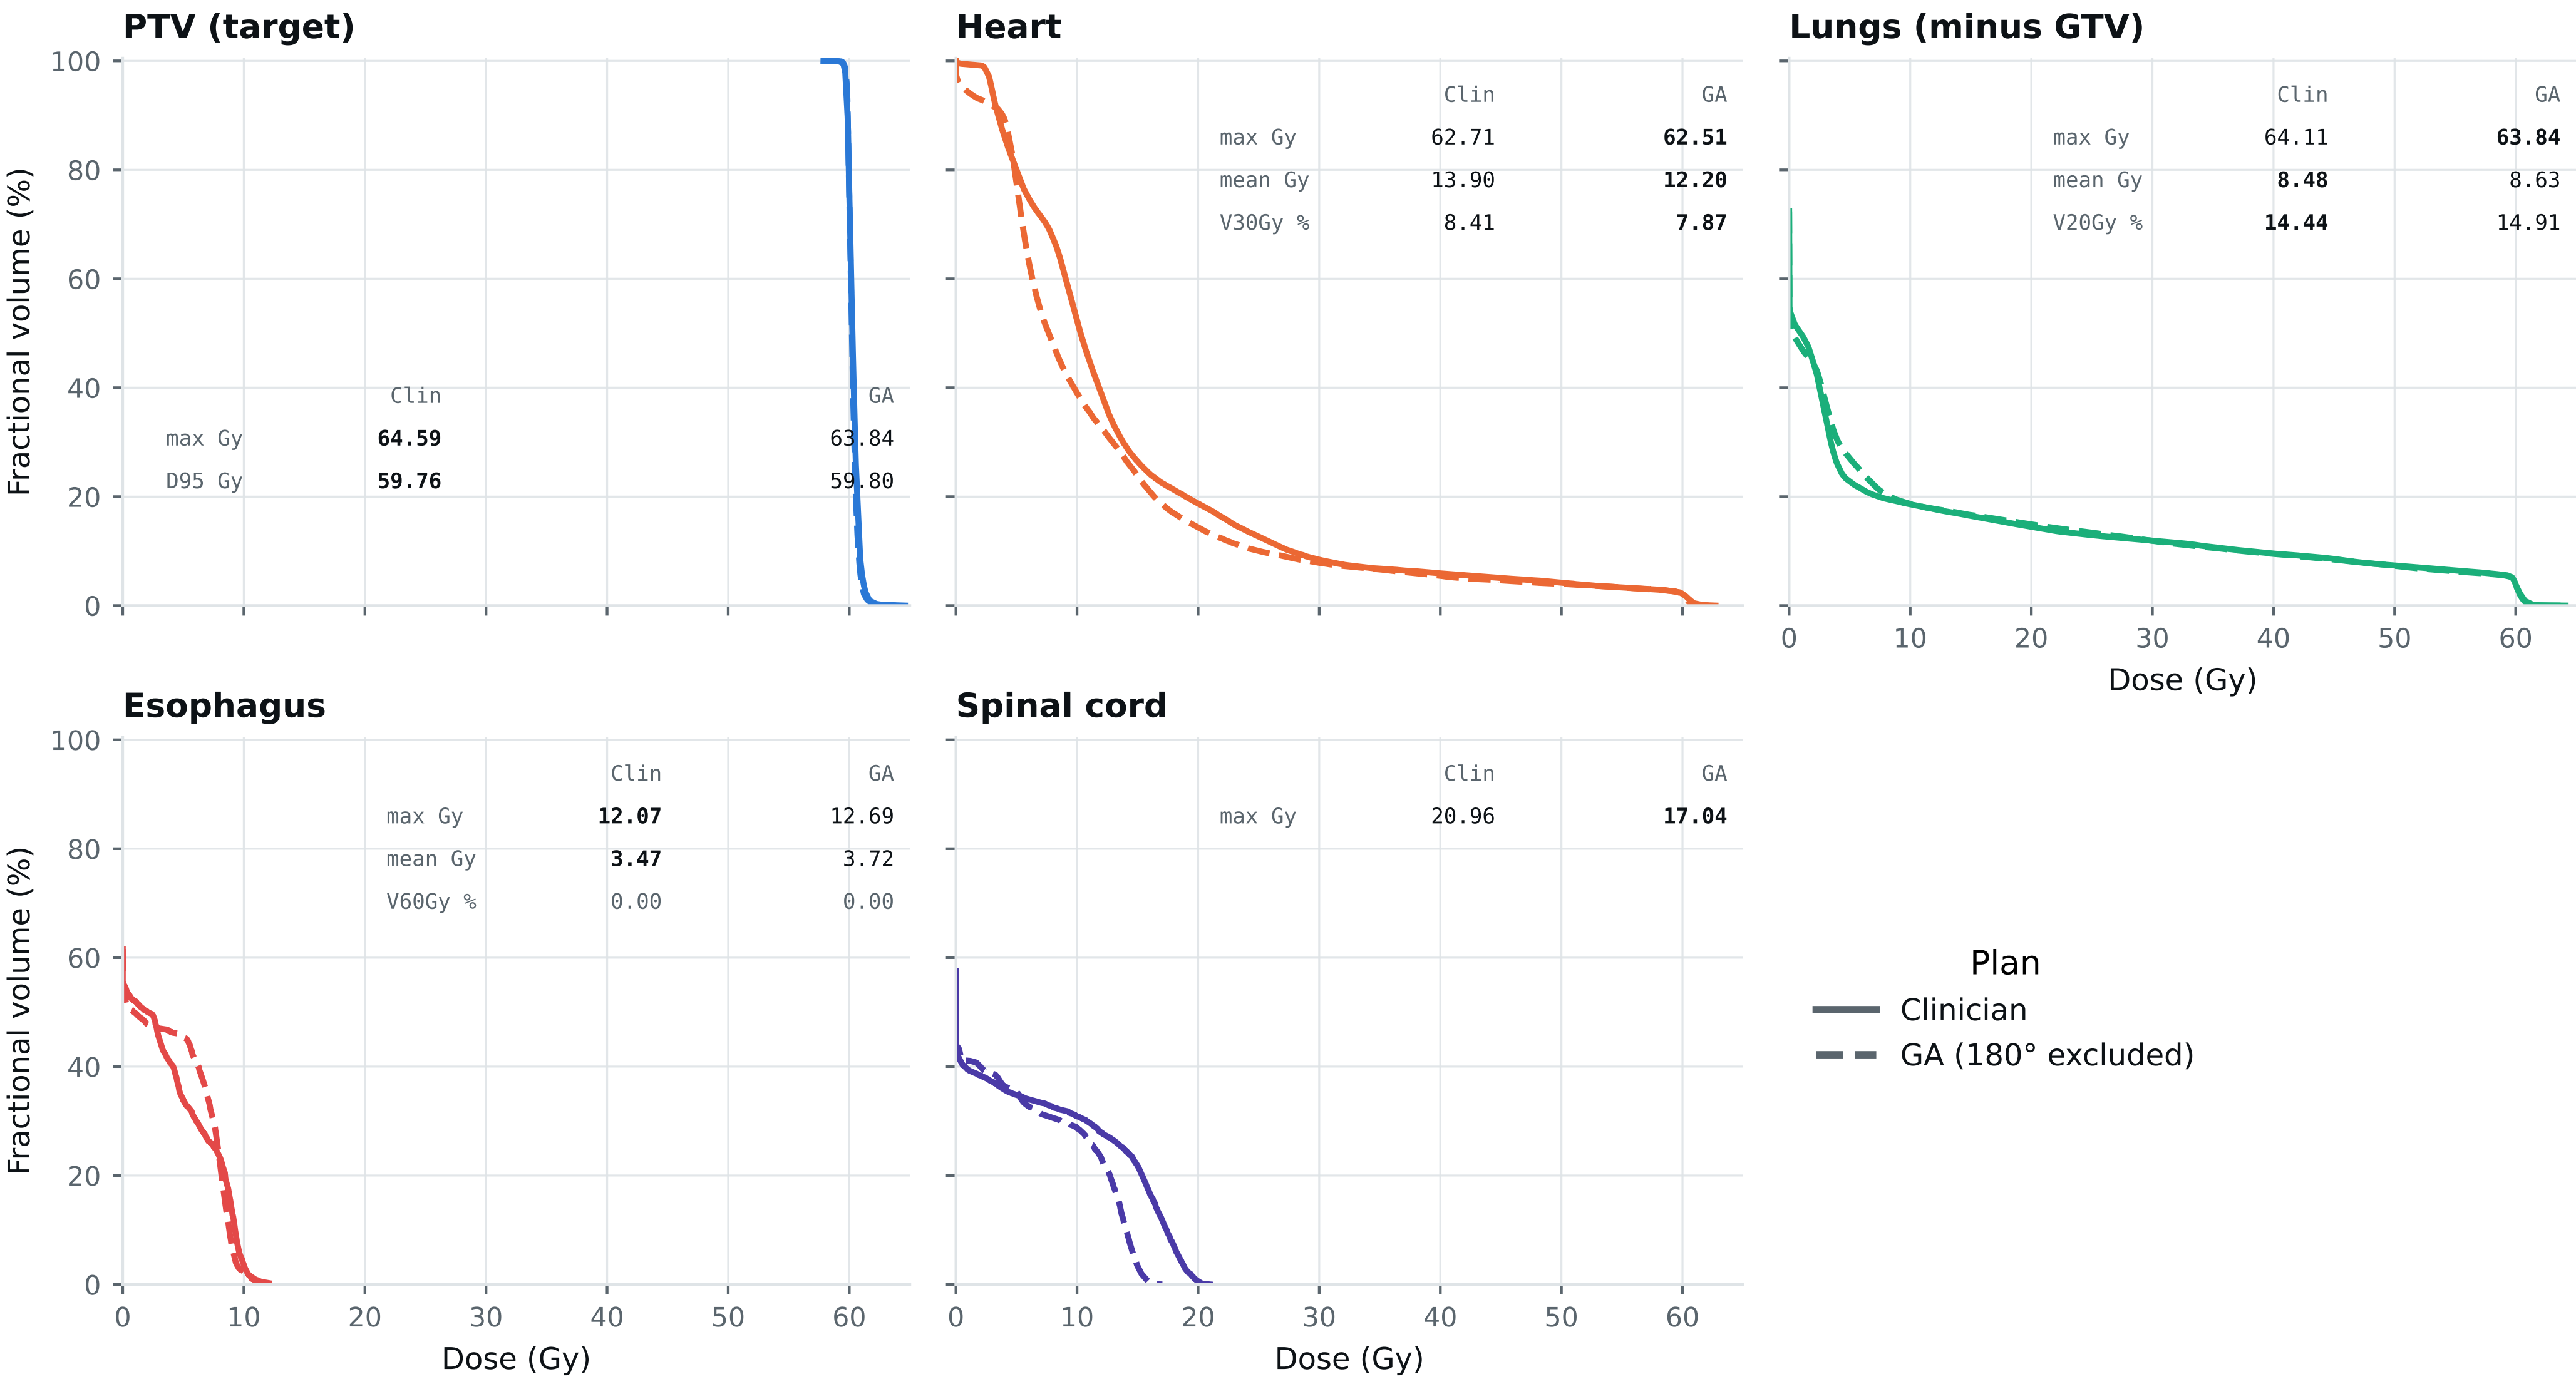

Clinical criteria — Lung_Patient_27

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	61.60	**61.58**	Gy
PTV max	69	66	**64.59**	63.84	Gy
ESOPHAGUS max	66	–	**12.07**	12.69	Gy
ESOPHAGUS mean	34	21	**3.47**	3.72	Gy
ESOPHAGUS V60Gy	17	–	0.00	0.00	%
HEART max	66	–	62.71	**62.51**	Gy
HEART mean	27	20	13.90	**12.20**	Gy
HEART V30Gy	50	48	8.41	**7.87**	%
LUNG_L max	66	–	64.11	**63.84**	Gy
LUNG_R max	66	–	**12.39**	13.60	Gy
CORD max	50	48	20.96	**17.04**	Gy
SKIN max	60	–	52.22	**46.38**	Gy
LUNGS_NOT_GTV max	66	–	64.11	**63.84**	Gy
LUNGS_NOT_GTV mean	21	20	**8.48**	8.63	Gy
LUNGS_NOT_GTV V20Gy	37	–	**14.44**	14.91	%
PTV D95 (target coverage)			59.76	59.80	
Objective value (search signal)			63.30	60.13	
MOSEK solve time			22 s	29 s	

Beam angles (gantry°)	Clinician	175°, 145°, 115°, 65°, 30°, 0°
	GA	175°, 145°, 30°, 60°, 90°, 195°, 345°

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_27_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.