Dose-volume histogram — Lung_Patient_14

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

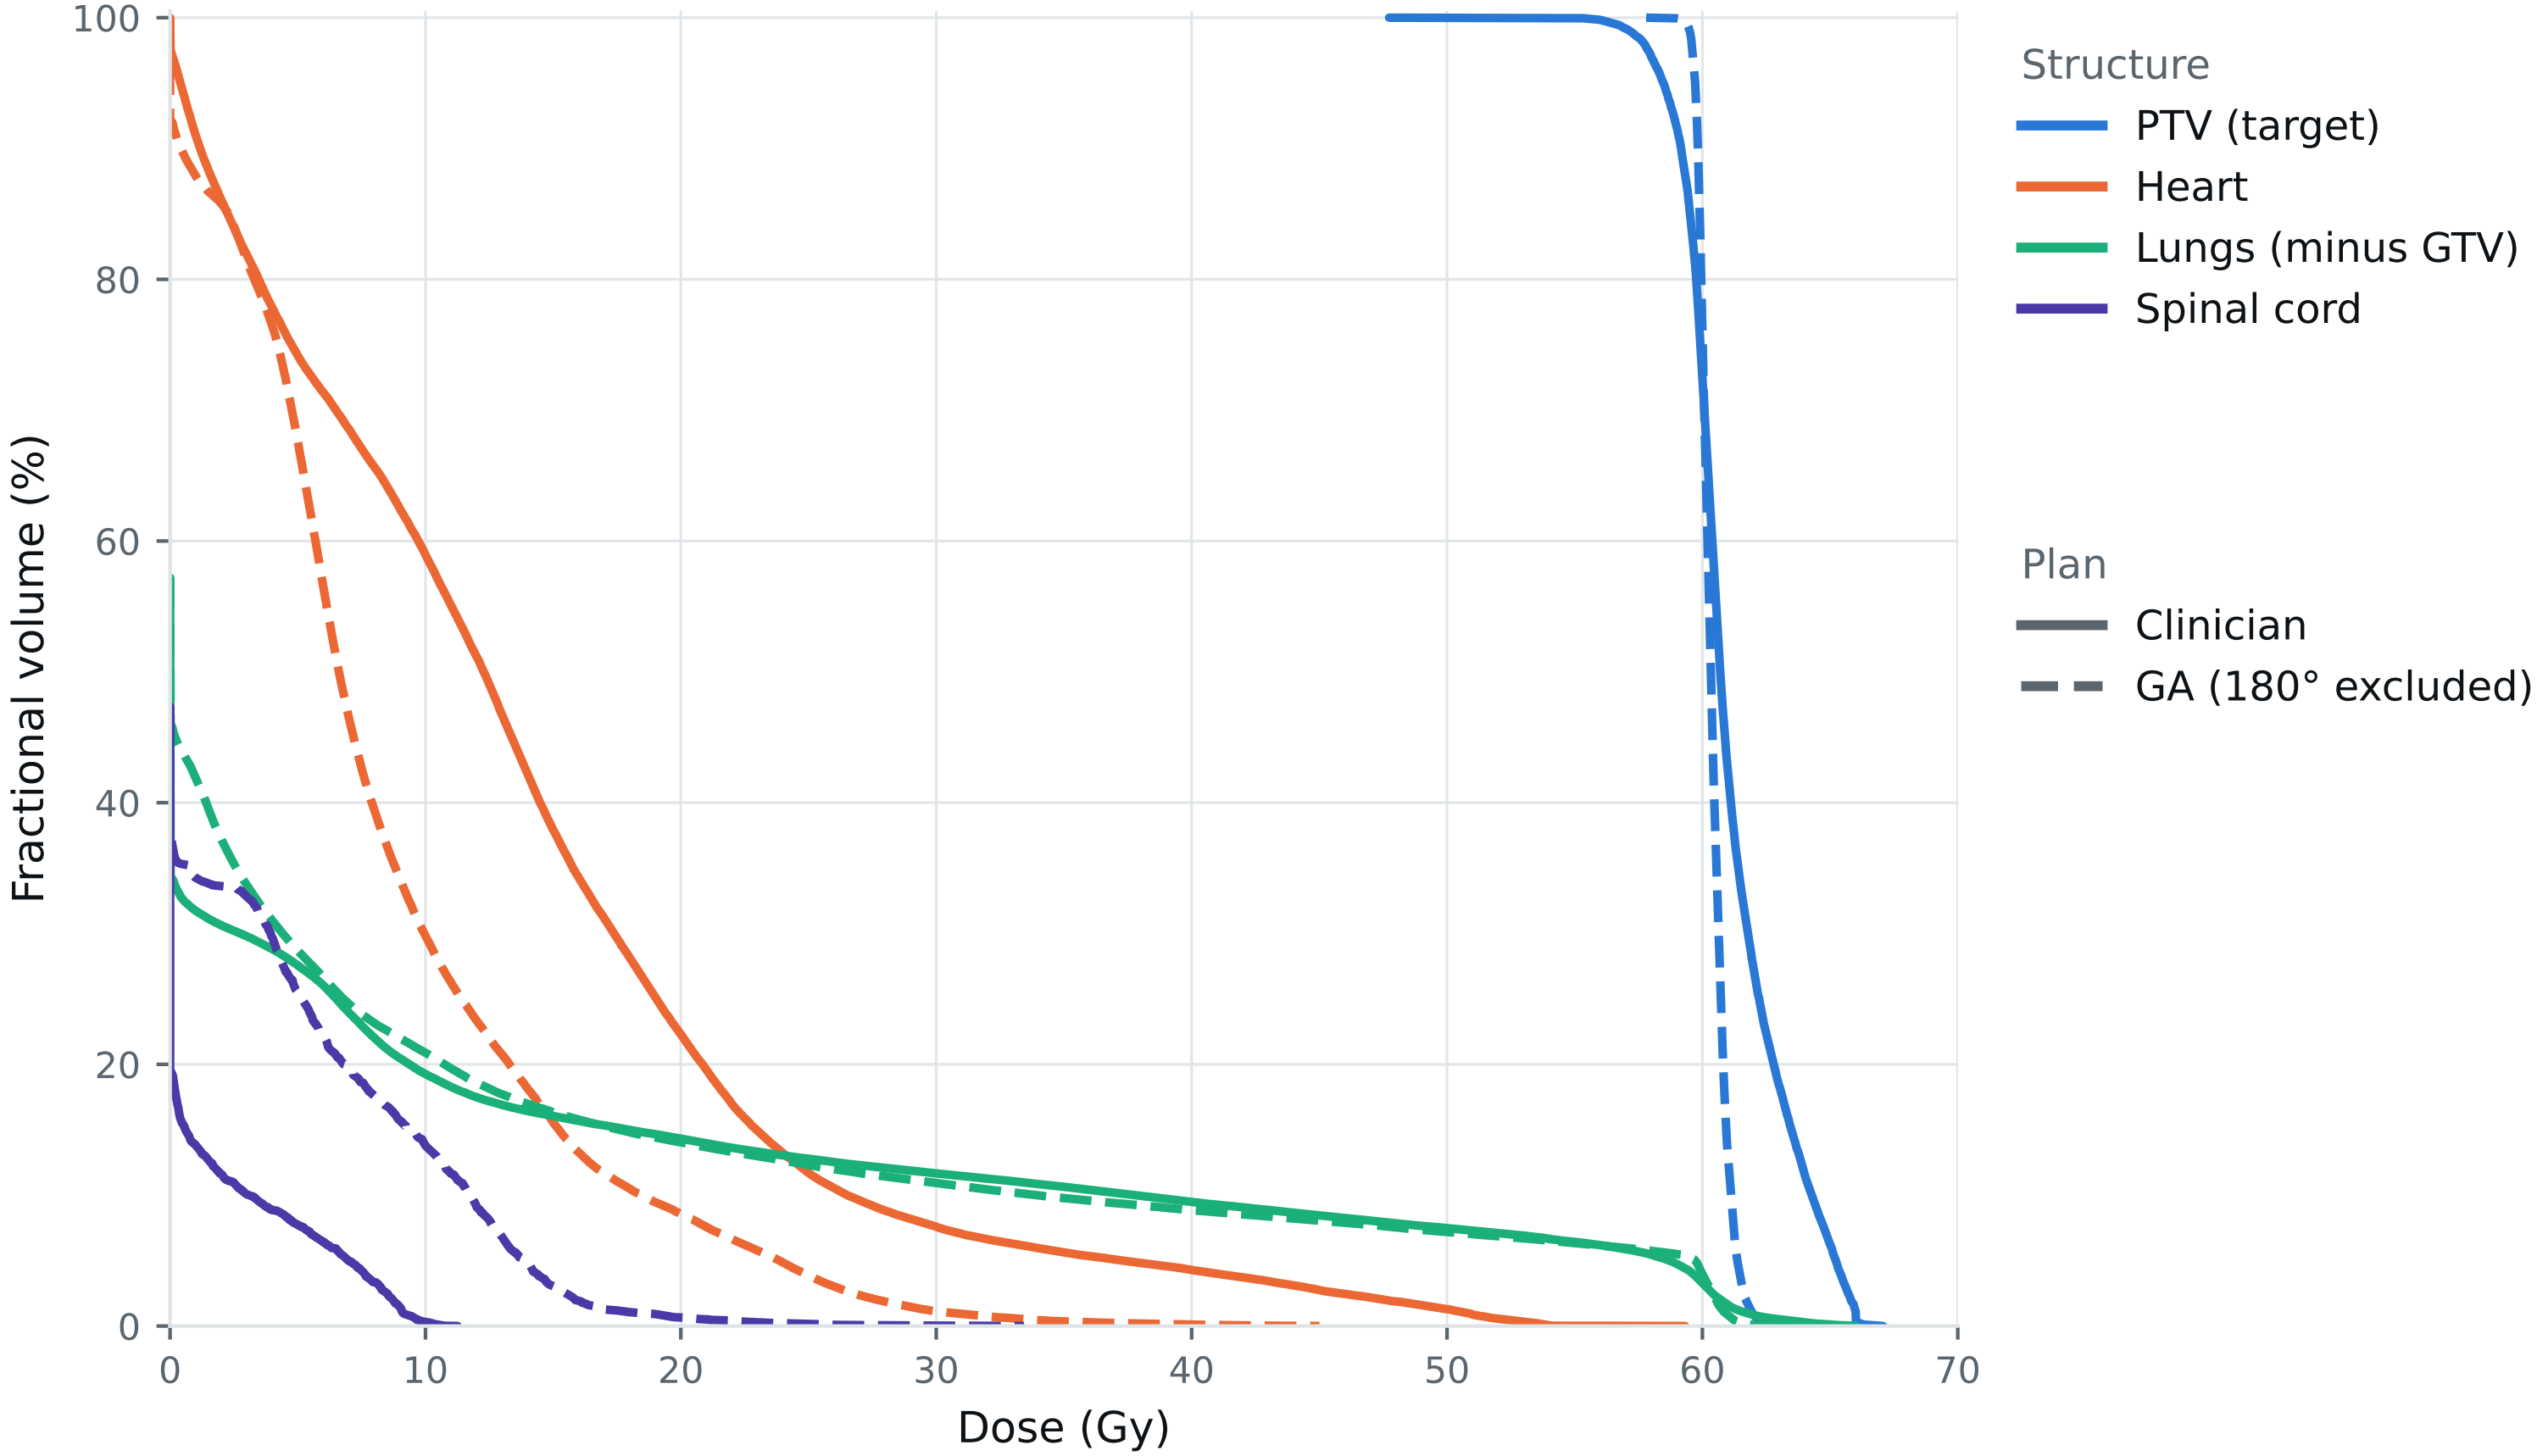

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_14

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

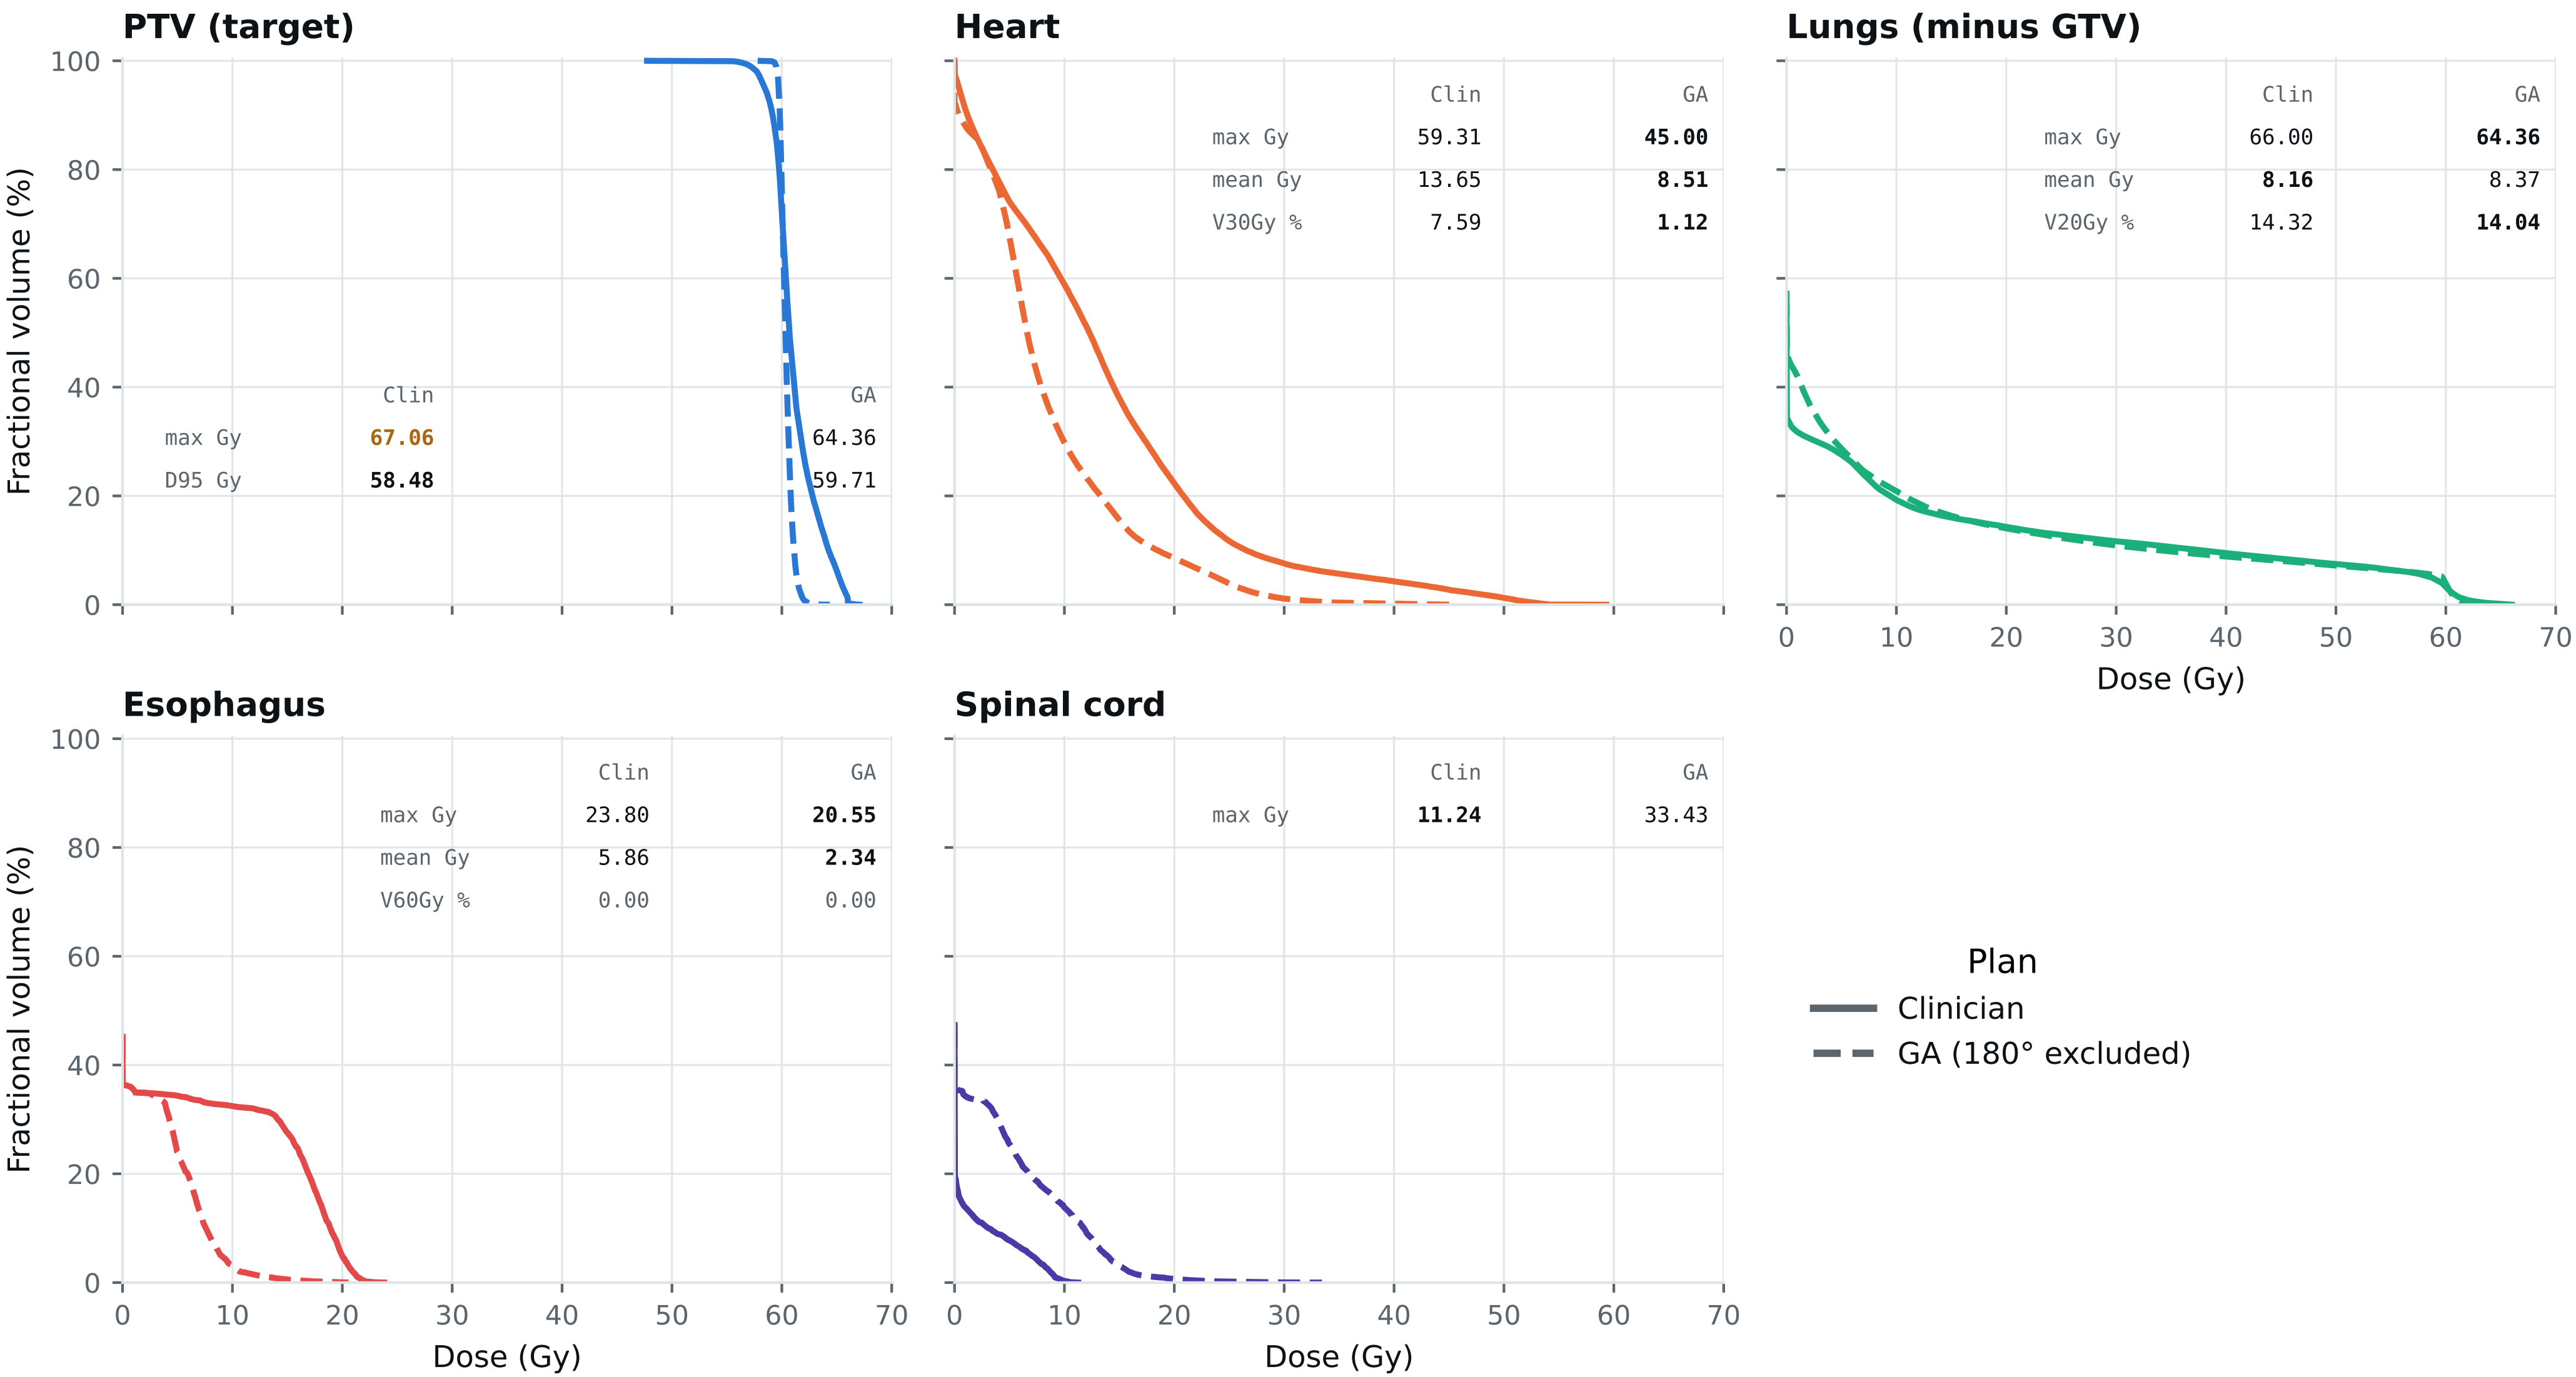

Clinical criteria — Lung_Patient_14

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	67.06	**62.69**	Gy
PTV max	69	66	**67.06**	64.36	Gy
ESOPHAGUS max	66	–	23.80	**20.55**	Gy
ESOPHAGUS mean	34	21	5.86	**2.34**	Gy
ESOPHAGUS V60Gy	17	–	0.00	0.00	%
HEART max	66	–	59.31	**45.00**	Gy
HEART mean	27	20	13.65	**8.51**	Gy
HEART V30Gy	50	48	7.59	**1.12**	%
LUNG_L max	66	–	66.00	**64.36**	Gy
LUNG_R max	66	–	**22.02**	36.22	Gy
CORD max	50	48	**11.24**	33.43	Gy
SKIN max	60	–	54.27	**49.92**	Gy
LUNGS_NOT_GTV max	66	–	66.00	**64.36**	Gy
LUNGS_NOT_GTV mean	21	20	**8.16**	8.37	Gy
LUNGS_NOT_GTV V20Gy	37	–	14.32	**14.04**	%
PTV D95 (target coverage)			58.48	59.71	
Objective value (search signal)			188.47	64.41	
Solve time			33 s	40 s	

Beam angles (gantry°)	Clinician	200°, 175°, 155°, 120°, 32°, 0°
	GA	120°, 45°, 75°, 90°, 165°, 195°, 210°

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_14_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.