Dose-volume histogram — Lung_Patient_25

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

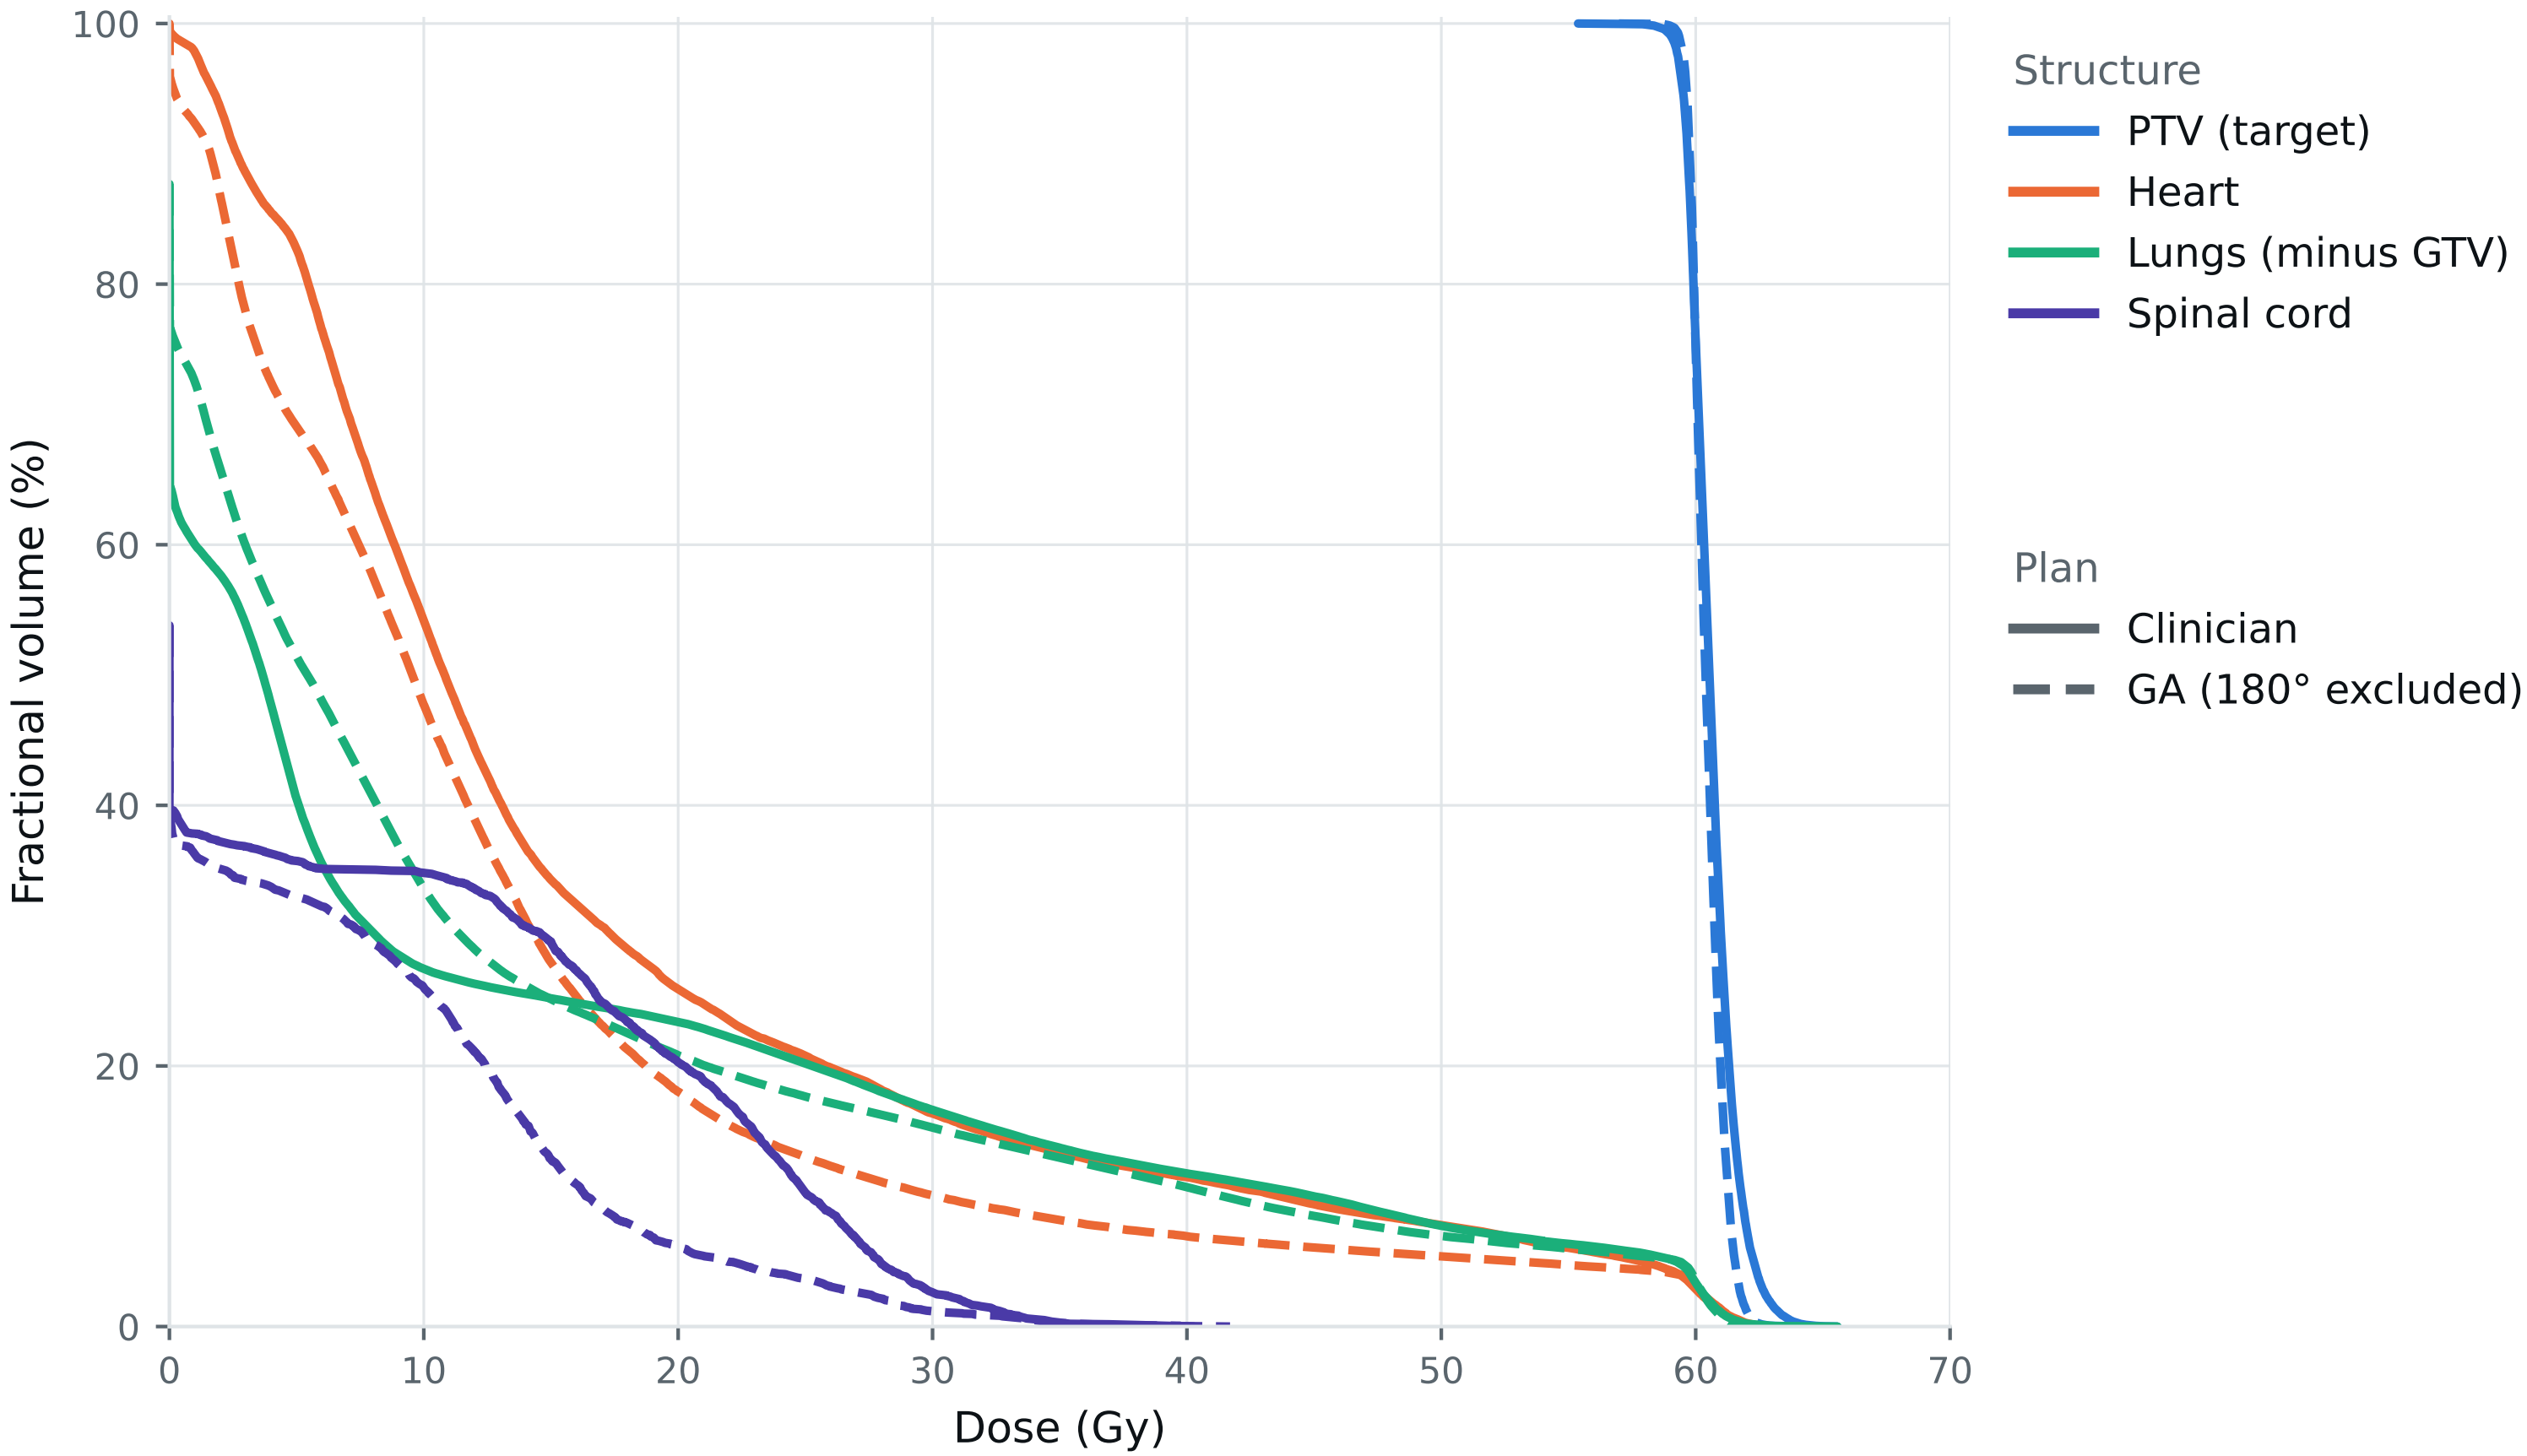

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_25

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

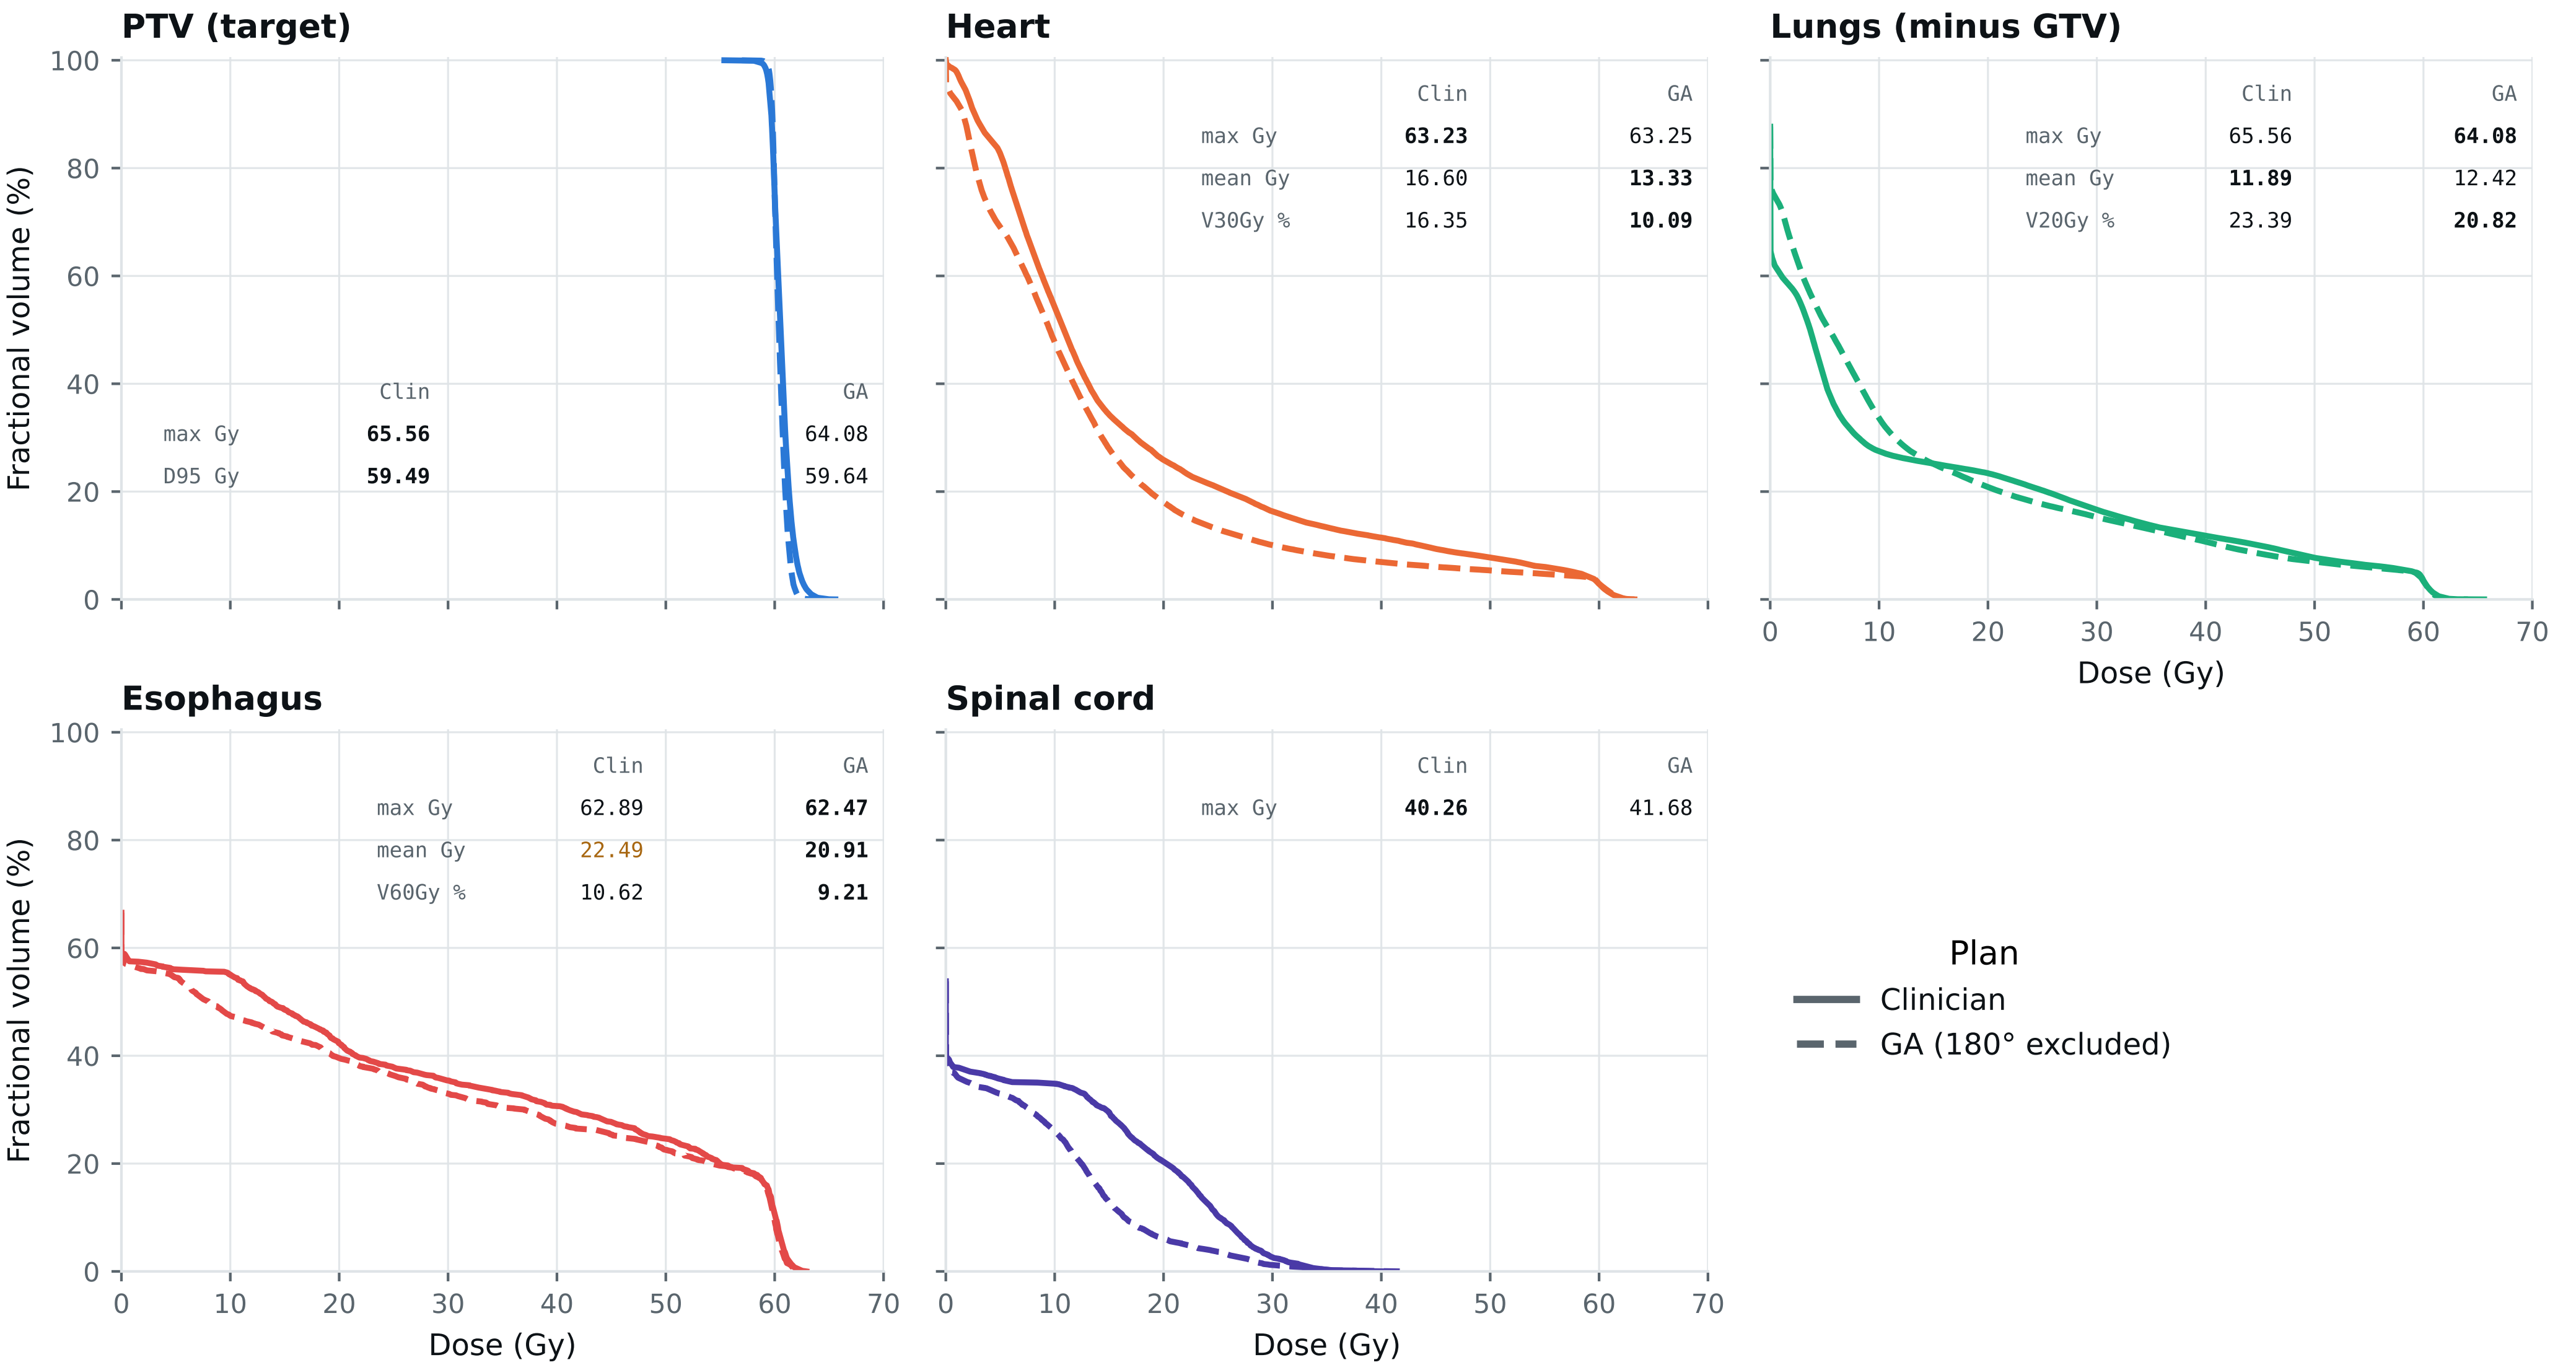

Clinical criteria — Lung_Patient_25

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	65.56	**62.50**	Gy
PTV max	69	66	**65.56**	64.08	Gy
ESOPHAGUS max	66	–	62.89	**62.47**	Gy
ESOPHAGUS mean	34	21	22.49	**20.91**	Gy
ESOPHAGUS V60Gy	17	–	10.62	**9.21**	%
HEART max	66	–	**63.23**	63.25	Gy
HEART mean	27	20	16.60	**13.33**	Gy
HEART V30Gy	50	48	16.35	**10.09**	%
LUNG_L max	66	–	54.83	**54.11**	Gy
LUNG_R max	66	–	65.56	**64.08**	Gy
CORD max	50	48	**40.26**	41.68	Gy
SKIN max	60	–	**43.94**	44.00	Gy
LUNGS_NOT_GTV max	66	–	65.56	**64.08**	Gy
LUNGS_NOT_GTV mean	21	20	**11.89**	12.42	Gy
LUNGS_NOT_GTV V20Gy	37	–	23.39	**20.82**	%
PTV D95 (target coverage)			59.49	59.64	
Objective value (search signal)			127.33	105.04	
MOSEK solve time			38 s	40 s	

```
Beam angles (gantry°)   Clinician  150°, 0°, 340°, 320°, 240°, 210°, 185°
                        GA         320°, 240°, 185°, 30°, 165°, 270°, 300°
```

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_25_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.