Dose-volume histogram — Lung_Patient_18

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

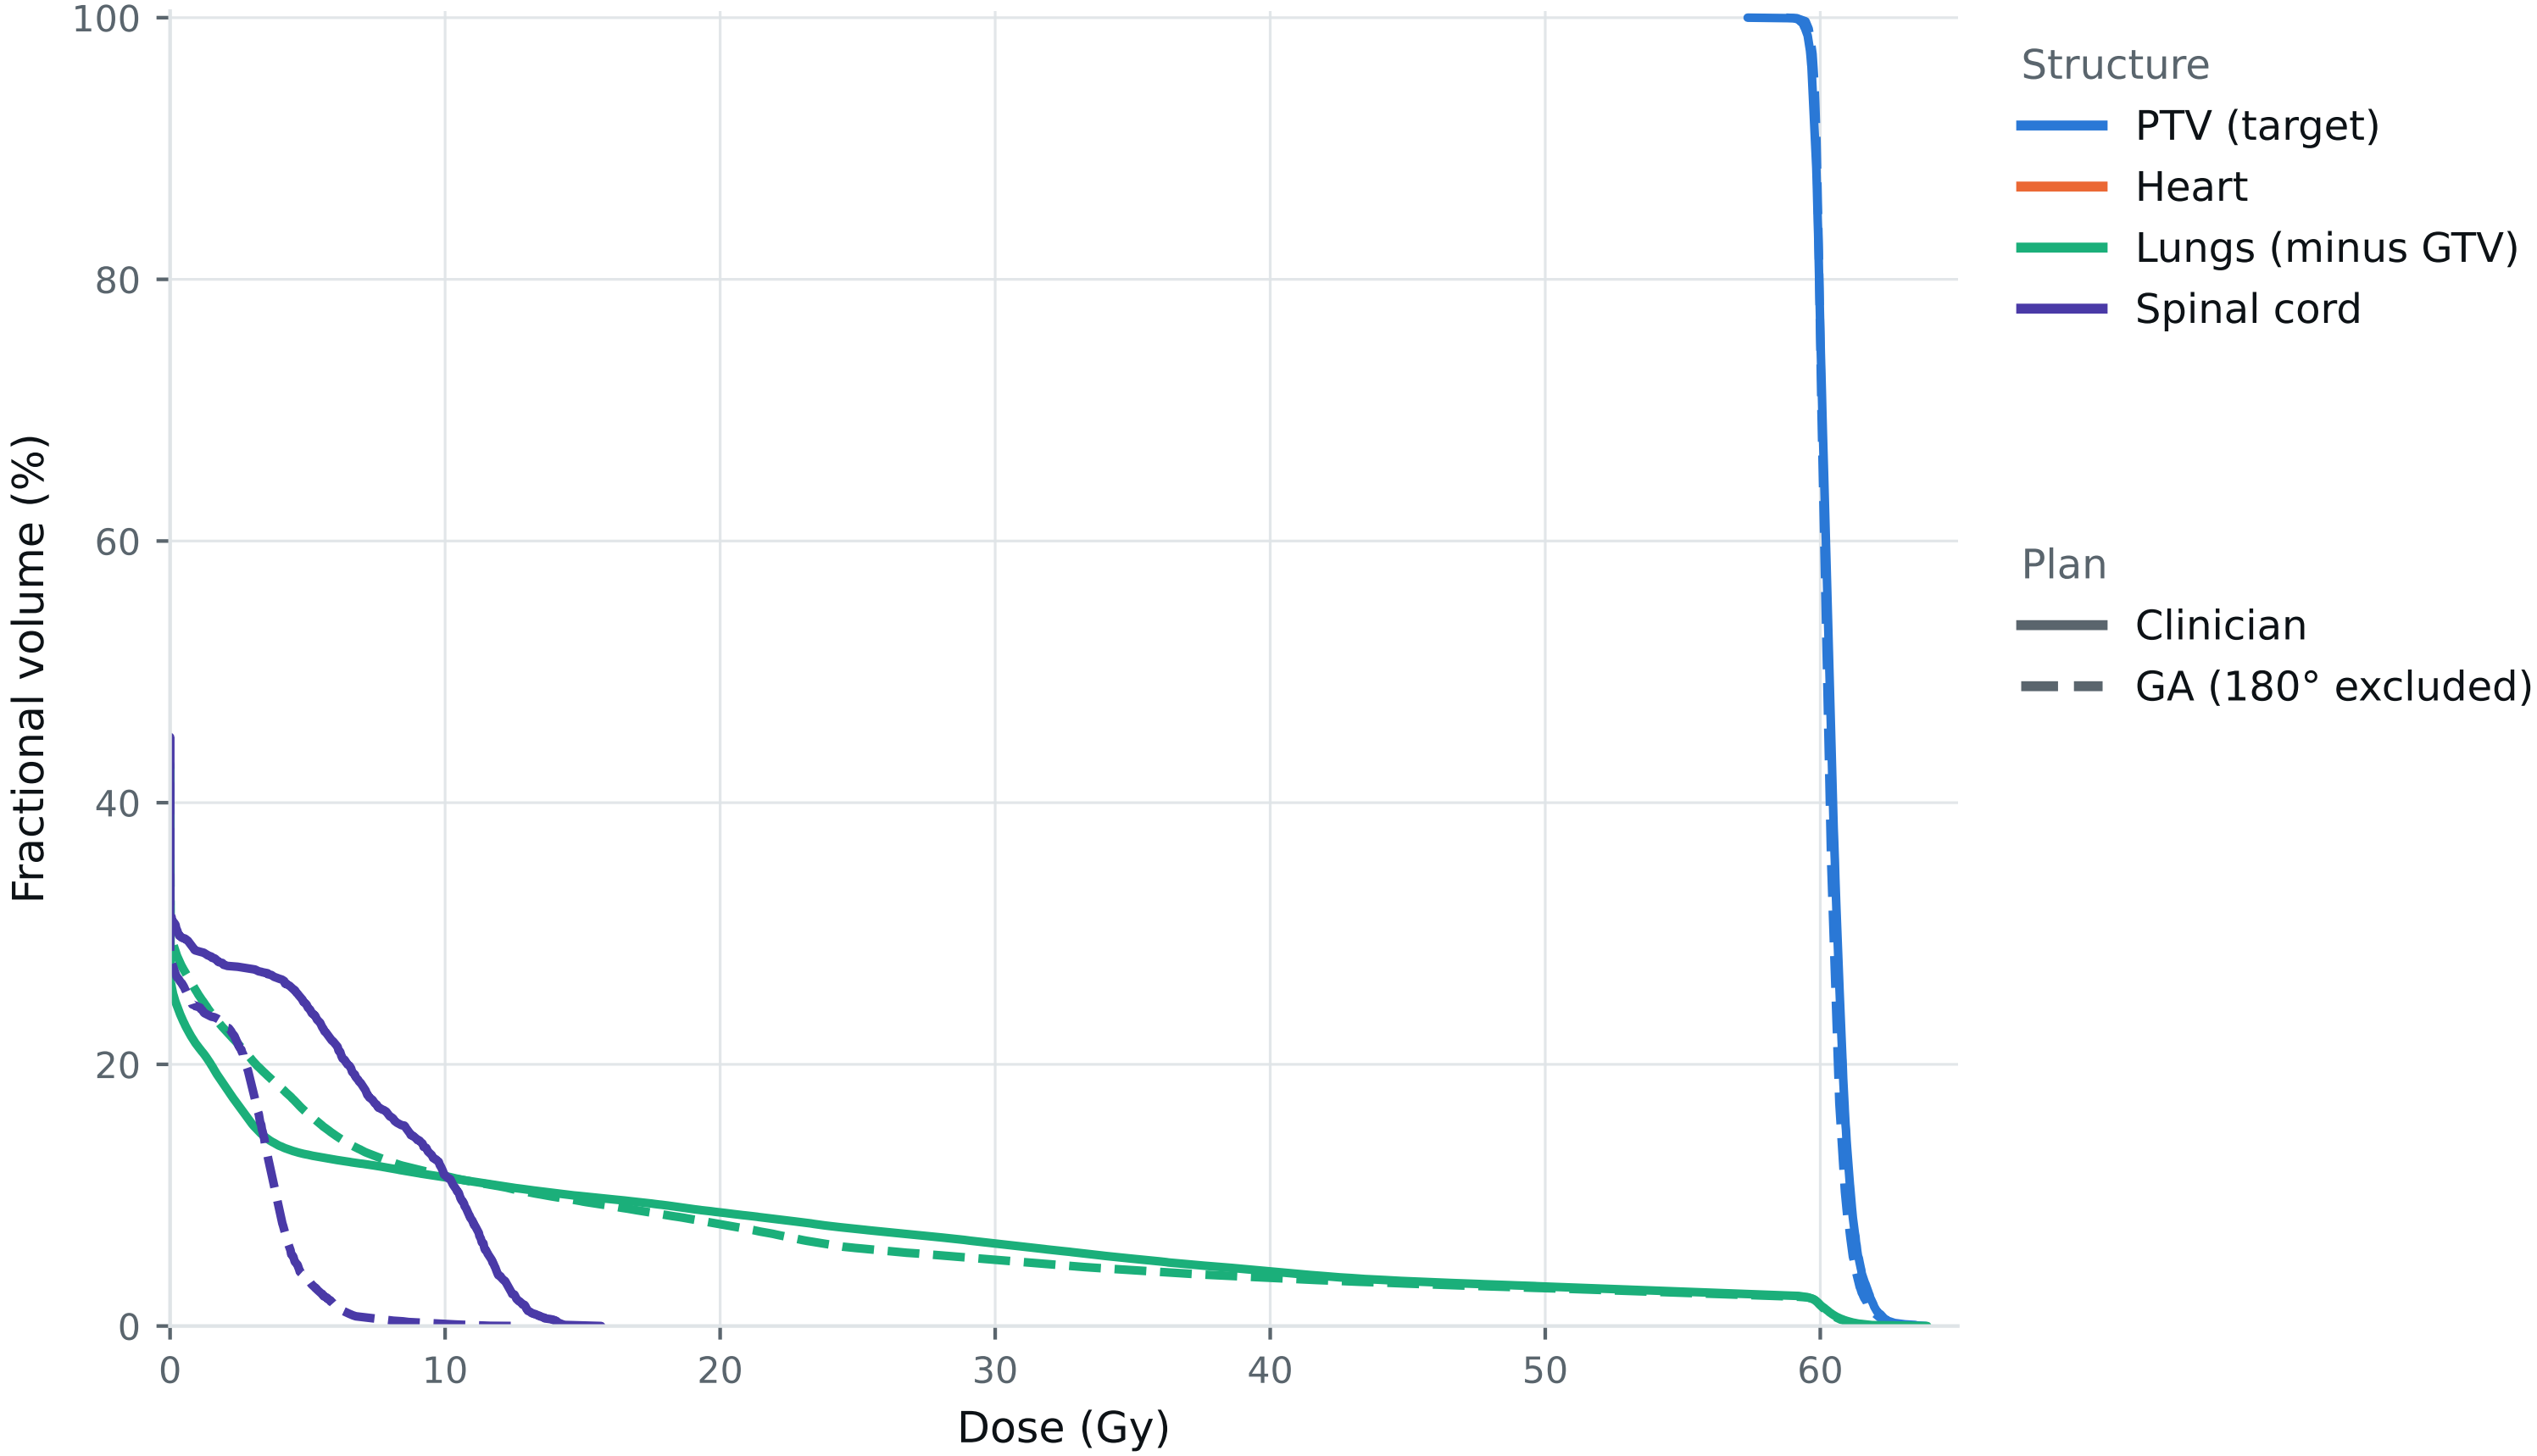

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_18

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

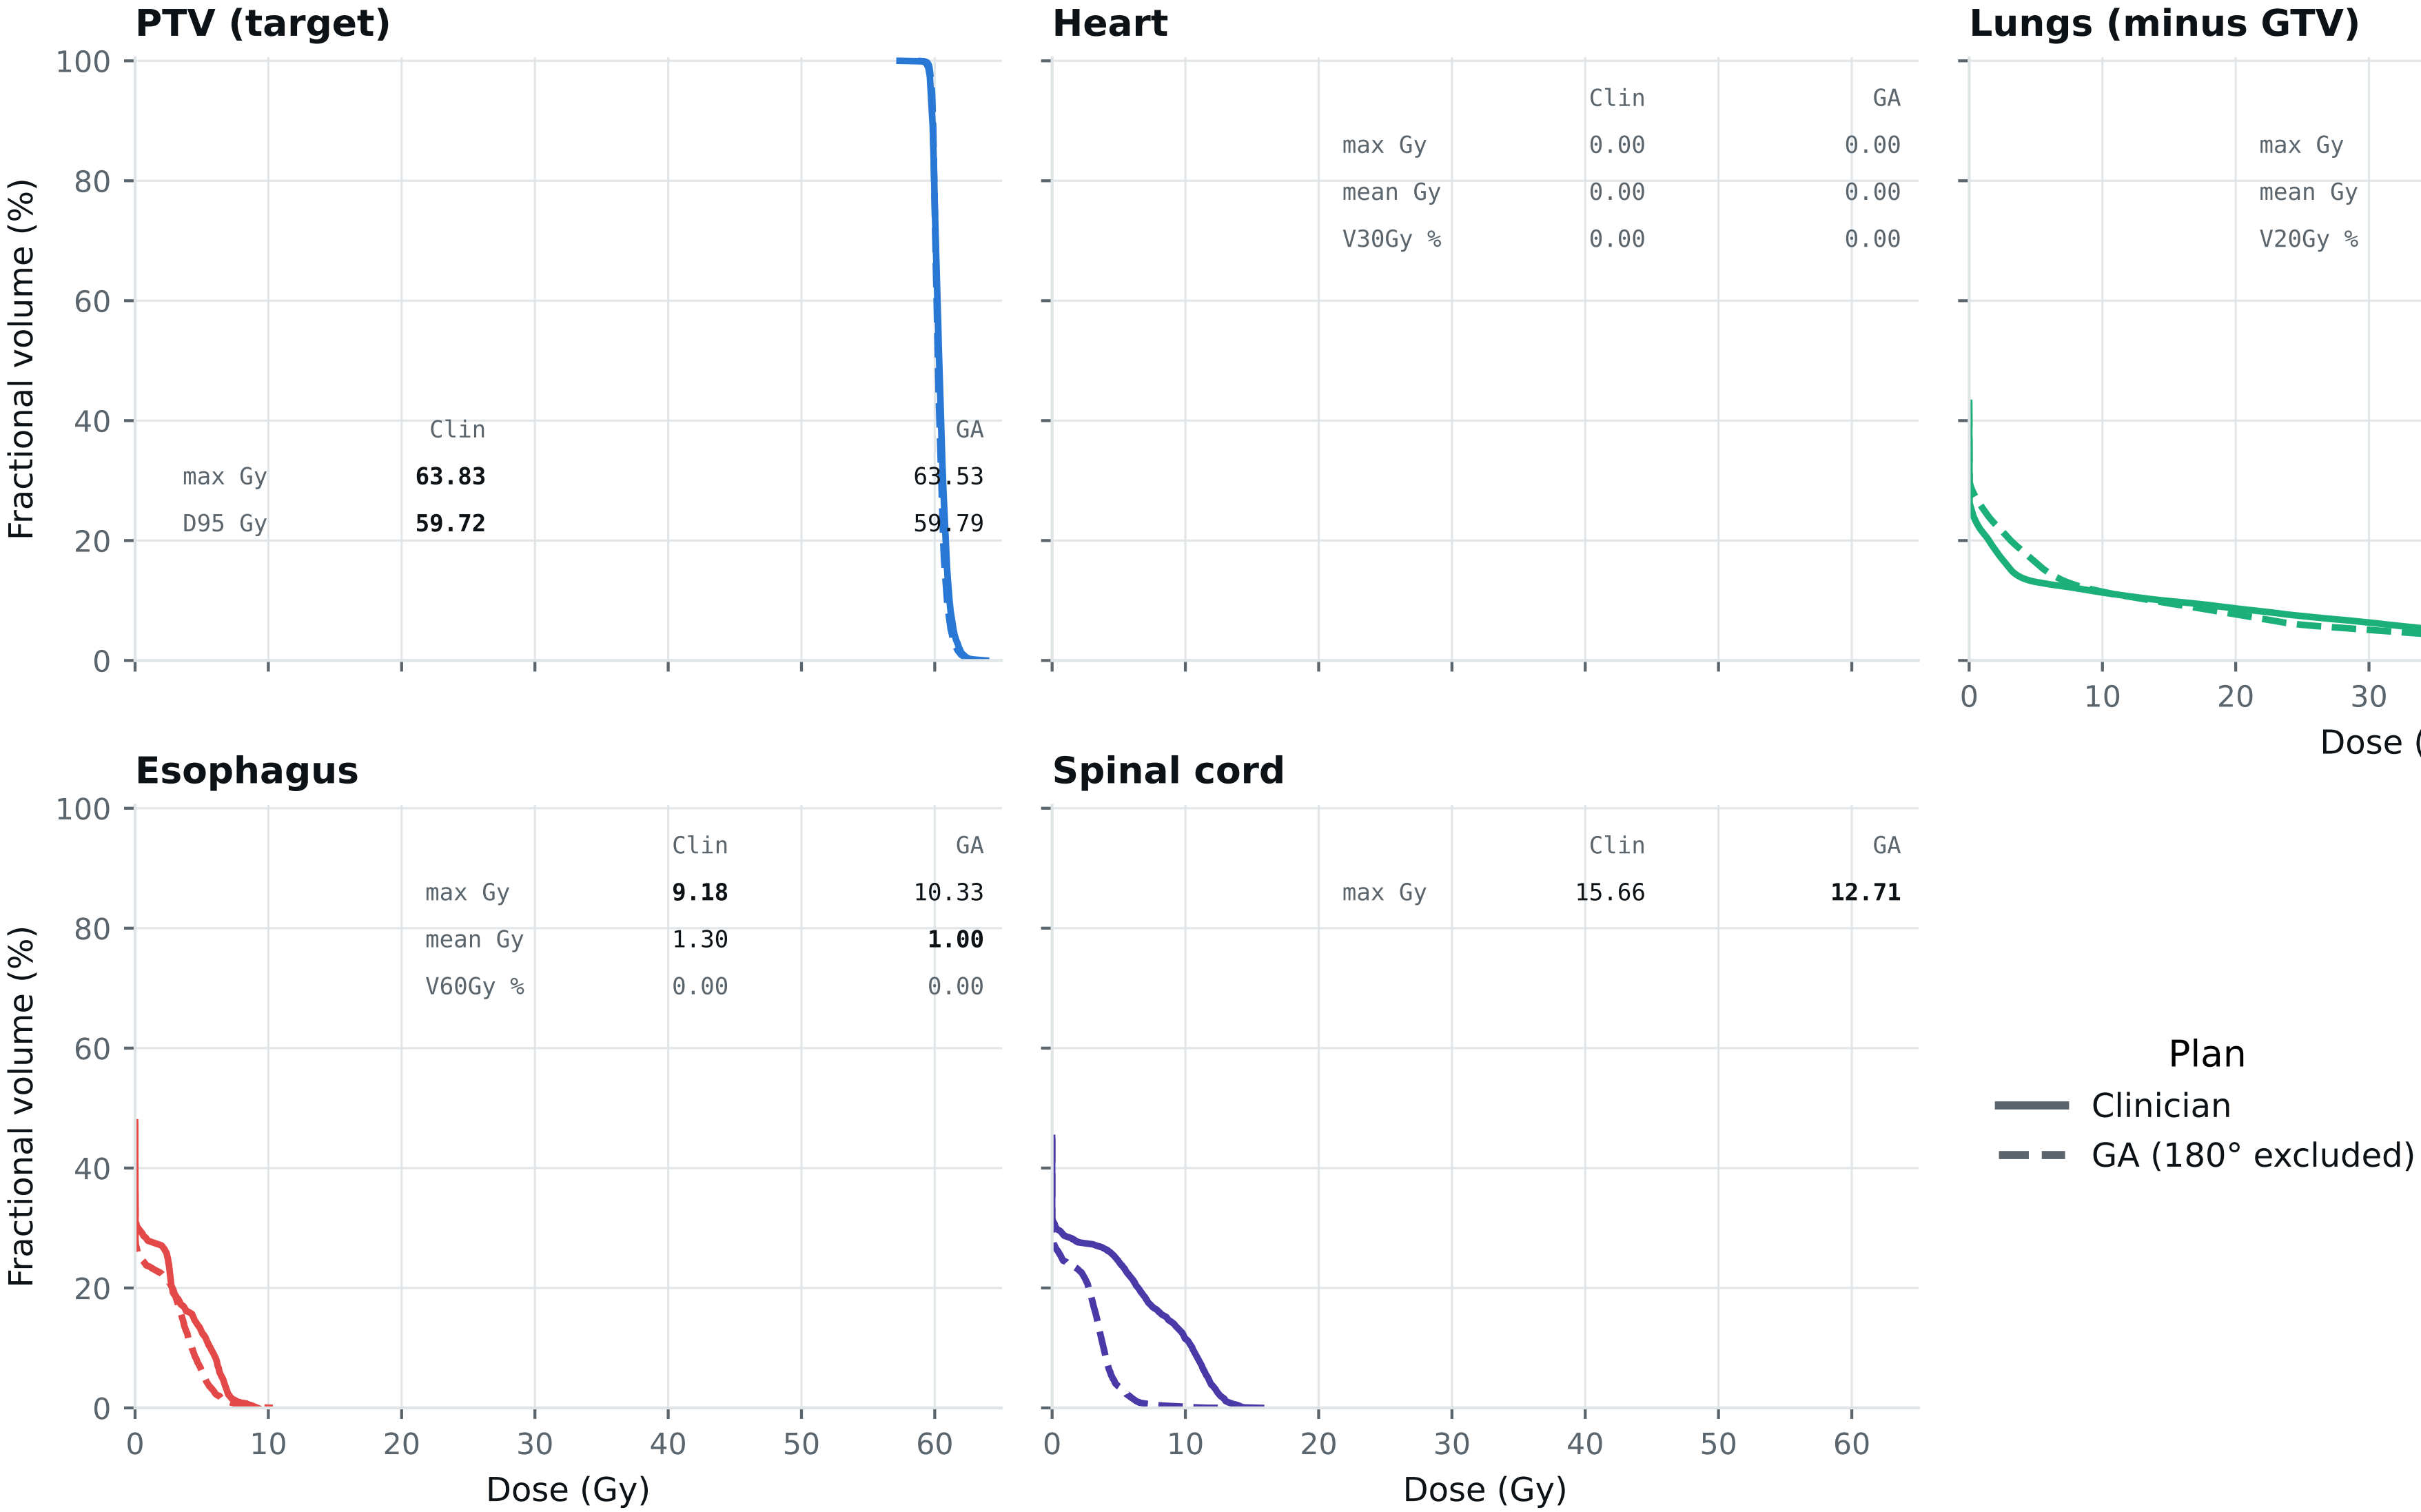

Clinical criteria — Lung_Patient_18

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	62.48	**61.65**	Gy
PTV max	69	66	**63.83**	63.53	Gy
ESOPHAGUS max	66	–	**9.18**	10.33	Gy
ESOPHAGUS mean	34	21	1.30	**1.00**	Gy
ESOPHAGUS V60Gy	17	–	0.00	0.00	%
HEART max	66	–	0.00	0.00	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	–	**7.74**	16.66	Gy
LUNG_R max	66	–	63.88	**63.53**	Gy
CORD max	50	48	15.66	**12.71**	Gy
SKIN max	60	–	60.00	**57.71**	Gy
LUNGS_NOT_GTV max	66	–	63.88	**63.53**	Gy
LUNGS_NOT_GTV mean	21	20	4.37	**4.35**	Gy
LUNGS_NOT_GTV V20Gy	37	–	8.68	**7.79**	%
PTV D95 (target coverage)			59.72	59.79	
Objective value (search signal)			47.89	42.22	
Pipeline time (setup + solve)			27 s	27 s	

```
Beam angles (gantry°)   Clinician  40°, 0°, 330°, 300°, 205°, 185°
                        GA         40°, 0°, 330°, 195°, 240°, 270°, 285°
```

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_18_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.